

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
 Data File : PL041499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 14:02
 Operator : AJ\SJ
 Sample : PB114299BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 04:02:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	4.104	100.7E6	49586011	15.800	16.098
28)	SA Decachlor...	8.220	9.238	103.6E6	41512675	15.638	16.202
Target Compounds							
2)	A alpha-BHC	3.877f	0.000	6043134	0	0.622	N.D. #
6)	B beta-BHC	0.000	4.916f	0	741287	N.D.	0.432 #
10)	B gamma-Chl...	0.000	6.239	0	354742	N.D.	0.105 #
11)	B alpha-Chl...	0.000	6.261f	0	5938860	N.D.	1.755 #
15)	B Endosulfa...	6.244f	7.007f	6533033	-1952699	0.945	N.D. #
25)	Chlordane-3	0.000	6.239	0	354742	N.D.	0.788 #
26)	Chlordane-4	0.000	6.261	0	5938860	N.D.	11.359 #
27)	Chlordane-5	6.244	0.000	6533033	0	26.199	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
Data File : PL041499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 14:02
Operator : AJ\SJ
Sample : PB114299BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 04:02:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

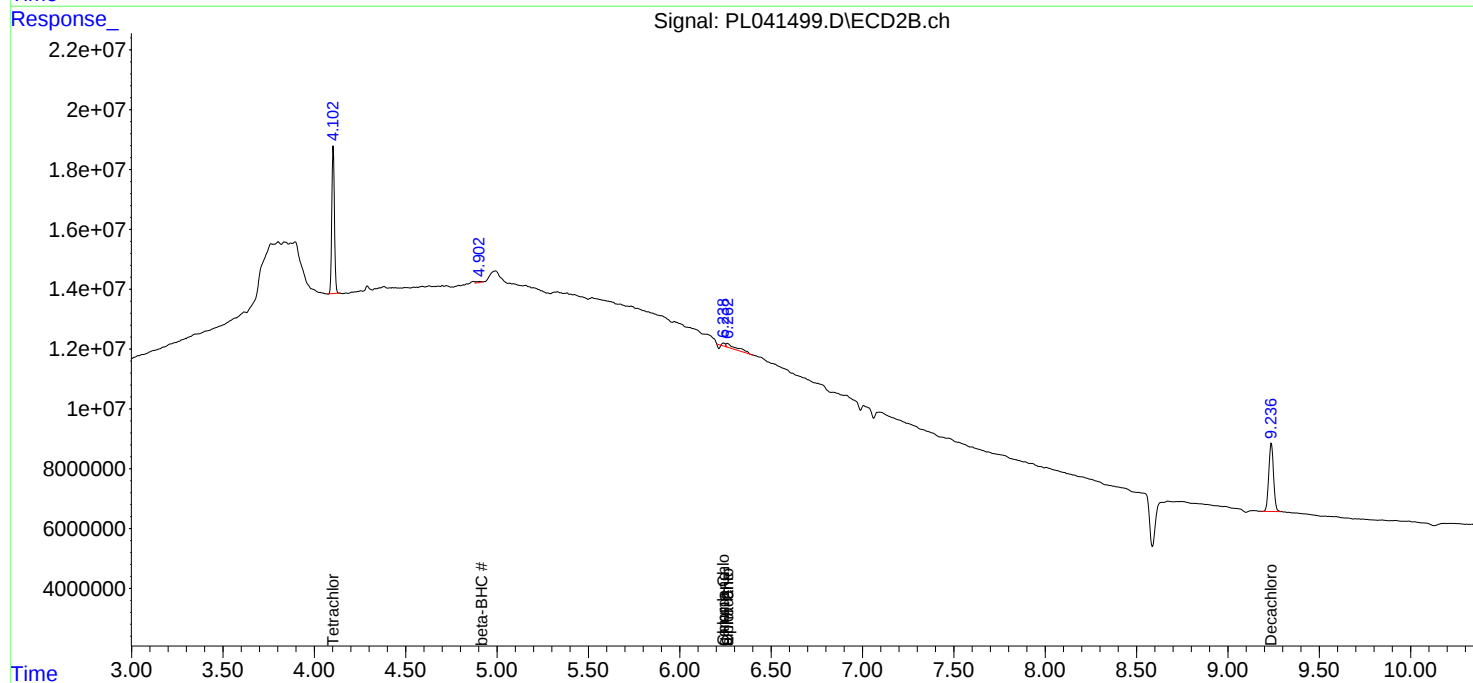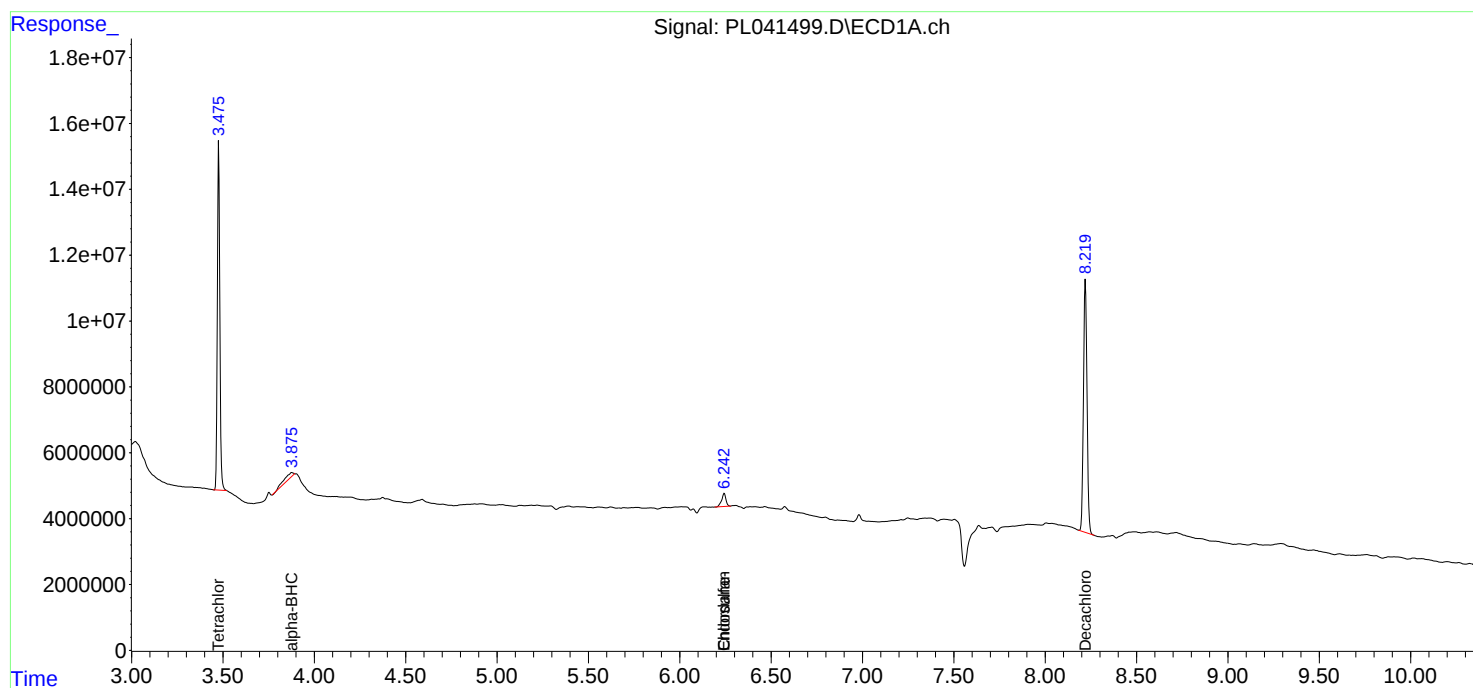


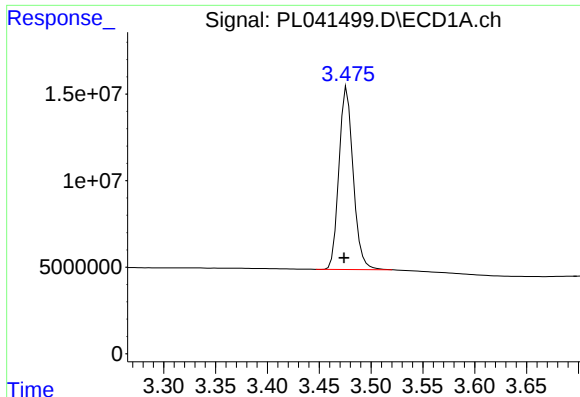

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.003 min
Response: 100652141
Conc: 15.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

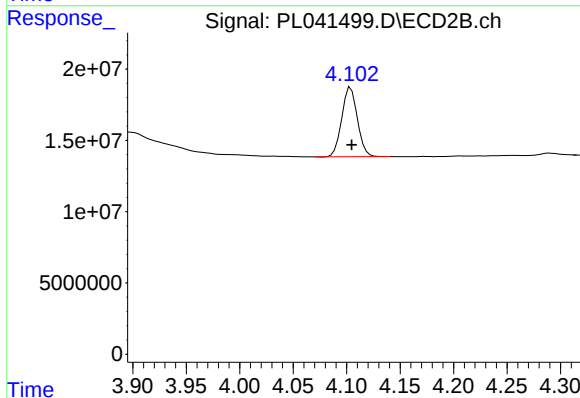


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 49586011
Conc: 16.10 ng/ml

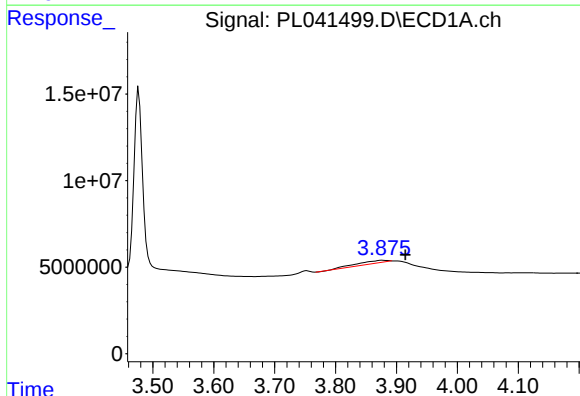


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: -0.038 min
Response: 6043134
Conc: 0.62 ng/ml

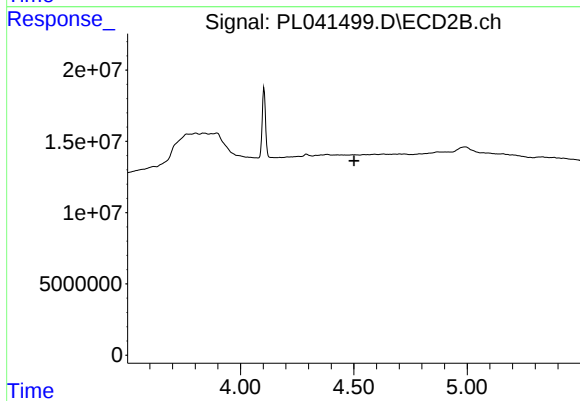

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

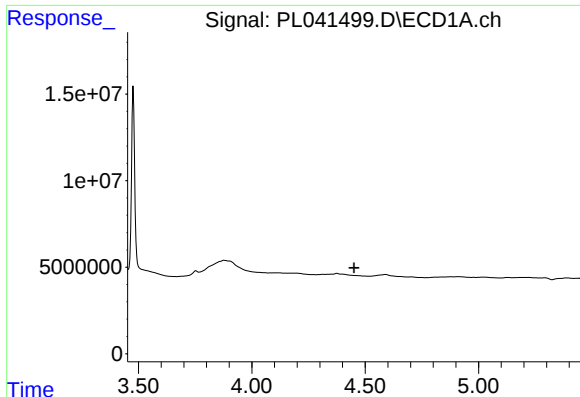

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

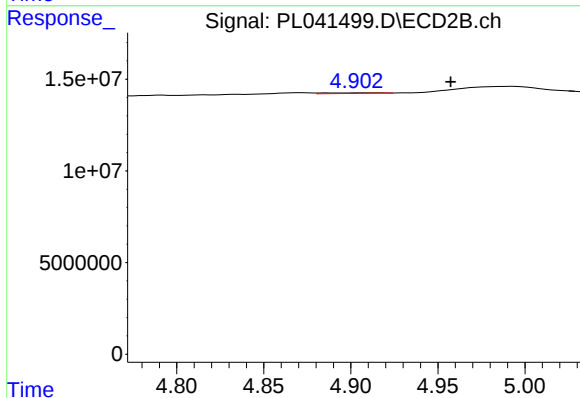


#6 beta-BHC

R.T.: 4.916 min
Delta R.T.: -0.042 min
Response: 741287
Conc: 0.43 ng/ml

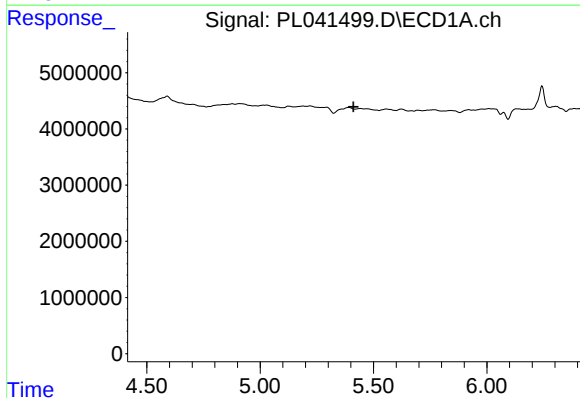


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.412 min
Response: 0
Conc: N.D.

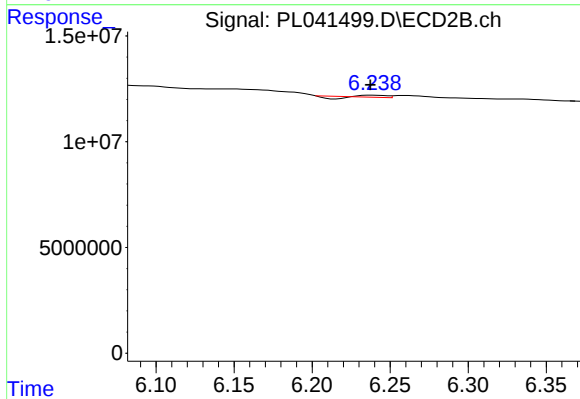

#10 gamma-Chlordane


R.T.: 6.239 min
Delta R.T.: 0.002 min
Response: 354742
Conc: 0.11 ng/ml

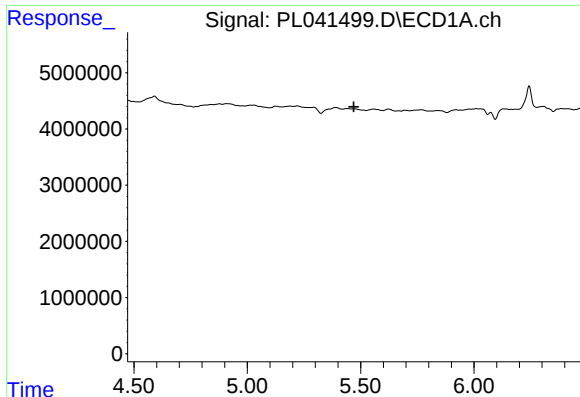

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

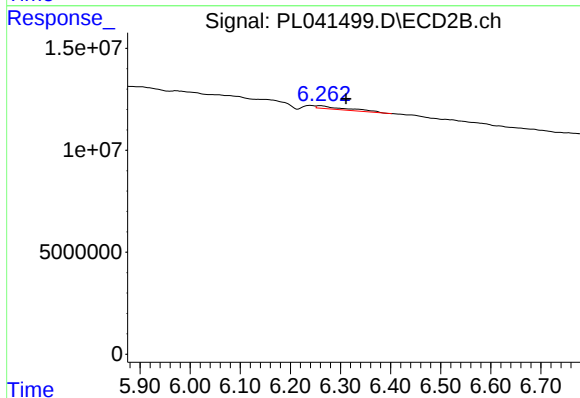


#11 alpha-Chlordane

R.T.: 6.261 min
Delta R.T.: -0.050 min
Response: 5938860
Conc: 1.75 ng/ml

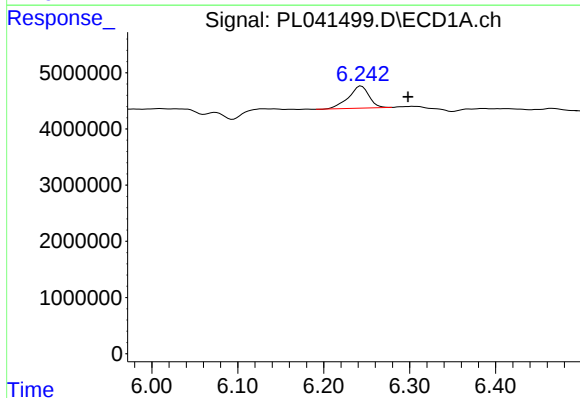


#15 Endosulfan II

R.T.: 6.244 min
Delta R.T.: -0.054 min
Response: 6533033
Conc: 0.95 ng/ml

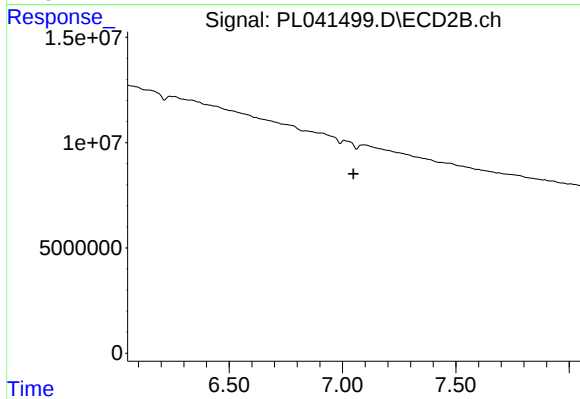

#15 Endosulfan II


R.T.: 7.007 min
Delta R.T.: -0.041 min
Response: -1952699
Conc: N.D.

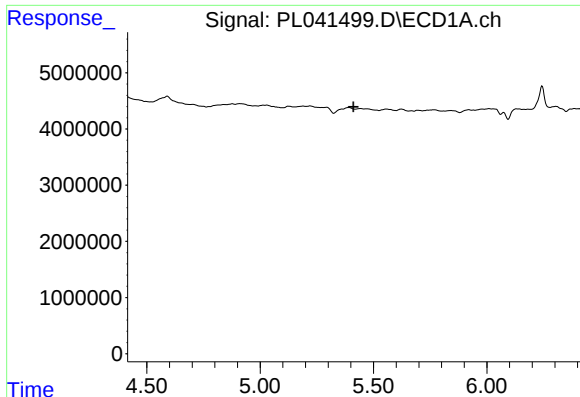

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

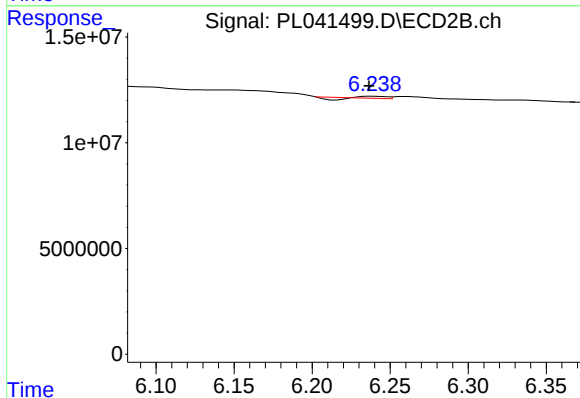


#25 Chlordane-3

R.T.: 6.239 min
Delta R.T.: 0.003 min
Response: 354742
Conc: 0.79 ng/ml

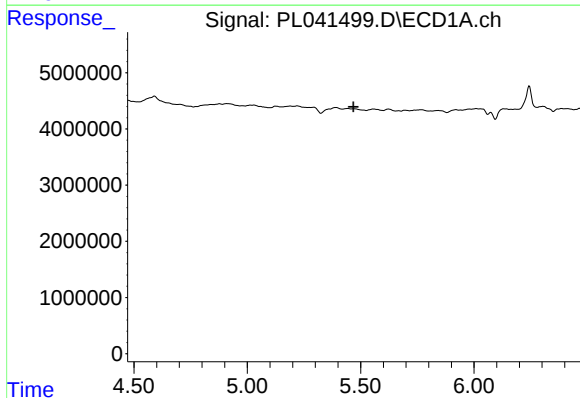


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

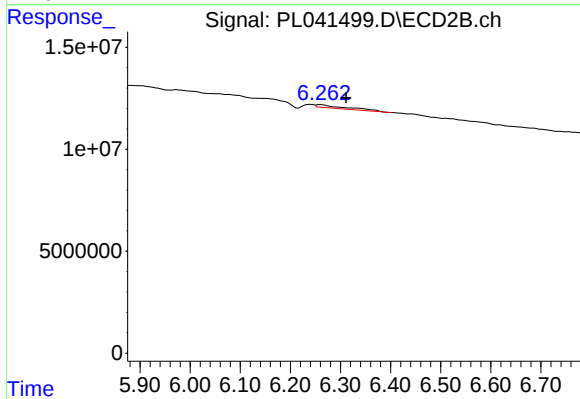

#26 Chlordane-4


R.T.: 6.261 min
Delta R.T.: -0.050 min
Response: 5938860
Conc: 11.36 ng/ml

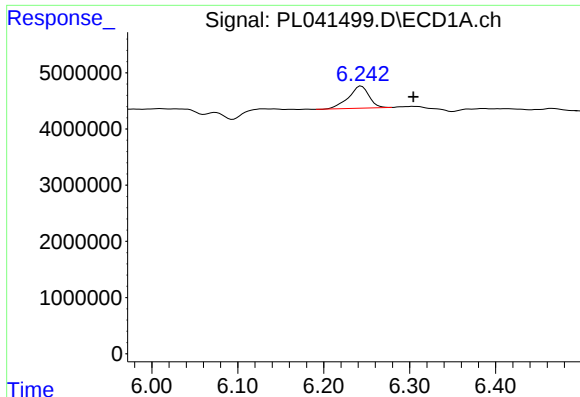

#27 Chlordane-5


R.T.: 6.244 min
Delta R.T.: -0.060 min
Response: 6533033
Conc: 26.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

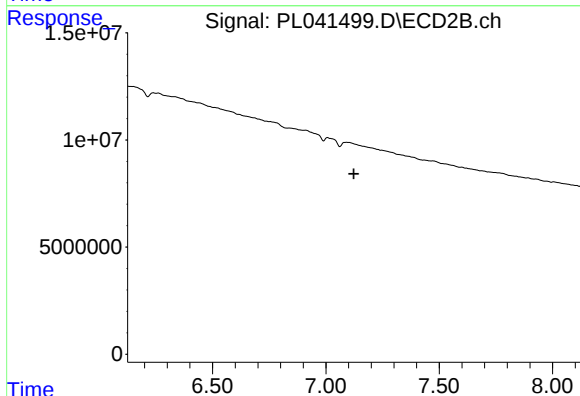


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.123 min
Response: 0
Conc: N.D.

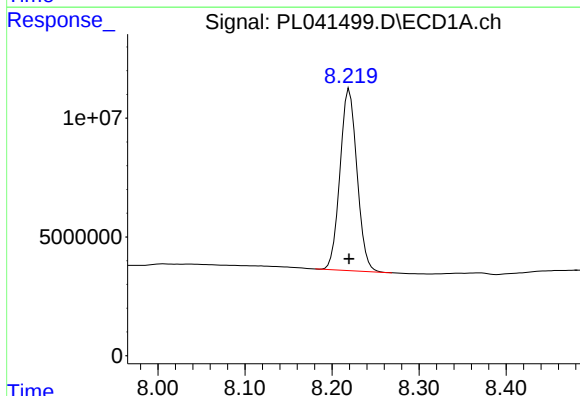

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 103588721
Conc: 15.64 ng/ml

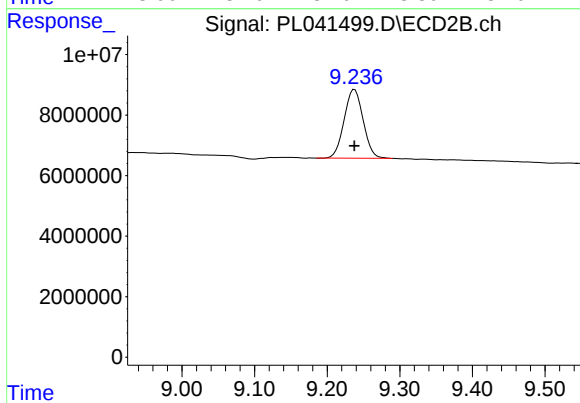

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.000 min
Response: 41512675
Conc: 16.20 ng/ml