

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
 Data File : PL041507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 15:55
 Operator : AJ\SJ
 Sample : PB114302BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 04:04:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.103	132.9E6	67268655	20.859	21.839
28)	SA Decachlor...	8.217	9.234	135.1E6	55204898	20.400	21.546
Target Compounds							
2)	A alpha-BHC	3.910	0.000	4666029	0	0.480	N.D. #
6)	B beta-BHC	4.420f	4.912f	4671138	919499	1.239	0.535 #
7)	B delta-BHC	0.000	5.148f	0	996062	N.D.	0.247 #
9)	A Endosulfan I	5.546	0.000	2580187	0	0.347	N.D. #
15)	B Endosulfa...	6.305	0.000	1218776	0	0.176	N.D. #
19)	B Endosulfa...	6.665	7.416	17248325	-2467882	2.701	N.D. #
23)	Chlordane-1	4.369	5.148	3250578	996062	11.464	7.172 #
24)	Chlordane-2	4.810	0.000	2030550	0	6.895	N.D. #
27)	Chlordane-5	6.305	0.000	1218776	0	4.888	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
Data File : PL041507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 15:55
Operator : AJ\SJ
Sample : PB114302BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 04:04:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

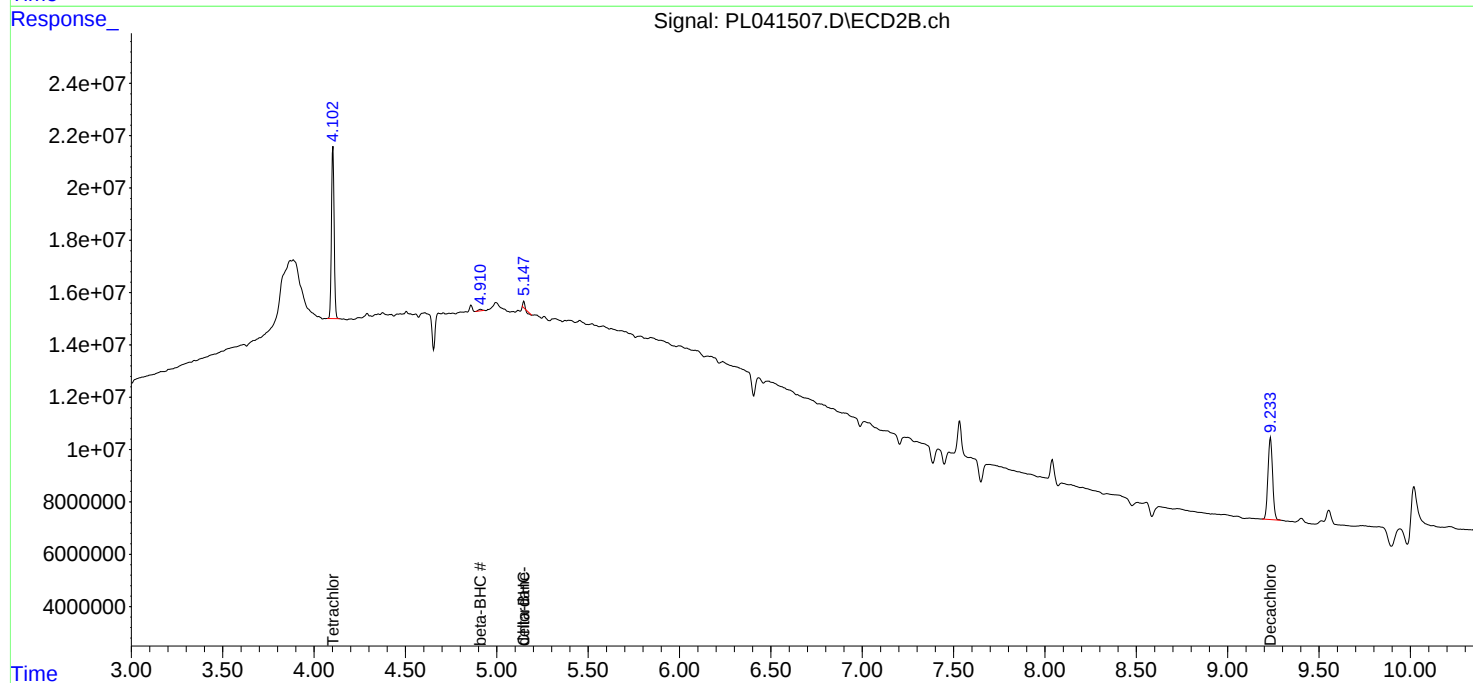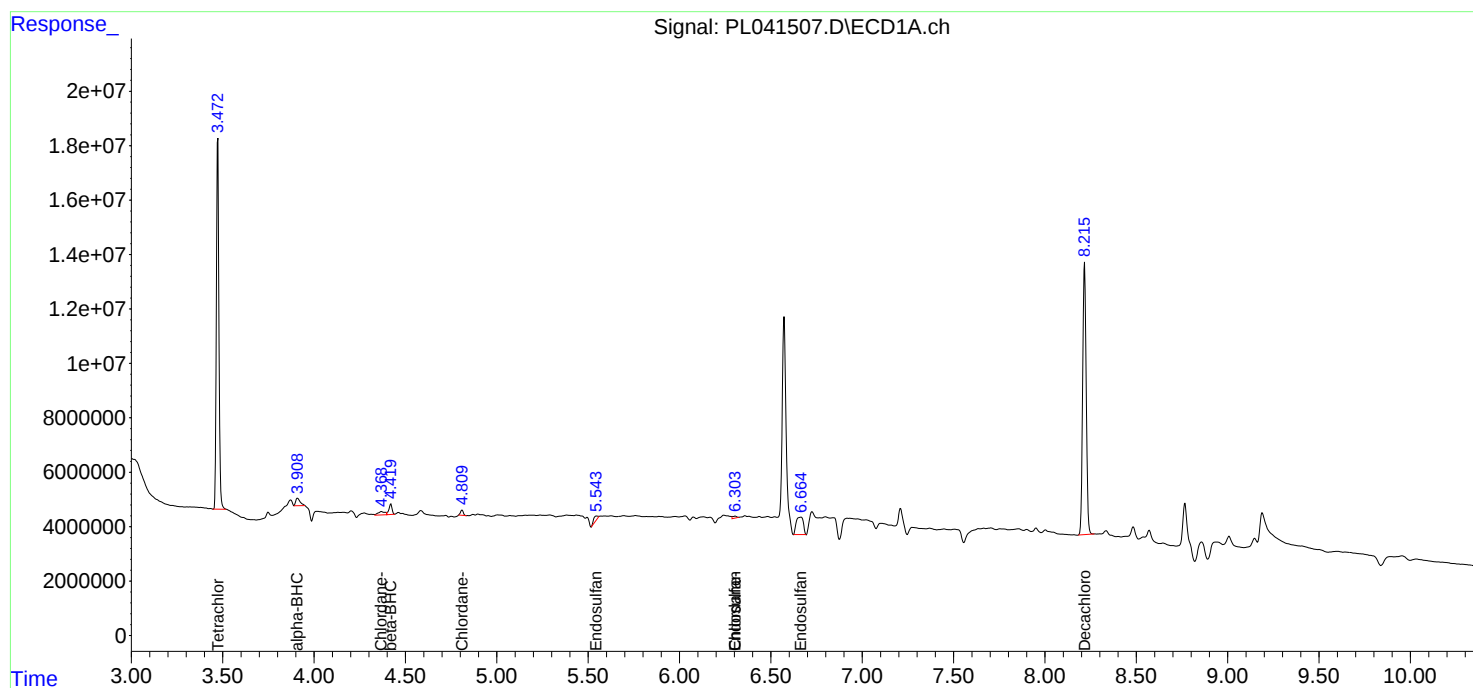


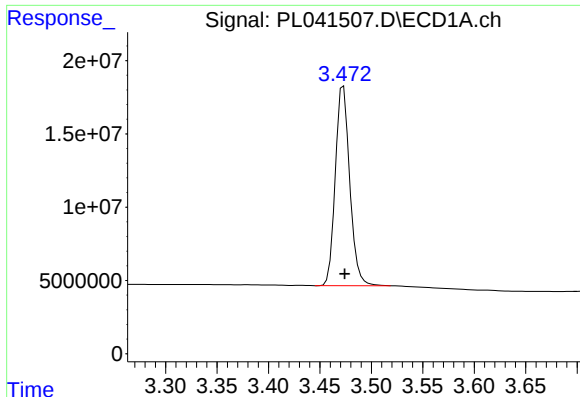

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 132874834
Conc: 20.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

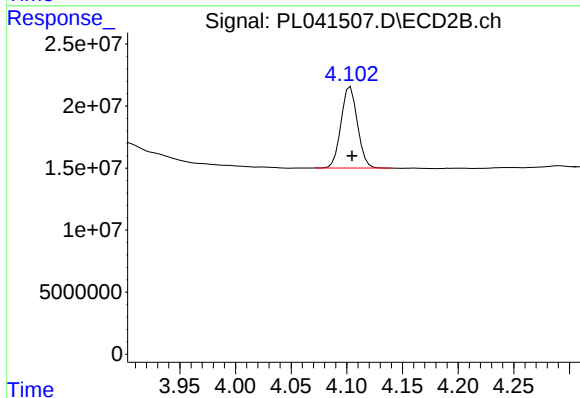


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.001 min
Response: 67268655
Conc: 21.84 ng/ml

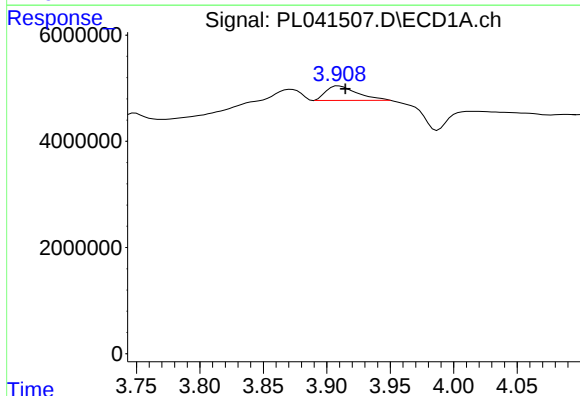


#2 alpha-BHC

R.T.: 3.910 min
Delta R.T.: -0.005 min
Response: 4666029
Conc: 0.48 ng/ml

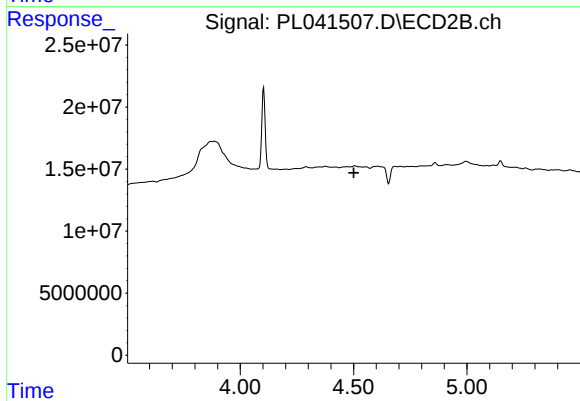

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

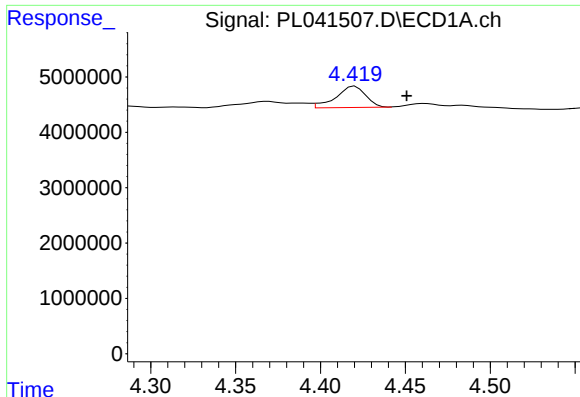

#6 beta-BHC


R.T.: 4.420 min
Delta R.T.: -0.030 min
Response: 4671138
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

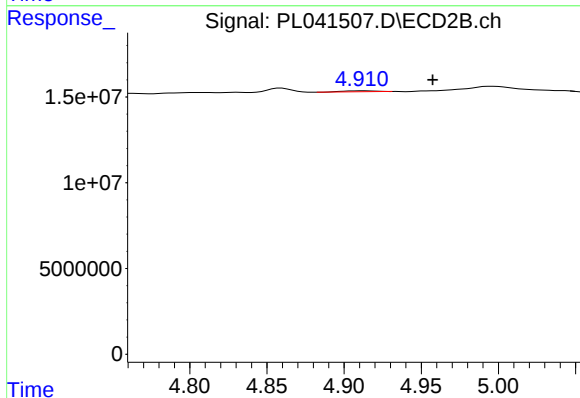


#6 beta-BHC

R.T.: 4.912 min
Delta R.T.: -0.046 min
Response: 919499
Conc: 0.54 ng/ml

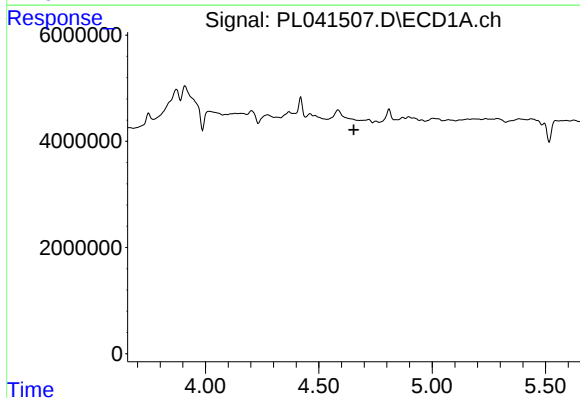


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

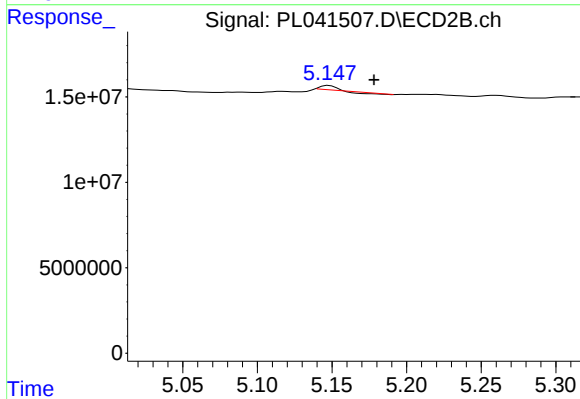

#7 delta-BHC


R.T.: 5.148 min
Delta R.T.: -0.030 min
Response: 996062
Conc: 0.25 ng/ml

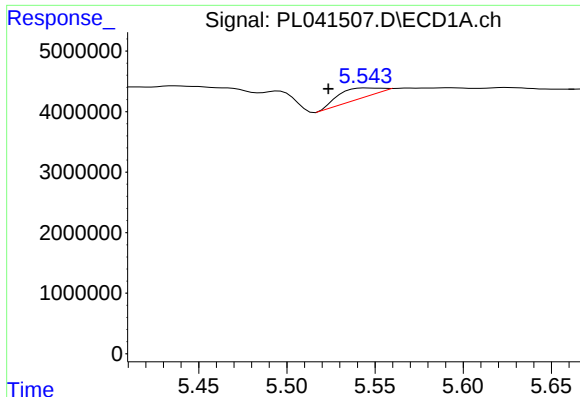

#9 Endosulfan I


R.T.: 5.546 min
Delta R.T.: 0.022 min
Response: 2580187
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

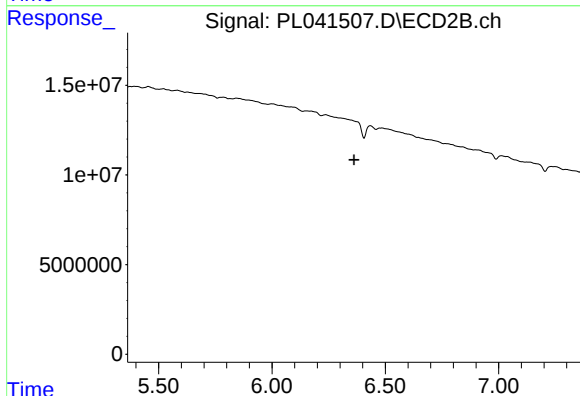


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

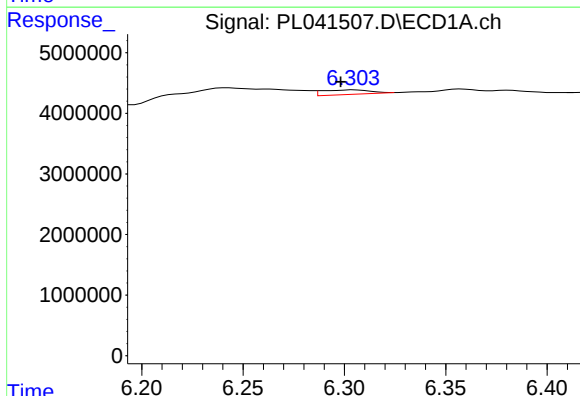


#15 Endosulfan II

R.T.: 6.305 min
Delta R.T.: 0.006 min
Response: 1218776
Conc: 0.18 ng/ml

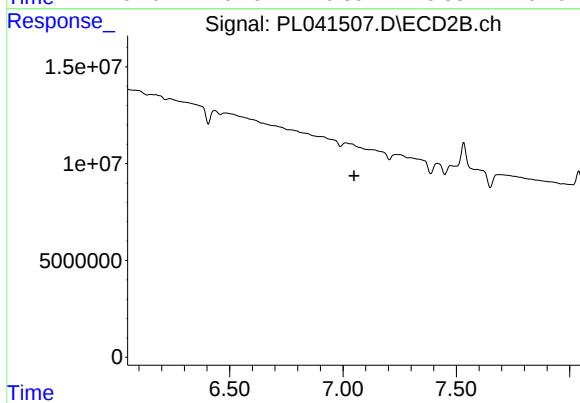

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

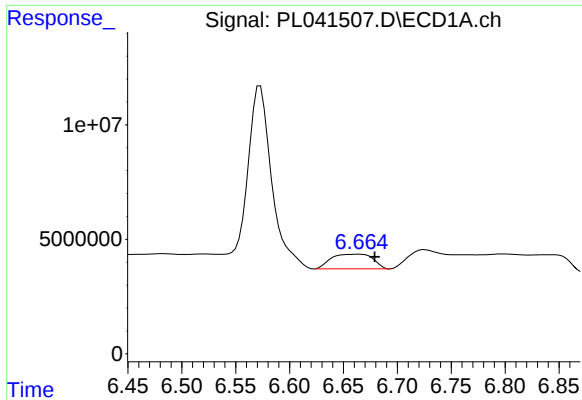

#19 Endosulfan Sulfate


R.T.: 6.665 min
Delta R.T.: -0.014 min
Response: 17248325
Conc: 2.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

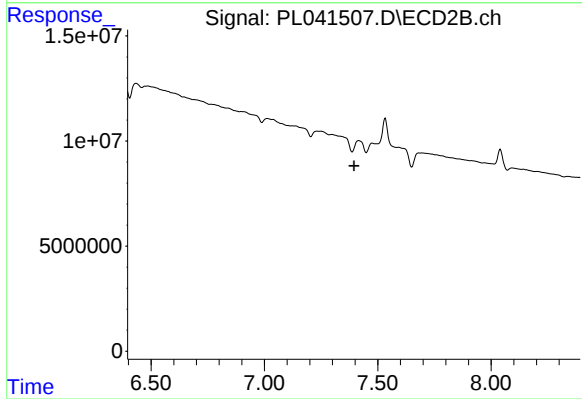


#19 Endosulfan Sulfate

R.T.: 7.416 min
Delta R.T.: 0.020 min
Response: -2467882
Conc: N.D.

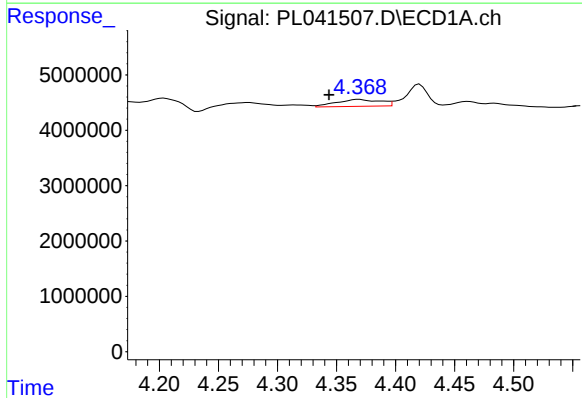


#23 Chlordane-1

R.T.: 4.369 min
Delta R.T.: 0.026 min
Response: 3250578
Conc: 11.46 ng/ml

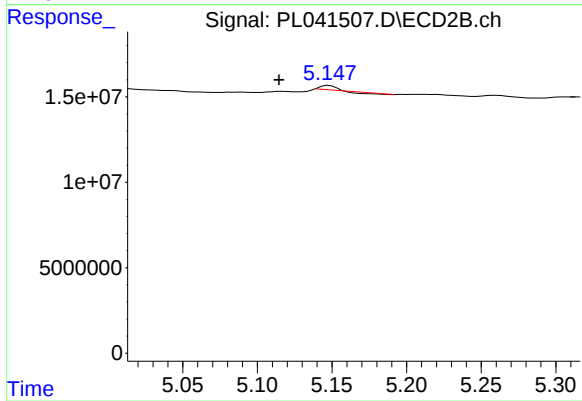

#23 Chlordane-1


R.T.: 5.148 min
Delta R.T.: 0.034 min
Response: 996062
Conc: 7.17 ng/ml

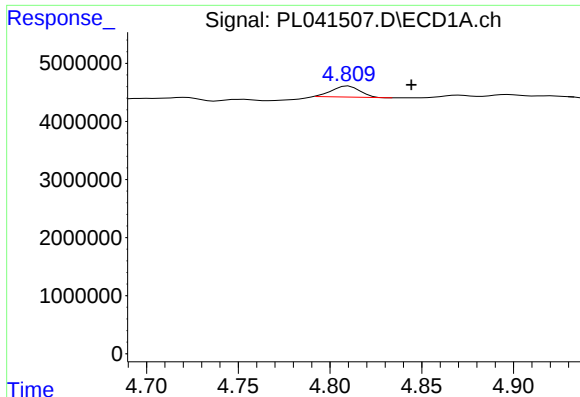

#24 Chlordane-2


R.T.: 4.810 min
Delta R.T.: -0.034 min
Response: 2030550
Conc: 6.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

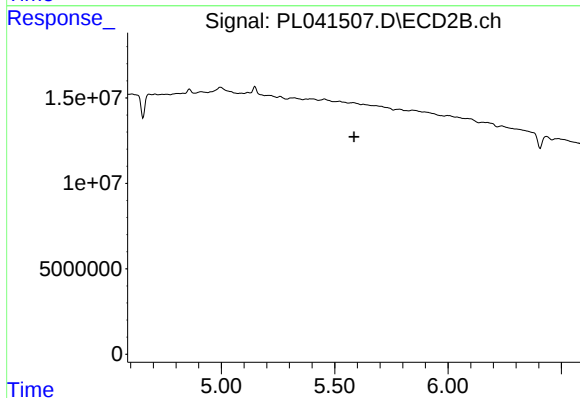


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.586 min
Response: 0
Conc: N.D.

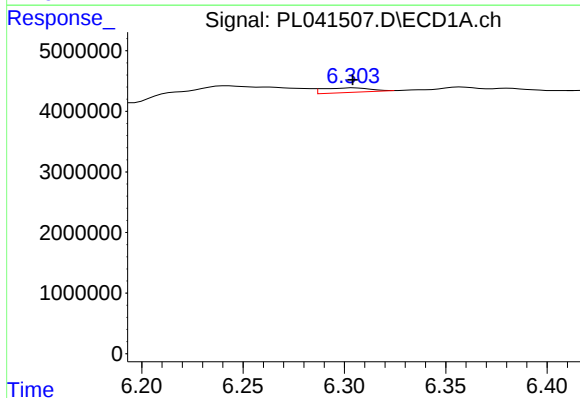


#27 Chlordane-5

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 1218776
Conc: 4.89 ng/ml

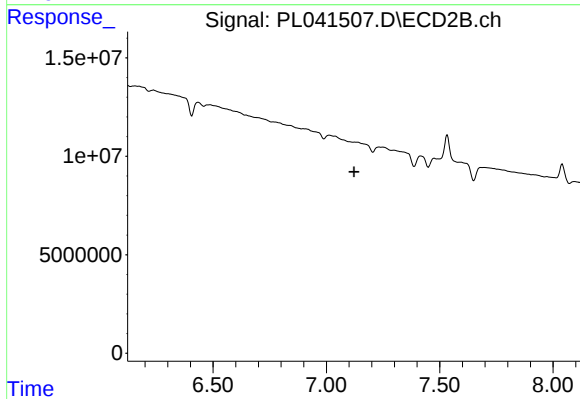

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.123 min
Response: 0
Conc: N.D.

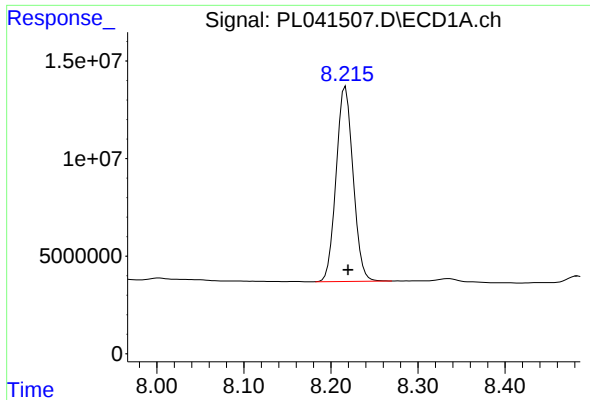

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 135128147
Conc: 20.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

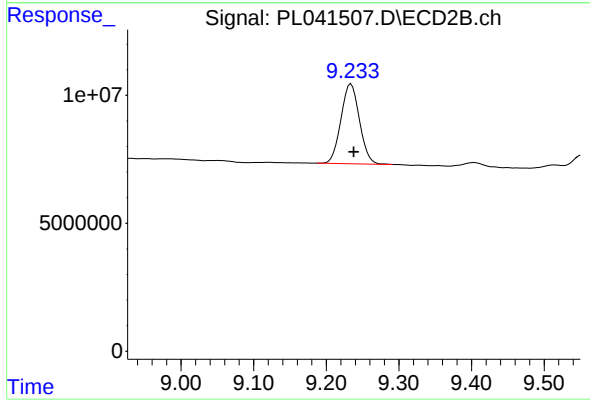

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.004 min
Response: 55204898
Conc: 21.55 ng/ml