

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
 Data File : PL041517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 18:16
 Operator : AJ\SJ
 Sample : J5724-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 04:06:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.103	50647887	26751947	7.951	8.685
28)	SA Decachlor...	8.217	9.234	29841033	12142057	4.505	4.739
Target Compounds							
8)	B Heptachlo...	5.237f	0.000	828642	0	0.103	N.D. #
10)	B gamma-Chl...	5.431	6.235	6977227	368613	0.857	0.109 #
11)	B alpha-Chl...	5.431f	0.000	6977227	0	0.862	N.D. #
12)	B 4,4'-DDE	5.632	6.460	2778657	4928042	0.388	1.506 #
13)	MA Dieldrin	5.757	0.000	3679954	0	0.463	N.D. #
17)	MA 4,4'-DDT	6.385	0.000	2785832	0	0.458	N.D. #
23)	Chlordane-1	4.346	0.000	3379200	0	11.918	N.D. #
25)	Chlordane-3	5.431	6.235	6977227	368613	7.828	0.819 #
26)	Chlordane-4	5.431	0.000	6977227	0	8.911	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
Data File : PL041517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 18:16
Operator : AJ\SJ
Sample : J5724-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 04:06:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

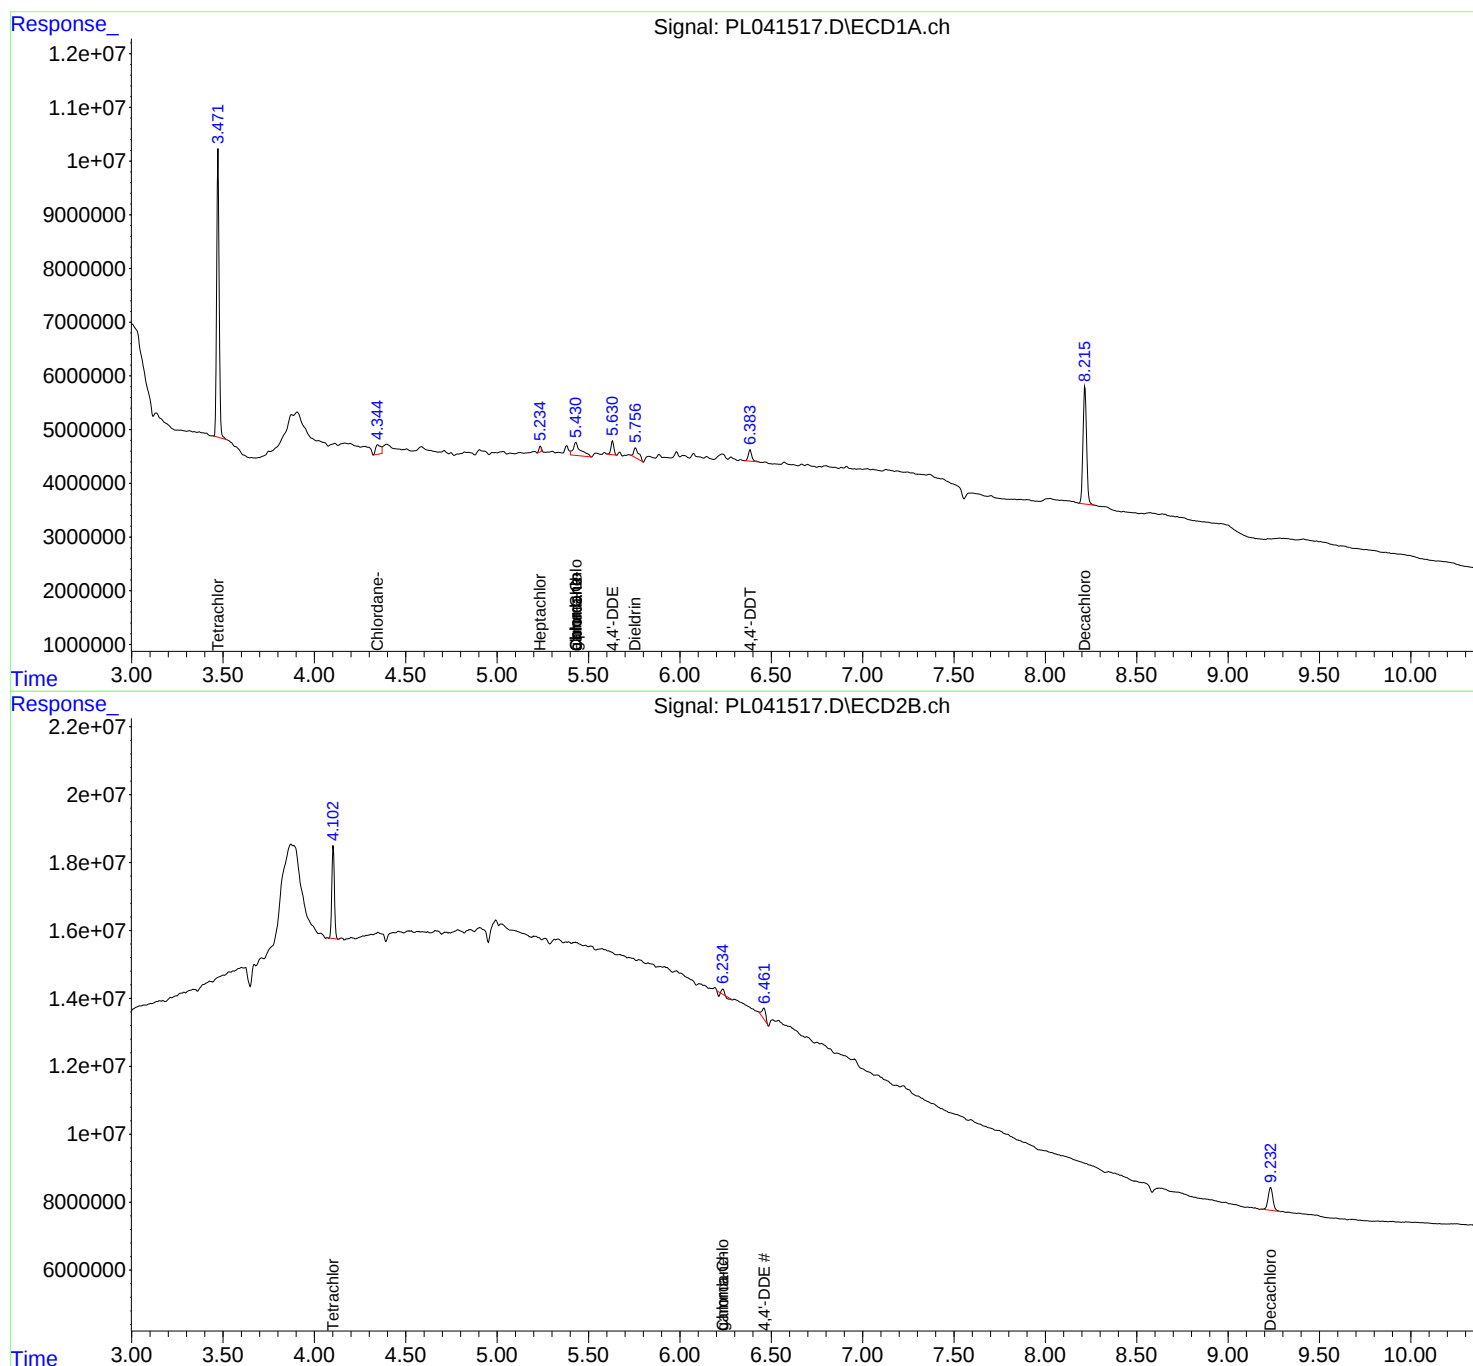


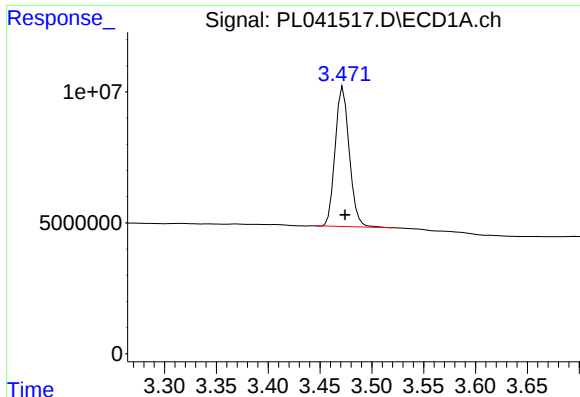

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 50647887
Conc: 7.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

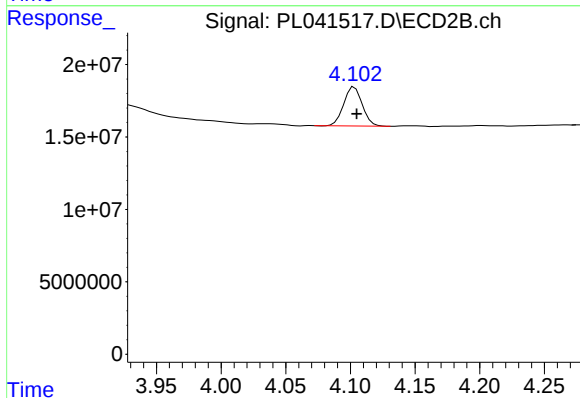


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.002 min
Response: 26751947
Conc: 8.69 ng/ml

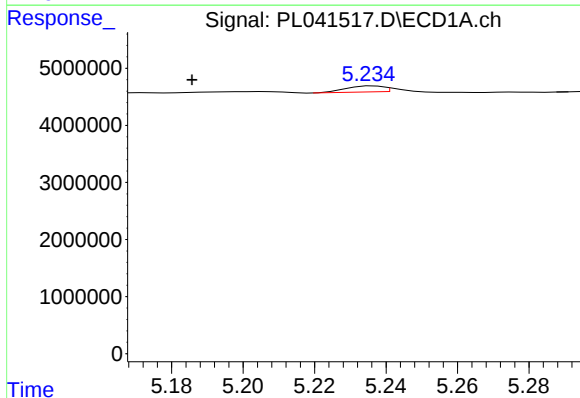


#8 Heptachlor epoxide

R.T.: 5.237 min
Delta R.T.: 0.051 min
Response: 828642
Conc: 0.10 ng/ml

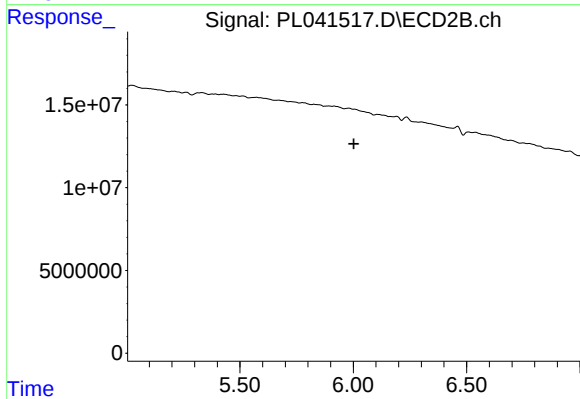

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

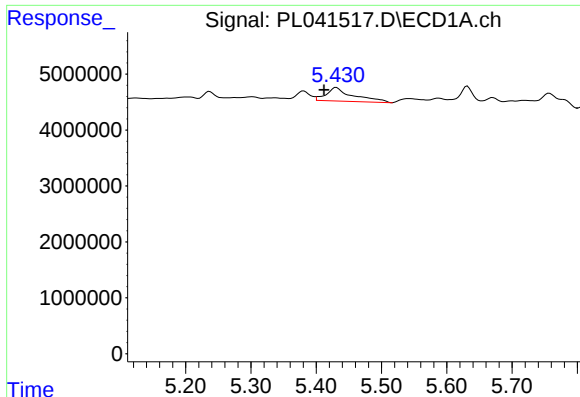

#10 gamma-Chlordane


R.T.: 5.431 min
Delta R.T.: 0.019 min
Response: 6977227
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

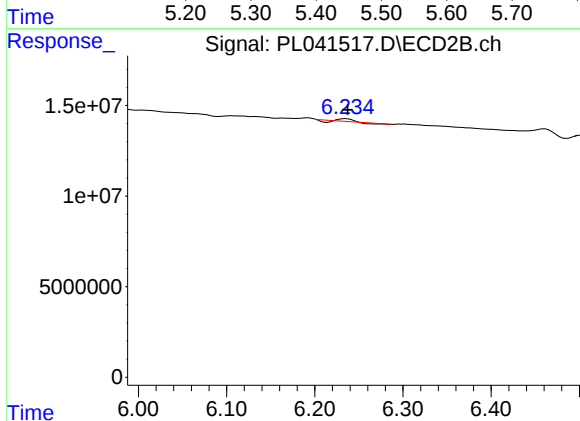


#10 gamma-Chlordane

R.T.: 6.235 min
Delta R.T.: -0.002 min
Response: 368613
Conc: 0.11 ng/ml

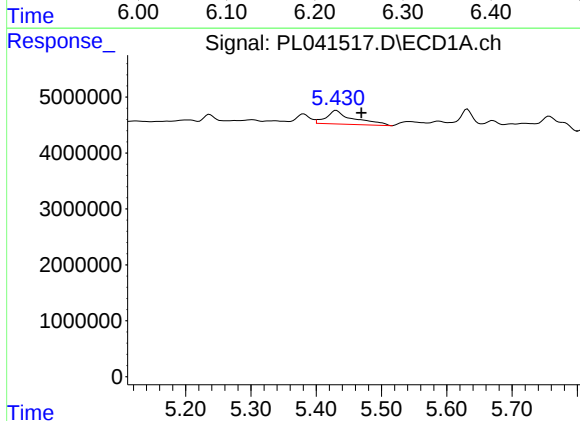


#11 alpha-Chlordane

R.T.: 5.431 min
Delta R.T.: -0.038 min
Response: 6977227
Conc: 0.86 ng/ml

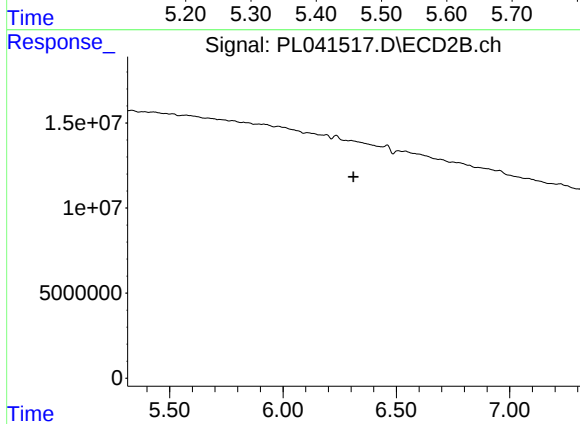

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.311 min
Response: 0
Conc: N.D.

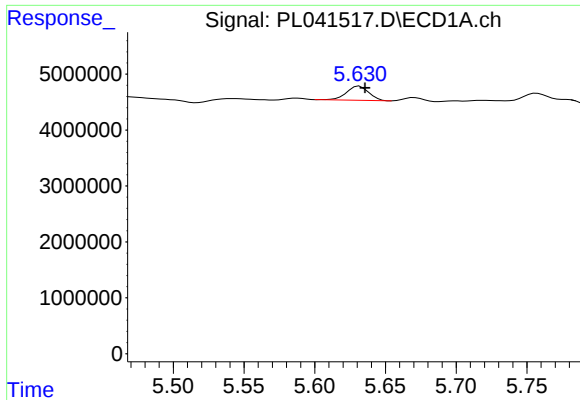

#12 4,4'-DDE


R.T.: 5.632 min
Delta R.T.: -0.004 min
Response: 2778657
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

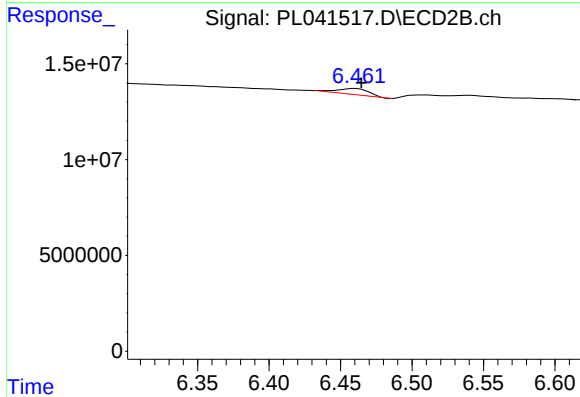


#12 4,4'-DDE

R.T.: 6.460 min
Delta R.T.: -0.004 min
Response: 4928042
Conc: 1.51 ng/ml

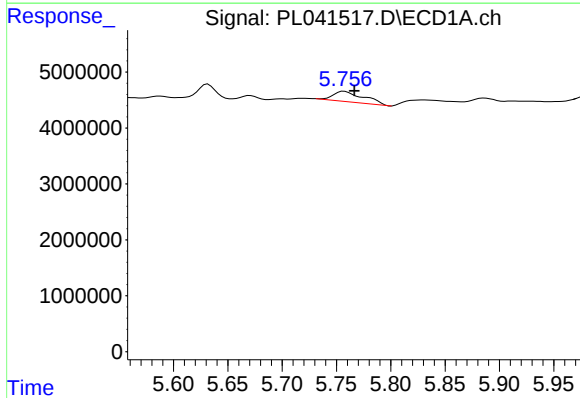


#13 Dieldrin

R.T.: 5.757 min
Delta R.T.: -0.009 min
Response: 3679954
Conc: 0.46 ng/ml

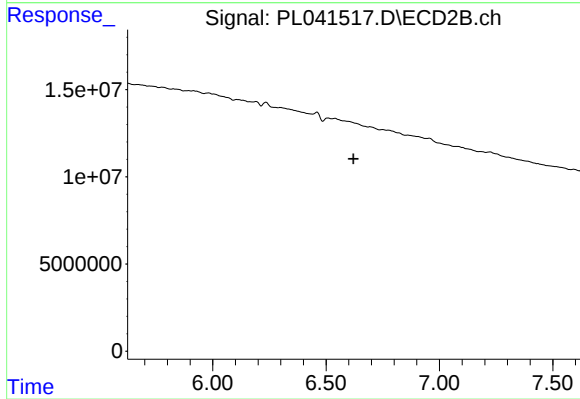

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.621 min
Response: 0
Conc: N.D.

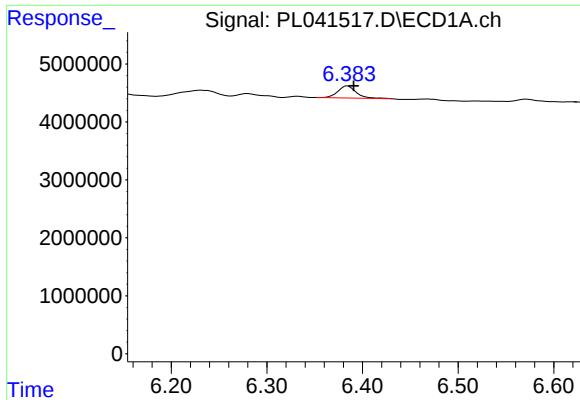

#17 4,4'-DDT


R.T.: 6.385 min
Delta R.T.: -0.006 min
Response: 2785832
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

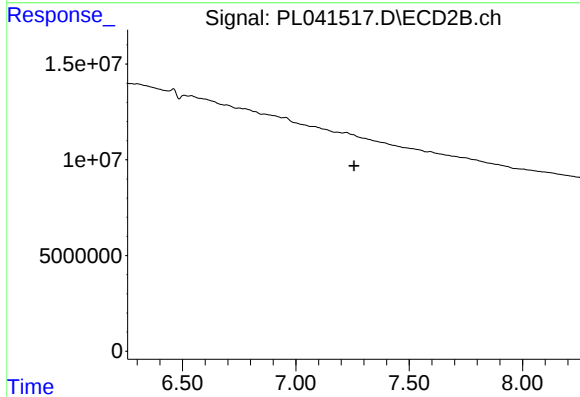


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.258 min
Response: 0
Conc: N.D.

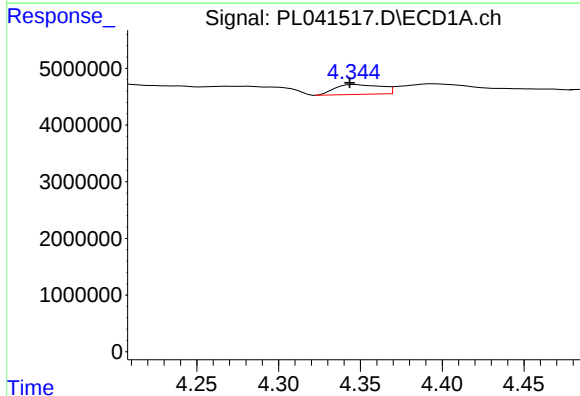


#23 Chlordane-1

R.T.: 4.346 min
Delta R.T.: 0.003 min
Response: 3379200
Conc: 11.92 ng/ml

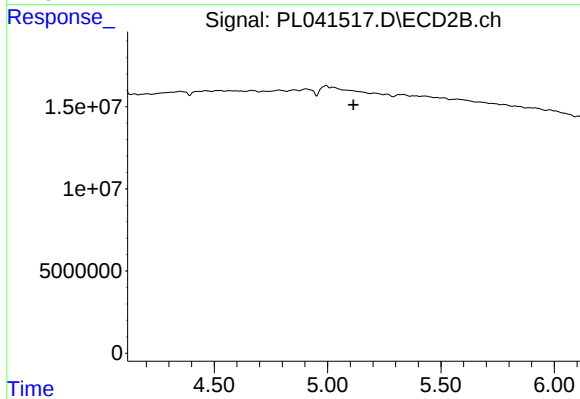

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

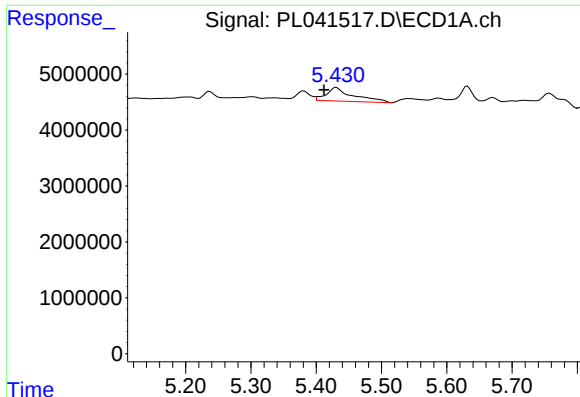

#25 Chlordane-3


R.T.: 5.431 min
Delta R.T.: 0.019 min
Response: 6977227
Conc: 7.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

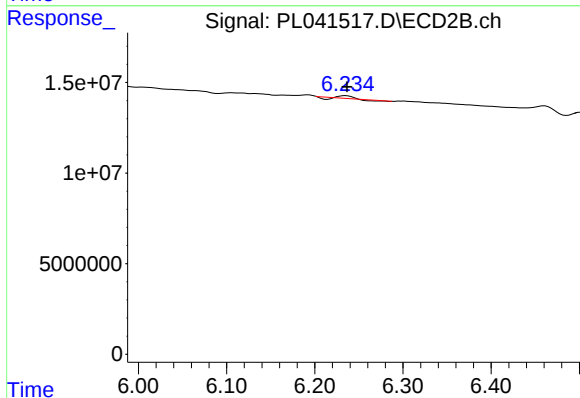


#25 Chlordane-3

R.T.: 6.235 min
Delta R.T.: -0.001 min
Response: 368613
Conc: 0.82 ng/ml

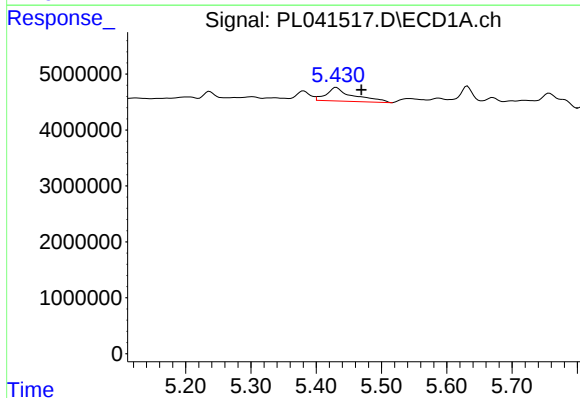


#26 Chlordane-4

R.T.: 5.431 min
Delta R.T.: -0.038 min
Response: 6977227
Conc: 8.91 ng/ml

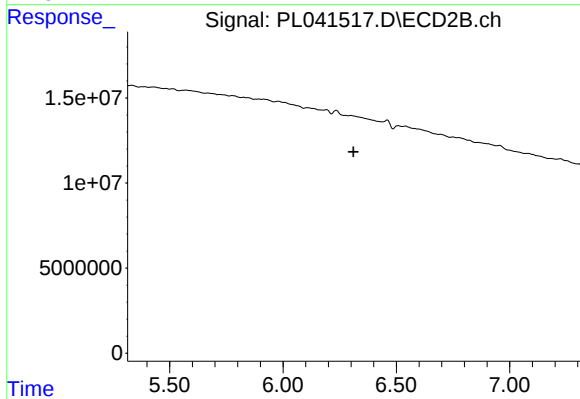

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.311 min
Response: 0
Conc: N.D.

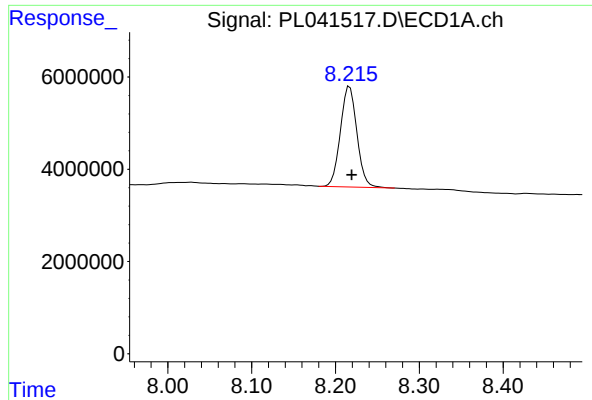

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 29841033
Conc: 4.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

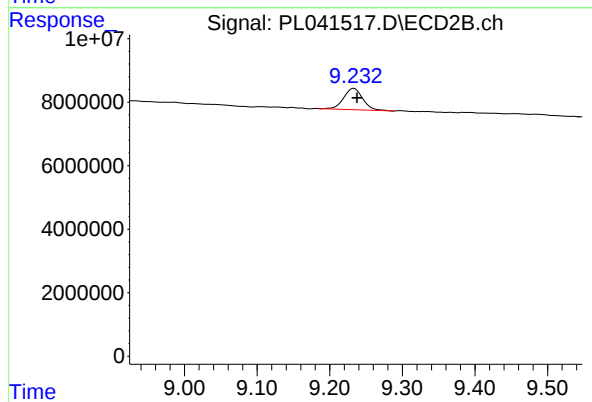

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.004 min
Response: 12142057
Conc: 4.74 ng/ml