

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
 Data File : PL041523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 19:41
 Operator : AJ\SJ
 Sample : J5194-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 04:07:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.103	122.8E6	61239651	19.270	19.882
28)	SA Decachlor...	8.217	9.234	125.7E6	52355864	18.979	20.434
Target Compounds							
2)	A alpha-BHC	3.907	0.000	3072989	0	0.316	N.D. #
4)	MA Heptachlor	4.451f	0.000	3655866	0	0.399	N.D. #
5)	MB Aldrin	0.000	5.637	0	2051802	N.D.	0.537 #
6)	B beta-BHC	4.451	0.000	3655866	0	0.970	N.D. #
9)	A Endosulfan I	5.550	0.000	2799308	0	0.376	N.D. #
15)	B Endosulfa...	6.237f	0.000	1929512	0	0.279	N.D. #
19)	B Endosulfa...	6.677	0.000	6808132	0	1.066	N.D. #
23)	Chlordane-1	4.371	0.000	2082463	0	7.345	N.D. #
24)	Chlordane-2	4.910	5.637	6840396	2051802	23.227	15.440 #
27)	Chlordane-5	6.237	0.000	1929512	0	7.738	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
Data File : PL041523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 19:41
Operator : AJ\SJ
Sample : J5194-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 04:07:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

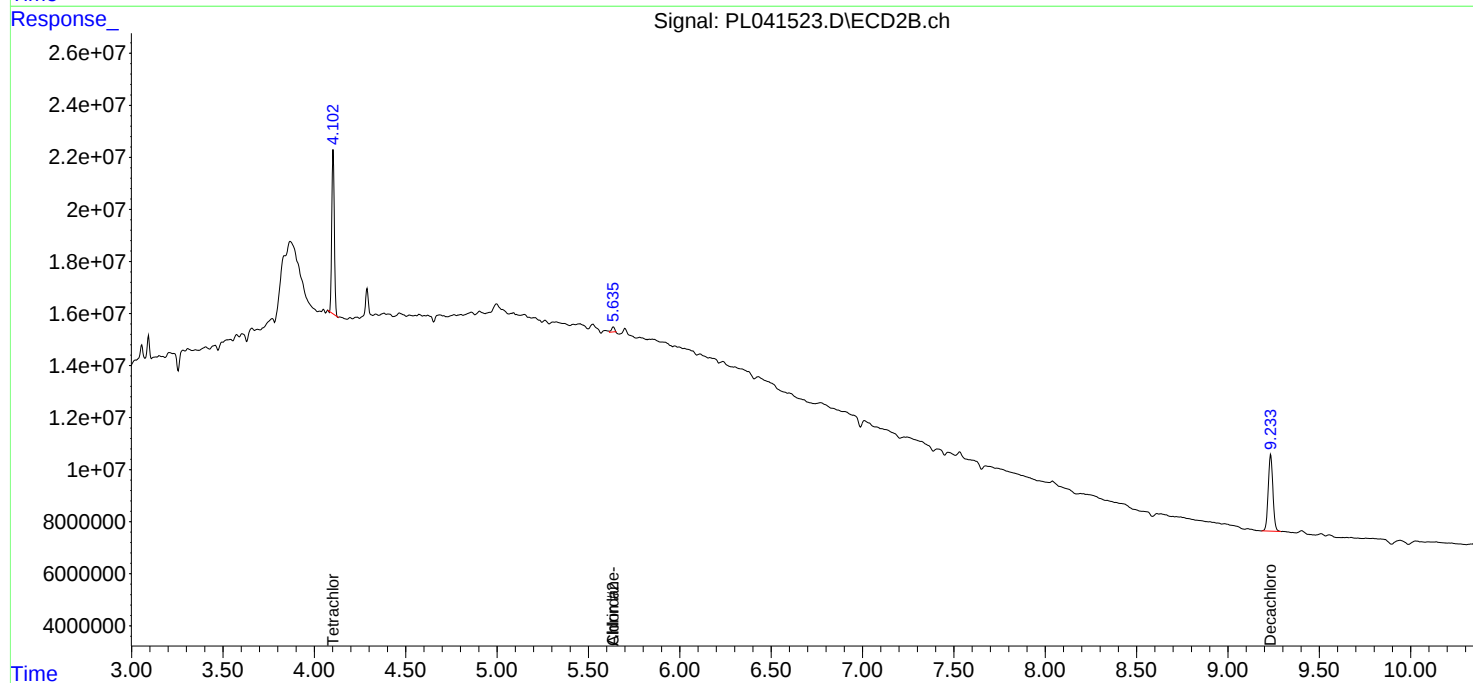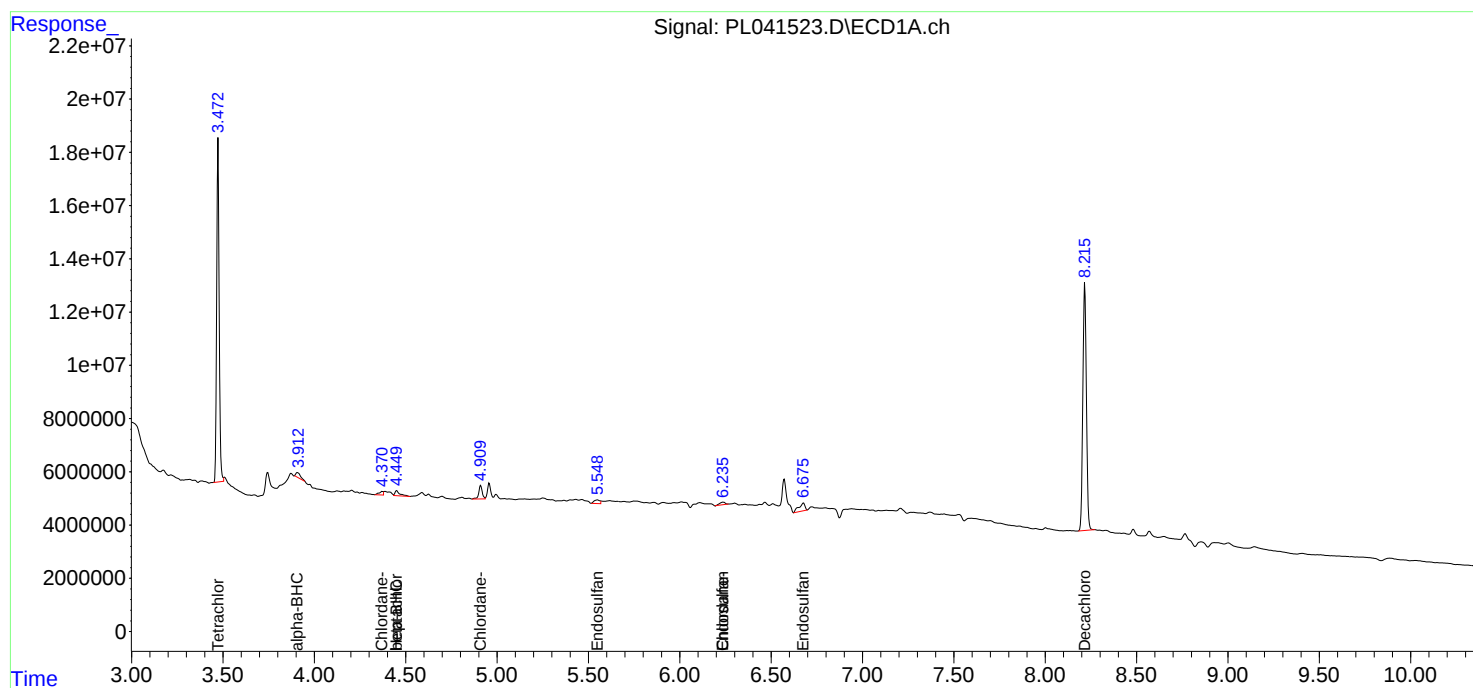


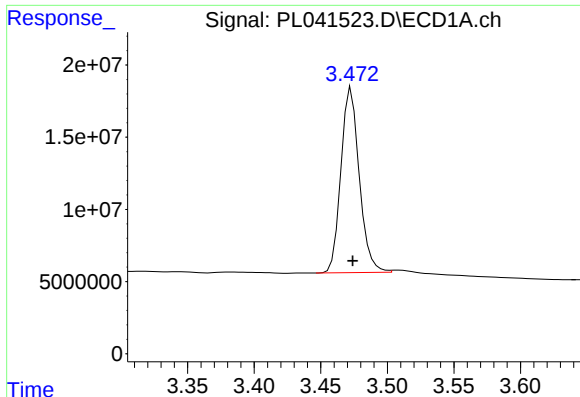

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 122755476
Conc: 19.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

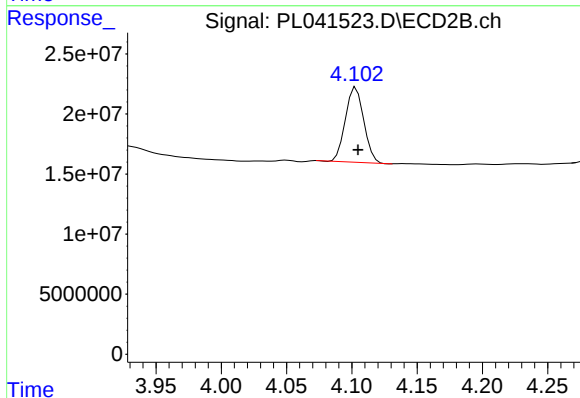


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.001 min
Response: 61239651
Conc: 19.88 ng/ml

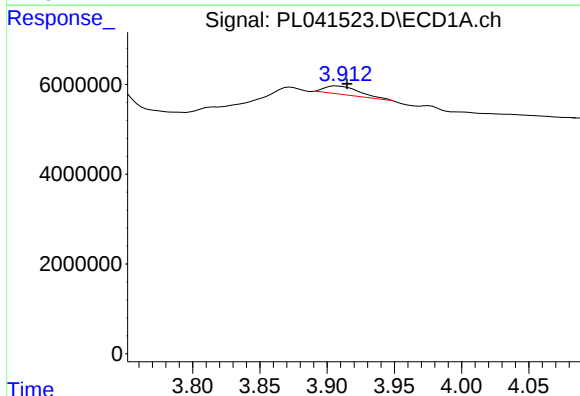


#2 alpha-BHC

R.T.: 3.907 min
Delta R.T.: -0.008 min
Response: 3072989
Conc: 0.32 ng/ml

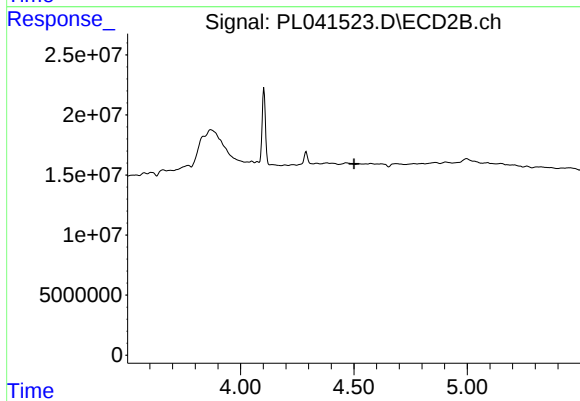

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.501 min
Response: 0
Conc: N.D.

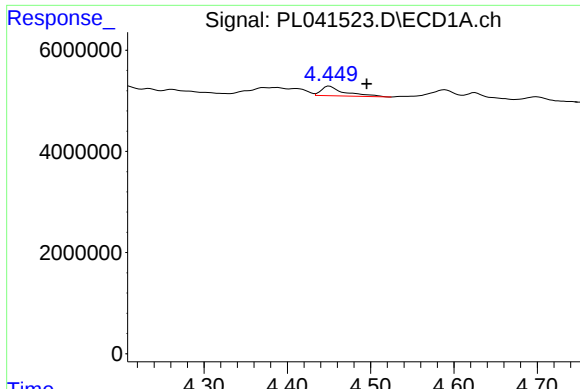

#4 Heptachlor


R.T.: 4.451 min
Delta R.T.: -0.044 min
Response: 3655866
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

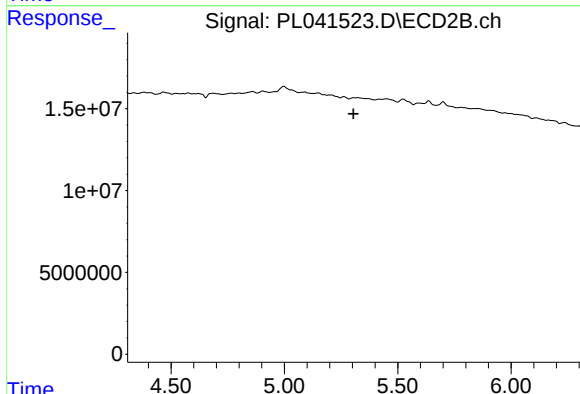


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.305 min
Response: 0
Conc: N.D.

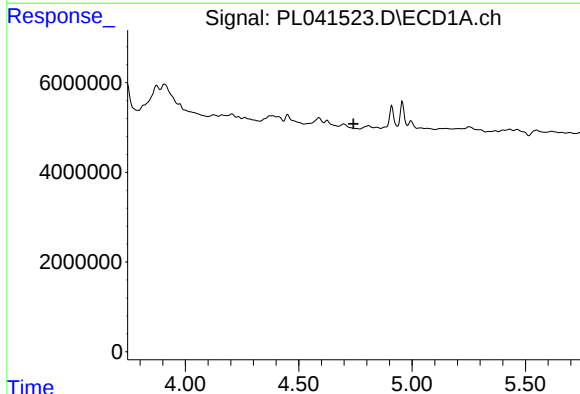


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.742 min
Response: 0
Conc: N.D.

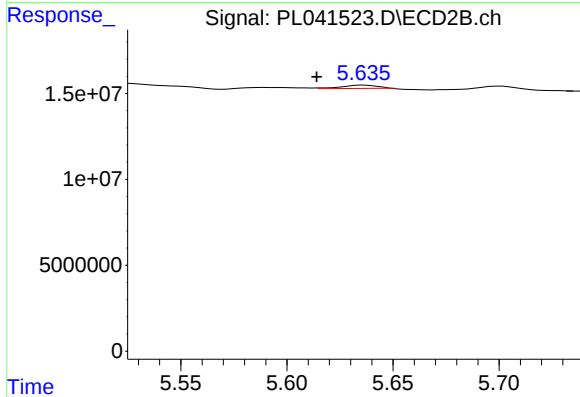

#5 Aldrin


R.T.: 5.637 min
Delta R.T.: 0.023 min
Response: 2051802
Conc: 0.54 ng/ml

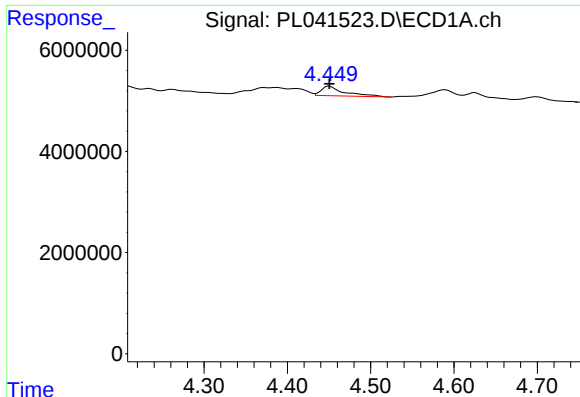

#6 beta-BHC


R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3655866
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

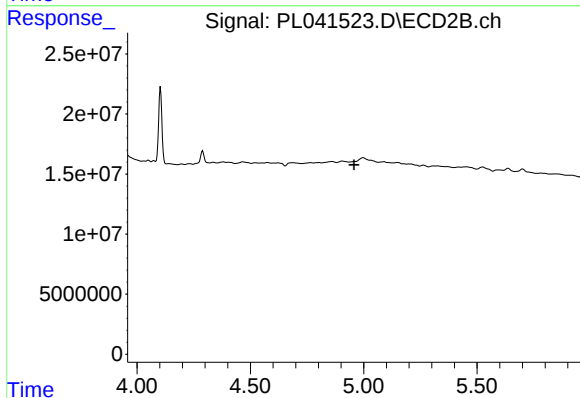


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

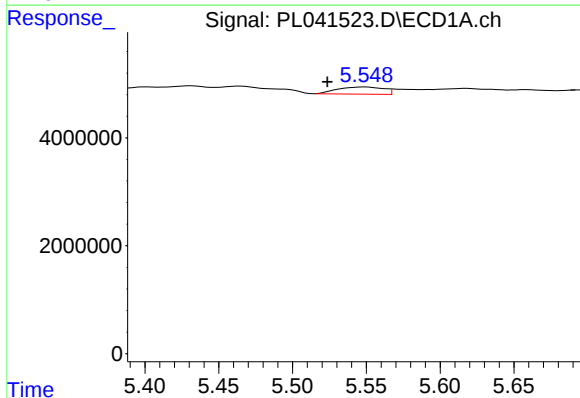


#9 Endosulfan I

R.T.: 5.550 min
Delta R.T.: 0.026 min
Response: 2799308
Conc: 0.38 ng/ml

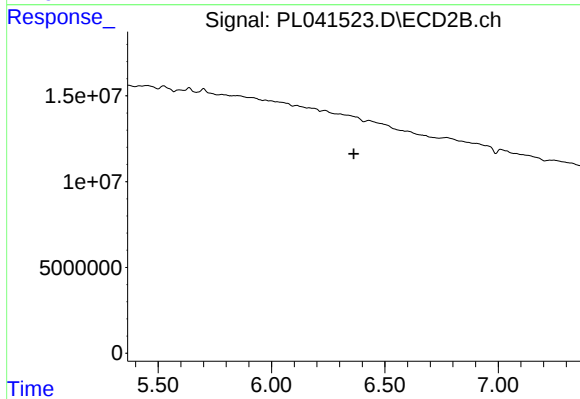

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

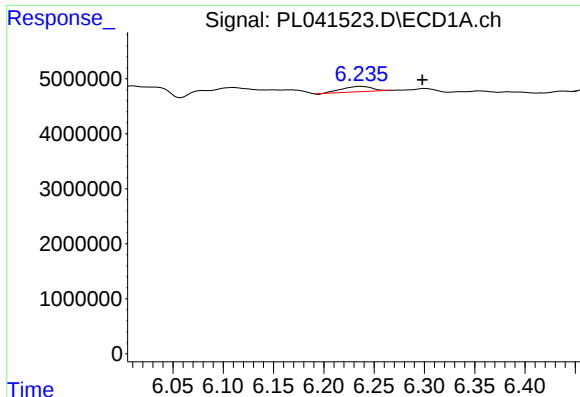

#15 Endosulfan II


R.T.: 6.237 min
Delta R.T.: -0.061 min
Response: 1929512
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

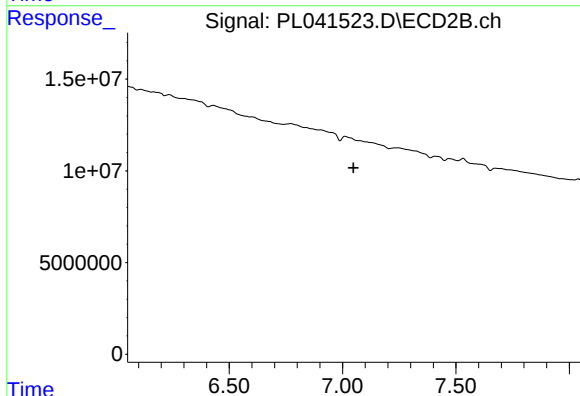


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

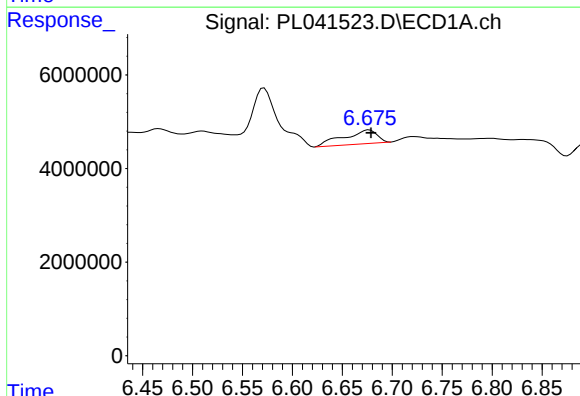


#19 Endosulfan Sulfate

R.T.: 6.677 min
Delta R.T.: -0.002 min
Response: 6808132
Conc: 1.07 ng/ml

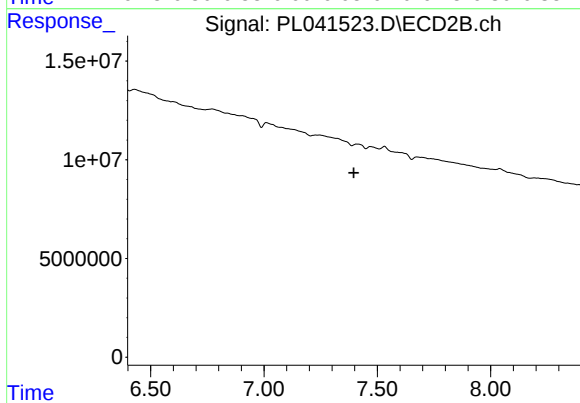

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.396 min
Response: 0
Conc: N.D.

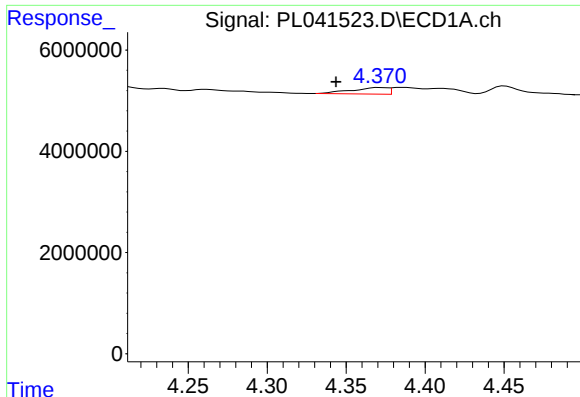

#23 Chlordane-1


R.T.: 4.371 min
Delta R.T.: 0.028 min
Response: 2082463
Conc: 7.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

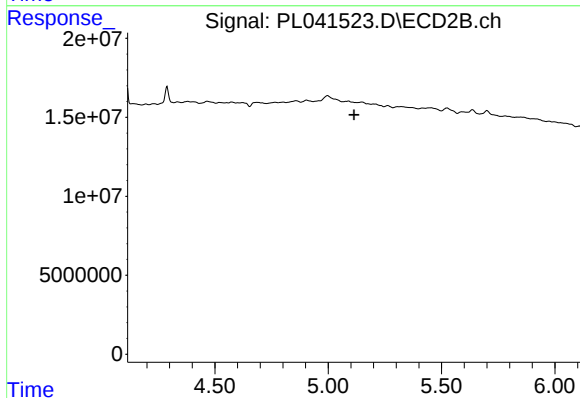


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

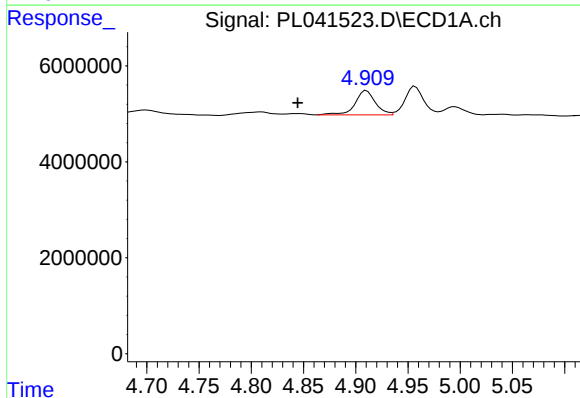


#24 Chlordane-2

R.T.: 4.910 min
Delta R.T.: 0.066 min
Response: 6840396
Conc: 23.23 ng/ml

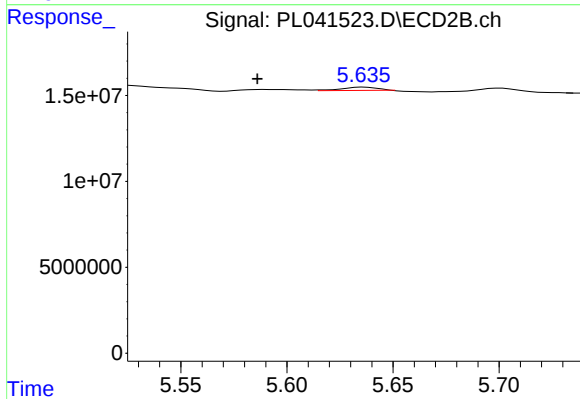

#24 Chlordane-2


R.T.: 5.637 min
Delta R.T.: 0.051 min
Response: 2051802
Conc: 15.44 ng/ml

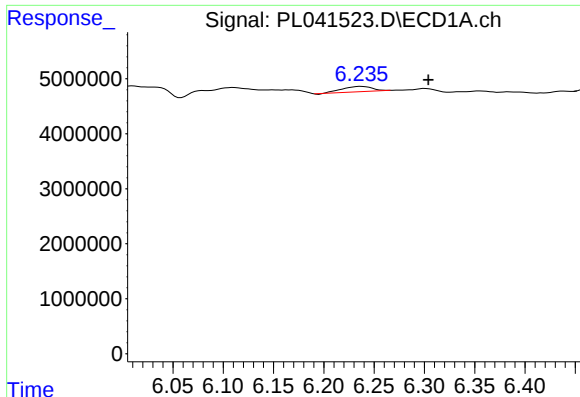

#27 Chlordane-5


R.T.: 6.237 min
Delta R.T.: -0.067 min
Response: 1929512
Conc: 7.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

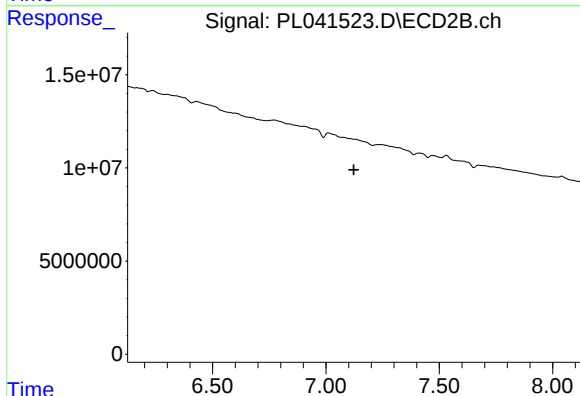


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.123 min
Response: 0
Conc: N.D.

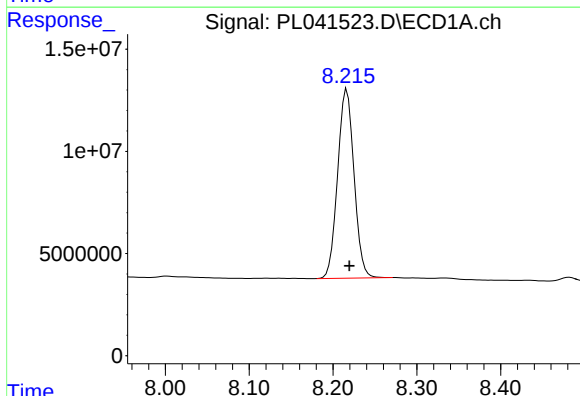

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 125716902
Conc: 18.98 ng/ml

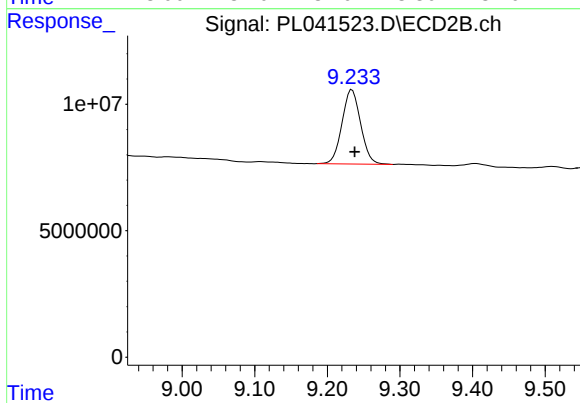

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.004 min
Response: 52355864
Conc: 20.43 ng/ml