

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103019\
 Data File : PL053929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 18:31
 Operator : SG\AJ
 Sample : K5599-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 Z3-23B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 00:45:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.044	224.3E6	54252229	20.690	21.680
28)	SA Decachlor...	8.326	9.122	178.0E6	54269912	18.140	19.272
Target Compounds							
8)	B Heptachlo...	0.000	5.931	0	1279851	N.D.	0.439 #
12)	B 4,4'-DDE	5.725	6.384	6818911	1148567	0.574	0.408 #
15)	B Endosulfa...	0.000	6.973	0	6503222	N.D.	2.546 #
16)	A 4,4'-DDD	6.244	0.000	4255525	0	0.478	N.D. #
17)	MA 4,4'-DDT	6.484	7.174	4924585	11909617	0.497	5.150 #
23)	Chlordane-1	4.447f	0.000	4557930	0	12.851	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103019\
Data File : PL053929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 18:31
Operator : SG\AJ
Sample : K5599-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
Z3-23B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 00:45:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

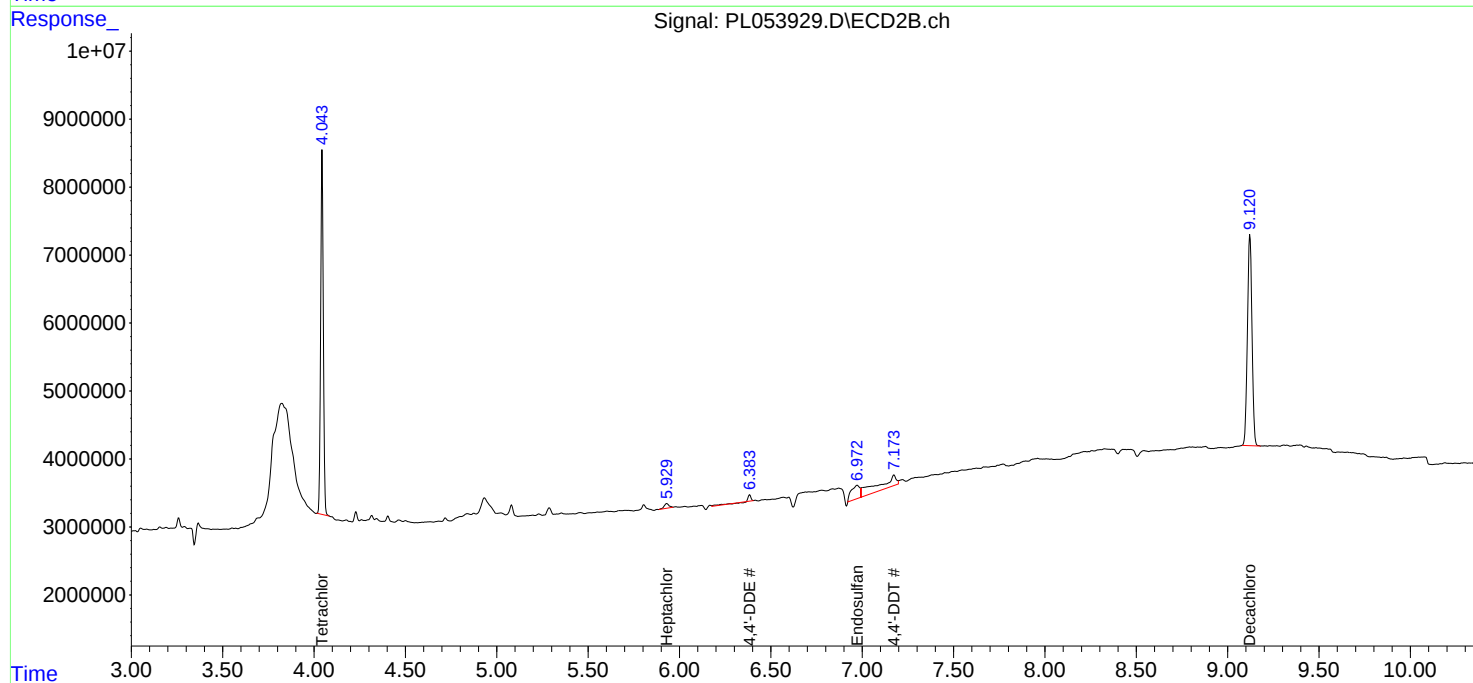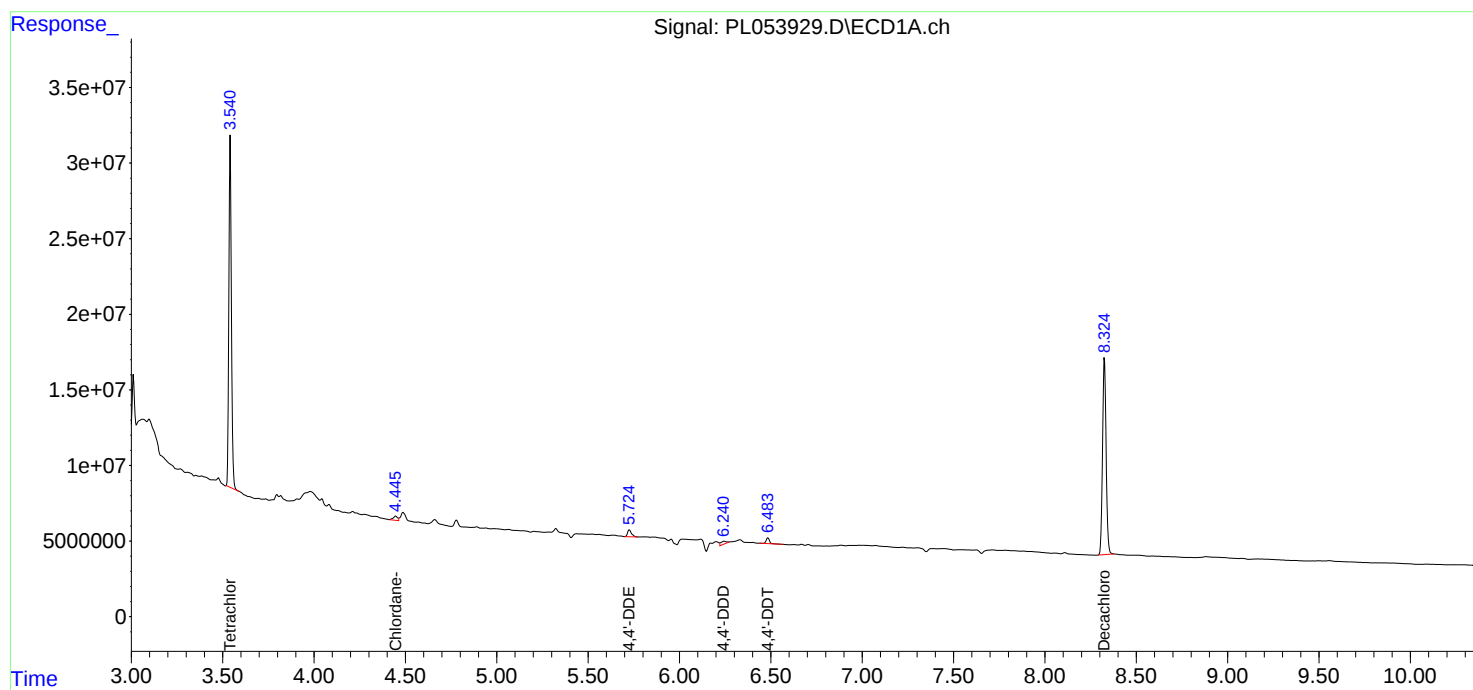


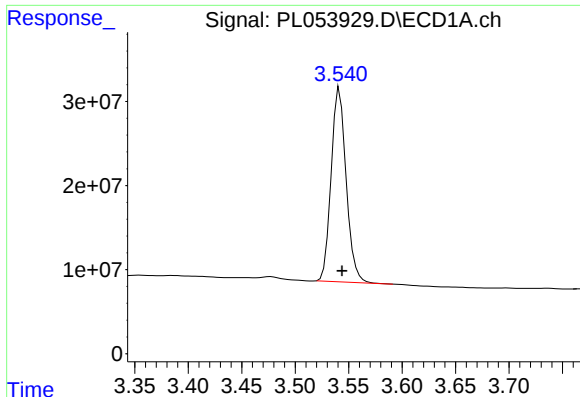

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 224267937
Conc: 20.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z3-23B

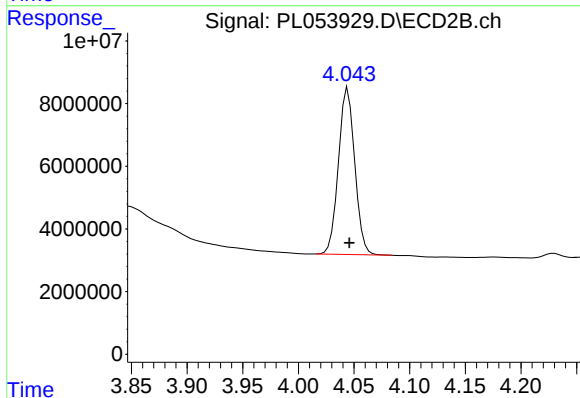


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 54252229
Conc: 21.68 ng/ml

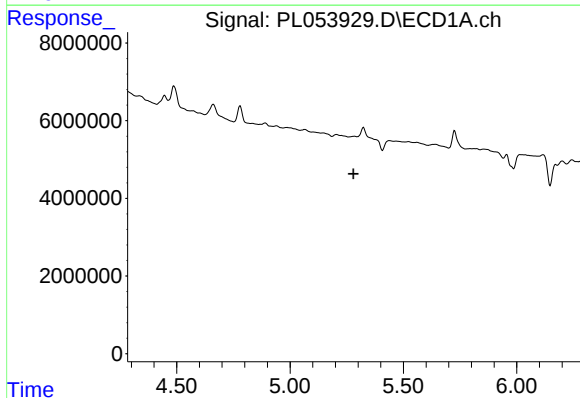


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

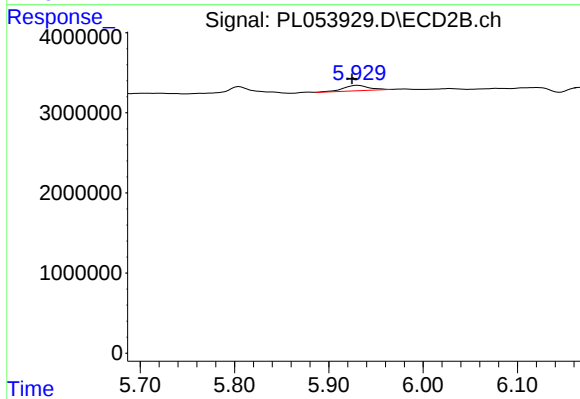

#8 Heptachlor epoxide


R.T.: 5.931 min
Delta R.T.: 0.006 min
Response: 1279851
Conc: 0.44 ng/ml

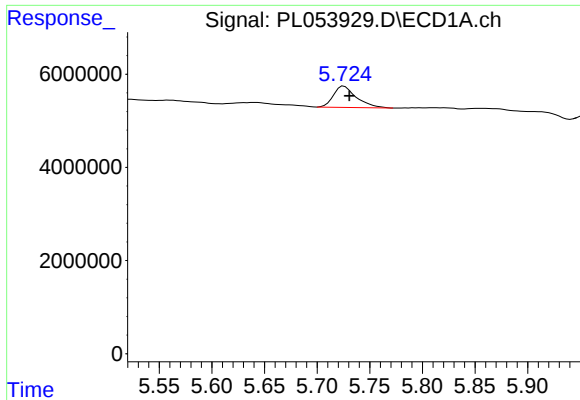

#12 4,4'-DDE


R.T.: 5.725 min
Delta R.T.: -0.005 min
Response: 6818911
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z3-23B

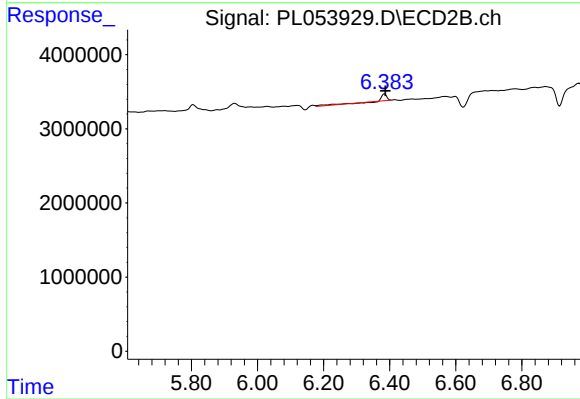


#12 4,4'-DDE

R.T.: 6.384 min
Delta R.T.: -0.003 min
Response: 1148567
Conc: 0.41 ng/ml

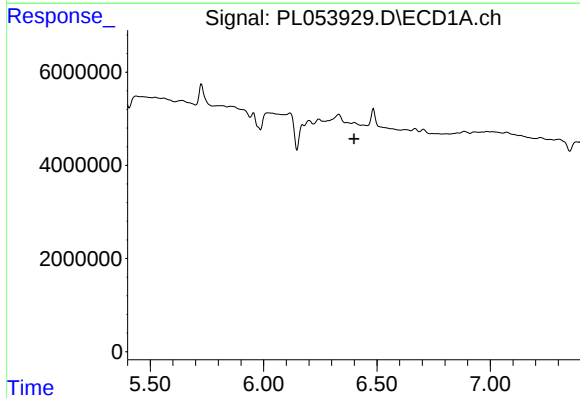


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

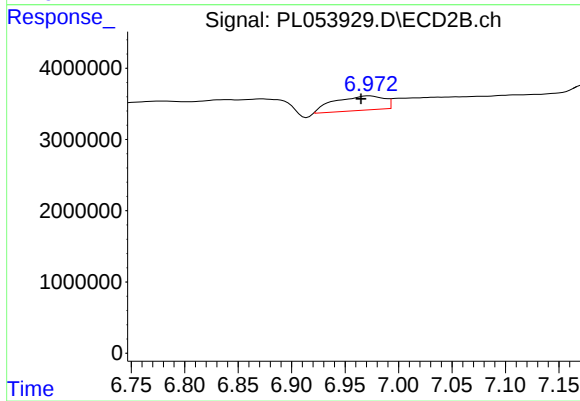

#15 Endosulfan II


R.T.: 6.973 min
Delta R.T.: 0.008 min
Response: 6503222
Conc: 2.55 ng/ml

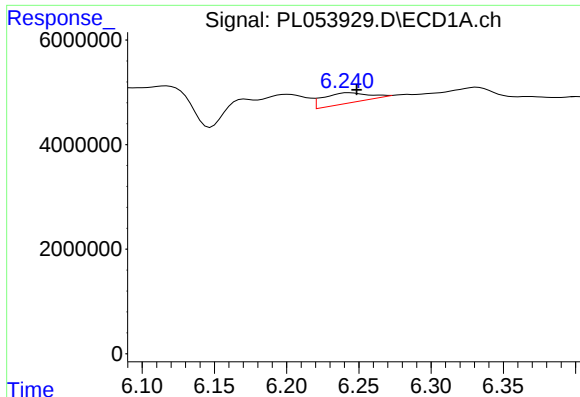

#16 4,4'-DDD


R.T.: 6.244 min
Delta R.T.: -0.005 min
Response: 4255525
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z3-23B

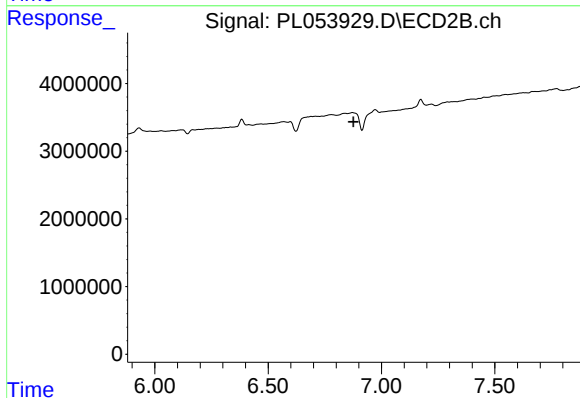


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.877 min
Response: 0
Conc: N.D.

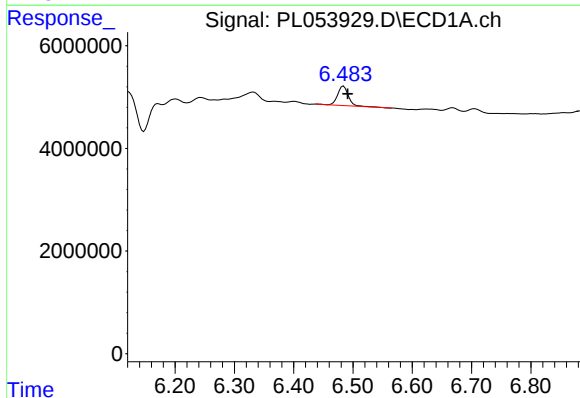


#17 4,4'-DDT

R.T.: 6.484 min
Delta R.T.: -0.007 min
Response: 4924585
Conc: 0.50 ng/ml

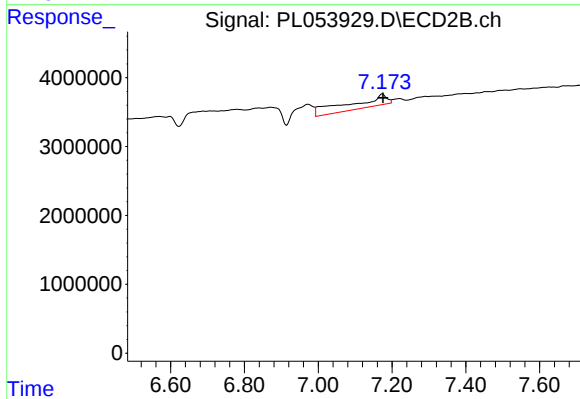

#17 4,4'-DDT


R.T.: 7.174 min
Delta R.T.: -0.002 min
Response: 11909617
Conc: 5.15 ng/ml

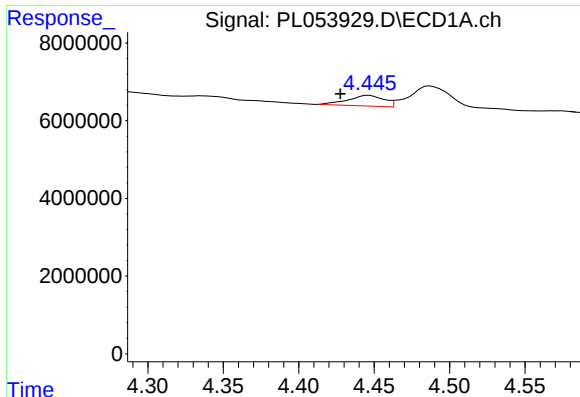

#23 Chlordane-1


R.T.: 4.447 min
Delta R.T.: 0.019 min
Response: 4557930
Conc: 12.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z3-23B

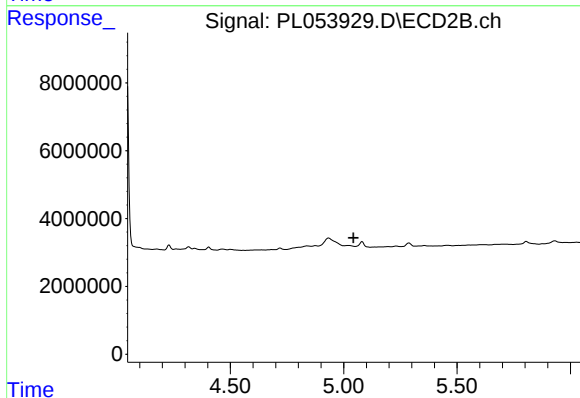


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.043 min
Response: 0
Conc: N.D.

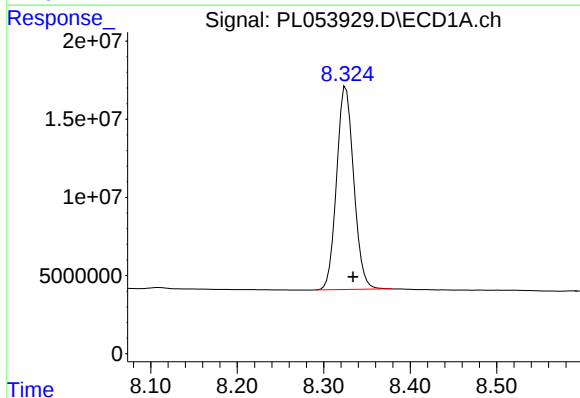

#28 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.008 min
Response: 177979072
Conc: 18.14 ng/ml

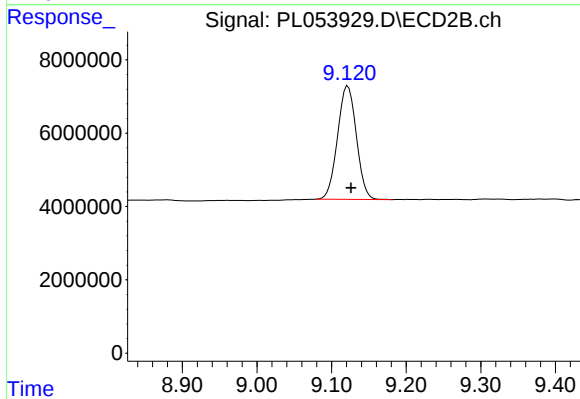

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 54269912
Conc: 19.27 ng/ml