

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103019\
 Data File : PL053938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 20:37
 Operator : SG\AJ
 Sample : K5603-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190949-AMND-COMPOSITE-KM-

Manual Integrations
 APPROVED

Ankita
 10/31/2019 10:22:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 00:46:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.045	105.7E6	26672438	9.747	10.659
28)	SA Decachlor...	8.326	9.122	70102988	20192243	7.145	7.170
Target Compounds							
12)	B 4,4'-DDE	5.725	6.383	6945267	2839864	0.585	1.008m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103019\
Data File : PL053938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 20:37
Operator : SG\AJ
Sample : K5603-02
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20190949-AMND-COMPOSITE-KM-


Manual Integrations
APPROVED

Ankita
10/31/2019 10:22:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 00:46:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

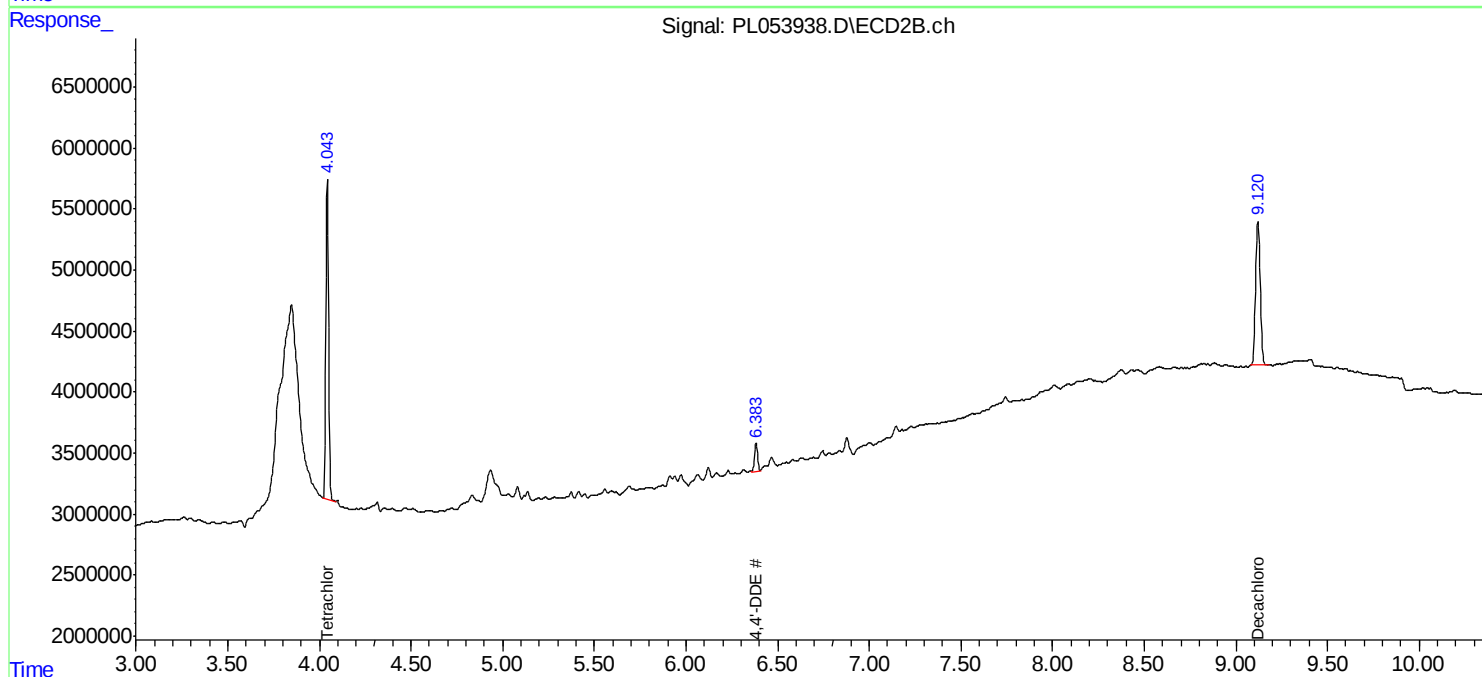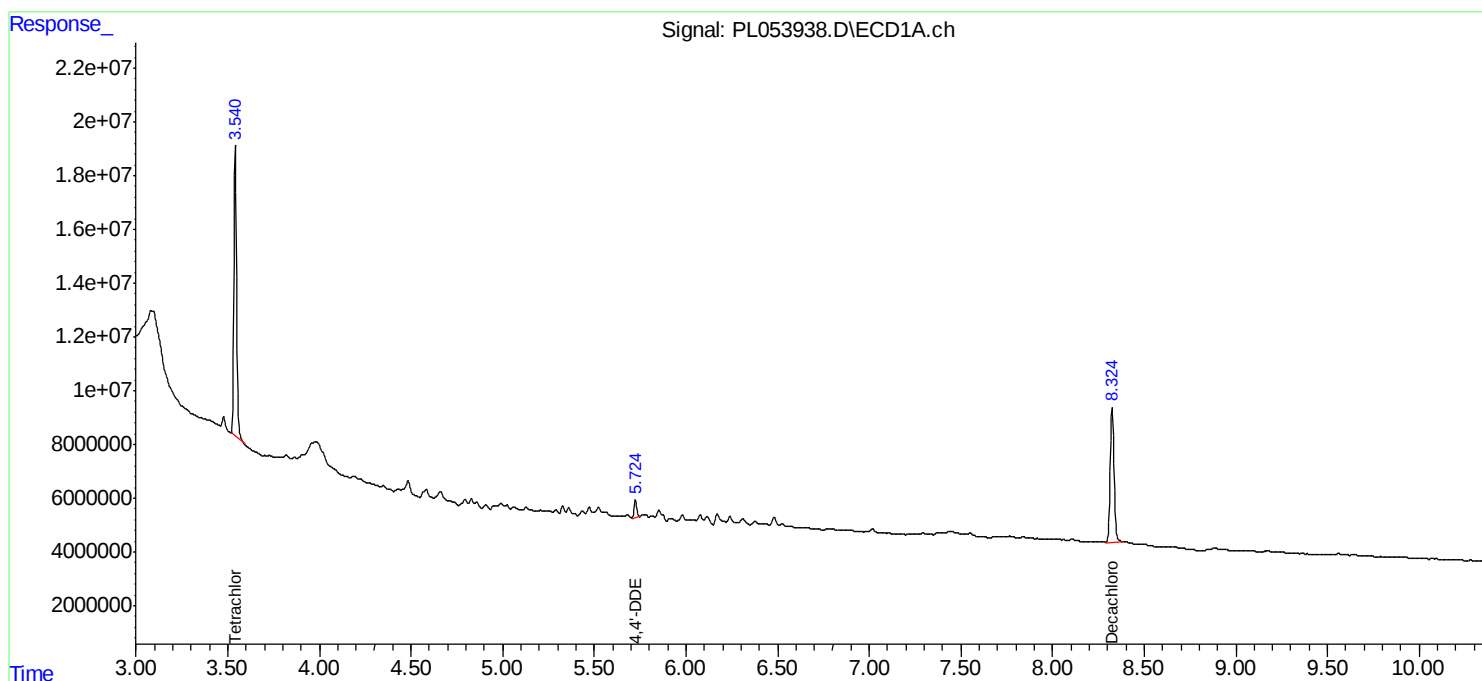

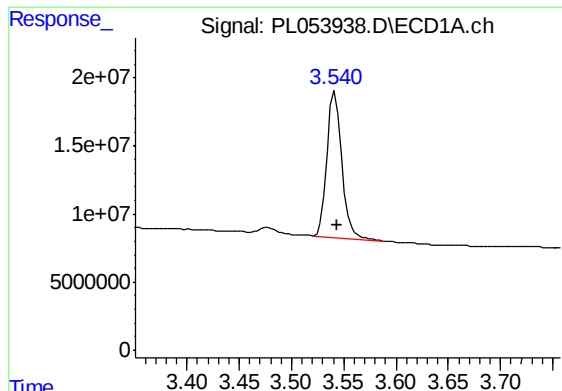


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 105651586
Conc: 9.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190949-AMND-COMPOSITE-KM-


Manual Integrations
APPROVED

Ankita
10/31/2019 10:22:20 AM

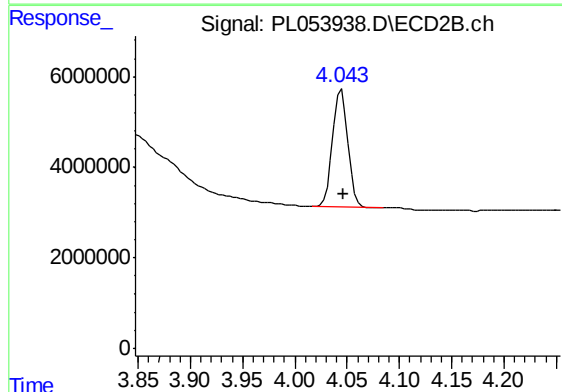


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 26672438
Conc: 10.66 ng/ml

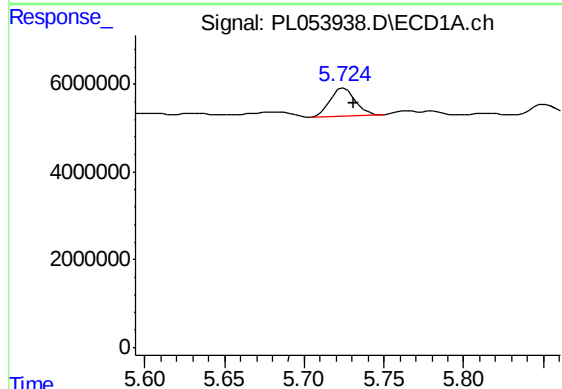


#12 4,4'-DDE

R.T.: 5.725 min
Delta R.T.: -0.006 min
Response: 6945267
Conc: 0.58 ng/ml

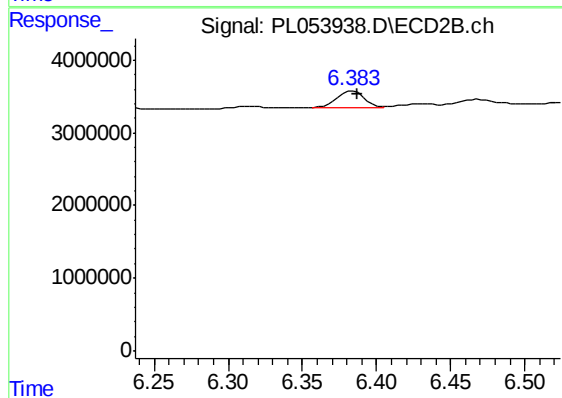

#12 4,4'-DDE

R.T.: 6.383 min
Delta R.T.: -0.004 min
Response: 2839864
Conc: 1.01 ng/ml m

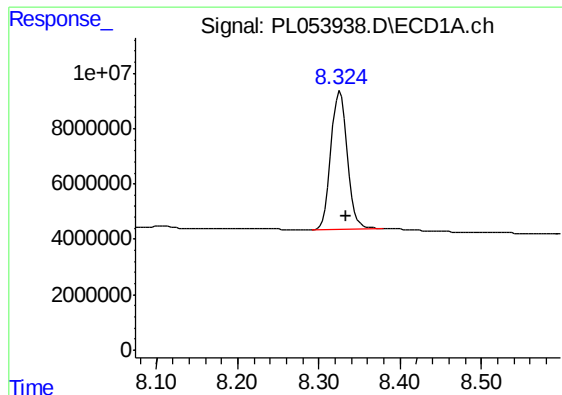


#28 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.008 min
Response: 70102988
Conc: 7.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190949-AMND-COMPOSITE-KM-

Manual Integrations
APPROVED

Ankita
10/31/2019 10:22:20 AM

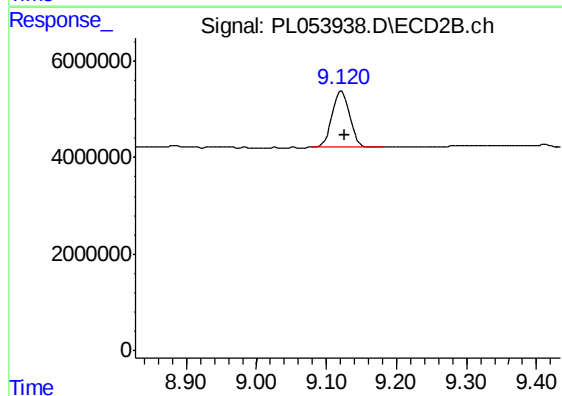

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 20192243
Conc: 7.17 ng/ml