

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 09:24
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 14:10:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	0.000	801579	0	0.466	N.D. #
Target Compounds							
16)	A 4,4'-DDD	6.070	0.000	3274134	0	2.315	N.D. #
17)	MA 4,4'-DDT	6.303	7.089f	6242013	8551495	4.677	3.809
18)	B Endrin al...	6.394f	0.000	4345107	0	2.992	N.D. #
20)	A Methoxychlor	6.858	0.000	572208	0	0.664	N.D. #
21)	B Endrin ke...	7.066	0.000	3509637	0	1.947	N.D. #
23)	Chlordane-1	4.258	0.000	626781	0	12.159	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 09:24
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 14:10:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

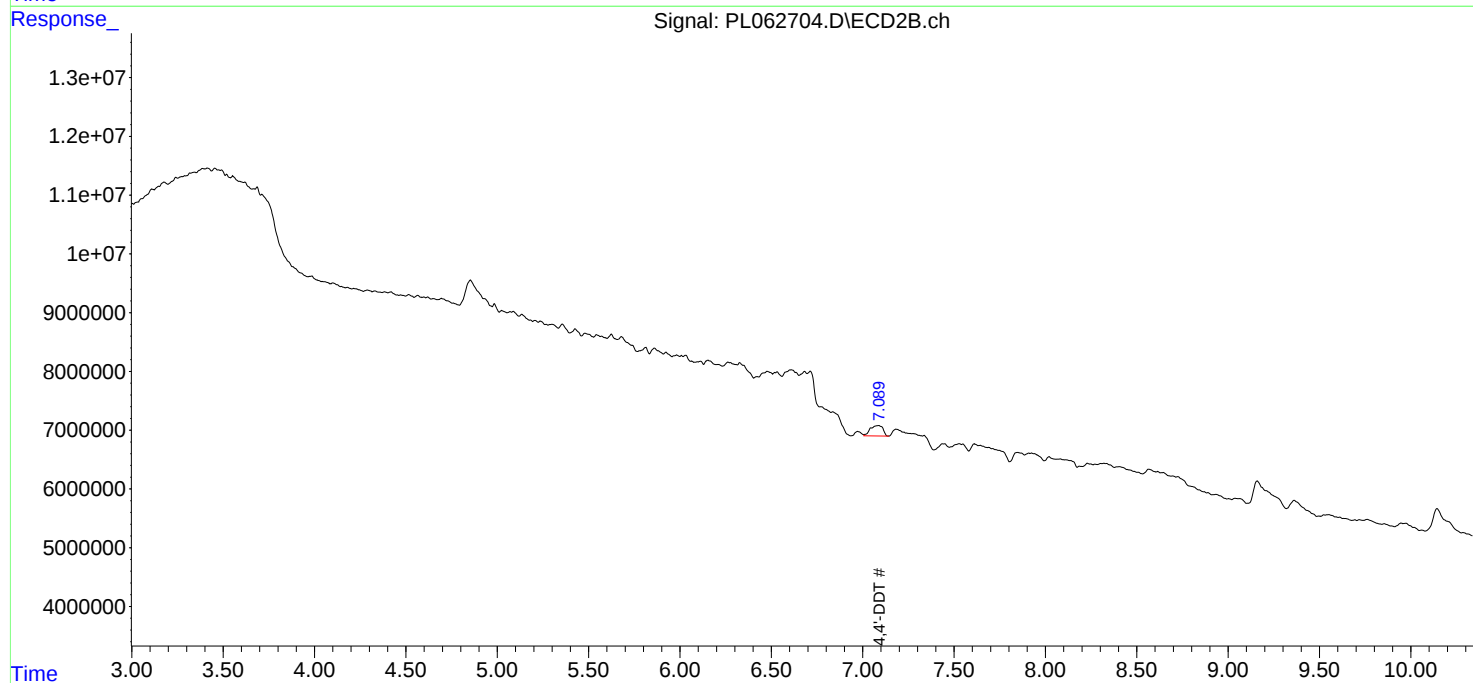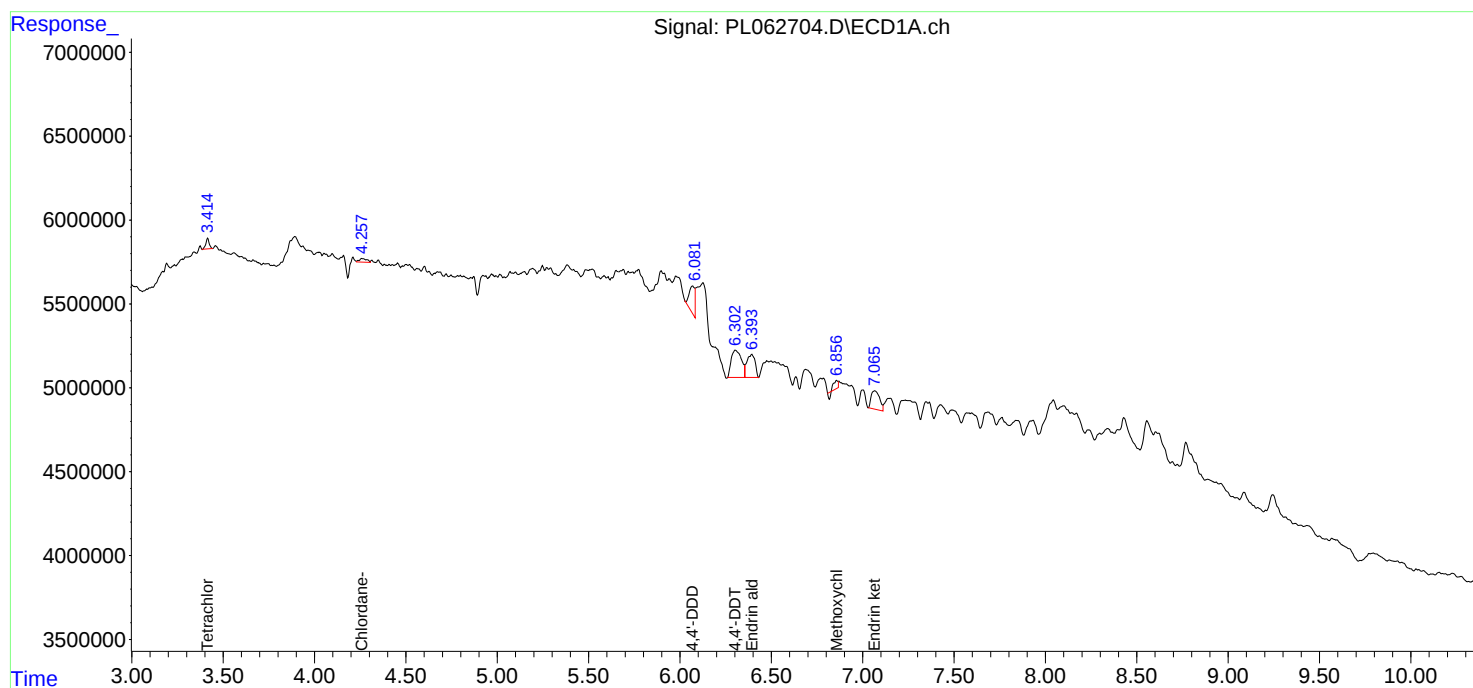


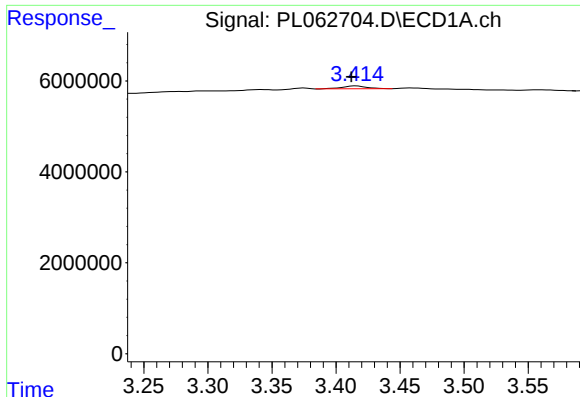

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.004 min
Response: 801579
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

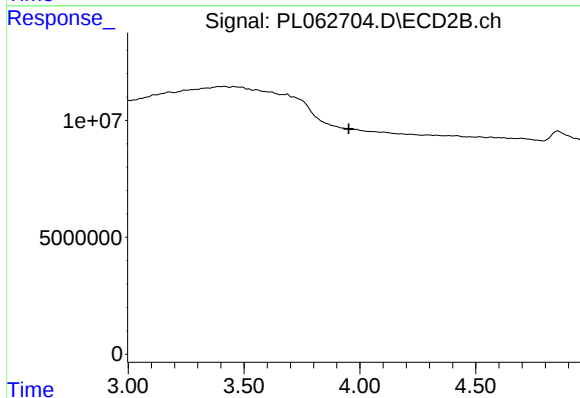


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

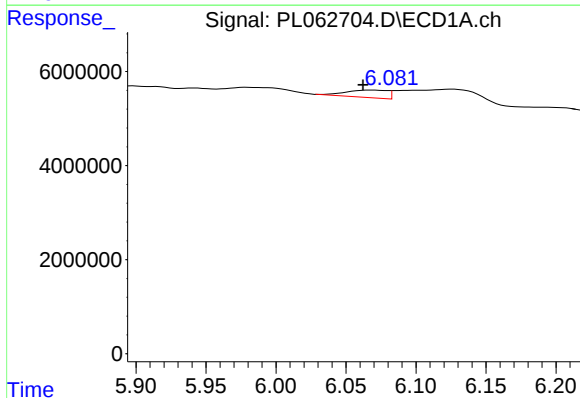


#16 4,4'-DDD

R.T.: 6.070 min
Delta R.T.: 0.007 min
Response: 3274134
Conc: 2.31 ng/ml

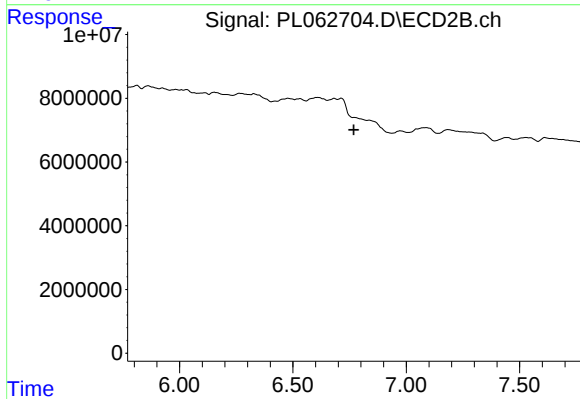

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

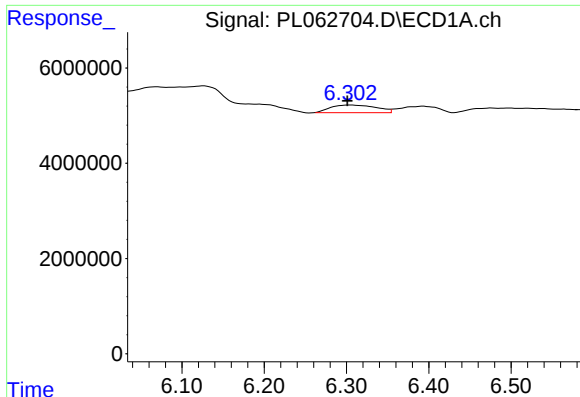

#17 4,4'-DDT


R.T.: 6.303 min
Delta R.T.: 0.002 min
Response: 6242013
Conc: 4.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

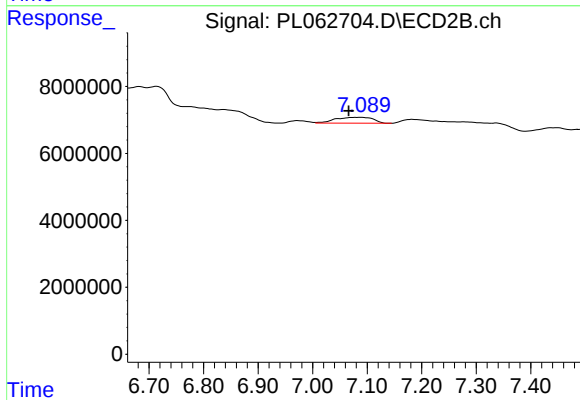


#17 4,4'-DDT

R.T.: 7.089 min
Delta R.T.: 0.023 min
Response: 8551495
Conc: 3.81 ng/ml

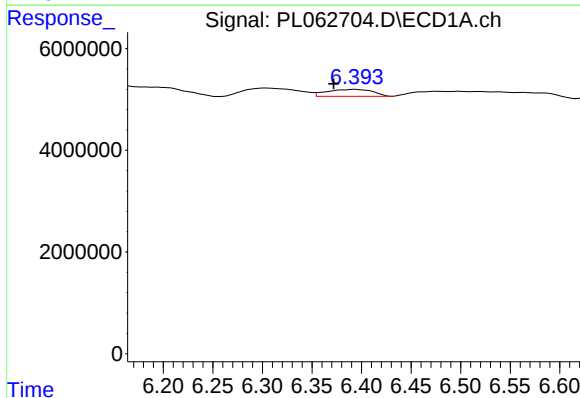


#18 Endrin aldehyde

R.T.: 6.394 min
Delta R.T.: 0.022 min
Response: 4345107
Conc: 2.99 ng/ml

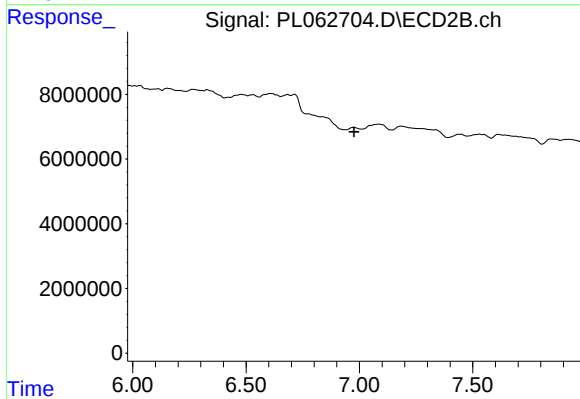

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.976 min
Response: 0
Conc: N.D.

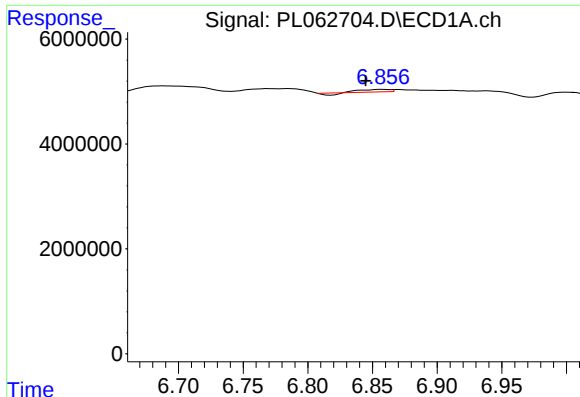

#20 Methoxychlor


R.T.: 6.858 min
Delta R.T.: 0.013 min
Response: 572208
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

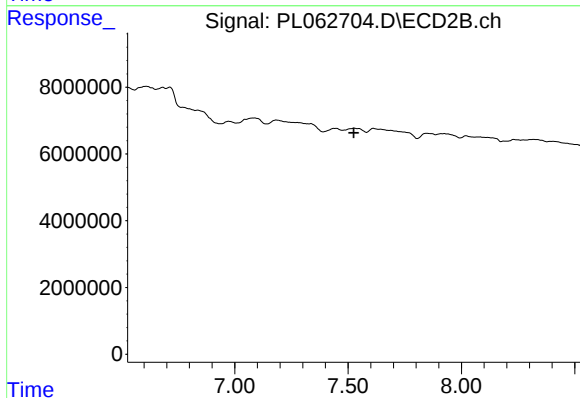


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

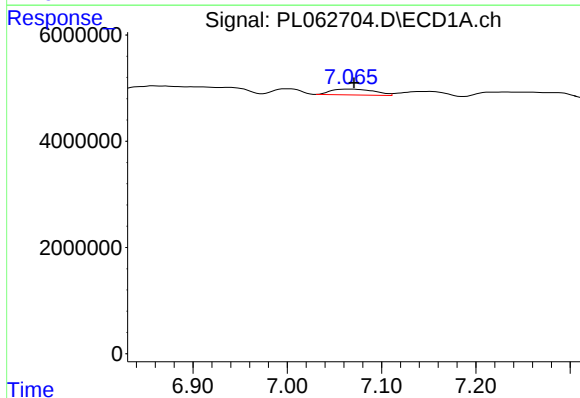


#21 Endrin ketone

R.T.: 7.066 min
Delta R.T.: -0.005 min
Response: 3509637
Conc: 1.95 ng/ml

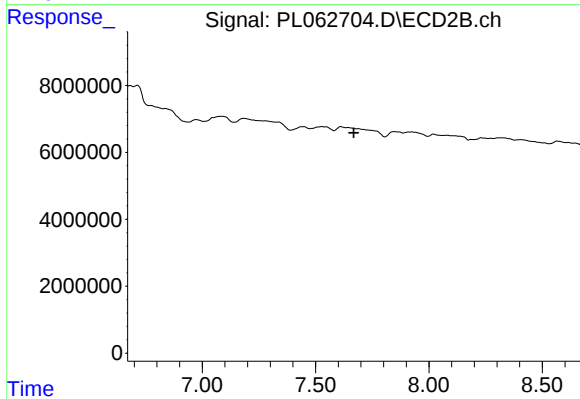

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

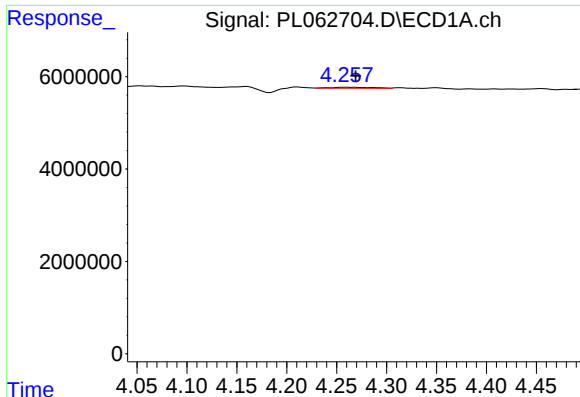

#23 Chlordane-1


R.T.: 4.258 min
Delta R.T.: -0.011 min
Response: 626781
Conc: 12.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

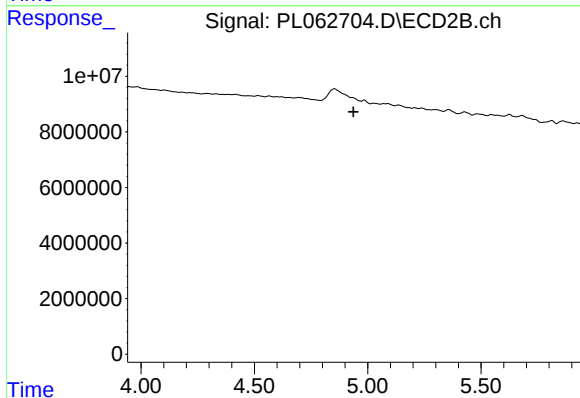


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

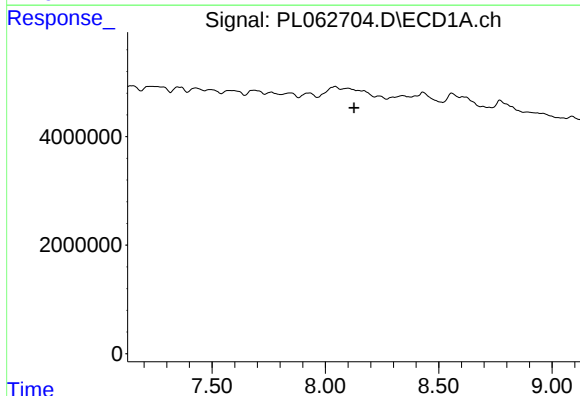

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

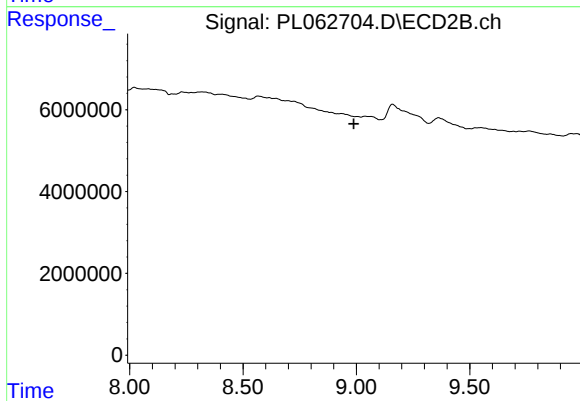

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.989 min
Response: 0
Conc: N.D.