

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 14:09
 Operator : DD\AJ
 Sample : L4215-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-102820

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 17:26:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	27247886	47671721	15.841	16.222
28)	SA Decachlor...	8.127	8.992	25121449	36165383	15.659	17.280
Target Compounds							
15)	B Endosulfa...	0.000	6.868f	0	2201153	N.D.	0.770 #
23)	Chlordane-1	4.299f	0.000	338097	0	6.559	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 14:09
Operator : DD\AJ
Sample : L4215-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 17:26:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

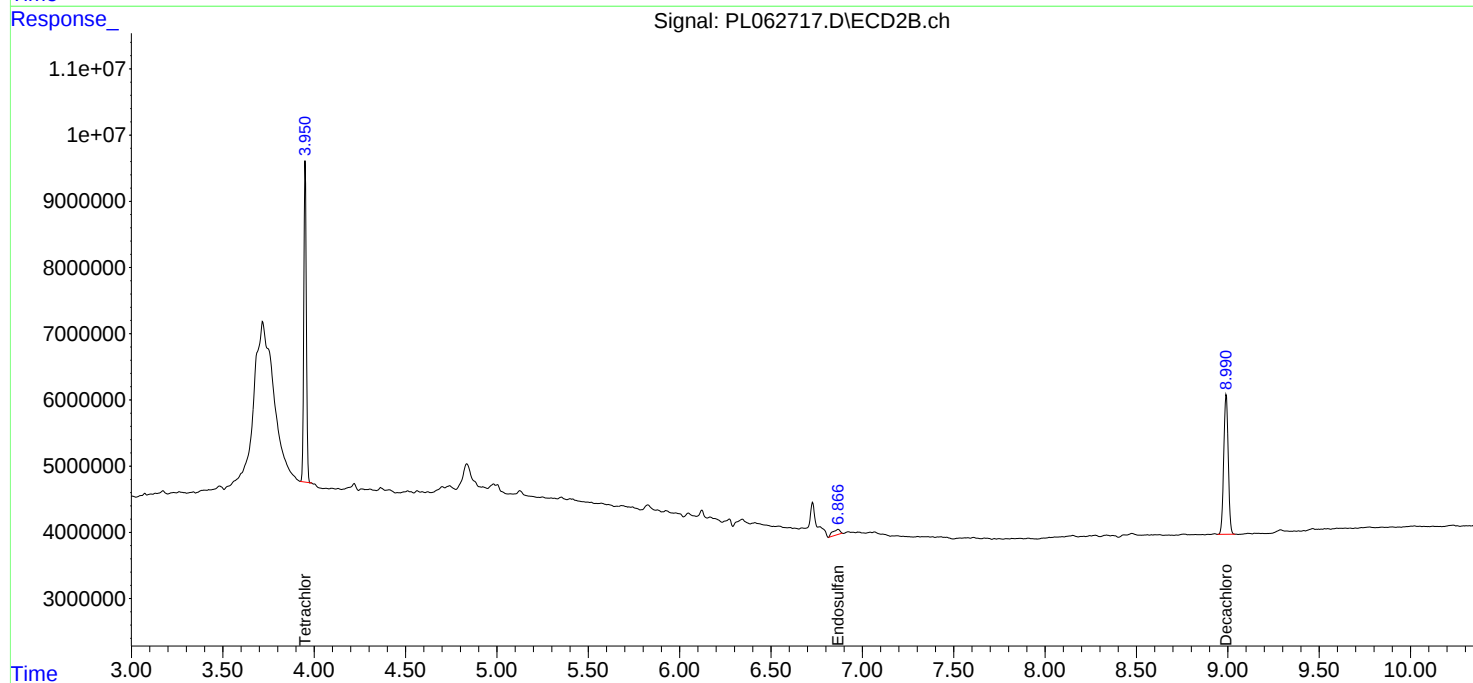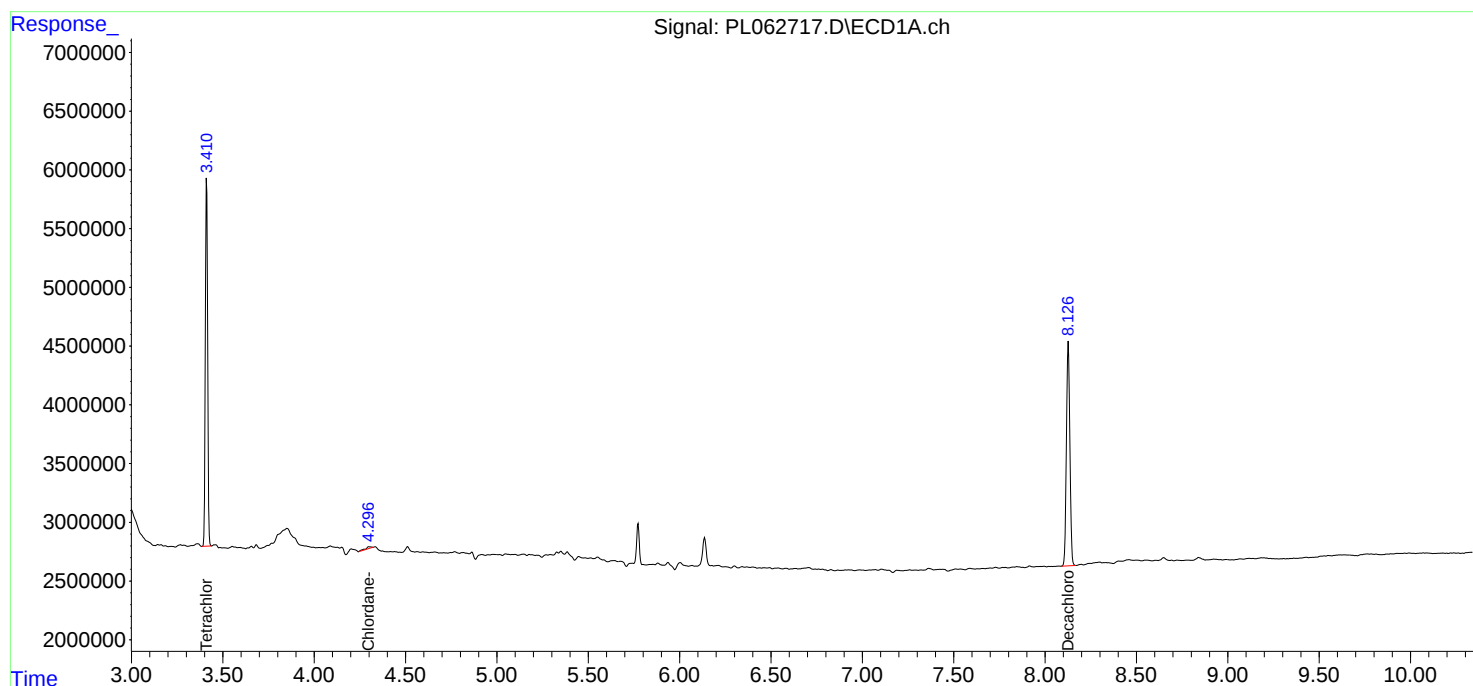


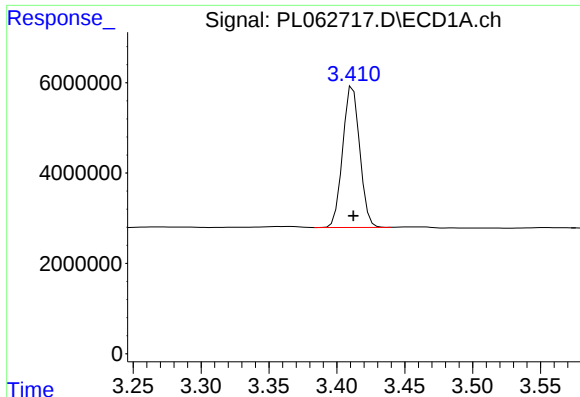

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 27247886
Conc: 15.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

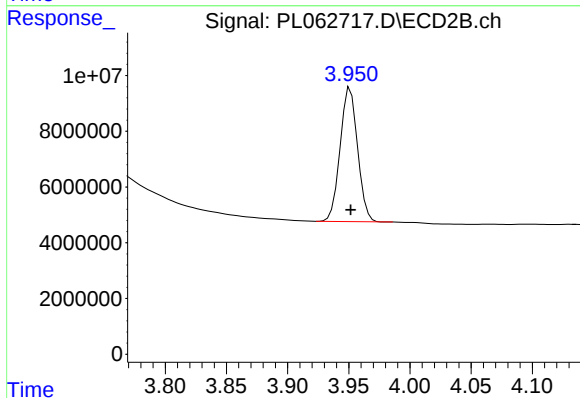


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 47671721
Conc: 16.22 ng/ml

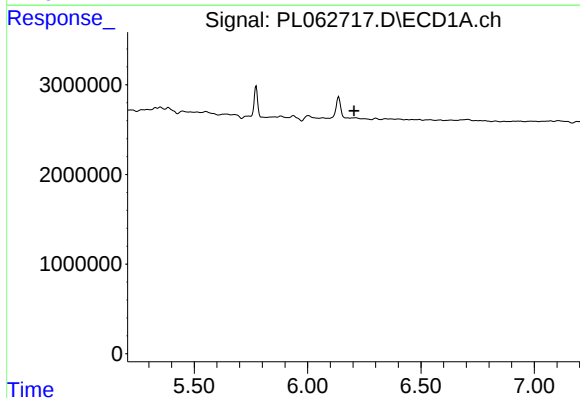


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

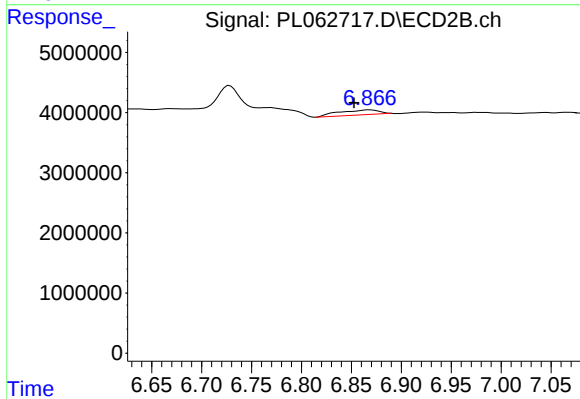

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 2201153
Conc: 0.77 ng/ml

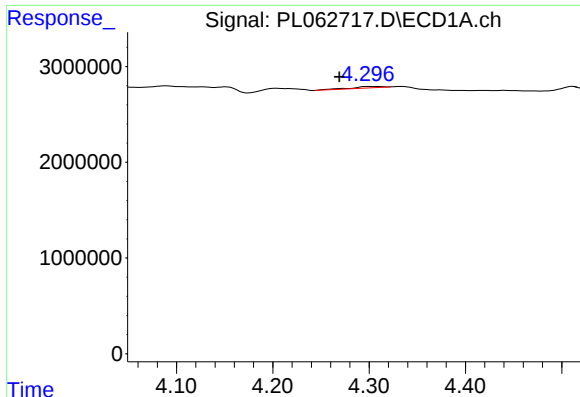

#23 Chlordane-1


R.T.: 4.299 min
Delta R.T.: 0.030 min
Response: 338097
Conc: 6.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

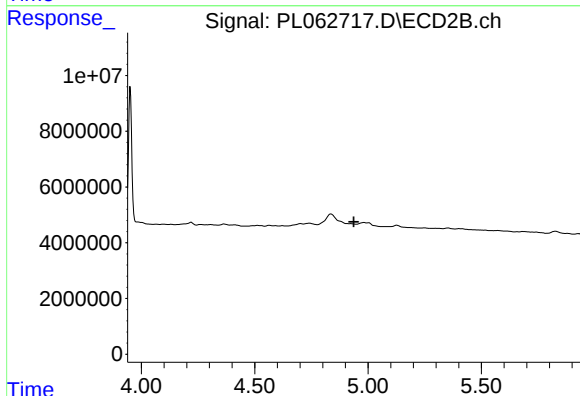


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

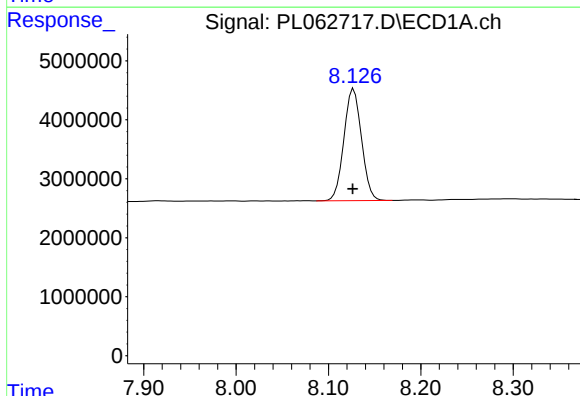

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.001 min
Response: 25121449
Conc: 15.66 ng/ml

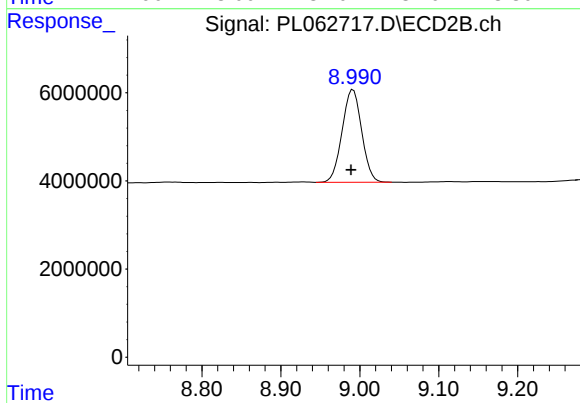

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 36165383
Conc: 17.28 ng/ml