

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 14:23
 Operator : DD\AJ
 Sample : L4222-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-102920

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 17:26:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	25673737	40680553	14.926	13.843
28)	SA Decachlor...	8.128	8.992	23851155	34082449	14.867	16.284
Target Compounds							
8)	B Heptachlo...	0.000	5.828	0	3826995	N.D.	1.182 #
10)	B gamma-Chl...	0.000	6.047	0	2697888	N.D.	0.801 #
11)	B alpha-Chl...	0.000	6.118	0	10808587	N.D.	3.208 #
12)	B 4,4'-DDE	5.551	6.272	923509	7988805	0.558	2.479 #
15)	B Endosulfa...	0.000	6.868f	0	2859065	N.D.	1.000 #
23)	Chlordane-1	4.262	0.000	1642885	0	31.870	N.D. #
25)	Chlordane-3	0.000	6.047	0	2697888	N.D.	6.679 #
26)	Chlordane-4	0.000	6.118	0	10808587	N.D.	22.319 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 14:23
Operator : DD\AJ
Sample : L4222-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-02-102920

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 17:26:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

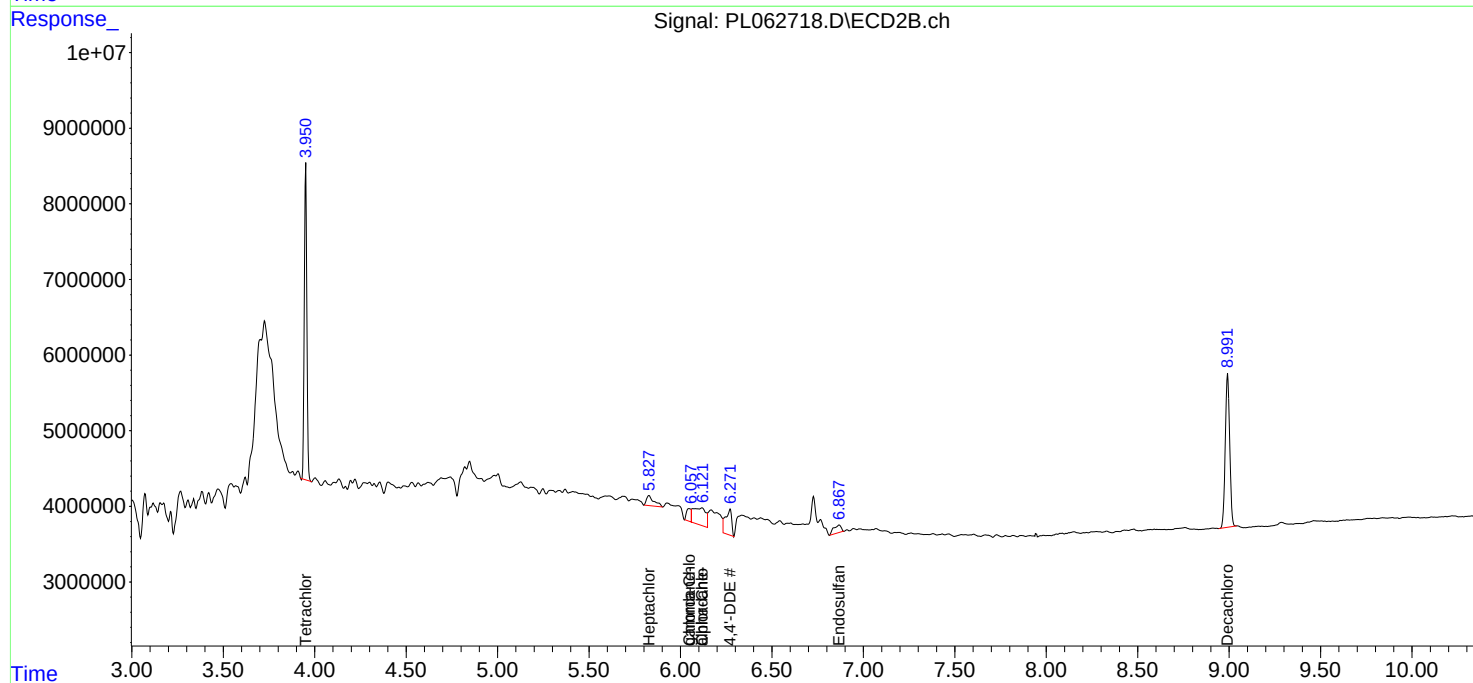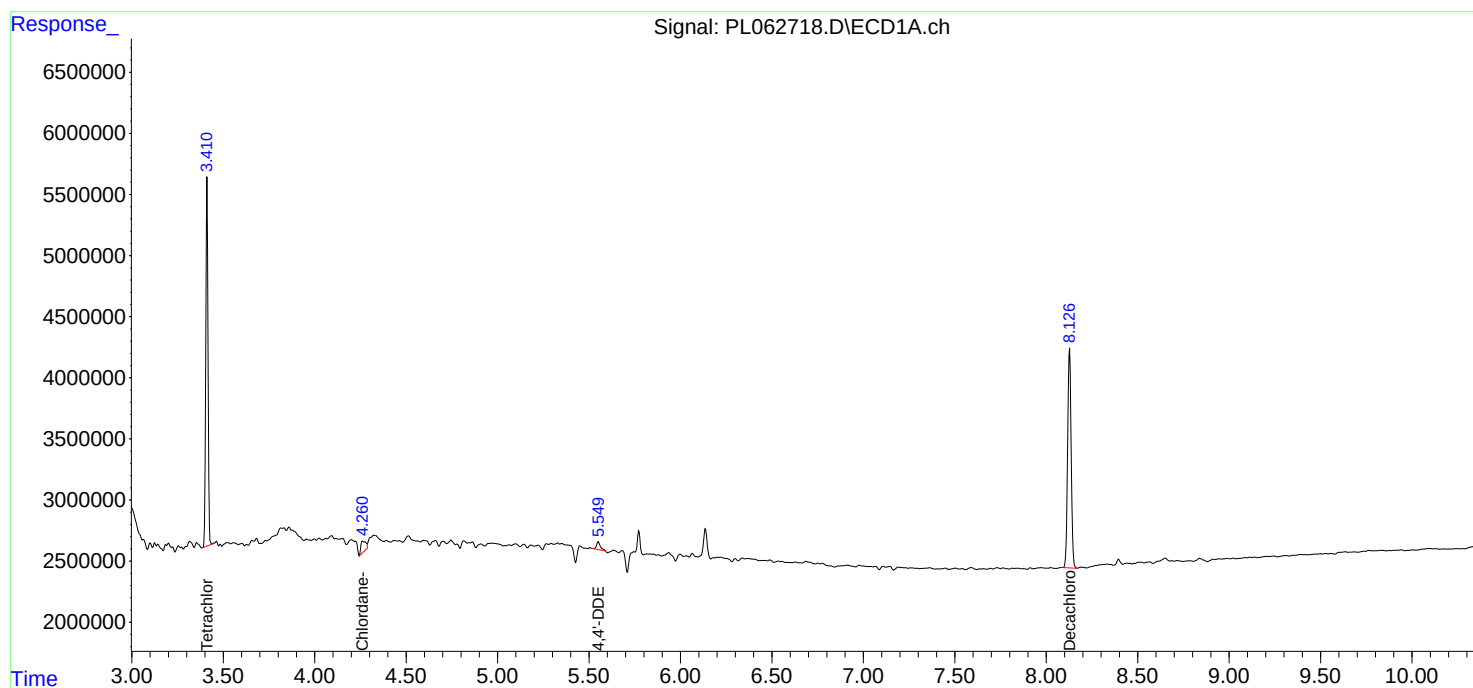


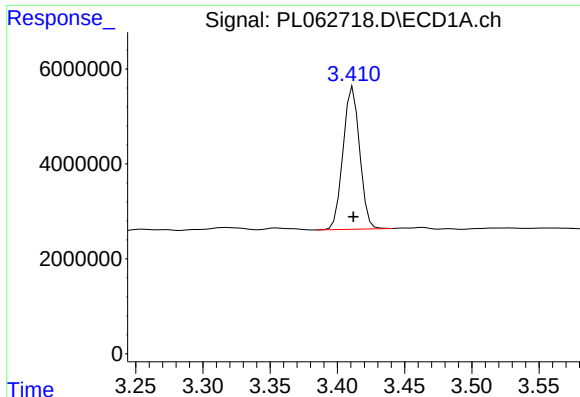

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 25673737
Conc: 14.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-102920

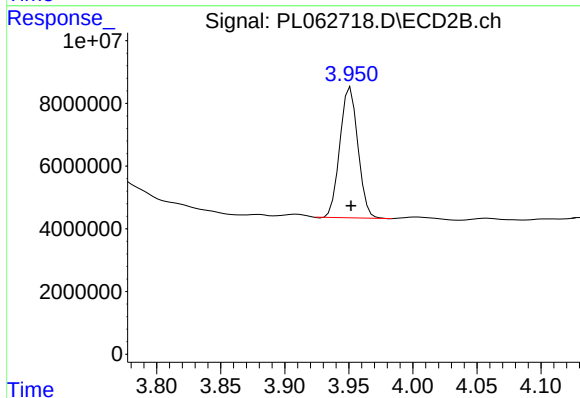


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 40680553
Conc: 13.84 ng/ml

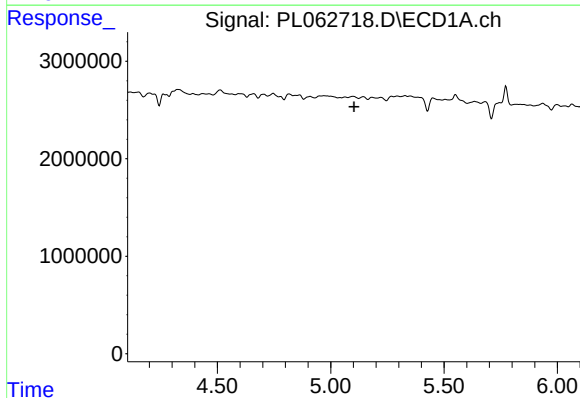


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

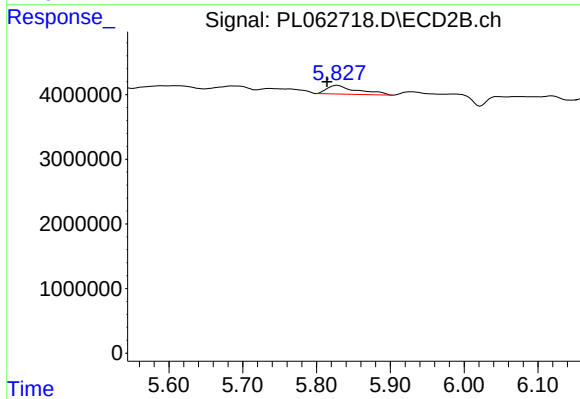

#8 Heptachlor epoxide


R.T.: 5.828 min
Delta R.T.: 0.014 min
Response: 3826995
Conc: 1.18 ng/ml

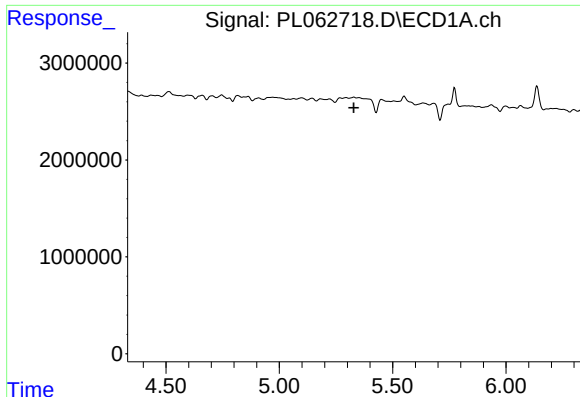

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-102920

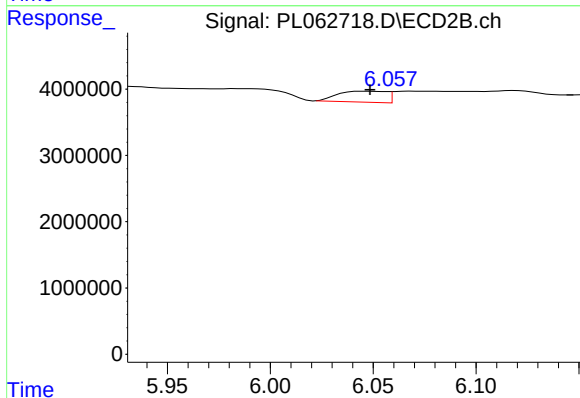


#10 gamma-Chlordane

R.T.: 6.047 min
Delta R.T.: -0.001 min
Response: 2697888
Conc: 0.80 ng/ml

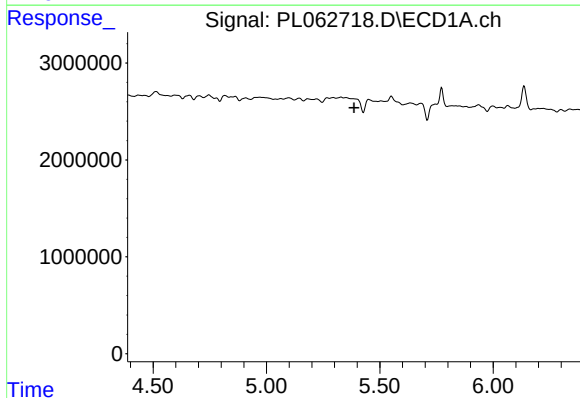


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.386 min
Response: 0
Conc: N.D.

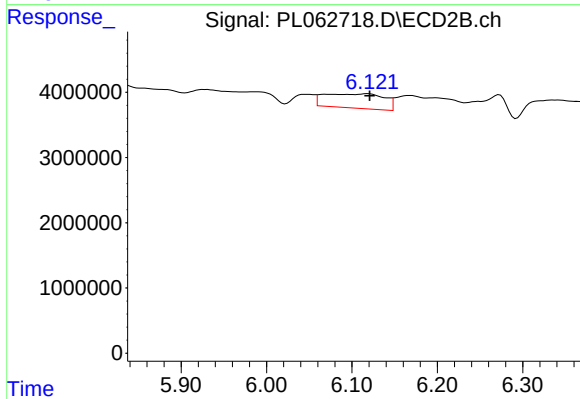

#11 alpha-Chlordane


R.T.: 6.118 min
Delta R.T.: -0.003 min
Response: 10808587
Conc: 3.21 ng/ml

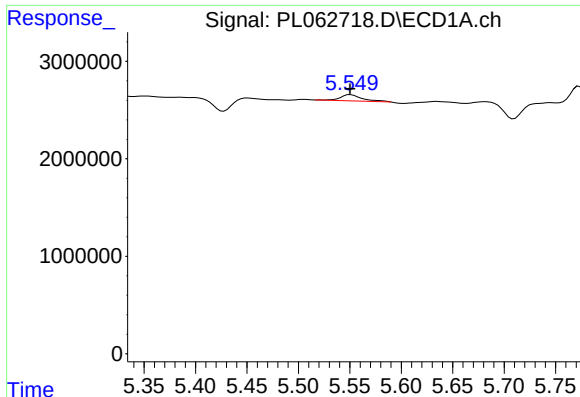

#12 4,4'-DDE


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 923509
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-102920

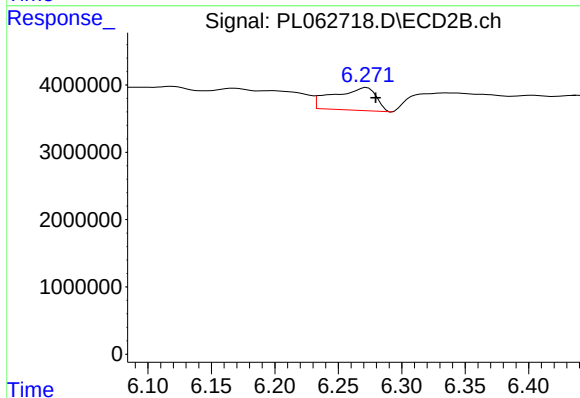


#12 4,4'-DDE

R.T.: 6.272 min
Delta R.T.: -0.007 min
Response: 7988805
Conc: 2.48 ng/ml

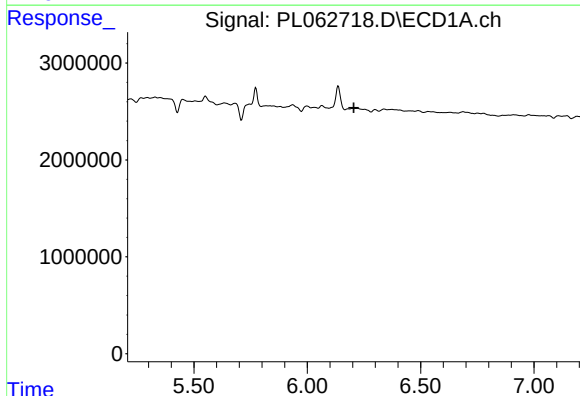


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

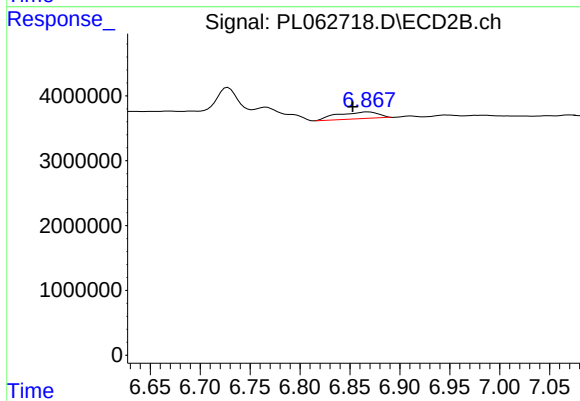

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 2859065
Conc: 1.00 ng/ml

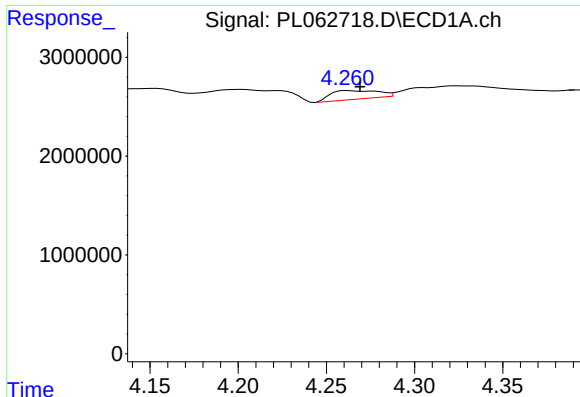

#23 Chlordane-1


R.T.: 4.262 min
Delta R.T.: -0.007 min
Response: 1642885
Conc: 31.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-102920

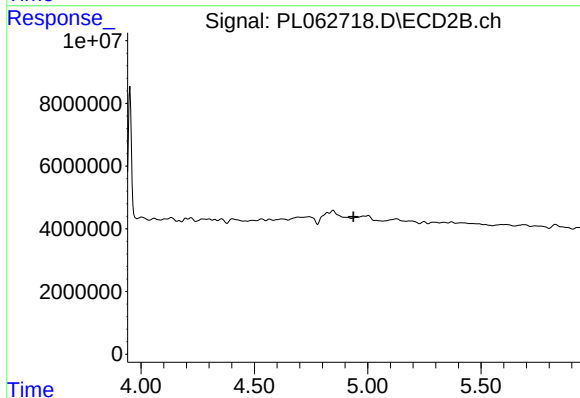


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

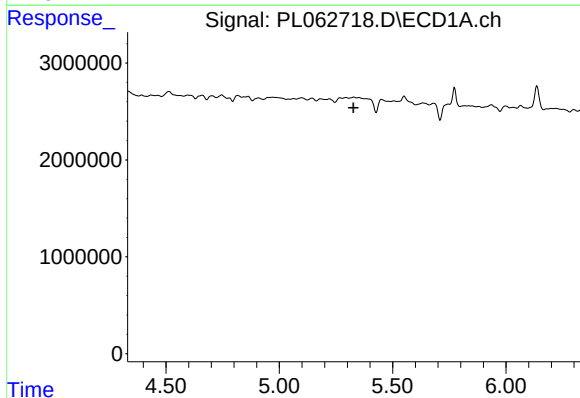


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

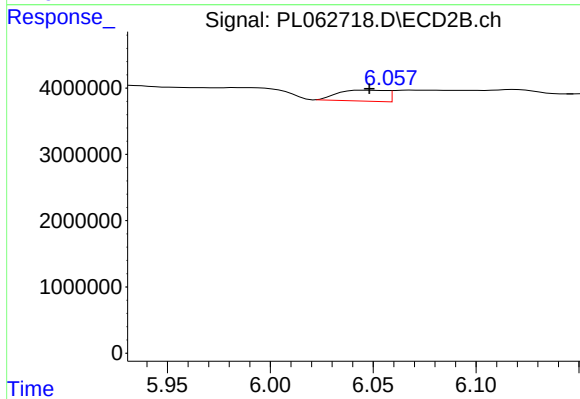

#25 Chlordane-3


R.T.: 6.047 min
Delta R.T.: -0.001 min
Response: 2697888
Conc: 6.68 ng/ml

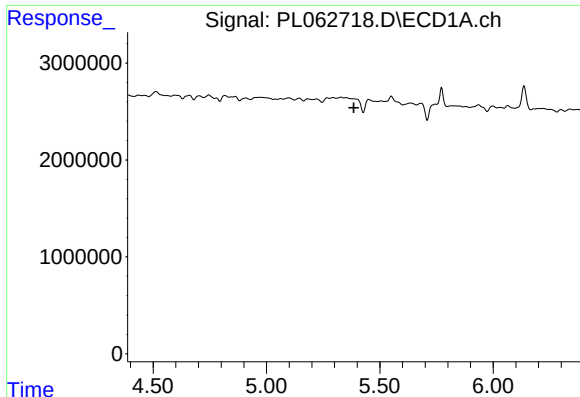

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-102920

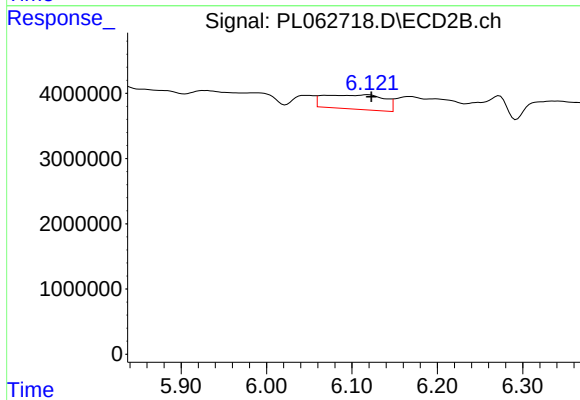


#26 Chlordane-4

R.T.: 6.118 min
Delta R.T.: -0.004 min
Response: 10808587
Conc: 22.32 ng/ml

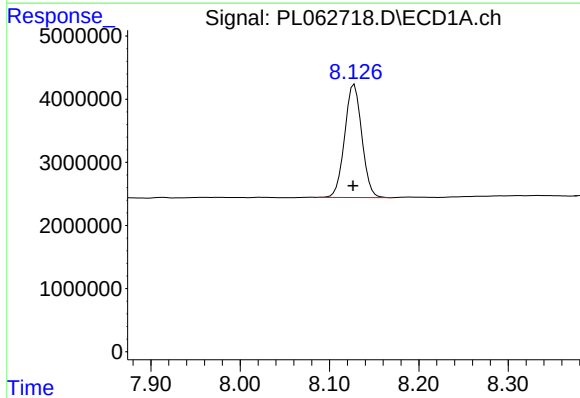

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 23851155
Conc: 14.87 ng/ml

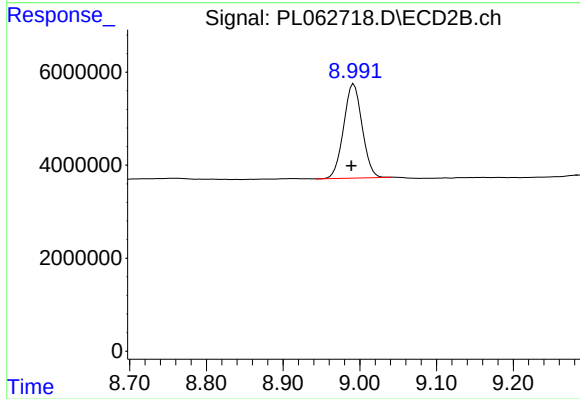

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 34082449
Conc: 16.28 ng/ml