

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 15:34
 Operator : DD\AJ
 Sample : L4541-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 124036

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 17:28:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	38625329	64786926	22.456	22.046
28)	SA Decachlor...	8.127	8.990	34817580	46320409	21.703	22.132
Target Compounds							
2)	A alpha-BHC	3.840	0.000	1626198	0	0.638	N.D. #
7)	B delta-BHC	0.000	5.003	0	4354838	N.D.	1.244 #
8)	B Heptachlo...	0.000	5.844f	0	7242697	N.D.	2.236 #
9)	A Endosulfan I	5.460f	0.000	3153176	0	1.886	N.D. #
10)	B gamma-Chl...	0.000	6.032f	0	1587013	N.D.	0.471 #
13)	MA Dieldrin	5.650f	0.000	569005	0	0.322	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	4349043	N.D.	1.521 #
23)	Chlordane-1	4.274	0.000	617444	0	11.978	N.D. #
25)	Chlordane-3	0.000	6.032f	0	1587013	N.D.	3.929 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 15:34
Operator : DD\AJ
Sample : L4541-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
124036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 17:28:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

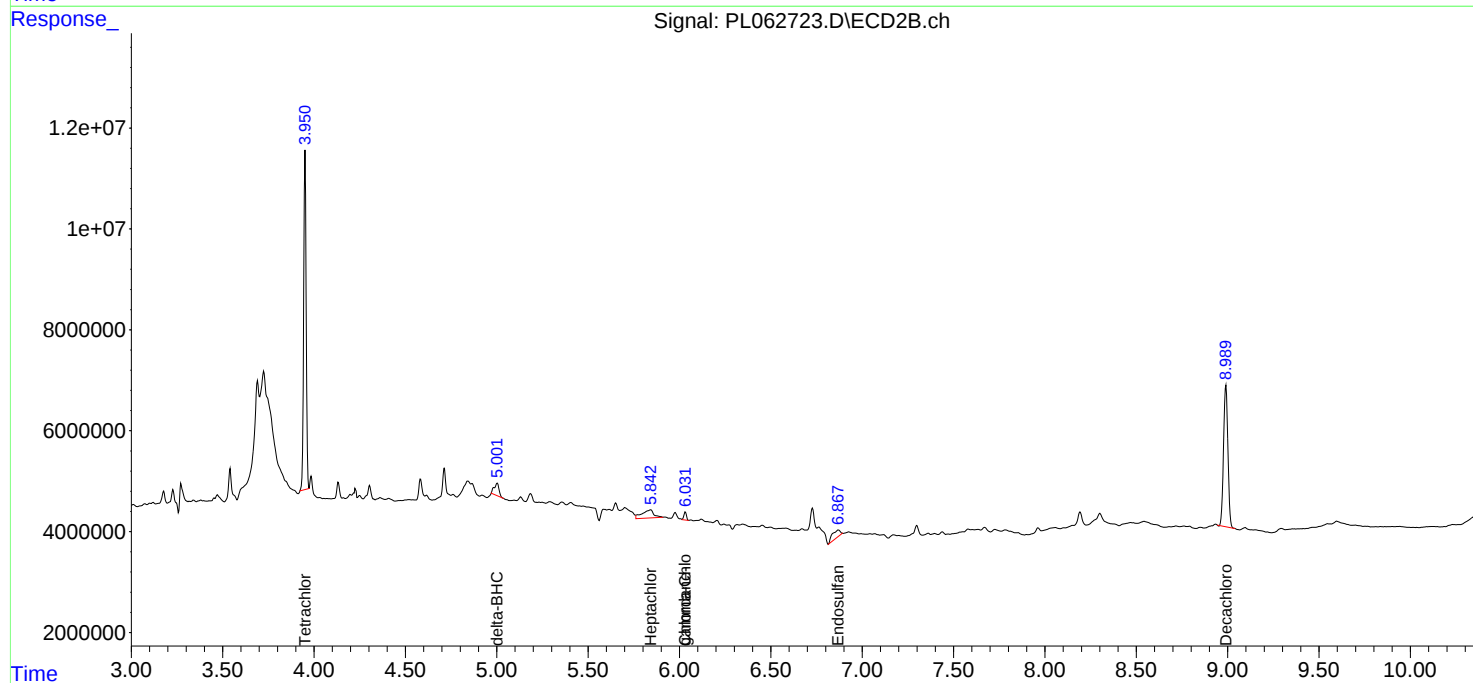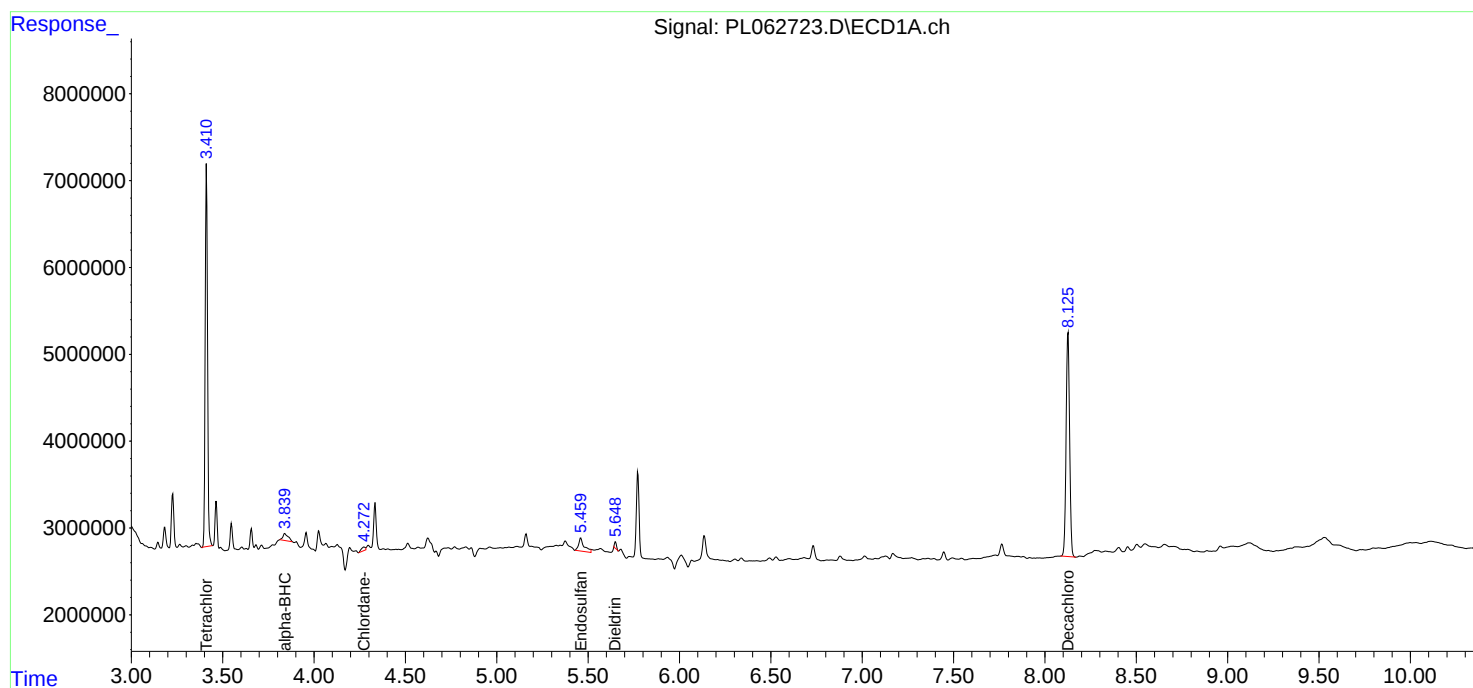


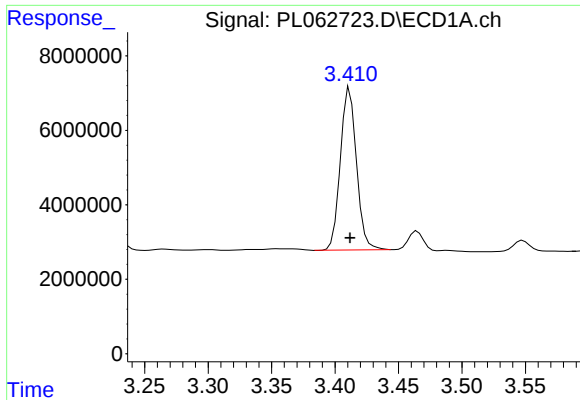

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 38625329
Conc: 22.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
124036

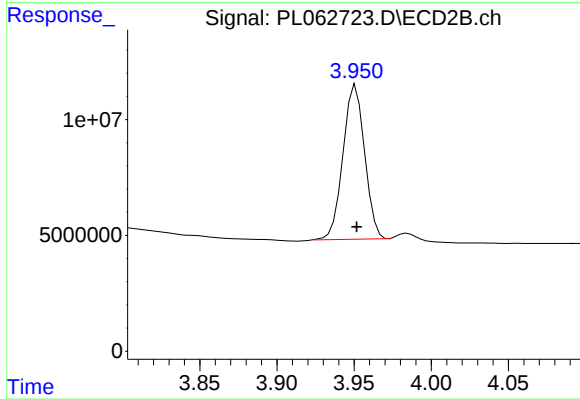


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 64786926
Conc: 22.05 ng/ml

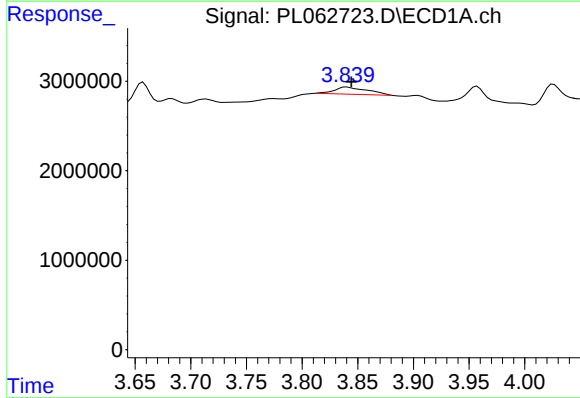


#2 alpha-BHC

R.T.: 3.840 min
Delta R.T.: -0.004 min
Response: 1626198
Conc: 0.64 ng/ml

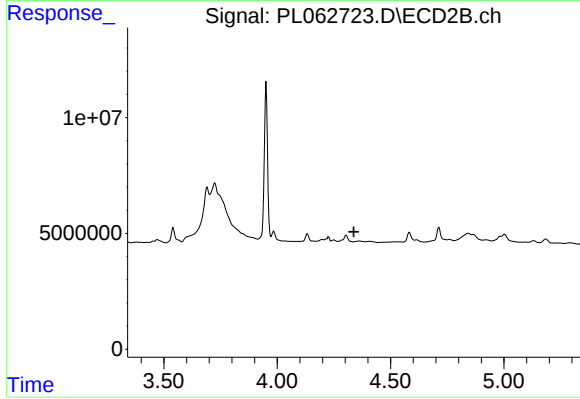

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.338 min
Response: 0
Conc: N.D.

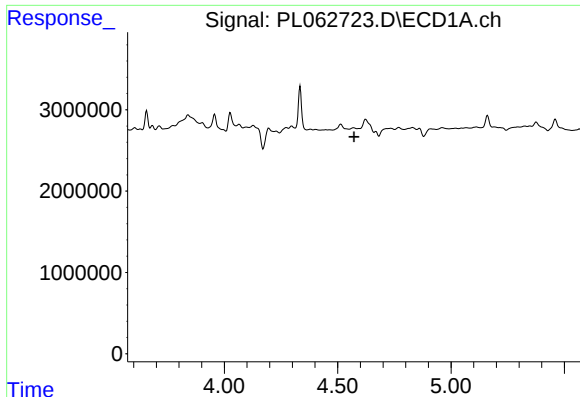

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
124036

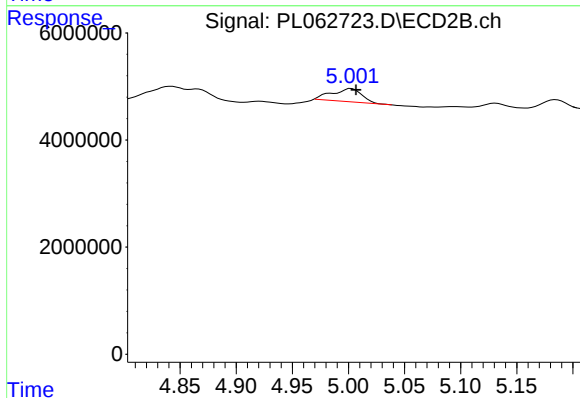


#7 delta-BHC

R.T.: 5.003 min
Delta R.T.: -0.004 min
Response: 4354838
Conc: 1.24 ng/ml

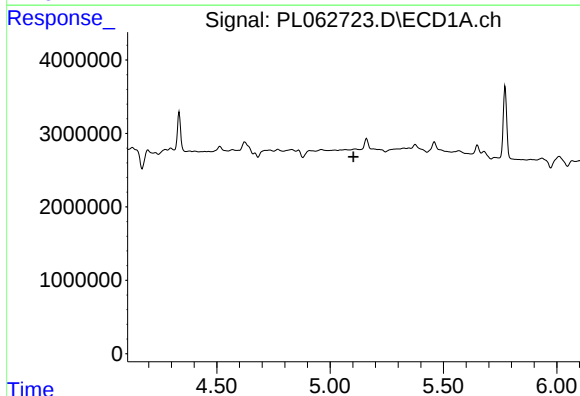


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

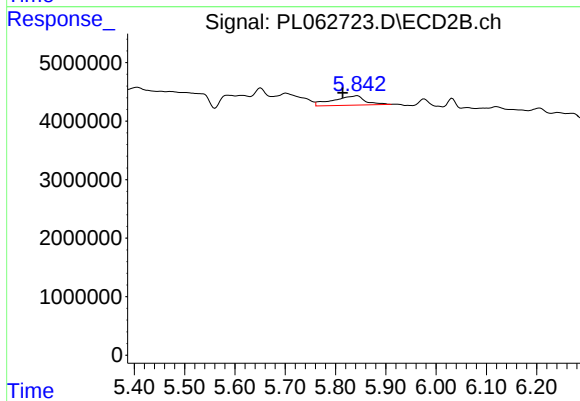

#8 Heptachlor epoxide


R.T.: 5.844 min
Delta R.T.: 0.029 min
Response: 7242697
Conc: 2.24 ng/ml

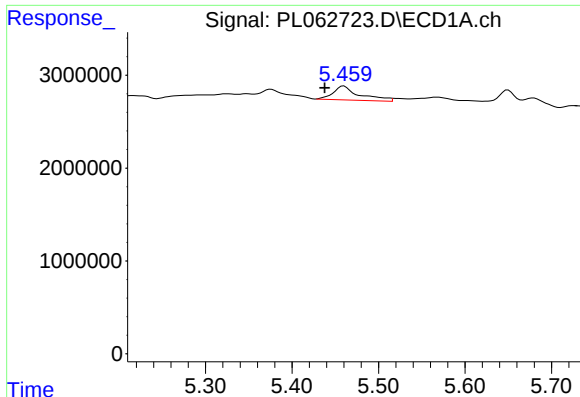

#9 Endosulfan I


R.T.: 5.460 min
Delta R.T.: 0.022 min
Response: 3153176
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
124036

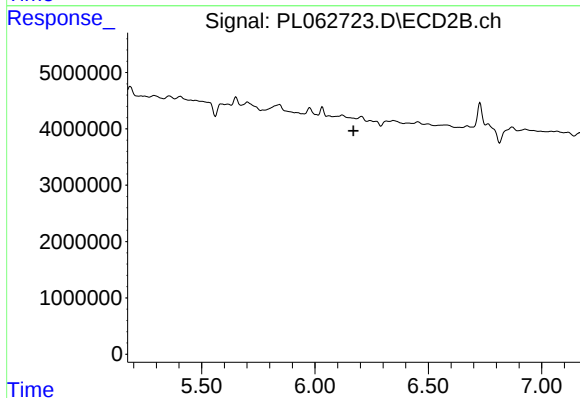


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

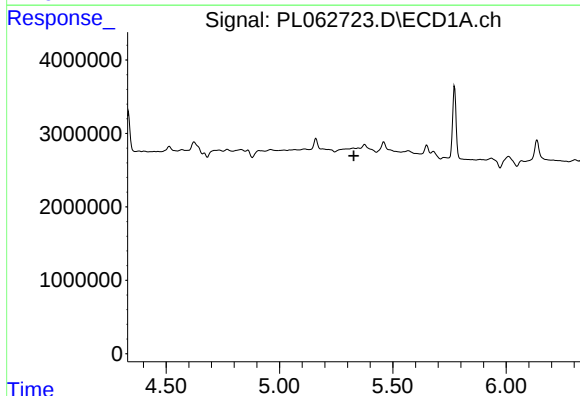


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

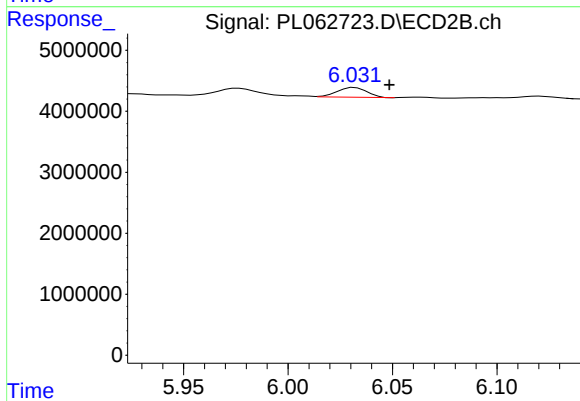

#10 gamma-Chlordane


R.T.: 6.032 min
Delta R.T.: -0.017 min
Response: 1587013
Conc: 0.47 ng/ml

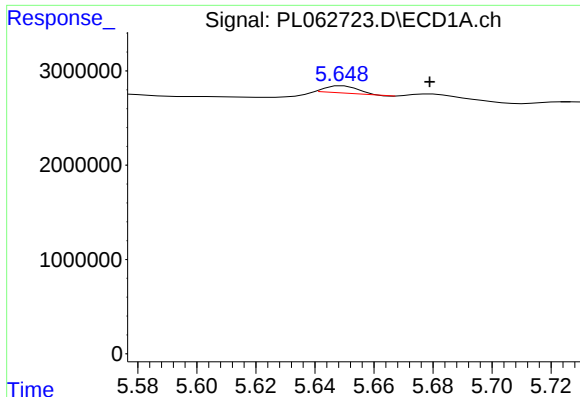

#13 Dieldrin


R.T.: 5.650 min
Delta R.T.: -0.029 min
Response: 569005
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
124036

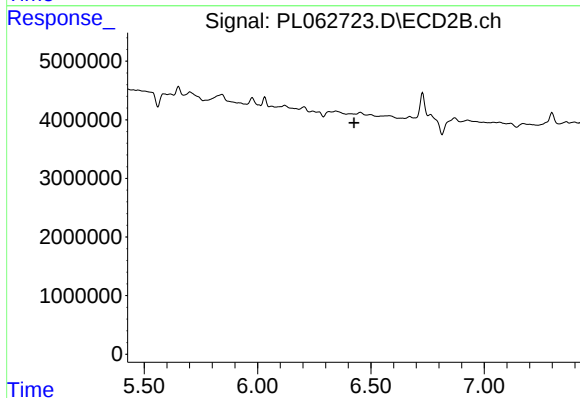


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.426 min
Response: 0
Conc: N.D.

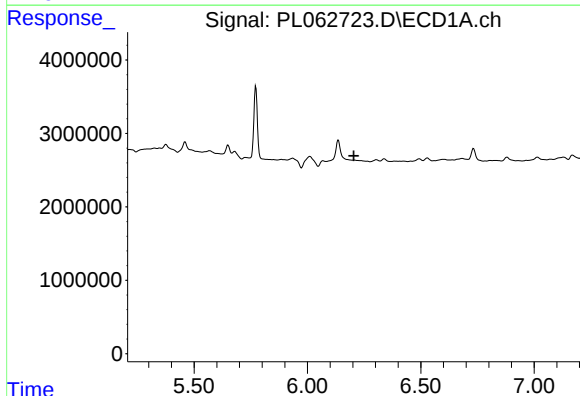


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

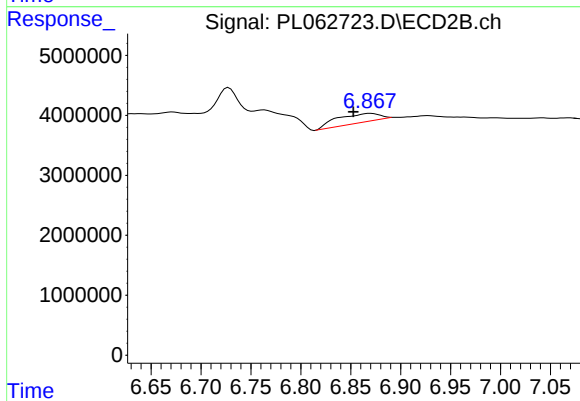

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.017 min
Response: 4349043
Conc: 1.52 ng/ml

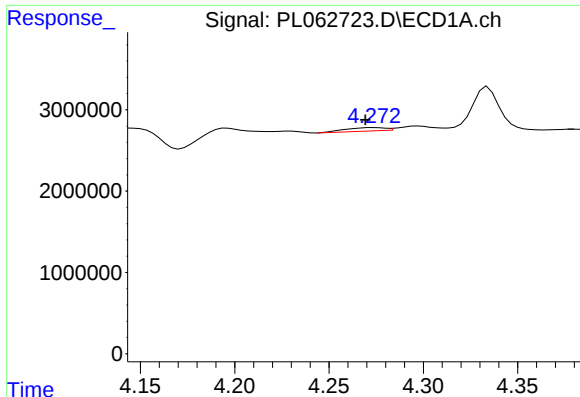

#23 Chlordane-1


R.T.: 4.274 min
Delta R.T.: 0.005 min
Response: 617444
Conc: 11.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
124036

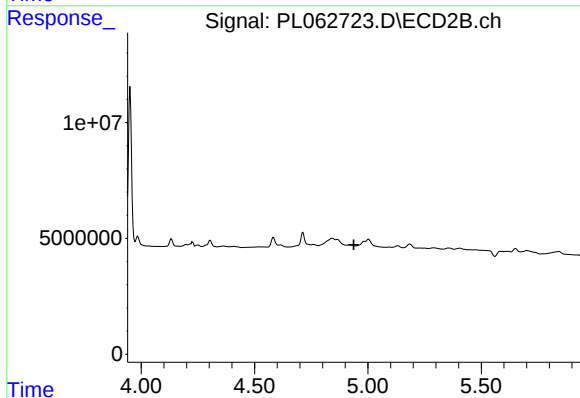


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

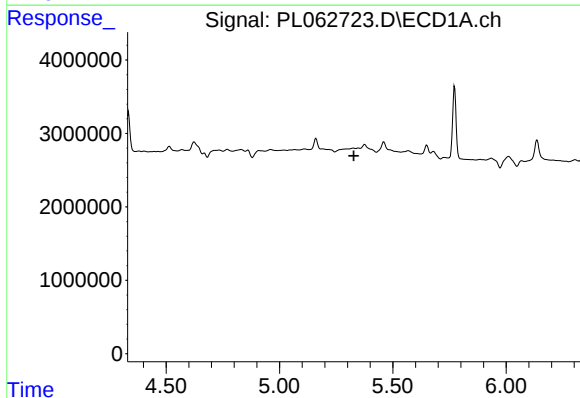


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

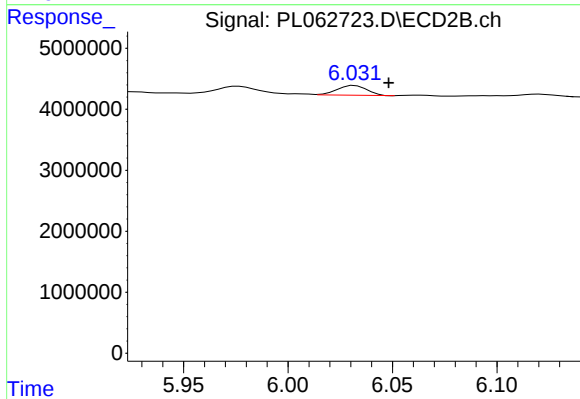

#25 Chlordane-3


R.T.: 6.032 min
Delta R.T.: -0.016 min
Response: 1587013
Conc: 3.93 ng/ml

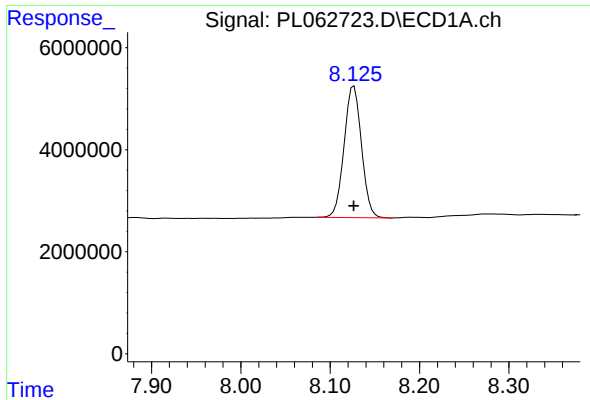

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 34817580
Conc: 21.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
124036

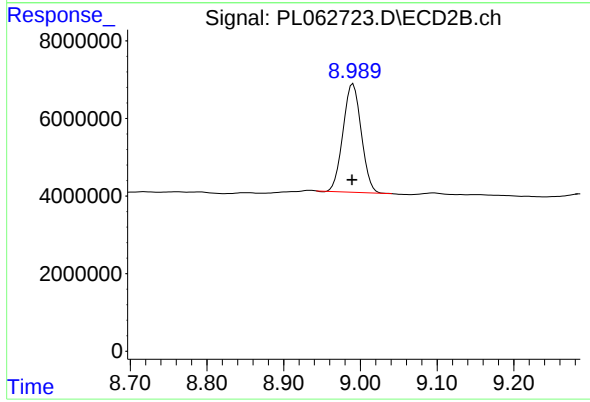

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 46320409
Conc: 22.13 ng/ml