

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 15:49
 Operator : DD\AJ
 Sample : L4541-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 17:28:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	12891233	20118651	7.495	6.846
28)	SA Decachlor...	8.126	8.991	4996322	5492597	3.114	2.624
Target Compounds							
4)	MA Heptachlor	0.000	5.144f	0	1724795	N.D.	0.433 #
9)	A Endosulfan I	5.459f	0.000	1687950	0	1.010	N.D. #
15)	B Endosulfa...	0.000	6.871f	0	4348282	N.D.	1.521 #
23)	Chlordane-1	4.275	0.000	629077	0	12.203	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 15:49
Operator : DD\AJ
Sample : L4541-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 17:28:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

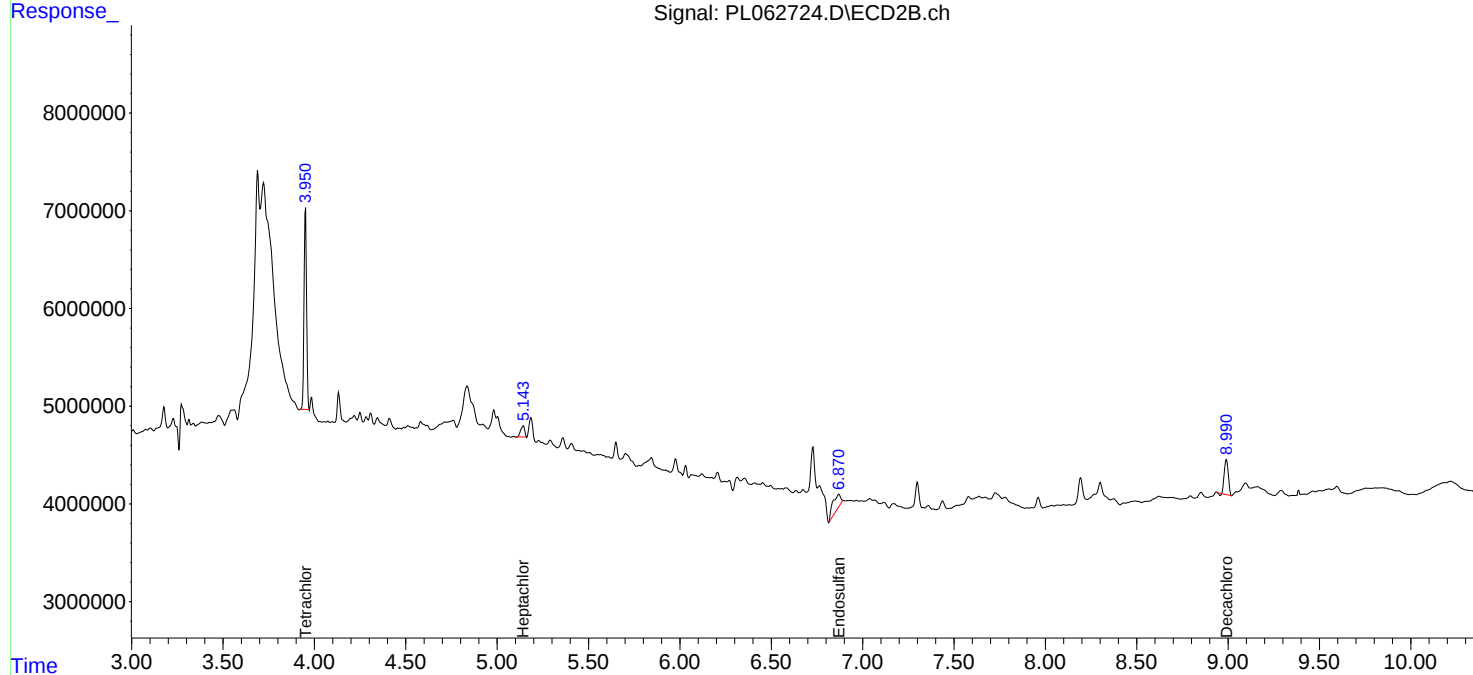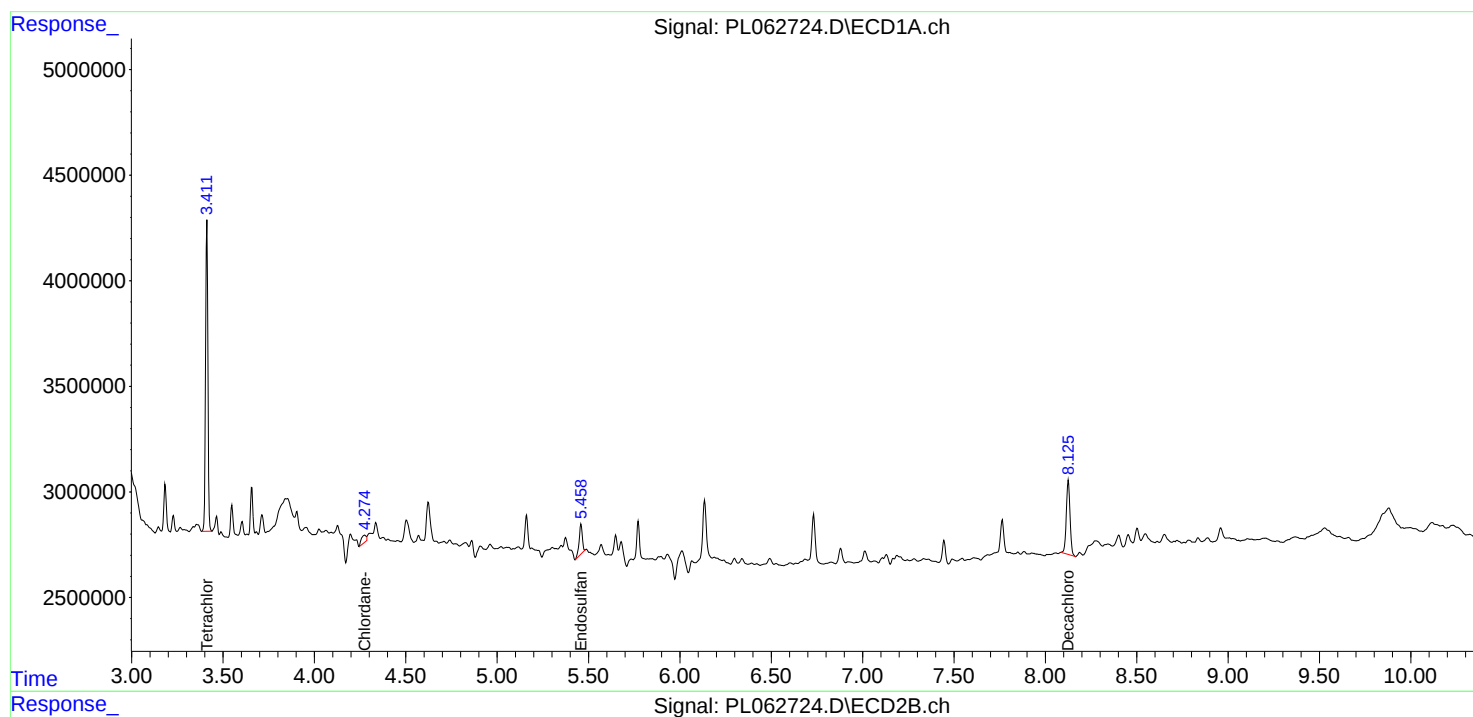


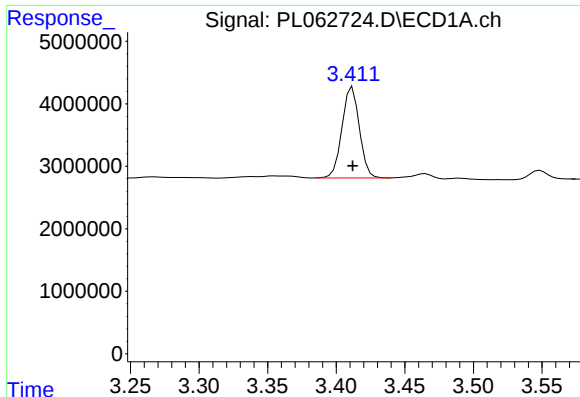

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 12891233
Conc: 7.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

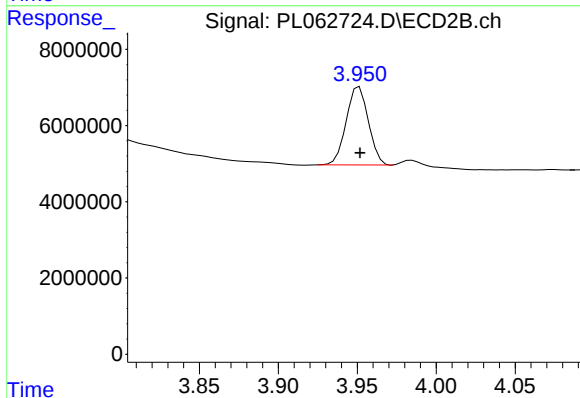


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 20118651
Conc: 6.85 ng/ml

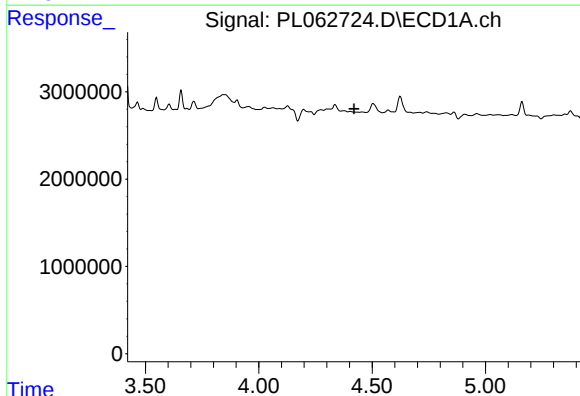


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.420 min
Response: 0
Conc: N.D.

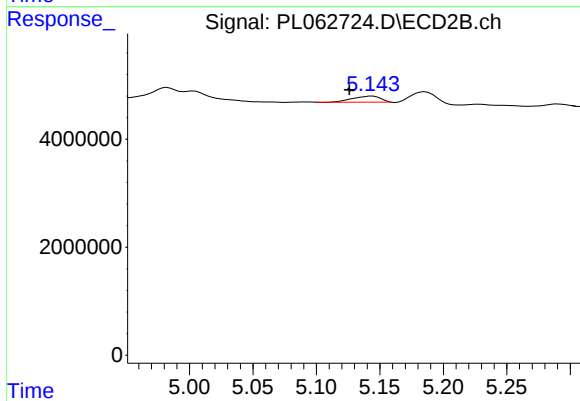

#4 Heptachlor


R.T.: 5.144 min
Delta R.T.: 0.018 min
Response: 1724795
Conc: 0.43 ng/ml

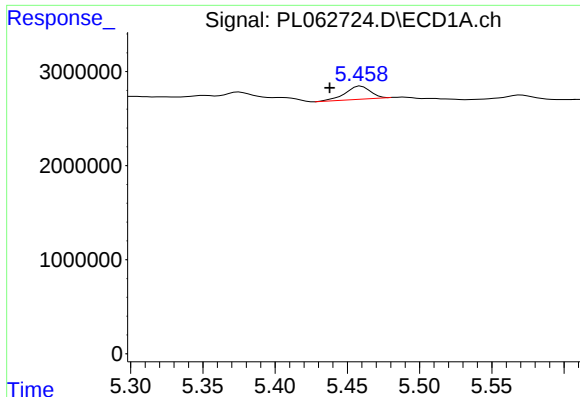

#9 Endosulfan I


R.T.: 5.459 min
Delta R.T.: 0.022 min
Response: 1687950
Conc: 1.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

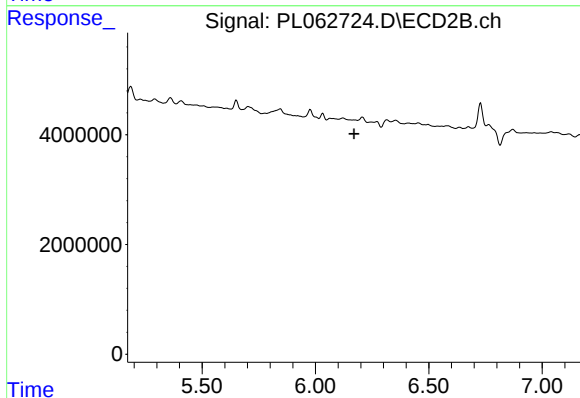


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

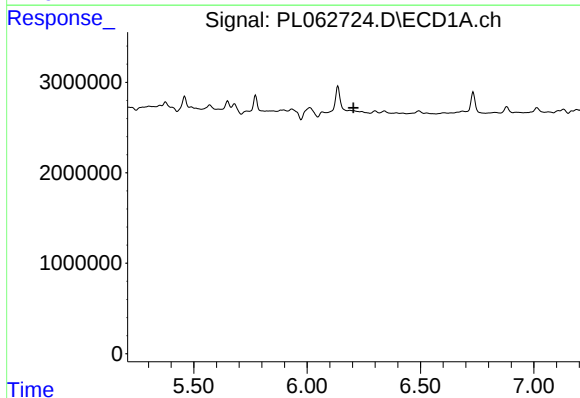


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

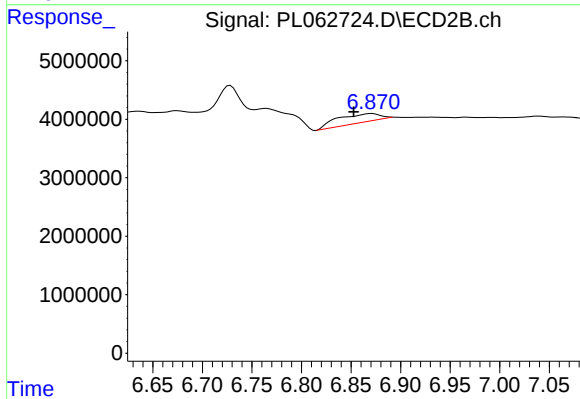

#15 Endosulfan II


R.T.: 6.871 min
Delta R.T.: 0.018 min
Response: 4348282
Conc: 1.52 ng/ml

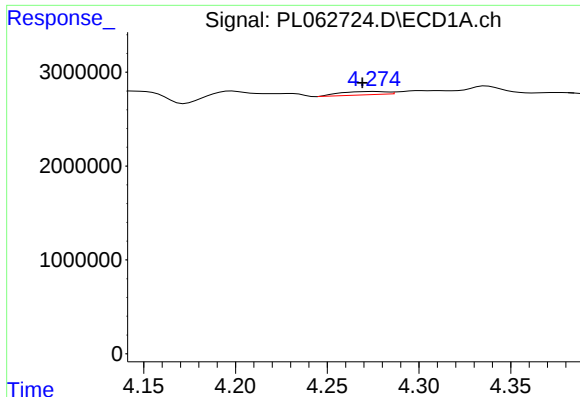

#23 Chlordane-1


R.T.: 4.275 min
Delta R.T.: 0.006 min
Response: 629077
Conc: 12.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

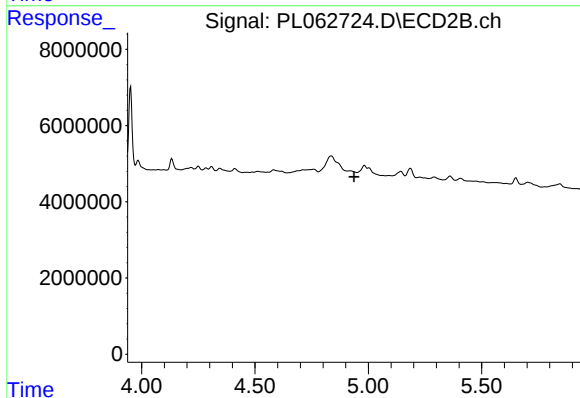


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

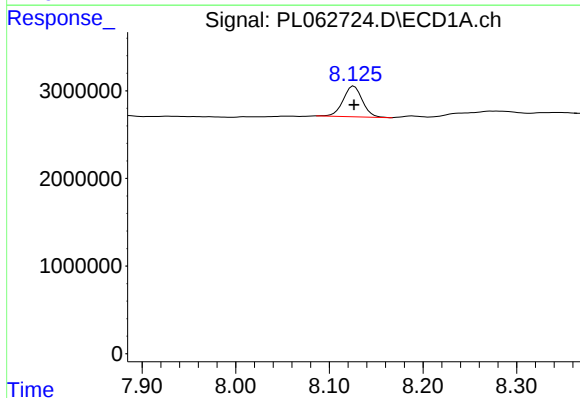

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 4996322
Conc: 3.11 ng/ml

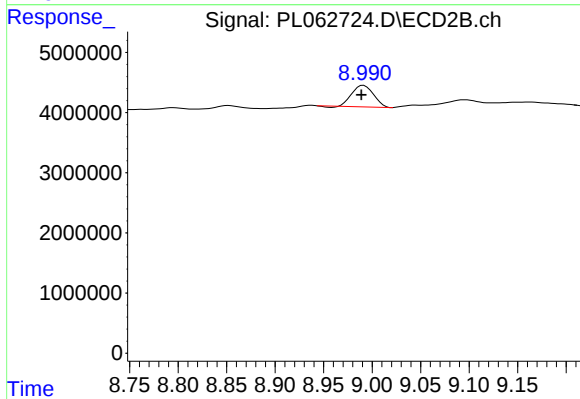

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 5492597
Conc: 2.62 ng/ml