

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 20:05
 Operator : DD\AJ
 Sample : L4549-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUS-WASH-RECLAMATION-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 01:47:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	32453209	49062848	18.867	16.695
28)	SA Decachlor...	8.126	8.991	32787555	45302618	20.437	21.645
Target Compounds							
2)	A alpha-BHC	3.870f	4.337	1198376	3783418	0.470	0.852 #
7)	B delta-BHC	0.000	4.983f	0	1946403	N.D.	0.556 #
8)	B Heptachlo...	5.090	0.000	1301176	0	0.713	N.D. #
11)	B alpha-Chl...	5.375	0.000	1586881	0	0.878	N.D. #
17)	MA 4,4'-DDT	0.000	7.071	0	2966144	N.D.	1.321 #
23)	Chlordane-1	4.278	0.000	564409	0	10.949	N.D. #
26)	Chlordane-4	5.375	0.000	1586881	0	12.182	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 20:05
Operator : DD\AJ
Sample : L4549-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:47:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

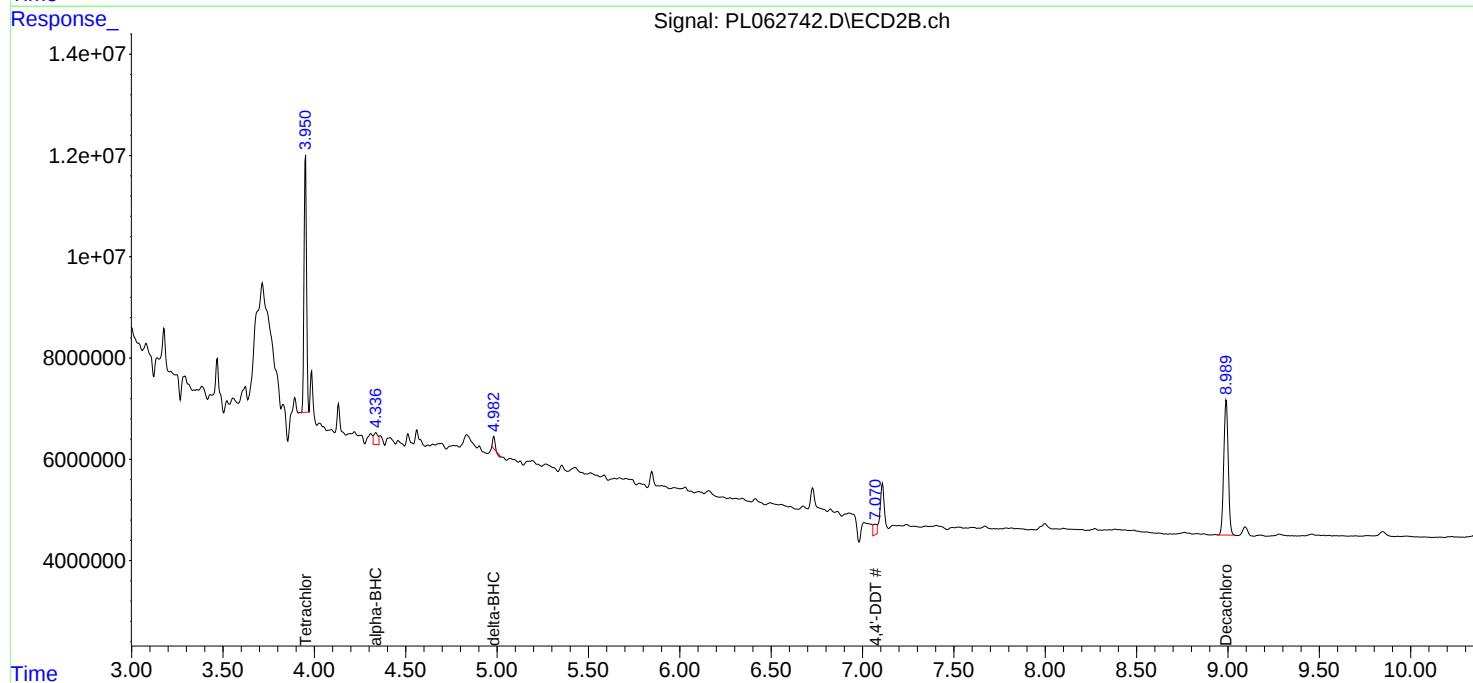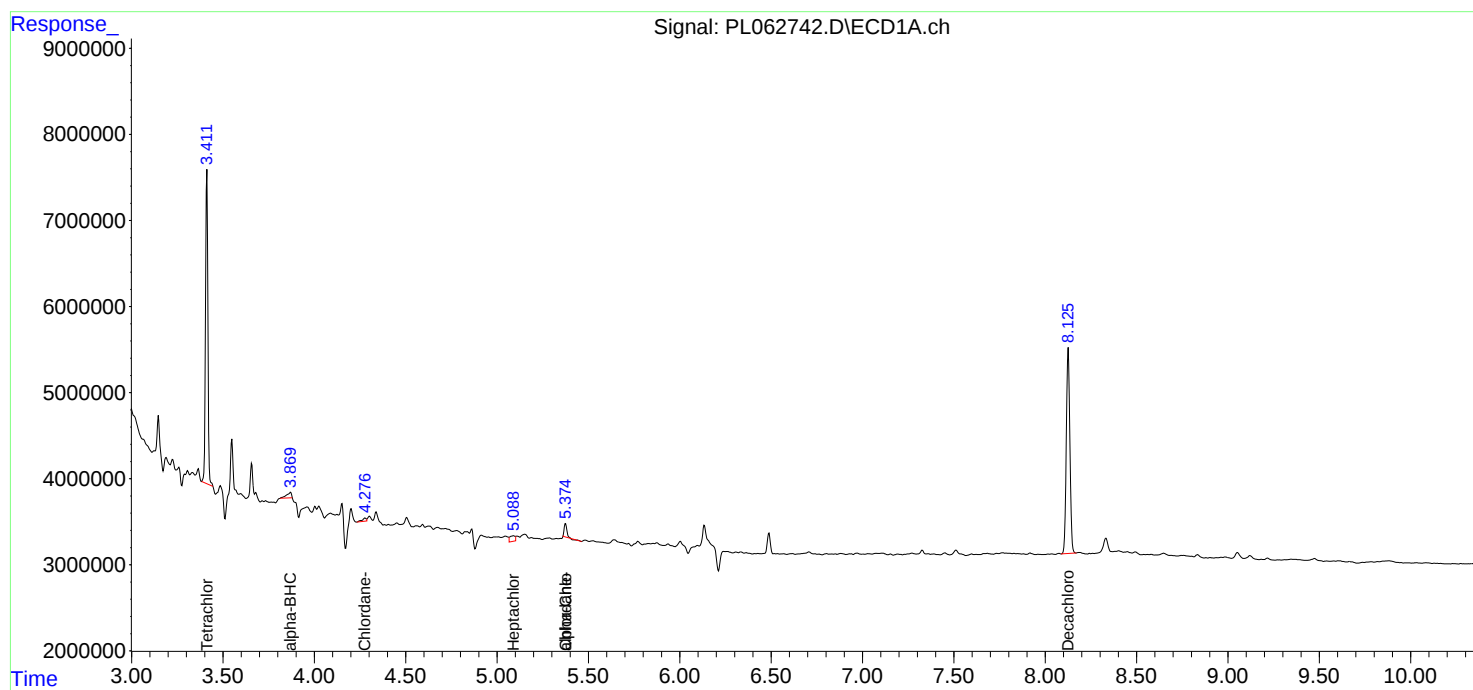


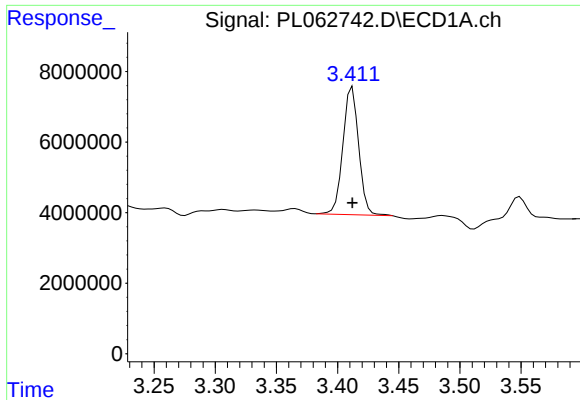

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 32453209
Conc: 18.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

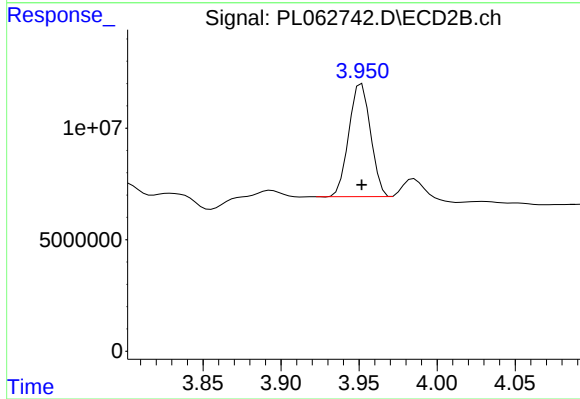


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 49062848
Conc: 16.70 ng/ml

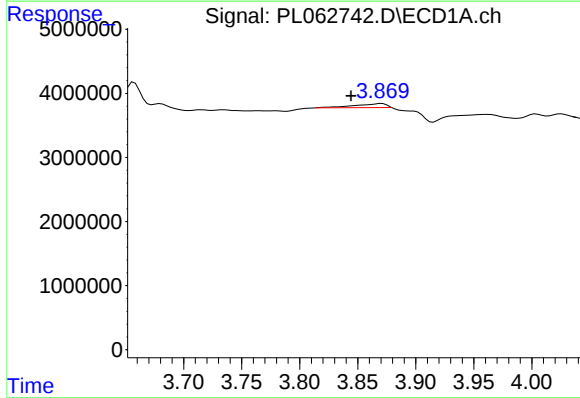


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: 0.026 min
Response: 1198376
Conc: 0.47 ng/ml

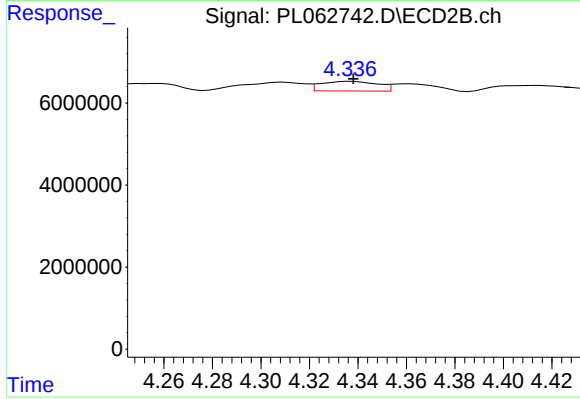

#2 alpha-BHC


R.T.: 4.337 min
Delta R.T.: -0.001 min
Response: 3783418
Conc: 0.85 ng/ml

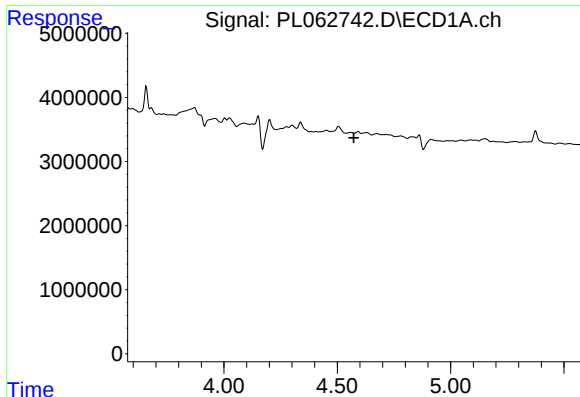

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

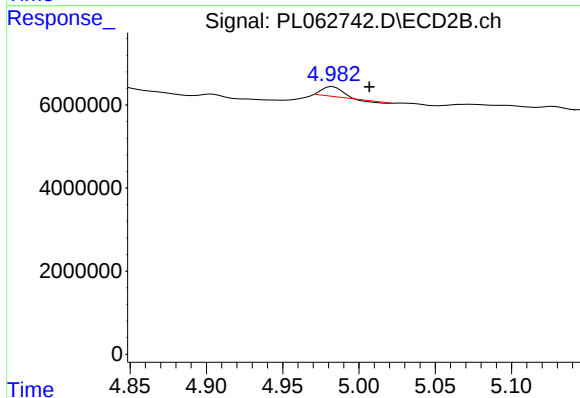


#7 delta-BHC

R.T.: 4.983 min
Delta R.T.: -0.024 min
Response: 1946403
Conc: 0.56 ng/ml

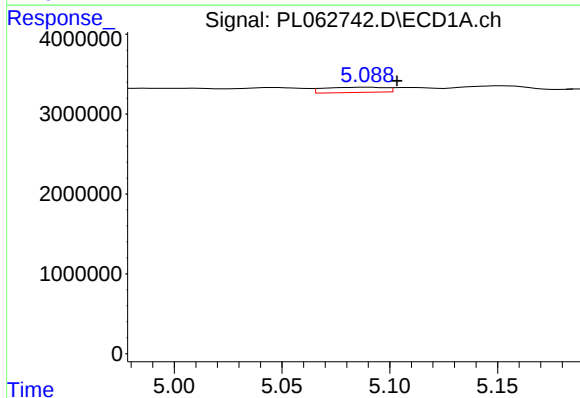


#8 Heptachlor epoxide

R.T.: 5.090 min
Delta R.T.: -0.013 min
Response: 1301176
Conc: 0.71 ng/ml

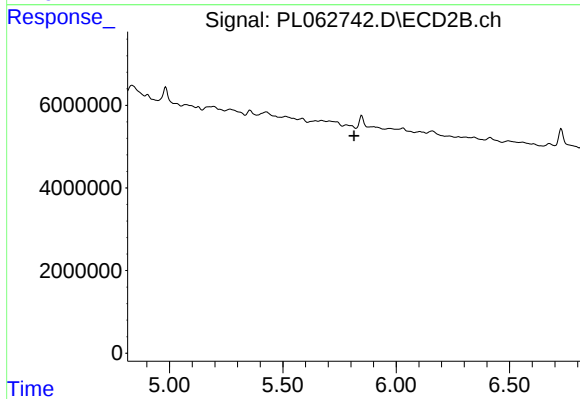

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.815 min
Response: 0
Conc: N.D.

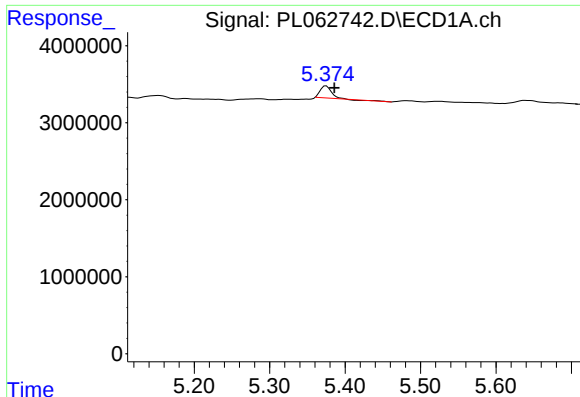

#11 alpha-Chlordane


R.T.: 5.375 min
Delta R.T.: -0.011 min
Response: 1586881
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

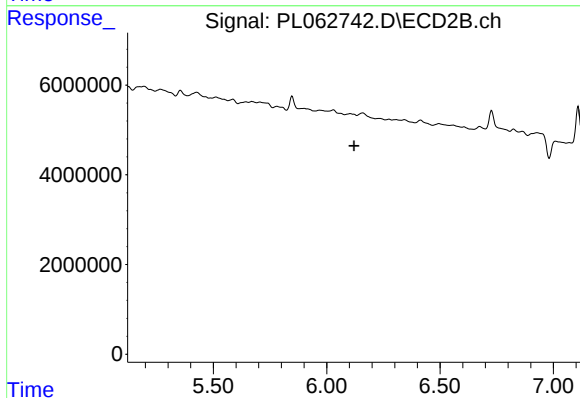


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

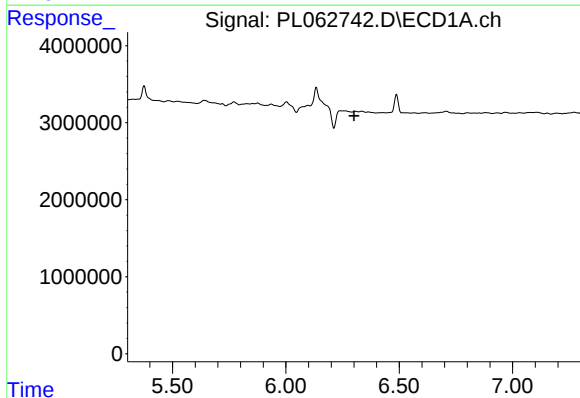


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.301 min
Response: 0
Conc: N.D.

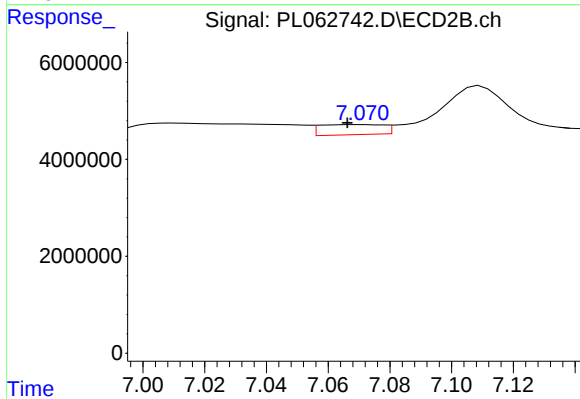

#17 4,4'-DDT


R.T.: 7.071 min
Delta R.T.: 0.005 min
Response: 2966144
Conc: 1.32 ng/ml

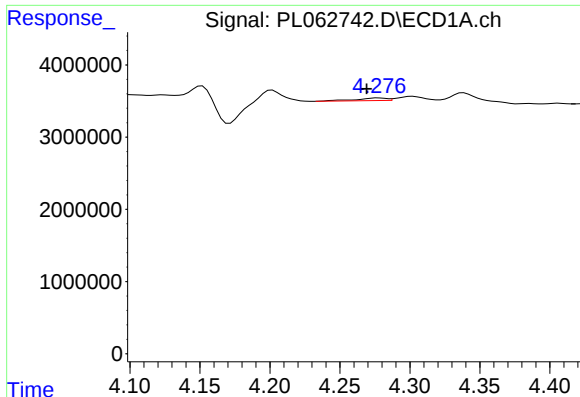

#23 Chlordane-1


R.T.: 4.278 min
Delta R.T.: 0.008 min
Response: 564409
Conc: 10.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

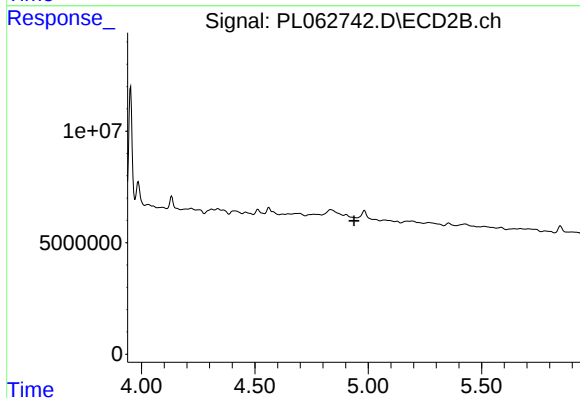


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

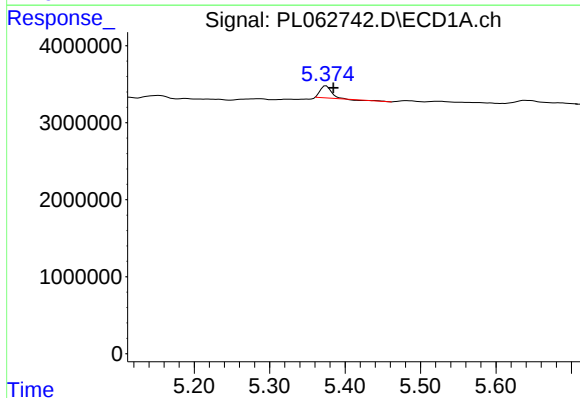


#26 Chlordane-4

R.T.: 5.375 min
Delta R.T.: -0.010 min
Response: 1586881
Conc: 12.18 ng/ml

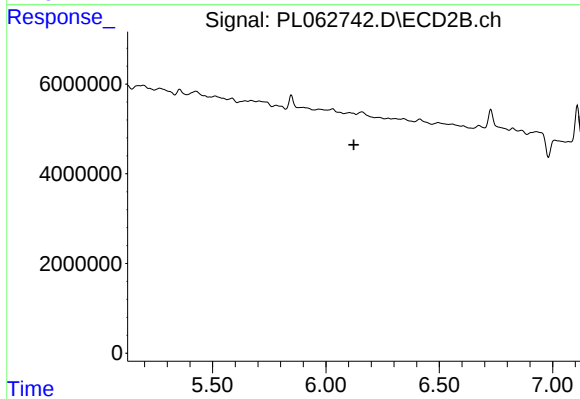

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

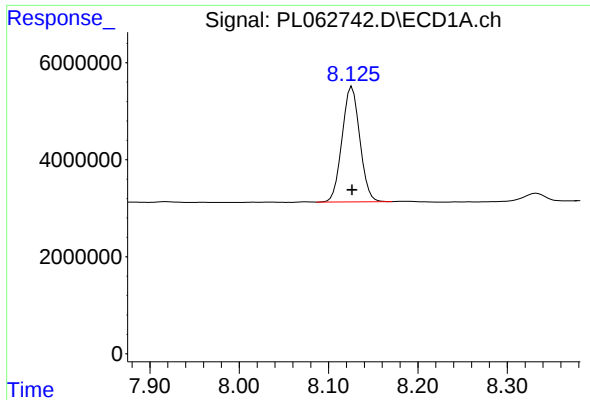

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 32787555
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

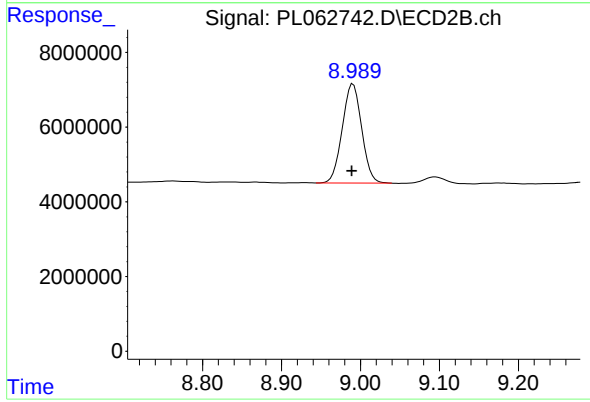

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 45302618
Conc: 21.65 ng/ml