

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 20:19
 Operator : DD\AJ
 Sample : L4549-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 01:47:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	34621112	50718362	20.128	17.259
28)	SA Decachlor...	8.126	8.990	32897583	46111765	20.506	22.032
Target Compounds							
2)	A alpha-BHC	0.000	4.312f	0	11802561	N.D.	2.656 #
7)	B delta-BHC	0.000	4.984f	0	5813340	N.D.	1.661 #
8)	B Heptachlo...	5.093	0.000	1700921	0	0.932	N.D. #
11)	B alpha-Chl...	5.375	0.000	3355103	0	1.856	N.D. #
15)	B Endosulfa...	0.000	6.824f	0	2685829	N.D.	0.940 #
21)	B Endrin ke...	0.000	7.668	0	3274366	N.D.	1.382 #
23)	Chlordane-1	4.277	0.000	1062598	0	20.613	N.D. #
26)	Chlordane-4	5.375	0.000	3355103	0	25.757	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 20:19
Operator : DD\AJ
Sample : L4549-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:47:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

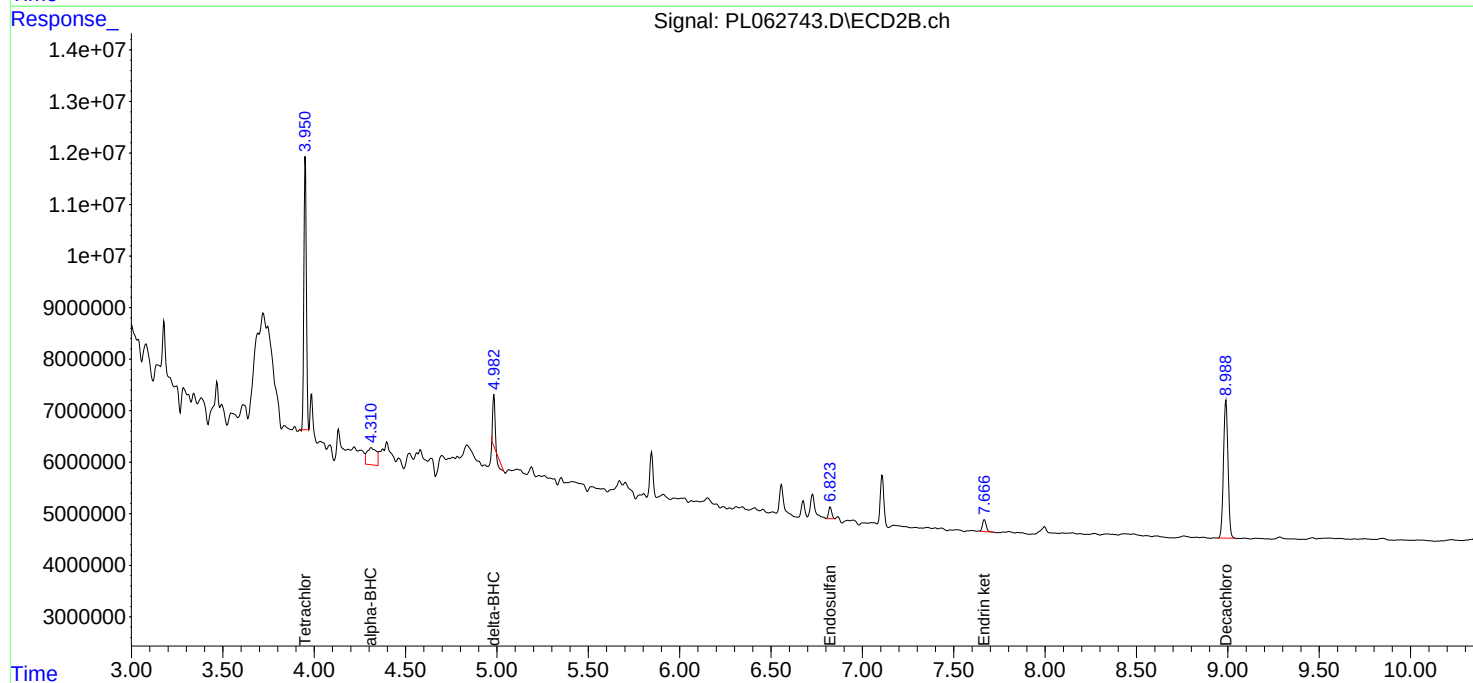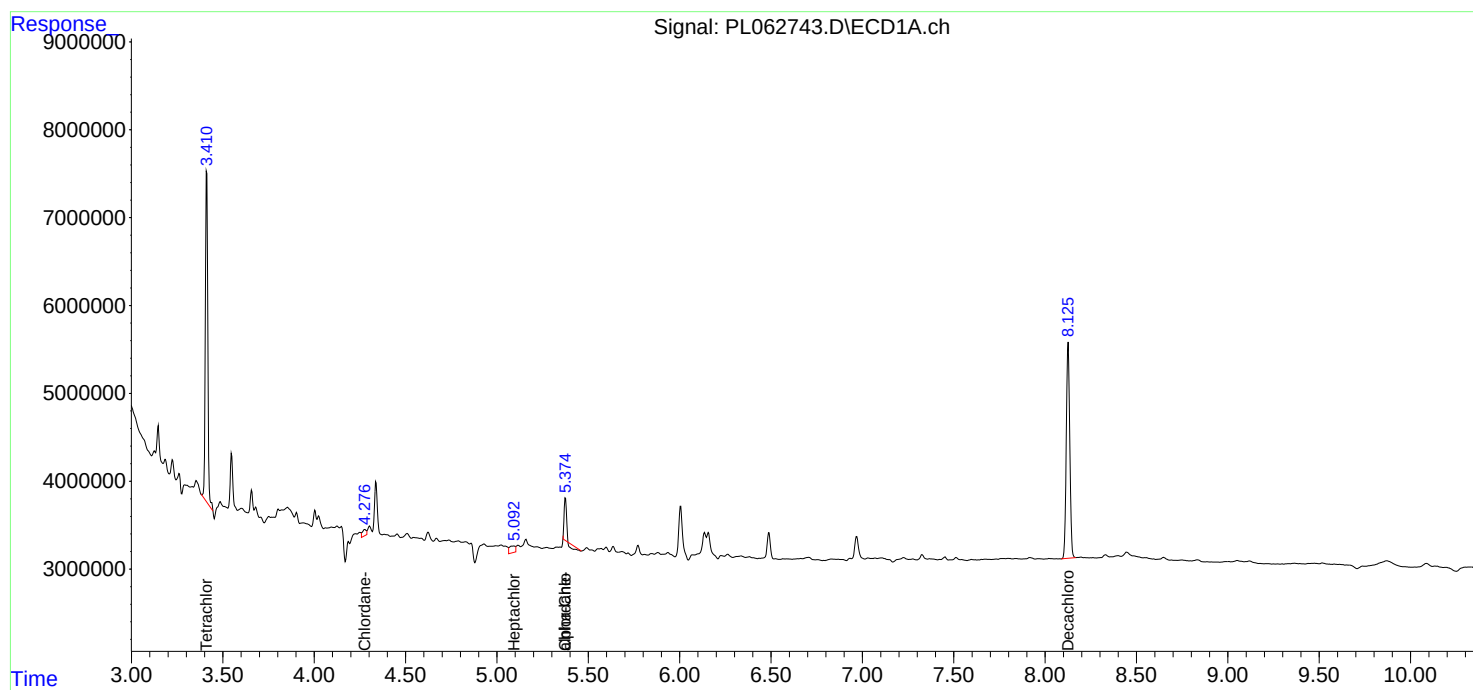


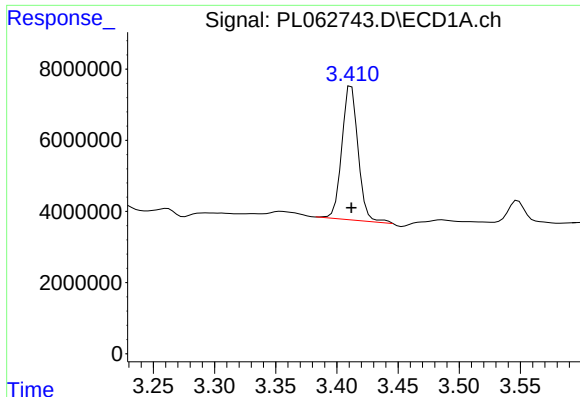

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 34621112
Conc: 20.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

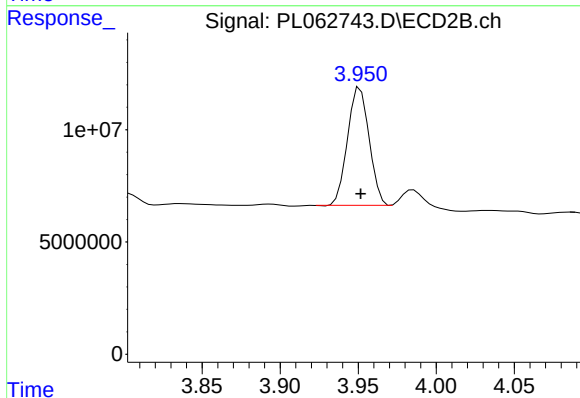


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 50718362
Conc: 17.26 ng/ml

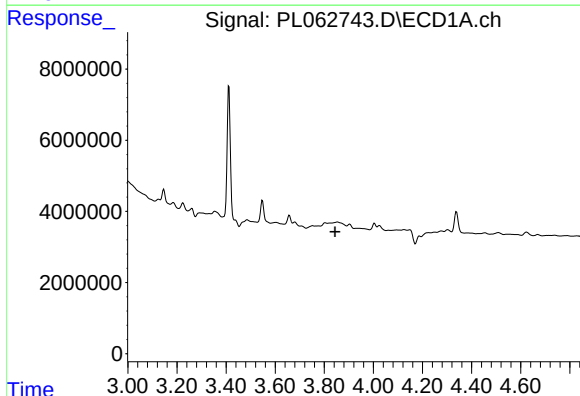


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

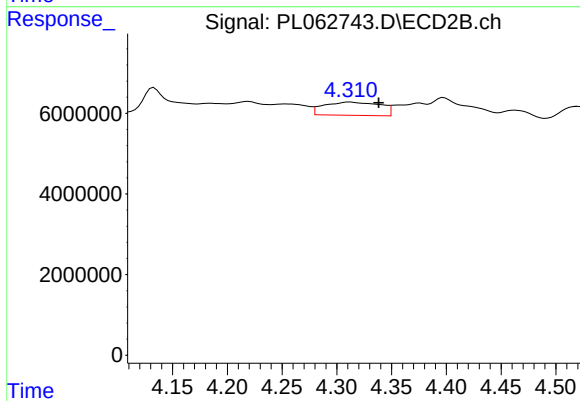

#2 alpha-BHC


R.T.: 4.312 min
Delta R.T.: -0.027 min
Response: 11802561
Conc: 2.66 ng/ml

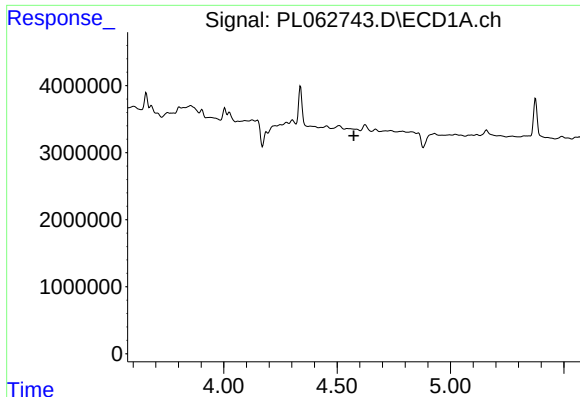

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

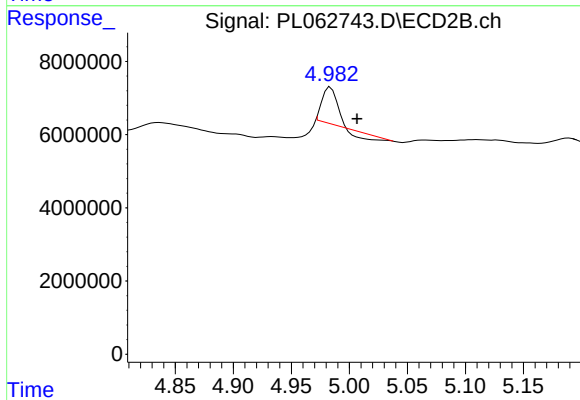


#7 delta-BHC

R.T.: 4.984 min
Delta R.T.: -0.023 min
Response: 5813340
Conc: 1.66 ng/ml

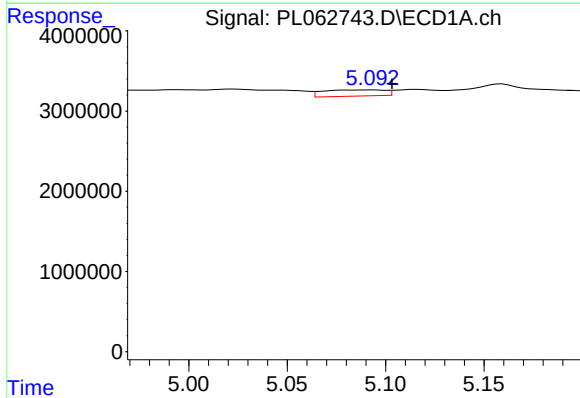


#8 Heptachlor epoxide

R.T.: 5.093 min
Delta R.T.: -0.010 min
Response: 1700921
Conc: 0.93 ng/ml

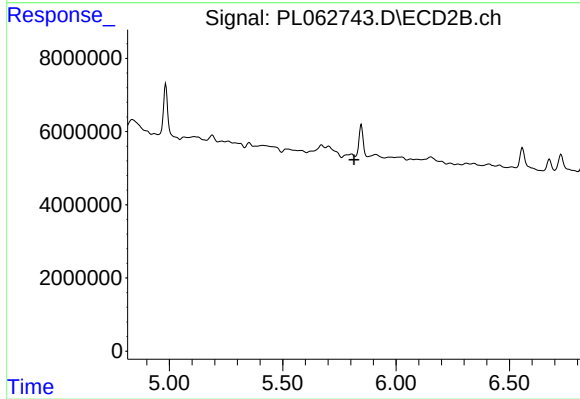

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.815 min
Response: 0
Conc: N.D.

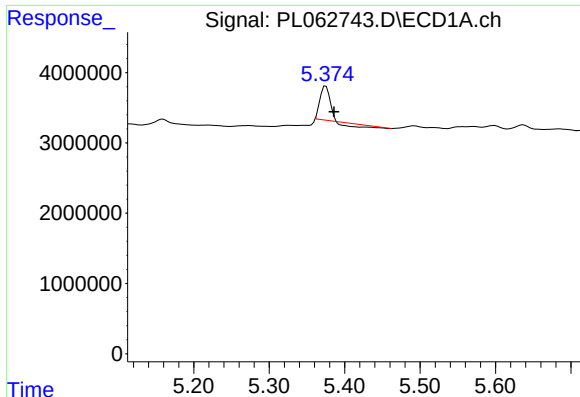

#11 alpha-Chlordane


R.T.: 5.375 min
Delta R.T.: -0.011 min
Response: 3355103
Conc: 1.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

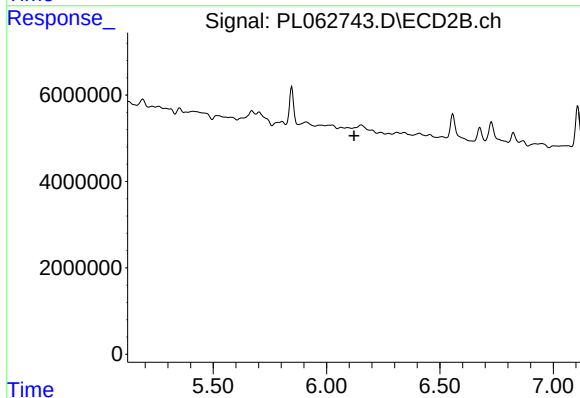


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

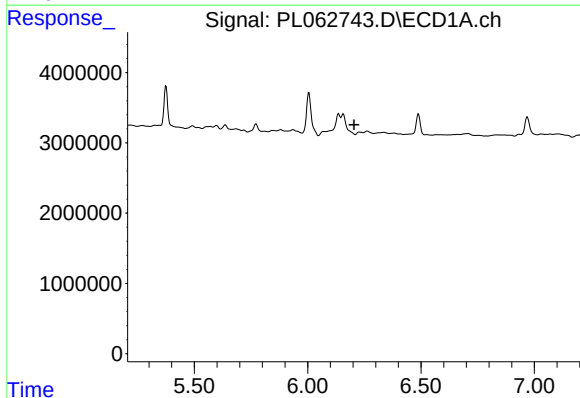


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

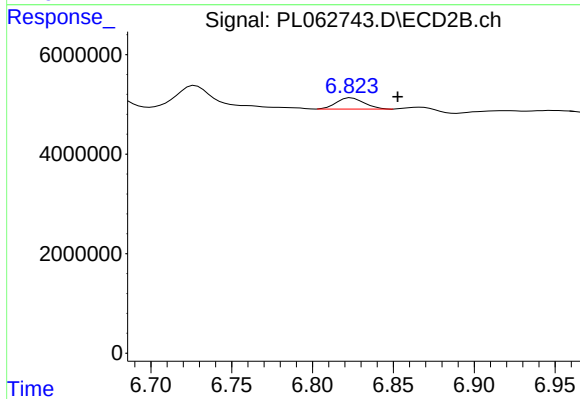

#15 Endosulfan II


R.T.: 6.824 min
Delta R.T.: -0.029 min
Response: 2685829
Conc: 0.94 ng/ml

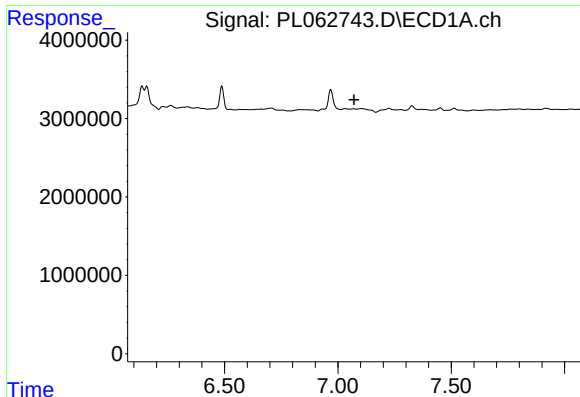

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

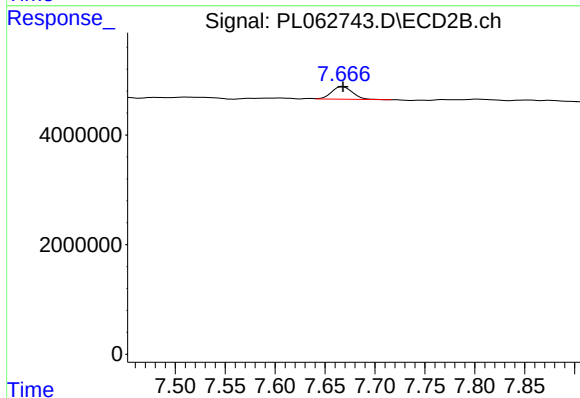


#21 Endrin ketone

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 3274366
Conc: 1.38 ng/ml

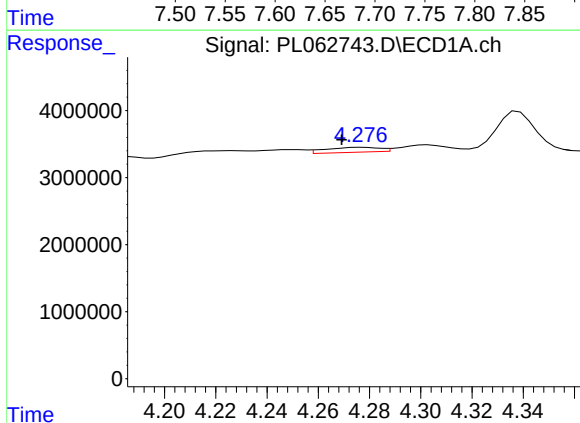


#23 Chlordane-1

R.T.: 4.277 min
Delta R.T.: 0.008 min
Response: 1062598
Conc: 20.61 ng/ml

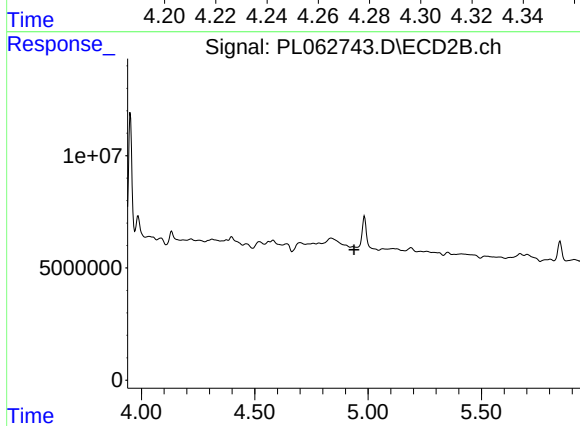

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

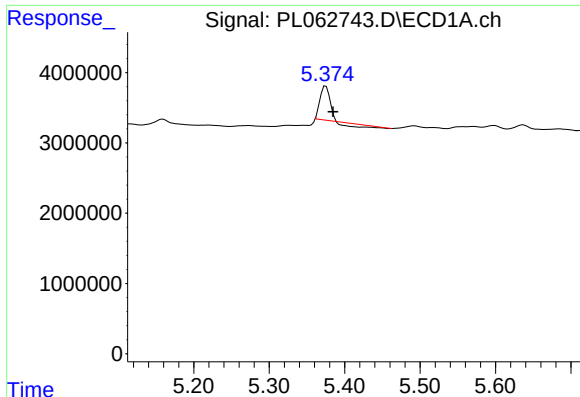

#26 Chlordane-4


R.T.: 5.375 min
Delta R.T.: -0.010 min
Response: 3355103
Conc: 25.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

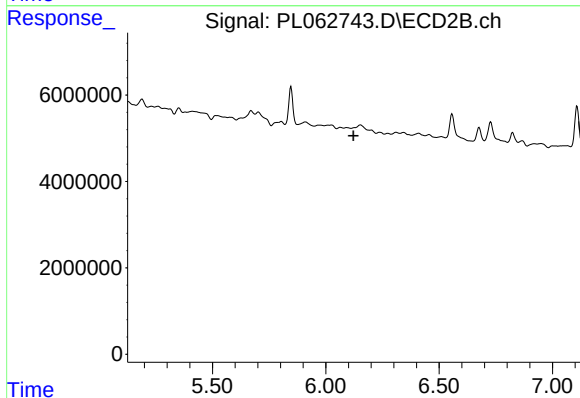


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

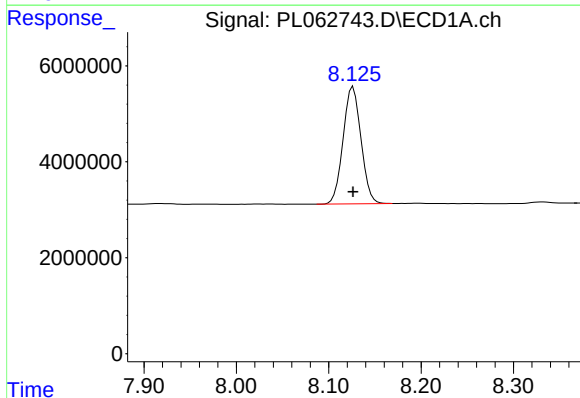

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 32897583
Conc: 20.51 ng/ml

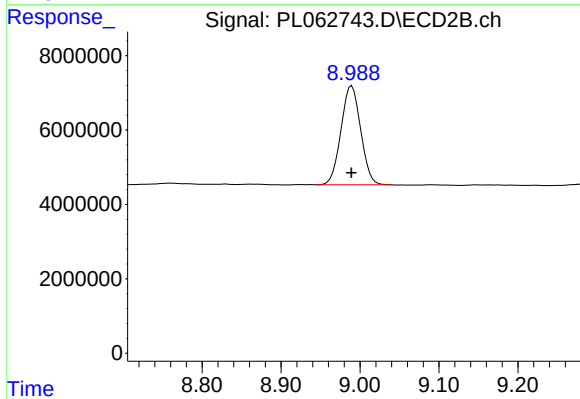

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 46111765
Conc: 22.03 ng/ml