

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL103020\  
 Data File : PL062746.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 30 Oct 2020 21:02  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 31 01:48:55 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL102120.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Oct 22 04:25:31 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|---------|
| -----                       |                 |        |        |          |          |        |         |
| System Monitoring Compounds |                 |        |        |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.412  | 3.951  | 35074539 | 59717680 | 20.391 | 20.321  |
| 28)                         | SA Decachlor... | 8.126  | 8.989  | 34676752 | 47819074 | 21.615 | 22.848  |
| Target Compounds            |                 |        |        |          |          |        |         |
| 8)                          | B Heptachlo...  | 5.090  | 5.809  | 1535163  | 10562939 | 0.841  | 3.262 # |
| 10)                         | B gamma-Chl...  | 0.000  | 6.025f | 0        | 948787   | N.D.   | 0.282 # |
| 14)                         | MA Endrin       | 5.936  | 0.000  | 589299   | 0        | 0.354  | N.D. #  |
| 15)                         | B Endosulfa...  | 0.000  | 6.867  | 0        | 1060559  | N.D.   | 0.371 # |
| 23)                         | Chlordane-1     | 4.298f | 0.000  | 796840   | 0        | 15.458 | N.D. #  |
| 25)                         | Chlordane-3     | 0.000  | 6.025f | 0        | 948787   | N.D.   | 2.349 # |
| -----                       |                 |        |        |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL103020\  
Data File : PL062746.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 30 Oct 2020 21:02  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 31 01:48:55 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL102120.M  
Quant Title : GC Extractables  
QLast Update : Thu Oct 22 04:25:31 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

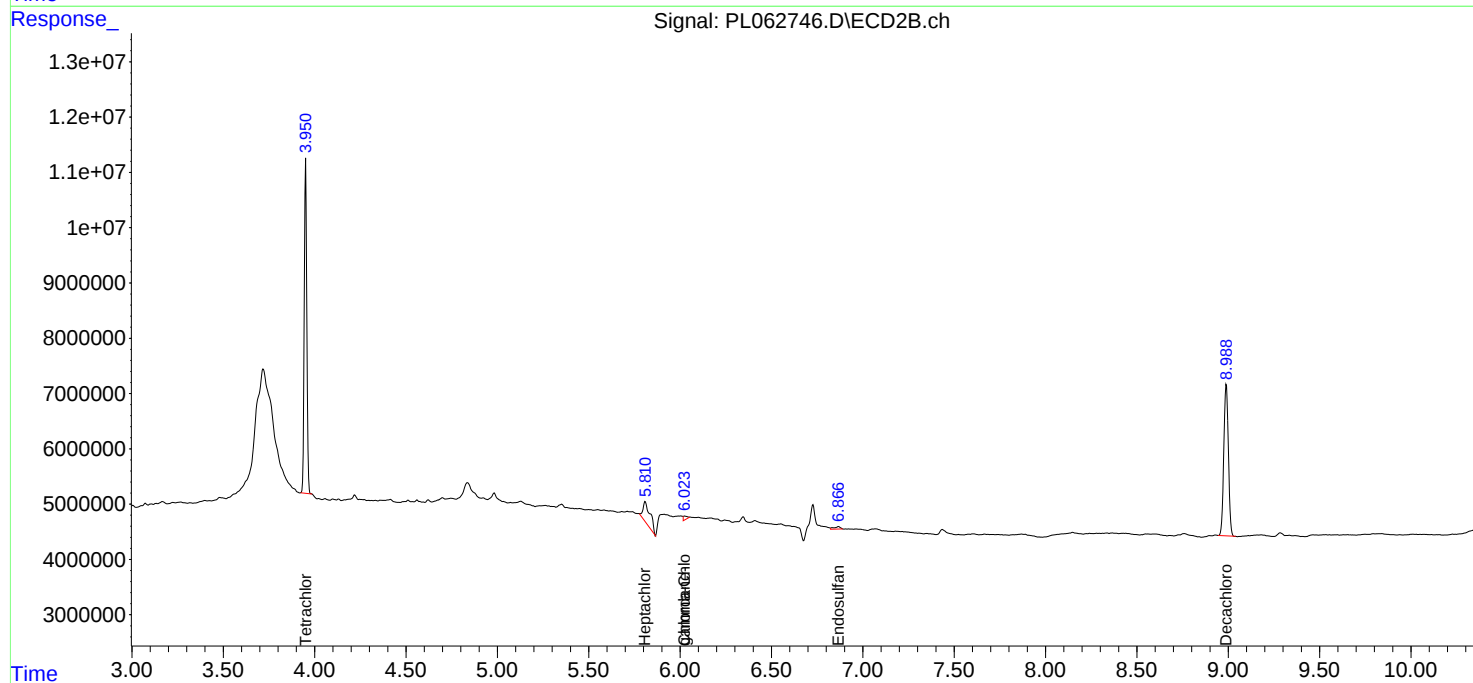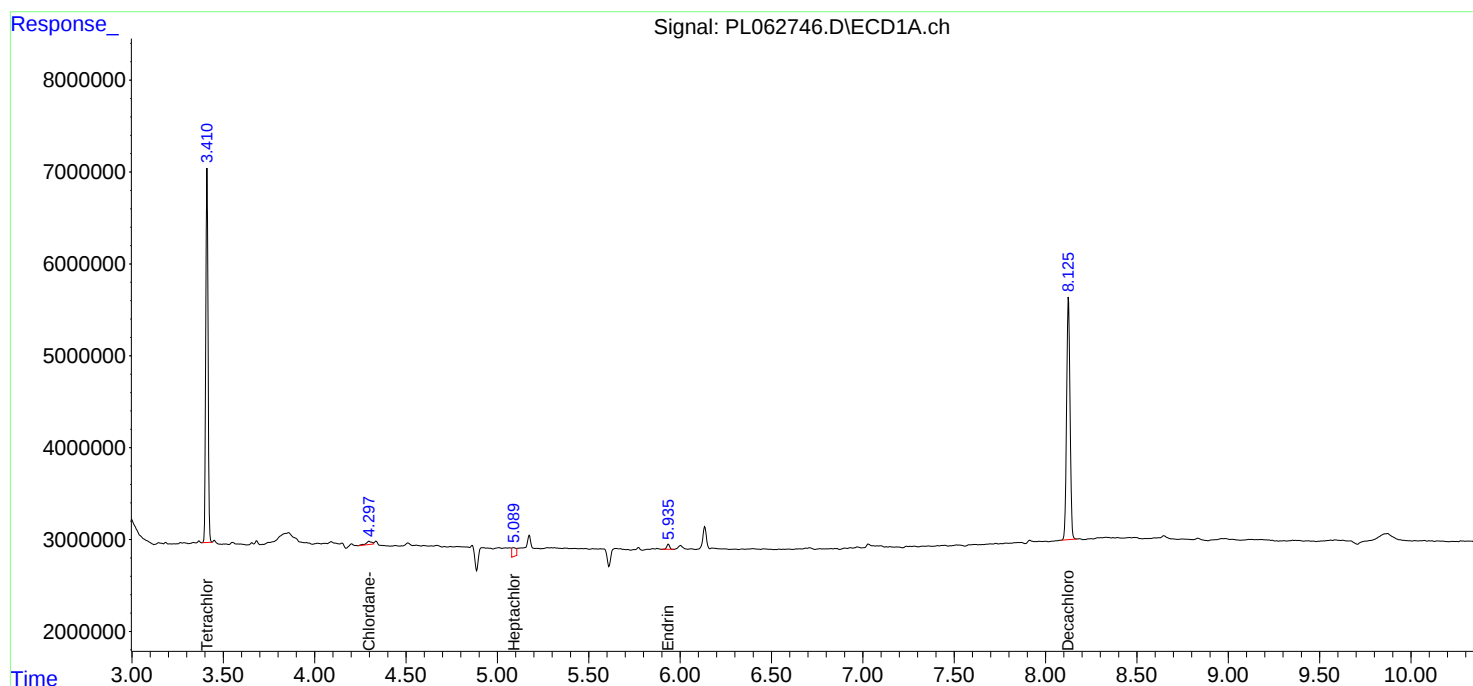


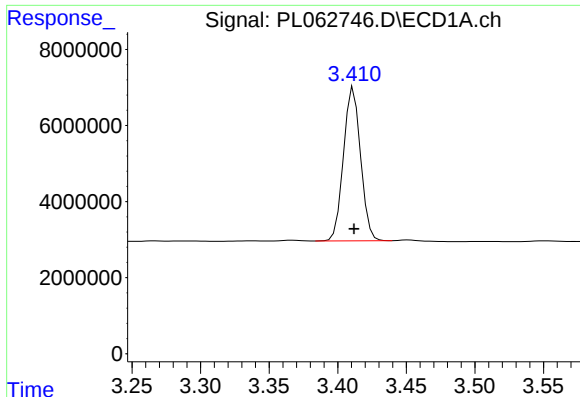

#1 Tetrachloro-m-xylene


R.T.: 3.412 min  
Delta R.T.: 0.000 min  
Response: 35074539  
Conc: 20.39 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

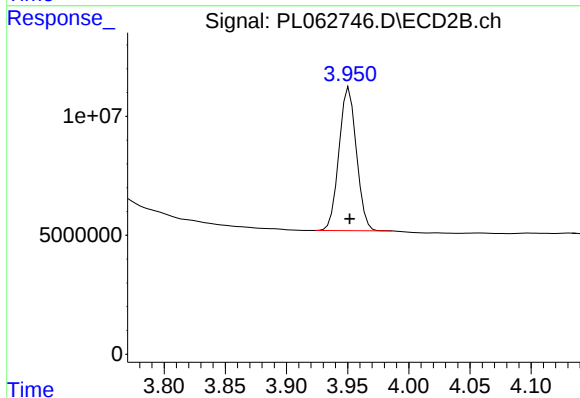


#1 Tetrachloro-m-xylene

R.T.: 3.951 min  
Delta R.T.: 0.000 min  
Response: 59717680  
Conc: 20.32 ng/ml

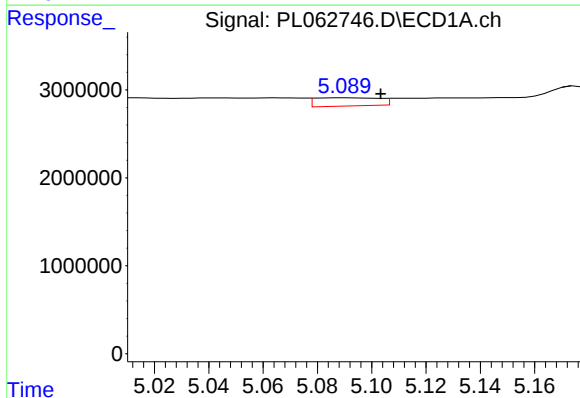


#8 Heptachlor epoxide

R.T.: 5.090 min  
Delta R.T.: -0.013 min  
Response: 1535163  
Conc: 0.84 ng/ml

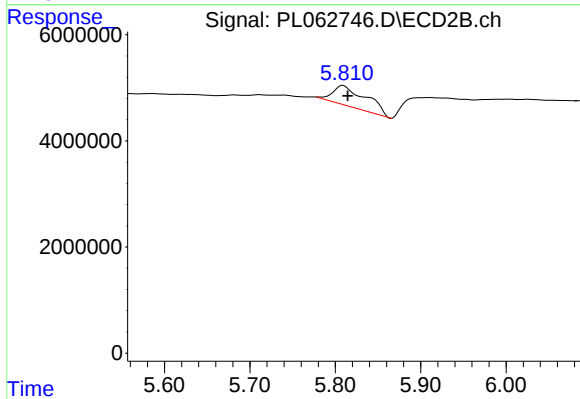

#8 Heptachlor epoxide


R.T.: 5.809 min  
Delta R.T.: -0.005 min  
Response: 10562939  
Conc: 3.26 ng/ml

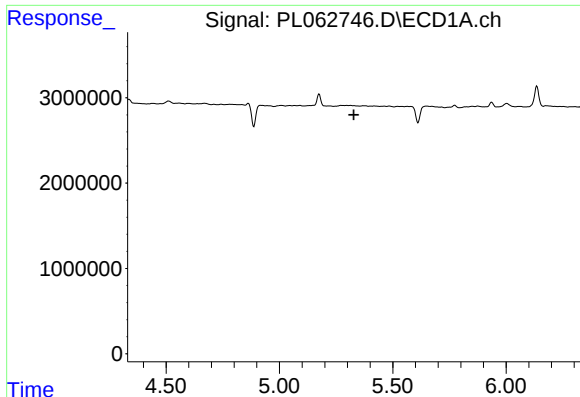

#10 gamma-Chlordane


R.T.: 0.000 min  
Exp R.T.: 5.328 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

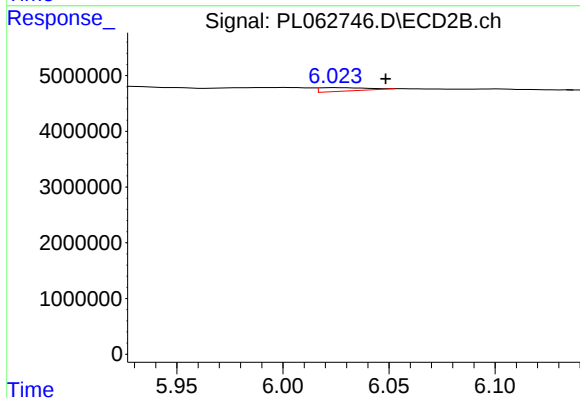


#10 gamma-Chlordane

R.T.: 6.025 min  
Delta R.T.: -0.023 min  
Response: 948787  
Conc: 0.28 ng/ml

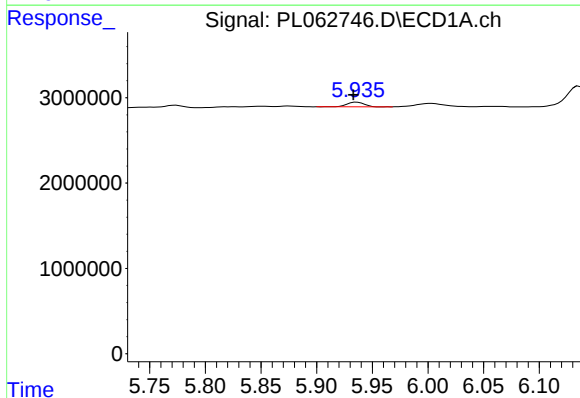


#14 Endrin

R.T.: 5.936 min  
Delta R.T.: 0.003 min  
Response: 589299  
Conc: 0.35 ng/ml

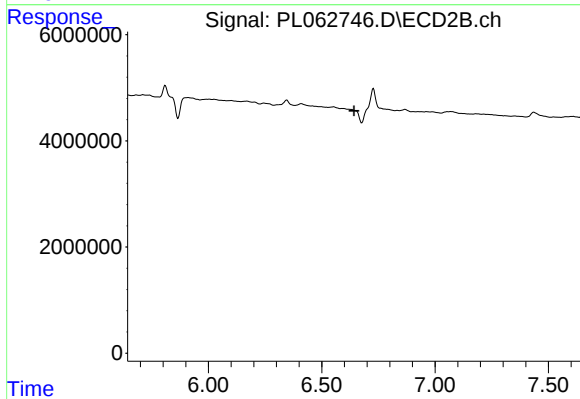

#14 Endrin


R.T.: 0.000 min  
Exp R.T.: 6.643 min  
Response: 0  
Conc: N.D.

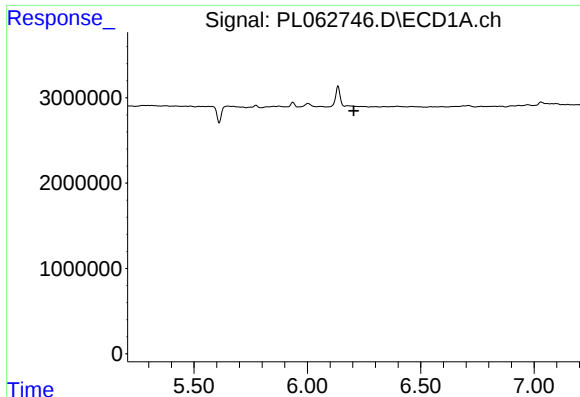

#15 Endosulfan II


R.T.: 0.000 min  
Exp R.T.: 6.205 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

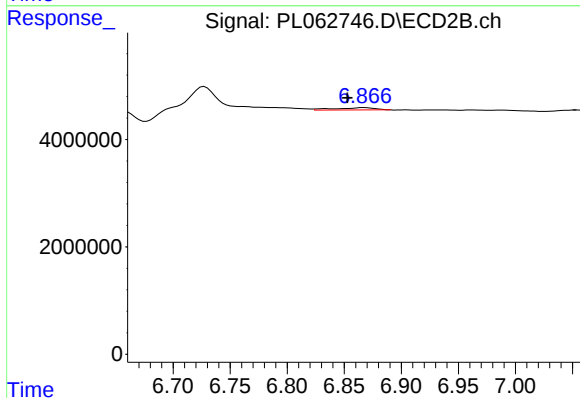


#15 Endosulfan II

R.T.: 6.867 min  
Delta R.T.: 0.015 min  
Response: 1060559  
Conc: 0.37 ng/ml

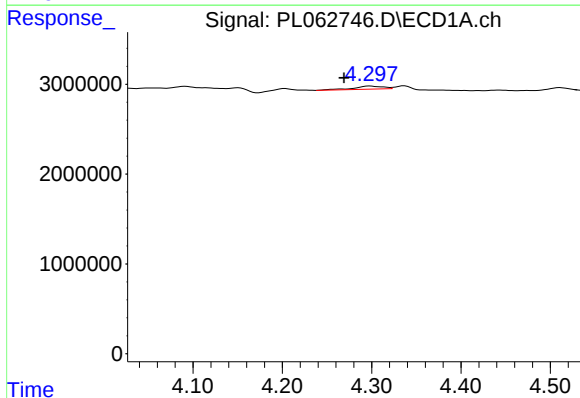


#23 Chlordane-1

R.T.: 4.298 min  
Delta R.T.: 0.029 min  
Response: 796840  
Conc: 15.46 ng/ml

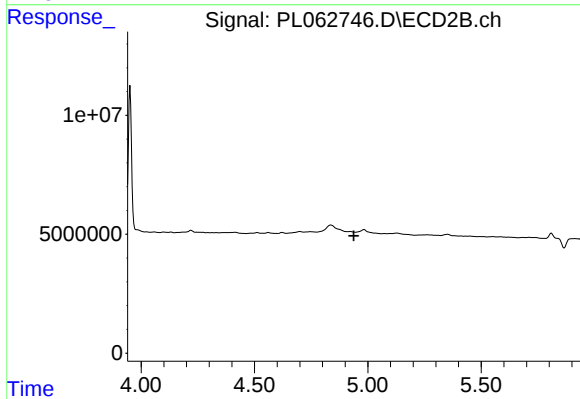

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T.: 4.938 min  
Response: 0  
Conc: N.D.

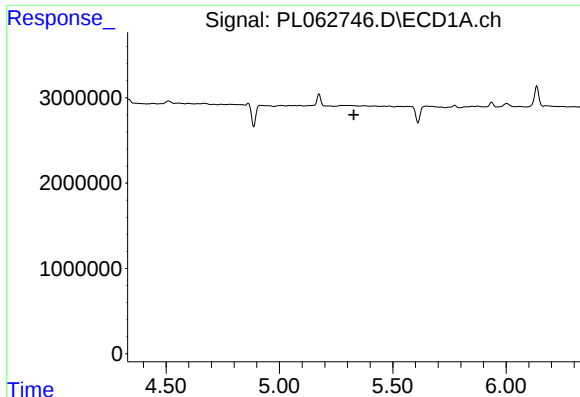

#25 Chlordane-3


R.T.: 0.000 min  
Exp R.T.: 5.328 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

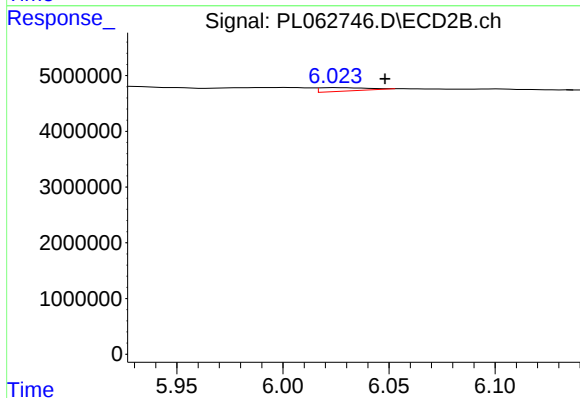


#25 Chlordane-3

R.T.: 6.025 min  
Delta R.T.: -0.023 min  
Response: 948787  
Conc: 2.35 ng/ml

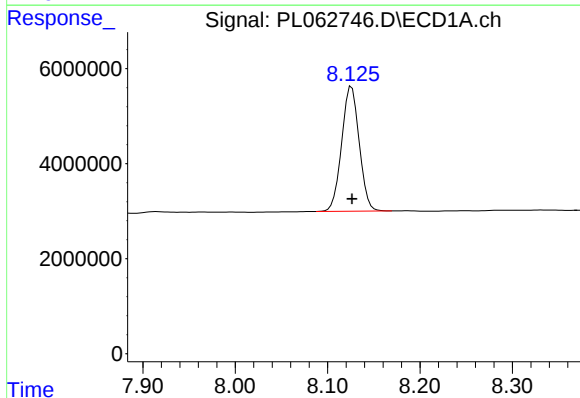

#28 Decachlorobiphenyl

R.T.: 8.126 min  
Delta R.T.: 0.000 min  
Response: 34676752  
Conc: 21.62 ng/ml

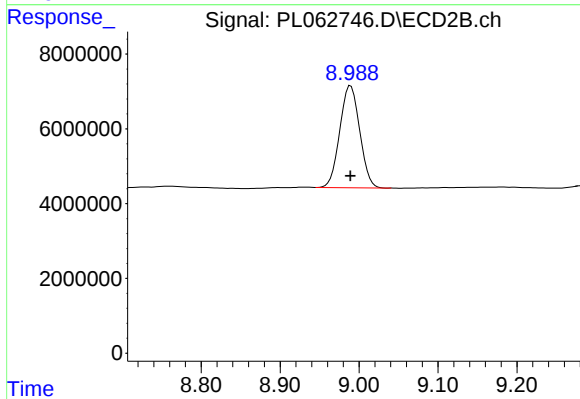

#28 Decachlorobiphenyl

R.T.: 8.989 min  
Delta R.T.: 0.000 min  
Response: 47819074  
Conc: 22.85 ng/ml