

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 21:02
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 01:48:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	35074539	59717680	20.391	20.321
28)	SA Decachlor...	8.126	8.989	34676752	47819074	21.615	22.848
Target Compounds							
8)	B Heptachlo...	5.090	5.809	1535163	10562939	0.841	3.262 #
10)	B gamma-Chl...	0.000	6.025f	0	948787	N.D.	0.282 #
14)	MA Endrin	5.936	0.000	589299	0	0.354	N.D. #
15)	B Endosulfa...	0.000	6.867	0	1060559	N.D.	0.371 #
23)	Chlordane-1	4.298f	0.000	796840	0	15.458	N.D. #
25)	Chlordane-3	0.000	6.025f	0	948787	N.D.	2.349 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 21:02
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:48:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

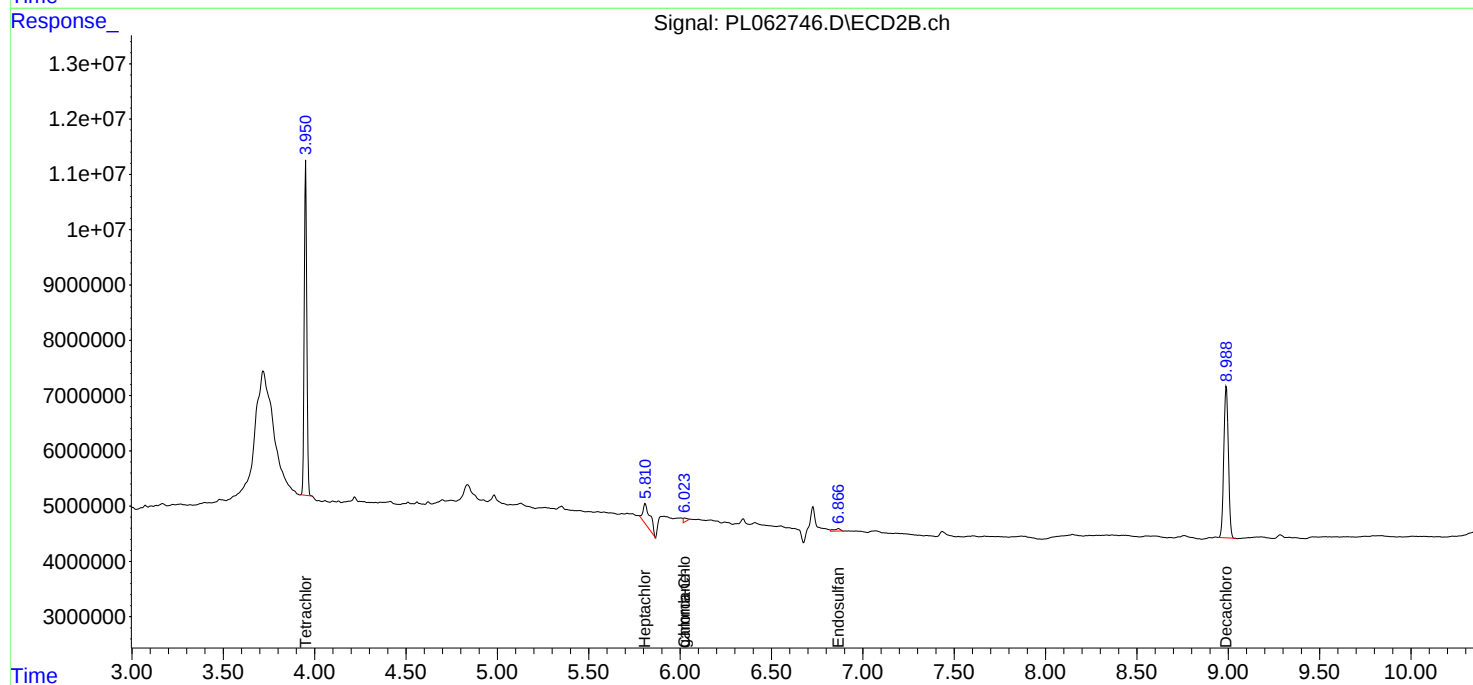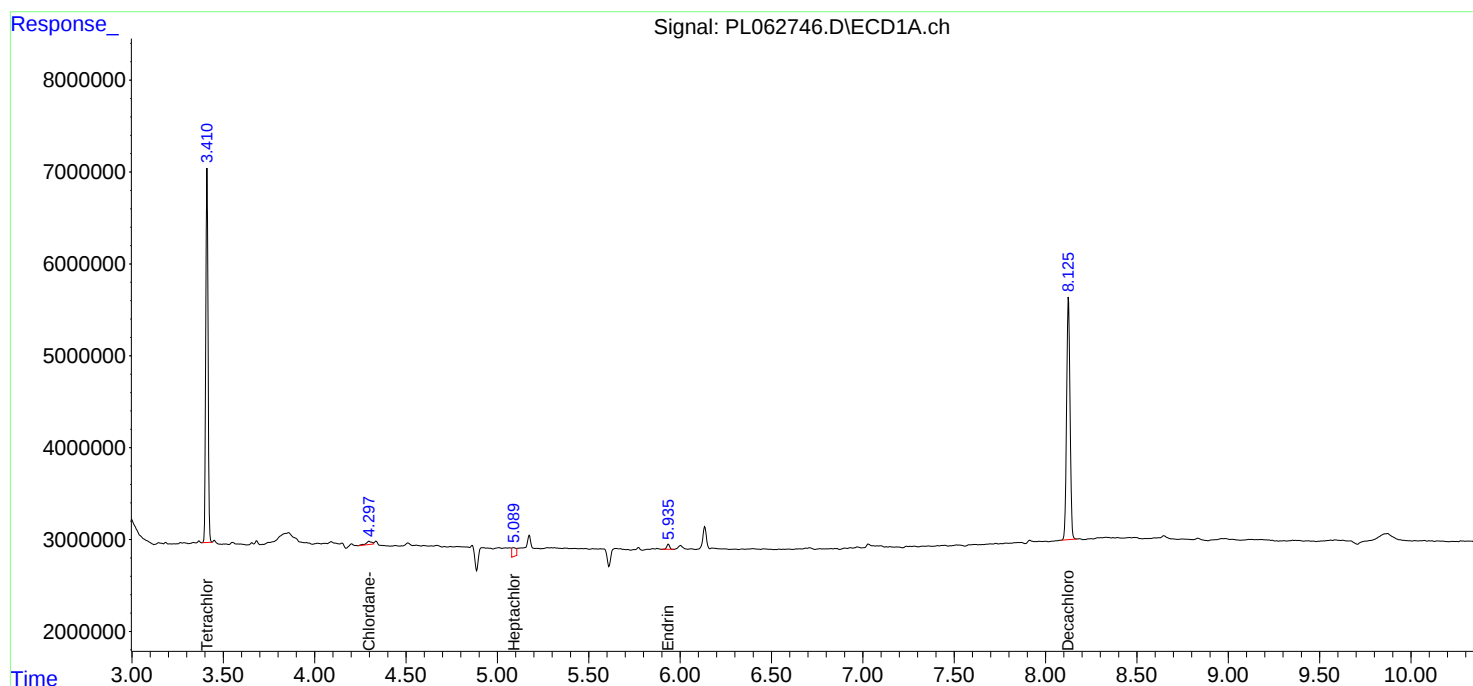


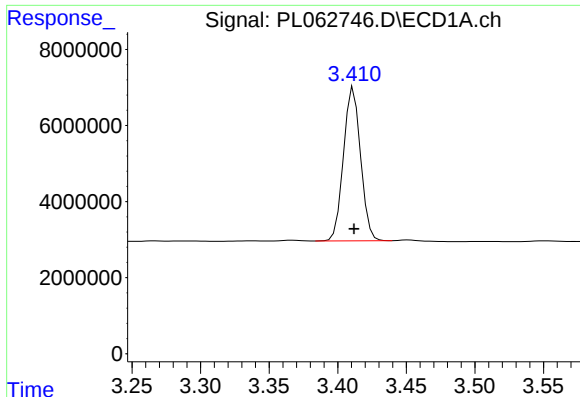

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 35074539
Conc: 20.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

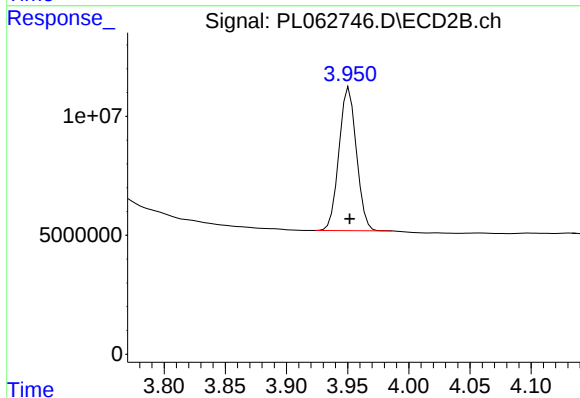


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 59717680
Conc: 20.32 ng/ml

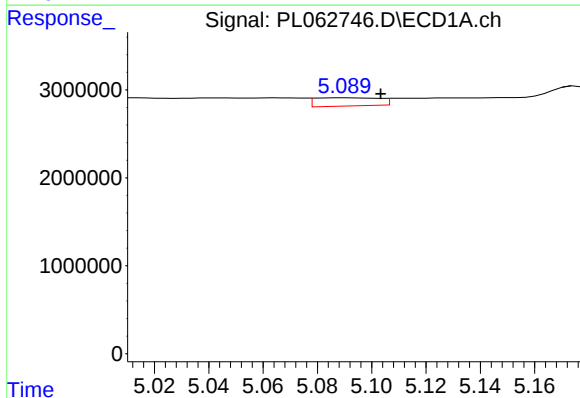


#8 Heptachlor epoxide

R.T.: 5.090 min
Delta R.T.: -0.013 min
Response: 1535163
Conc: 0.84 ng/ml

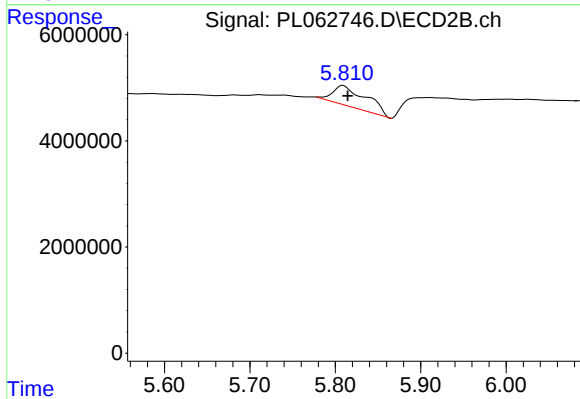

#8 Heptachlor epoxide


R.T.: 5.809 min
Delta R.T.: -0.005 min
Response: 10562939
Conc: 3.26 ng/ml

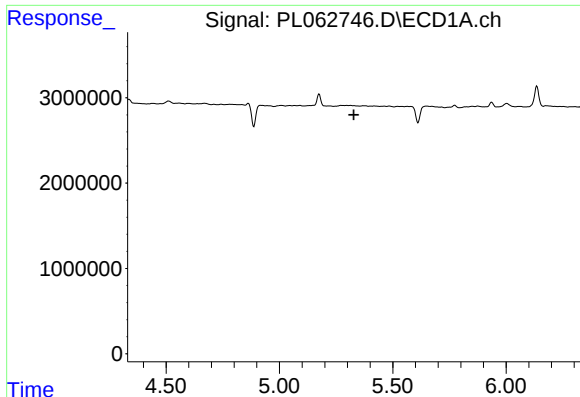

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

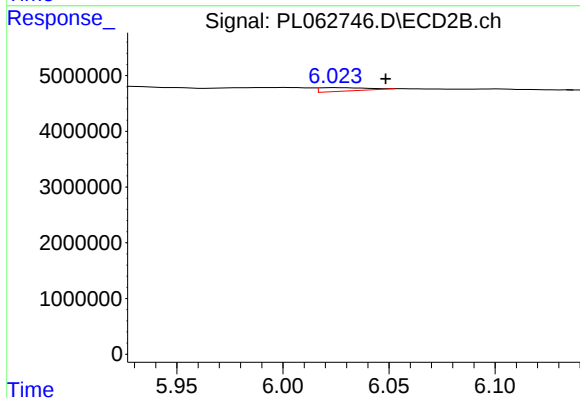


#10 gamma-Chlordane

R.T.: 6.025 min
Delta R.T.: -0.023 min
Response: 948787
Conc: 0.28 ng/ml

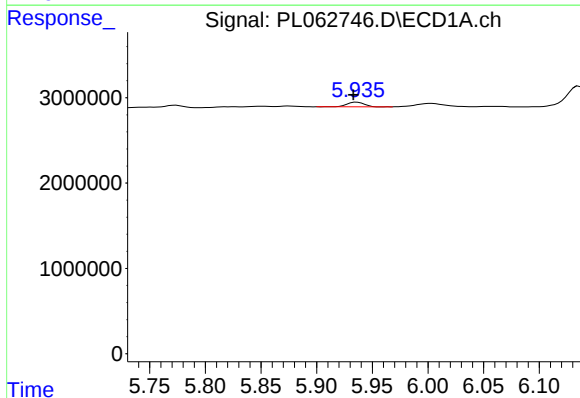


#14 Endrin

R.T.: 5.936 min
Delta R.T.: 0.003 min
Response: 589299
Conc: 0.35 ng/ml

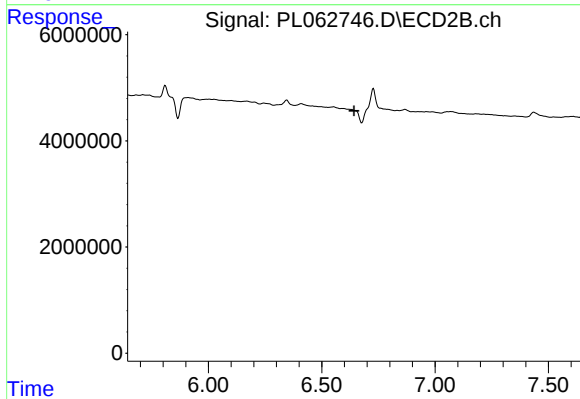

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.643 min
Response: 0
Conc: N.D.

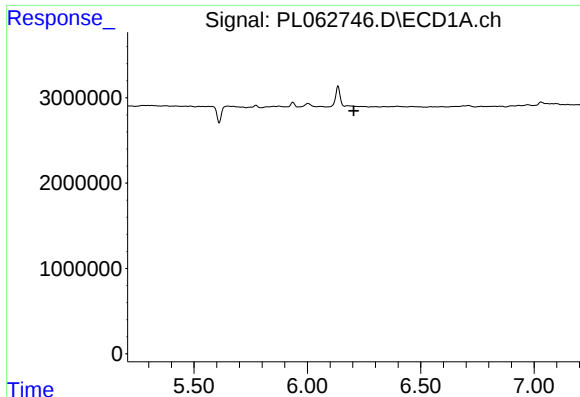

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

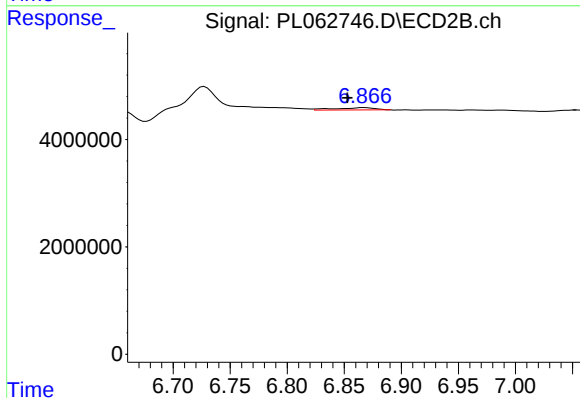


#15 Endosulfan II

R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 1060559
Conc: 0.37 ng/ml

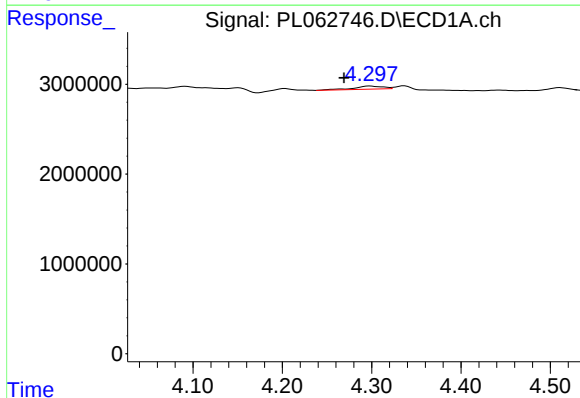


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.029 min
Response: 796840
Conc: 15.46 ng/ml

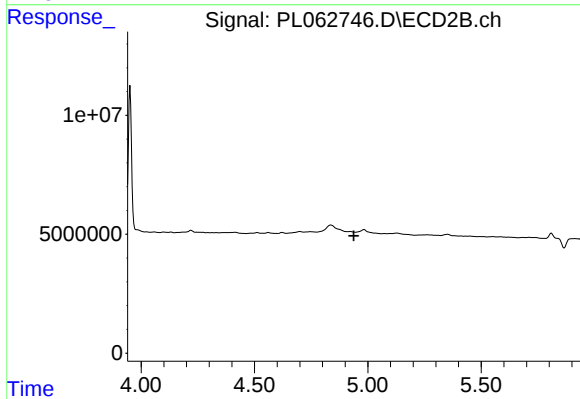

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

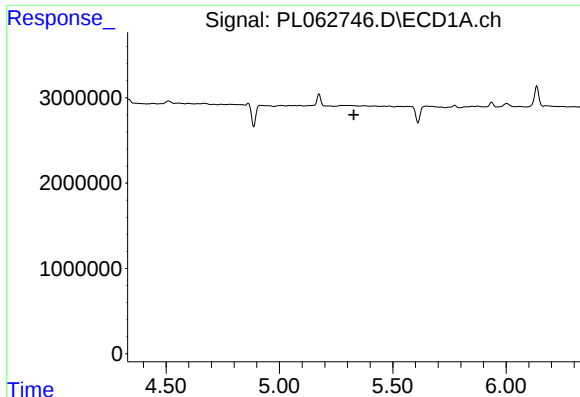

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

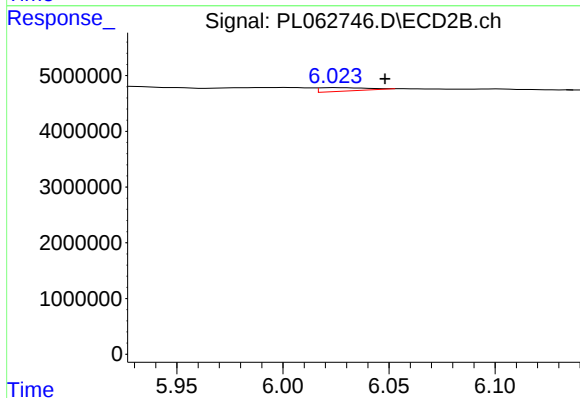


#25 Chlordane-3

R.T.: 6.025 min
Delta R.T.: -0.023 min
Response: 948787
Conc: 2.35 ng/ml

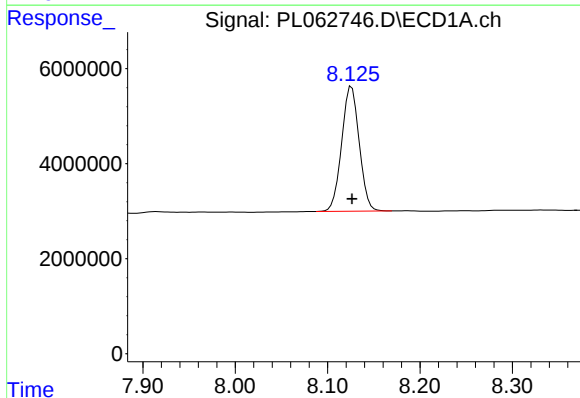

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 34676752
Conc: 21.62 ng/ml

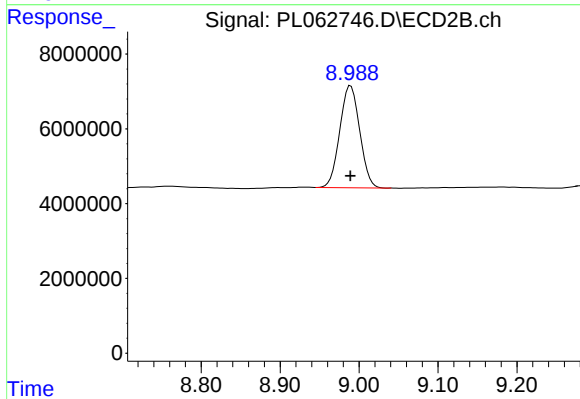

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 47819074
Conc: 22.85 ng/ml