

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 21:16
 Operator : DD\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 01:49:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	84527410	150.5E6	49.142	51.208
2)	SA Decachlor...	8.125	8.990	81996744	113.7E6	51.111	54.342
Target Compounds							
2)	A alpha-BHC	3.844	4.337	123.5E6	230.3E6	48.453	51.820
3)	MA gamma-BHC...	4.123	4.620	111.0E6	211.7E6	47.896	50.702
4)	MA Heptachlor	4.420	5.125	97853103	187.7E6	45.602	47.064
5)	MB Aldrin	4.664	5.428	92510373	184.2E6	48.467	50.903
6)	B beta-BHC	4.372	4.791	46454147	90600552	48.633	48.114
7)	B delta-BHC	4.572	5.006	104.1E6	193.2E6	47.920	55.197
8)	B Heptachlo...	5.103	5.814	89144796	171.4E6	48.857	52.913
9)	A Endosulfan I	5.437	6.168	81316705	152.2E6	48.646	48.246
10)	B gamma-Chl...	5.328	6.047	87995179	166.3E6	48.843	49.407
11)	B alpha-Chl...	5.385	6.119	86739281	164.4E6	47.982	48.792
12)	B 4,4'-DDE	5.550	6.278	80681290	157.2E6	48.766	48.797
13)	MA Dieldrin	5.678	6.425	86095784	154.6E6	48.725	48.299
14)	MA Endrin	5.933	6.641	69054888	113.8E6	41.505	40.756
15)	B Endosulfa...	6.205	6.852	79123073	130.3E6	47.993	45.586
16)	A 4,4'-DDD	6.062	6.767	79494392	137.0E6	56.200	53.498
17)	MA 4,4'-DDT	6.300	7.065	49562531	87488751	37.138	38.966
18)	B Endrin al...	6.372	6.976	69216680	112.3E6	47.667	49.260
19)	B Endosulfa...	6.584	7.199	77696953	120.1E6	47.082	50.075
20)	A Methoxychlor	6.844	7.525	33473962	50401496	38.865	40.794
21)	B Endrin ke...	7.070	7.668	95609375	133.4E6	53.027	56.288
22)	Mirex	7.256	8.121	67567458	87244870	47.660	51.198
23)	Chlordane-1	4.297f	0.000	318430	0	6.177	N.D. #
24)	Chlordane-2	0.000	5.428f	0	184.2E6	N.D.	1689.759 #
25)	Chlordane-3	5.328	6.047	87995179	166.3E6	574.648	411.748 #
26)	Chlordane-4	5.385	6.119	86739281	164.4E6	665.890	339.416 #
27)	Chlordane-5	6.205	0.000	79123073	0	1640.004	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 21:16
Operator : DD\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:49:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

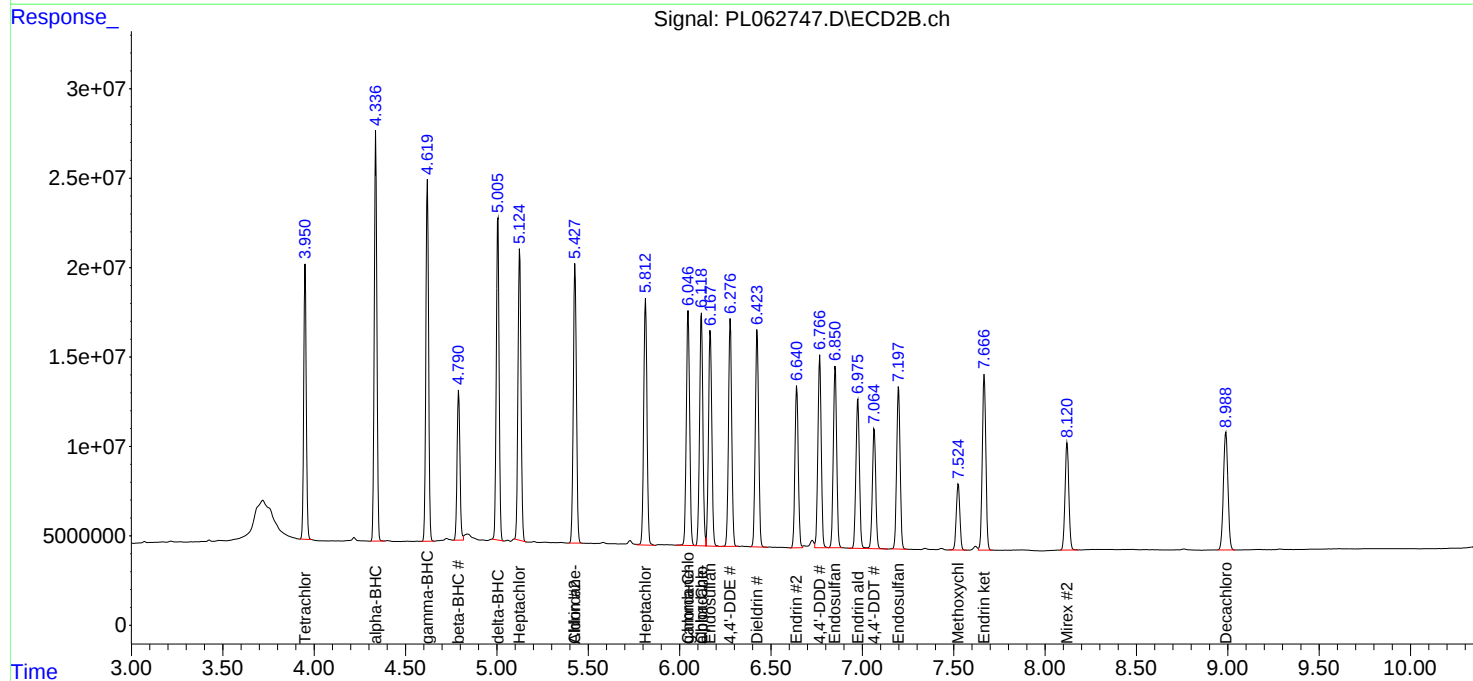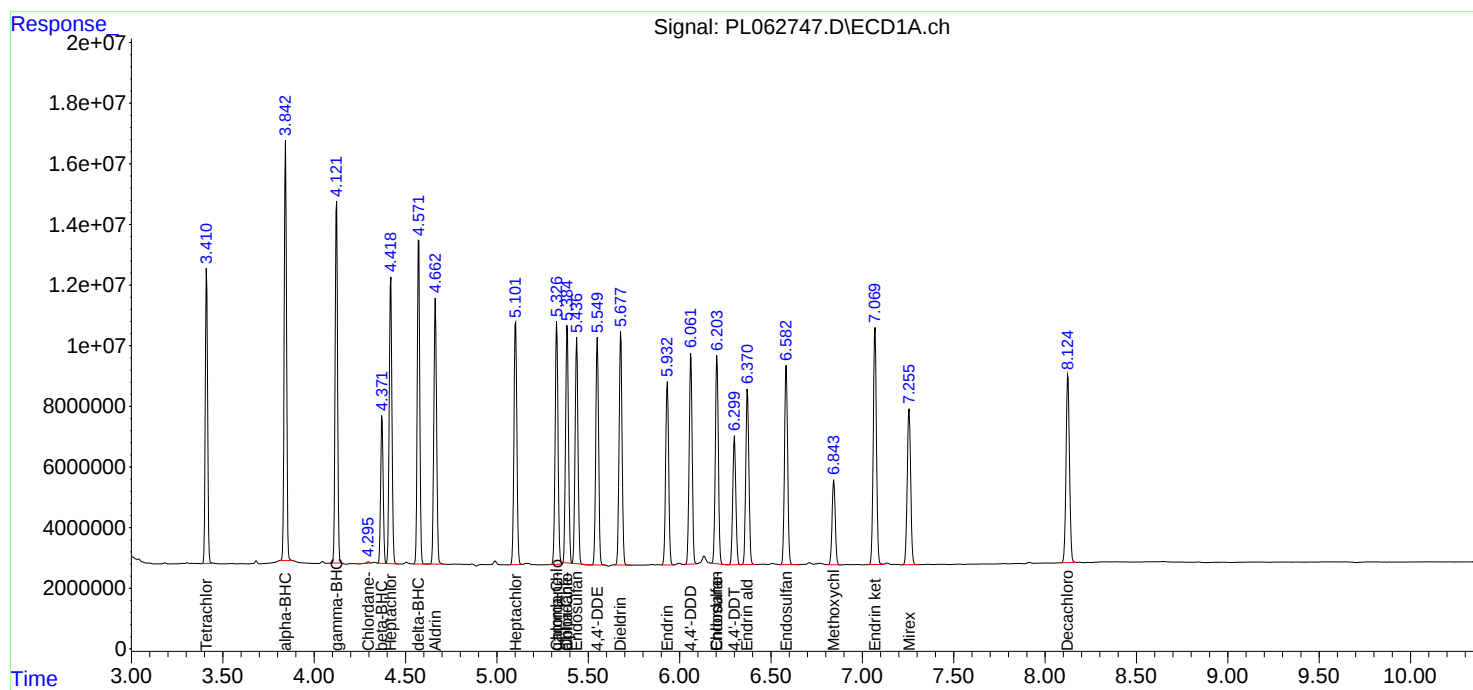


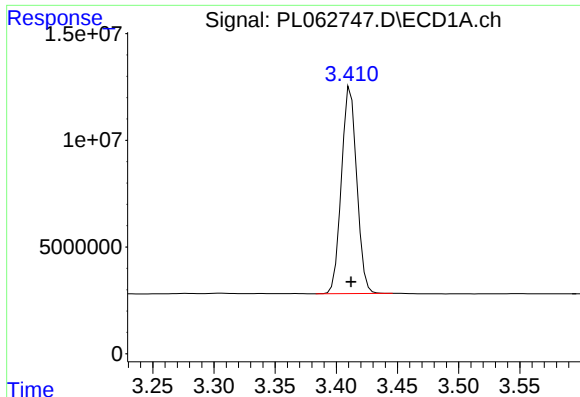

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 84527410
Conc: 49.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

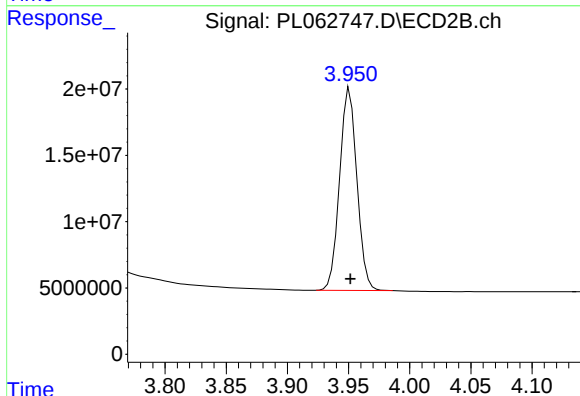


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 150487190
Conc: 51.21 ng/ml

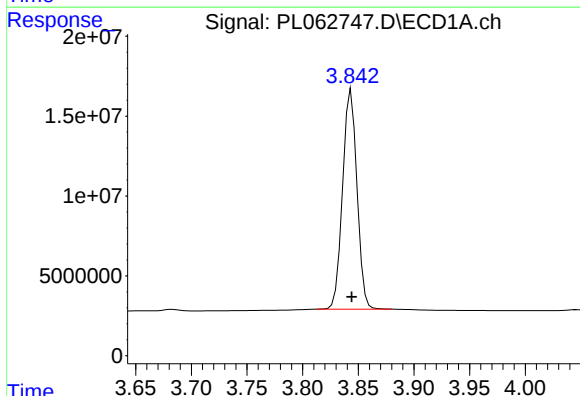


#2 alpha-BHC

R.T.: 3.844 min
Delta R.T.: 0.000 min
Response: 123541537
Conc: 48.45 ng/ml

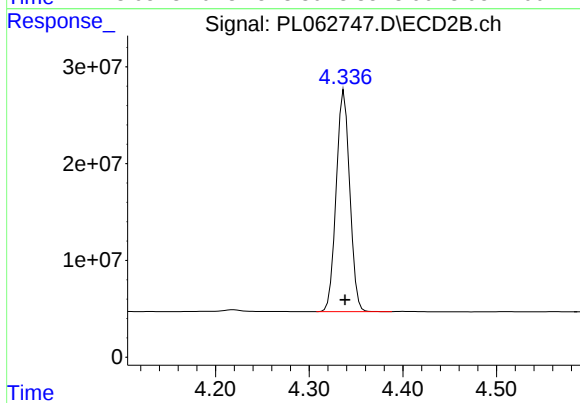

#2 alpha-BHC


R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 230250162
Conc: 51.82 ng/ml

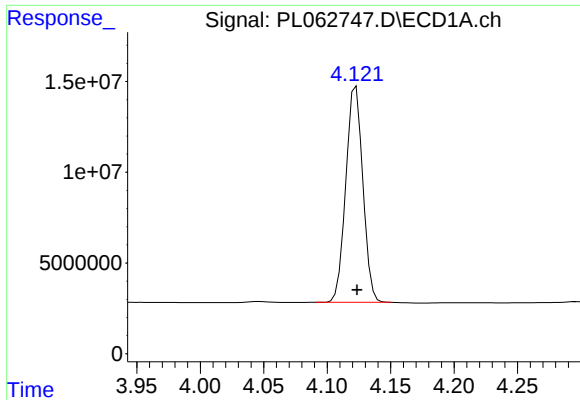

#3 gamma-BHC (Lindane)


R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 110959223
Conc: 47.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

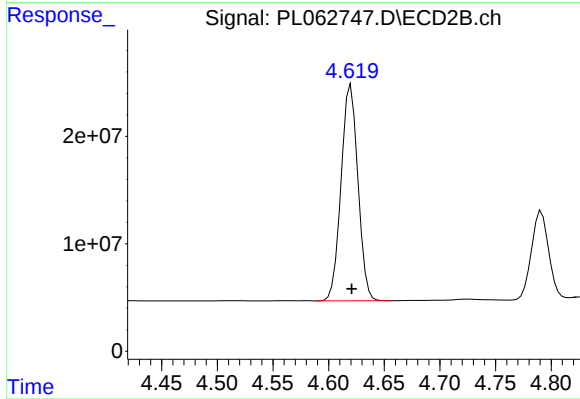


#3 gamma-BHC (Lindane)

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 211716682
Conc: 50.70 ng/ml

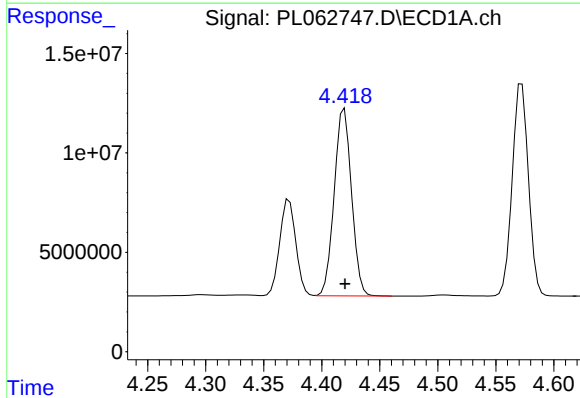


#4 Heptachlor

R.T.: 4.420 min
Delta R.T.: 0.000 min
Response: 97853103
Conc: 45.60 ng/ml

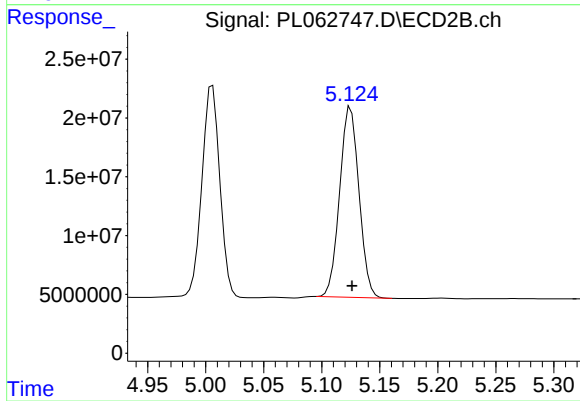

#4 Heptachlor


R.T.: 5.125 min
Delta R.T.: -0.001 min
Response: 187688393
Conc: 47.06 ng/ml

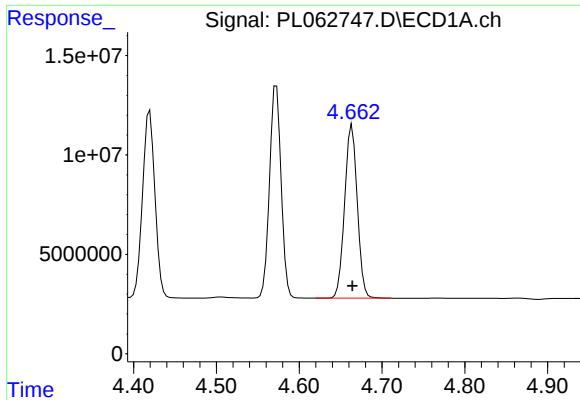

#5 Aldrin


R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 92510373
Conc: 48.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

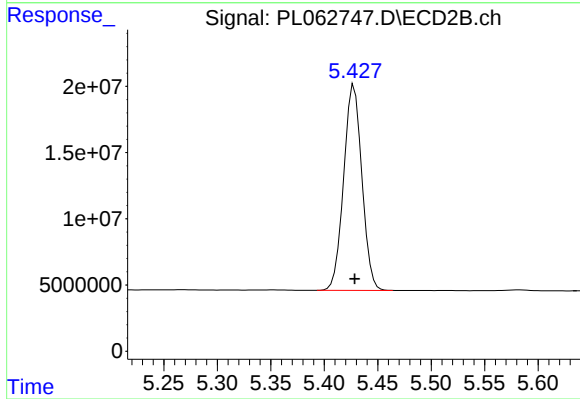


#5 Aldrin

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 184244420
Conc: 50.90 ng/ml

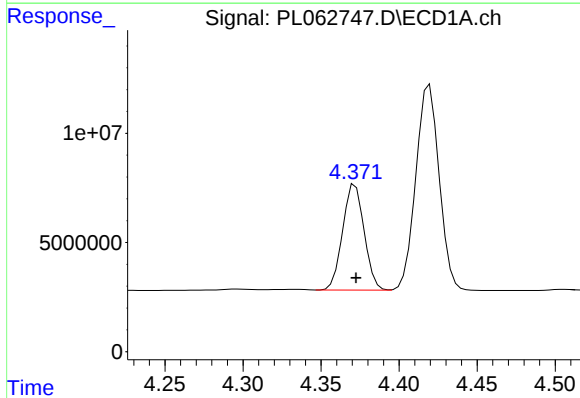


#6 beta-BHC

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 46454147
Conc: 48.63 ng/ml

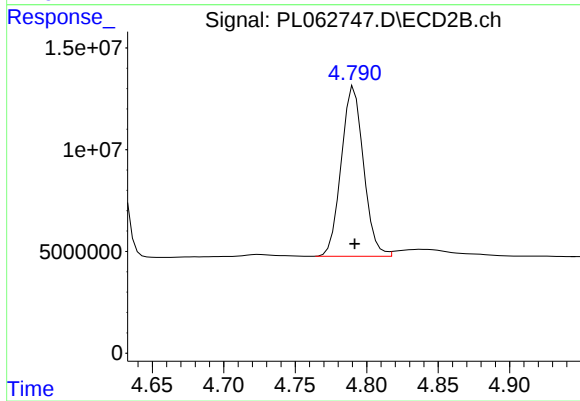

#6 beta-BHC


R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 90600552
Conc: 48.11 ng/ml

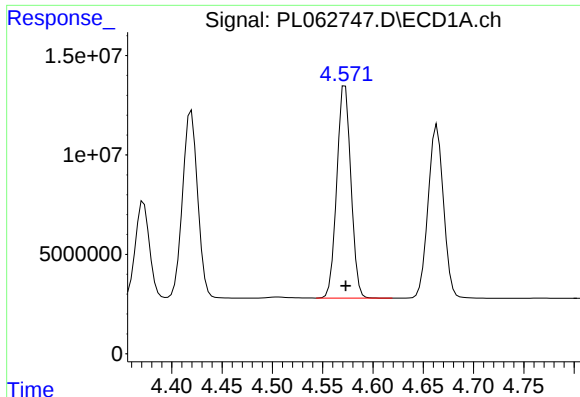

#7 delta-BHC


R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 104140822
Conc: 47.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

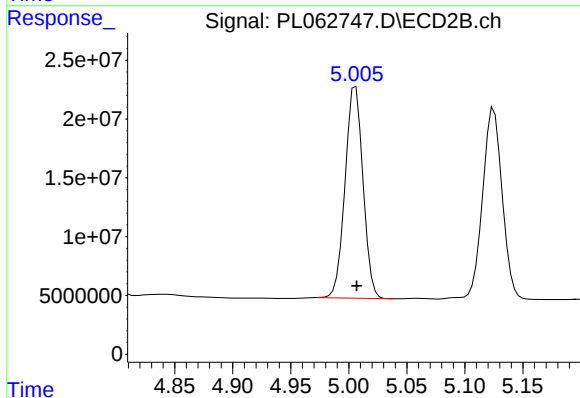


#7 delta-BHC

R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 193159148
Conc: 55.20 ng/ml

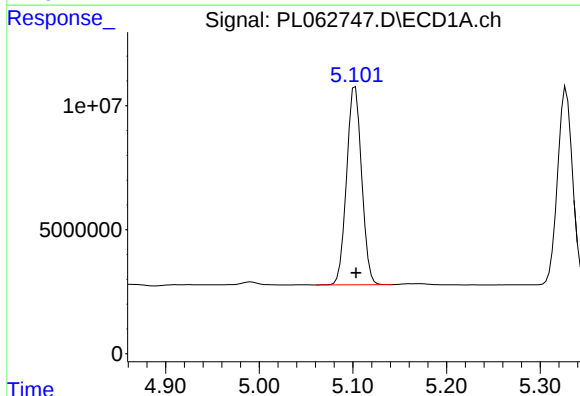


#8 Heptachlor epoxide

R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 89144796
Conc: 48.86 ng/ml

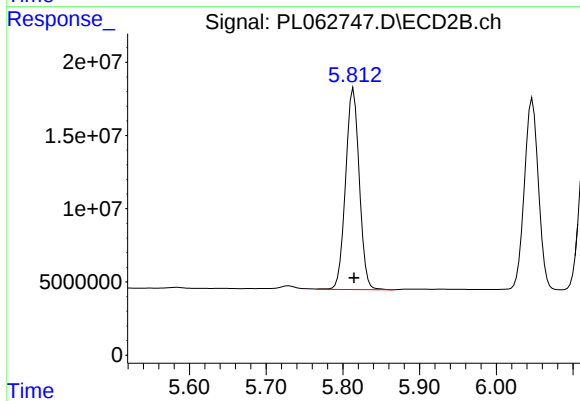

#8 Heptachlor epoxide


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 171366105
Conc: 52.91 ng/ml

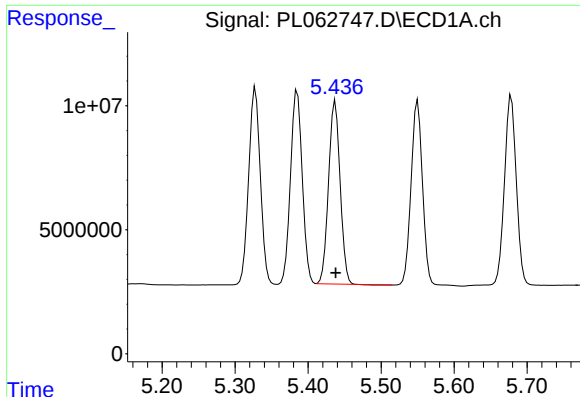

#9 Endosulfan I


R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 81316705
Conc: 48.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

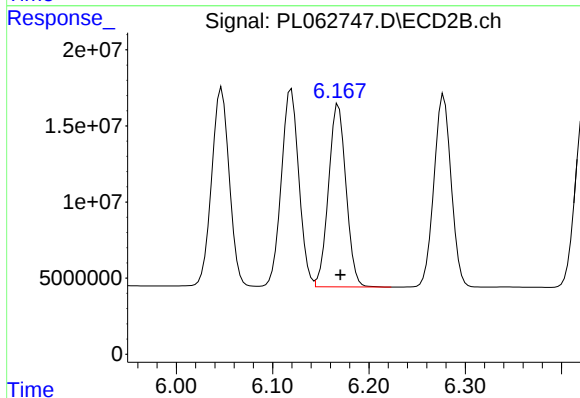


#9 Endosulfan I

R.T.: 6.168 min
Delta R.T.: -0.002 min
Response: 152160349
Conc: 48.25 ng/ml

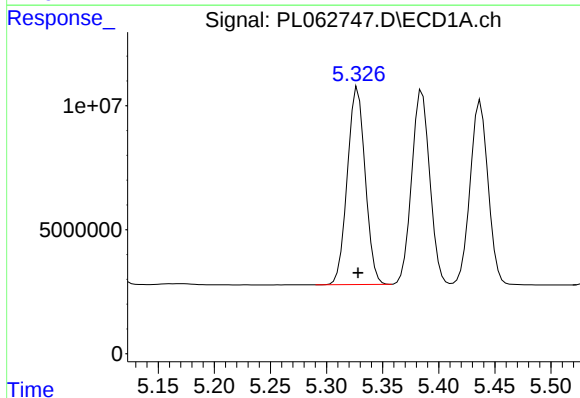


#10 gamma-Chlordane

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 87995179
Conc: 48.84 ng/ml

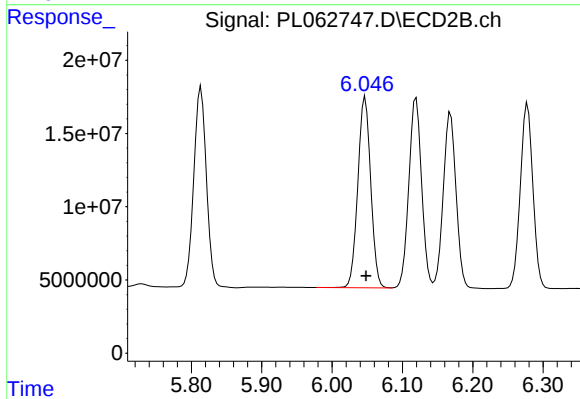

#10 gamma-Chlordane


R.T.: 6.047 min
Delta R.T.: -0.001 min
Response: 166321956
Conc: 49.41 ng/ml

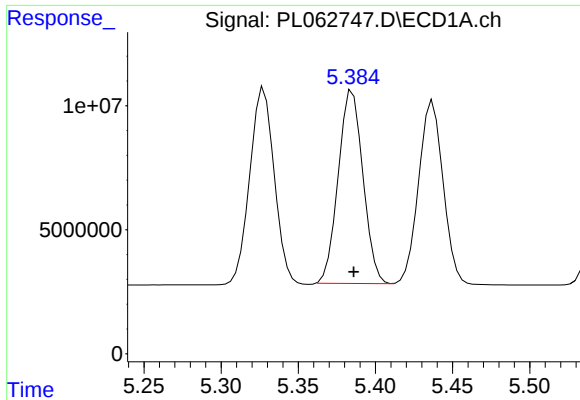

#11 alpha-Chlordane


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 86739281
Conc: 47.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

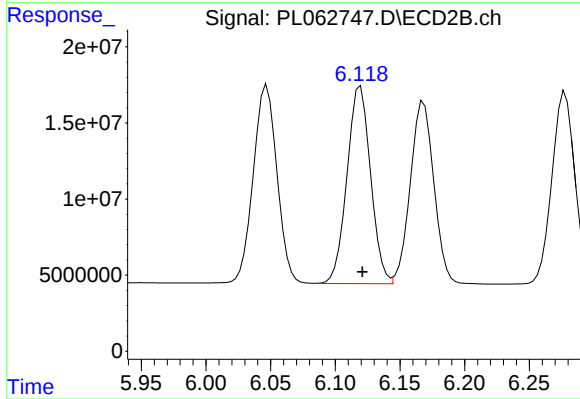


#11 alpha-Chlordane

R.T.: 6.119 min
Delta R.T.: -0.002 min
Response: 164374888
Conc: 48.79 ng/ml

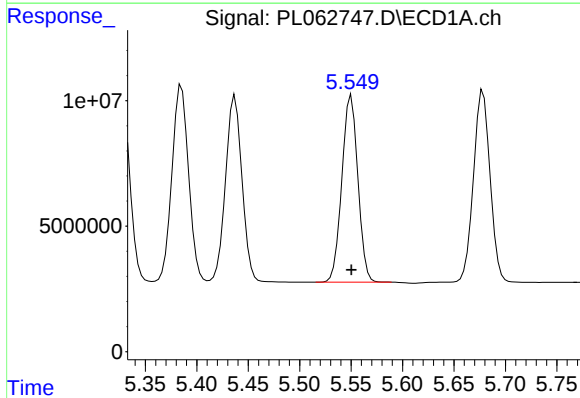


#12 4,4'-DDE

R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 80681290
Conc: 48.77 ng/ml

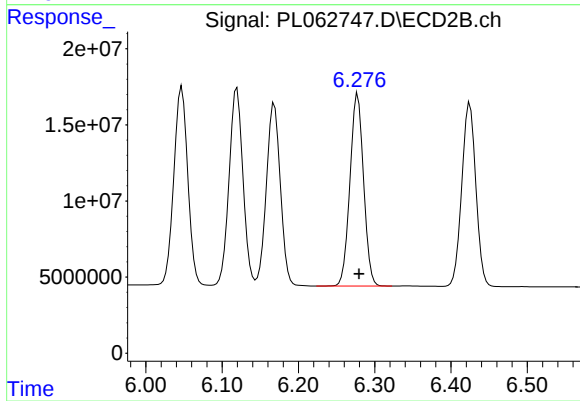

#12 4,4'-DDE


R.T.: 6.278 min
Delta R.T.: -0.002 min
Response: 157225899
Conc: 48.80 ng/ml

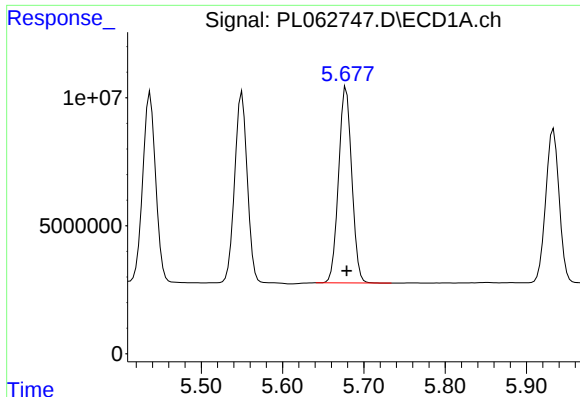

#13 Dieldrin


R.T.: 5.678 min
Delta R.T.: 0.000 min
Response: 86095784
Conc: 48.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

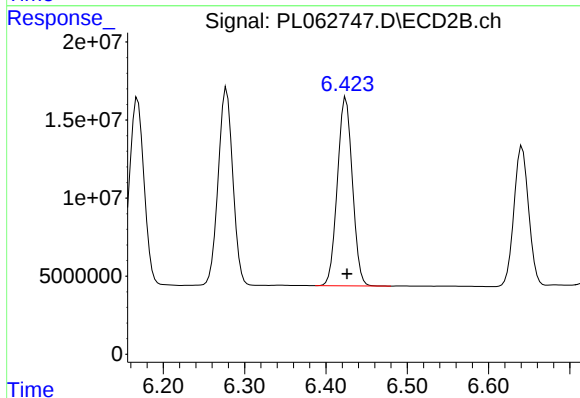


#13 Dieldrin

R.T.: 6.425 min
Delta R.T.: -0.002 min
Response: 154599333
Conc: 48.30 ng/ml

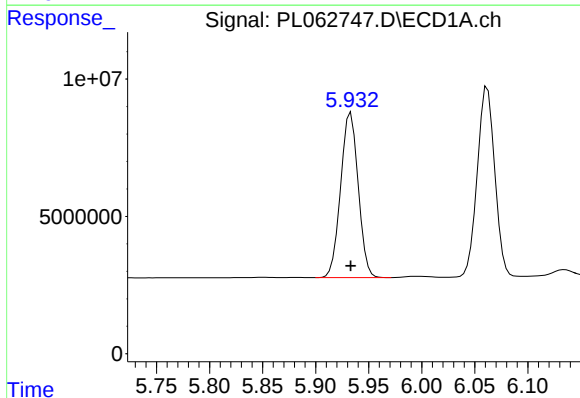


#14 Endrin

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 69054888
Conc: 41.50 ng/ml

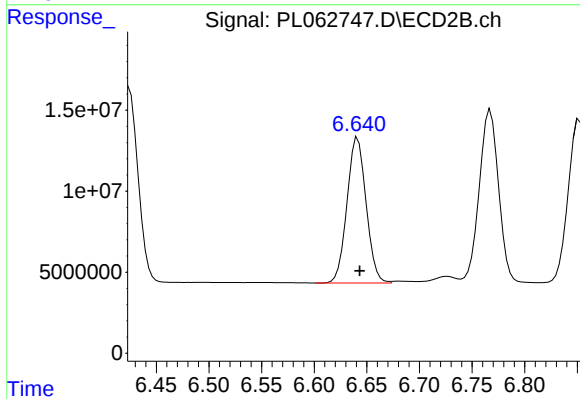

#14 Endrin


R.T.: 6.641 min
Delta R.T.: -0.002 min
Response: 113753970
Conc: 40.76 ng/ml

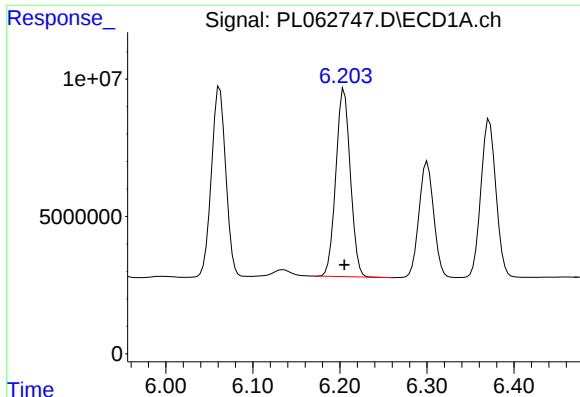

#15 Endosulfan II


R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 79123073
Conc: 47.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

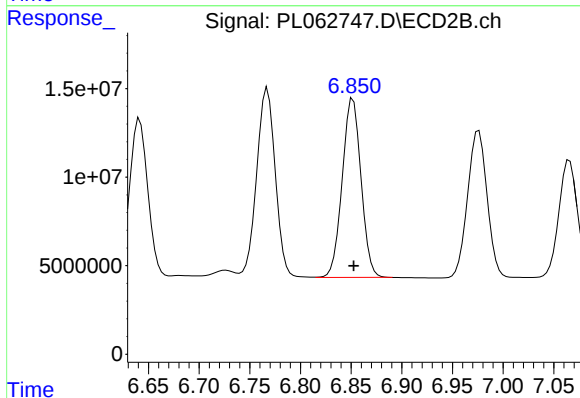


#15 Endosulfan II

R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 130315245
Conc: 45.59 ng/ml

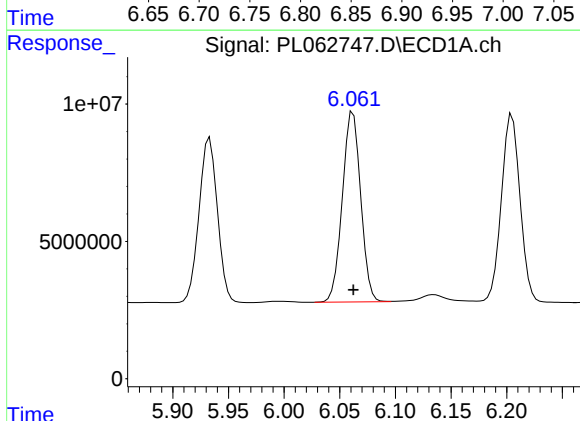


#16 4,4'-DDD

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 79494392
Conc: 56.20 ng/ml

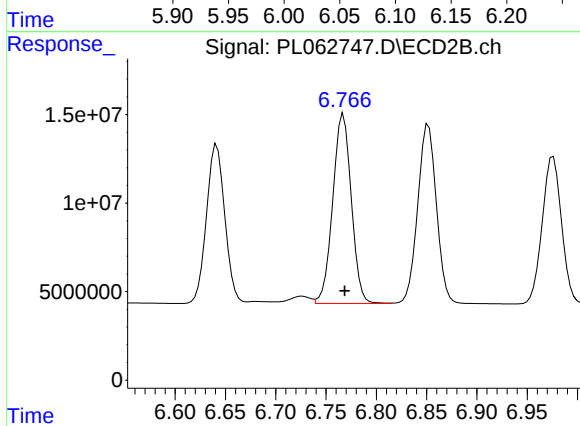

#16 4,4'-DDD


R.T.: 6.767 min
Delta R.T.: -0.001 min
Response: 136953897
Conc: 53.50 ng/ml

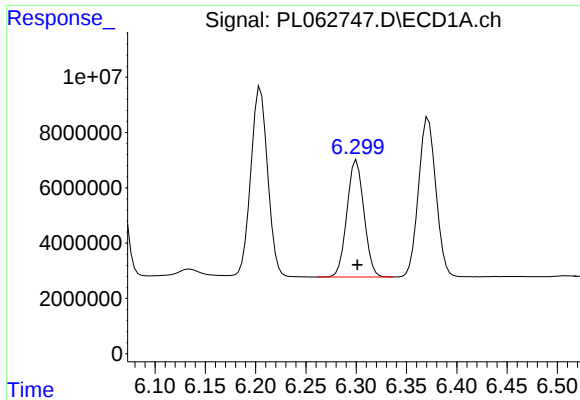

#17 4,4'-DDT


R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 49562531
Conc: 37.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

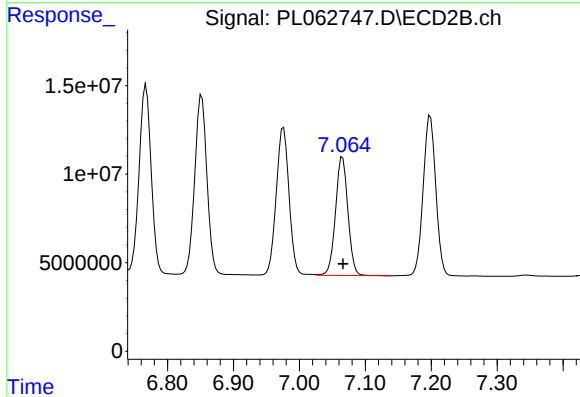


#17 4,4'-DDT

R.T.: 7.065 min
Delta R.T.: 0.000 min
Response: 87488751
Conc: 38.97 ng/ml

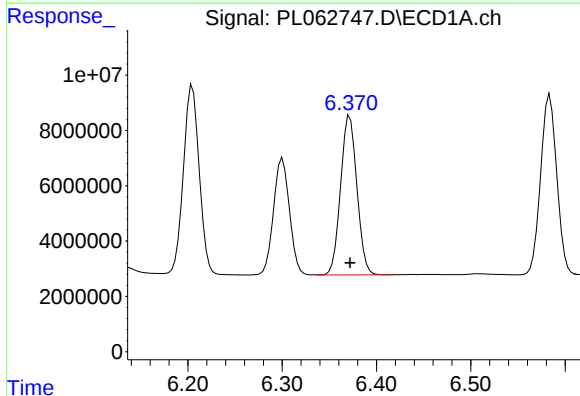


#18 Endrin aldehyde

R.T.: 6.372 min
Delta R.T.: 0.000 min
Response: 69216680
Conc: 47.67 ng/ml

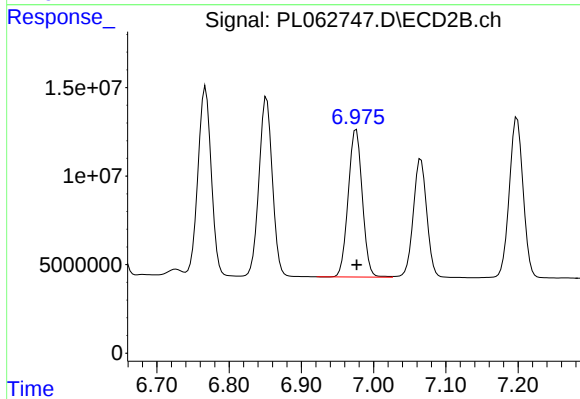

#18 Endrin aldehyde


R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 112342610
Conc: 49.26 ng/ml

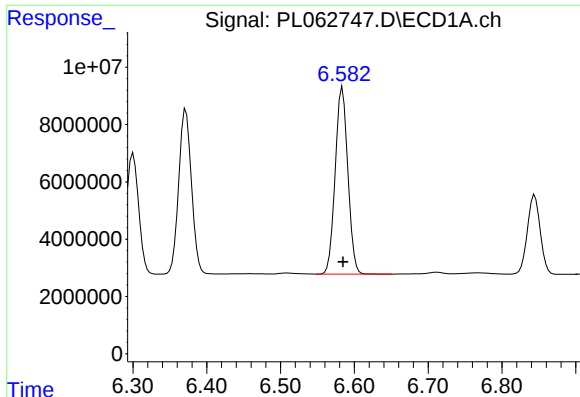

#19 Endosulfan Sulfate


R.T.: 6.584 min
Delta R.T.: 0.000 min
Response: 77696953
Conc: 47.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

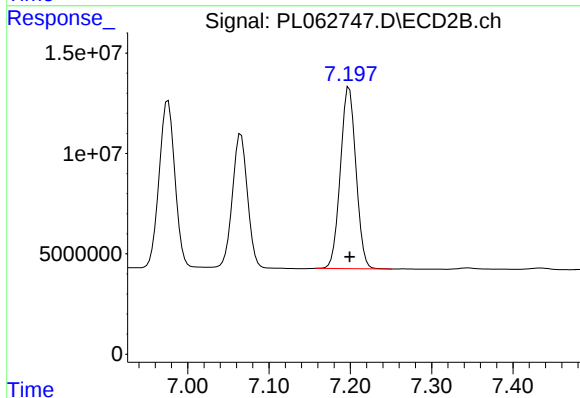


#19 Endosulfan Sulfate

R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 120140438
Conc: 50.07 ng/ml

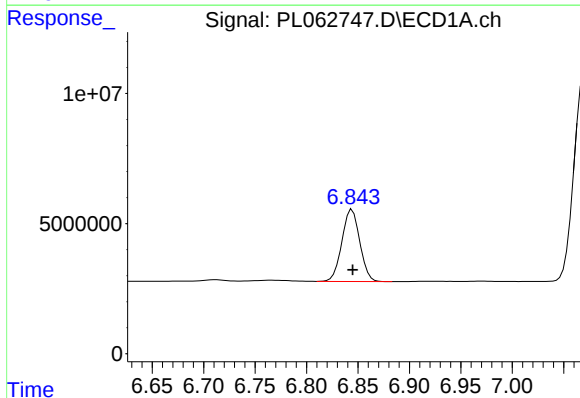


#20 Methoxychlor

R.T.: 6.844 min
Delta R.T.: 0.000 min
Response: 33473962
Conc: 38.86 ng/ml

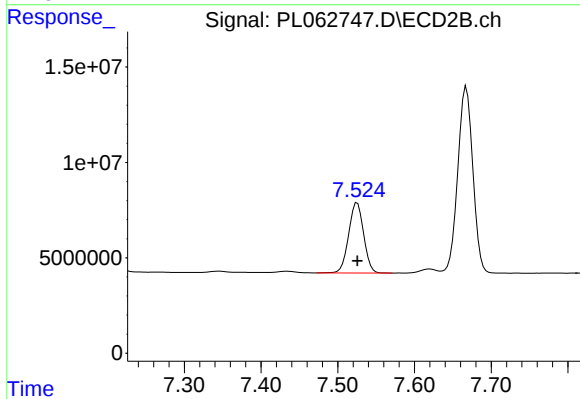

#20 Methoxychlor


R.T.: 7.525 min
Delta R.T.: 0.000 min
Response: 50401496
Conc: 40.79 ng/ml

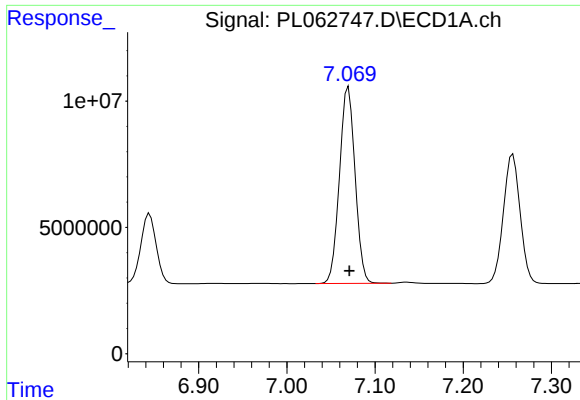

#21 Endrin ketone


R.T.: 7.070 min
Delta R.T.: -0.001 min
Response: 95609375
Conc: 53.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

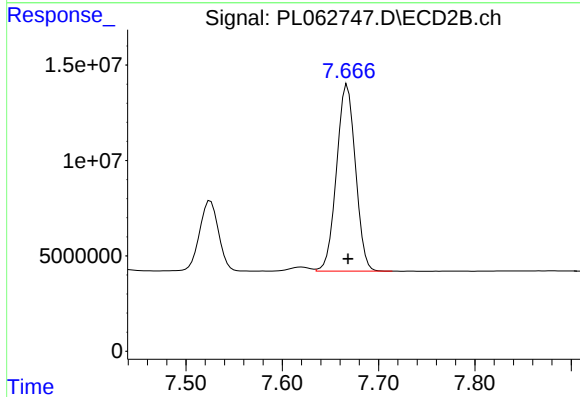


#21 Endrin ketone

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 133392546
Conc: 56.29 ng/ml

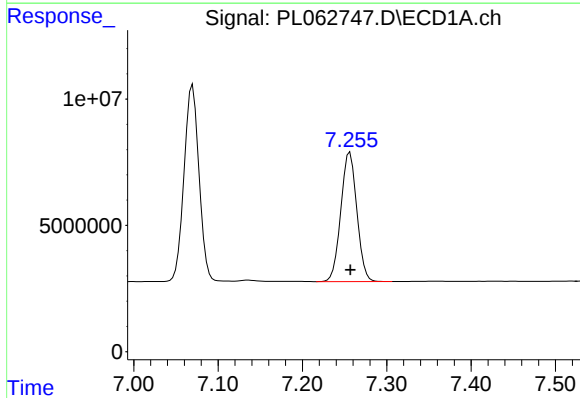


#22 Mirex

R.T.: 7.256 min
Delta R.T.: 0.000 min
Response: 67567458
Conc: 47.66 ng/ml

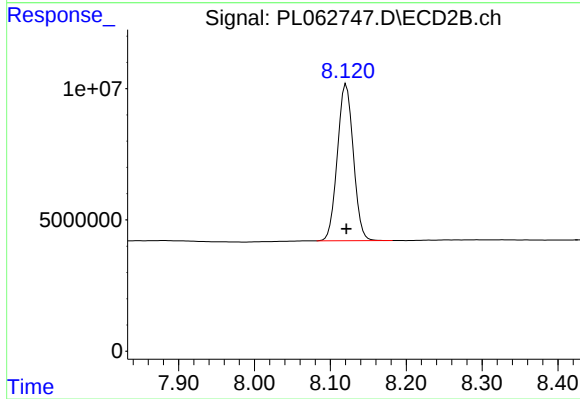

#22 Mirex


R.T.: 8.121 min
Delta R.T.: 0.000 min
Response: 87244870
Conc: 51.20 ng/ml

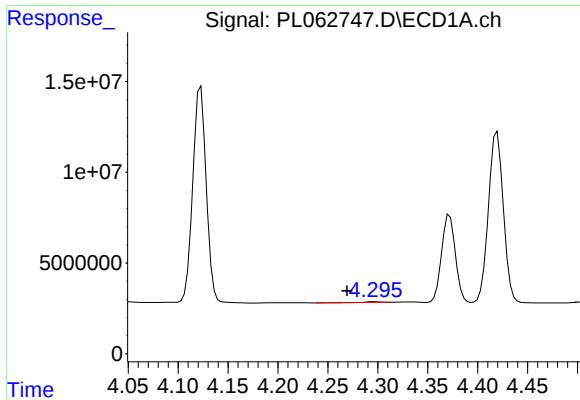

#23 Chlordane-1


R.T.: 4.297 min
Delta R.T.: 0.027 min
Response: 318430
Conc: 6.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

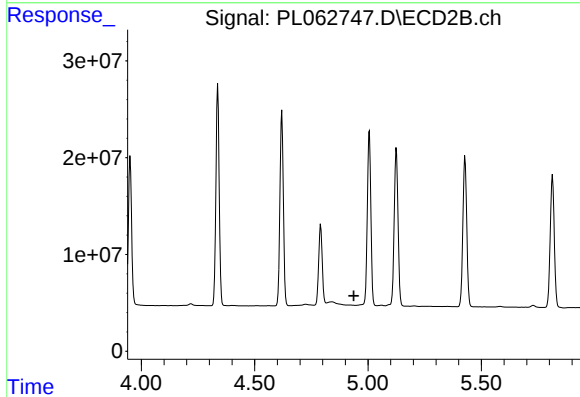


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

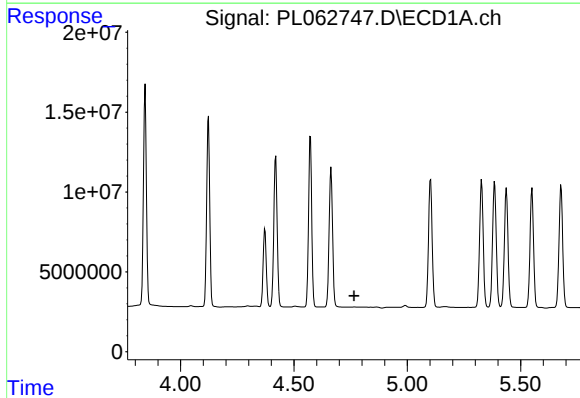


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

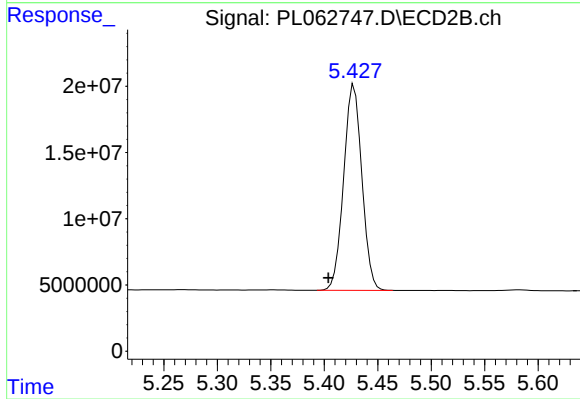

#24 Chlordane-2


R.T.: 5.428 min
Delta R.T.: 0.024 min
Response: 184244420
Conc: 1689.76 ng/ml

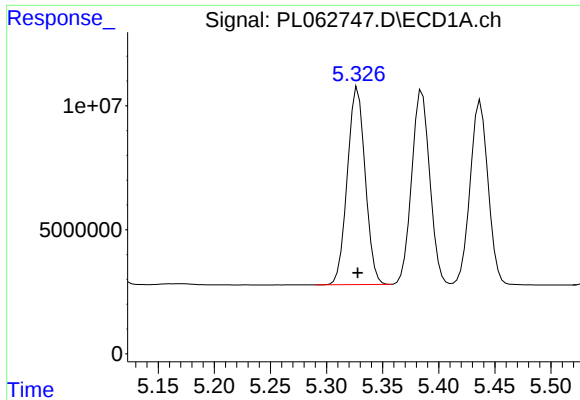

#25 Chlordane-3


R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 87995179
Conc: 574.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

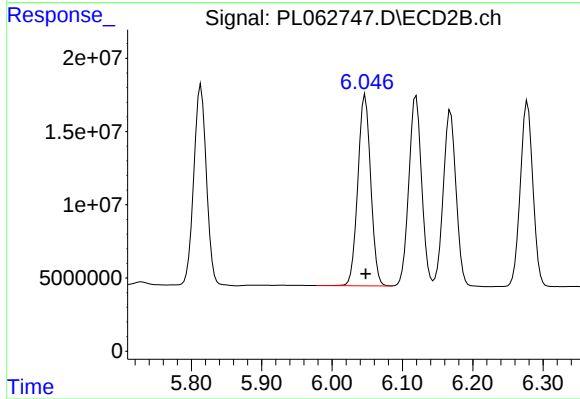


#25 Chlordane-3

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 166321956
Conc: 411.75 ng/ml

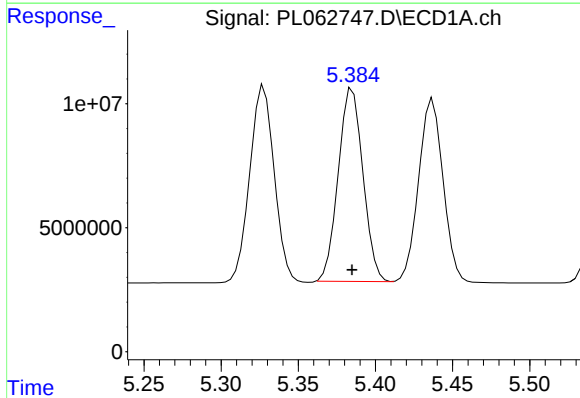


#26 Chlordane-4

R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 86739281
Conc: 665.89 ng/ml

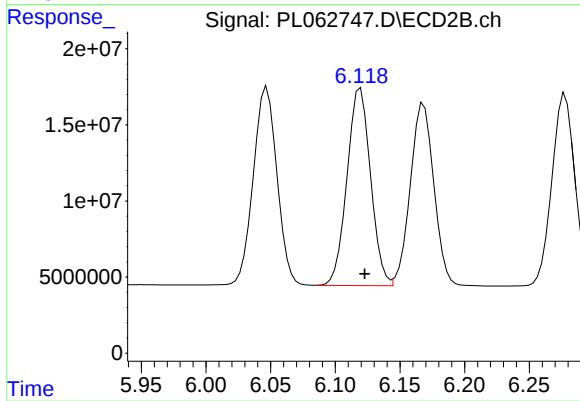

#26 Chlordane-4


R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 164374888
Conc: 339.42 ng/ml

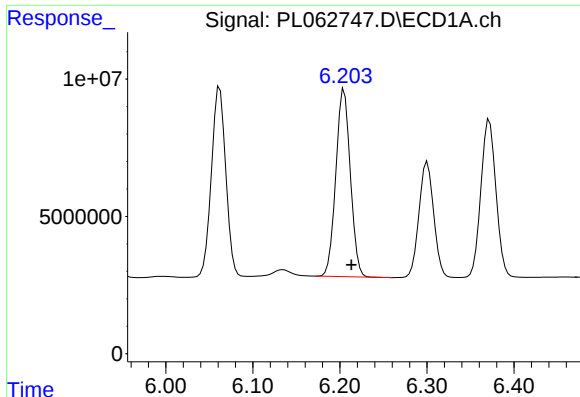

#27 Chlordane-5


R.T.: 6.205 min
Delta R.T.: -0.008 min
Response: 79123073
Conc: 1640.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

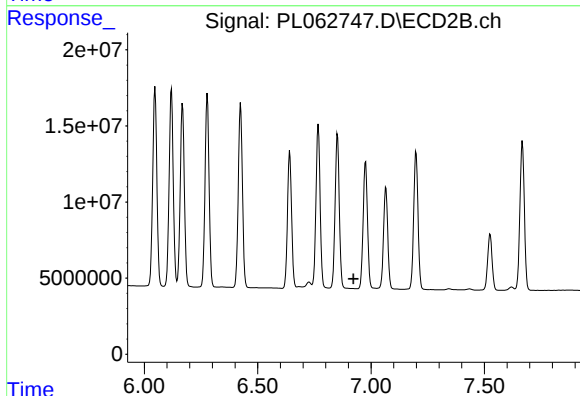


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.923 min
Response: 0
Conc: N.D.

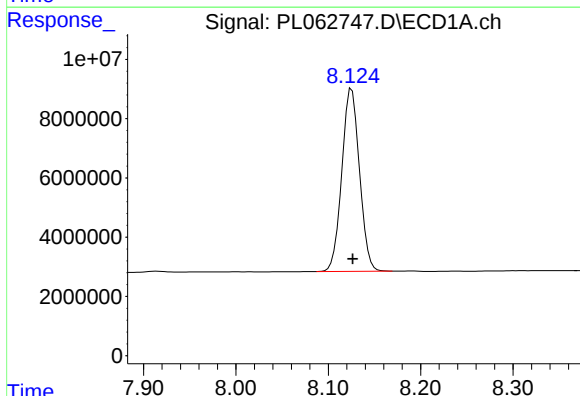

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 81996744
Conc: 51.11 ng/ml

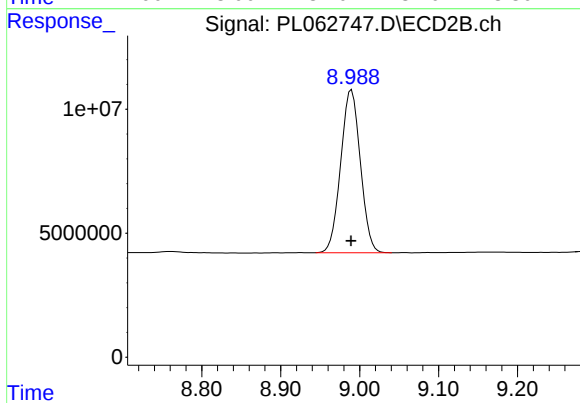

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 113734705
Conc: 54.34 ng/ml