

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
 Data File : PL062725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 16:03
 Operator : DD\AJ
 Sample : L4541-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2015

Manual Integrations
 APPROVED

Ankita
 11/2/2020 3:02:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 17:28:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	21768983	35328119	12.656	12.022
28)	SA Decachlor...	8.126	8.990	8757619	10480865	5.459	5.008m
Target Compounds							
10)	B gamma-Chl...	5.328	6.034	774827	3379496	0.430m	1.004m#
11)	B alpha-Chl...	5.379	6.120	1535367	2542310	0.849m	0.755m
17)	MA 4,4'-DDT	6.301	7.067	919307	1024936	0.689m	0.456m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103020\
Data File : PL062725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 16:03
Operator : DD\AJ
Sample : L4541-10
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
2015


Manual Integrations
APPROVED

Ankita
11/2/2020 3:02:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 17:28:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

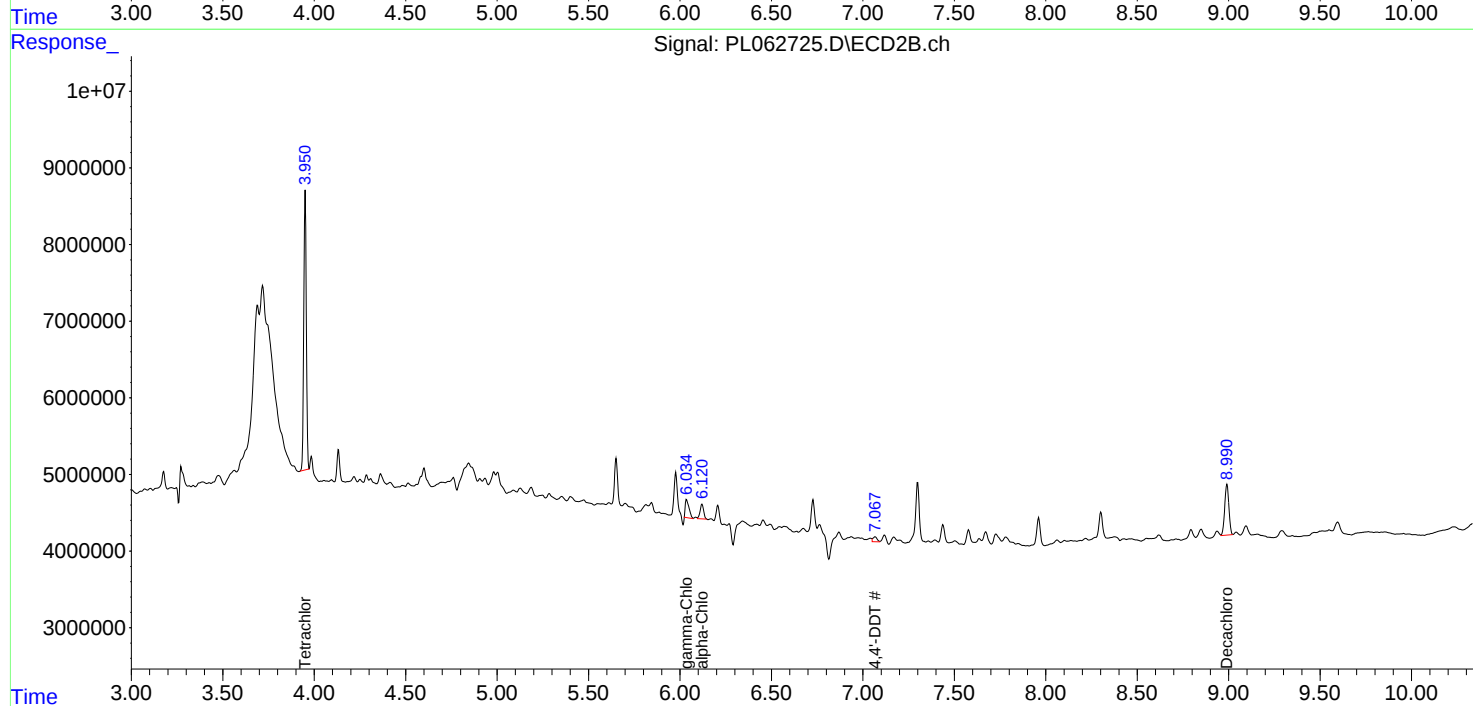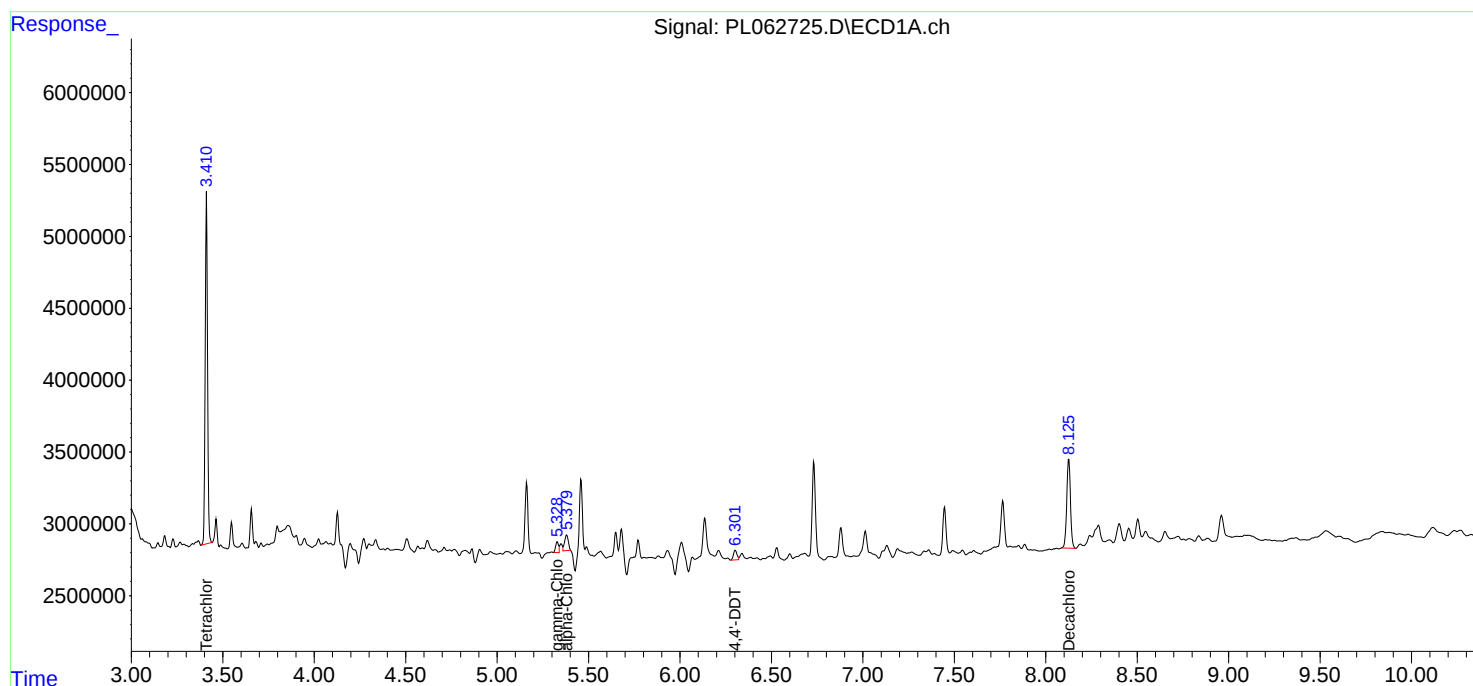

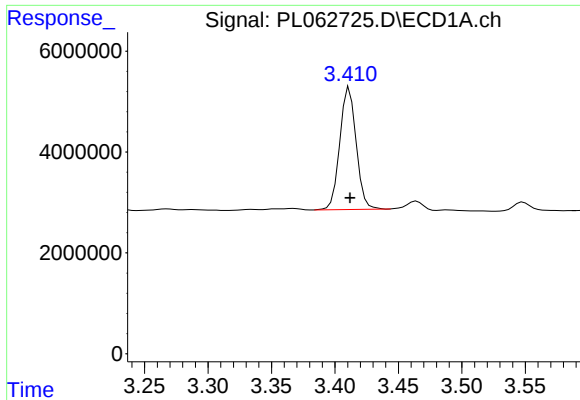


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 21768983
Conc: 12.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
2015


Manual Integrations
APPROVED

Ankita
11/2/2020 3:02:35 PM

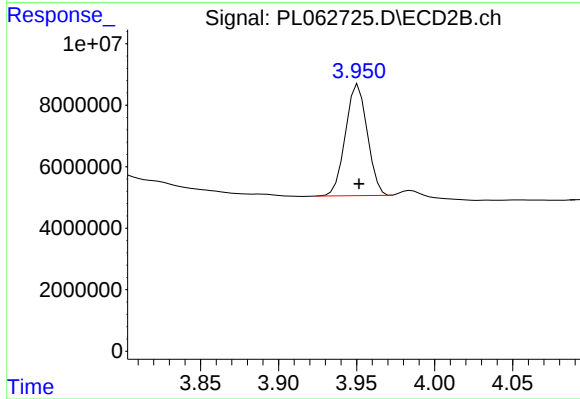


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 35328119
Conc: 12.02 ng/ml

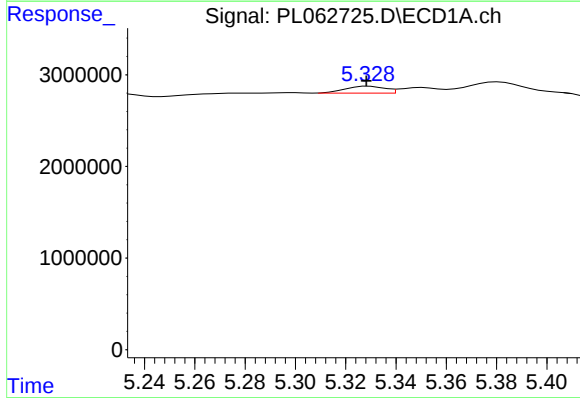


#10 gamma-Chlordane

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 774827
Conc: 0.43 ng/ml m

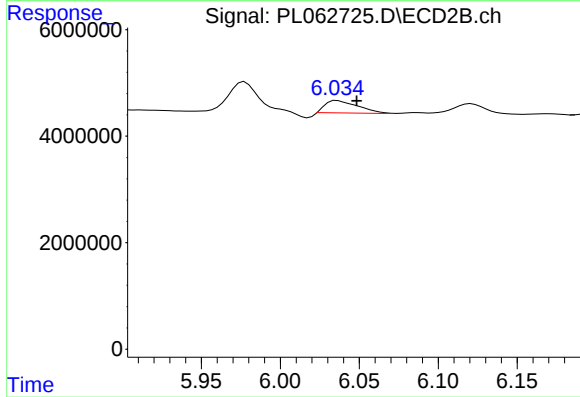

#10 gamma-Chlordane

R.T.: 6.034 min
Delta R.T.: -0.014 min
Response: 3379496
Conc: 1.00 ng/ml m

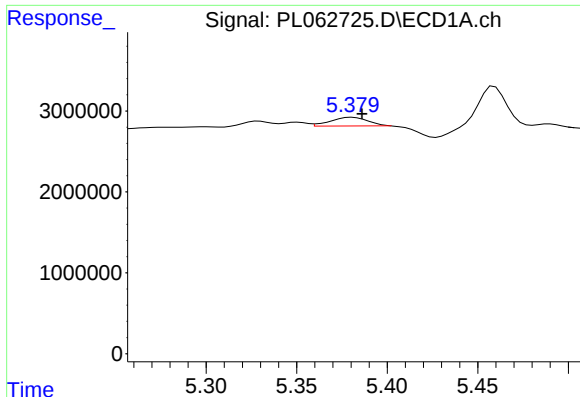


#11 alpha-Chlordane

R.T.: 5.379 min
Delta R.T.: -0.007 min
Response: 1535367
Conc: 0.85 ng/ml m

Instrument :
ECD_L
ClientSampleId :
2015


Manual Integrations
APPROVED

Ankita
11/2/2020 3:02:35 PM

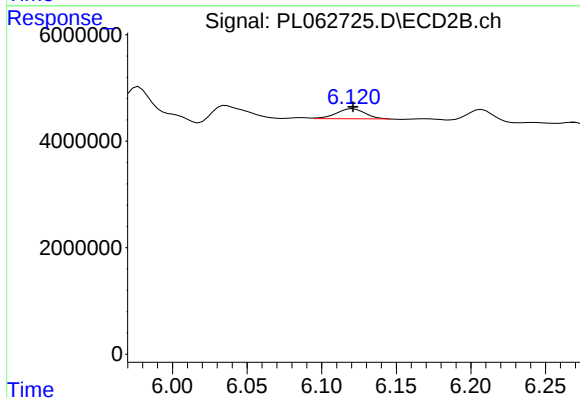


#11 alpha-Chlordane

R.T.: 6.120 min
Delta R.T.: -0.001 min
Response: 2542310
Conc: 0.75 ng/ml m

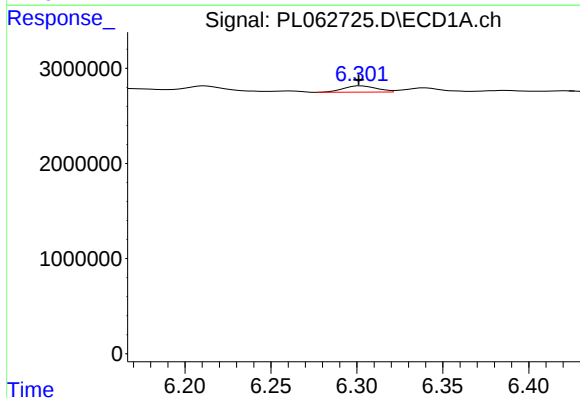


#17 4,4'-DDT

R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 919307
Conc: 0.69 ng/ml m

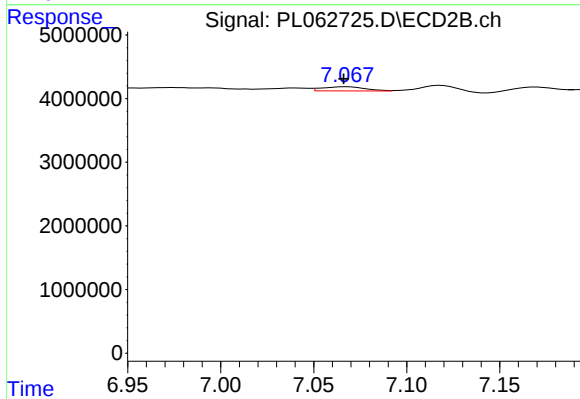

#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 1024936
Conc: 0.46 ng/ml m

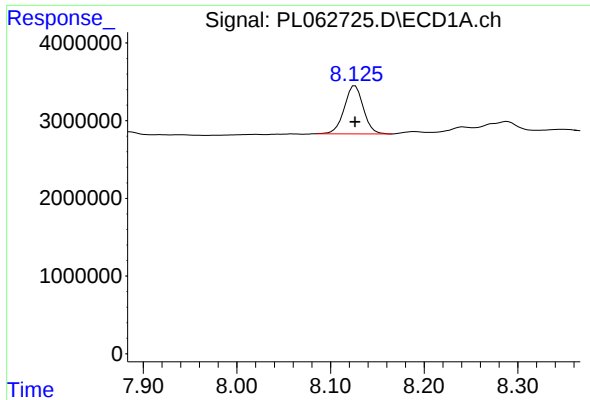


#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 8757619
Conc: 5.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
2015

Manual Integrations
APPROVED

Ankita
11/2/2020 3:02:35 PM

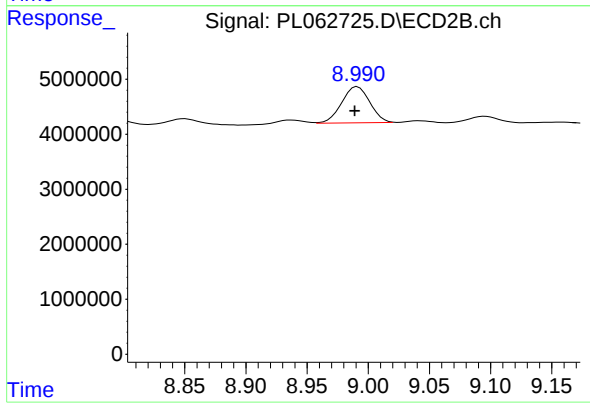

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 10480865
Conc: 5.01 ng/ml m