

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103021\
 Data File : PL070672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 14:49
 Operator : AR\AJ
 Sample : M4406-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:31:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 29 09:09:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.584	5.519	5397944	15891516	11.971	11.424
28)	SA Decachlor...	10.347	11.421	7298926	16346657	12.226	11.435
Target Compounds							
7)	B delta-BHC	0.000	7.039f	0	3291444	N.D.	1.453 #
10)	B gamma-Chl...	0.000	8.250	0	1852733	N.D.	1.019 #
11)	B alpha-Chl...	0.000	8.332	0	921111	N.D.	0.517 #
12)	B 4,4'-DDE	0.000	8.518	0	1243014	N.D.	0.689 #
14)	MA Endrin	8.013	0.000	1711021	0	3.186	N.D. #
17)	MA 4,4'-DDT	8.428	9.376	827433	1555473	1.595	0.962 #
25)	Chlordane-3	0.000	8.250	0	1852733	N.D.	7.580 #
26)	Chlordane-4	0.000	8.332	0	921111	N.D.	3.157 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103021\
Data File : PL070672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 14:49
Operator : AR\AJ
Sample : M4406-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:31:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
Quant Title : GC Extractables
QLast Update : Fri Oct 29 09:09:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

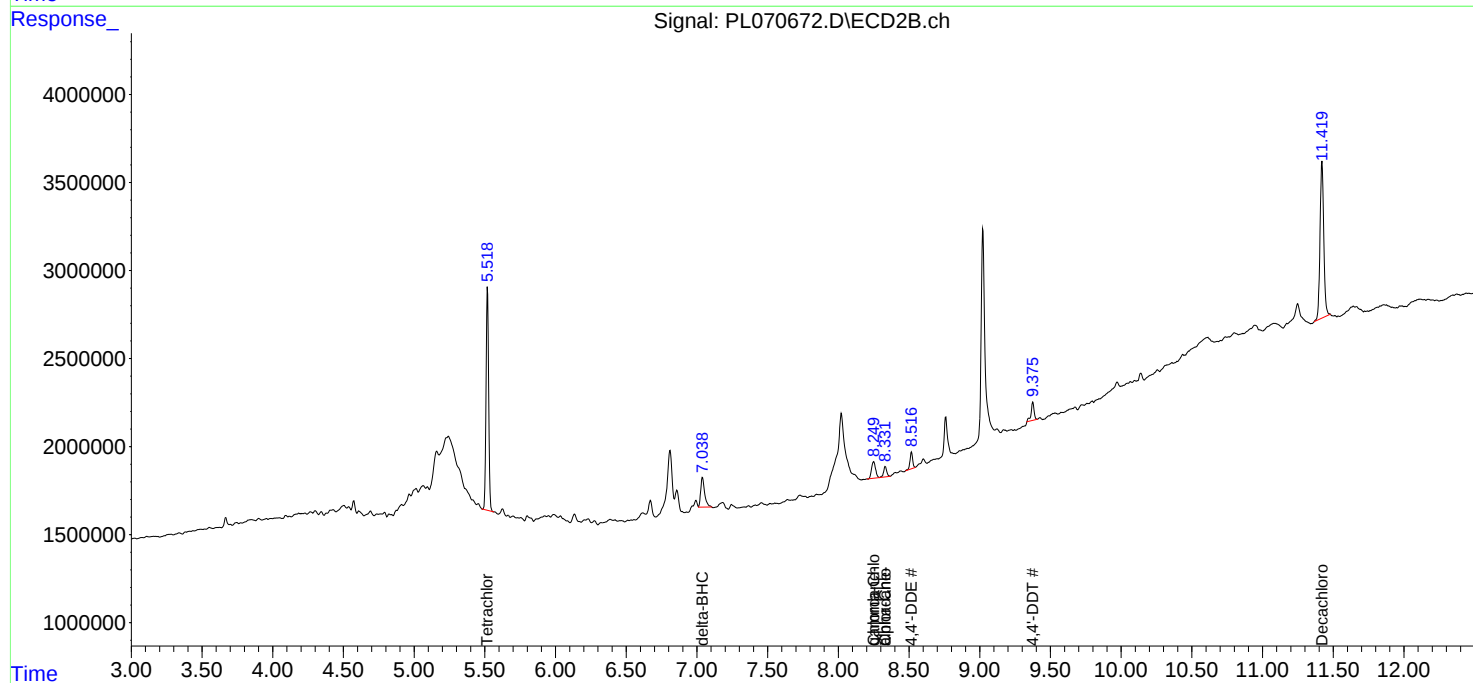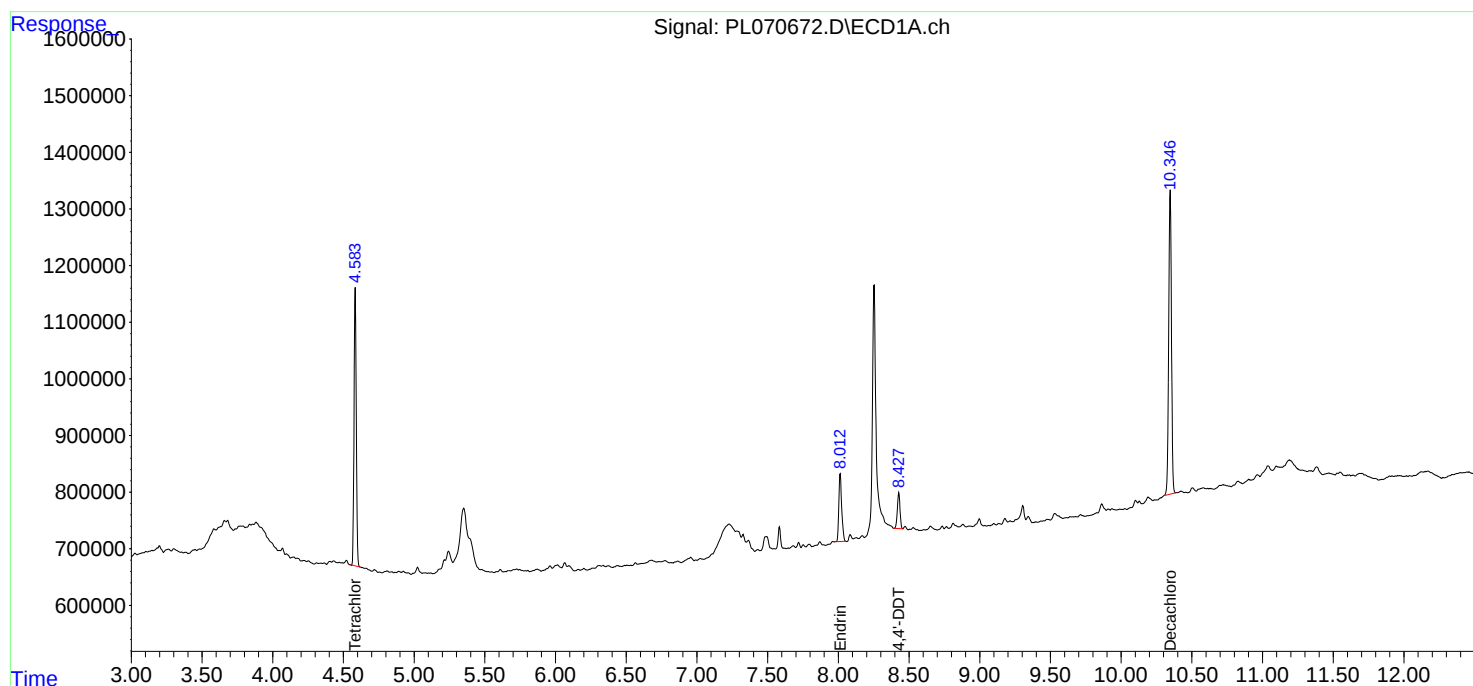


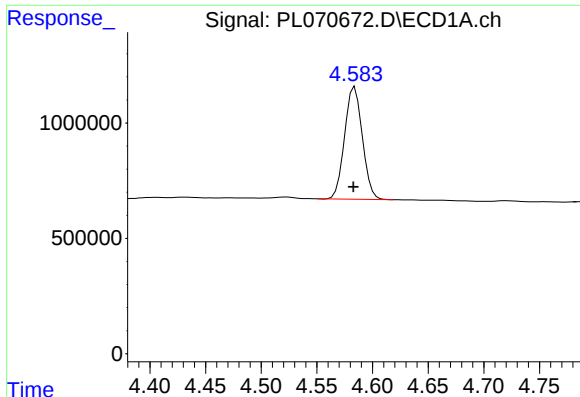

#1 Tetrachloro-m-xylene


R.T.: 4.584 min
Delta R.T.: 0.000 min
Response: 5397944
Conc: 11.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

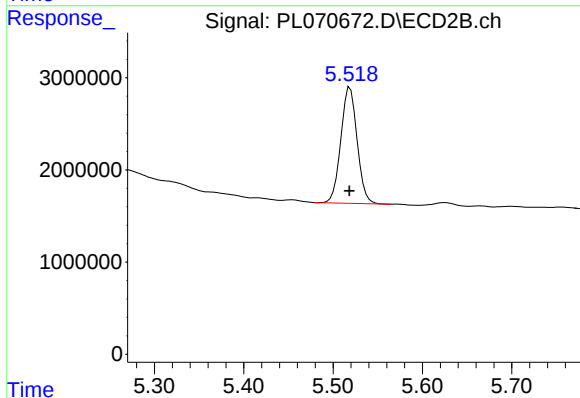


#1 Tetrachloro-m-xylene

R.T.: 5.519 min
Delta R.T.: 0.000 min
Response: 15891516
Conc: 11.42 ng/ml

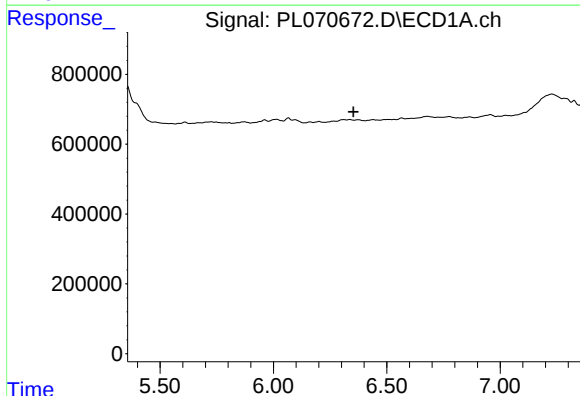


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

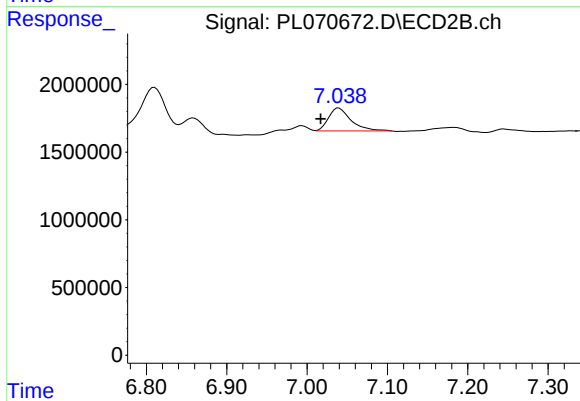

#7 delta-BHC


R.T.: 7.039 min
Delta R.T.: 0.022 min
Response: 3291444
Conc: 1.45 ng/ml

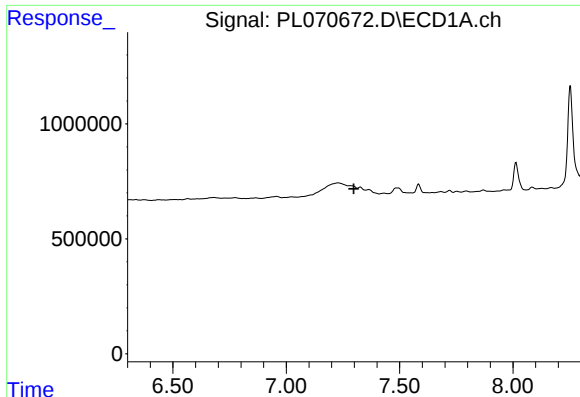

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

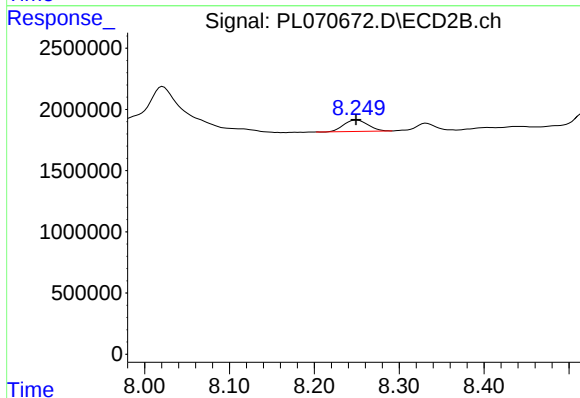


#10 gamma-Chlordane

R.T.: 8.250 min
Delta R.T.: 0.001 min
Response: 1852733
Conc: 1.02 ng/ml

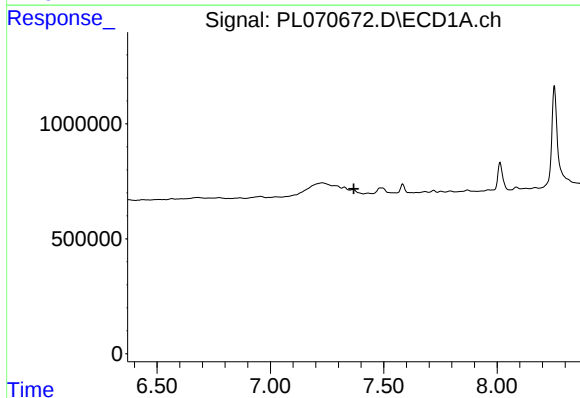


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.368 min
Response: 0
Conc: N.D.

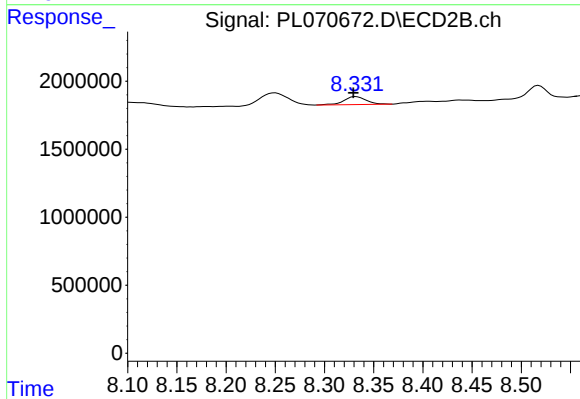

#11 alpha-Chlordane

R.T.: 8.332 min
Delta R.T.: 0.002 min
Response: 921111
Conc: 0.52 ng/ml

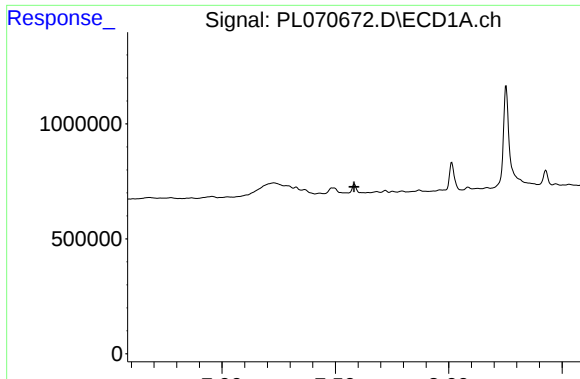

#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#12 4,4'-DDE


R.T.: 8.518 min
Delta R.T.: -0.001 min
Response: 1243014
Conc: 0.69 ng/ml

#14 Endrin

R.T.: 8.013 min
Delta R.T.: 0.013 min
Response: 1711021
Conc: 3.19 ng/ml

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.913 min
Response: 0
Conc: N.D.

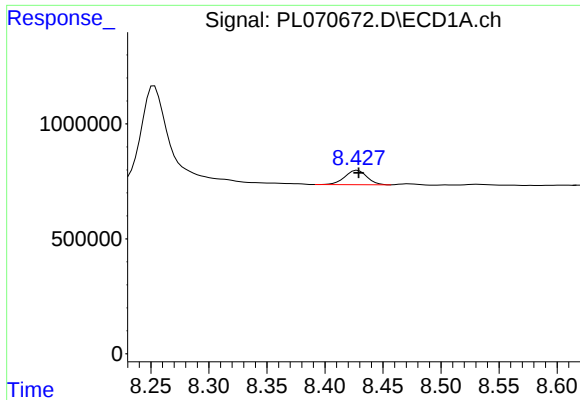

#17 4,4'-DDT


R.T.: 8.428 min
Delta R.T.: 0.000 min
Response: 827433
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

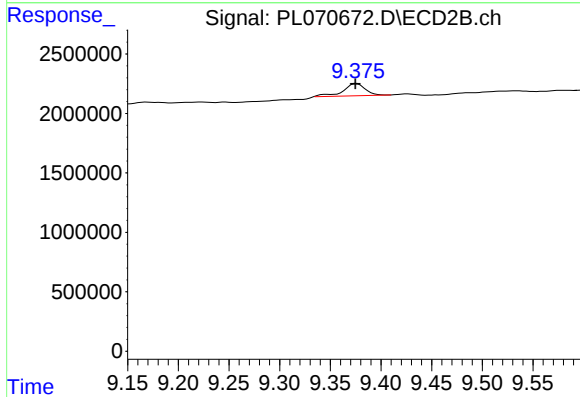


#17 4,4'-DDT

R.T.: 9.376 min
Delta R.T.: 0.001 min
Response: 1555473
Conc: 0.96 ng/ml

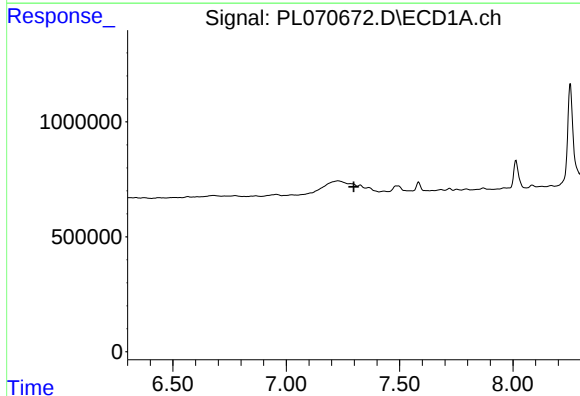


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.299 min
Response: 0
Conc: N.D.

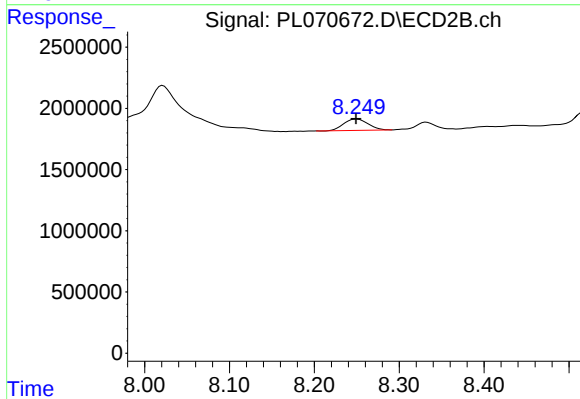

#25 Chlordane-3


R.T.: 8.250 min
Delta R.T.: 0.001 min
Response: 1852733
Conc: 7.58 ng/ml

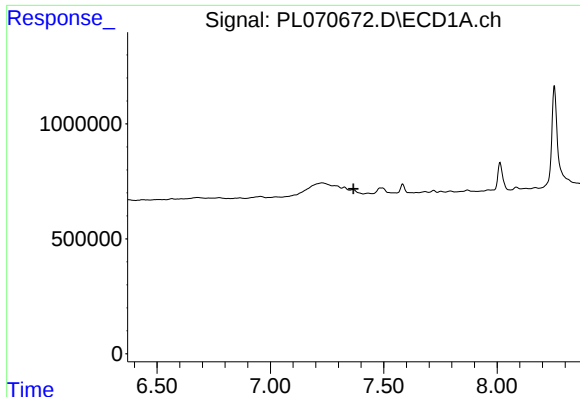

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

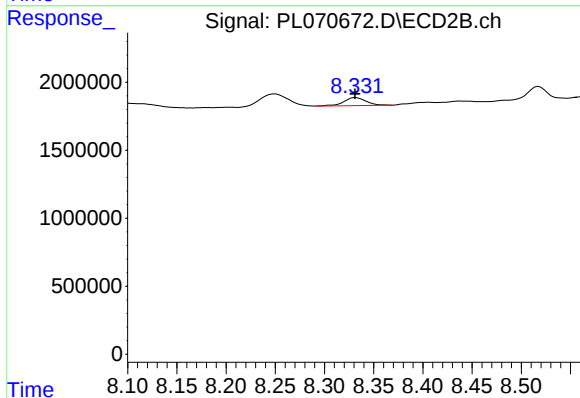


#26 Chlordane-4

R.T.: 8.332 min
Delta R.T.: 0.001 min
Response: 921111
Conc: 3.16 ng/ml

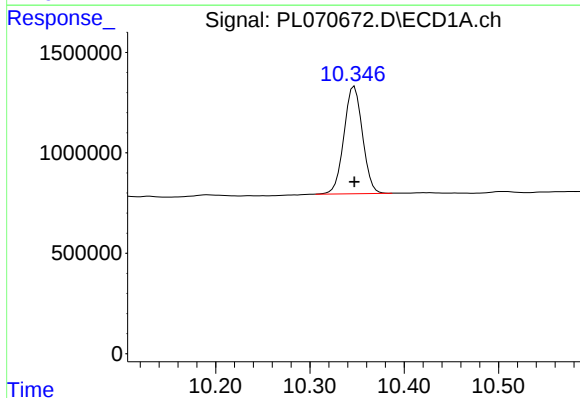

#28 Decachlorobiphenyl

R.T.: 10.347 min
Delta R.T.: 0.000 min
Response: 7298926
Conc: 12.23 ng/ml

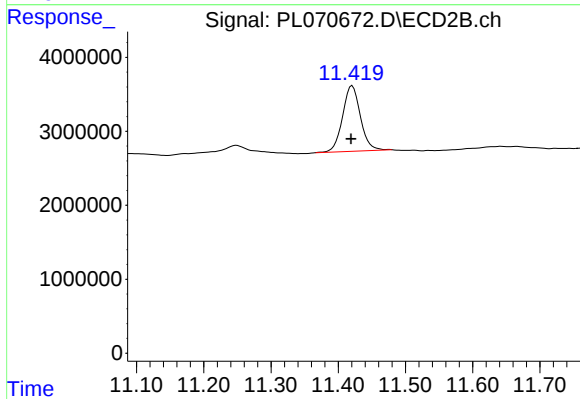

#28 Decachlorobiphenyl

R.T.: 11.421 min
Delta R.T.: 0.002 min
Response: 16346657
Conc: 11.43 ng/ml