

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
 Data File : PL086312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 23:09
 Operator : AR\AJ
 Sample : PIBLK210
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 05:01:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.619	71583103	21214597	25.116	23.389
27)	SA Decachlor...	8.855	7.771	126.0E6	53235598	50.576	46.376
Target Compounds							
3)	MA gamma-BHC...	4.135	0.000	277890	0	<MDL	N.D. #
4)	MA Heptachlor	4.734	0.000	98694	0	<MDL	N.D. #
7)	B delta-BHC	4.589	0.000	3574953	0	0.961	N.D. #
8)	B Heptachlo...	5.428f	0.000	14715889	0	4.340	N.D. #
9)	A Endosulfan I	5.821f	0.000	1215230	0	0.378	N.D. #
10)	B trans-Chl...	5.821f	0.000	1215230	0	0.348	N.D. #
11)	B cis-Chlor...	5.821	0.000	1215230	0	0.346	N.D. #
14)	MA Endrin	6.392	0.000	377874	0	0.129	N.D. #
15)	B Endosulfa...	6.609	0.000	5110027	0	1.633	N.D. #
19)	B Endosulfa...	6.960	0.000	554600	0	0.195	N.D. #
20)	A Methoxychlor	7.399f	0.000	5174197	0	4.103	N.D. #
21)	B Endrin ke...	7.512f	0.000	212199	0	<MDL	N.D. #
24)	Toxaphene-3	6.960	0.000	554600	0	8.836	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
Data File : PL086312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 23:09
Operator : AR\AJ
Sample : PIBLK210
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 05:01:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 27 01:35:51 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

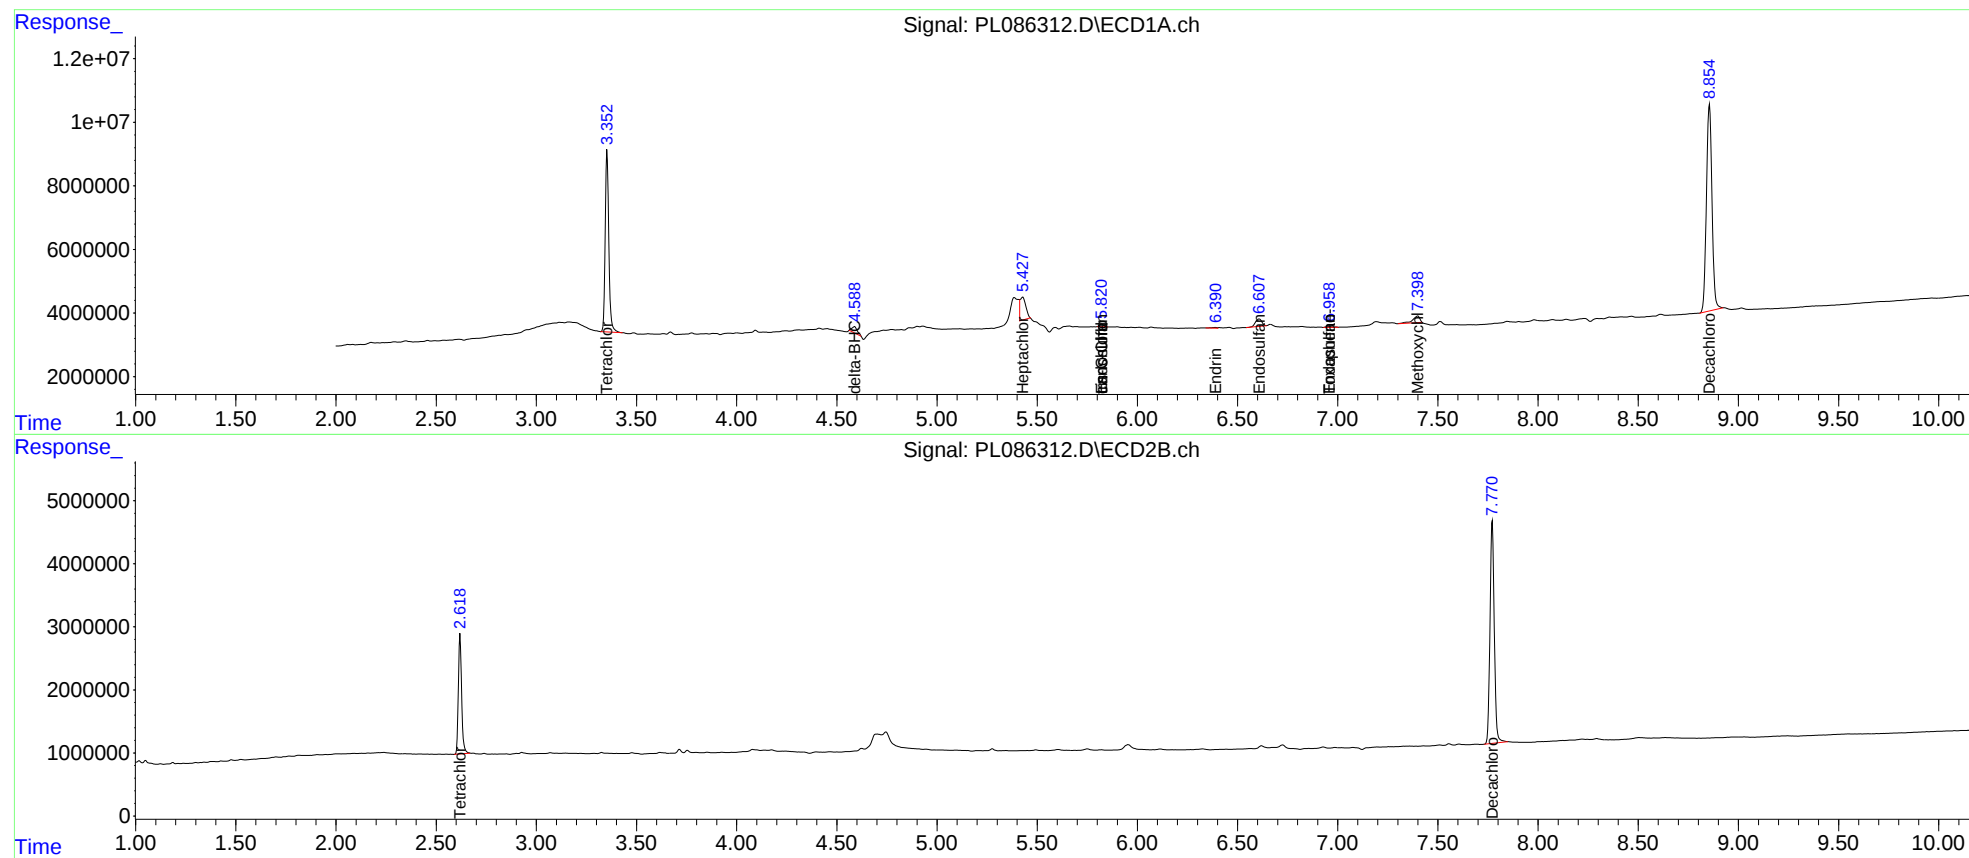

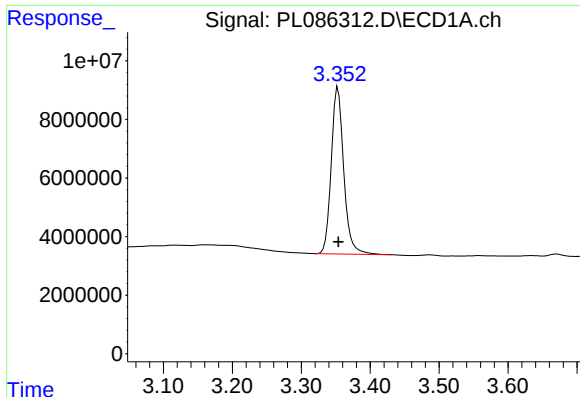


#1 Tetrachloro-m-xylene

R.T.: 3.353 min
Delta R.T.: 0.000 min
Response: 71583103
Conc: 25.12 ng/ml

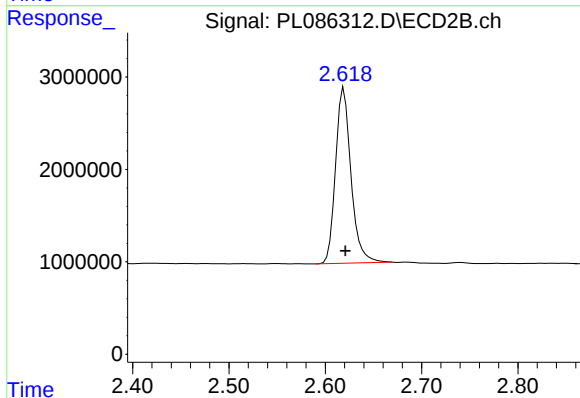


#1 Tetrachloro-m-xylene

R.T.: 2.619 min
Delta R.T.: -0.002 min
Response: 21214597
Conc: 23.39 ng/ml

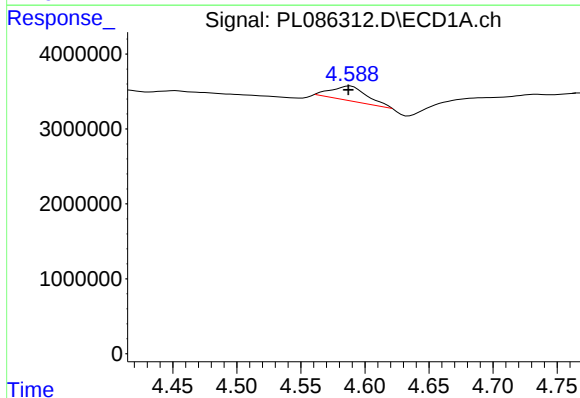


#7 delta-BHC

R.T.: 4.589 min
Delta R.T.: 0.002 min
Response: 3574953
Conc: 0.96 ng/ml

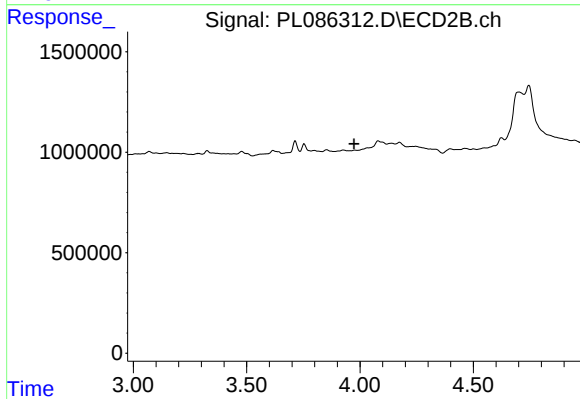


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 3.974 min
Response: 0
Conc: N.D.

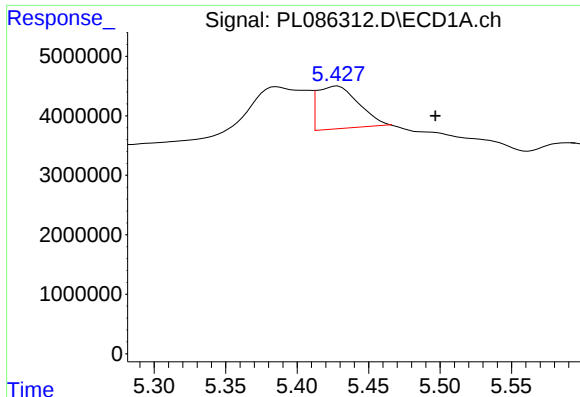


#8 Heptachlor epoxide

R.T.: 5.428 min
Delta R.T.: -0.068 min
Response: 14715889
Conc: 4.34 ng/ml

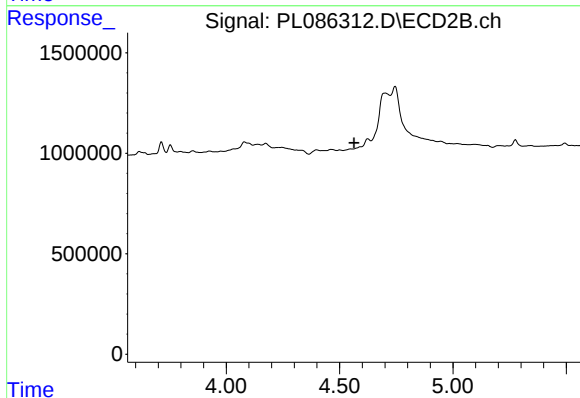


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.564 min
Response: 0
Conc: N.D.

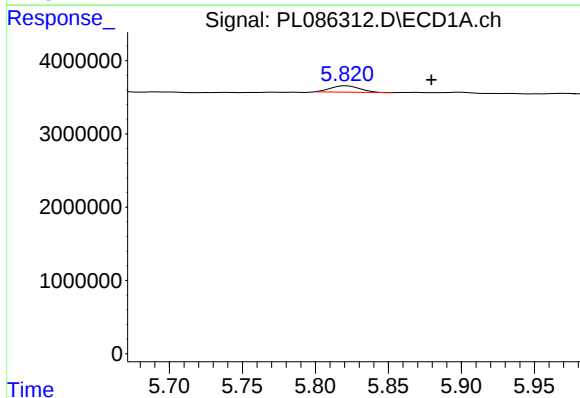


#9 Endosulfan I

R.T.: 5.821 min
Delta R.T.: -0.058 min
Response: 1215230
Conc: 0.38 ng/ml

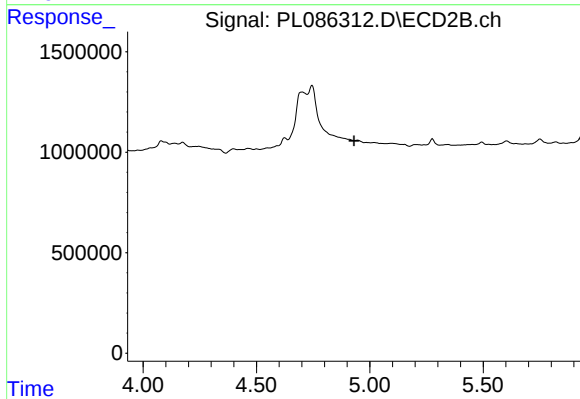


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 4.931 min
Response: 0
Conc: N.D.

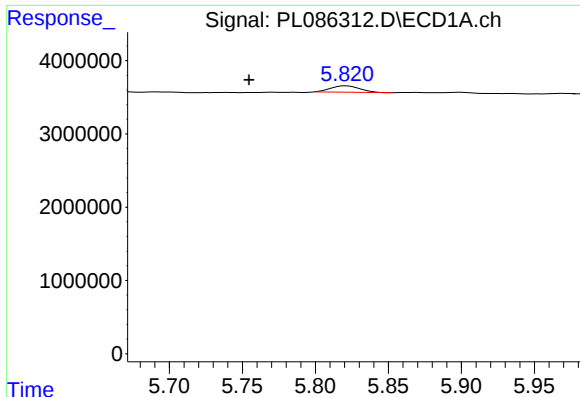


#10 trans-Chlordane

R.T.: 5.821 min
Delta R.T.: 0.067 min
Response: 1215230
Conc: 0.35 ng/ml

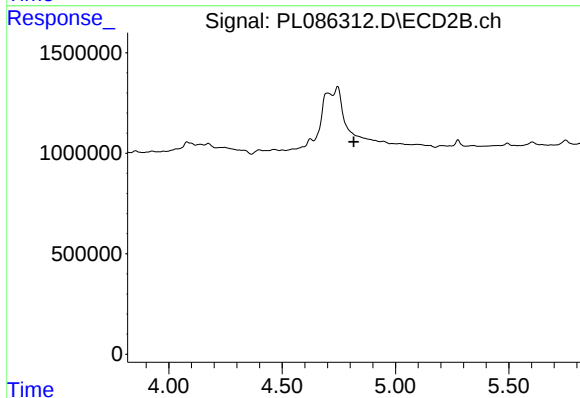


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.816 min
Response: 0
Conc: N.D.

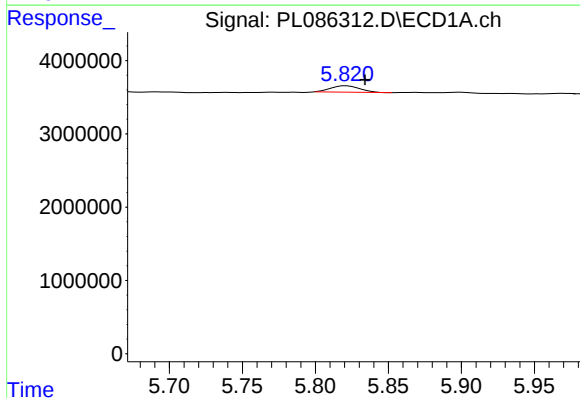


#11 cis-Chlordane

R.T.: 5.821 min
Delta R.T.: -0.013 min
Response: 1215230
Conc: 0.35 ng/ml

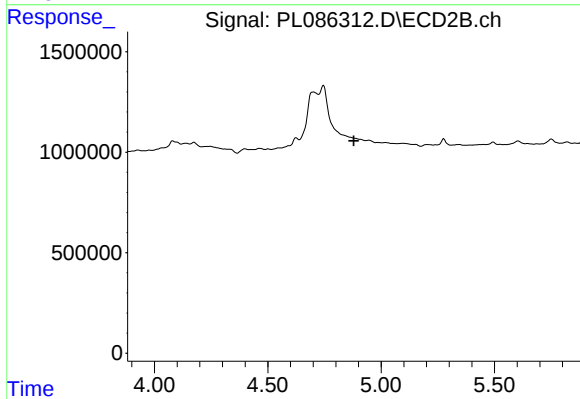


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.880 min
Response: 0
Conc: N.D.

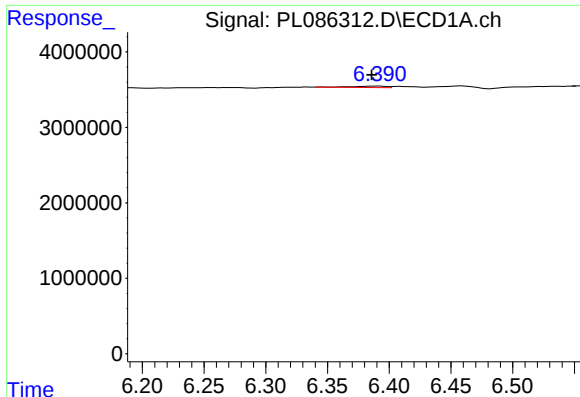


#14 Endrin

R.T.: 6.392 min
Delta R.T.: 0.006 min
Response: 377874
Conc: 0.13 ng/ml

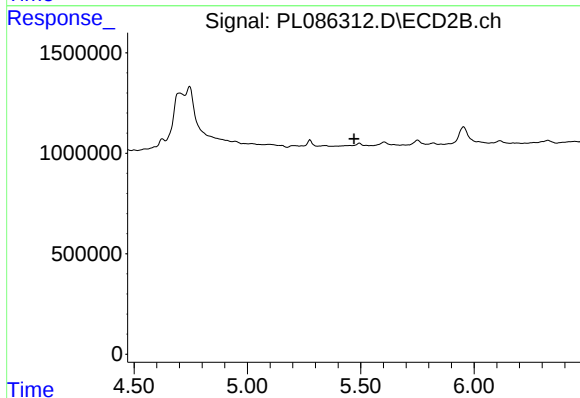


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.471 min
Response: 0
Conc: N.D.

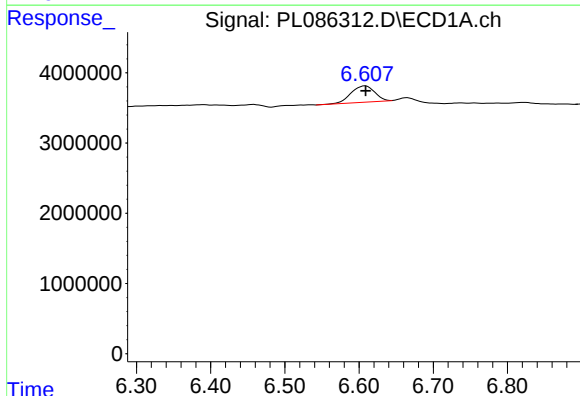


#15 Endosulfan II

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 5110027
Conc: 1.63 ng/ml

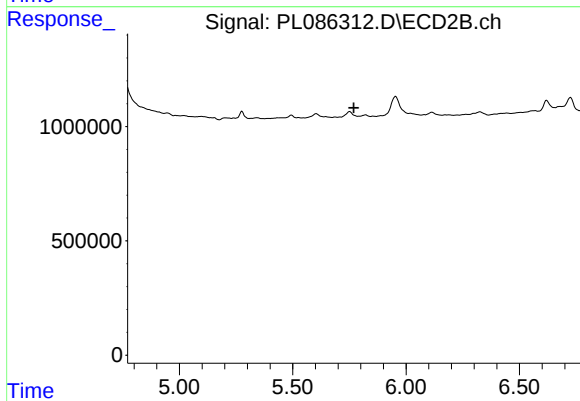


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.769 min
Response: 0
Conc: N.D.

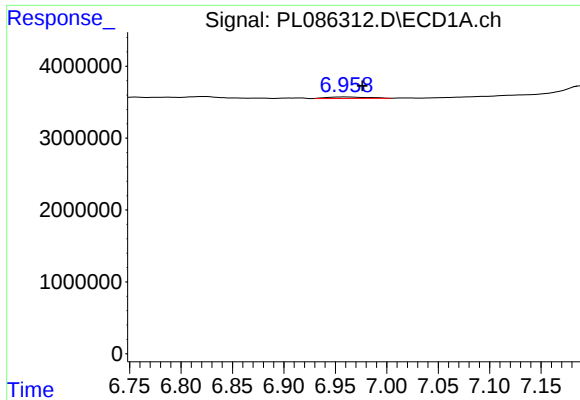


#19 Endosulfan Sulfate

R.T.: 6.960 min
Delta R.T.: -0.017 min
Response: 554600
Conc: 0.20 ng/ml

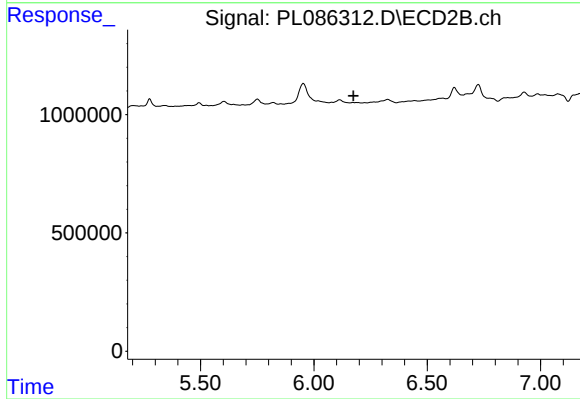


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.175 min
Response: 0
Conc: N.D.

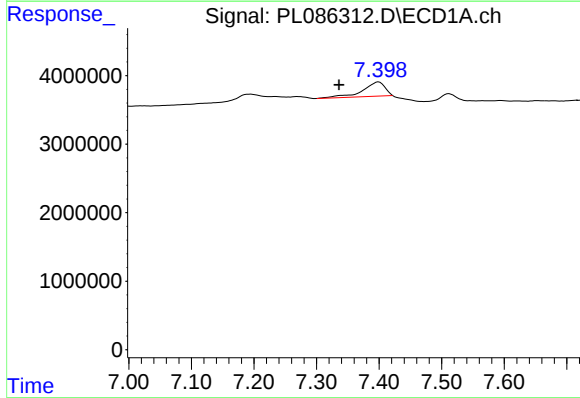


#20 Methoxychlor

R.T.: 7.399 min
Delta R.T.: 0.063 min
Response: 5174197
Conc: 4.10 ng/ml

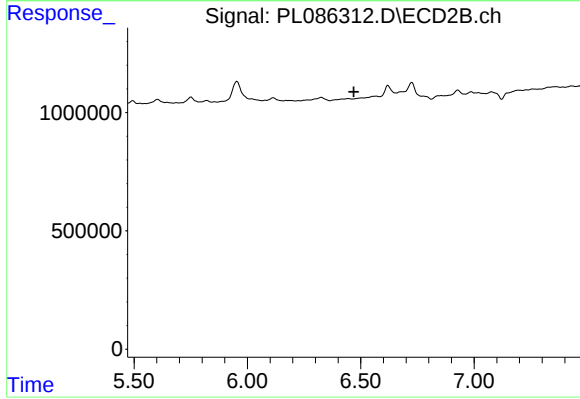


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.470 min
Response: 0
Conc: N.D.

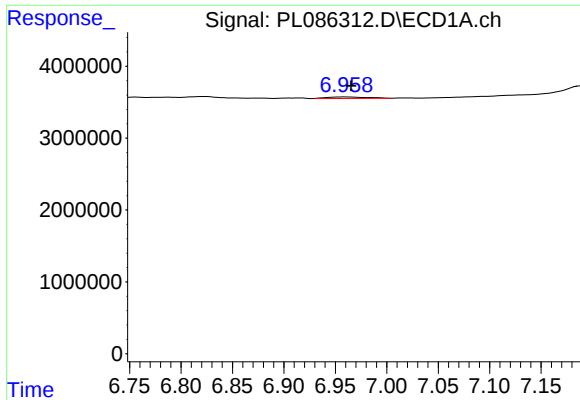


#24 Toxaphene-3

R.T.: 6.960 min
Delta R.T.: -0.006 min
Response: 554600
Conc: 8.84 ng/ml

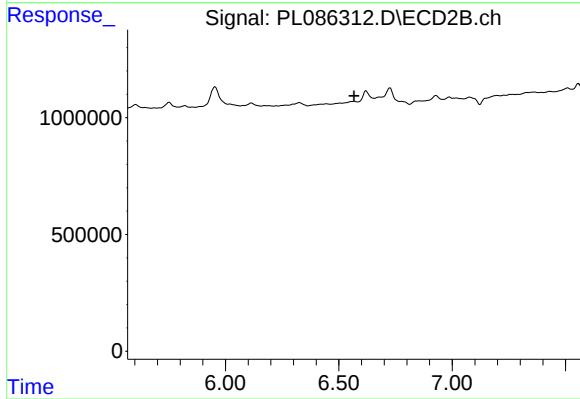


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 6.567 min
Response: 0
Conc: N.D.

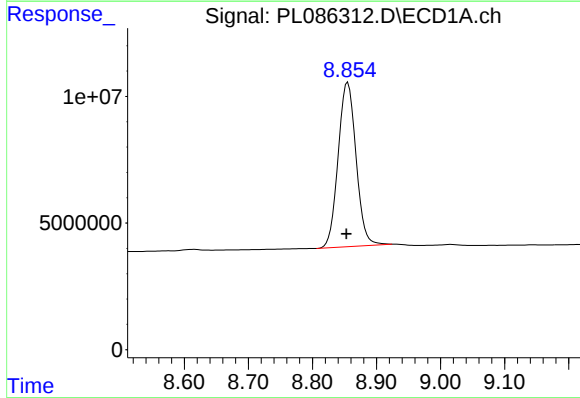

#27 Decachlorobiphenyl

R.T.: 8.855 min
Delta R.T.: 0.002 min
Response: 126042884
Conc: 50.58 ng/ml

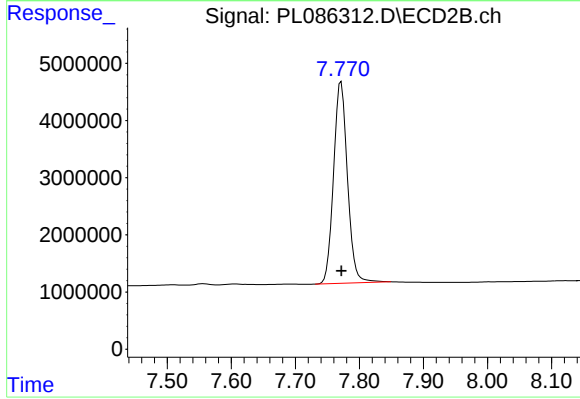

#27 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: 0.000 min
Response: 53235598
Conc: 46.38 ng/ml