

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
 Data File : PL086346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 07:12
 Operator : AR\AJ
 Sample : PIBLK212
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 09:10:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.354	2.620	68792676	20564379	24.137	22.673
27)	SA Decachlor...	8.854	7.771	120.8E6	52164078	48.460	45.442
Target Compounds							
3)	MA gamma-BHC...	4.148	0.000	170860	0	<MDL	N.D. #
4)	MA Heptachlor	4.732	0.000	120214	0	<MDL	N.D. #
7)	B delta-BHC	4.589	0.000	3529445	0	0.949	N.D. #
8)	B Heptachlo...	5.498	0.000	556070	0	0.164	N.D. #
9)	A Endosulfan I	5.867	0.000	179507	0	<MDL	N.D. #
10)	B trans-Chl...	5.822f	0.000	1038306	0	0.297	N.D. #
11)	B cis-Chlor...	5.822	0.000	1038306	0	0.295	N.D. #
12)	B 4,4'-DDE	6.068f	0.000	266066	0	<MDL	N.D. #
14)	MA Endrin	6.333f	0.000	780577	0	0.266	N.D. #
15)	B Endosulfa...	6.609	0.000	3476352	0	1.111	N.D. #
18)	B Endrin al...	6.760	0.000	34123	0	<MDL	N.D. #
19)	B Endosulfa...	6.963	0.000	318244	0	0.112	N.D. #
20)	A Methoxychlor	7.343	0.000	576728	0	0.457	N.D. #
21)	B Endrin ke...	7.511f	0.000	370125	0	0.128	N.D. #
22)	Toxaphene-1	6.068	0.000	266066	0	11.799	N.D. #
24)	Toxaphene-3	6.963	0.000	318244	0	5.071	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
Data File : PL086346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 07:12
Operator : AR\AJ
Sample : PIBLK212
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 09:10:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 27 01:35:51 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

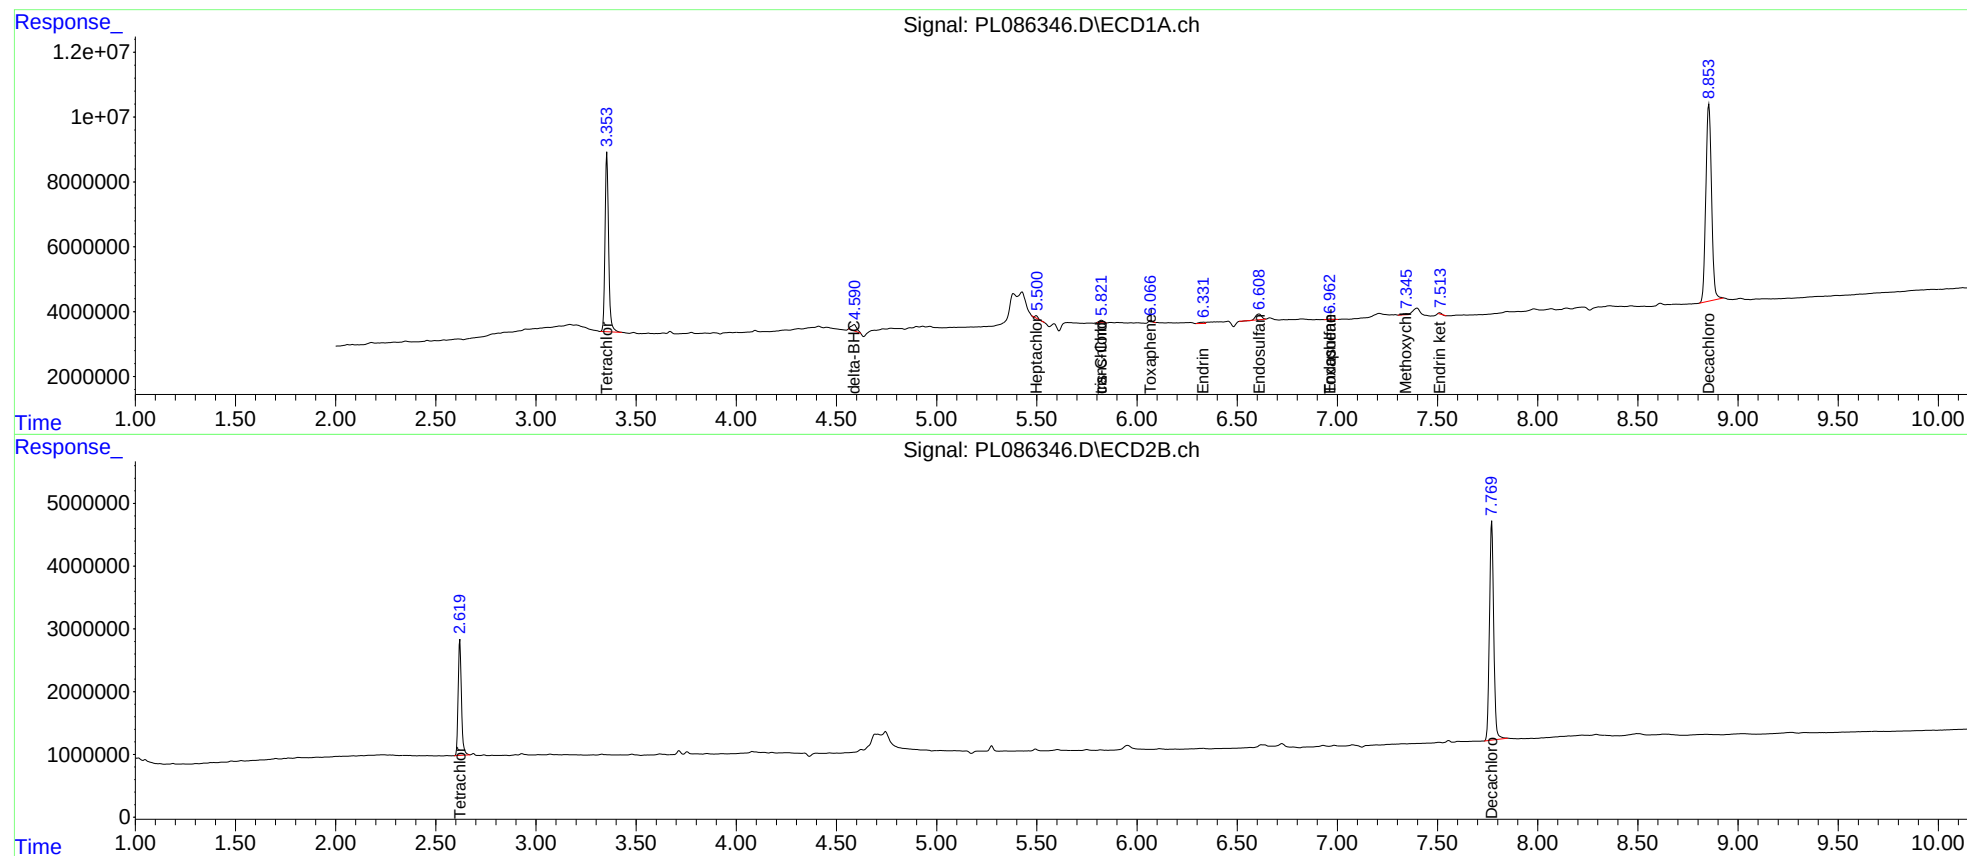

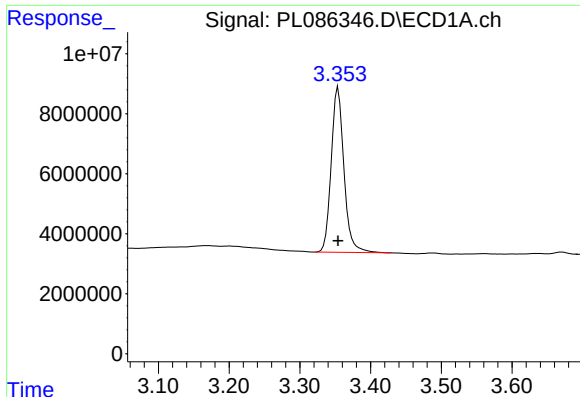


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: 0.000 min
Response: 68792676
Conc: 24.14 ng/ml

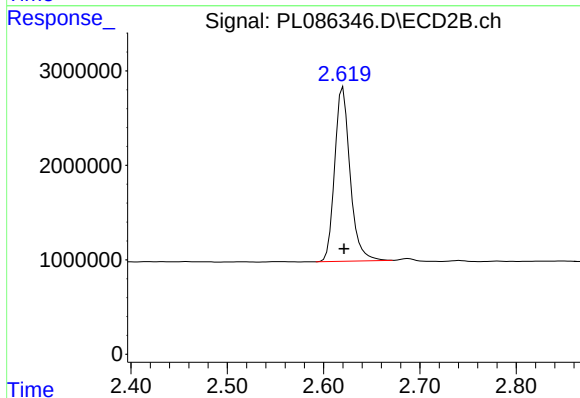


#1 Tetrachloro-m-xylene

R.T.: 2.620 min
Delta R.T.: 0.000 min
Response: 20564379
Conc: 22.67 ng/ml

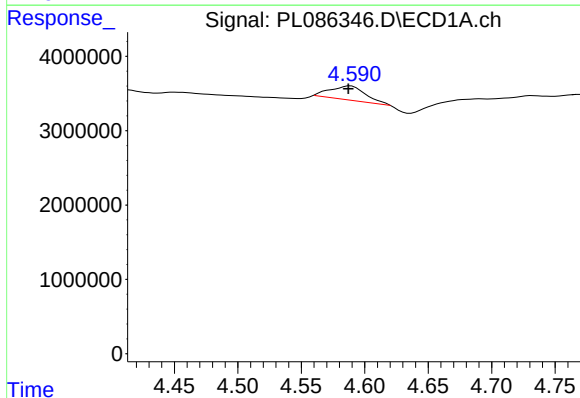


#7 delta-BHC

R.T.: 4.589 min
Delta R.T.: 0.002 min
Response: 3529445
Conc: 0.95 ng/ml

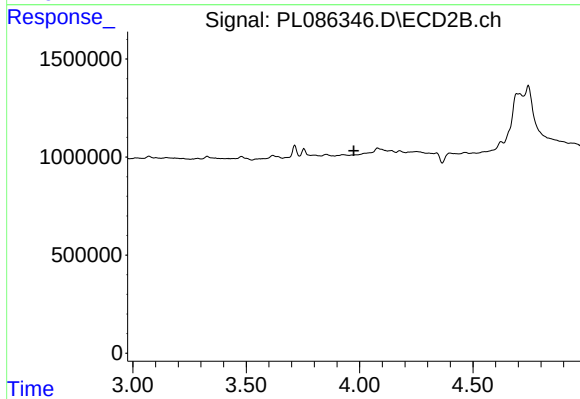


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 3.974 min
Response: 0
Conc: N.D.

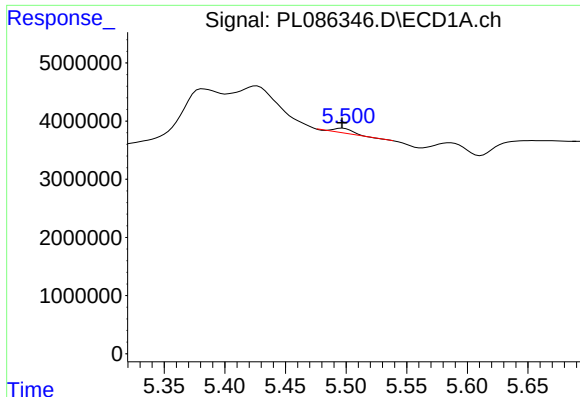


#8 Heptachlor epoxide

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 556070
Conc: 0.16 ng/ml

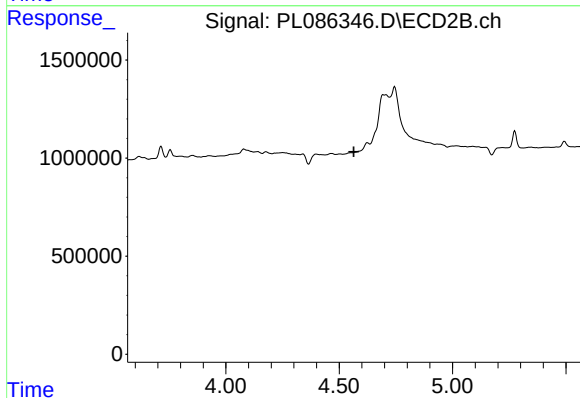


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.564 min
Response: 0
Conc: N.D.

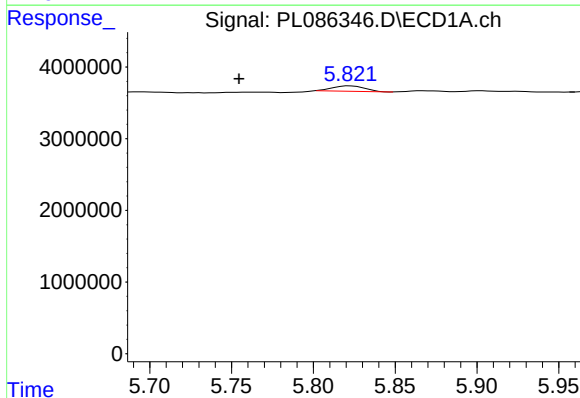


#10 trans-Chlordane

R.T.: 5.822 min
Delta R.T.: 0.068 min
Response: 1038306
Conc: 0.30 ng/ml

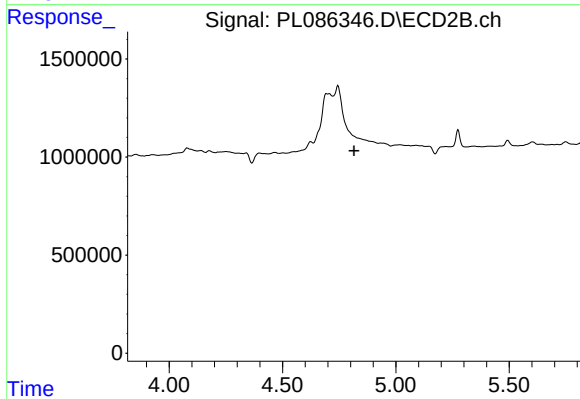


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.816 min
Response: 0
Conc: N.D.

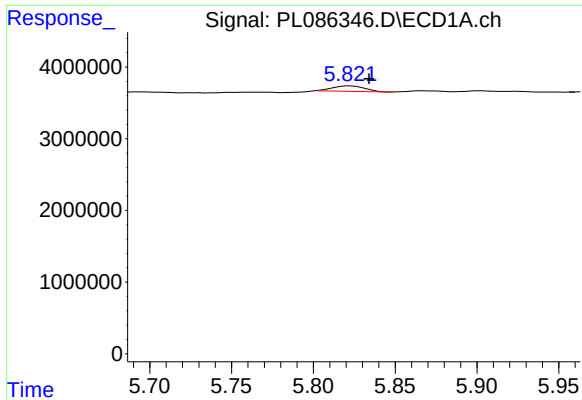


#11 cis-Chlordane

R.T.: 5.822 min
Delta R.T.: -0.012 min
Response: 1038306
Conc: 0.30 ng/ml

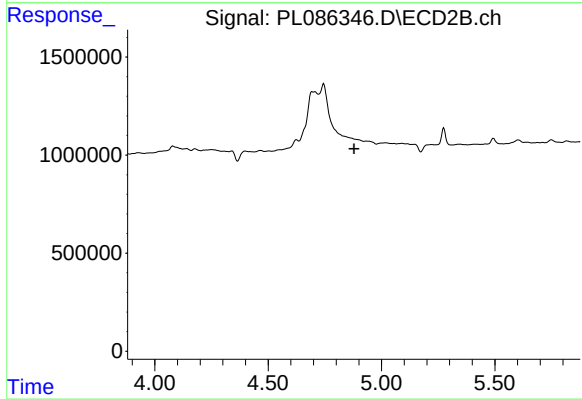


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.880 min
Response: 0
Conc: N.D.

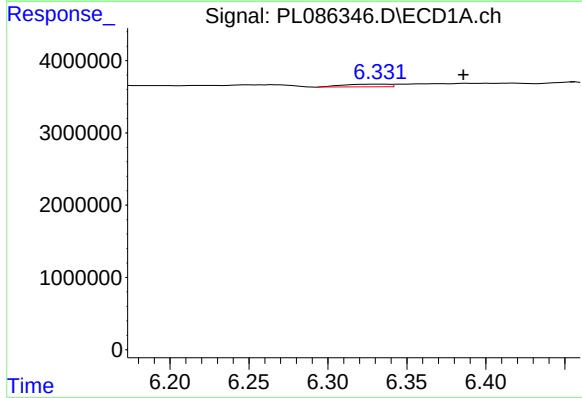


#14 Endrin

R.T.: 6.333 min
Delta R.T.: -0.053 min
Response: 780577
Conc: 0.27 ng/ml

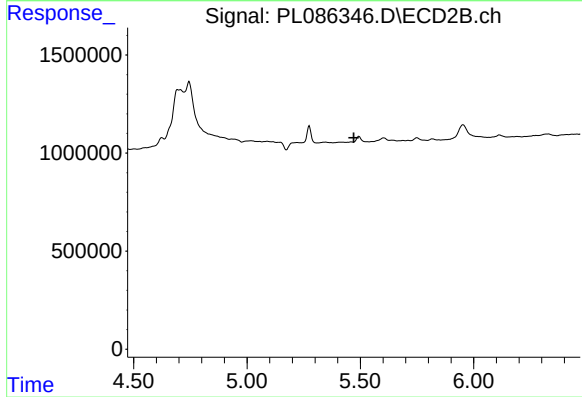


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.471 min
Response: 0
Conc: N.D.

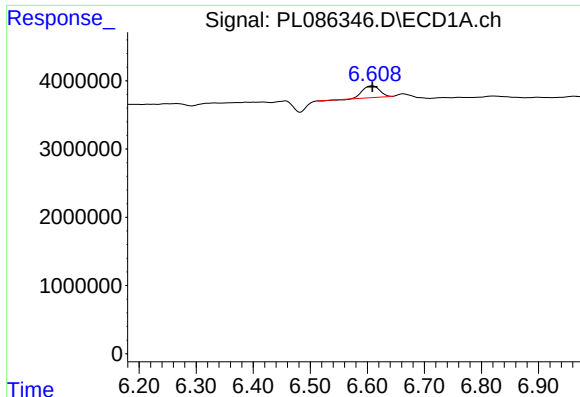


#15 Endosulfan II

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 3476352
Conc: 1.11 ng/ml

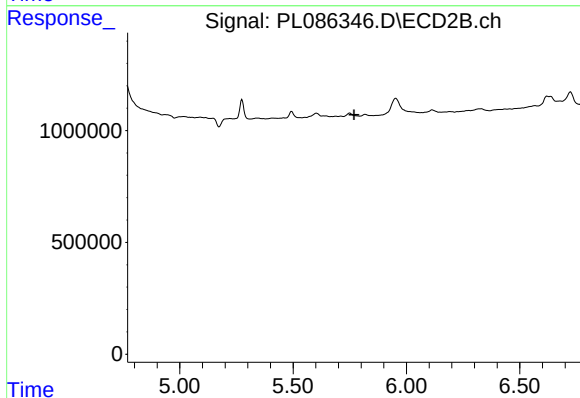


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.769 min
Response: 0
Conc: N.D.

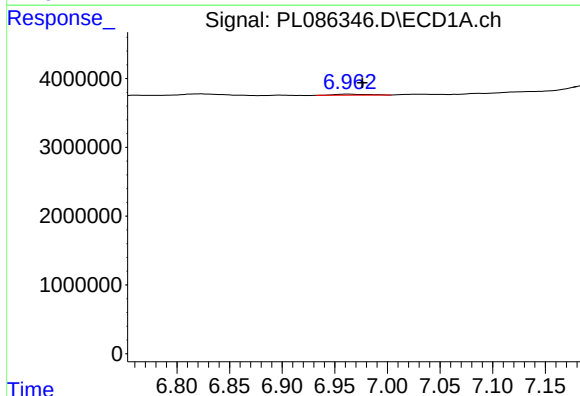


#19 Endosulfan Sulfate

R.T.: 6.963 min
Delta R.T.: -0.013 min
Response: 318244
Conc: 0.11 ng/ml

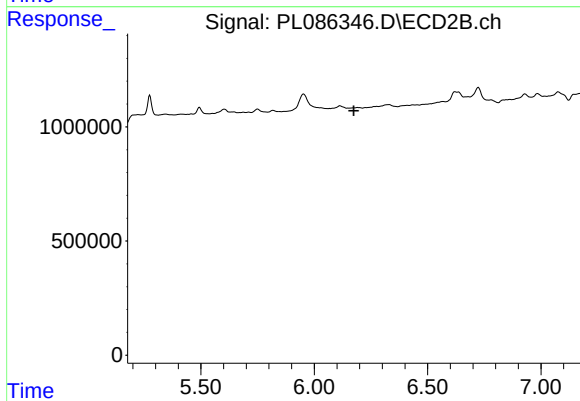


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.175 min
Response: 0
Conc: N.D.

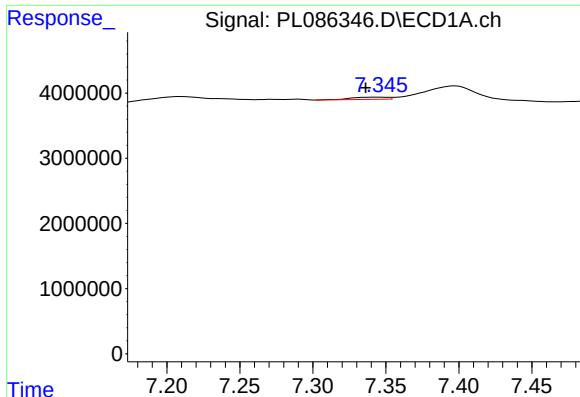


#20 Methoxychlor

R.T.: 7.343 min
Delta R.T.: 0.007 min
Response: 576728
Conc: 0.46 ng/ml

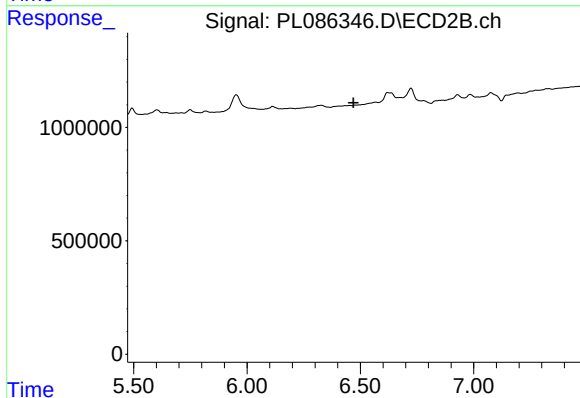


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.470 min
Response: 0
Conc: N.D.

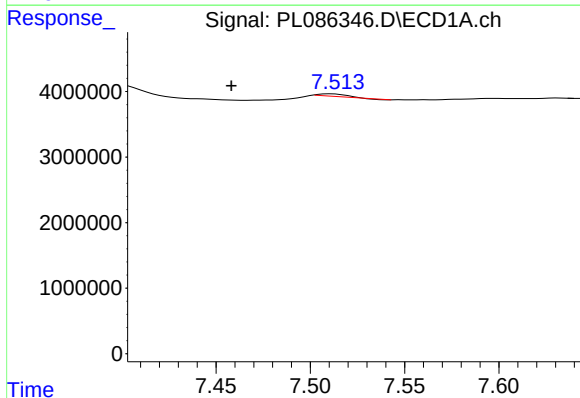


#21 Endrin ketone

R.T.: 7.511 min
Delta R.T.: 0.053 min
Response: 370125
Conc: 0.13 ng/ml

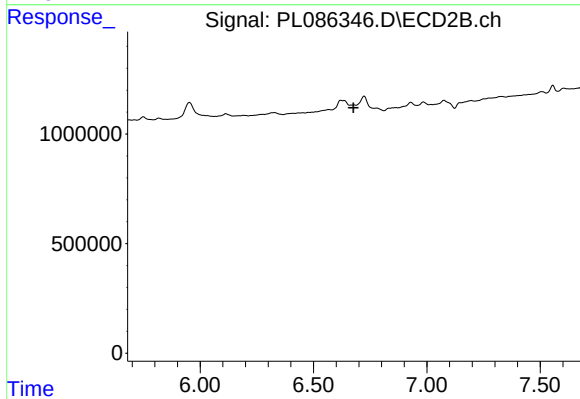


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.677 min
Response: 0
Conc: N.D.

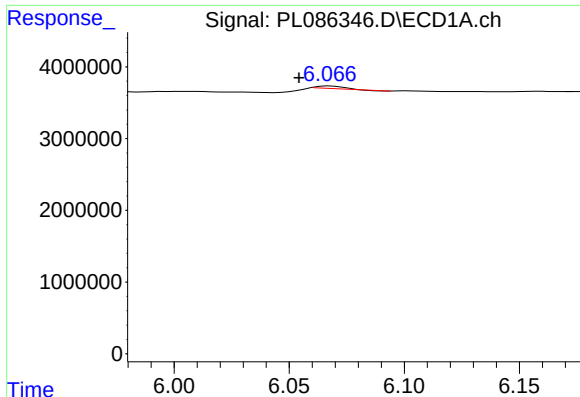


#22 Toxaphene-1

R.T.: 6.068 min
Delta R.T.: 0.014 min
Response: 266066
Conc: 11.80 ng/ml

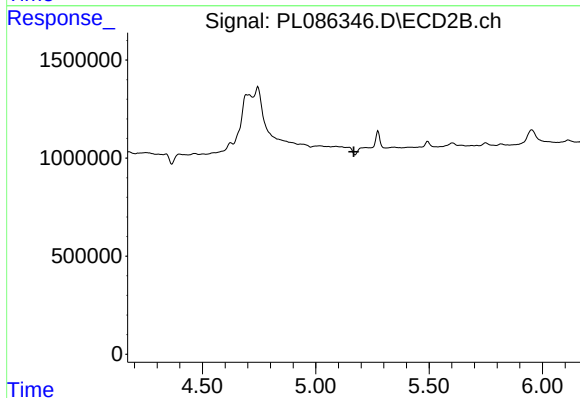


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

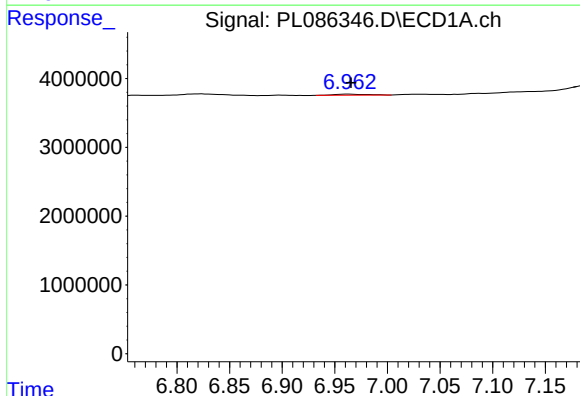


#24 Toxaphene-3

R.T.: 6.963 min
Delta R.T.: -0.002 min
Response: 318244
Conc: 5.07 ng/ml

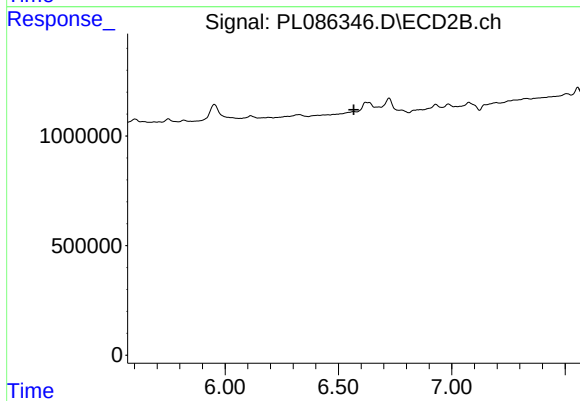

#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 6.567 min
Response: 0
Conc: N.D.

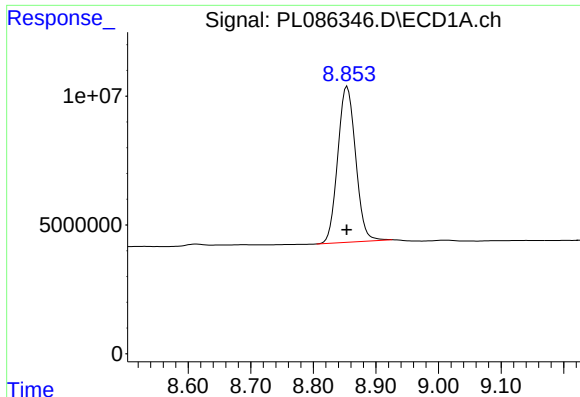


#27 Decachlorobiphenyl

R.T.: 8.854 min

Delta R.T.: 0.000 min

Response: 120769217

Conc: 48.46 ng/ml

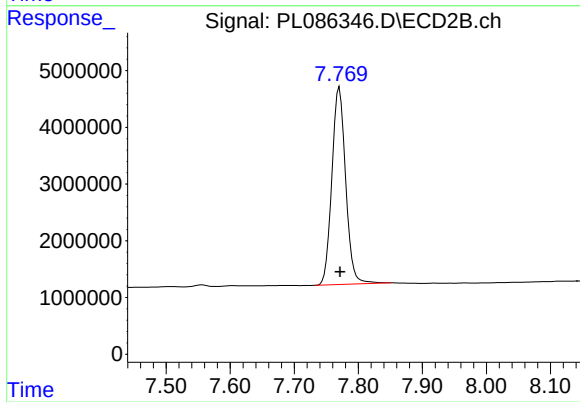

#27 Decachlorobiphenyl

R.T.: 7.771 min

Delta R.T.: -0.001 min

Response: 52164078

Conc: 45.44 ng/ml