

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
 Data File : PL086320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 01:13
 Operator : AR\AJ
 Sample : 04953-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAS9

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/31/2023
 Supervised By : mohammad ahmed 11/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 05:04:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.620	33456448	10116556	11.738m	11.154
2)	SA Decachlor...	8.856	7.771	31936689	13808918	12.815	12.030
Target Compounds							
12)	B 4,4'-DDE	6.016	5.077	2215299	1269734	0.706m	1.159 #
15)	B Endosulfa...	6.611	5.761	3488363	1313487	1.115	1.206m
16)	A 4,4'-DDD	6.536	5.633	4947065	1675223	2.085	1.914
17)	MA 4,4'-DDT	6.849	5.884	12697310	4501915	5.305m	5.002

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
Data File : PL086320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 01:13
Operator : AR\AJ
Sample : 04953-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 05:04:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 27 01:35:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

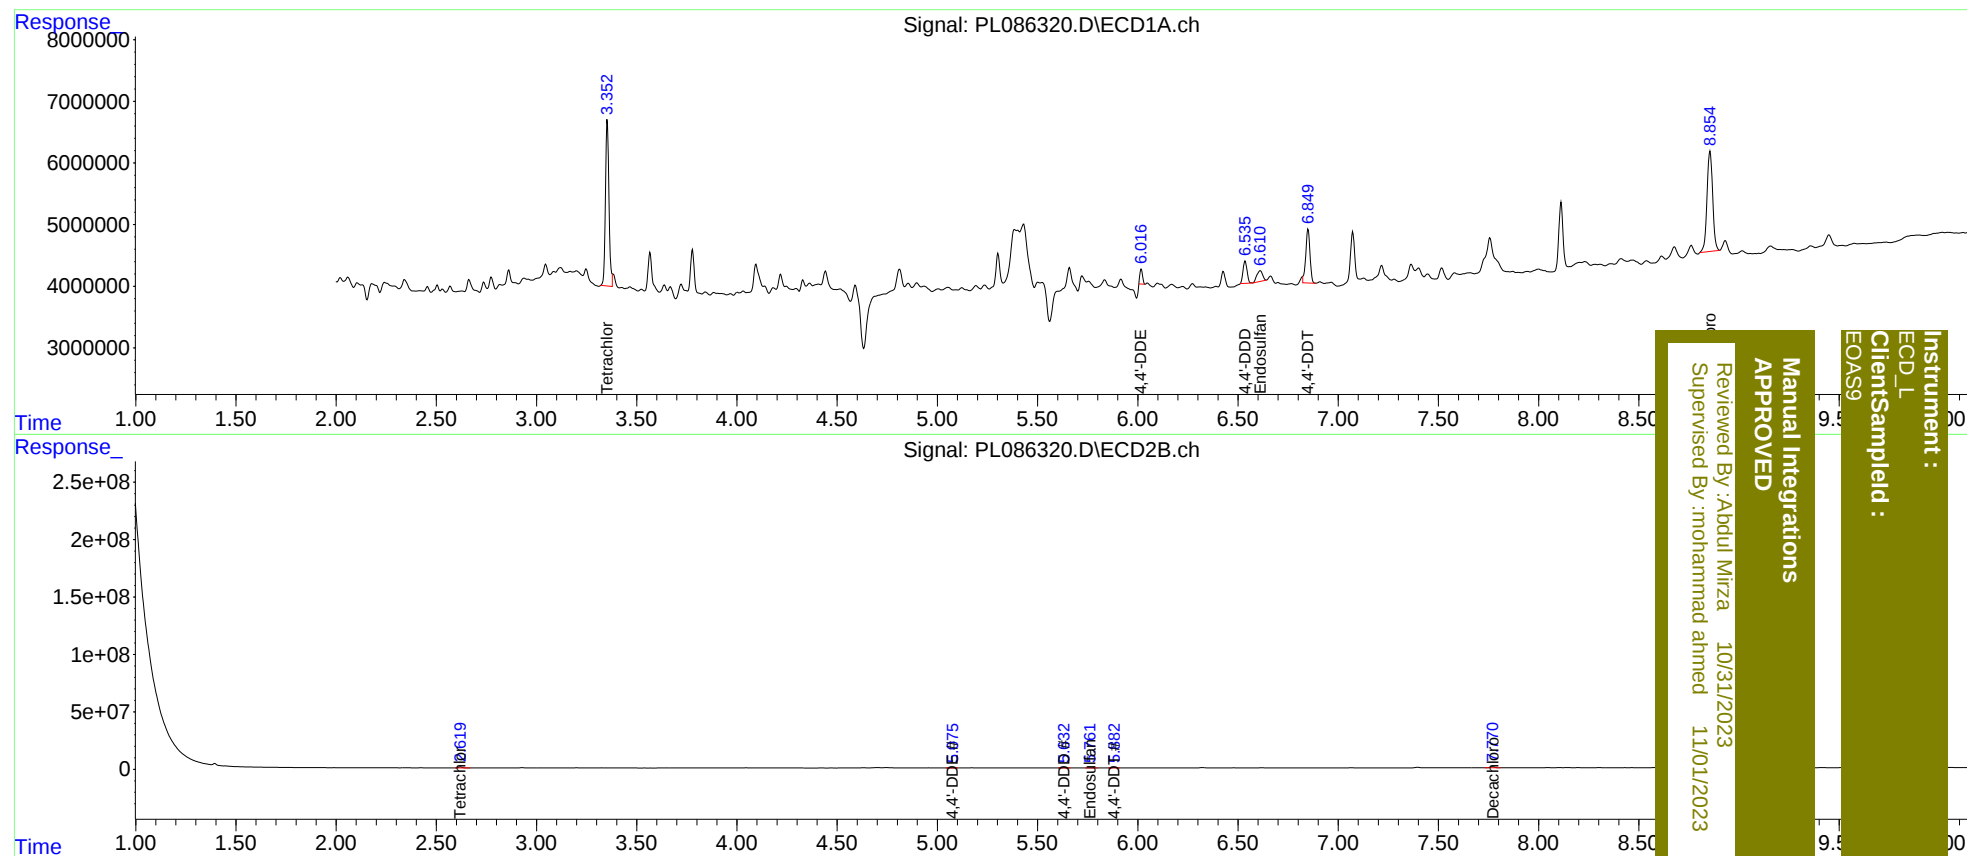

Reviewed By: Abdul Miza 10/31/2023
Supervised By: mohammad ahmed 11/01/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
EOAS9