

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
 Data File : PL086323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 01:55
 Operator : AR\AJ
 Sample : 04953-10MSD
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAT5MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/02/2023
 Supervised By : mohammad ahmed 11/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 05:05:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.354	2.620	38200892	12089551	13.403	13.329
2)	SA Decachlor...	8.856	7.771	32310436	14357576	12.965	12.508
Target Compounds							
2)	A alpha-BHC	3.806	3.118	261.4E6	75650200	62.317m	60.183
3)	MA gamma-BHC...	4.139	3.445	241.7E6	68917602	60.182	57.451
4)	MA Heptachlor	4.727	3.782	241.9E6	72507265	60.963	57.148
5)	MB Aldrin	5.066	4.057	237.7E6	83884076	59.842	69.460
6)	B beta-BHC	4.343	3.747	103.4E6	30871029	55.815	50.376
7)	B delta-BHC	4.584	3.973	230.9E6	66955929	62.070m	53.677
8)	B Heptachlo...	5.495	4.563	192.4E6	62476380	56.742m	53.570
9)	A Endosulfan I	5.880	4.930	187.5E6	57694638	58.348	53.739m
10)	B trans-Chl...	5.752	4.815	209.2E6	63924850	59.811m	55.826
11)	B cis-Chlor...	5.833	4.879	208.0E6	64383610	59.171	54.554
12)	B 4,4'-DDE	6.017	5.078	376.6E6	127.5E6	119.991	116.458
13)	MA Dieldrin	6.158	5.196	427.5E6	140.4E6	121.642	115.756
14)	MA Endrin	6.386	5.470	377.8E6	129.3E6	128.803	125.483
15)	B Endosulfa...	6.609	5.767	352.5E6	122.0E6	112.634	112.066
16)	A 4,4'-DDD	6.534	5.634	305.5E6	105.1E6	128.747m	120.125
17)	MA 4,4'-DDT	6.850	5.884	309.1E6	116.0E6	129.121	128.901
18)	B Endrin al...	6.740	5.949	258.3E6	91090206	110.954	96.187
19)	B Endosulfa...	6.975	6.174	337.3E6	118.4E6	118.602	108.035
20)	A Methoxychlor	7.337	6.469	853.8E6	327.0E6	677.044	570.049
21)	B Endrin ke...	7.457	6.675	354.0E6	135.6E6	122.888m	110.046

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
 Data File : PL086323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 01:55
 Operator : AR\AJ
 Sample : 04953-10MSD
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 05:05:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

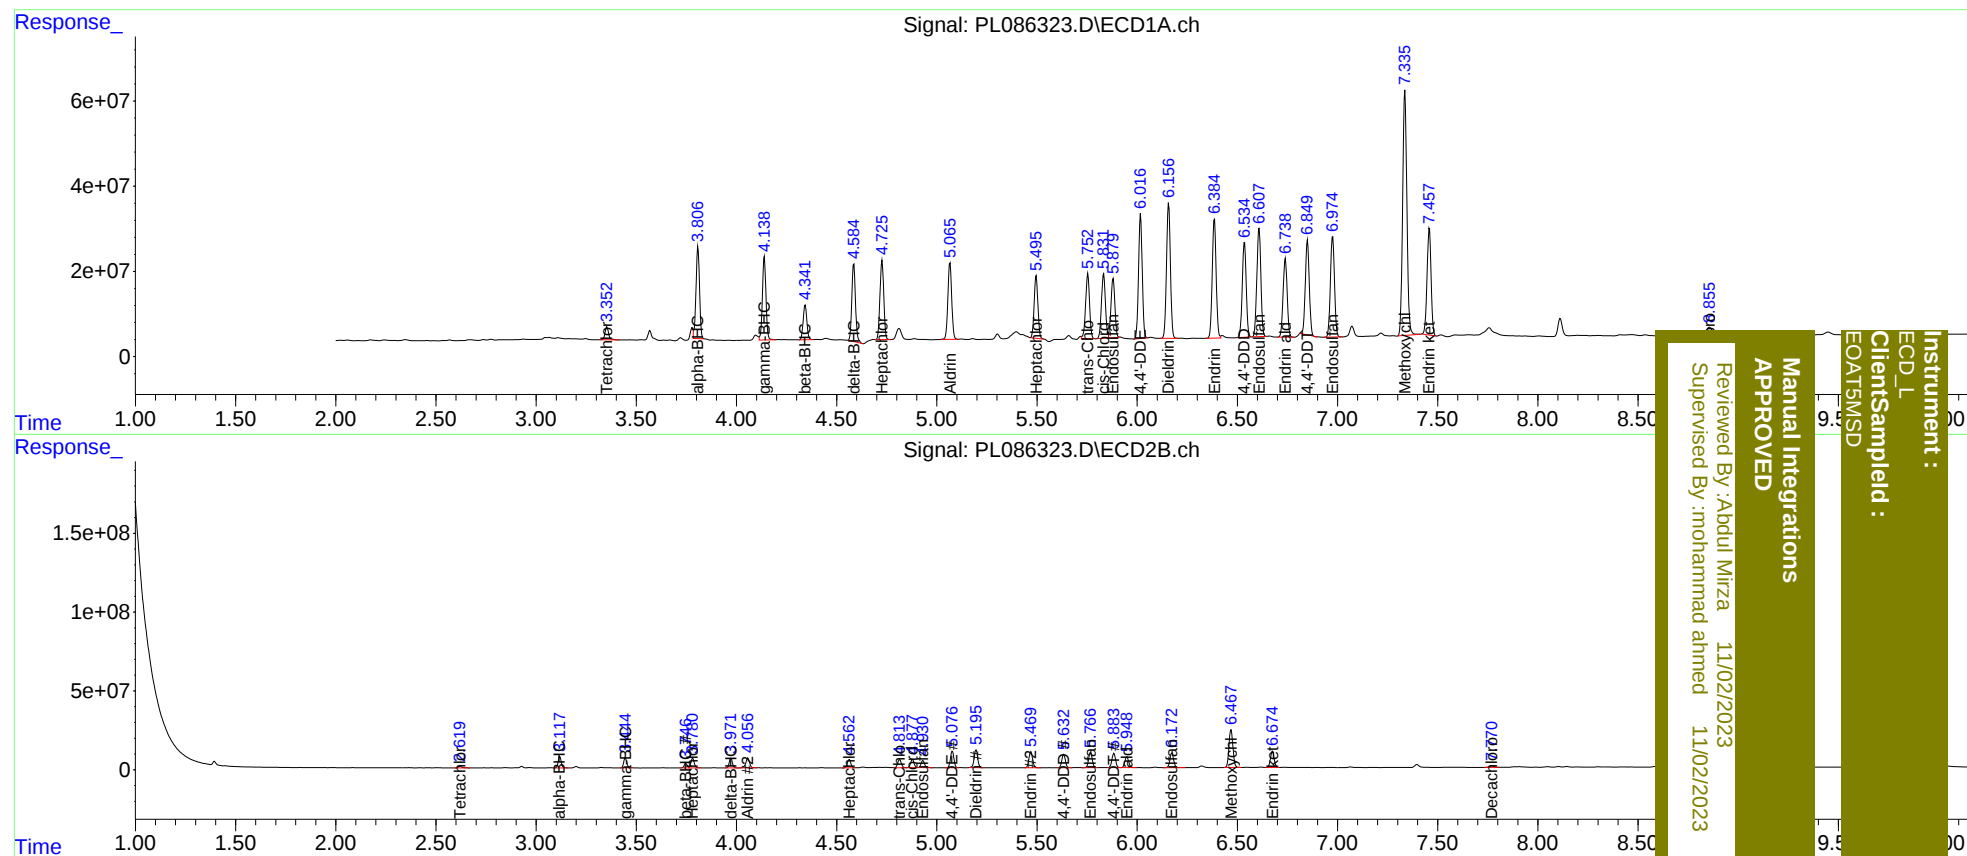

Reviewed By: Abdul Miza 11/02/2023
 Supervised By: mohammad ahmed 11/02/2023

Manual Integrations
 APPROVED

Instrument :
 ECD_L
 Client Sampled :
 EOAT5MSD