

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
 Data File : PL086321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 01:27
 Operator : AR\AJ
 Sample : 04953-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAT5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 05:04:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.354	2.620	44172109	13374632	15.498	14.746
2)	SA Decachlor...	8.854	7.771	35795096	16095299	14.363m	14.021
Target Compounds							
12)	B 4,4'-DDE	6.017	5.075	2234478	1284541	0.712m	1.173m#
15)	B Endosulfa...	6.610	5.762	3077820	3076784	0.983	2.826 #
16)	A 4,4'-DDD	6.535	5.632	3409220	1700496	1.437	1.943 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
Data File : PL086321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 01:27
Operator : AR\AJ
Sample : 04953-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 05:04:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 27 01:35:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

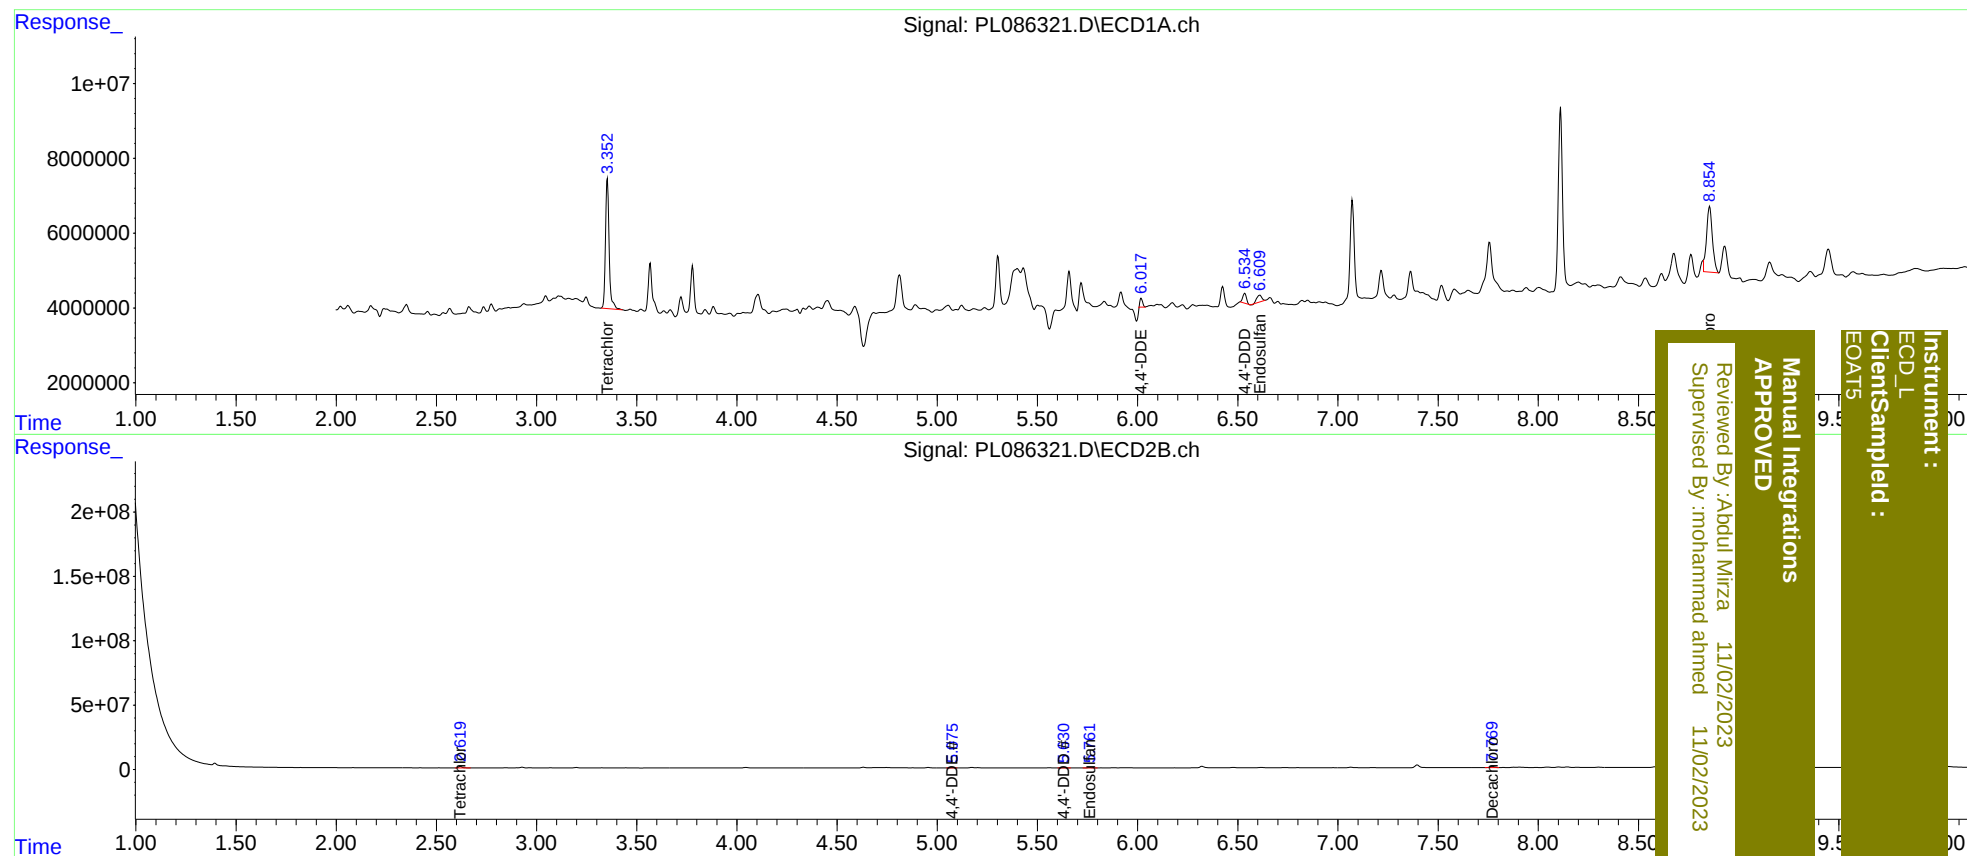

Reviewed By: Abdul Miza 11/02/2023
Supervised By: mohammad ahmed 11/02/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
EOAT5