

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
 Data File : PL086322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 01:41
 Operator : AR\AJ
 Sample : 04953-09MS
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAT5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/31/2023
 Supervised By : mohammad ahmed 11/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 05:05:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.620	37861823	11995805	13.284	13.226
27)	SA Decachlor...	8.855	7.770	33737731	14956469	13.538	13.029
Target Compounds							
2)	A alpha-BHC	3.806	3.118	256.1E6	74647397	61.045m	59.385
3)	MA gamma-BHC...	4.139	3.446	239.9E6	68353681	59.733	56.981
4)	MA Heptachlor	4.726	3.781	240.1E6	71622685	60.513	56.451
5)	MB Aldrin	5.065	4.057	235.9E6	82800491	59.391	68.563
6)	B beta-BHC	4.342	3.747	103.0E6	30312907	55.589	49.465
7)	B delta-BHC	4.585	3.973	222.3E6	66244419	59.755	53.107
8)	B Heptachlo...	5.494	4.563	190.4E6	62152629	56.146m	53.292
9)	A Endosulfan I	5.879	4.929	187.0E6	57418978	58.202	53.482m
10)	B trans-Chl...	5.751	4.814	198.7E6	63805150	56.828m	55.722
11)	B cis-Chlor...	5.832	4.878	206.6E6	64098522	58.765	54.312
12)	B 4,4'-DDE	6.016	5.077	374.7E6	127.1E6	119.372	116.083
13)	MA Dieldrin	6.156	5.196	425.1E6	139.0E6	120.974	114.594
14)	MA Endrin	6.385	5.469	376.3E6	128.7E6	128.311	124.970
15)	B Endosulfa...	6.608	5.768	351.0E6	121.5E6	112.140	111.557
16)	A 4,4'-DDD	6.534	5.634	304.5E6	105.1E6	128.358m	120.122
17)	MA 4,4'-DDT	6.851	5.884	307.3E6	115.7E6	128.382	128.502
18)	B Endrin al...	6.739	5.949	258.1E6	90894056	110.885	95.979
19)	B Endosulfa...	6.975	6.173	337.1E6	117.8E6	118.530	107.438
20)	A Methoxychlor	7.336	6.469	853.1E6	327.1E6	676.422	570.268
21)	B Endrin ke...	7.457	6.675	344.5E6	135.2E6	119.562	109.690

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103023\
Data File : PL086322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 01:41
Operator : AR\AJ
Sample : 04953-09MS
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 05:05:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 27 01:35:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

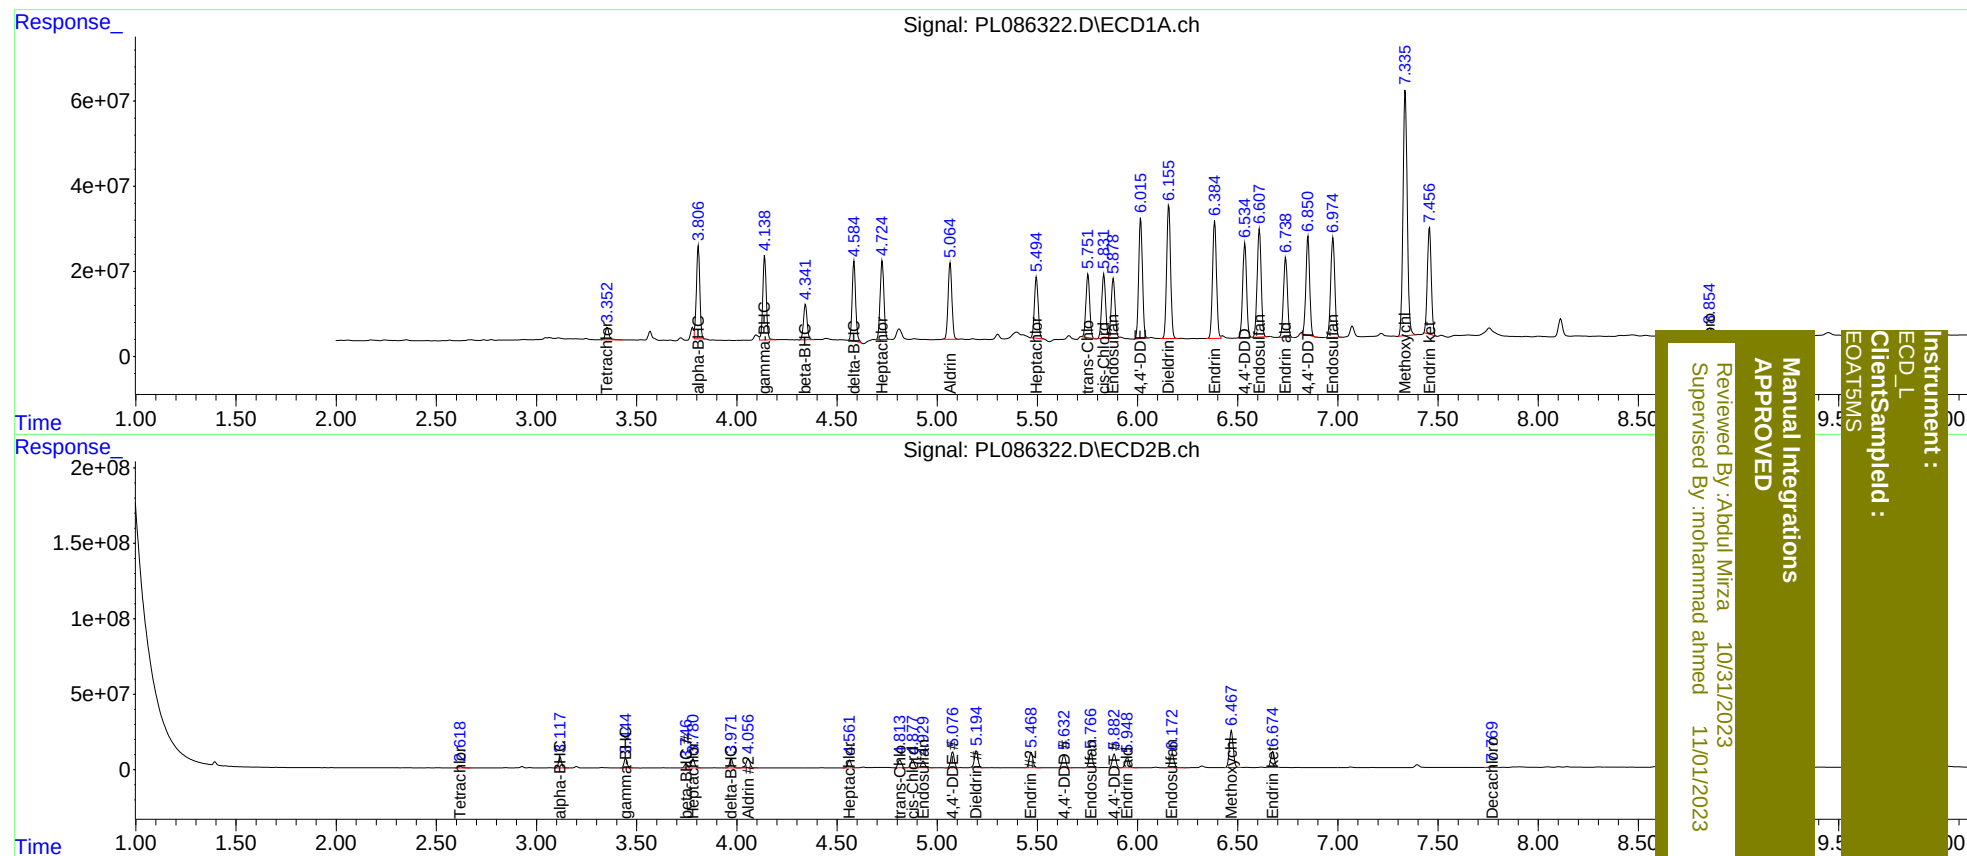

Reviewed By: Abdul Miza 10/31/2023
Supervised By: mohammad ahmed 11/01/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
EOAT5MS