

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103024\
 Data File : PL092734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2024 14:36
 Operator : AR\AJ
 Sample : P4611-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/01/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 11:17:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.777	31764673	36650276	12.964m	13.469m
28) SA Decachlor...	9.056	7.917	36126714	49729993	18.772	18.221
Target Compounds						
13) MA Dieldrin	6.336	5.367	1914320	6634751	0.726	1.986m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103024\
Data File : PL092734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2024 14:36
Operator : AR\AJ
Sample : P4611-07
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/01/2024
Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 11:17:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

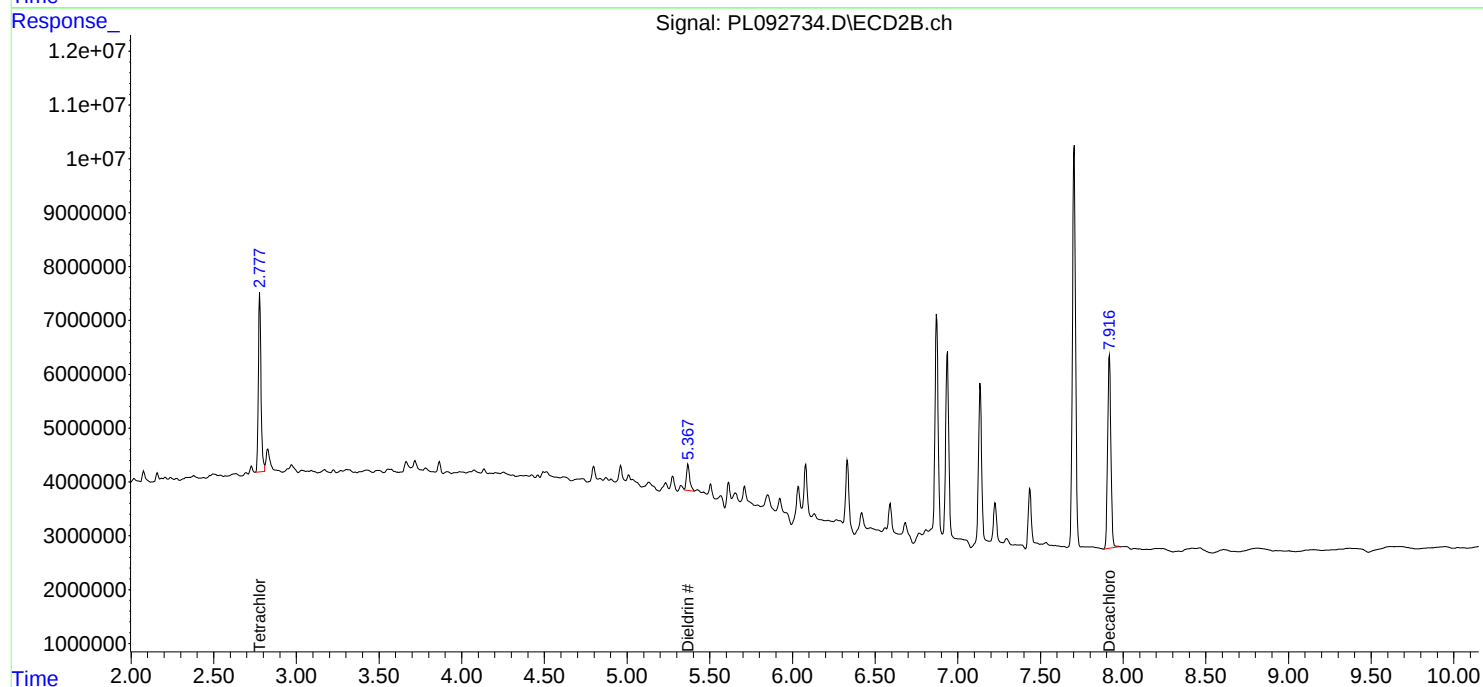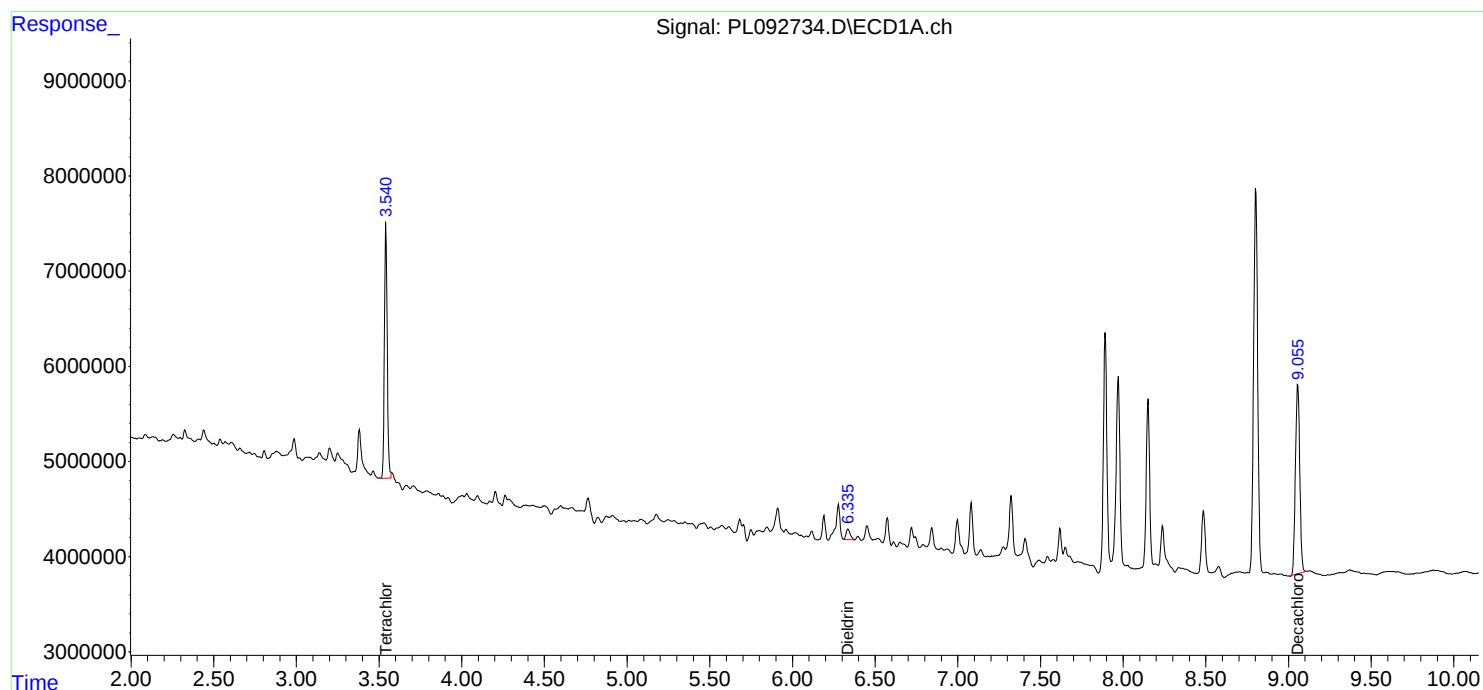

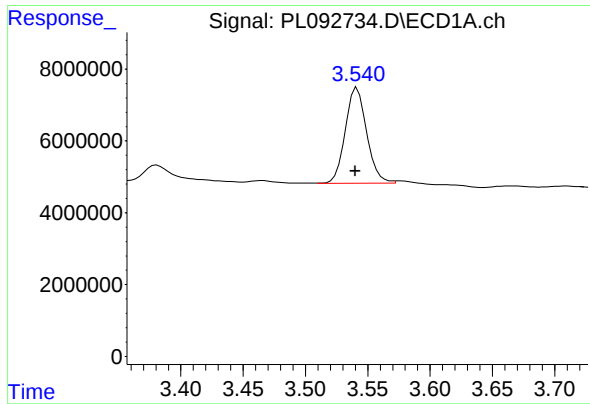


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 31764673
Conc: 12.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/01/2024
Supervised By :Ankita Jodhani 11/04/2024

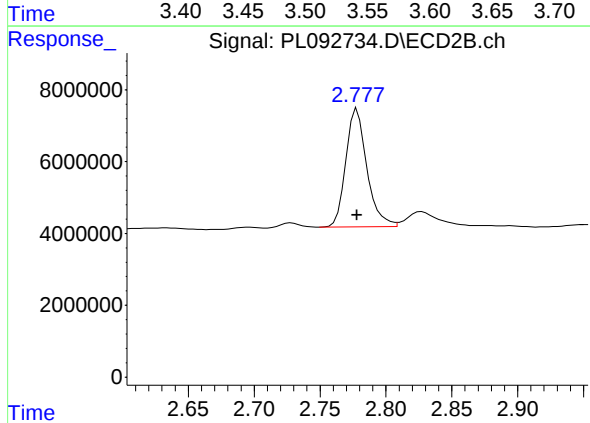


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: -0.001 min
Response: 36650276
Conc: 13.47 ng/ml m

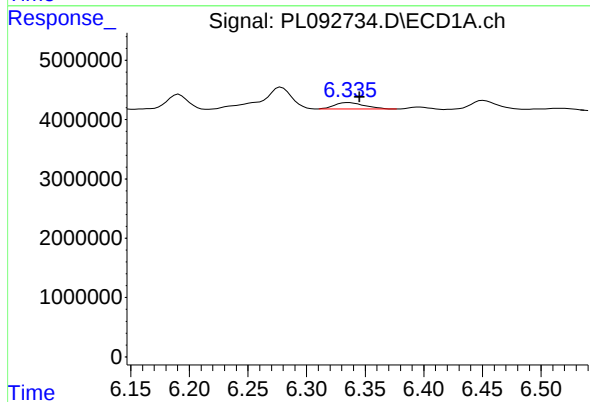


#13 Dieldrin

R.T.: 6.336 min
Delta R.T.: -0.009 min
Response: 1914320
Conc: 0.73 ng/ml

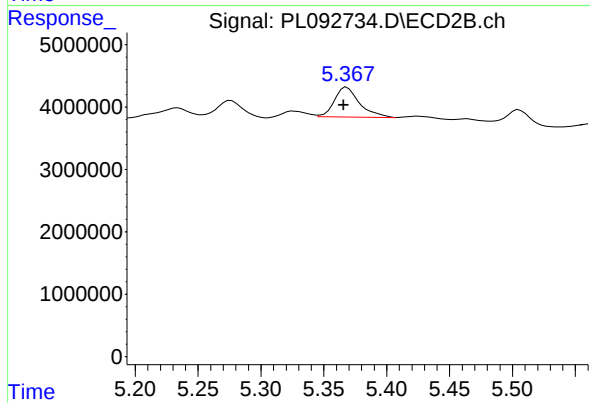

#13 Dieldrin

R.T.: 5.367 min
Delta R.T.: 0.001 min
Response: 6634751
Conc: 1.99 ng/ml m

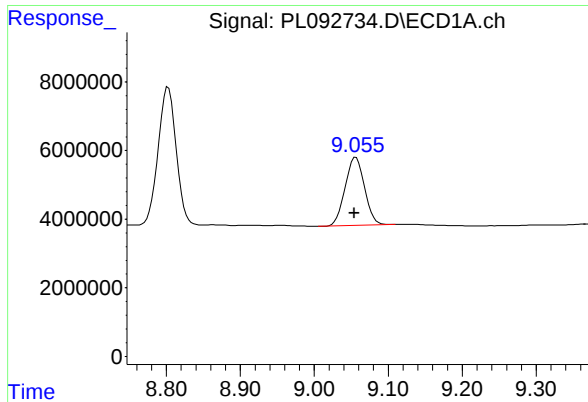

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.002 min
Response: 36126714
Conc: 18.77 ng/ml

Instrument :

ECD_L

ClientSampleId :


TP-3

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 11/01/2024

Supervised By :Ankita Jodhani 11/04/2024

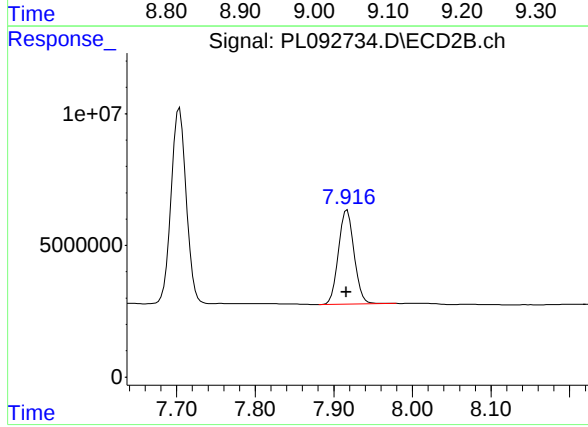

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: 0.001 min
Response: 49729993
Conc: 18.22 ng/ml