

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103025\
 Data File : PL097696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2025 16:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 23:20:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.523	2.821	90835664	135.6E6	22.199	22.531
28)	SA Decachlor...	8.999	7.982	74599085	96245889	25.074	18.007 #
Target Compounds							
15)	B Endosulfa...	6.744	0.000	3946001	0	0.867	N.D. #
18)	B Endrin al...	0.000	6.166	0	10367091	N.D.	1.801 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103025\
Data File : PL097696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2025 16:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 23:20:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

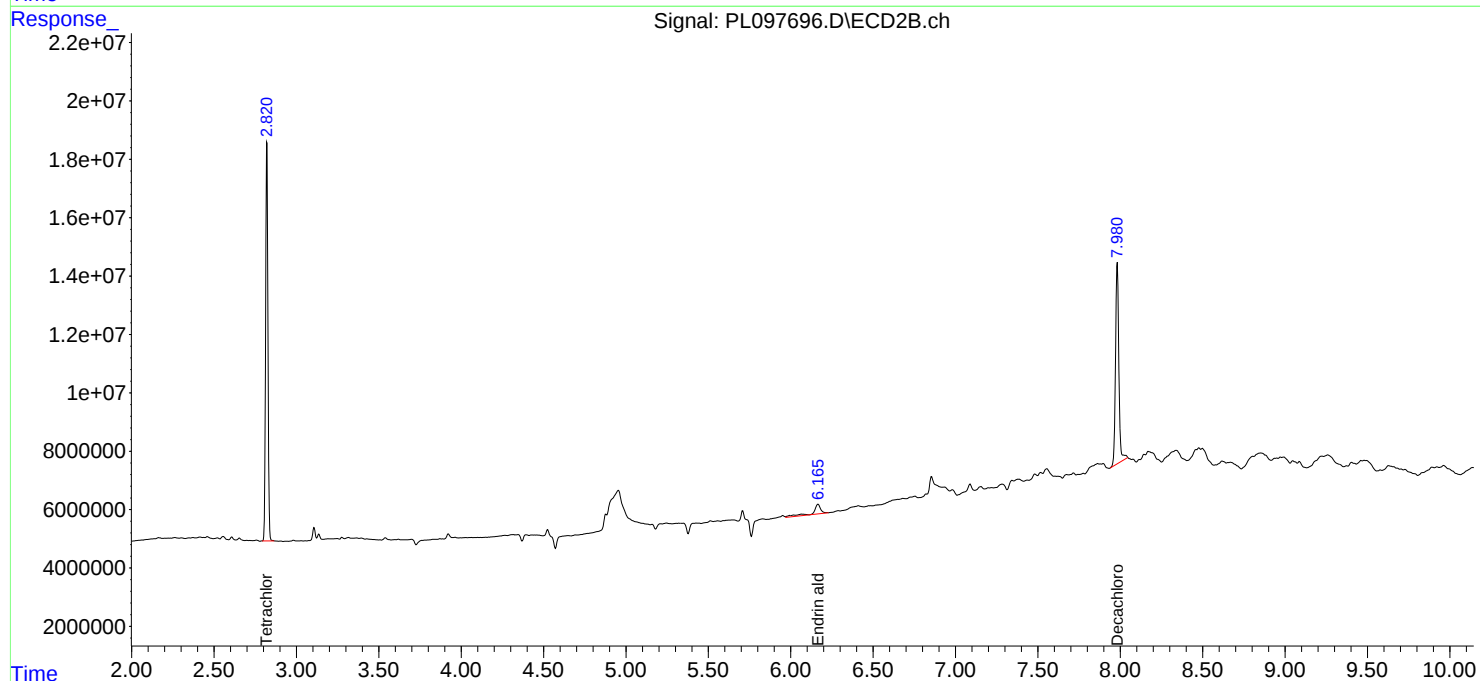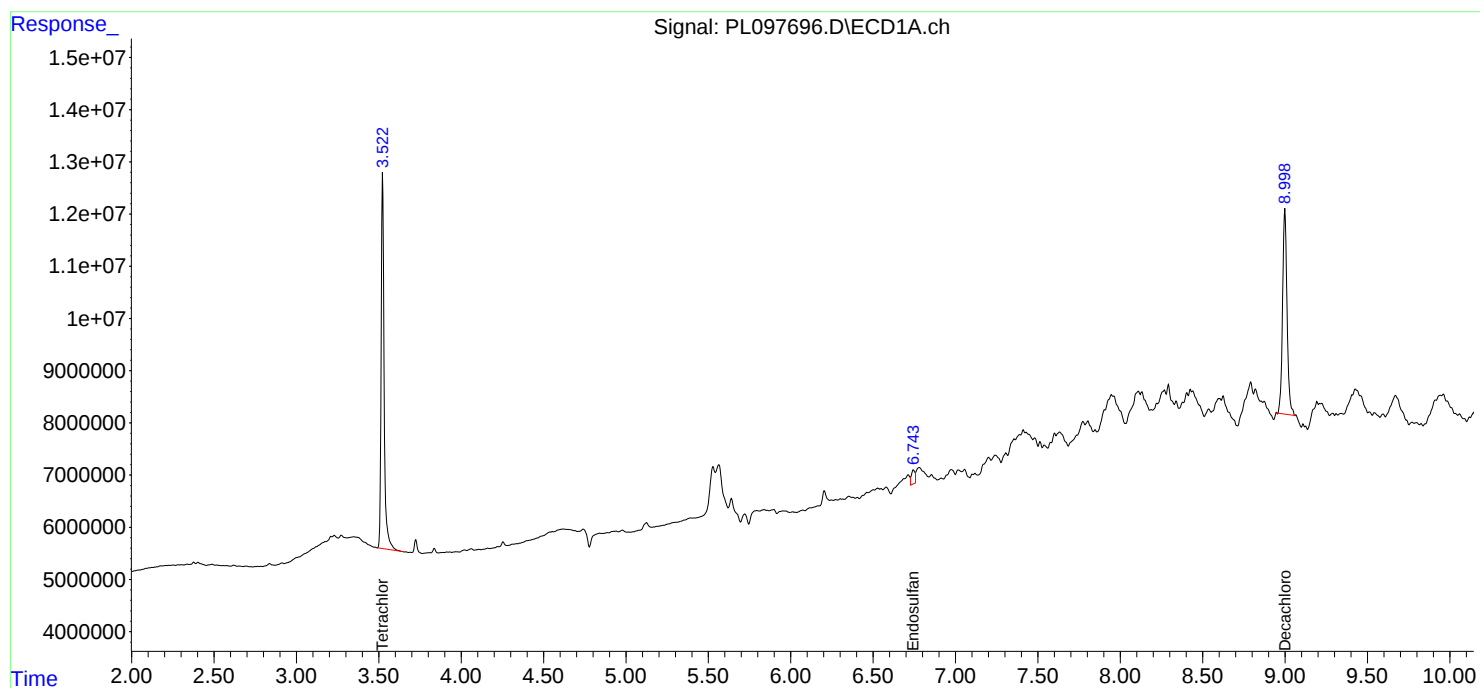


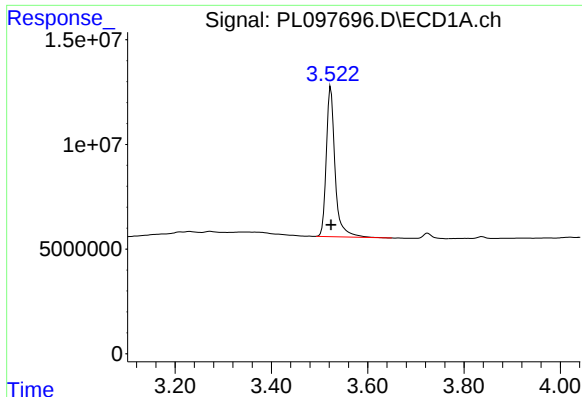

#1 Tetrachloro-m-xylene


R.T.: 3.523 min
Delta R.T.: 0.000 min
Response: 90835664
Conc: 22.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

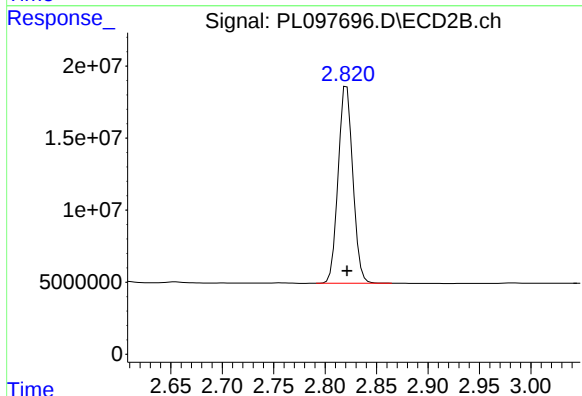


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: 0.000 min
Response: 135617001
Conc: 22.53 ng/ml

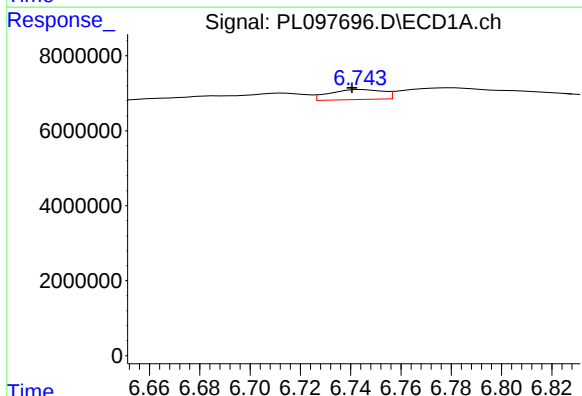


#15 Endosulfan II

R.T.: 6.744 min
Delta R.T.: 0.004 min
Response: 3946001
Conc: 0.87 ng/ml

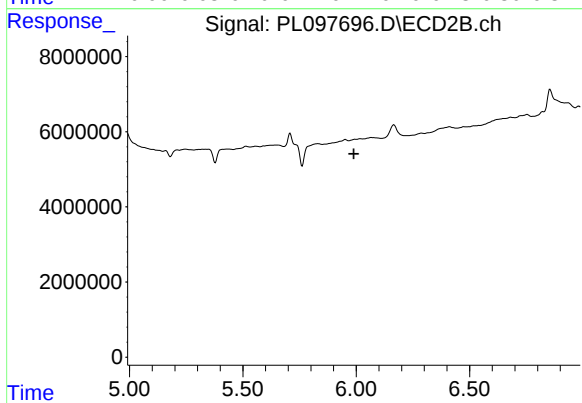

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.990 min
Response: 0
Conc: N.D.

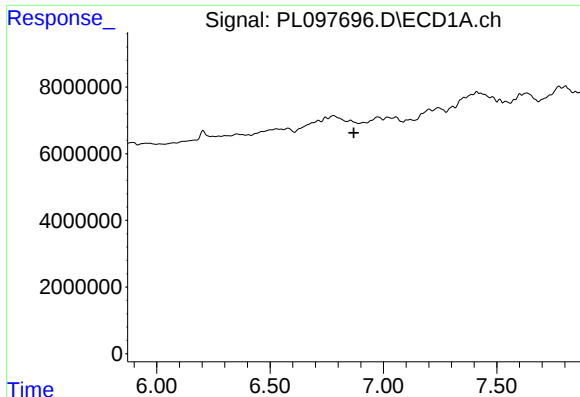

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.869 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

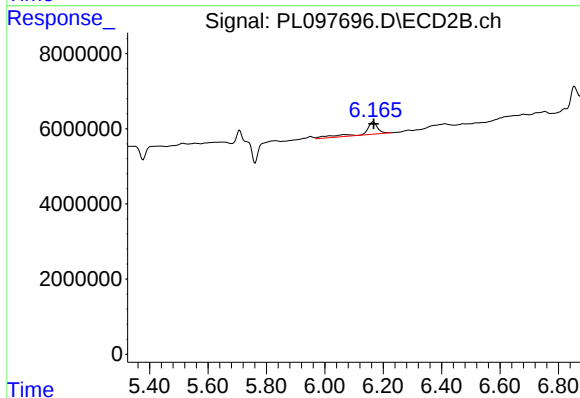


#18 Endrin aldehyde

R.T.: 6.166 min
Delta R.T.: -0.002 min
Response: 10367091
Conc: 1.80 ng/ml

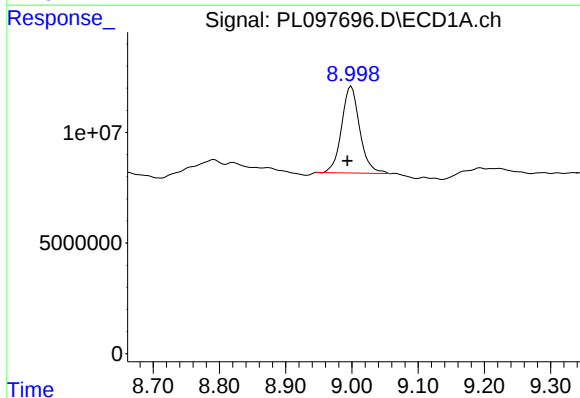

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.006 min
Response: 74599085
Conc: 25.07 ng/ml

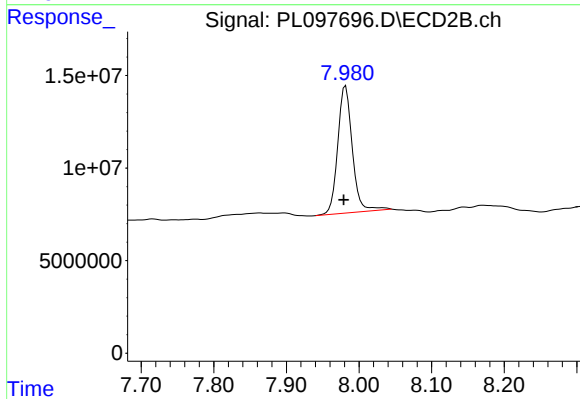

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.002 min
Response: 96245889
Conc: 18.01 ng/ml