

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103025\
 Data File : PL097686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2025 13:04
 Operator : AR\AJ
 Sample : Q3486-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP3

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 10/31/2025
 Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 23:18:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.524	2.822	73773372	103.9E6	18.029m	17.262
2) SA Decachlor...	9.000	7.982	52098523	70453526	17.511	13.182

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103025\
Data File : PL097686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2025 13:04
Operator : AR\AJ
Sample : Q3486-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP3


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 23:18:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

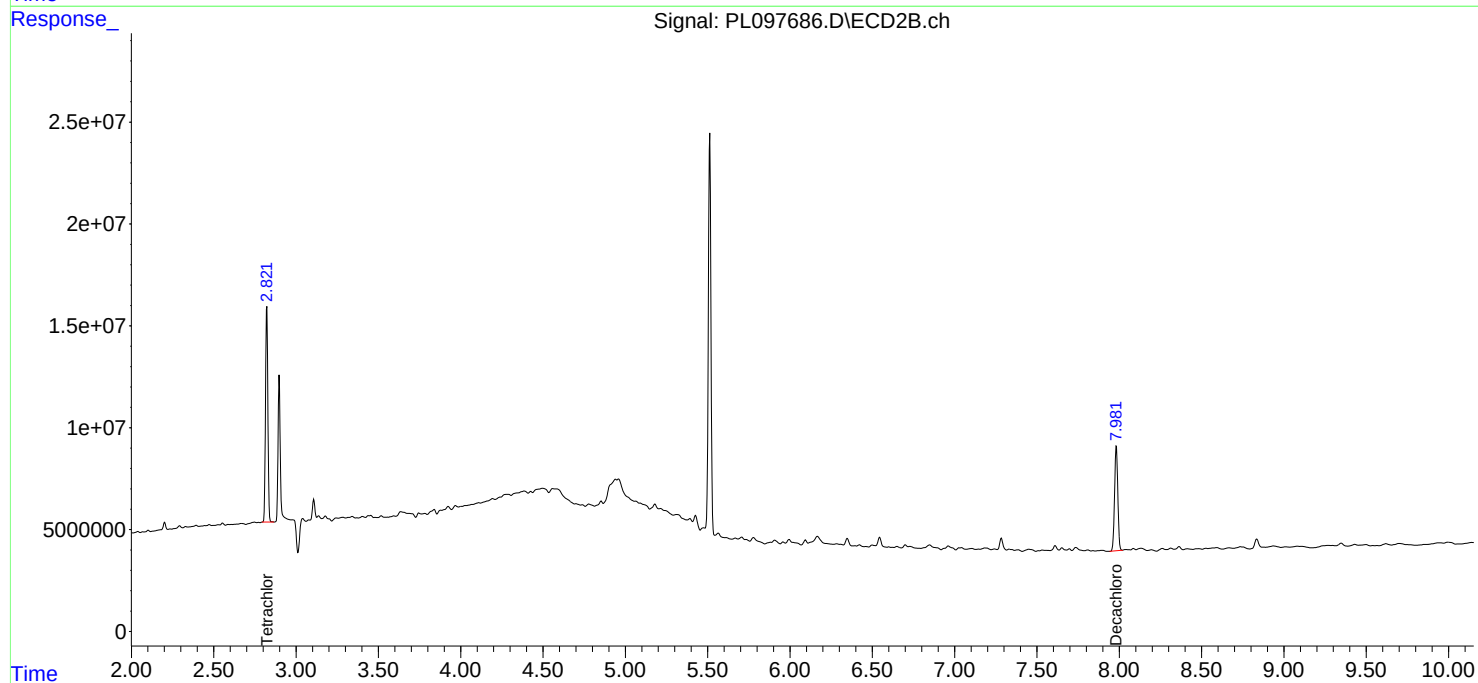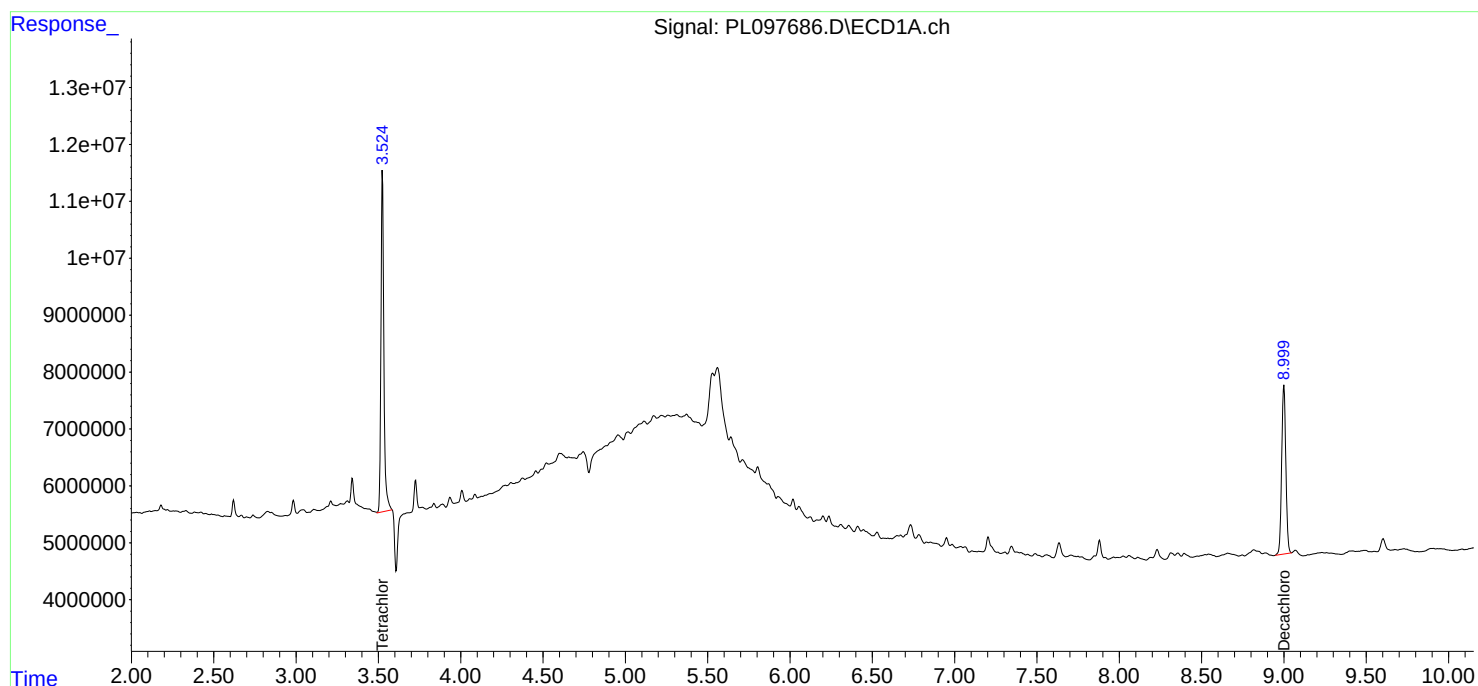

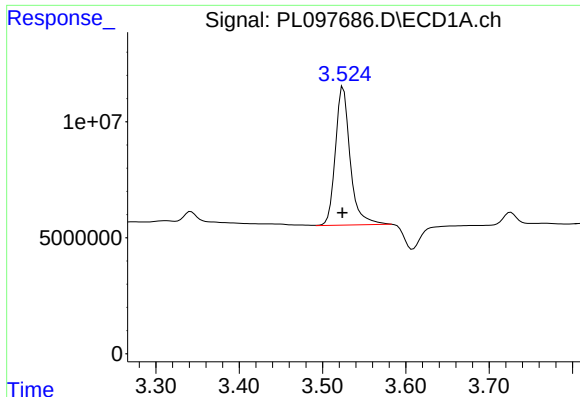


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 73773372
Conc: 18.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP3


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

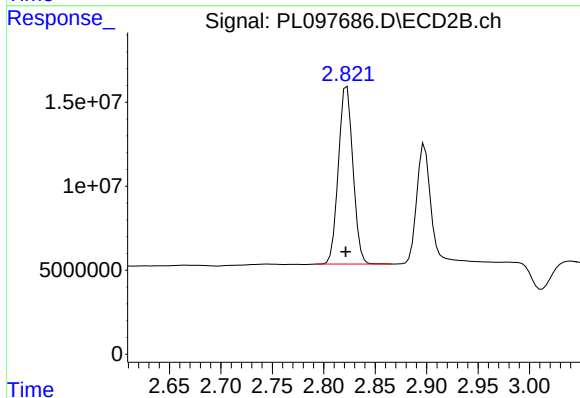


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.001 min
Response: 103901058
Conc: 17.26 ng/ml

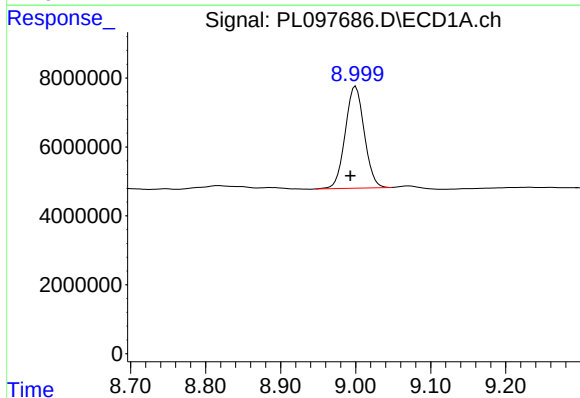

#28 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: 0.007 min
Response: 52098523
Conc: 17.51 ng/ml

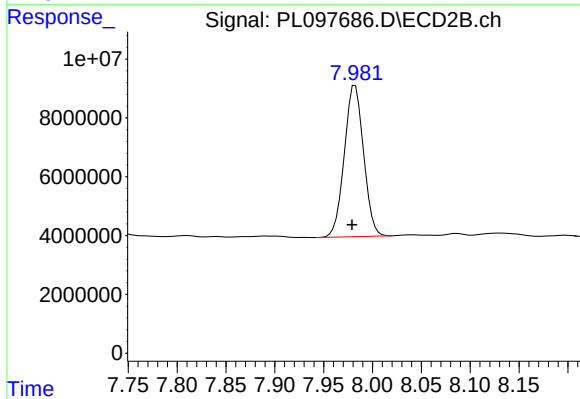

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.003 min
Response: 70453526
Conc: 13.18 ng/ml