

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
 Data File : PL041557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 17:12
 Operator : AJ\SJ
 Sample : J5205-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:24:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.103	53848990	28820878	8.453	9.357
28)	SA Decachlor...	8.217	9.235	68441500	28820098	10.332	11.248
Target Compounds							
4)	MA Heptachlor	4.493	5.305	2783497	1177300	0.304	0.290
6)	B beta-BHC	4.493f	0.000	2783497	0	0.738	N.D. #
9)	A Endosulfan I	5.467f	6.309f	1927192	5570963	0.259	1.792 #
10)	B gamma-Chl...	5.430	0.000	7519409	0	0.923	N.D. #
11)	B alpha-Chl...	5.467	6.309	1927192	5570963	0.238	1.646 #
12)	B 4,4'-DDE	5.633	6.462	22689603	13863233	3.170	4.236 #
14)	MA Endrin	6.023	0.000	2075724	0	0.284	N.D. #
17)	MA 4,4'-DDT	6.387	7.254	6007379	2737665	0.987	1.089
25)	Chlordane-3	5.430	0.000	7519409	0	8.437	N.D. #
26)	Chlordane-4	5.467	6.309	1927192	5570963	2.461	10.656 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
Data File : PL041557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 17:12
Operator : AJ\SJ
Sample : J5205-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:24:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

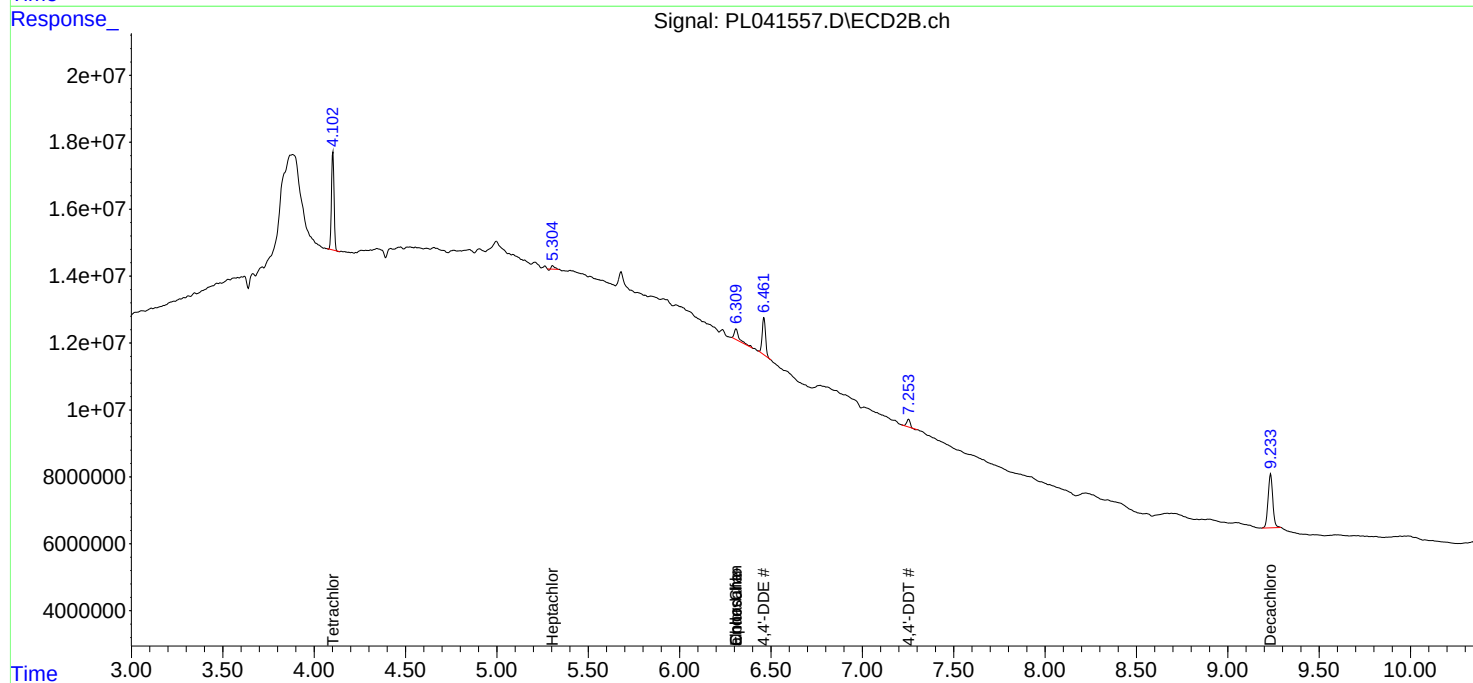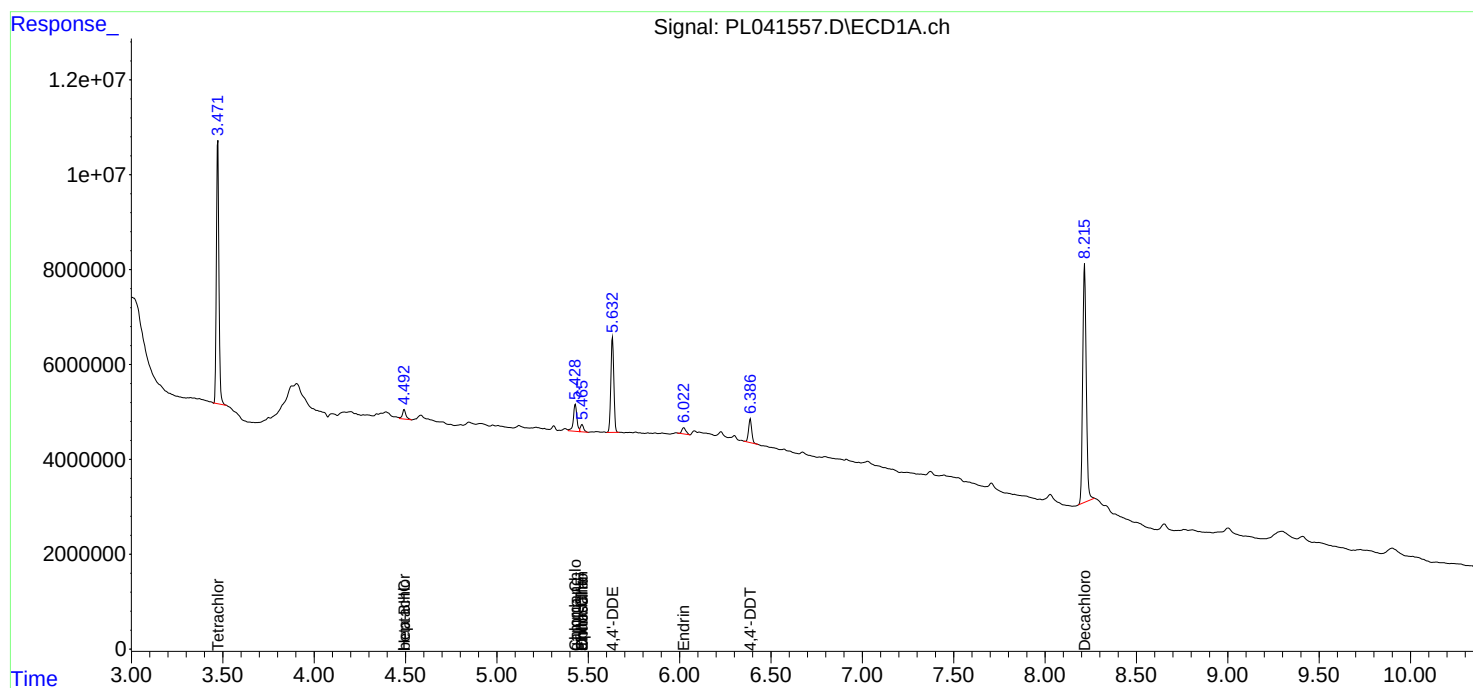


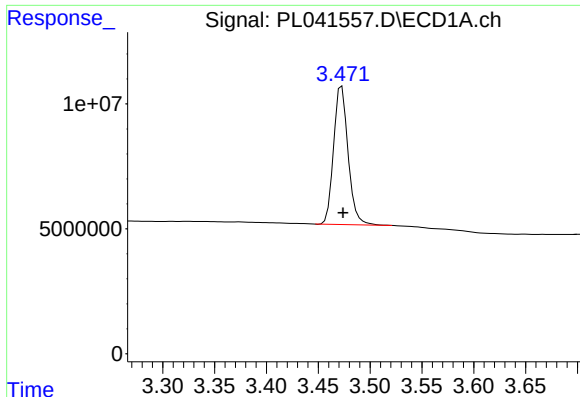

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 53848990
Conc: 8.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

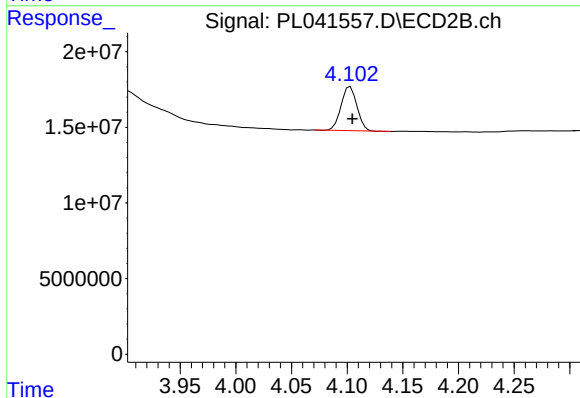


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.002 min
Response: 28820878
Conc: 9.36 ng/ml

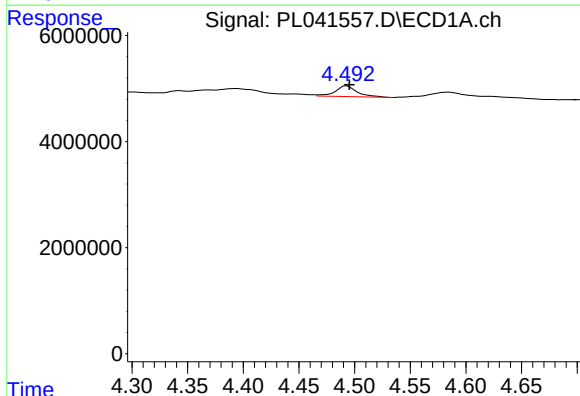


#4 Heptachlor

R.T.: 4.493 min
Delta R.T.: -0.002 min
Response: 2783497
Conc: 0.30 ng/ml

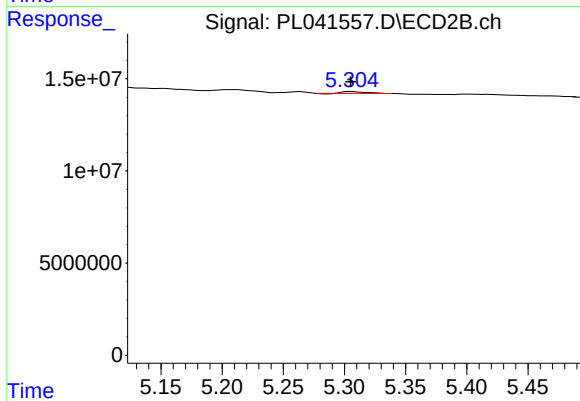

#4 Heptachlor


R.T.: 5.305 min
Delta R.T.: 0.000 min
Response: 1177300
Conc: 0.29 ng/ml

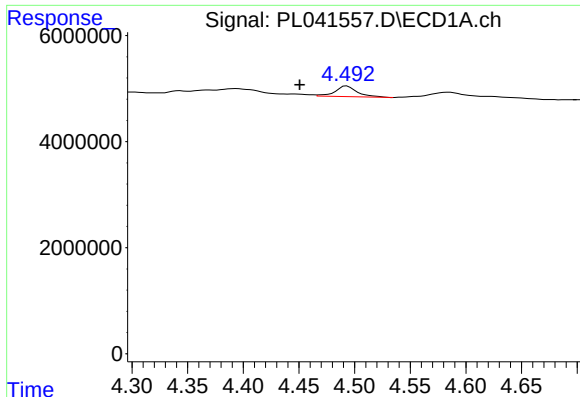

#6 beta-BHC


R.T.: 4.493 min
Delta R.T.: 0.042 min
Response: 2783497
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

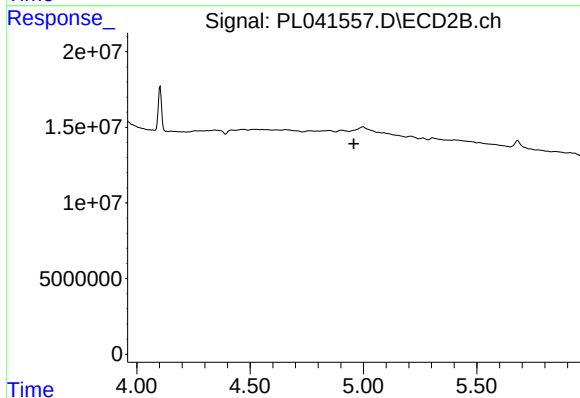


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

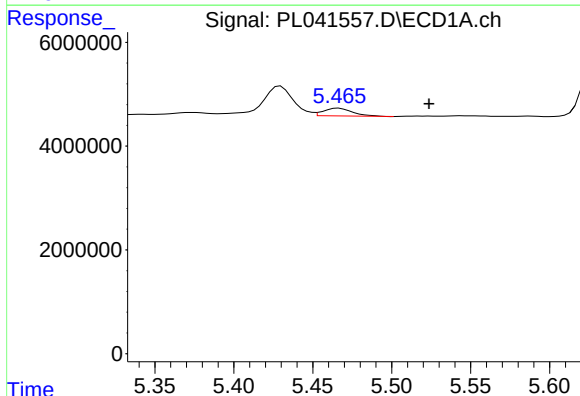


#9 Endosulfan I

R.T.: 5.467 min
Delta R.T.: -0.057 min
Response: 1927192
Conc: 0.26 ng/ml

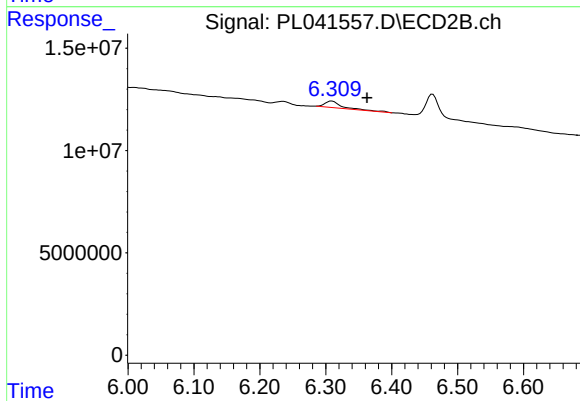

#9 Endosulfan I


R.T.: 6.309 min
Delta R.T.: -0.053 min
Response: 5570963
Conc: 1.79 ng/ml

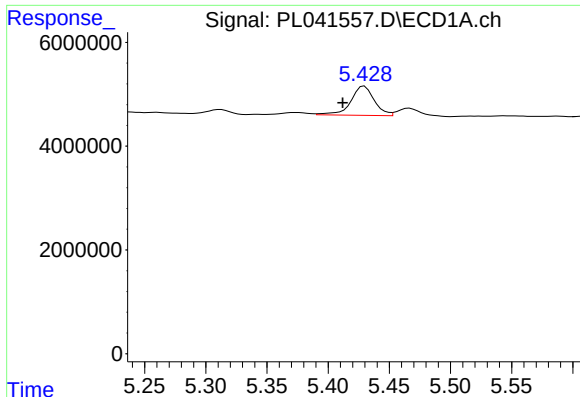

#10 gamma-Chlordane


R.T.: 5.430 min
Delta R.T.: 0.018 min
Response: 7519409
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

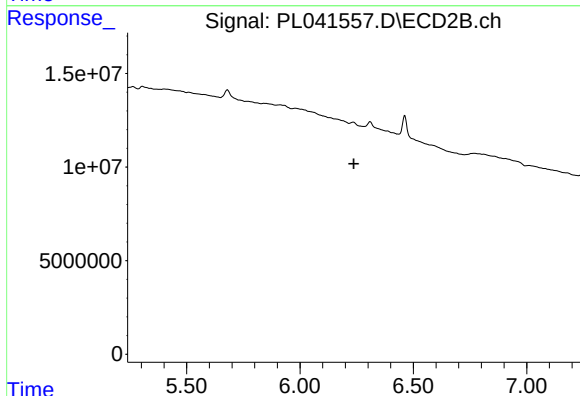


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

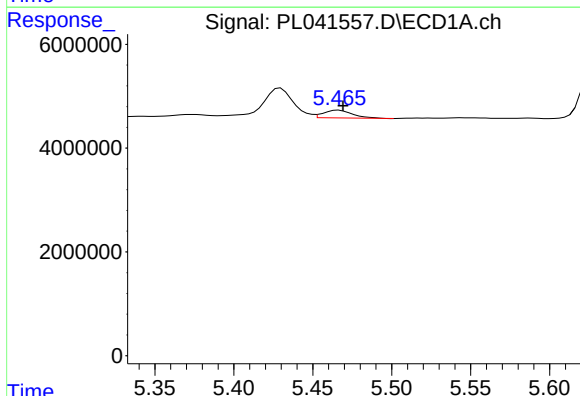


#11 alpha-Chlordane

R.T.: 5.467 min
Delta R.T.: -0.002 min
Response: 1927192
Conc: 0.24 ng/ml

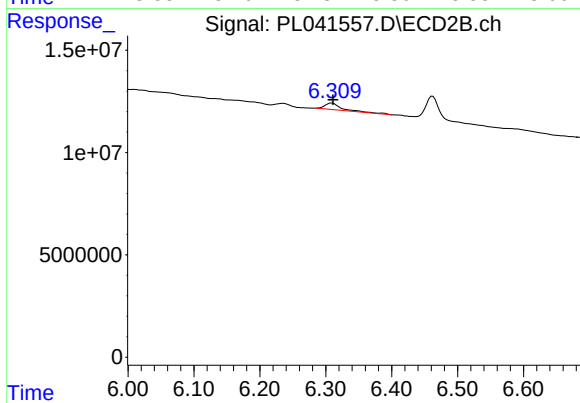

#11 alpha-Chlordane


R.T.: 6.309 min
Delta R.T.: -0.002 min
Response: 5570963
Conc: 1.65 ng/ml

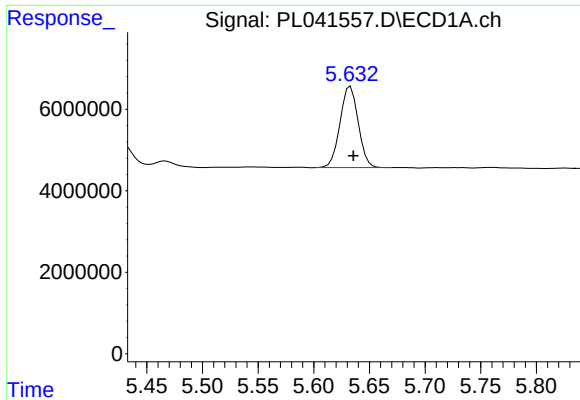

#12 4,4'-DDE


R.T.: 5.633 min
Delta R.T.: -0.002 min
Response: 22689603
Conc: 3.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

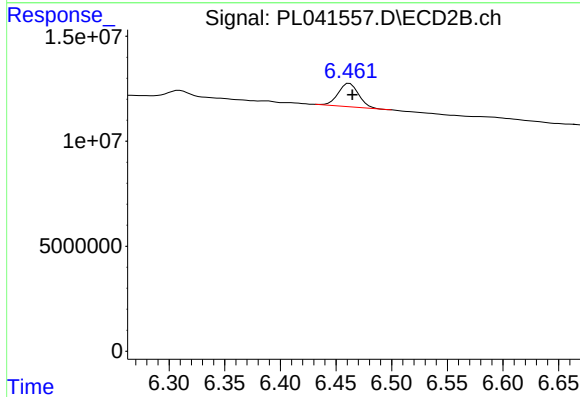


#12 4,4'-DDE

R.T.: 6.462 min
Delta R.T.: -0.002 min
Response: 13863233
Conc: 4.24 ng/ml

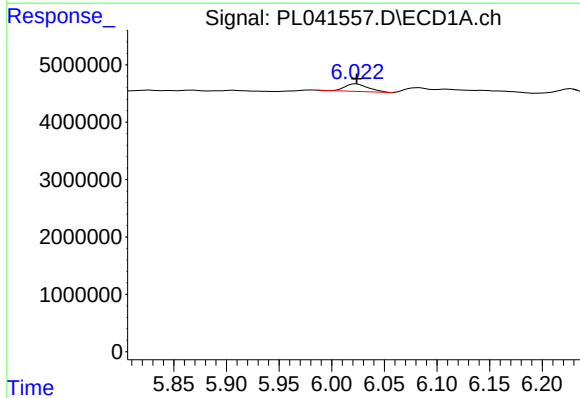


#14 Endrin

R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 2075724
Conc: 0.28 ng/ml

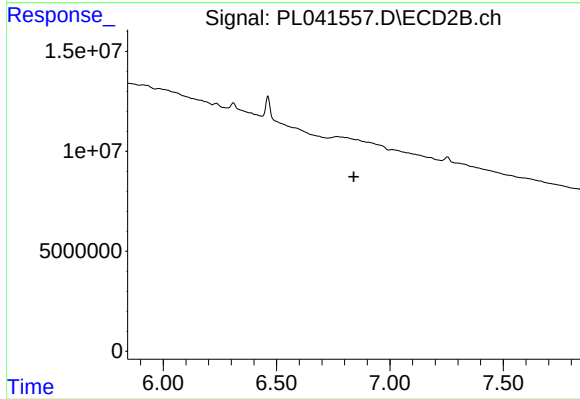

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.840 min
Response: 0
Conc: N.D.

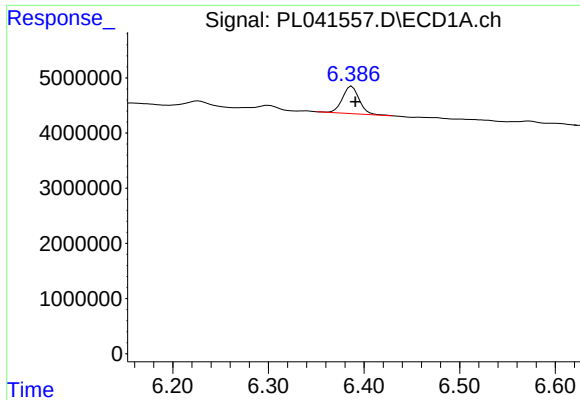

#17 4,4'-DDT


R.T.: 6.387 min
Delta R.T.: -0.004 min
Response: 6007379
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

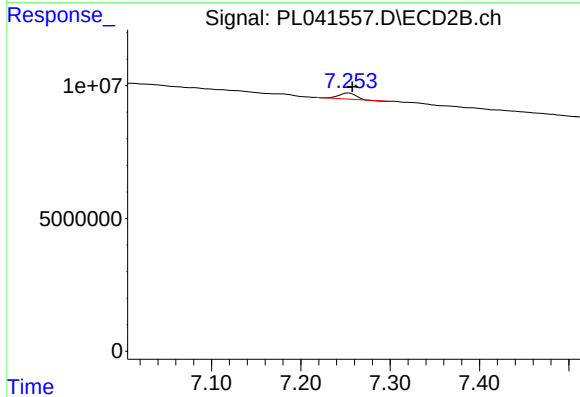


#17 4,4'-DDT

R.T.: 7.254 min
Delta R.T.: -0.004 min
Response: 2737665
Conc: 1.09 ng/ml

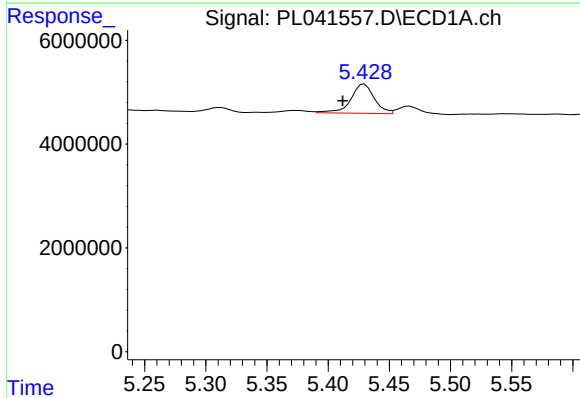


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.018 min
Response: 7519409
Conc: 8.44 ng/ml

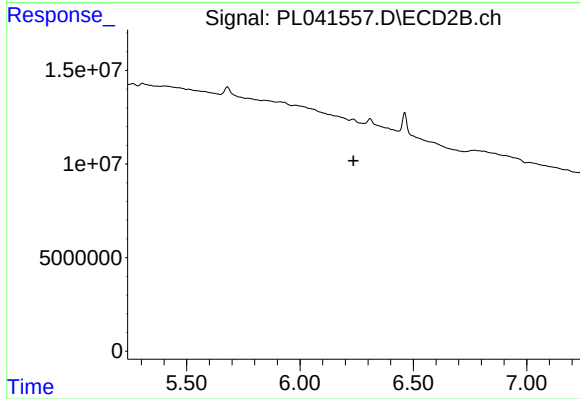

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

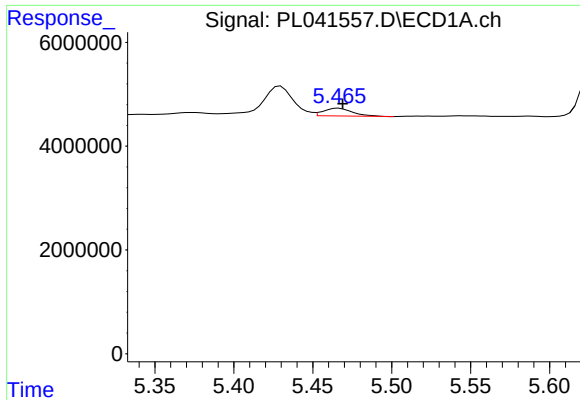

#26 Chlordane-4


R.T.: 5.467 min
Delta R.T.: -0.002 min
Response: 1927192
Conc: 2.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

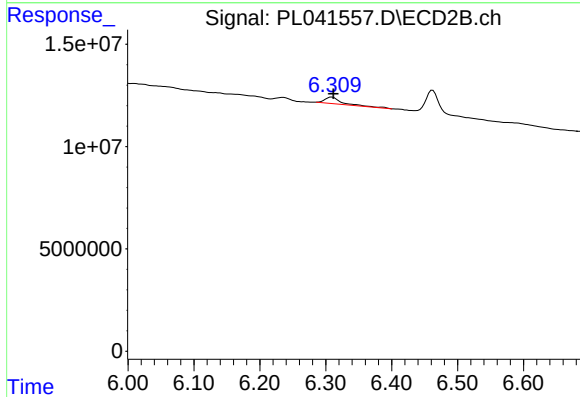


#26 Chlordane-4

R.T.: 6.309 min
Delta R.T.: -0.002 min
Response: 5570963
Conc: 10.66 ng/ml

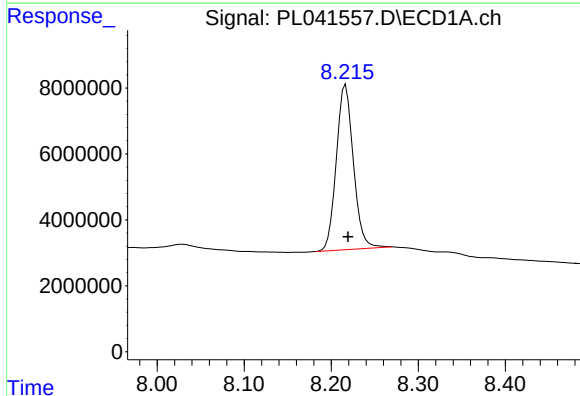

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 68441500
Conc: 10.33 ng/ml

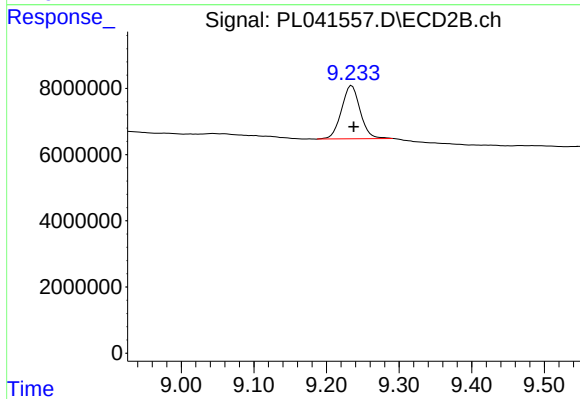

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.003 min
Response: 28820098
Conc: 11.25 ng/ml