

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
 Data File : PL041559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 17:40
 Operator : AJ\SJ
 Sample : J5728-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:25:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.103	92545195	49101426	14.528	15.941
28)	SA Decachlor...	8.216	9.235	72513267	31106810	10.947	12.141
Target Compounds							
4)	MA Heptachlor	4.457f	0.000	2213747	0	0.242	N.D. #
6)	B beta-BHC	4.457	0.000	2213747	0	0.587	N.D. #
9)	A Endosulfan I	5.545	0.000	3848335	0	0.517	N.D. #
10)	B gamma-Chl...	5.469f	6.237	5769761	-1545846	0.709	N.D. #
11)	B alpha-Chl...	5.469	0.000	5769761	0	0.713	N.D. #
15)	B Endosulfa...	6.230f	0.000	2669919	0	0.386	N.D. #
23)	Chlordane-1	4.362	0.000	5540118	0	19.539	N.D. #
25)	Chlordane-3	5.469	6.237	5769761	-1545846	6.474	N.D. #
26)	Chlordane-4	5.469	0.000	5769761	0	7.369	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
Data File : PL041559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 17:40
Operator : AJ\SJ
Sample : J5728-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:25:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

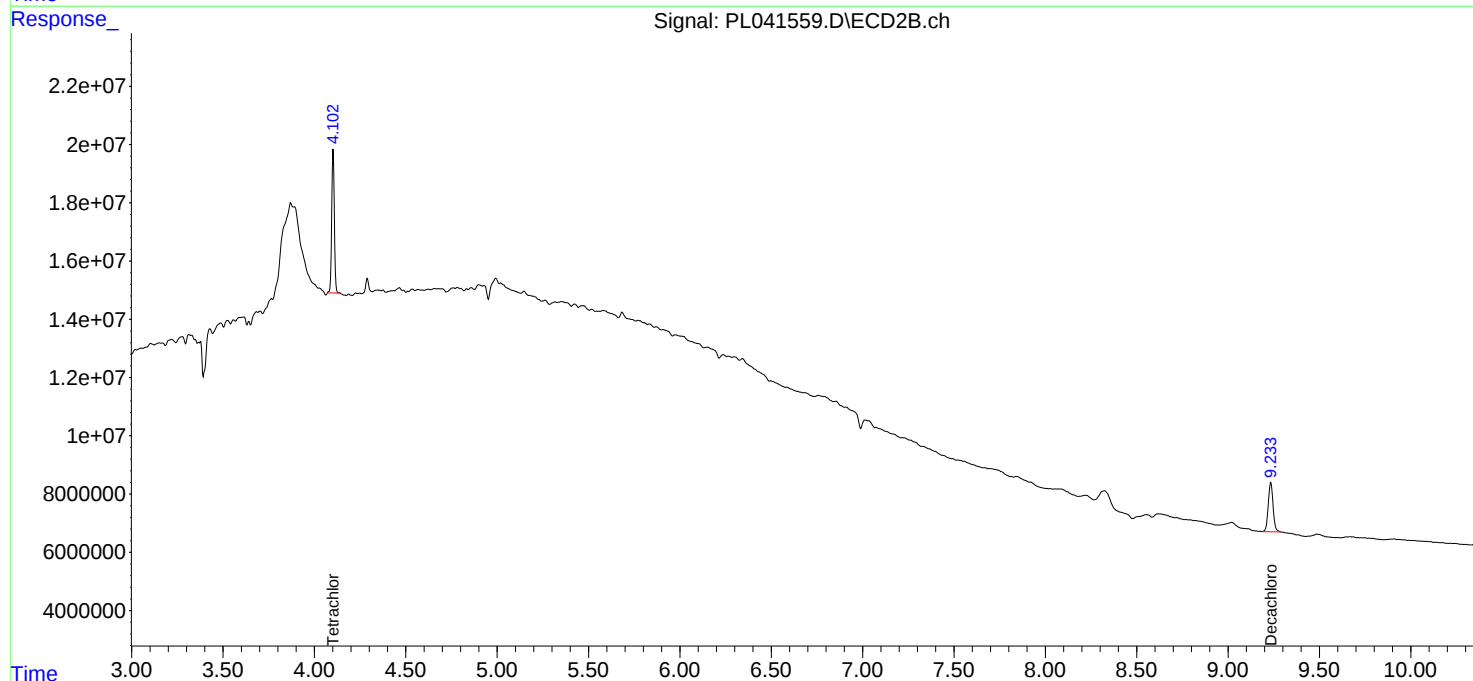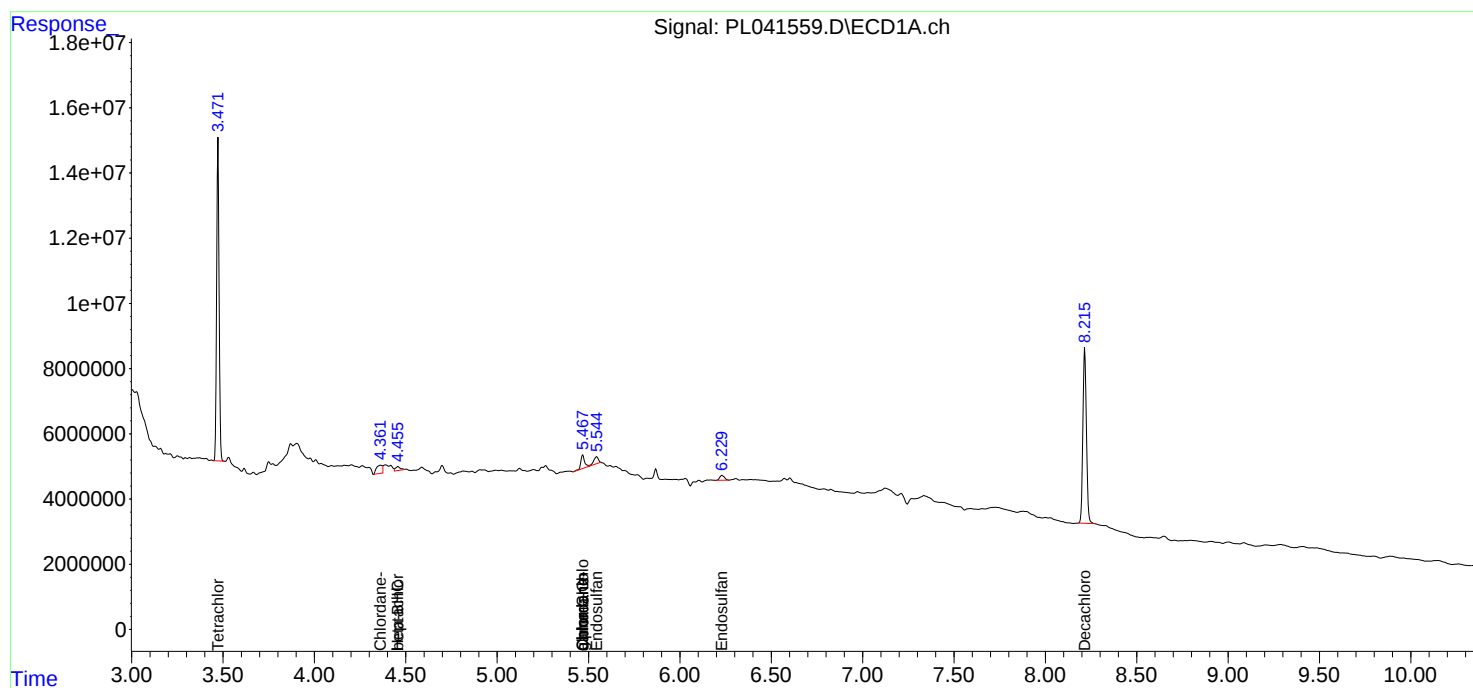


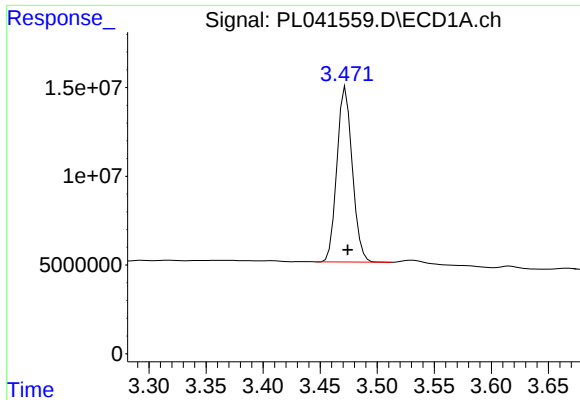

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 92545195
Conc: 14.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

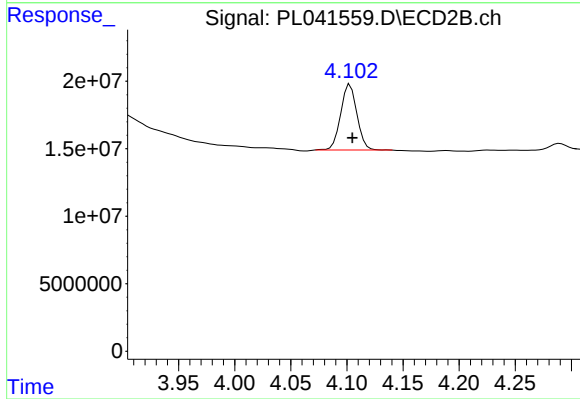


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.002 min
Response: 49101426
Conc: 15.94 ng/ml

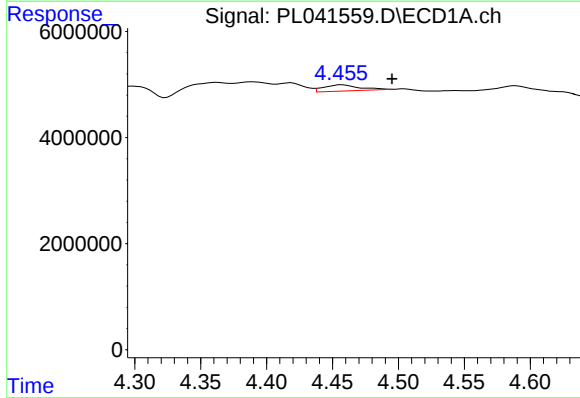


#4 Heptachlor

R.T.: 4.457 min
Delta R.T.: -0.038 min
Response: 2213747
Conc: 0.24 ng/ml

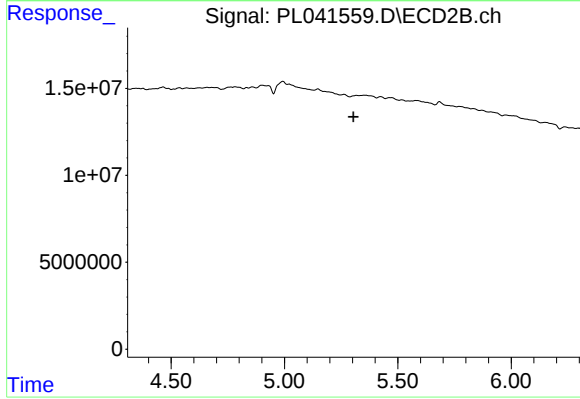

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.305 min
Response: 0
Conc: N.D.

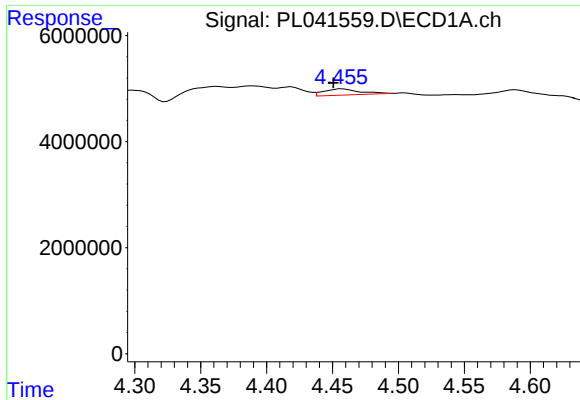

#6 beta-BHC


R.T.: 4.457 min
Delta R.T.: 0.007 min
Response: 2213747
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

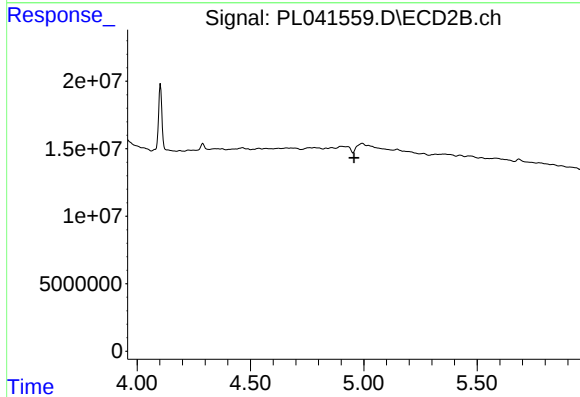


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

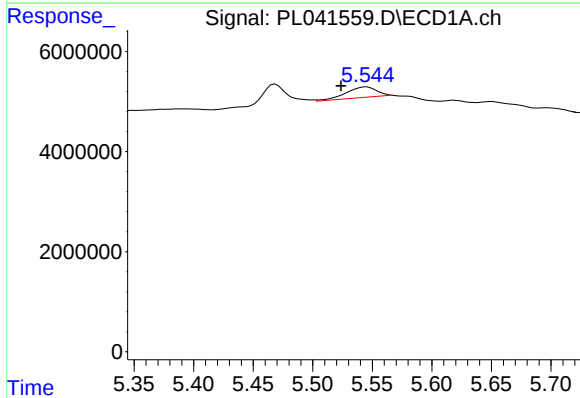


#9 Endosulfan I

R.T.: 5.545 min
Delta R.T.: 0.021 min
Response: 3848335
Conc: 0.52 ng/ml

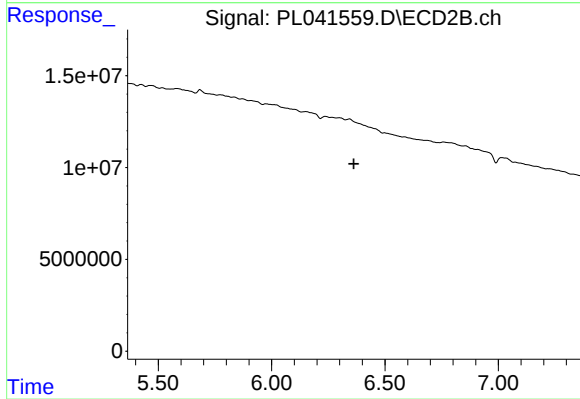

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

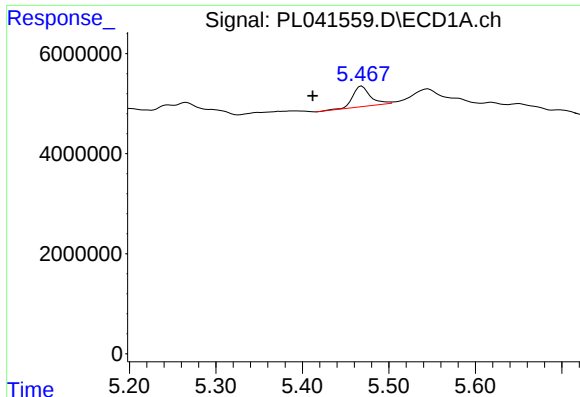

#10 gamma-Chlordane


R.T.: 5.469 min
Delta R.T.: 0.057 min
Response: 5769761
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

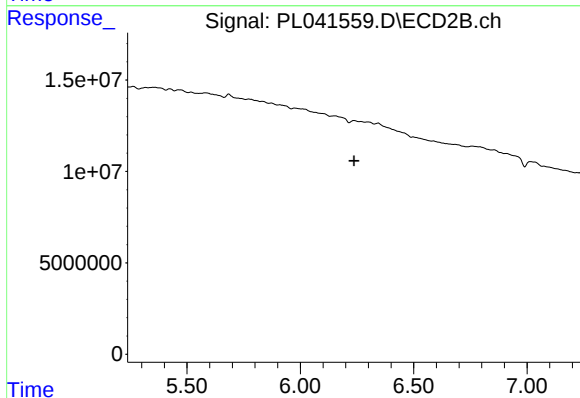


#10 gamma-Chlordane

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: -1545846
Conc: N.D.

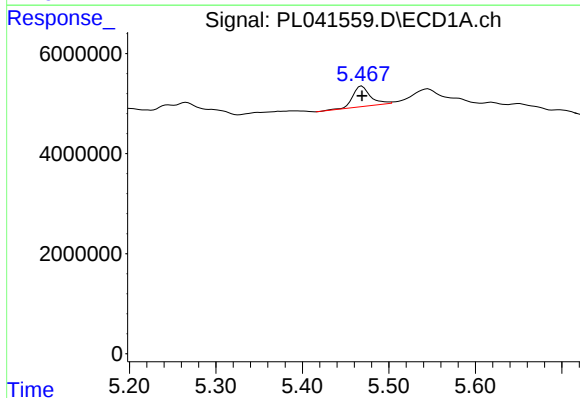


#11 alpha-Chlordane

R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 5769761
Conc: 0.71 ng/ml

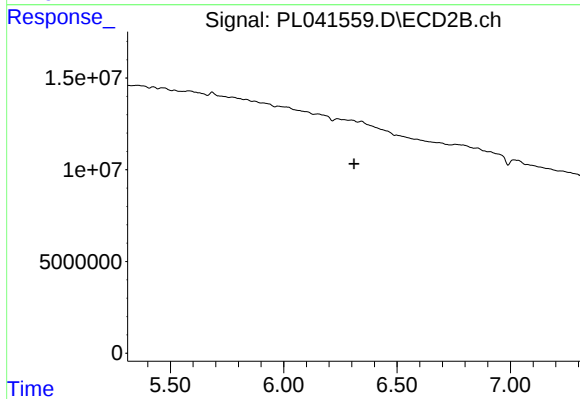

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

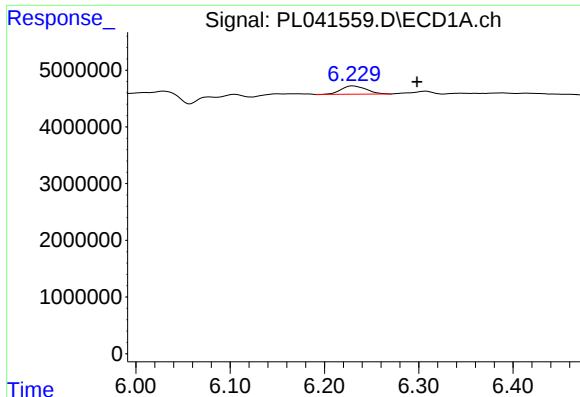

#15 Endosulfan II


R.T.: 6.230 min
Delta R.T.: -0.068 min
Response: 2669919
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

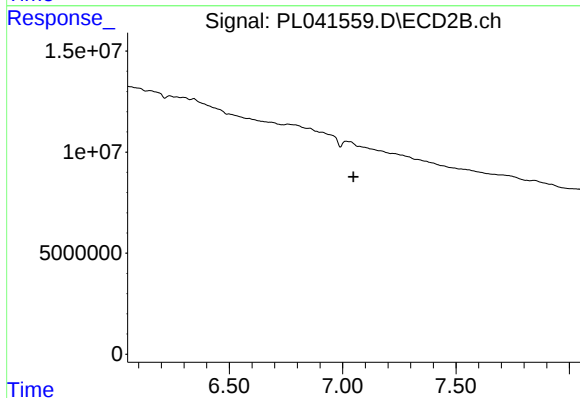


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

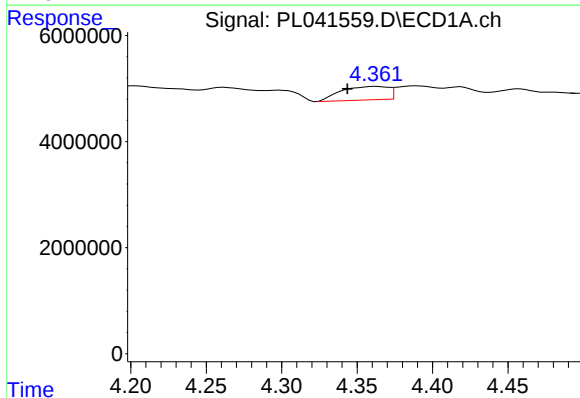


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.019 min
Response: 5540118
Conc: 19.54 ng/ml

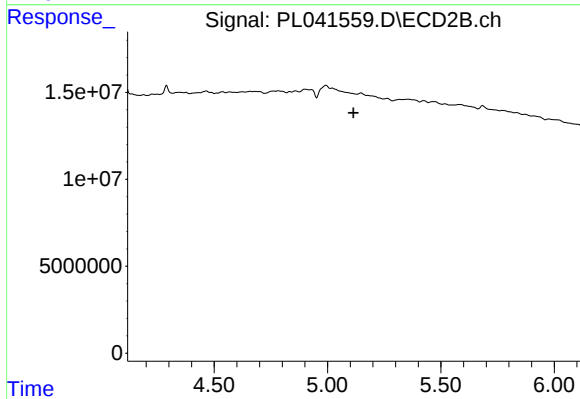

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

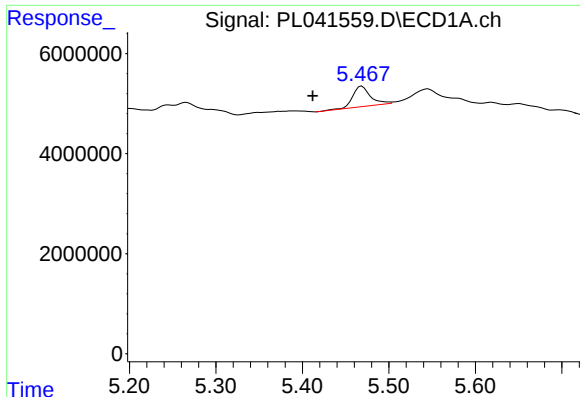

#25 Chlordane-3


R.T.: 5.469 min
Delta R.T.: 0.057 min
Response: 5769761
Conc: 6.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

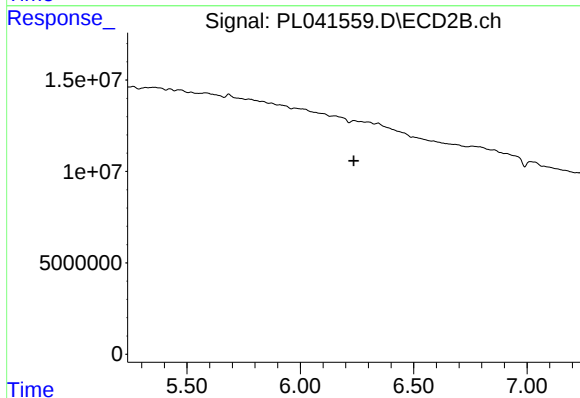


#25 Chlordane-3

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: -1545846
Conc: N.D.

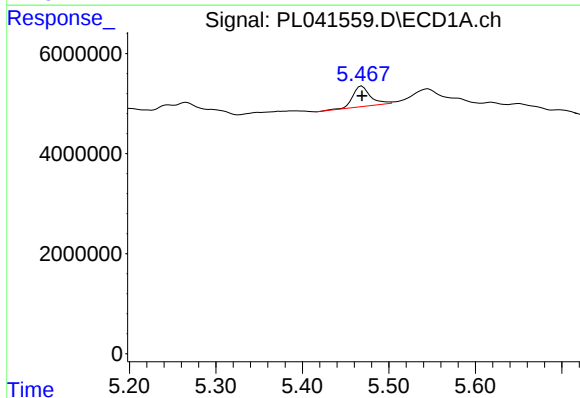


#26 Chlordane-4

R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 5769761
Conc: 7.37 ng/ml

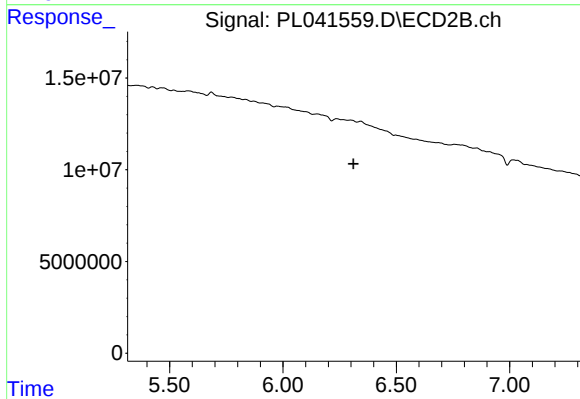

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

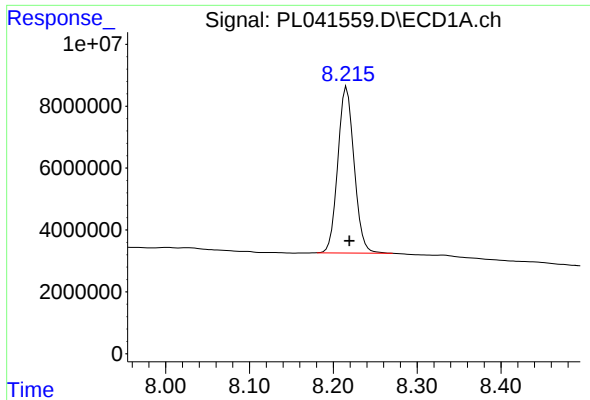

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.003 min
Response: 72513267
Conc: 10.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

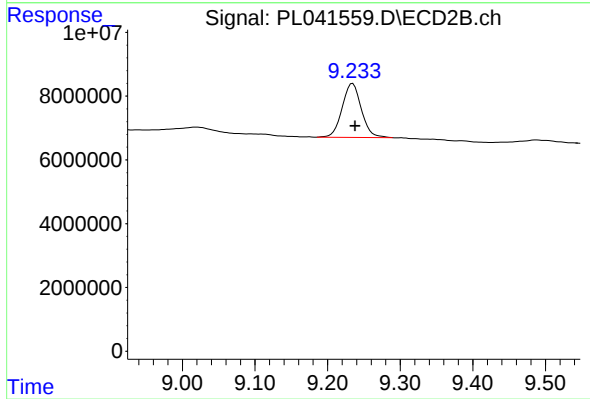

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.003 min
Response: 31106810
Conc: 12.14 ng/ml