

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
 Data File : PL041560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 17:54
 Operator : AJ\SJ
 Sample : J5737-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:25:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.103	116.9E6	61798625	18.354	20.063
28)	SA Decachlor...	8.216	9.234	97390170	42789008	14.703	16.700
Target Compounds							
4)	MA Heptachlor	0.000	5.314	0	211492	N.D.	0.052 #
6)	B beta-BHC	0.000	4.908f	0	1517204	N.D.	0.883 #
9)	A Endosulfan I	5.468f	0.000	2023856	0	0.272	N.D. #
10)	B gamma-Chl...	5.434	6.239	3812940	2497464	0.468	0.740 #
11)	B alpha-Chl...	5.468	0.000	2023856	0	0.250	N.D. #
15)	B Endosulfa...	6.230f	0.000	2583431	0	0.374	N.D. #
23)	Chlordane-1	4.367	0.000	1447774	0	5.106	N.D. #
25)	Chlordane-3	5.434	6.239	3812940	2497464	4.278	5.550 #
26)	Chlordane-4	5.468	0.000	2023856	0	2.585	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
Data File : PL041560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 17:54
Operator : AJ\SJ
Sample : J5737-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:25:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

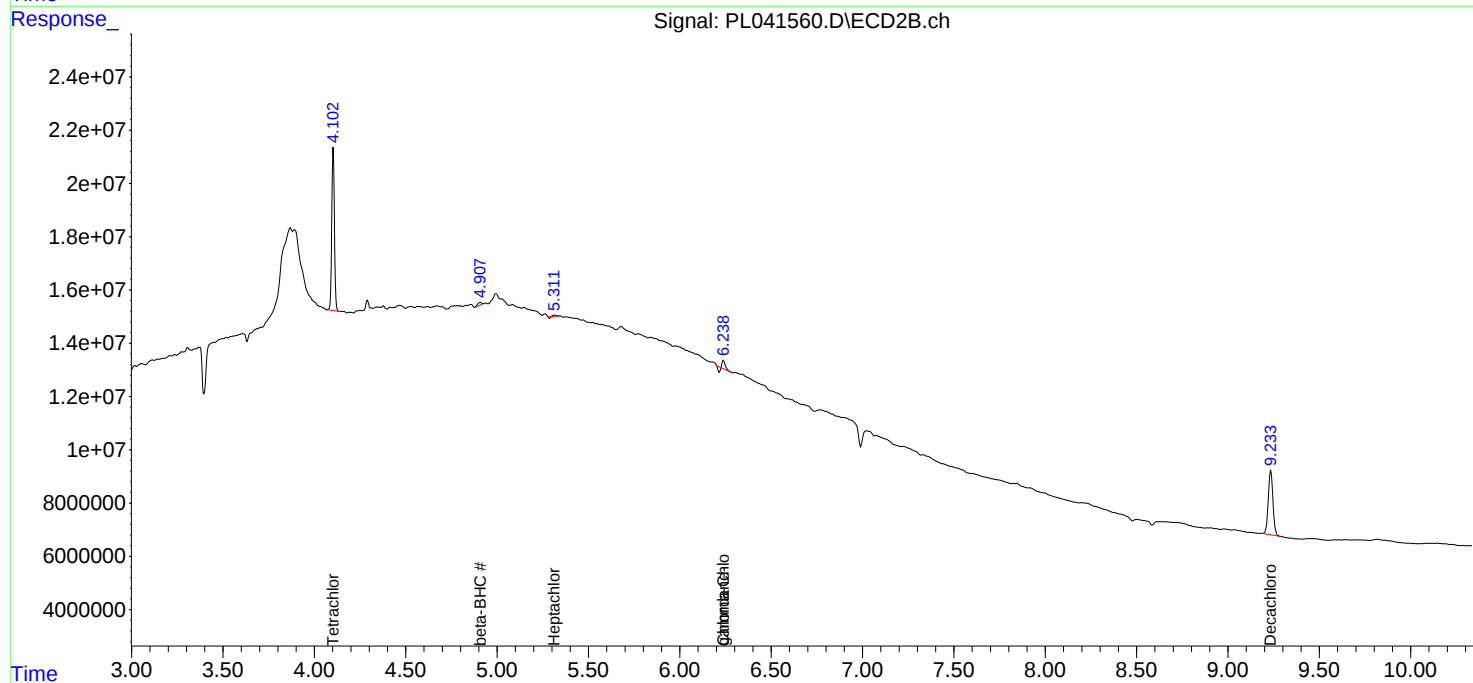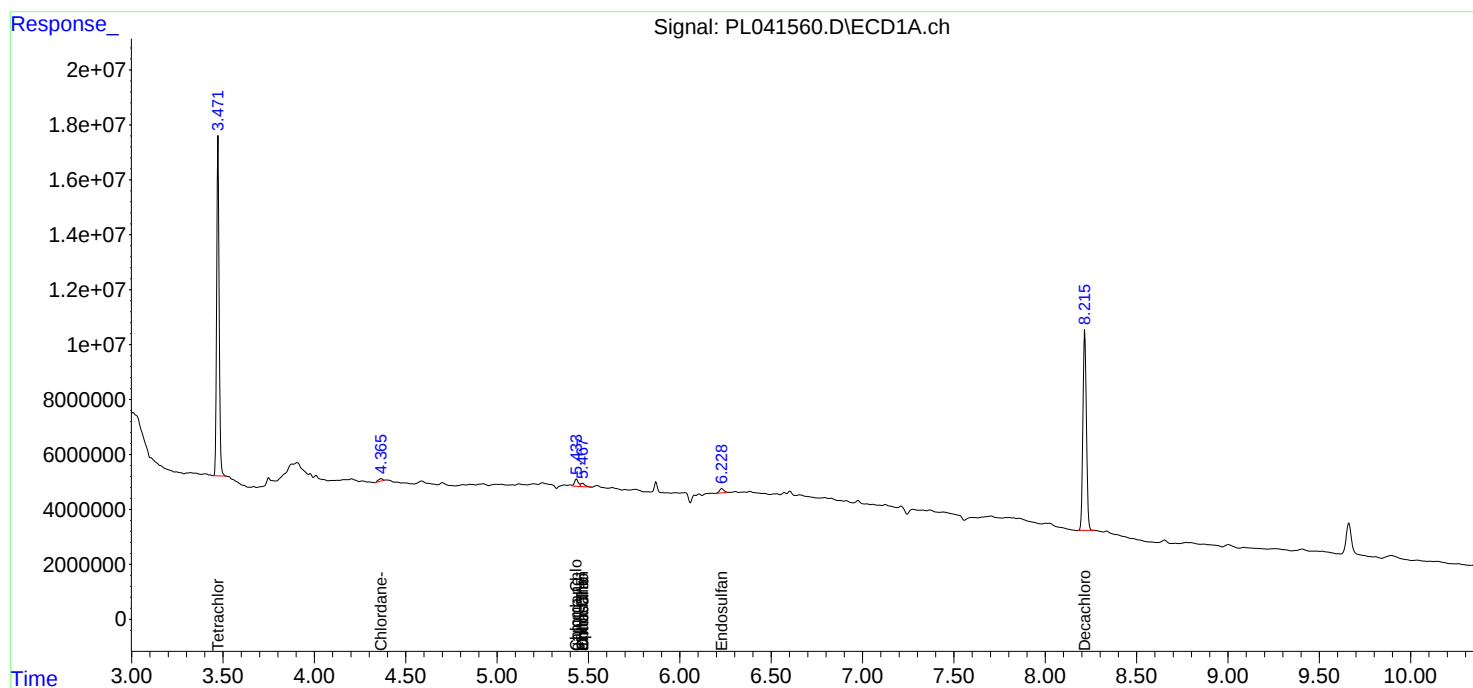


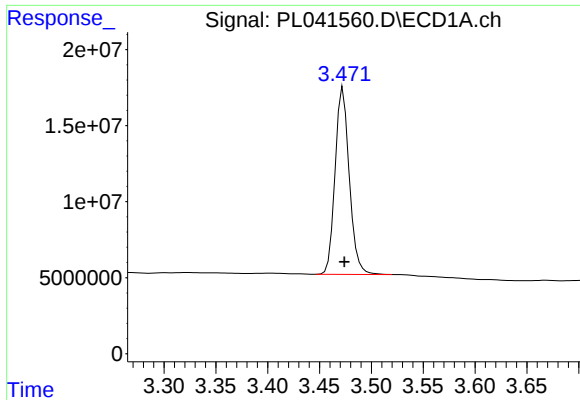

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 116920101
Conc: 18.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

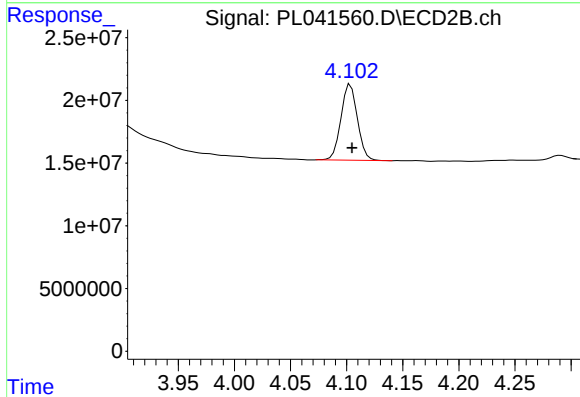


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.001 min
Response: 61798625
Conc: 20.06 ng/ml

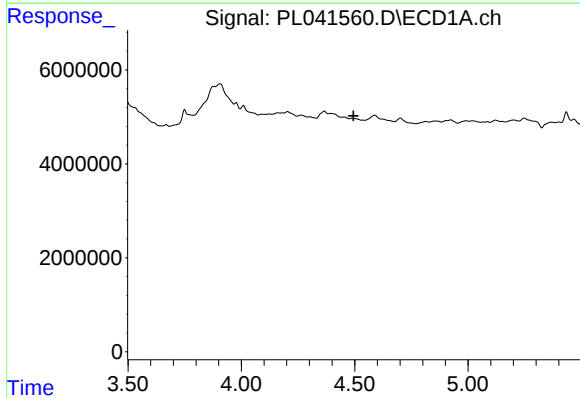


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.495 min
Response: 0
Conc: N.D.

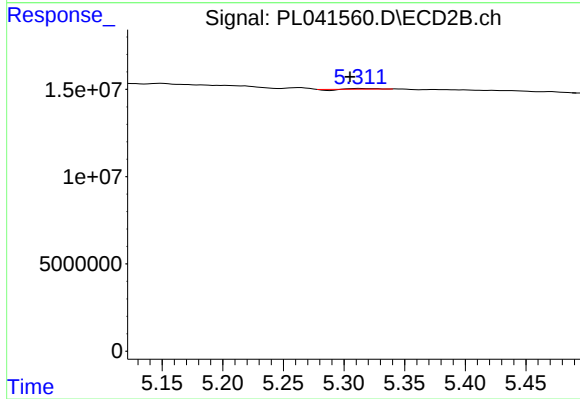

#4 Heptachlor


R.T.: 5.314 min
Delta R.T.: 0.008 min
Response: 211492
Conc: 0.05 ng/ml

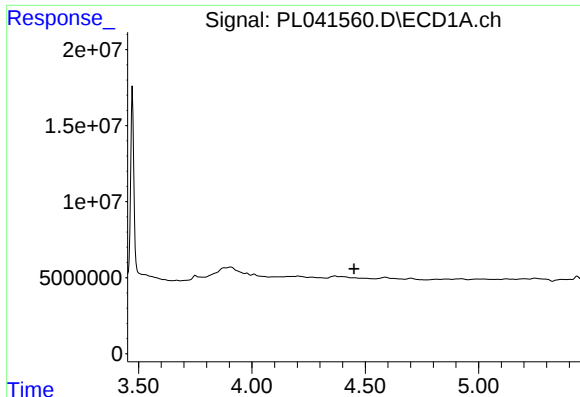

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

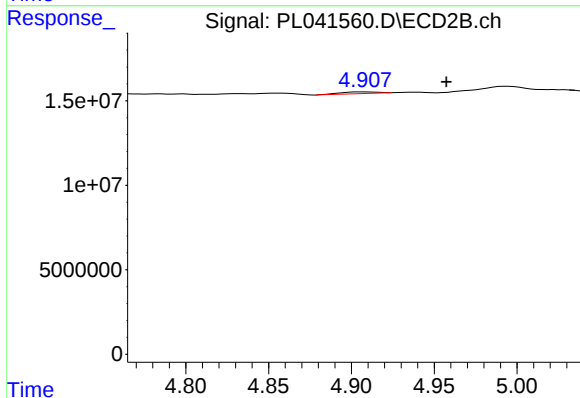


#6 beta-BHC

R.T.: 4.908 min
Delta R.T.: -0.050 min
Response: 1517204
Conc: 0.88 ng/ml

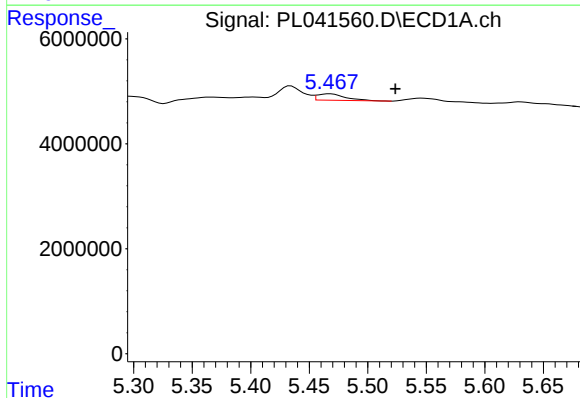


#9 Endosulfan I

R.T.: 5.468 min
Delta R.T.: -0.055 min
Response: 2023856
Conc: 0.27 ng/ml

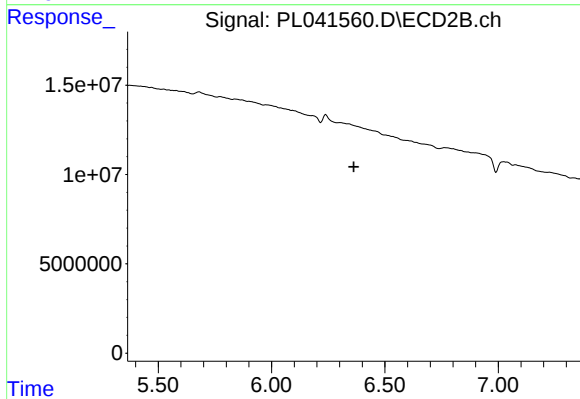

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

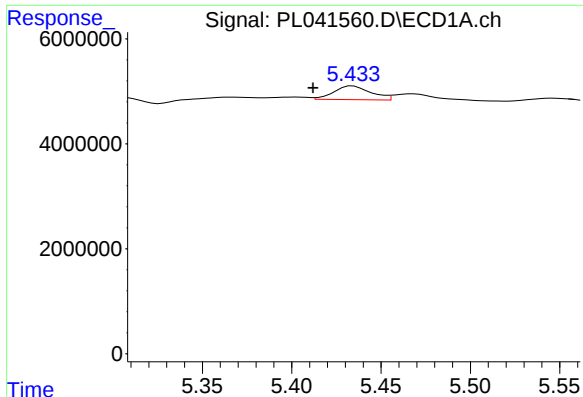

#10 gamma-Chlordane


R.T.: 5.434 min
Delta R.T.: 0.022 min
Response: 3812940
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

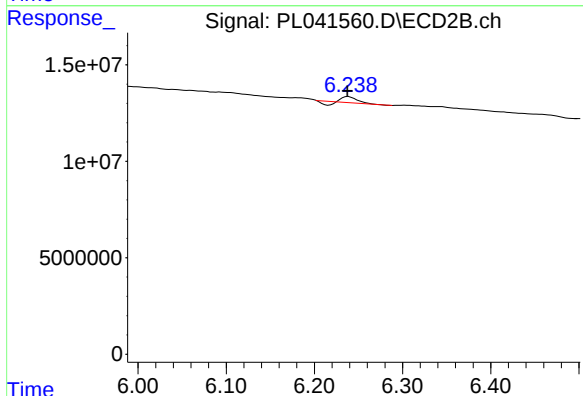


#10 gamma-Chlordane

R.T.: 6.239 min
Delta R.T.: 0.001 min
Response: 2497464
Conc: 0.74 ng/ml

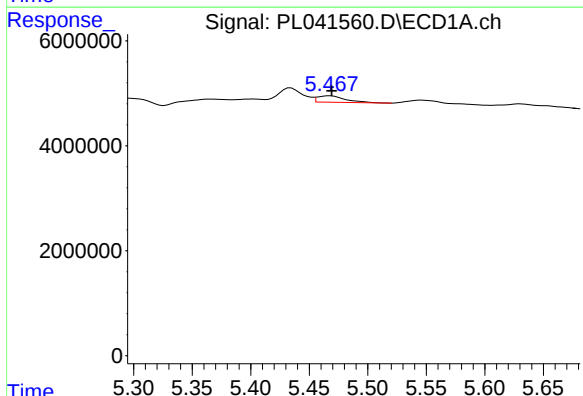


#11 alpha-Chlordane

R.T.: 5.468 min
Delta R.T.: 0.000 min
Response: 2023856
Conc: 0.25 ng/ml

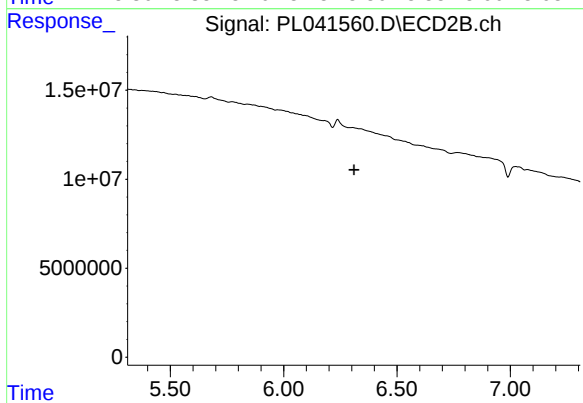

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

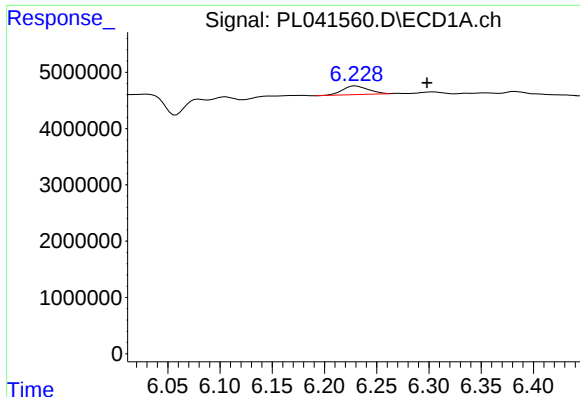

#15 Endosulfan II


R.T.: 6.230 min
Delta R.T.: -0.069 min
Response: 2583431
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

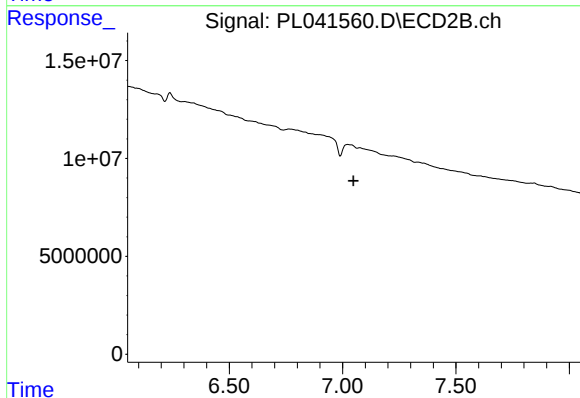


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

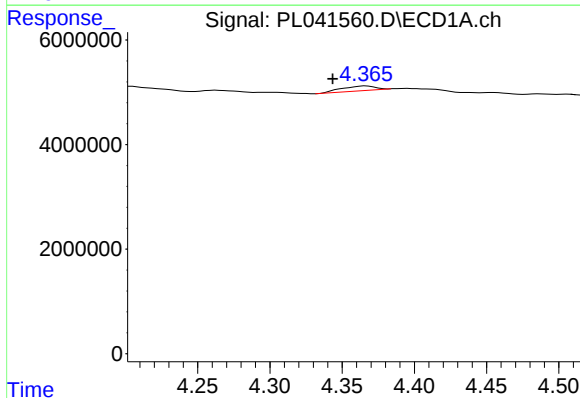


#23 Chlordane-1

R.T.: 4.367 min
Delta R.T.: 0.023 min
Response: 1447774
Conc: 5.11 ng/ml

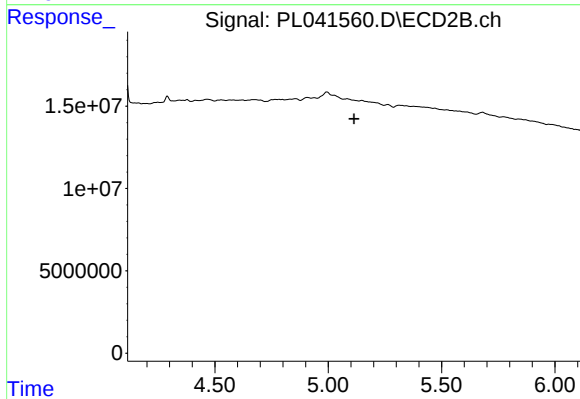

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

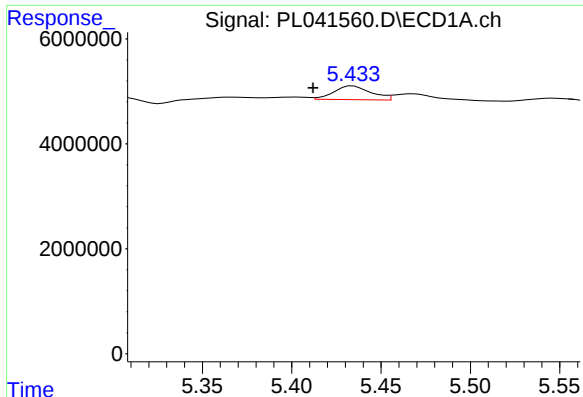

#25 Chlordane-3


R.T.: 5.434 min
Delta R.T.: 0.022 min
Response: 3812940
Conc: 4.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

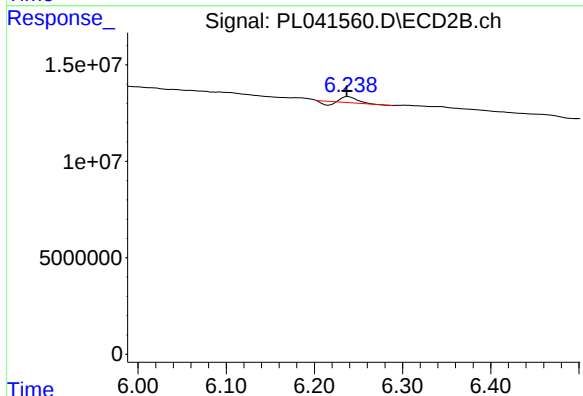


#25 Chlordane-3

R.T.: 6.239 min
Delta R.T.: 0.002 min
Response: 2497464
Conc: 5.55 ng/ml

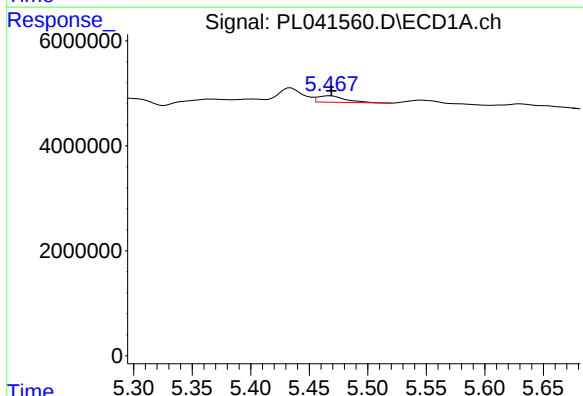


#26 Chlordane-4

R.T.: 5.468 min
Delta R.T.: 0.000 min
Response: 2023856
Conc: 2.58 ng/ml

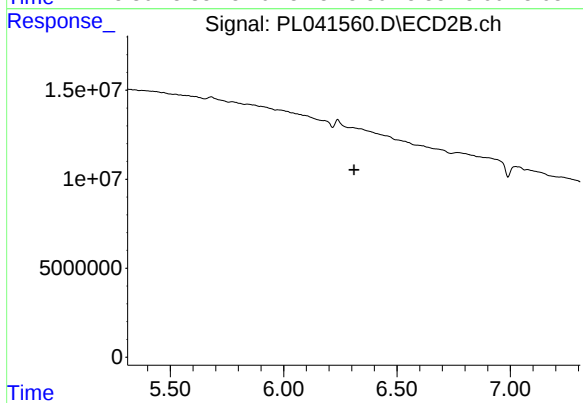

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.311 min
Response: 0
Conc: N.D.

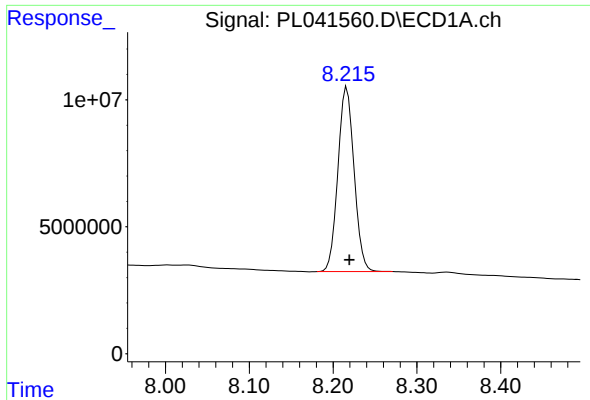

#28 Decachlorobiphenyl


R.T.: 8.216 min

Delta R.T.: -0.003 min

Response: 97390170

Conc: 14.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

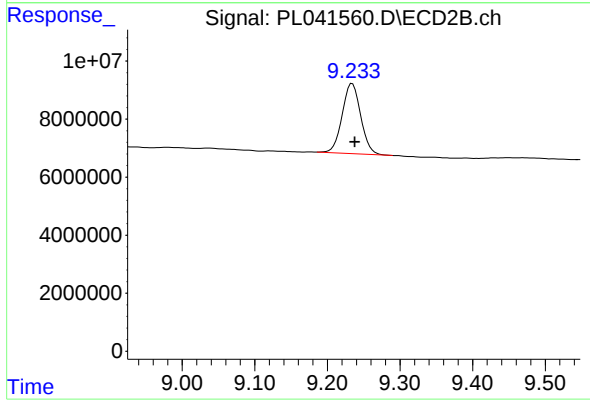

#28 Decachlorobiphenyl

R.T.: 9.234 min

Delta R.T.: -0.004 min

Response: 42789008

Conc: 16.70 ng/ml