

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
 Data File : PL041571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 20:29
 Operator : AJ\SJ
 Sample : J5202-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:28:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.103	131.3E6	72208508	20.617	23.443
28)	SA Decachlor...	8.216	9.234	123.2E6	54448357	18.596	21.251
Target Compounds							
2)	A alpha-BHC	3.878f	0.000	1105765	0	0.114	N.D. #
3)	MA gamma-BHC...	4.165f	0.000	134682	0	0.015	N.D. #
4)	MA Heptachlor	4.504	0.000	2335869	0	0.255	N.D. #
6)	B beta-BHC	4.410f	0.000	2883178	0	0.765	N.D. #
23)	Chlordane-1	4.350	0.000	1380898	0	4.870	N.D. #
24)	Chlordane-2	4.905	0.000	1884483	0	6.399	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
Data File : PL041571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 20:29
Operator : AJ\SJ
Sample : J5202-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:28:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

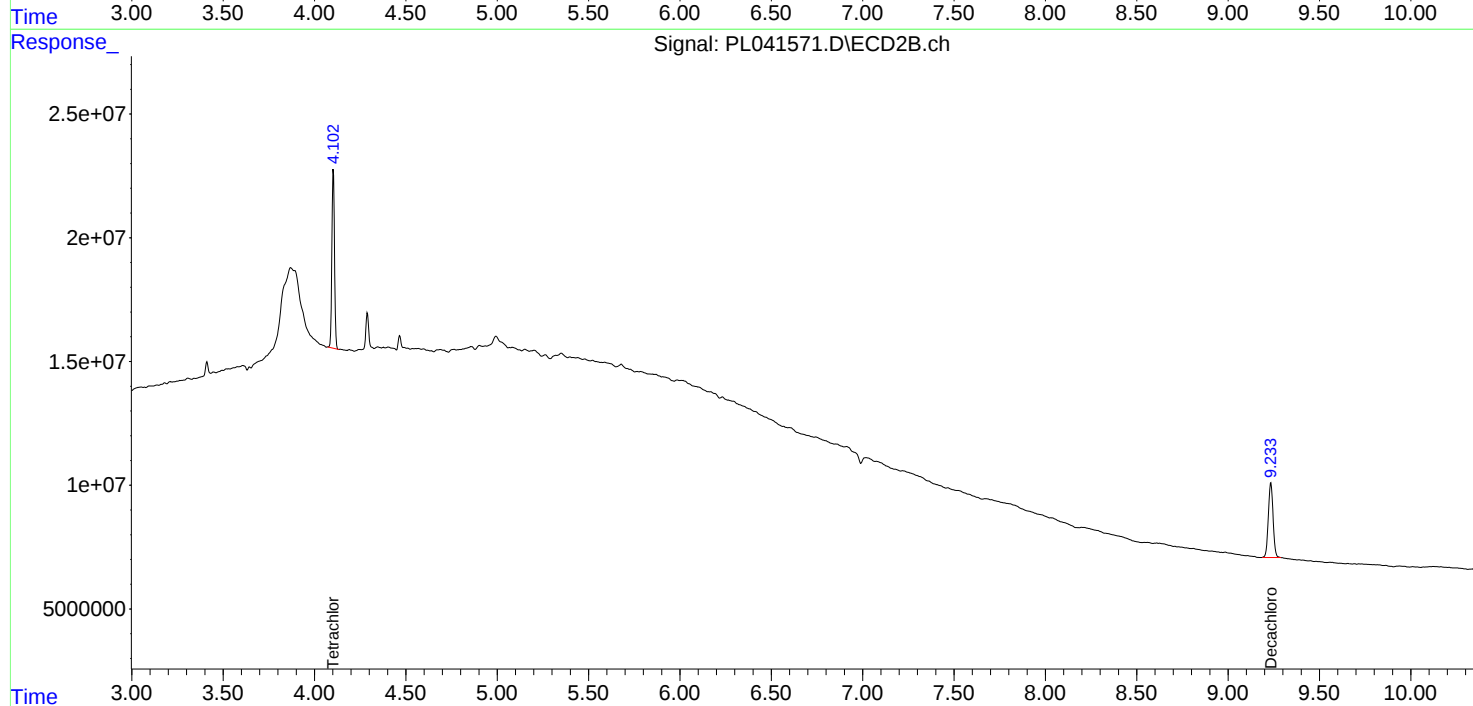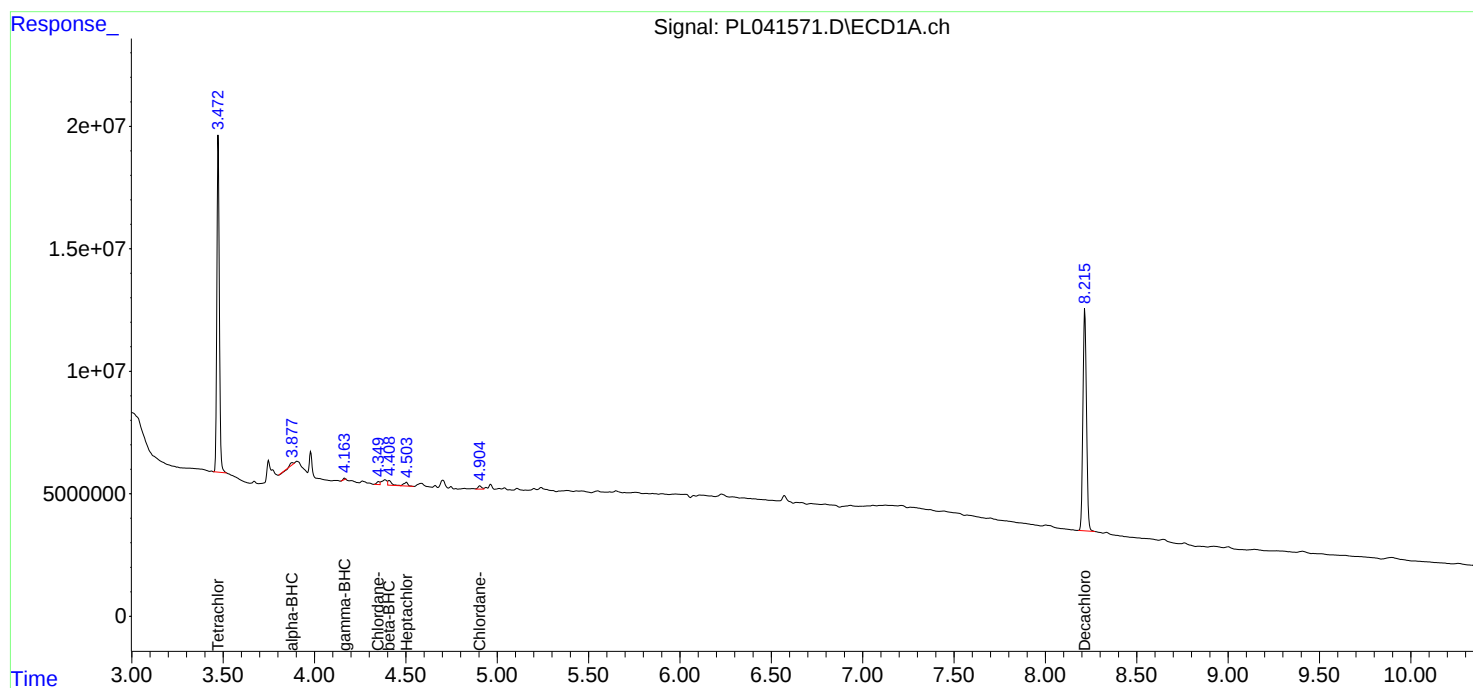


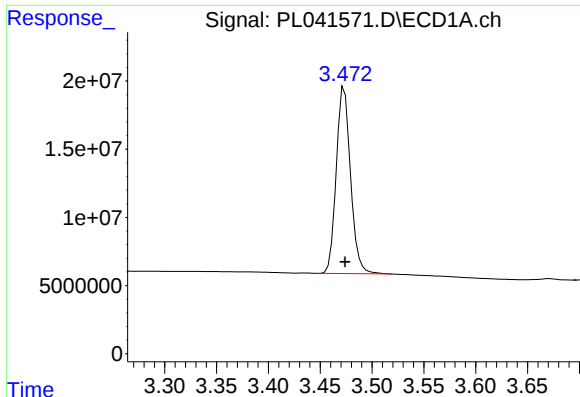

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 131334292
Conc: 20.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

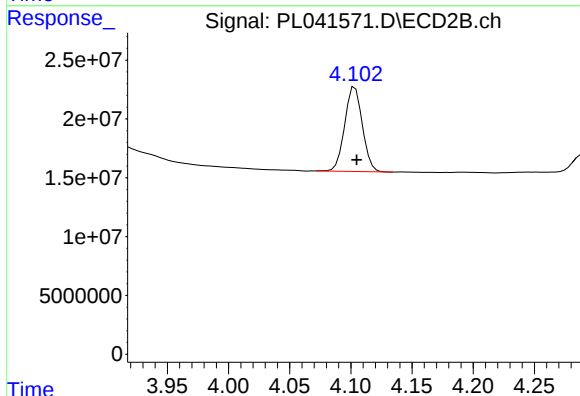


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.001 min
Response: 72208508
Conc: 23.44 ng/ml

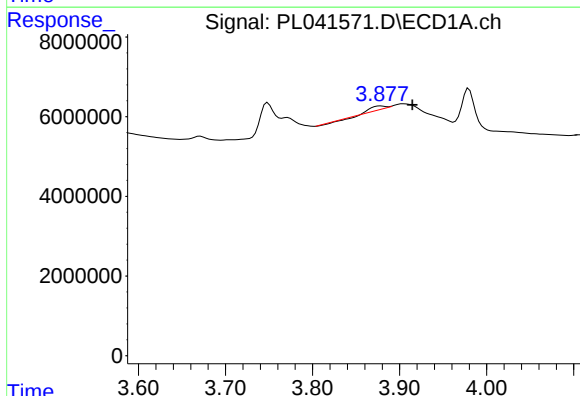


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: -0.037 min
Response: 1105765
Conc: 0.11 ng/ml

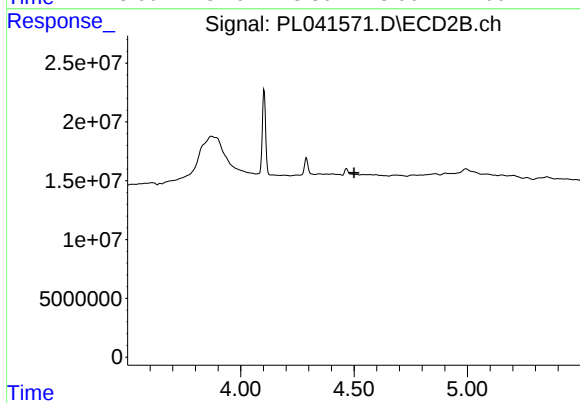

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

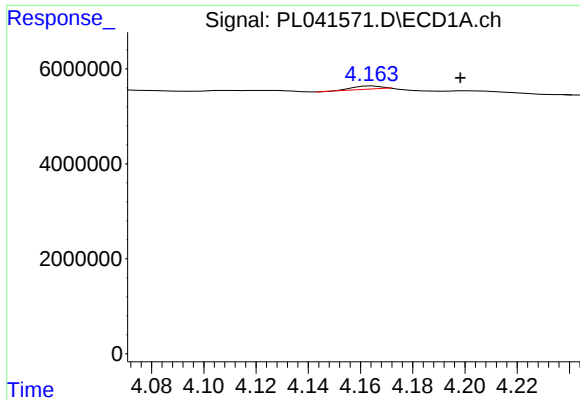

#3 gamma-BHC (Lindane)


R.T.: 4.165 min
Delta R.T.: -0.034 min
Response: 134682
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

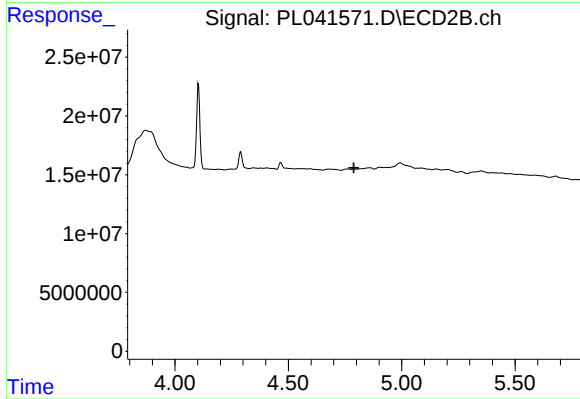


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.789 min
Response: 0
Conc: N.D.

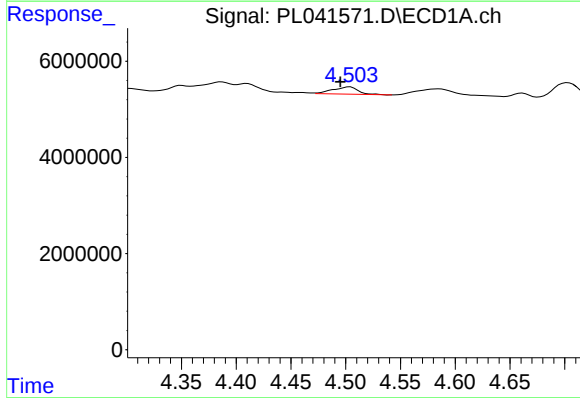


#4 Heptachlor

R.T.: 4.504 min
Delta R.T.: 0.009 min
Response: 2335869
Conc: 0.25 ng/ml

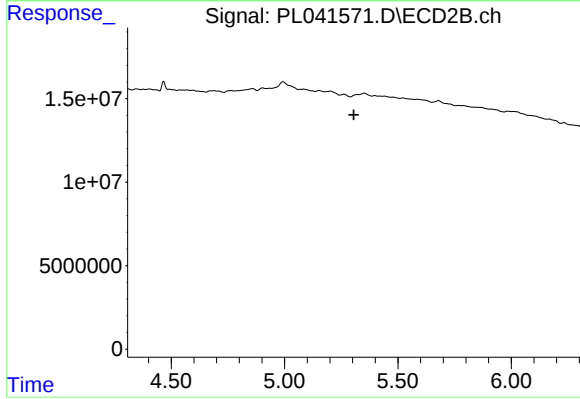

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.305 min
Response: 0
Conc: N.D.

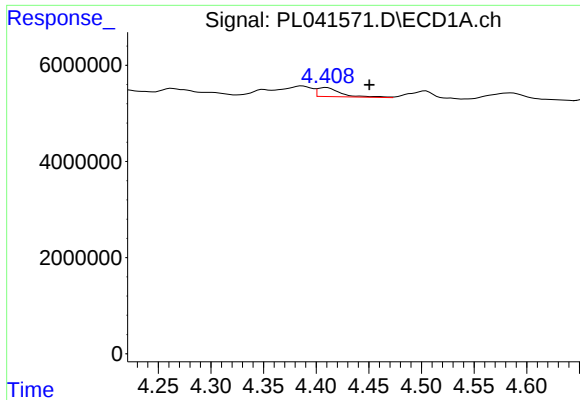

#6 beta-BHC


R.T.: 4.410 min
Delta R.T.: -0.041 min
Response: 2883178
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

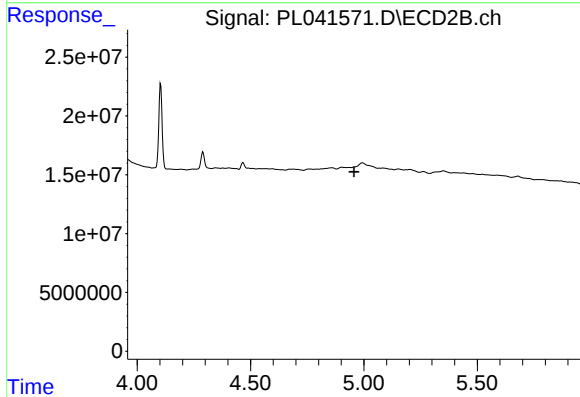


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

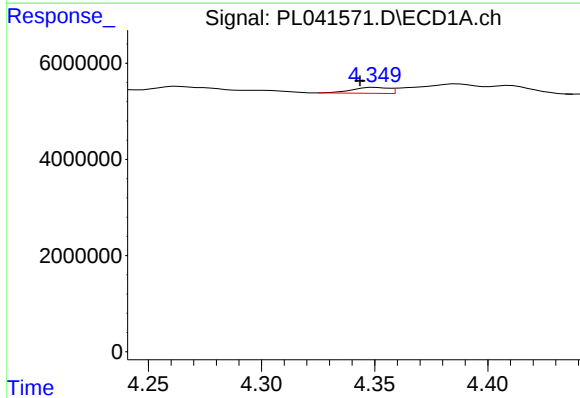


#23 Chlordane-1

R.T.: 4.350 min
Delta R.T.: 0.007 min
Response: 1380898
Conc: 4.87 ng/ml

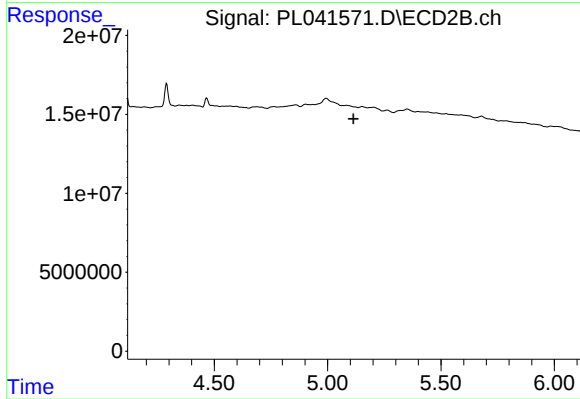

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

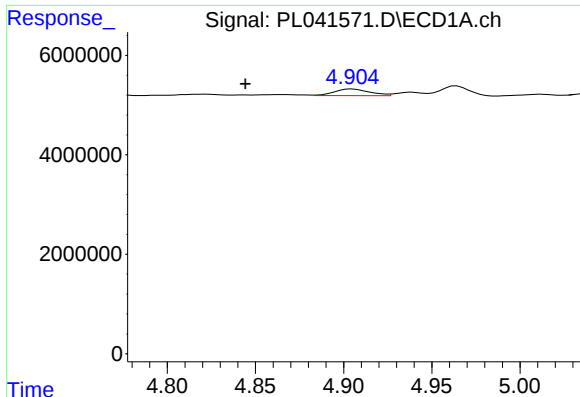

#24 Chlordane-2


R.T.: 4.905 min
Delta R.T.: 0.061 min
Response: 1884483
Conc: 6.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

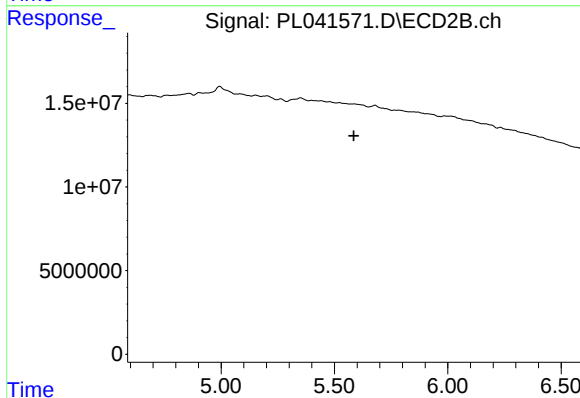


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.586 min
Response: 0
Conc: N.D.

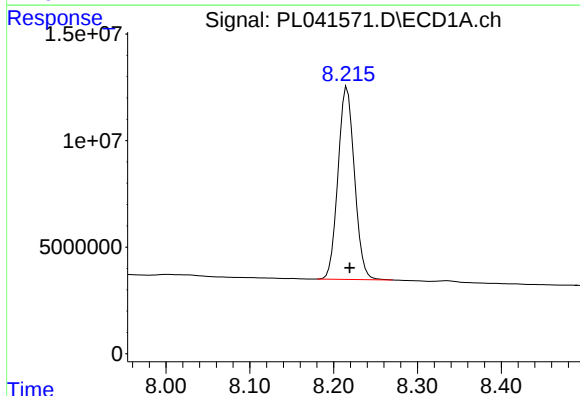

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.003 min
Response: 123179318
Conc: 18.60 ng/ml

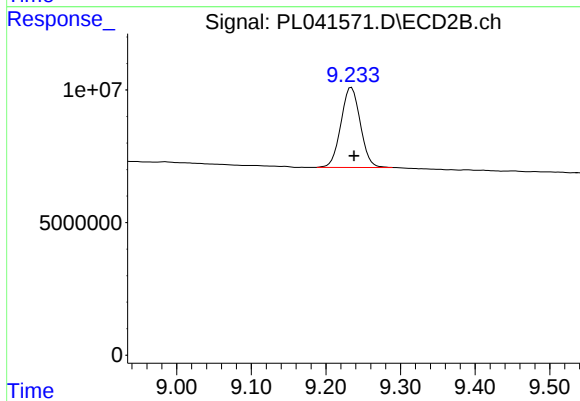

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.004 min
Response: 54448357
Conc: 21.25 ng/ml