

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
 Data File : PL041574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 21:12
 Operator : AJ\SJ
 Sample : J5202-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:29:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.103	105.1E6	57309398	16.505	18.606
28)	SA Decachlor...	8.216	9.235	123.3E6	53320162	18.617	20.811
Target Compounds							
2)	A alpha-BHC	3.869f	4.538f	3310764	1280184	0.341	0.279
4)	MA Heptachlor	4.493	5.307	1826093	922432	0.199	0.227
6)	B beta-BHC	4.493f	0.000	1826093	0	0.484	N.D. #
15)	B Endosulfa...	6.228f	0.000	2486911	0	0.360	N.D. #
23)	Chlordane-1	4.387	0.000	3701170	0	13.054	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103118\
Data File : PL041574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 21:12
Operator : AJ\SJ
Sample : J5202-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:29:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

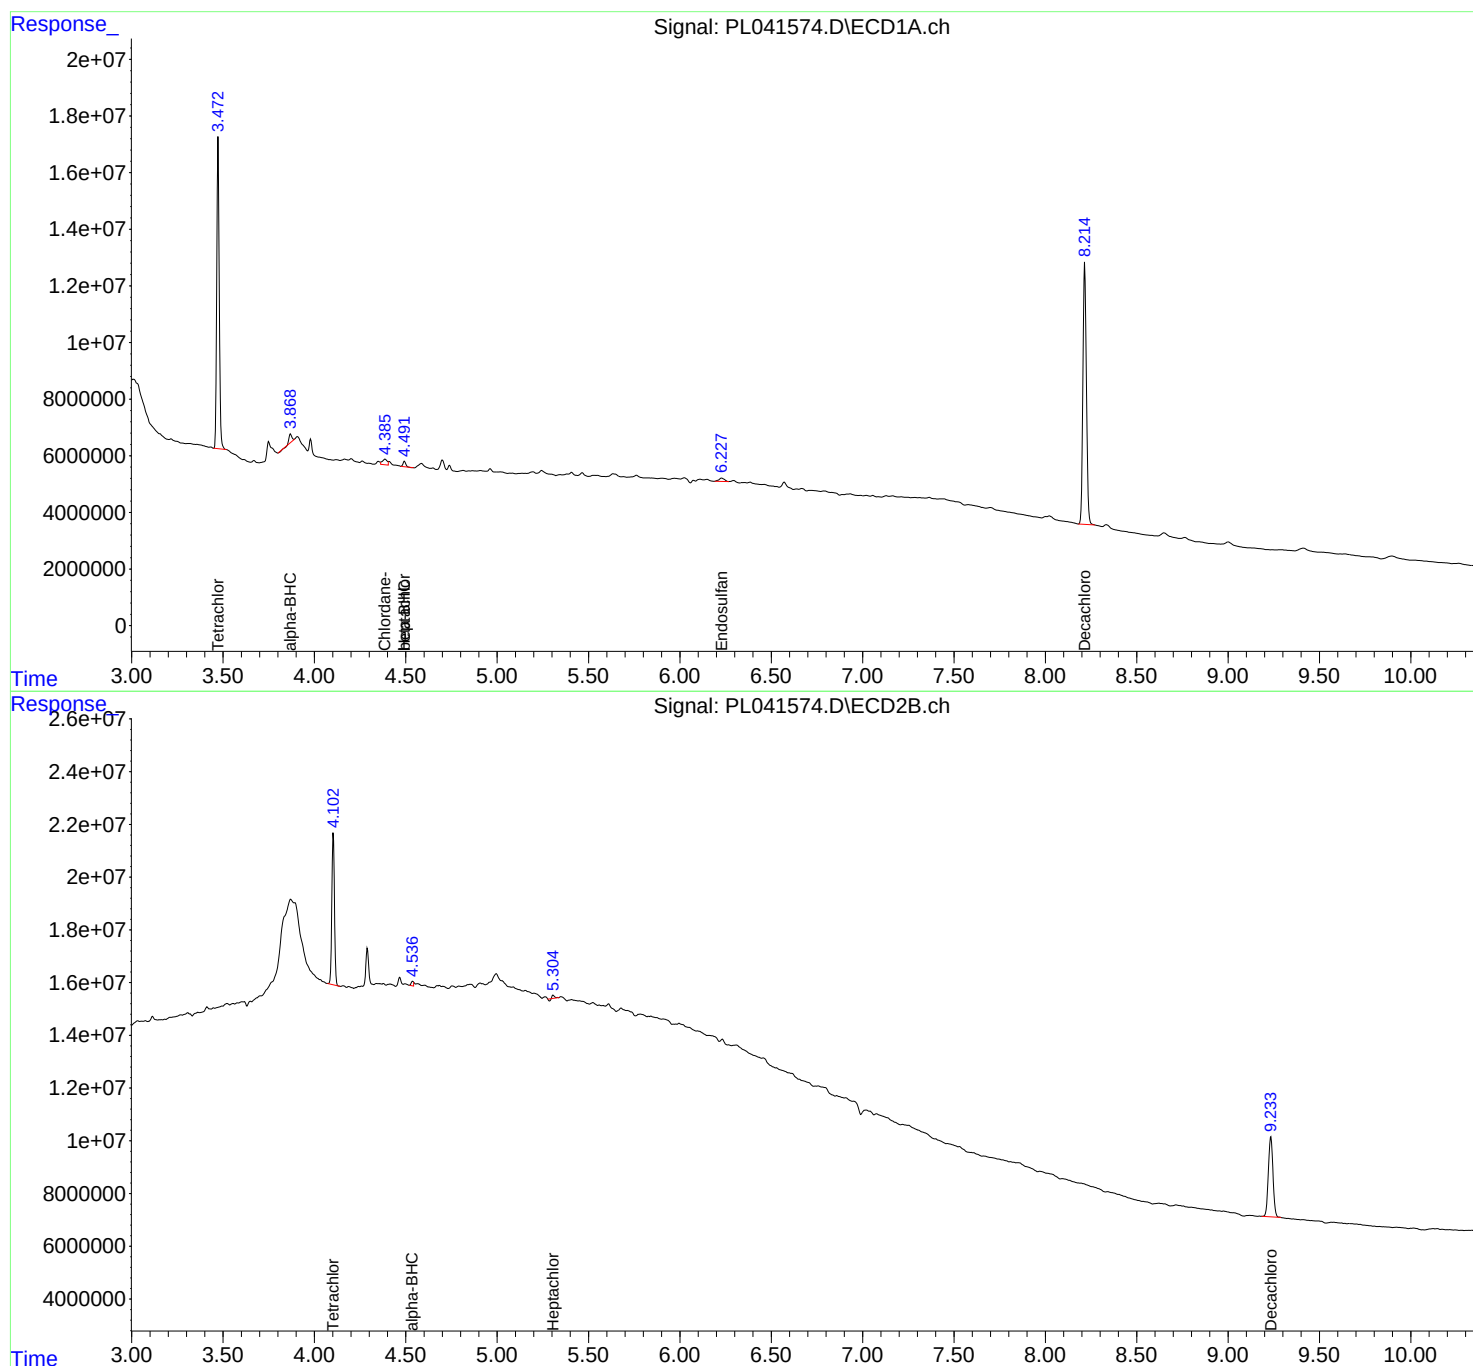


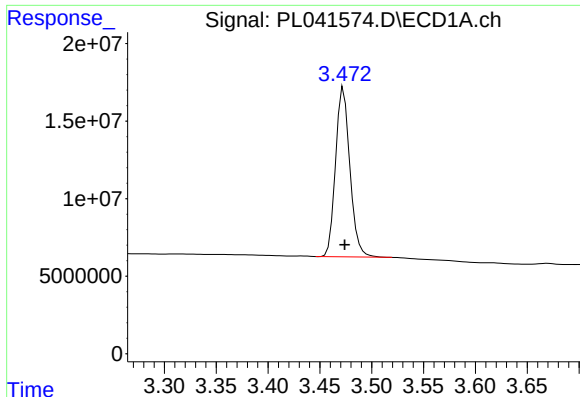

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 105141390
Conc: 16.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

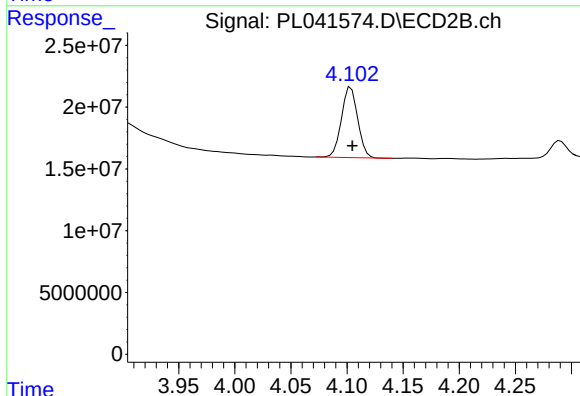


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.001 min
Response: 57309398
Conc: 18.61 ng/ml

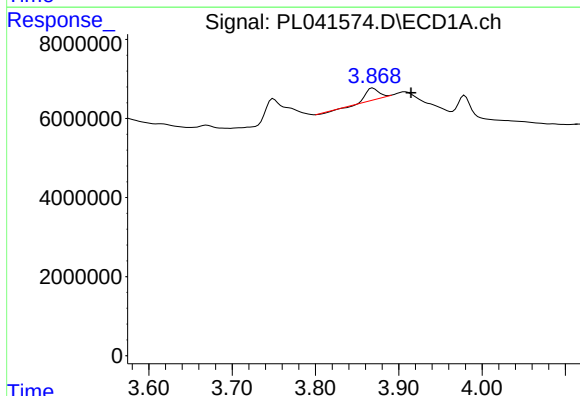


#2 alpha-BHC

R.T.: 3.869 min
Delta R.T.: -0.046 min
Response: 3310764
Conc: 0.34 ng/ml

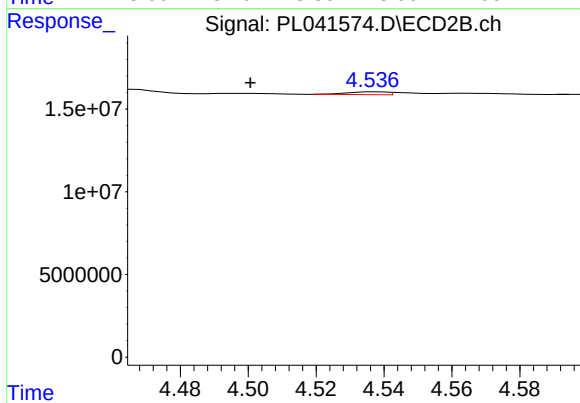

#2 alpha-BHC


R.T.: 4.538 min
Delta R.T.: 0.037 min
Response: 1280184
Conc: 0.28 ng/ml

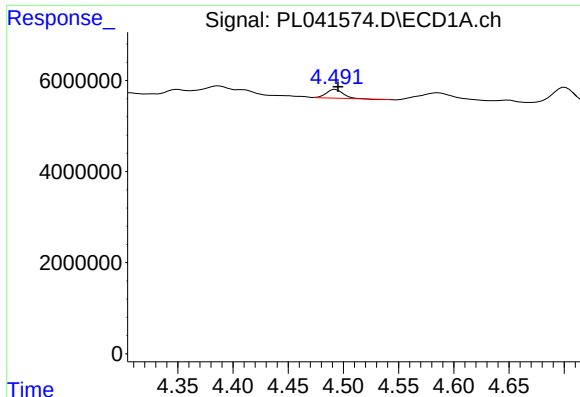

#4 Heptachlor


R.T.: 4.493 min
Delta R.T.: -0.002 min
Response: 1826093
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

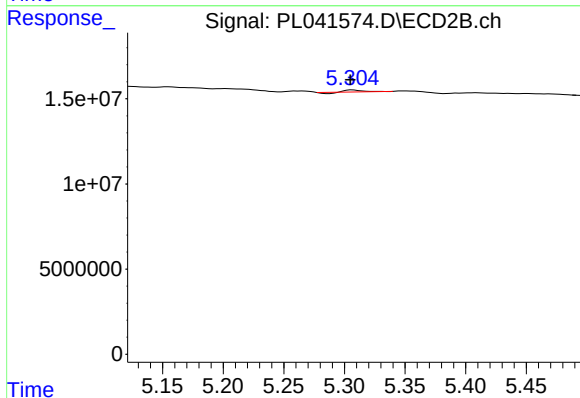


#4 Heptachlor

R.T.: 5.307 min
Delta R.T.: 0.001 min
Response: 922432
Conc: 0.23 ng/ml

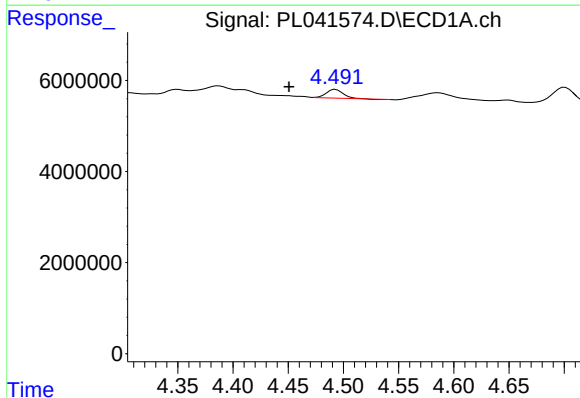


#6 beta-BHC

R.T.: 4.493 min
Delta R.T.: 0.042 min
Response: 1826093
Conc: 0.48 ng/ml

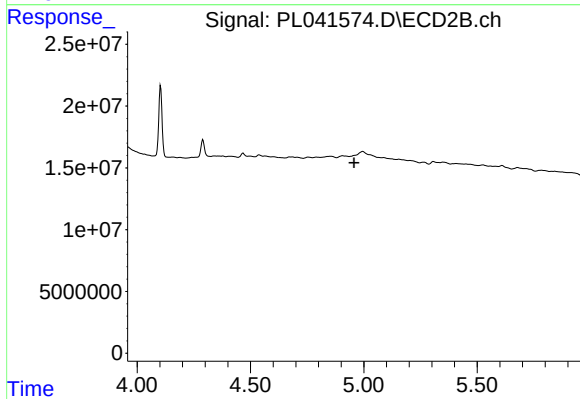

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

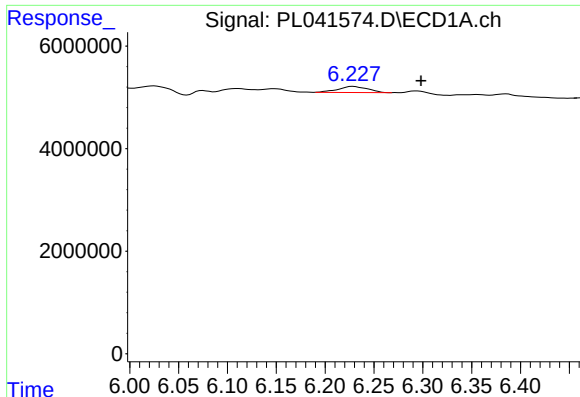

#15 Endosulfan II


R.T.: 6.228 min
Delta R.T.: -0.070 min
Response: 2486911
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

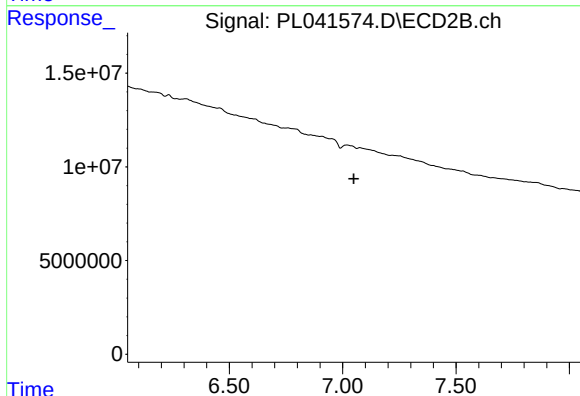


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

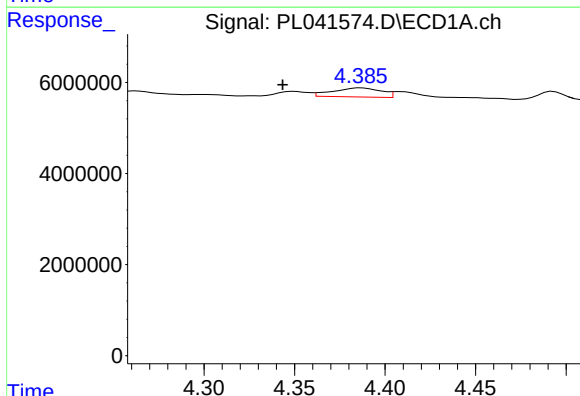


#23 Chlordane-1

R.T.: 4.387 min
Delta R.T.: 0.043 min
Response: 3701170
Conc: 13.05 ng/ml

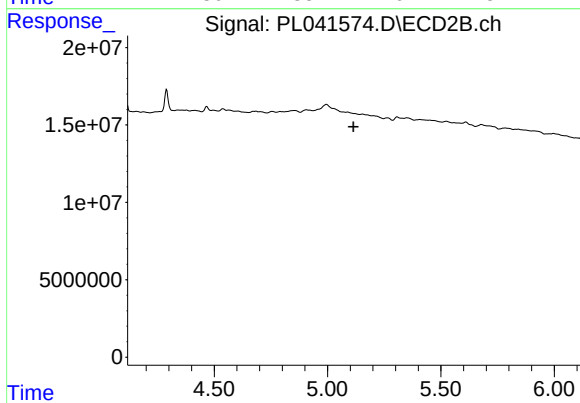

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

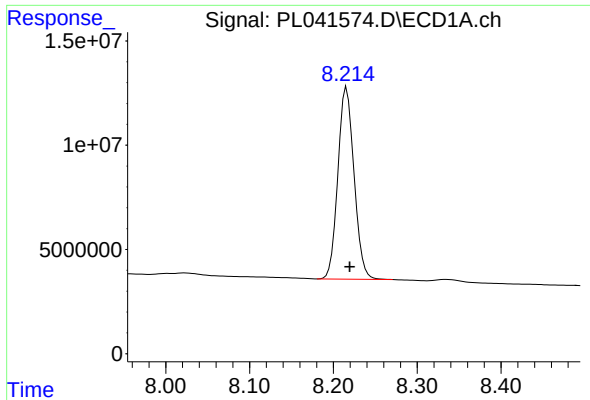

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.004 min
Response: 123321407
Conc: 18.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

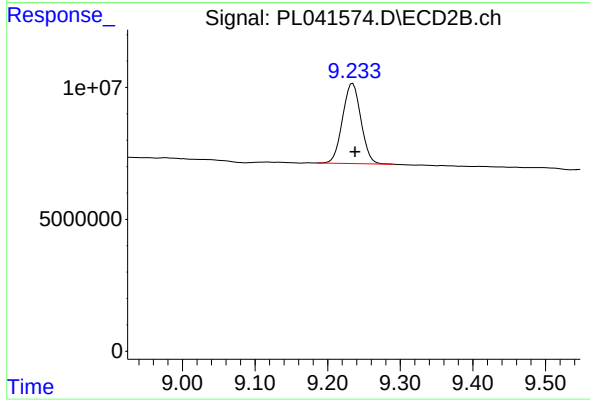

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.003 min
Response: 53320162
Conc: 20.81 ng/ml