

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
 Data File : PL053941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 08:59
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:14:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.918	0	29699004	N.D. 10.183 #
9) A	Endosulfan I	5.635	0.000	78863569	0	6.416 N.D. #
11) B	alpha-Chl...	5.542f	0.000	72171893	0	5.425 N.D. #
12) B	4,4'-DDE	5.759f	0.000	12894508	0	1.085 N.D. #
14) MA	Endrin	6.131	6.750	37395675	9096357	3.226 3.748
17) MA	4,4'-DDT	6.467f	0.000	41436643	0	4.183 N.D. #
18) B	Endrin al...	6.542f	0.000	20082354	0	2.190 N.D. #
23)	Chlordane-1	4.455f	0.000	6308880	0	17.788 N.D. #
24)	Chlordane-2	4.929	0.000	69467684	0	180.288 N.D. #
26)	Chlordane-4	5.542f	0.000	72171893	0	76.987 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
Data File : PL053941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 08:59
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:14:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

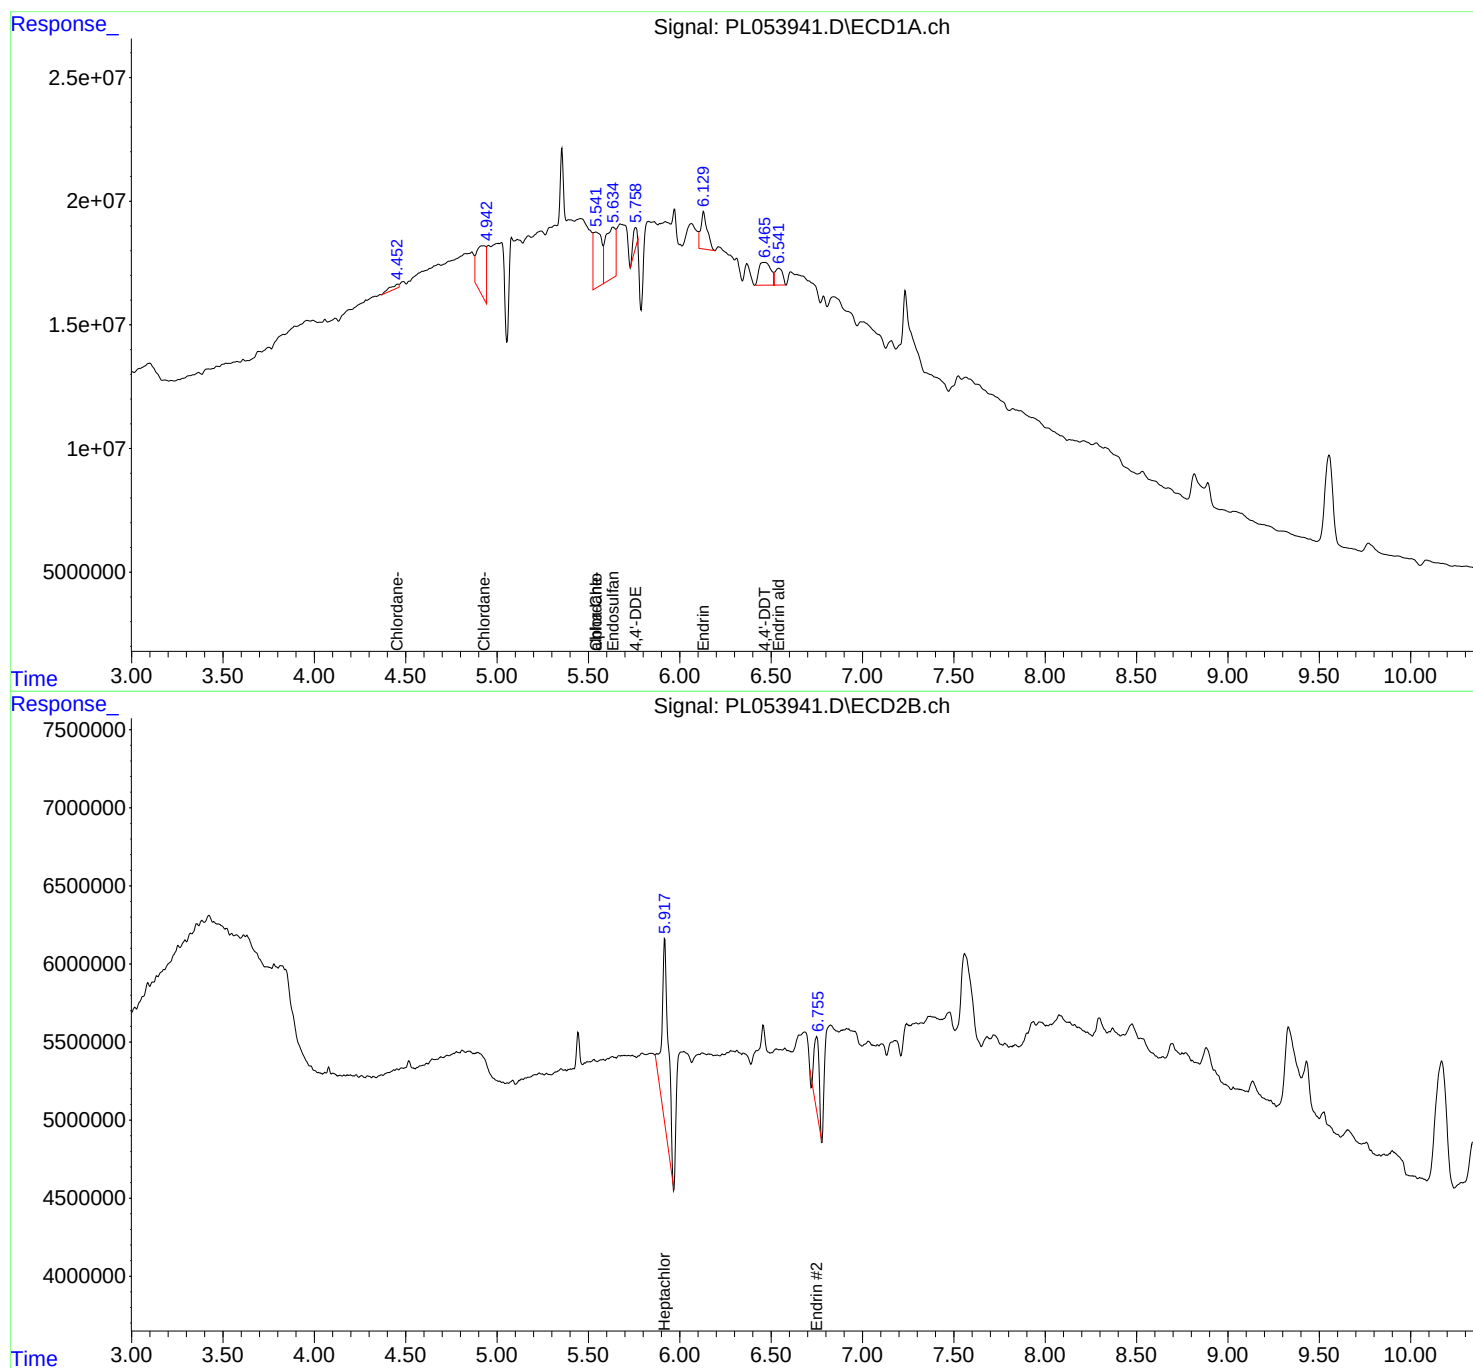


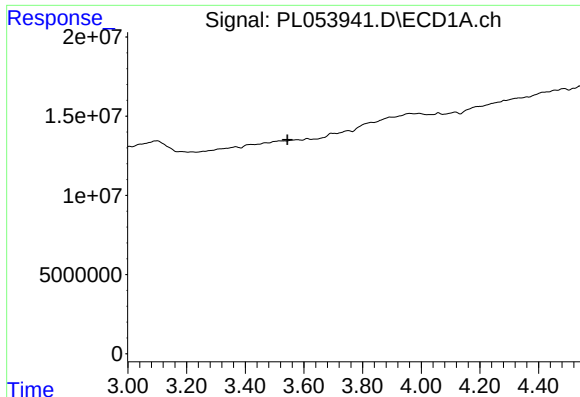

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

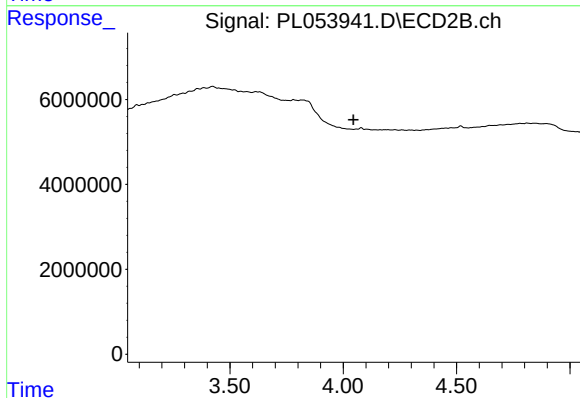


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.046 min
Response: 0
Conc: N.D.

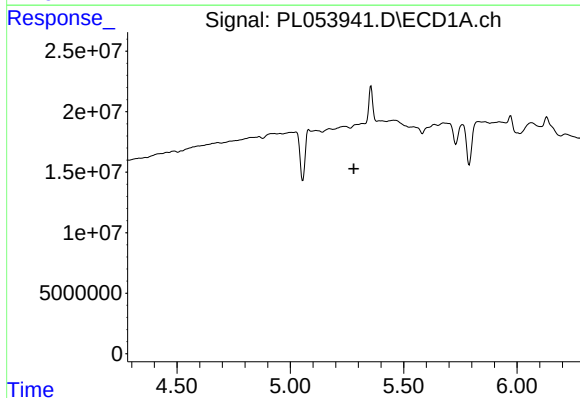


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.280 min
Response: 0
Conc: N.D.

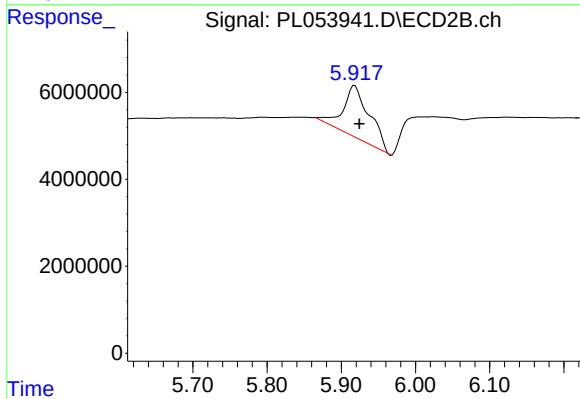

#8 Heptachlor epoxide


R.T.: 5.918 min
Delta R.T.: -0.006 min
Response: 29699004
Conc: 10.18 ng/ml

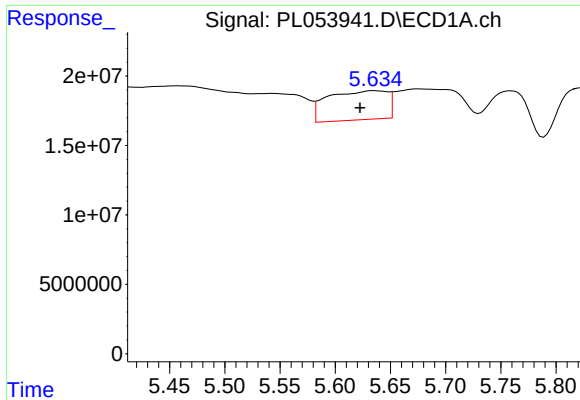

#9 Endosulfan I


R.T.: 5.635 min
Delta R.T.: 0.013 min
Response: 78863569
Conc: 6.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

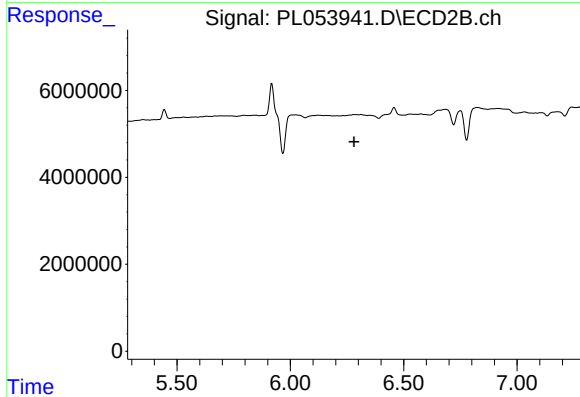


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

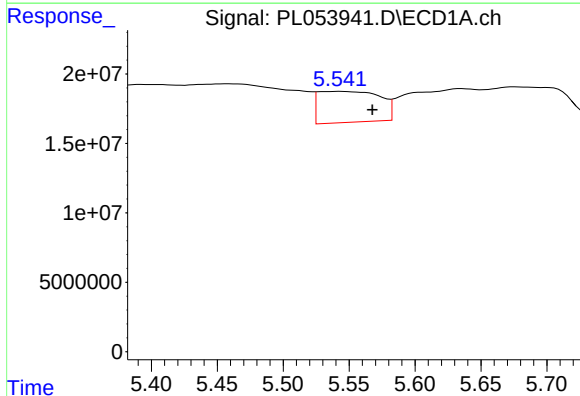


#11 alpha-Chlordane

R.T.: 5.542 min
Delta R.T.: -0.025 min
Response: 72171893
Conc: 5.43 ng/ml

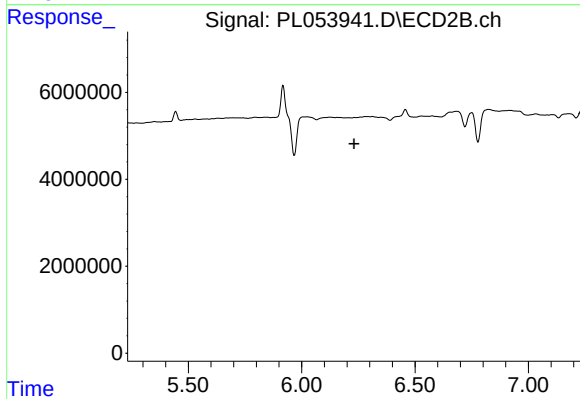

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

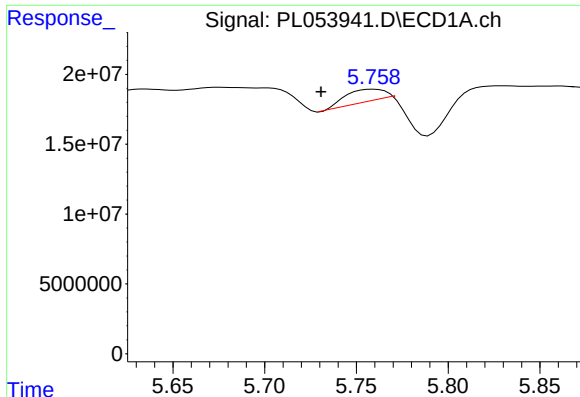

#12 4,4'-DDE


R.T.: 5.759 min
Delta R.T.: 0.029 min
Response: 12894508
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

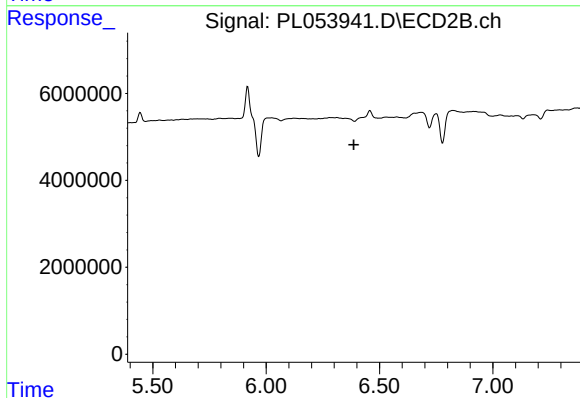


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

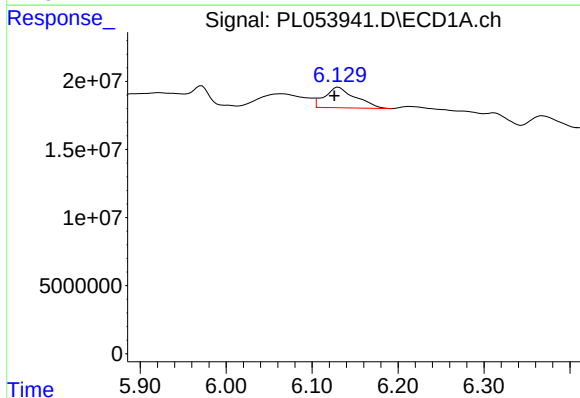


#14 Endrin

R.T.: 6.131 min
Delta R.T.: 0.005 min
Response: 37395675
Conc: 3.23 ng/ml

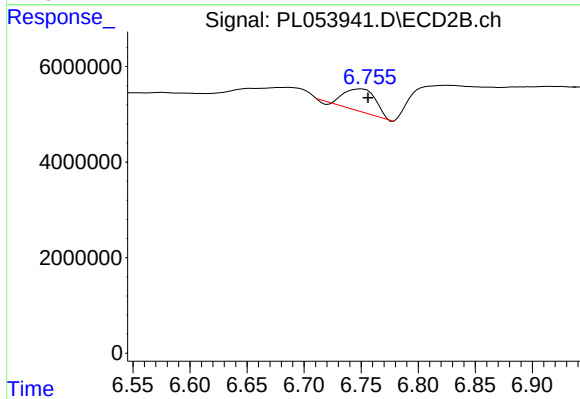

#14 Endrin


R.T.: 6.750 min
Delta R.T.: -0.006 min
Response: 9096357
Conc: 3.75 ng/ml

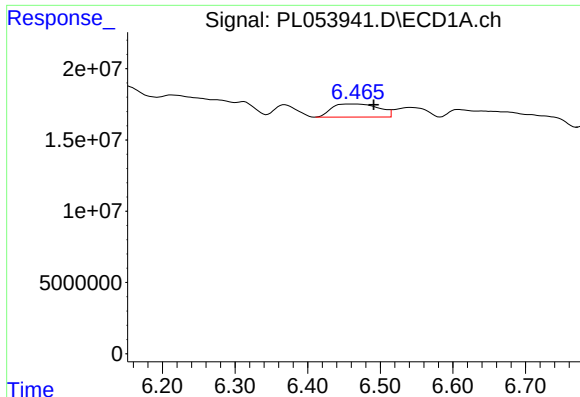

#17 4,4'-DDT


R.T.: 6.467 min
Delta R.T.: -0.024 min
Response: 41436643
Conc: 4.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

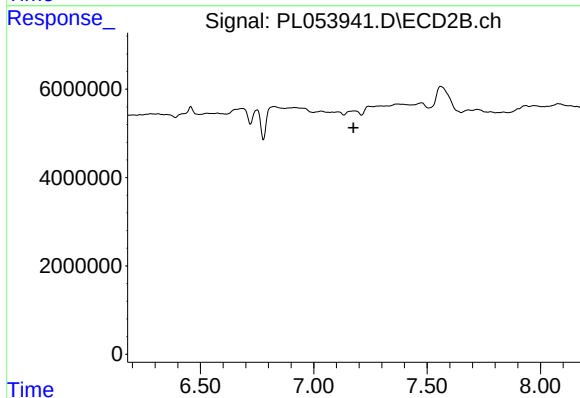


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

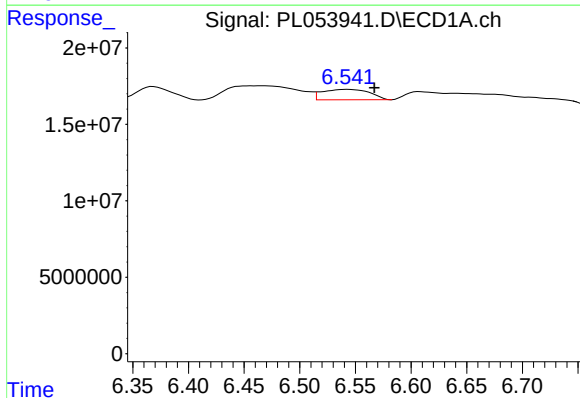


#18 Endrin aldehyde

R.T.: 6.542 min
Delta R.T.: -0.025 min
Response: 20082354
Conc: 2.19 ng/ml

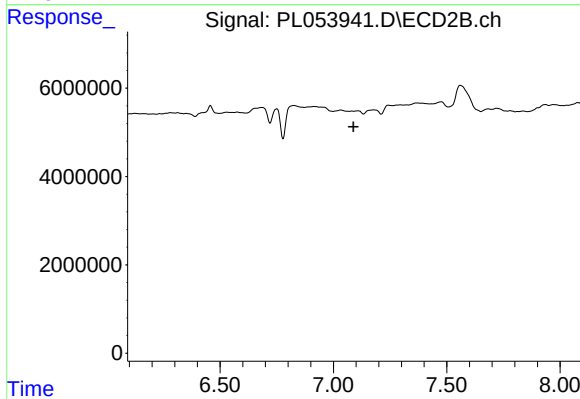

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

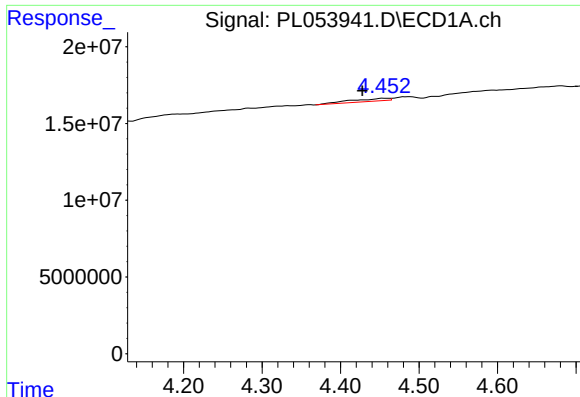

#23 Chlordane-1


R.T.: 4.455 min
Delta R.T.: 0.028 min
Response: 6308880
Conc: 17.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

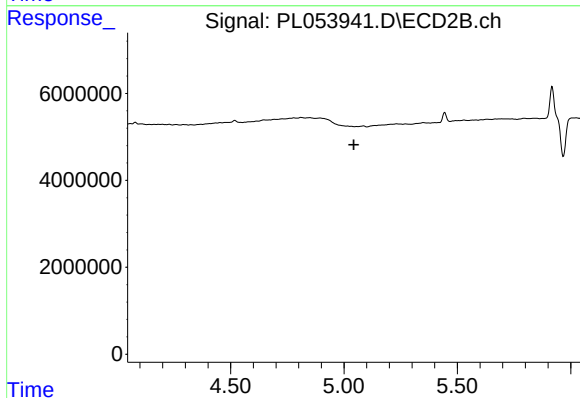


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

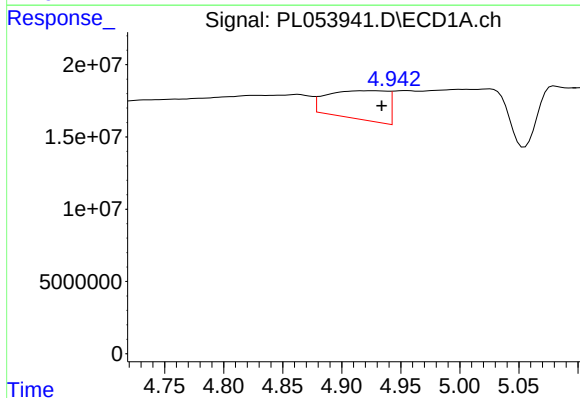


#24 Chlordane-2

R.T.: 4.929 min
Delta R.T.: -0.005 min
Response: 69467684
Conc: 180.29 ng/ml

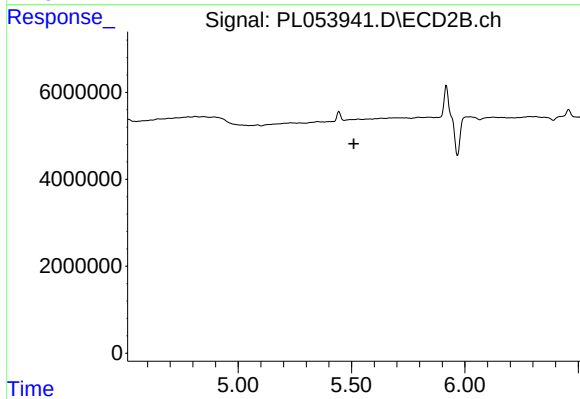

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.510 min
Response: 0
Conc: N.D.

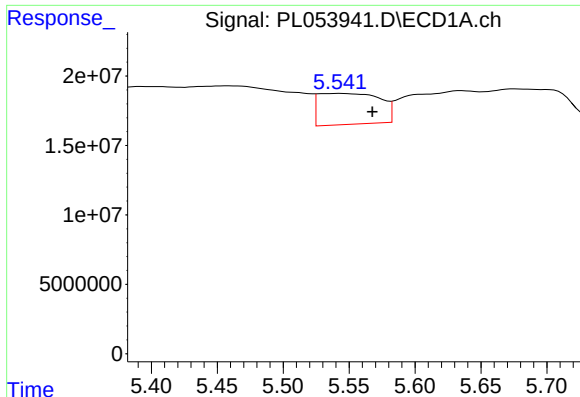

#26 Chlordane-4


R.T.: 5.542 min
Delta R.T.: -0.025 min
Response: 72171893
Conc: 76.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

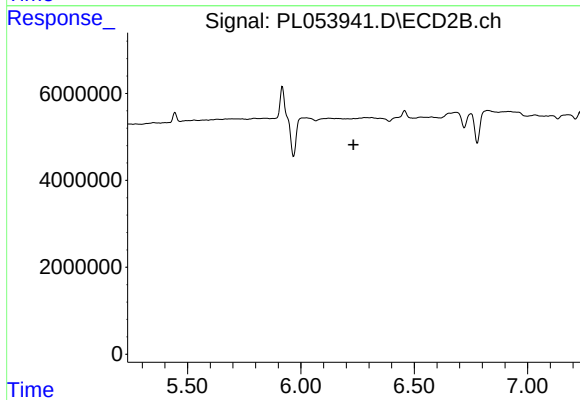


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

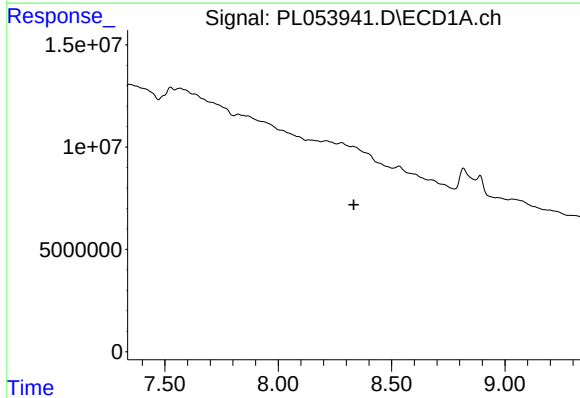

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.334 min
Response: 0
Conc: N.D.

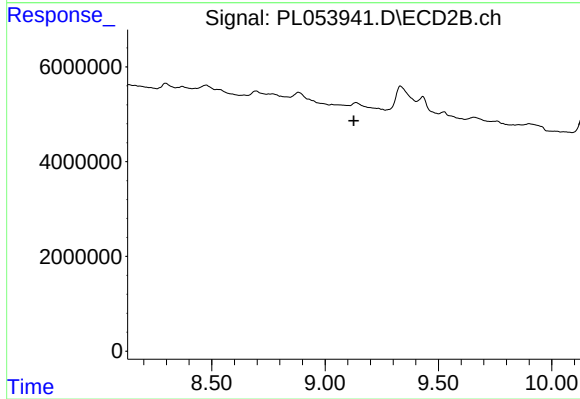

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.