

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
 Data File : PL053962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 17:11
 Operator : SG\AJ
 Sample : K5620-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:18:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.045	140.9E6	35933839	12.998	14.360
28)	SA Decachlor...	8.329	9.125	109.6E6	33184803	11.172	11.784
Target Compounds							
10)	B gamma-Chl...	5.526f	0.000	3625197	0	0.266	N.D. #
11)	B alpha-Chl...	0.000	6.232	0	1113320	N.D.	0.381 #
17)	MA 4,4'-DDT	0.000	7.152f	0	15181783	N.D.	6.565 #
25)	Chlordane-3	5.526f	0.000	3625197	0	3.145	N.D. #
26)	Chlordane-4	0.000	6.232	0	1113320	N.D.	2.480 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
Data File : PL053962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 17:11
Operator : SG\AJ
Sample : K5620-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:18:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

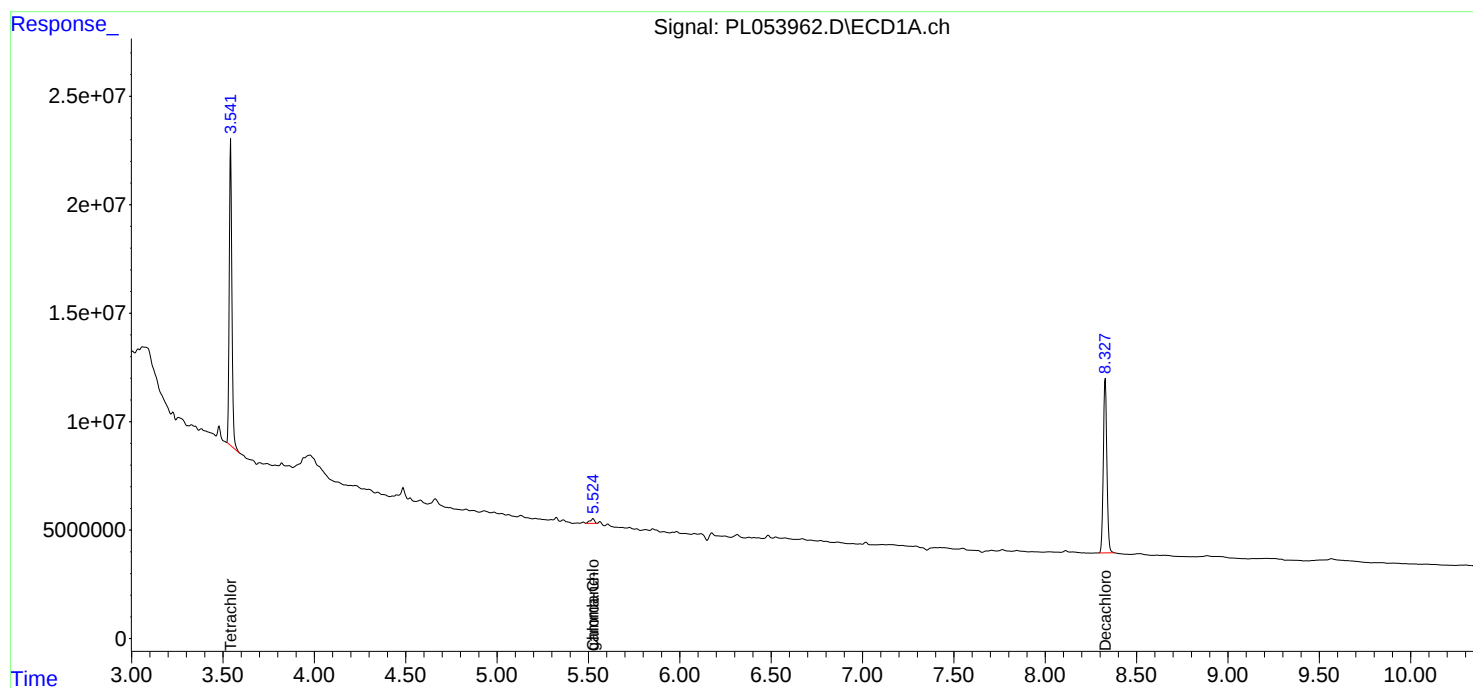


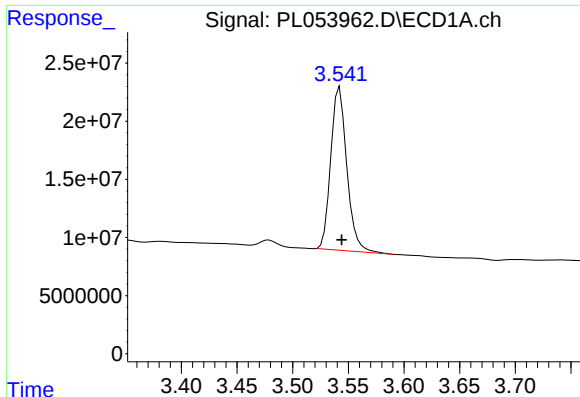

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 140885787
Conc: 13.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

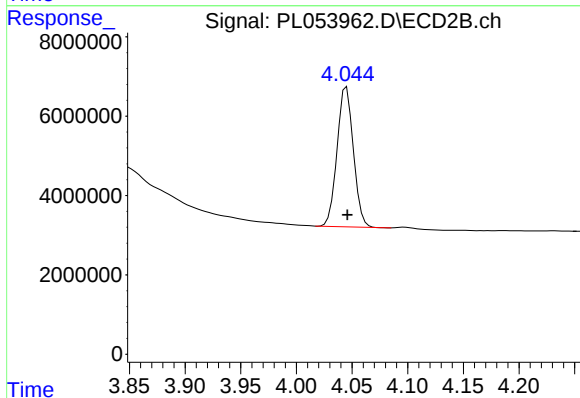


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 35933839
Conc: 14.36 ng/ml

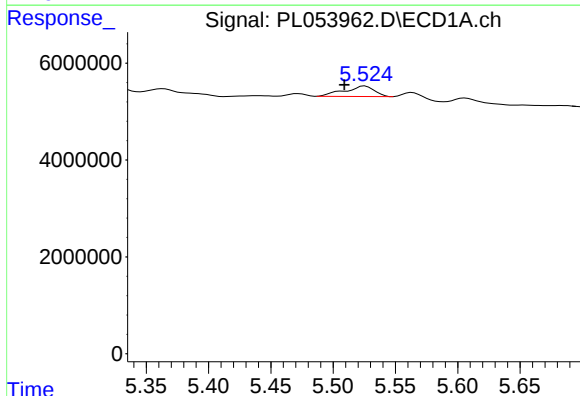


#10 gamma-Chlordane

R.T.: 5.526 min
Delta R.T.: 0.017 min
Response: 3625197
Conc: 0.27 ng/ml

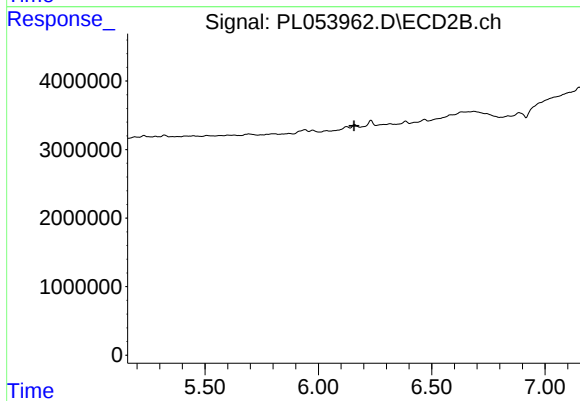

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

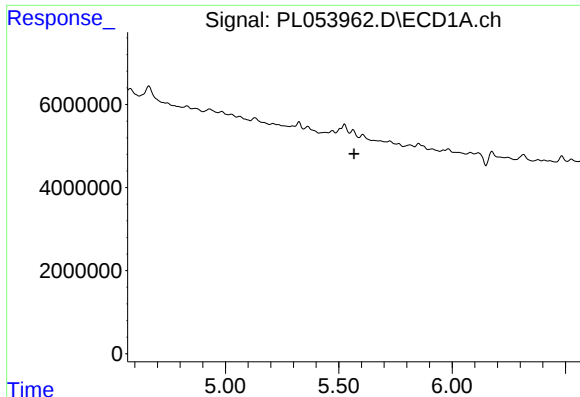

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

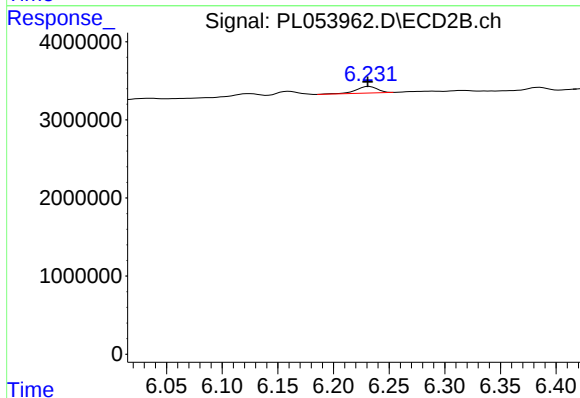


#11 alpha-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.001 min
Response: 1113320
Conc: 0.38 ng/ml

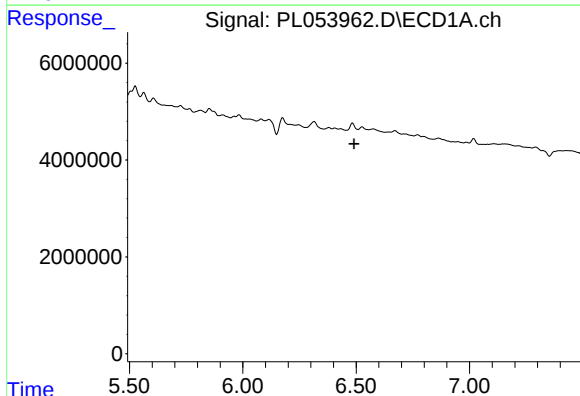


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

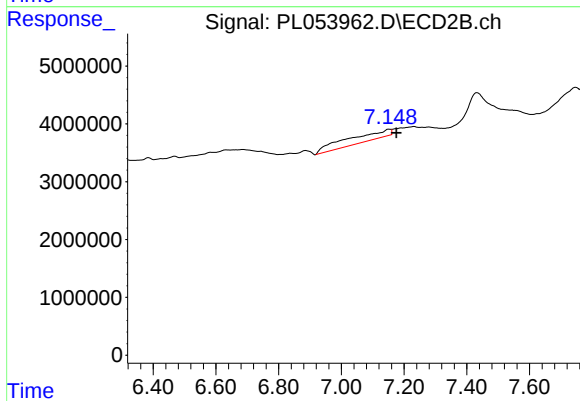

#17 4,4'-DDT


R.T.: 7.152 min
Delta R.T.: -0.024 min
Response: 15181783
Conc: 6.57 ng/ml

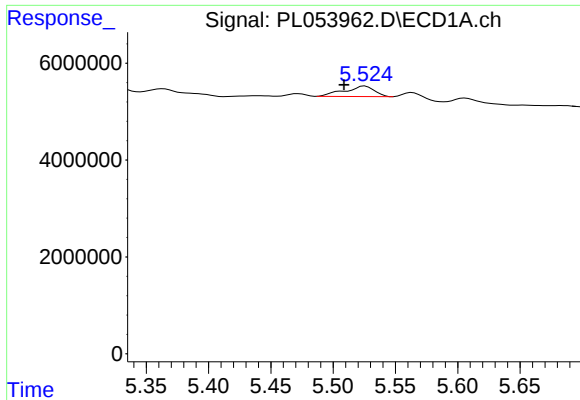

#25 Chlordane-3


R.T.: 5.526 min
Delta R.T.: 0.017 min
Response: 3625197
Conc: 3.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

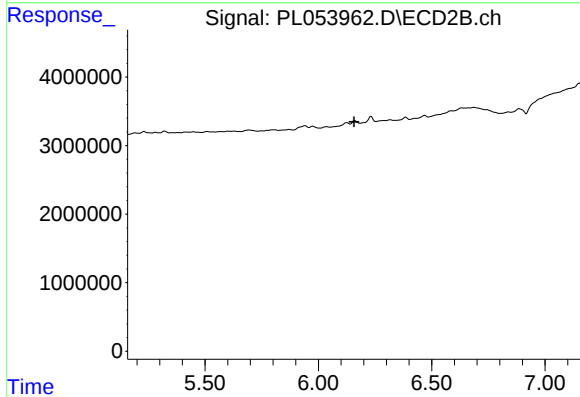


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

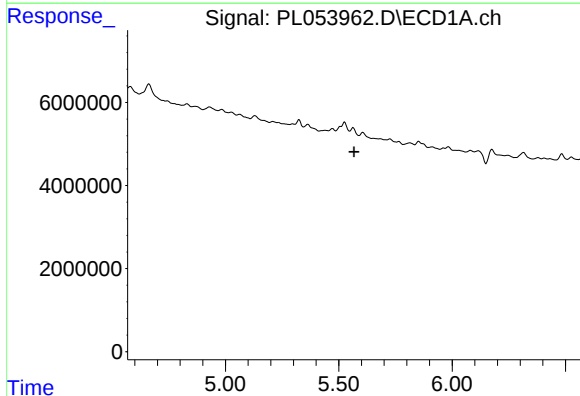


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.568 min
Response: 0
Conc: N.D.

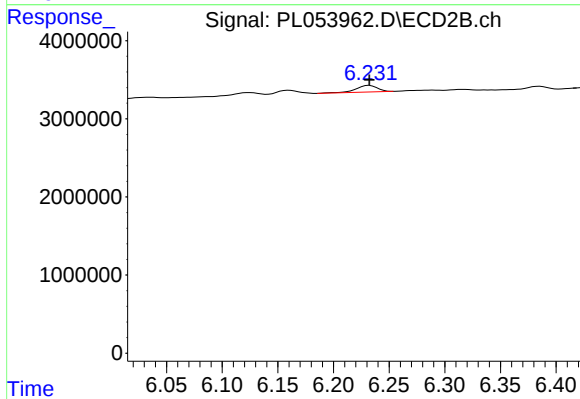

#26 Chlordane-4


R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 1113320
Conc: 2.48 ng/ml

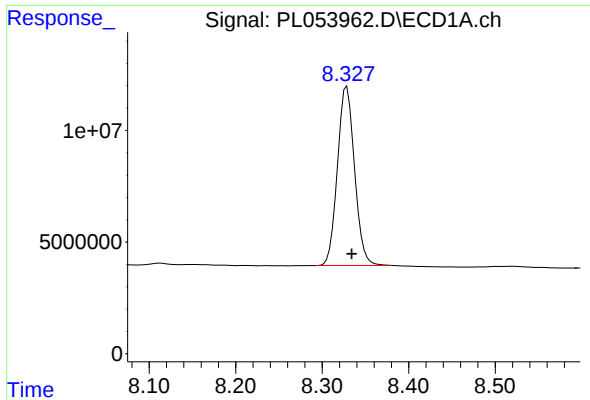

#28 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: -0.005 min
Response: 109615618
Conc: 11.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

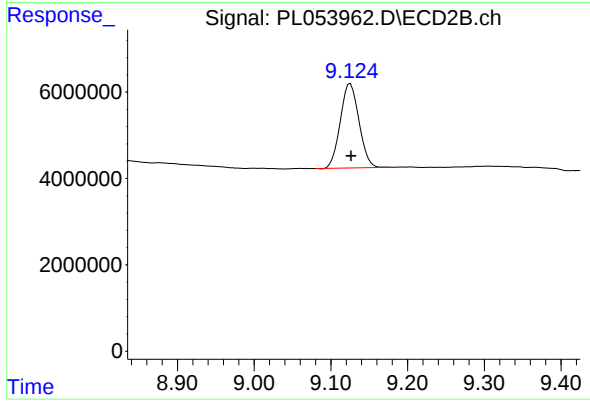

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 33184803
Conc: 11.78 ng/ml