

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
 Data File : PL053950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 14:20
 Operator : SG\AJ
 Sample : K5147-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-103019

Manual Integrations
 APPROVED

Ankita
 11/1/2019 11:42:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:16:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	149.7E6	34154187	13.813	13.649
28)	SA Decachlor...	8.329	9.126	90674363	28159380	9.242	10.000
Target Compounds							
11)	B alpha-Chl...	5.562	6.229	10023486	3681149	0.753m	1.261m#
12)	B 4,4'-DDE	5.726	6.382	7740900	1863304	0.651	0.662m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
Data File : PL053950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 14:20
Operator : SG\AJ
Sample : K5147-08
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
OK-01-103019


Manual Integrations
APPROVED

Ankita
11/1/2019 11:42:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:16:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

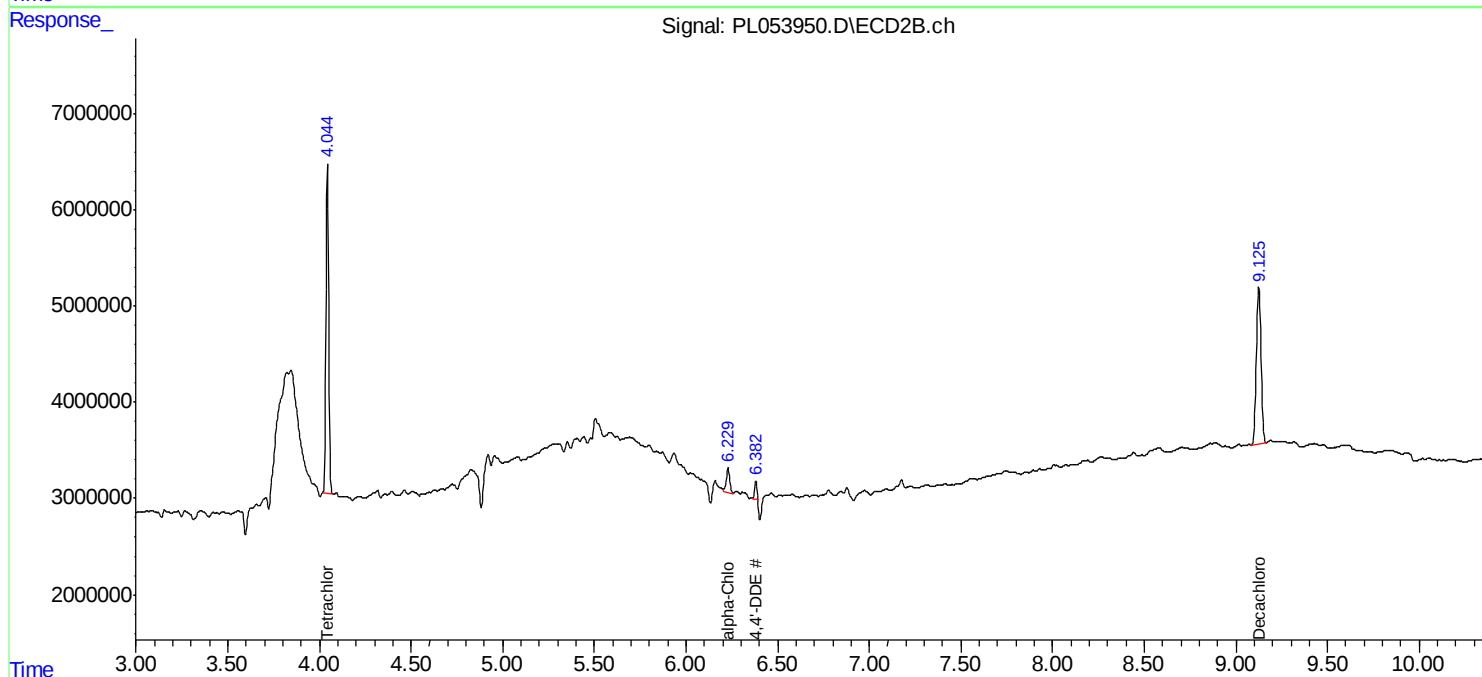

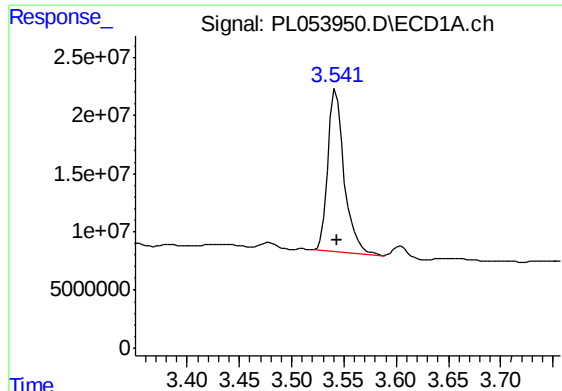


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 149728693
Conc: 13.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-103019


Manual Integrations
APPROVED

Ankita
11/1/2019 11:42:10 AM

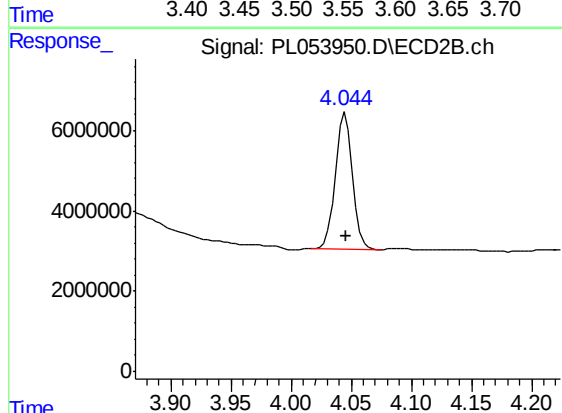


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 34154187
Conc: 13.65 ng/ml

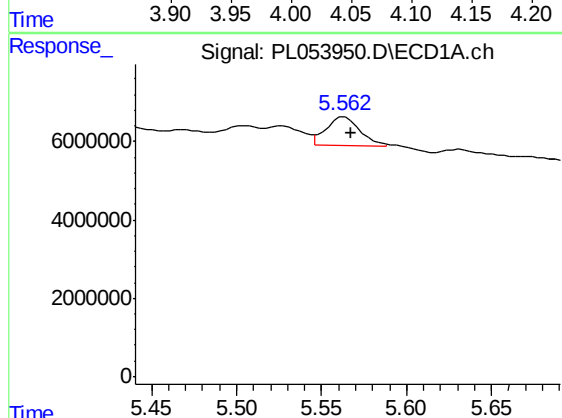


#11 alpha-Chlordane

R.T.: 5.562 min
Delta R.T.: -0.005 min
Response: 10023486
Conc: 0.75 ng/ml m

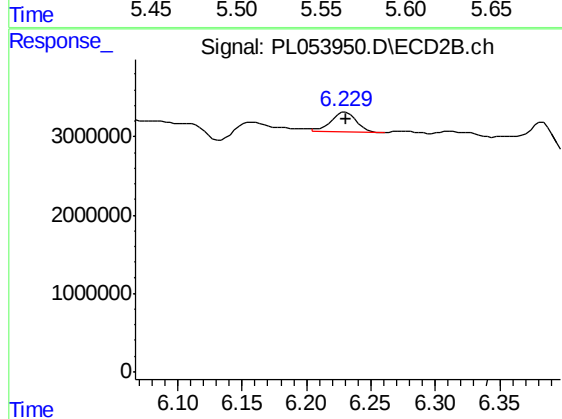

#11 alpha-Chlordane

R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 3681149
Conc: 1.26 ng/ml m

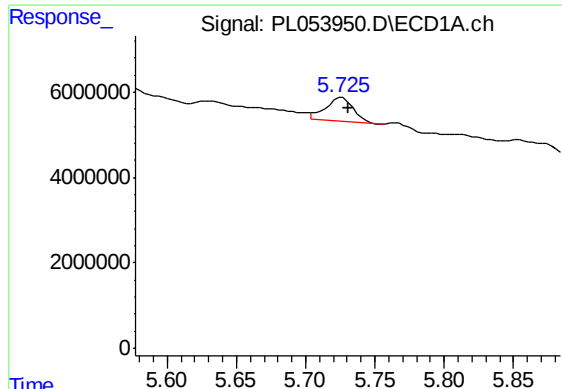


#12 4,4'-DDE

R.T.: 5.726 min
Delta R.T.: -0.004 min
Response: 7740900
Conc: 0.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-103019


Manual Integrations
APPROVED

Ankita
11/1/2019 11:42:10 AM

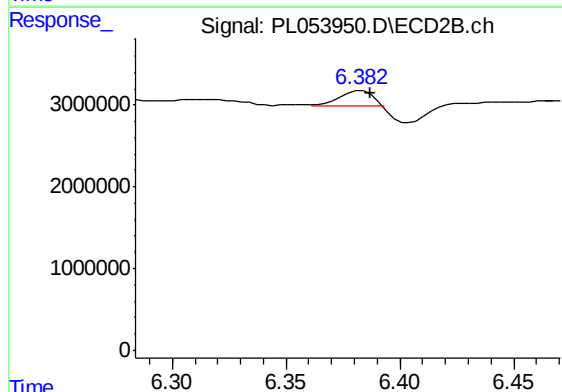


#12 4,4'-DDE

R.T.: 6.382 min
Delta R.T.: -0.005 min
Response: 1863304
Conc: 0.66 ng/ml m

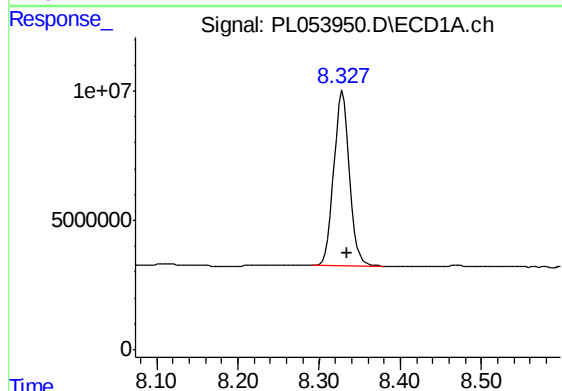

#28 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: -0.005 min
Response: 90674363
Conc: 9.24 ng/ml

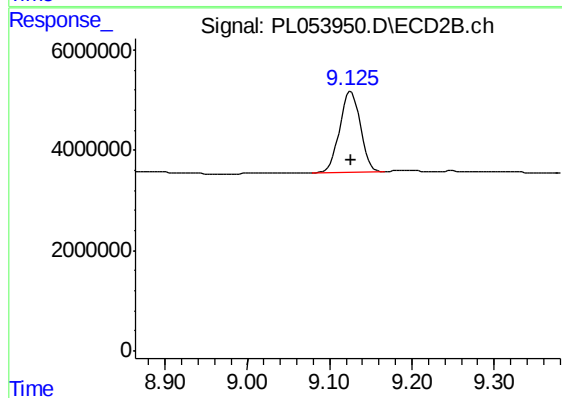

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 28159380
Conc: 10.00 ng/ml