

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
 Data File : PL053967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 18:21
 Operator : SG\AJ
 Sample : K5138-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-08-103019

Manual Integrations
 APPROVED

Ankita
 11/1/2019 11:42:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:19:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.046	179.6E6	46537324	16.565	18.597
28)	SA Decachlor...	8.328	9.126	140.2E6	44369777	14.288	15.756
Target Compounds							
15)	B Endosulfa...	6.401	6.972	6109408	3206916	0.546m	1.255m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103119\
Data File : PL053967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 18:21
Operator : SG\AJ
Sample : K5138-06
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AU-08-103019


Manual Integrations
APPROVED

Ankita
11/1/2019 11:42:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:19:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

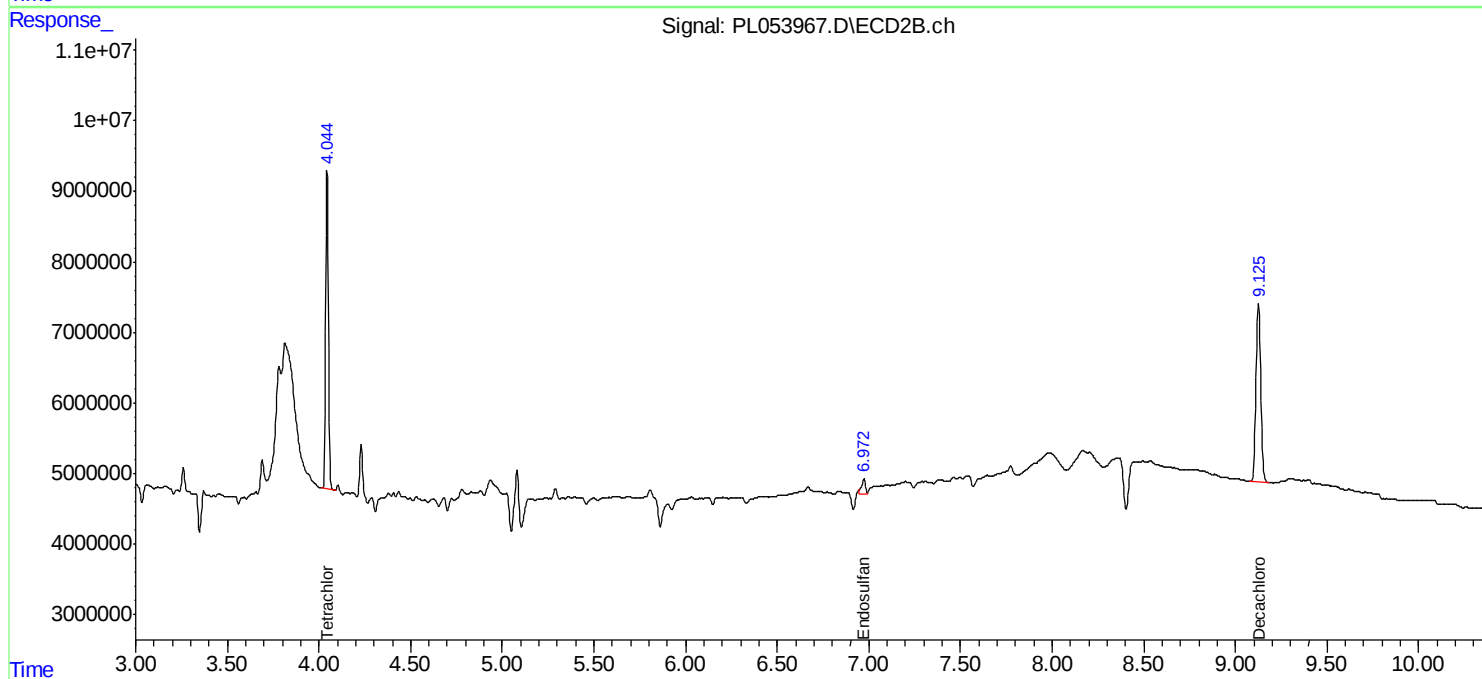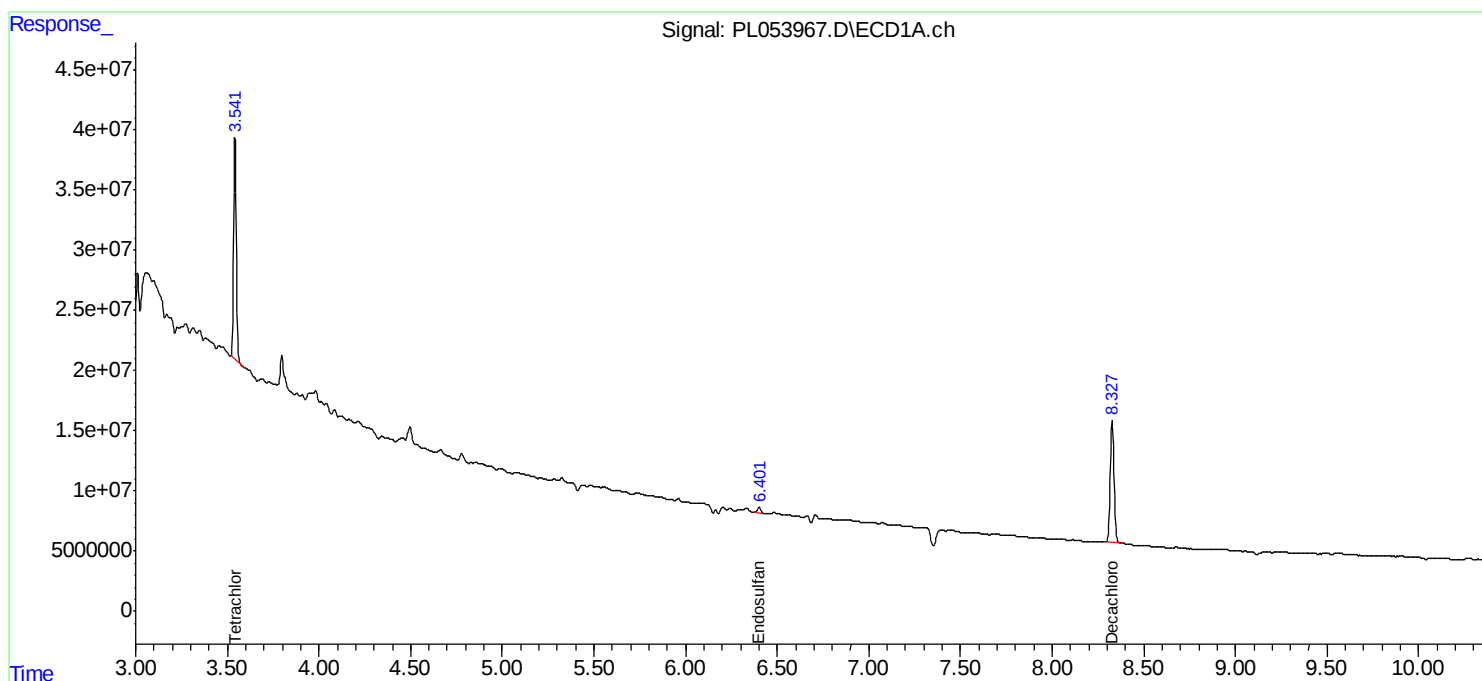

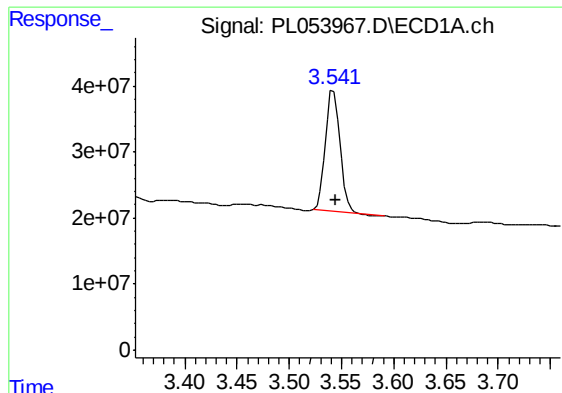


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 179552331
Conc: 16.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-08-103019


Manual Integrations
APPROVED

Ankita
11/1/2019 11:42:46 AM

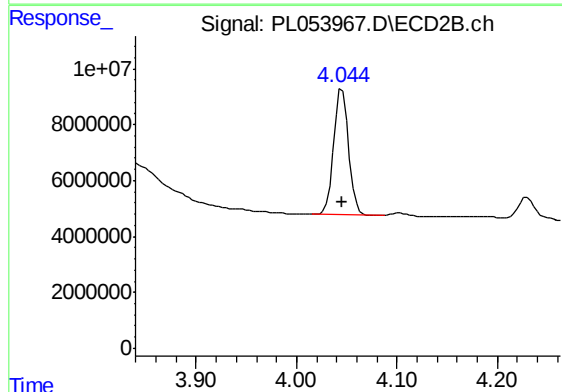


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 46537324
Conc: 18.60 ng/ml

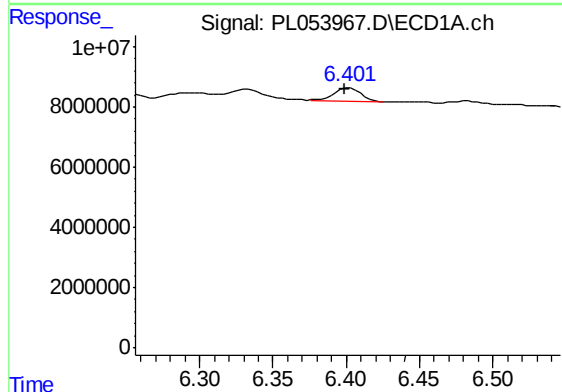


#15 Endosulfan II

R.T.: 6.401 min
Delta R.T.: 0.002 min
Response: 6109408
Conc: 0.55 ng/ml m

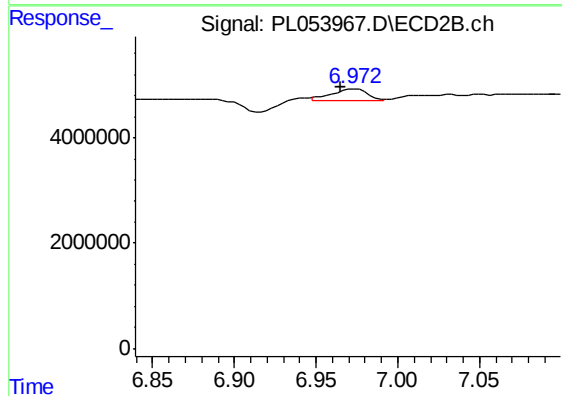

#15 Endosulfan II

R.T.: 6.972 min
Delta R.T.: 0.007 min
Response: 3206916
Conc: 1.26 ng/ml m

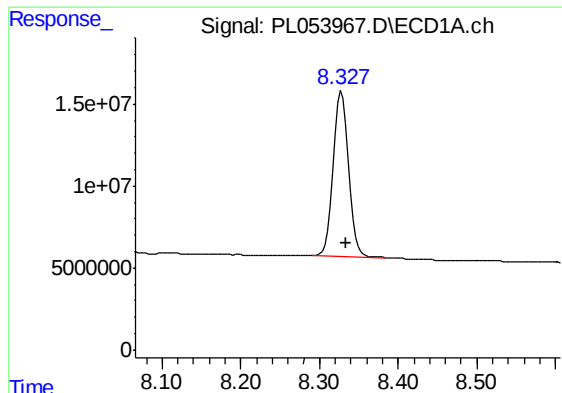


#28 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: -0.006 min
Response: 140191244
Conc: 14.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-08-103019

Manual Integrations
APPROVED

Ankita
11/1/2019 11:42:46 AM

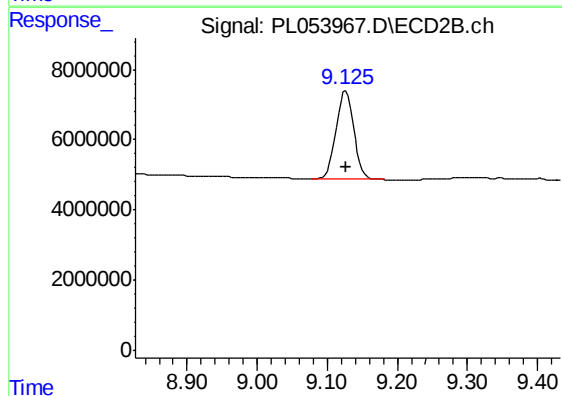

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 44369777
Conc: 15.76 ng/ml