

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103122\
 Data File : PL078656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2022 16:10
 Operator : AR\AJ
 Sample : N5313-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 22:12:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	2.573	29778894	42578006	15.615	16.676
28)	SA Decachlor...	8.774	7.641	27905491	36281342	18.550	19.155
Target Compounds							
2)	A alpha-BHC	3.757f	0.000	774011	0	0.270	N.D. #
5)	MB Aldrin	0.000	3.963f	0	922586	N.D.	0.263 #
7)	B delta-BHC	4.545f	0.000	3175553	0	1.395	N.D. #
10)	B gamma-Chl...	5.710	0.000	438993	0	0.194	N.D. #
13)	MA Dieldrin	6.148f	0.000	95775	0	0.044	N.D. #
14)	MA Endrin	6.327f	0.000	103421	0	0.054	N.D. #
17)	MA 4,4'-DDT	6.829f	0.000	294280	0	0.164	N.D. #
20)	A Methoxychlor	7.295	0.000	11633	0	0.013	N.D. #
21)	B Endrin ke...	0.000	6.563	0	43461	N.D.	0.017 #
25)	Chlordane-3	5.710	0.000	438993	0	1.314	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103122\
Data File : PL078656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2022 16:10
Operator : AR\AJ
Sample : N5313-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 22:12:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

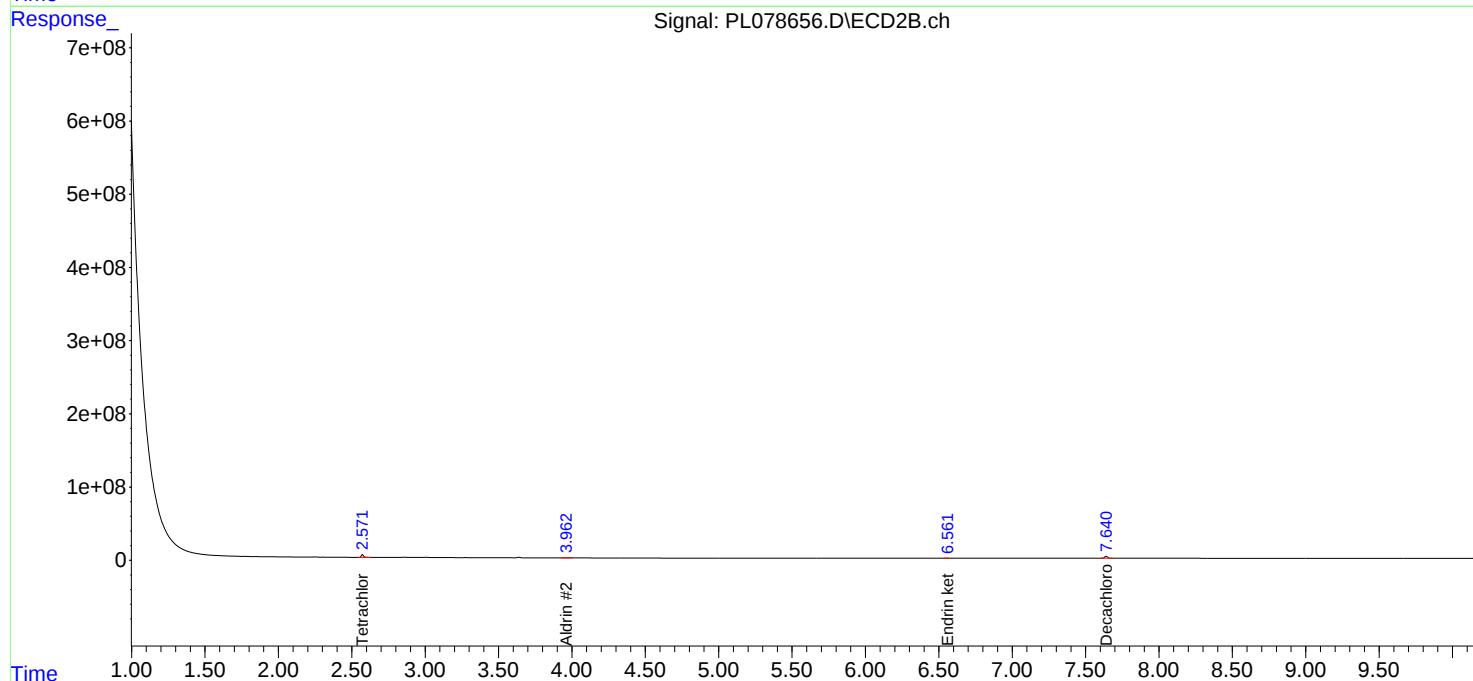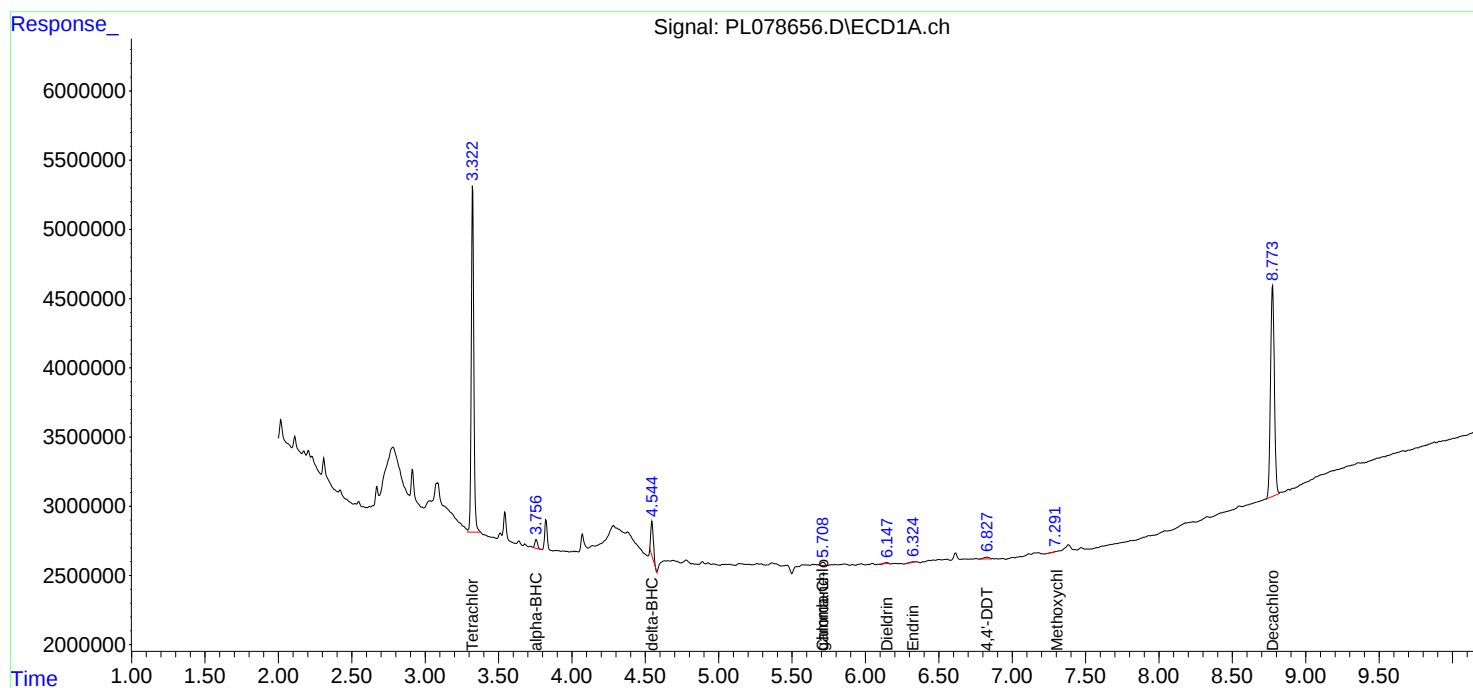


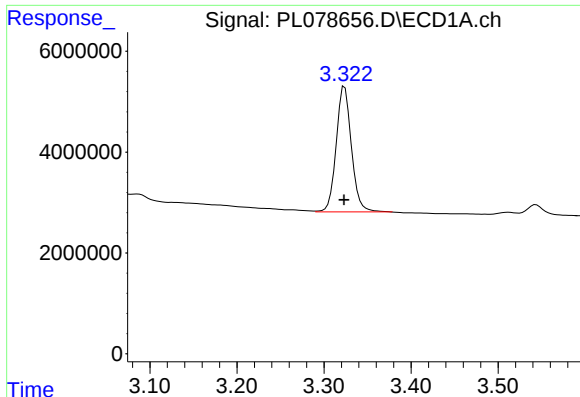

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 29778894
Conc: 15.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

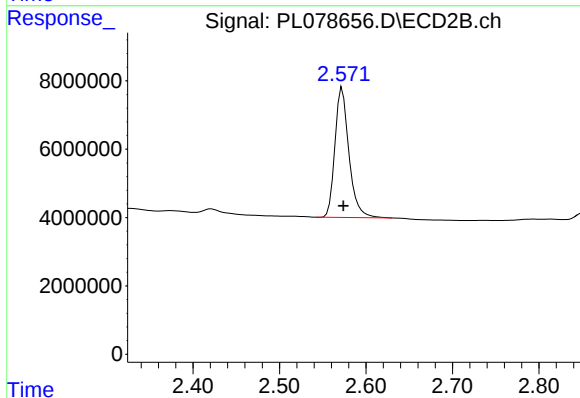


#1 Tetrachloro-m-xylene

R.T.: 2.573 min
Delta R.T.: -0.001 min
Response: 42578006
Conc: 16.68 ng/ml

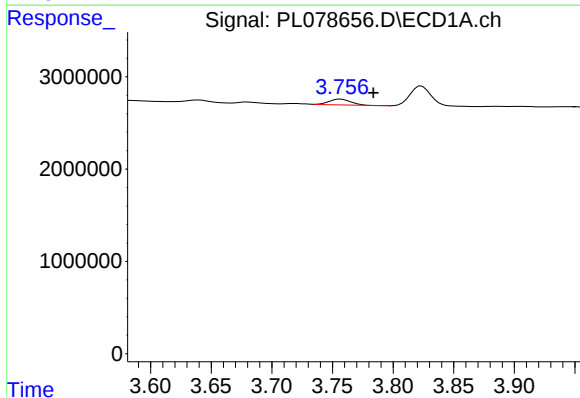


#2 alpha-BHC

R.T.: 3.757 min
Delta R.T.: -0.027 min
Response: 774011
Conc: 0.27 ng/ml

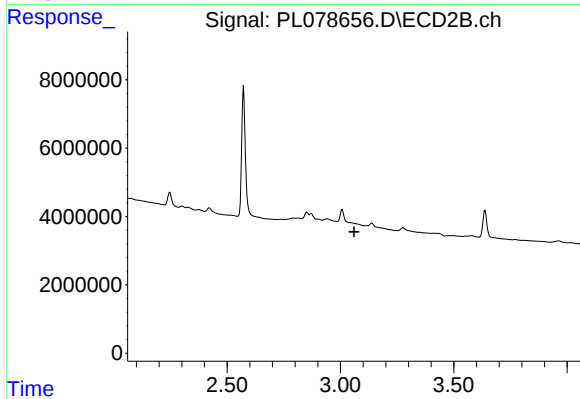

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.061 min
Response: 0
Conc: N.D.

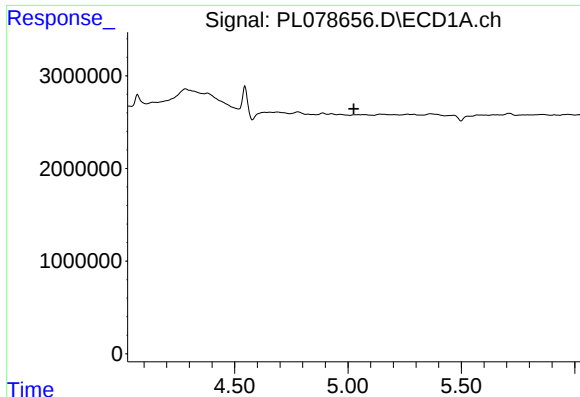

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.025 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

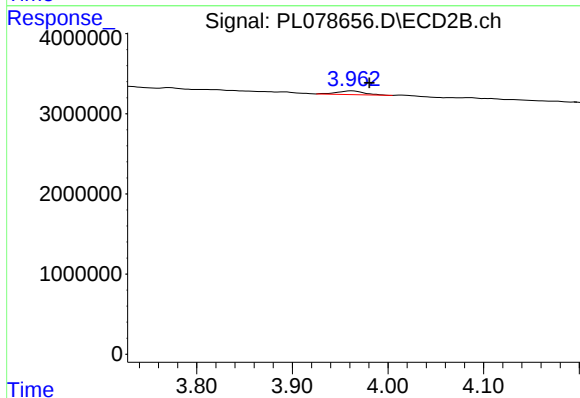


#5 Aldrin

R.T.: 3.963 min
Delta R.T.: -0.017 min
Response: 922586
Conc: 0.26 ng/ml

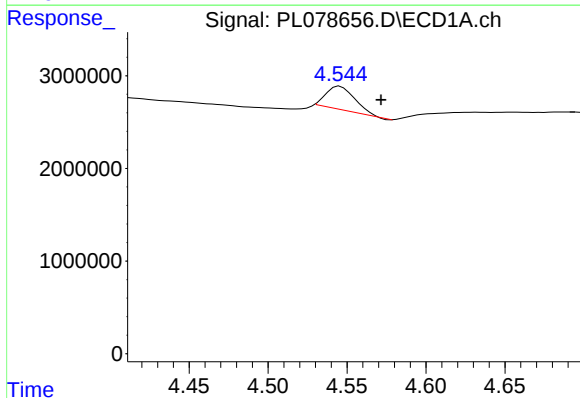


#7 delta-BHC

R.T.: 4.545 min
Delta R.T.: -0.026 min
Response: 3175553
Conc: 1.39 ng/ml

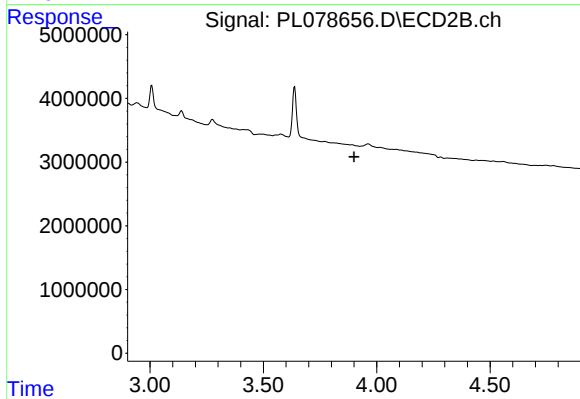

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 3.901 min
Response: 0
Conc: N.D.

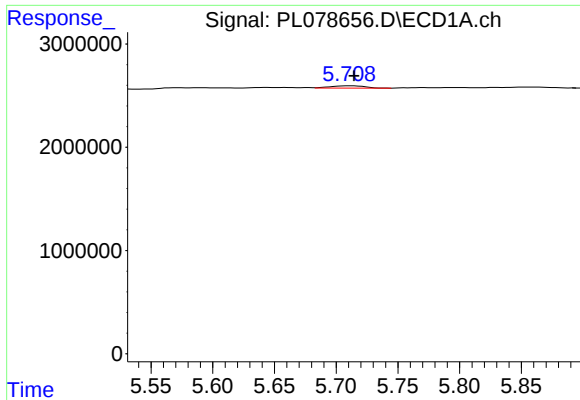

#10 gamma-Chlordane


R.T.: 5.710 min
Delta R.T.: -0.004 min
Response: 438993
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

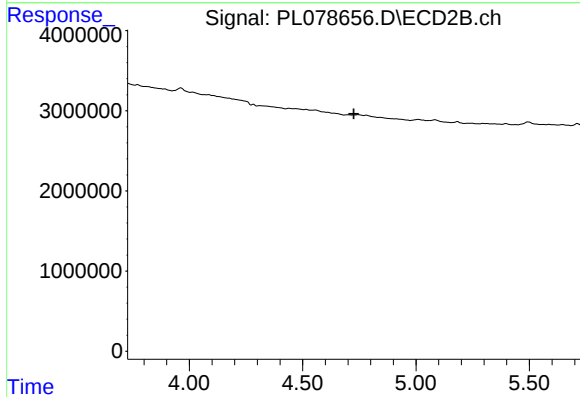


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

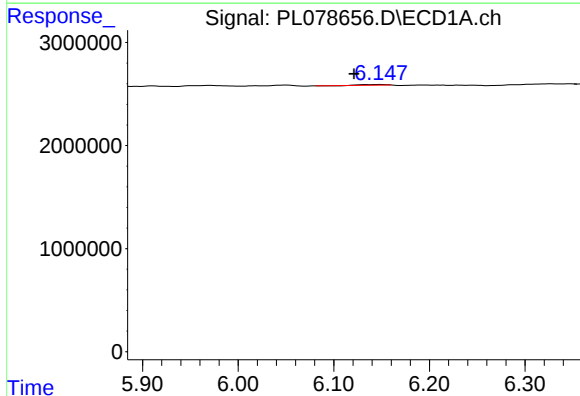


#13 Dieldrin

R.T.: 6.148 min
Delta R.T.: 0.026 min
Response: 95775
Conc: 0.04 ng/ml

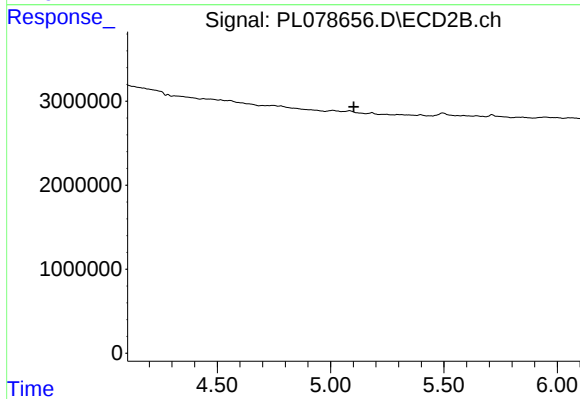

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.102 min
Response: 0
Conc: N.D.

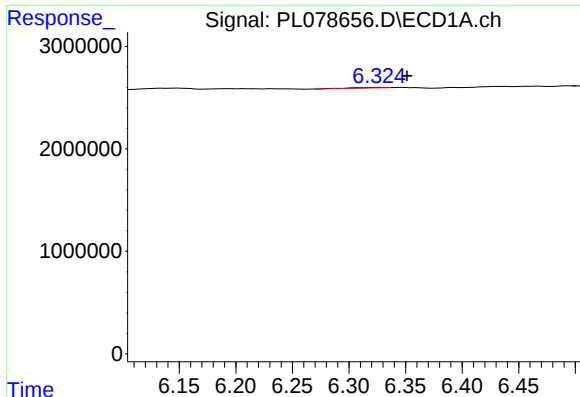

#14 Endrin


R.T.: 6.327 min
Delta R.T.: -0.025 min
Response: 103421
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

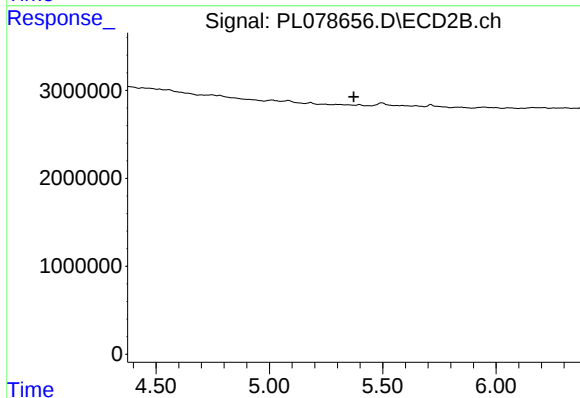


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.373 min
Response: 0
Conc: N.D.

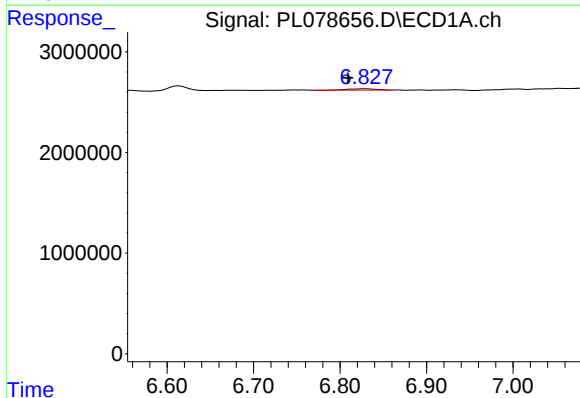


#17 4,4'-DDT

R.T.: 6.829 min
Delta R.T.: 0.020 min
Response: 294280
Conc: 0.16 ng/ml

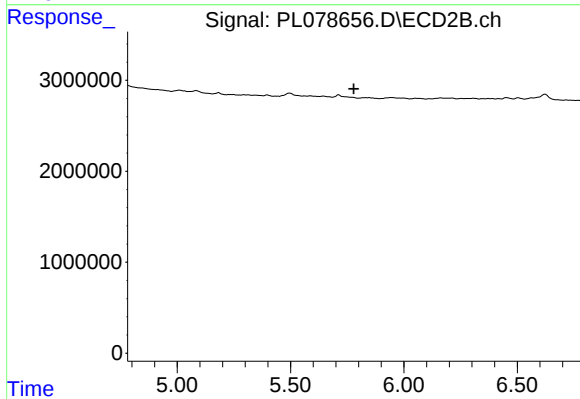

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 5.779 min
Response: 0
Conc: N.D.

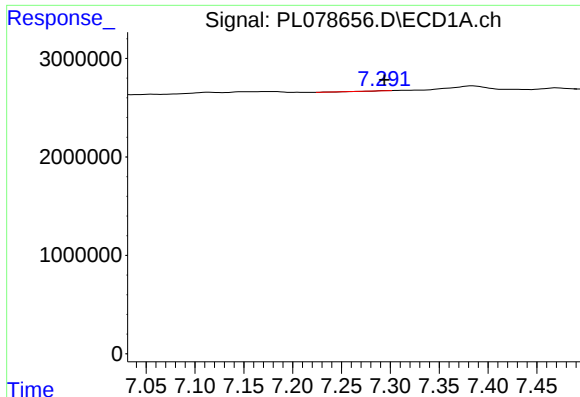

#20 Methoxychlor


R.T.: 7.295 min
Delta R.T.: 0.001 min
Response: 11633
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

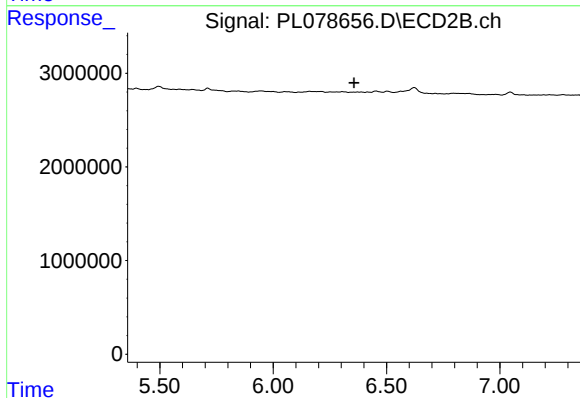


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

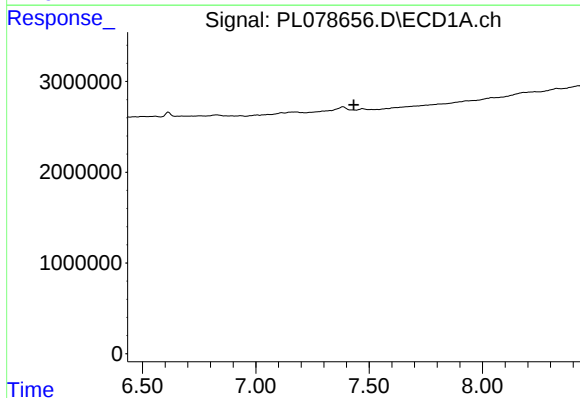


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

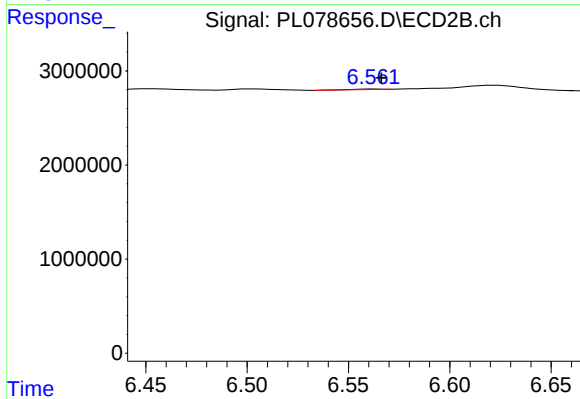

#21 Endrin ketone


R.T.: 6.563 min
Delta R.T.: -0.003 min
Response: 43461
Conc: 0.02 ng/ml

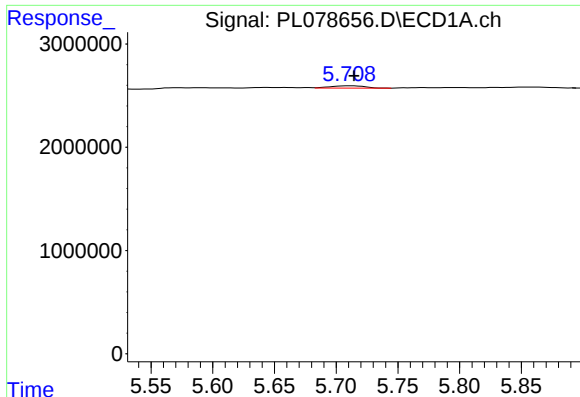

#25 Chlordane-3


R.T.: 5.710 min
Delta R.T.: -0.004 min
Response: 438993
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

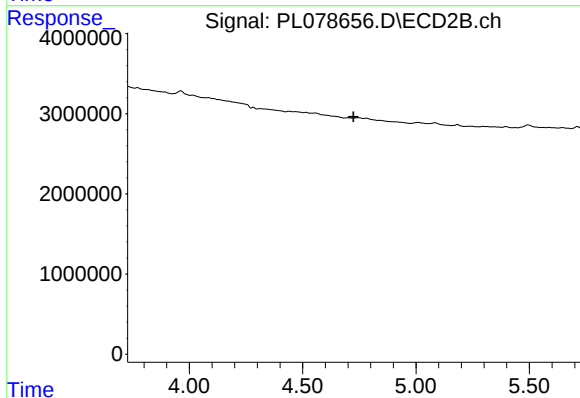


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

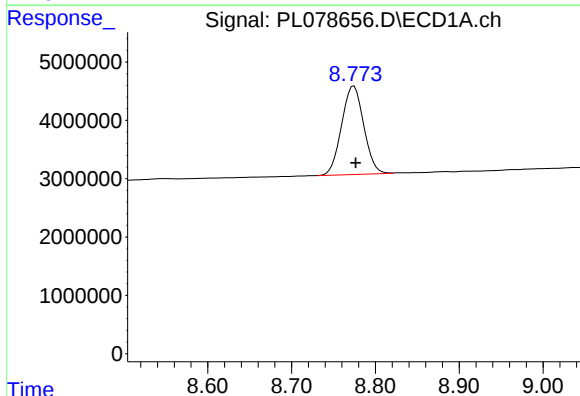

#28 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.002 min
Response: 27905491
Conc: 18.55 ng/ml

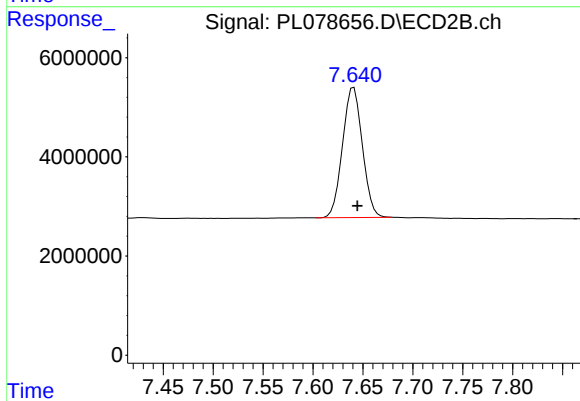

#28 Decachlorobiphenyl

R.T.: 7.641 min
Delta R.T.: -0.003 min
Response: 36281342
Conc: 19.15 ng/ml