

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103123\
 Data File : PL086365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 15:30
 Operator : AR\AJ
 Sample : PIBLK215
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 22:22:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.354	2.620	65840404	20175031	23.101	22.243
27)	SA Decachlor...	8.857	7.772	116.9E6	50865666	46.915	44.311
Target Compounds							
3)	MA gamma-BHC...	4.132	0.000	224652	0	<MDL	N.D. #
4)	MA Heptachlor	4.735	0.000	160934	0	<MDL	N.D. #
7)	B delta-BHC	4.590	0.000	3286208	0	0.883	N.D. #
8)	B Heptachlo...	5.498	0.000	471101	0	0.139	N.D. #
9)	A Endosulfan I	5.823f	0.000	1029329	0	0.320	N.D. #
10)	B trans-Chl...	5.823f	0.000	1029329	0	0.294	N.D. #
11)	B cis-Chlor...	5.823	0.000	1029329	0	0.293	N.D. #
12)	B 4,4'-DDE	6.069f	0.000	313198	0	<MDL	N.D. #
15)	B Endosulfa...	6.611	0.000	3404779	0	1.088	N.D. #
16)	A 4,4'-DDD	6.537	0.000	42583	0	<MDL	N.D. #
19)	B Endosulfa...	6.965	0.000	376821	0	0.133	N.D. #
20)	A Methoxychlor	7.287f	0.000	183134	0	0.145	N.D. #
21)	B Endrin ke...	7.514f	0.000	372397	0	0.129	N.D. #
22)	Toxaphene-1	6.069	0.000	313198	0	13.889	N.D. #
24)	Toxaphene-3	6.965	0.000	376821	0	6.004	N.D. #
26)	Toxaphene-5	7.706f	0.000	113518	0	2.572	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103123\
Data File : PL086365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 15:30
Operator : AR\AJ
Sample : PIBLK215
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 22:22:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 27 01:35:51 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

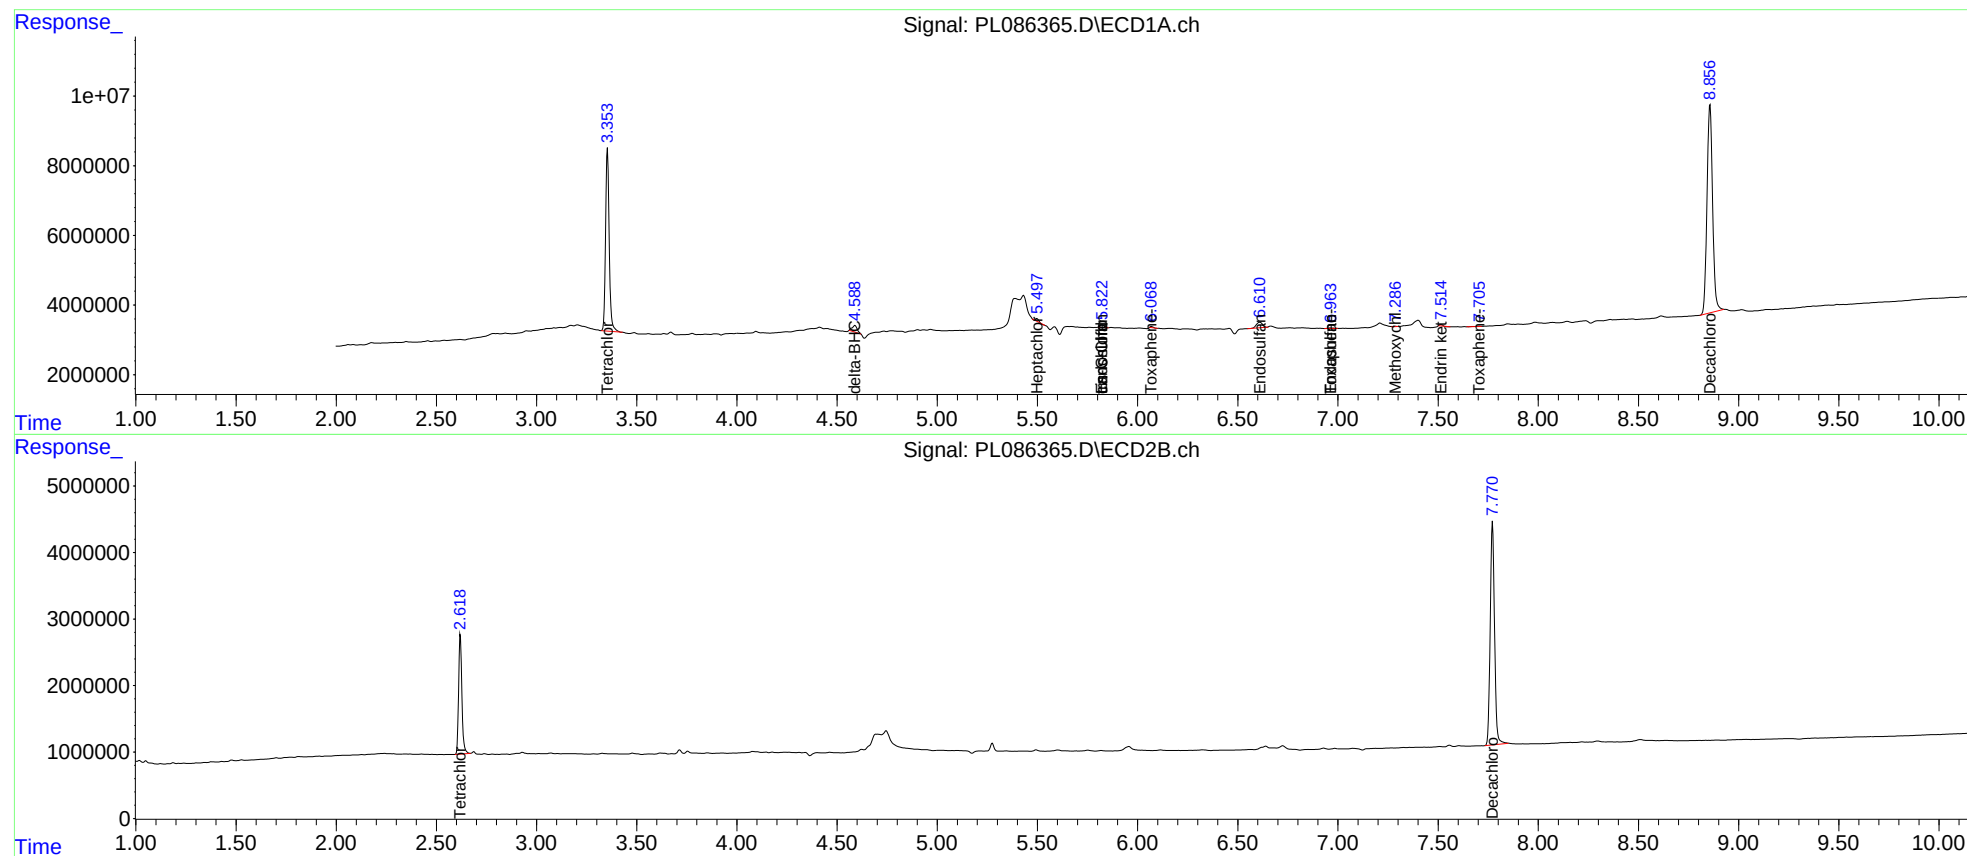

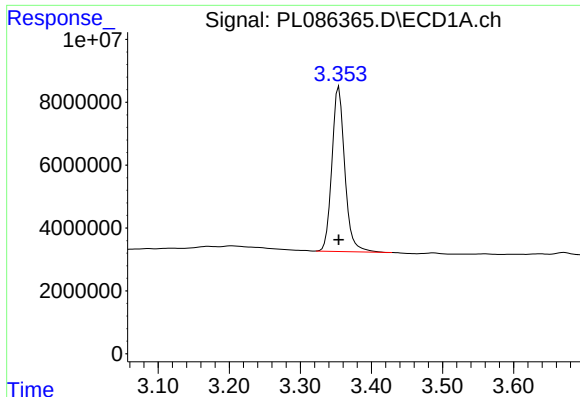


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: 0.000 min
Response: 65840404
Conc: 23.10 ng/ml

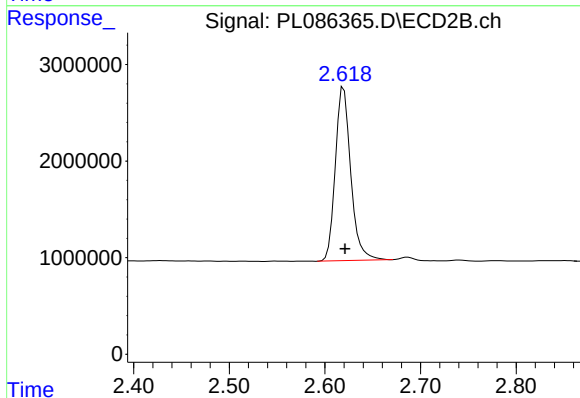


#1 Tetrachloro-m-xylene

R.T.: 2.620 min
Delta R.T.: -0.001 min
Response: 20175031
Conc: 22.24 ng/ml

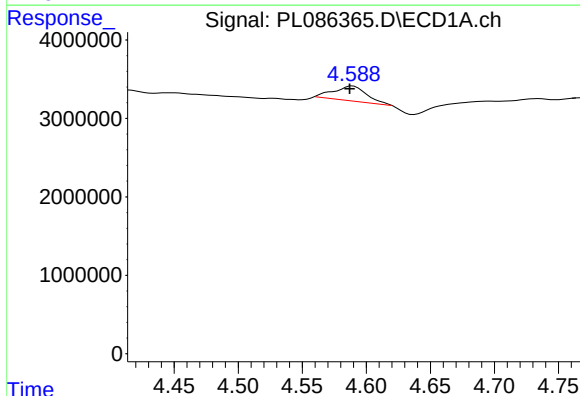


#7 delta-BHC

R.T.: 4.590 min
Delta R.T.: 0.002 min
Response: 3286208
Conc: 0.88 ng/ml

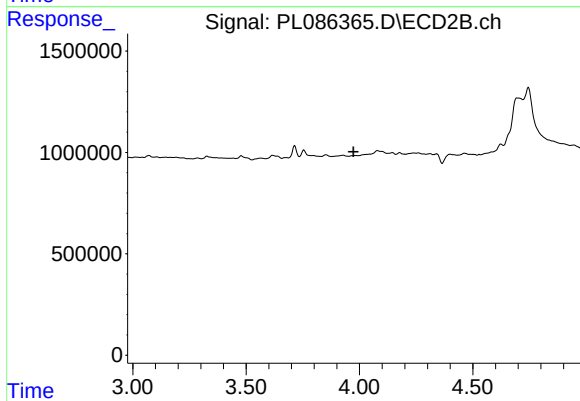


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 3.974 min
Response: 0
Conc: N.D.

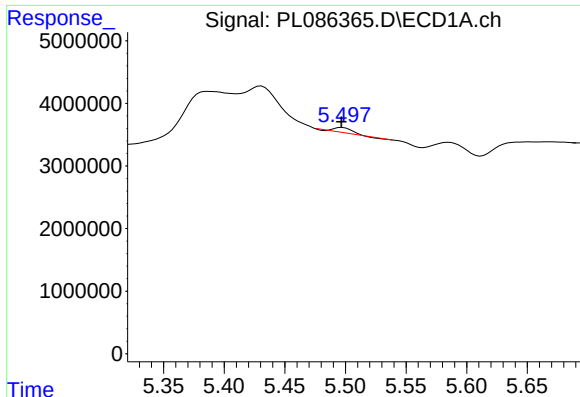


#8 Heptachlor epoxide

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 471101
Conc: 0.14 ng/ml

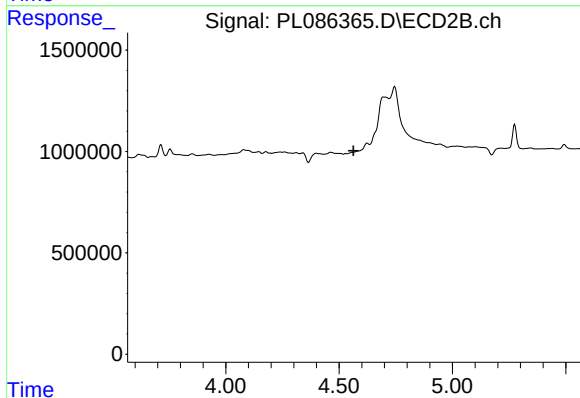


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.564 min
Response: 0
Conc: N.D.

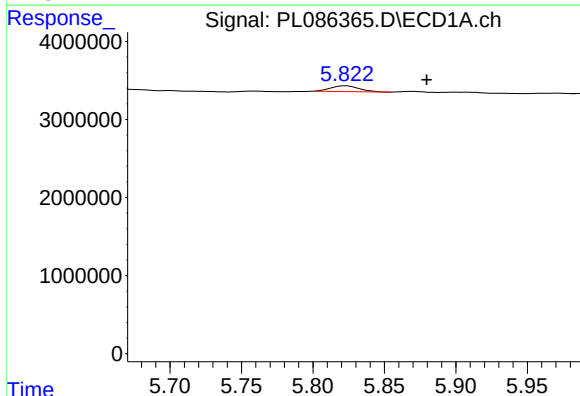


#9 Endosulfan I

R.T.: 5.823 min
Delta R.T.: -0.056 min
Response: 1029329
Conc: 0.32 ng/ml

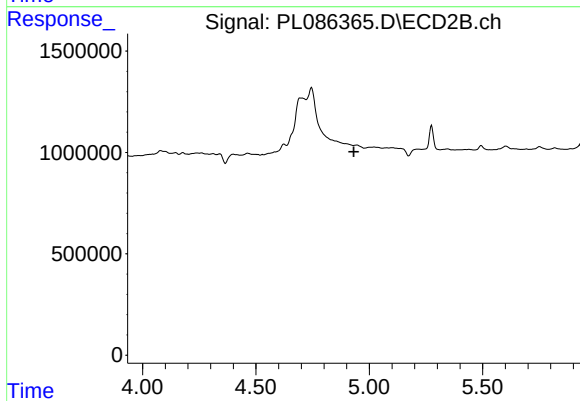


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 4.931 min
Response: 0
Conc: N.D.

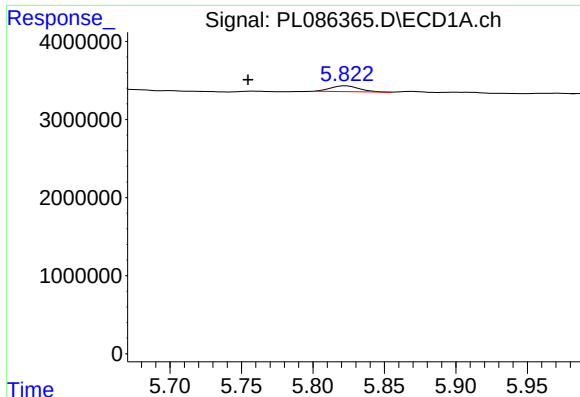


#10 trans-Chlordane

R.T.: 5.823 min
Delta R.T.: 0.069 min
Response: 1029329
Conc: 0.29 ng/ml

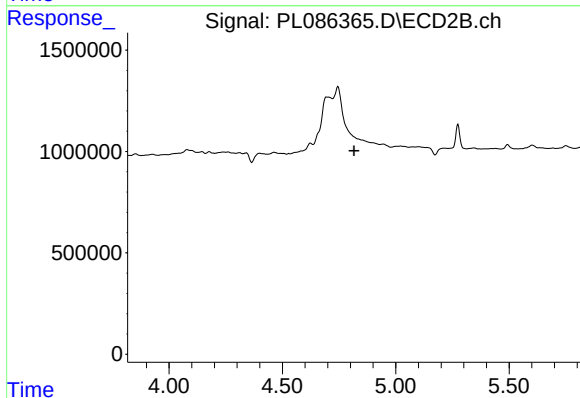


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.816 min
Response: 0
Conc: N.D.

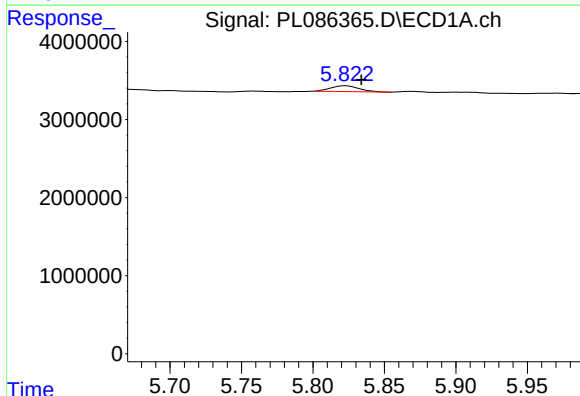


#11 cis-Chlordane

R.T.: 5.823 min
Delta R.T.: -0.011 min
Response: 1029329
Conc: 0.29 ng/ml

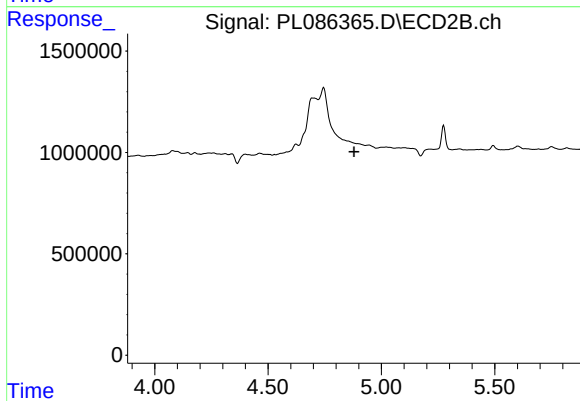


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.880 min
Response: 0
Conc: N.D.

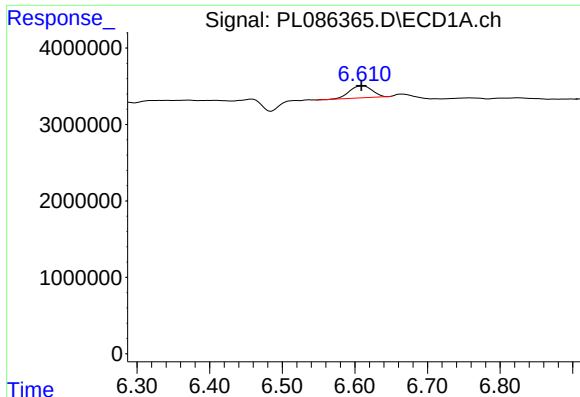


#15 Endosulfan II

R.T.: 6.611 min
Delta R.T.: 0.002 min
Response: 3404779
Conc: 1.09 ng/ml

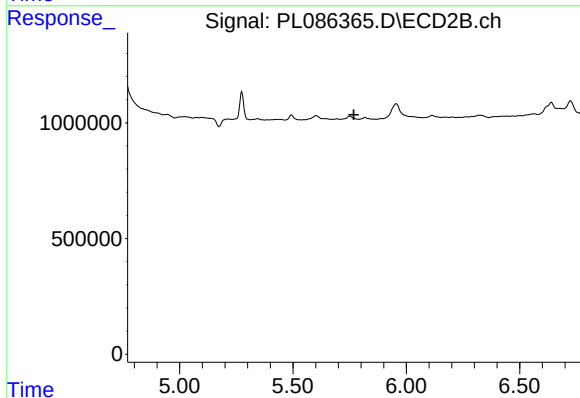


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.769 min
Response: 0
Conc: N.D.

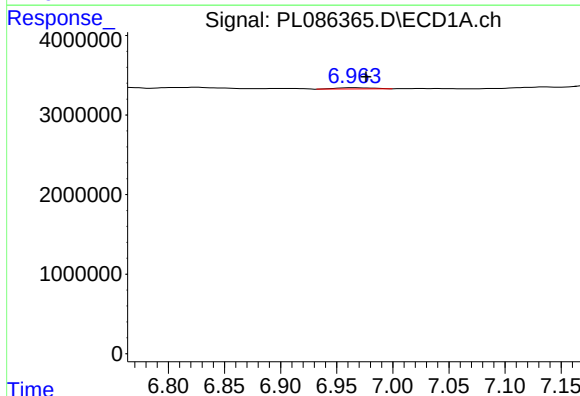


#19 Endosulfan Sulfate

R.T.: 6.965 min
Delta R.T.: -0.012 min
Response: 376821
Conc: 0.13 ng/ml

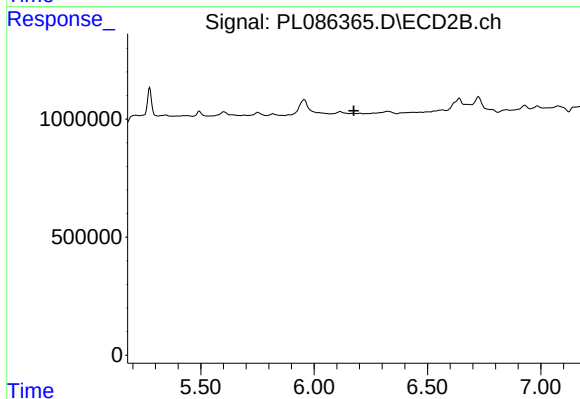


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.175 min
Response: 0
Conc: N.D.

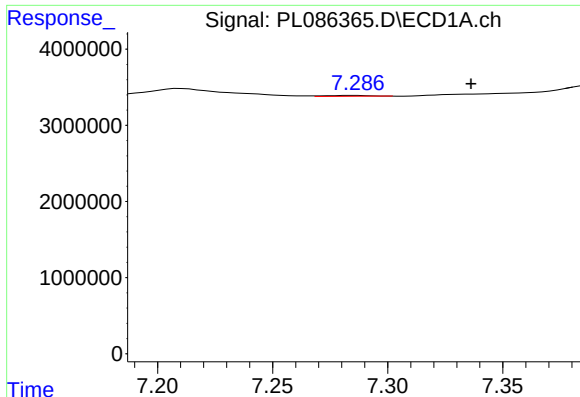


#20 Methoxychlor

R.T.: 7.287 min
Delta R.T.: -0.049 min
Response: 183134
Conc: 0.15 ng/ml

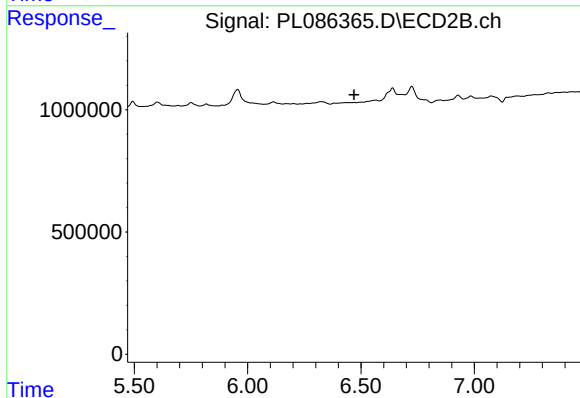


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.470 min
Response: 0
Conc: N.D.

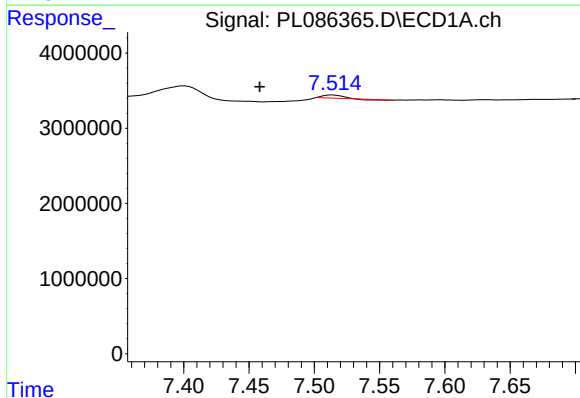


#21 Endrin ketone

R.T.: 7.514 min
Delta R.T.: 0.056 min
Response: 372397
Conc: 0.13 ng/ml

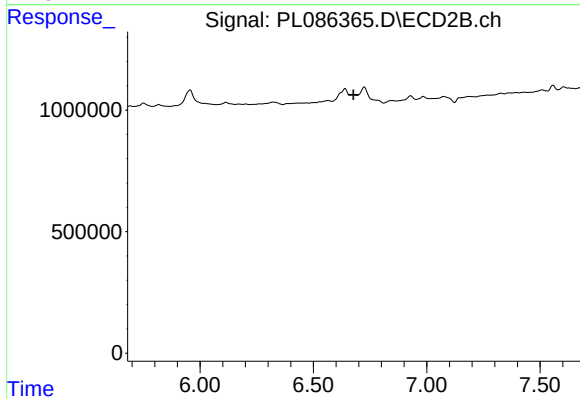


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.677 min
Response: 0
Conc: N.D.

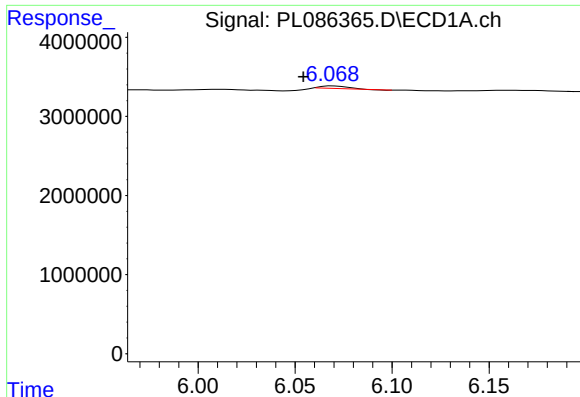


#22 Toxaphene-1

R.T.: 6.069 min
Delta R.T.: 0.015 min
Response: 313198
Conc: 13.89 ng/ml

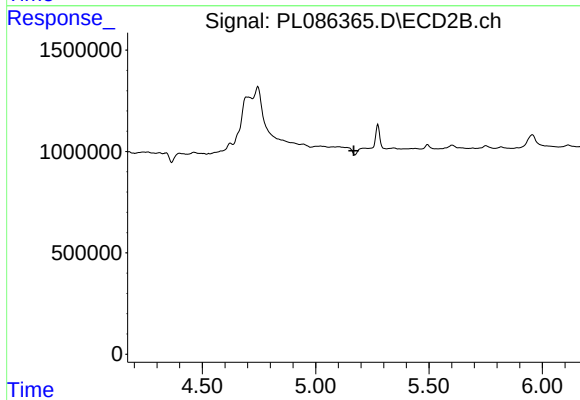


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

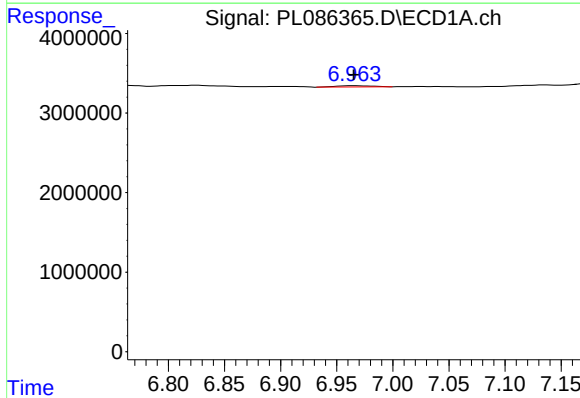


#24 Toxaphene-3

R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 376821
Conc: 6.00 ng/ml

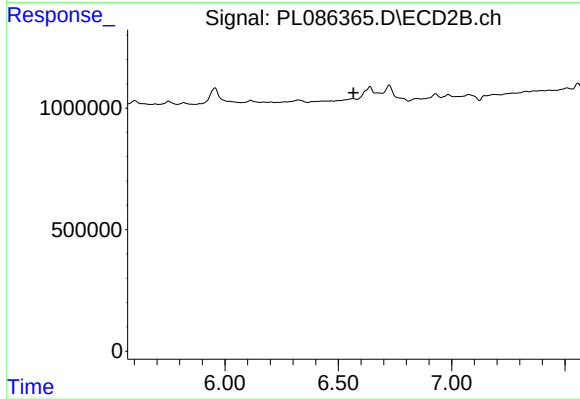


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 6.567 min
Response: 0
Conc: N.D.

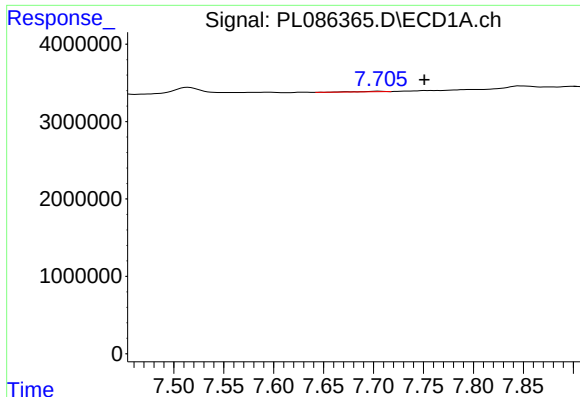


#26 Toxaphene-5

R.T.: 7.706 min
Delta R.T.: -0.045 min
Response: 113518
Conc: 2.57 ng/ml

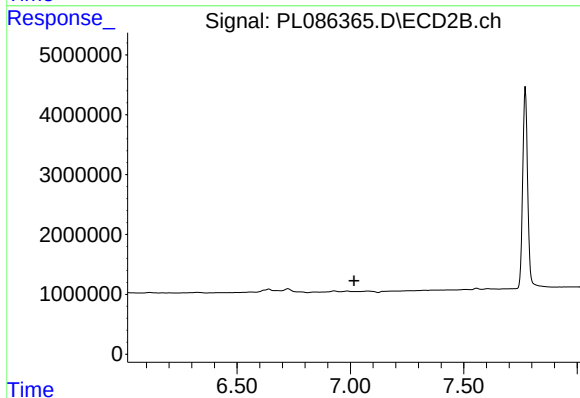


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.016 min
Response: 0
Conc: N.D.

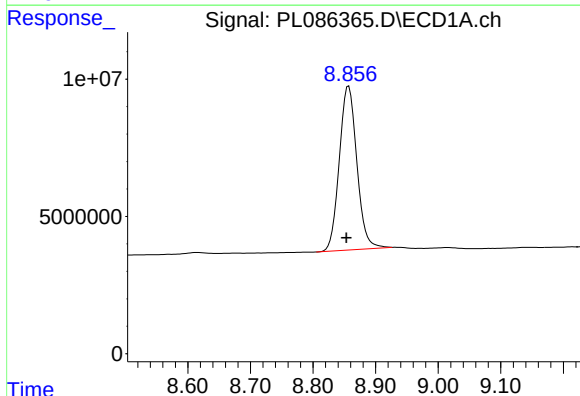

#27 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: 0.004 min
Response: 116920456
Conc: 46.92 ng/ml

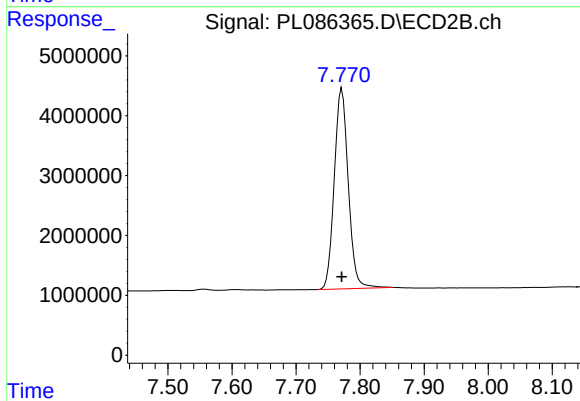

#27 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: 0.000 min
Response: 50865666
Conc: 44.31 ng/ml