

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
 Data File : PL092771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 19:01
 Operator : AR\AJ
 Sample : PB164557BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164557BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:50:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.779	51719811	55641641	21.108	20.448
28)	SA Decachlor...	9.058	7.918	44493609	63486739	23.119	23.262
Target Compounds							
2)	A alpha-BHC	0.000	3.269	0	198243	N.D.	0.050 #
5)	MB Aldrin	0.000	4.248f	0	58742	N.D.	0.016 #
7)	B delta-BHC	4.767	4.131	3905773	229866	1.248	0.060 #
10)	B gamma-Chl...	0.000	4.977	0	92626	N.D.	0.028 #
11)	B alpha-Chl...	0.000	5.046	0	81942	N.D.	0.025 #
14)	MA Endrin	0.000	5.661f	0	631807	N.D.	0.218 #
18)	B Endrin al...	0.000	6.091f	0	185598	N.D.	0.080 #
22)	Mirex	0.000	7.051f	0	53200	N.D.	0.020 #
23)	Chlordane-1	0.000	3.777	0	73483	N.D.	0.692 #
24)	Chlordane-2	0.000	4.356	0	176818	N.D.	1.428 #
25)	Chlordane-3	0.000	4.977	0	92626	N.D.	0.255 #
26)	Chlordane-4	0.000	5.046	0	81942	N.D.	0.234 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
Data File : PL092771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 19:01
Operator : AR\AJ
Sample : PB164557BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164557BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:50:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

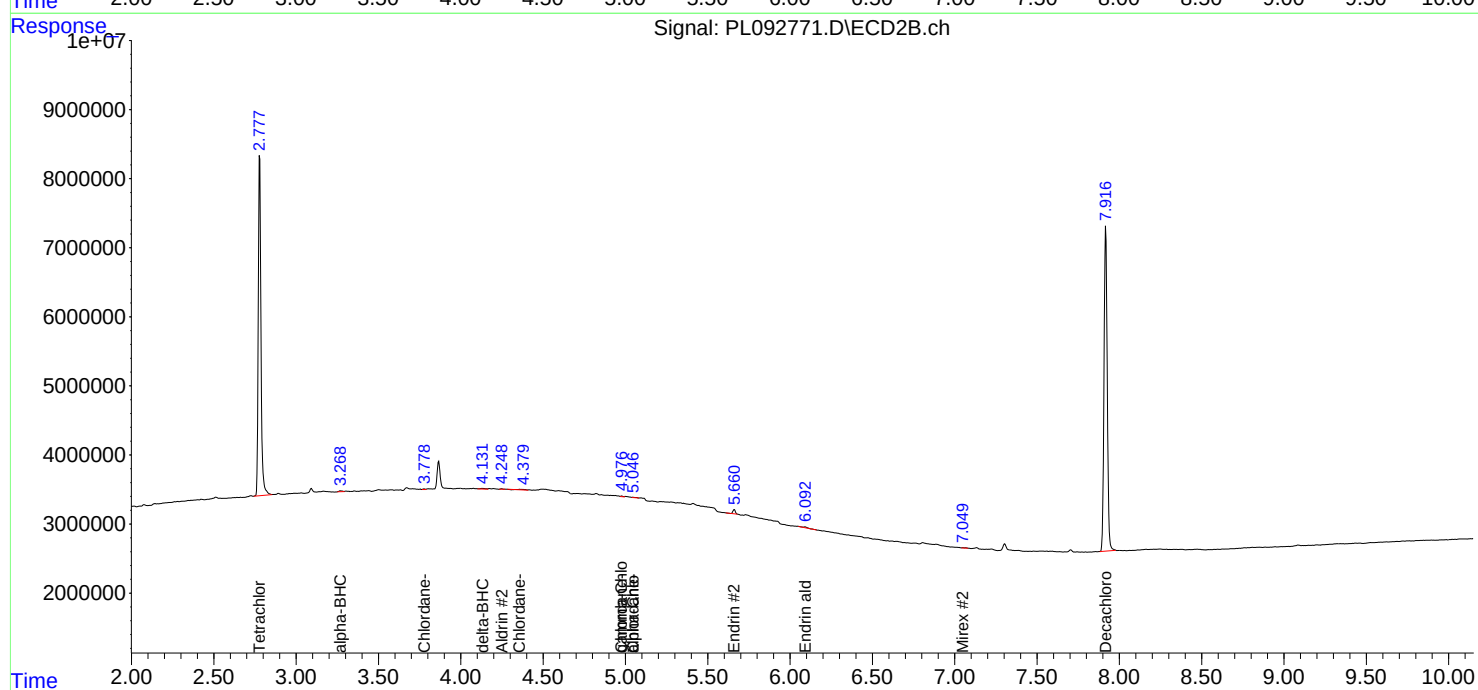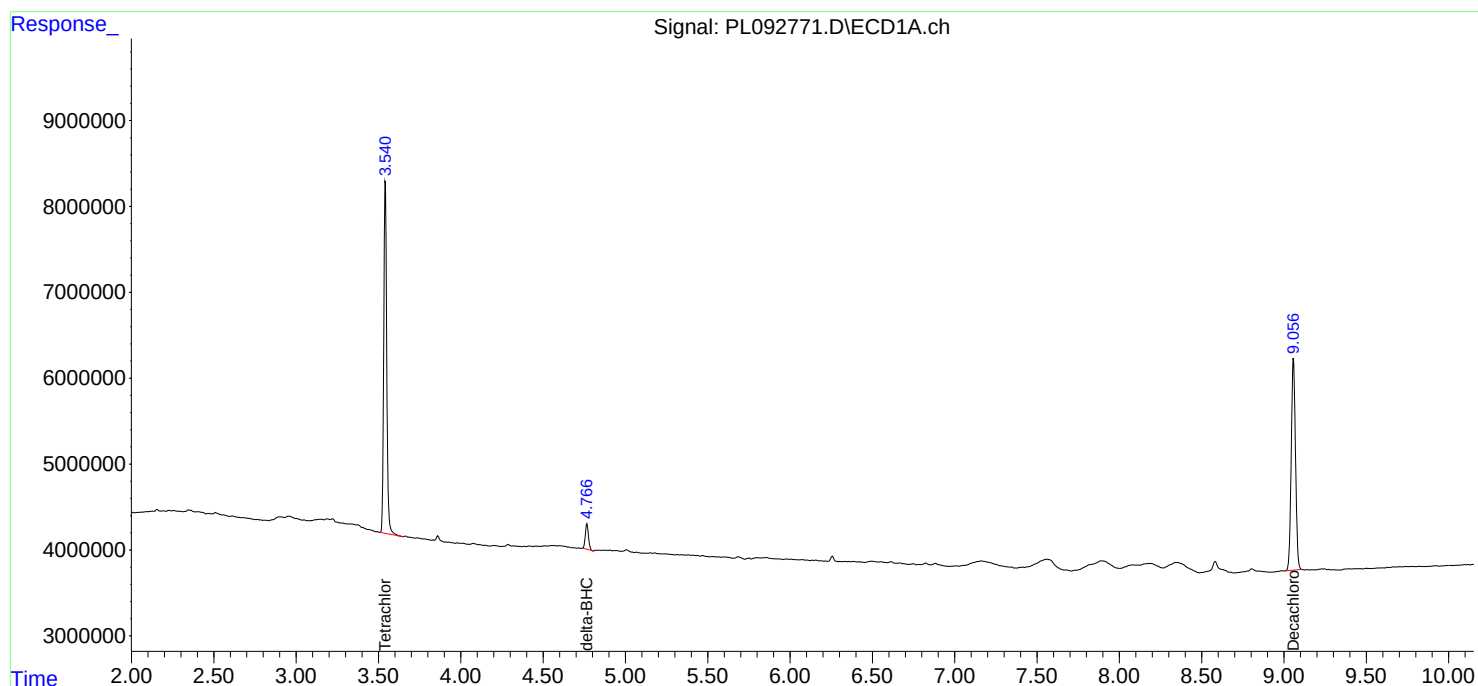


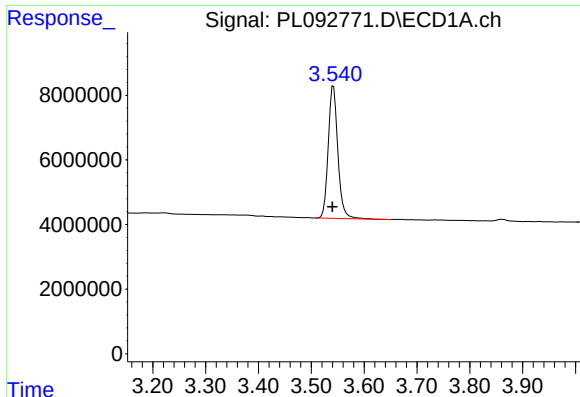

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 51719811
Conc: 21.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164557BL

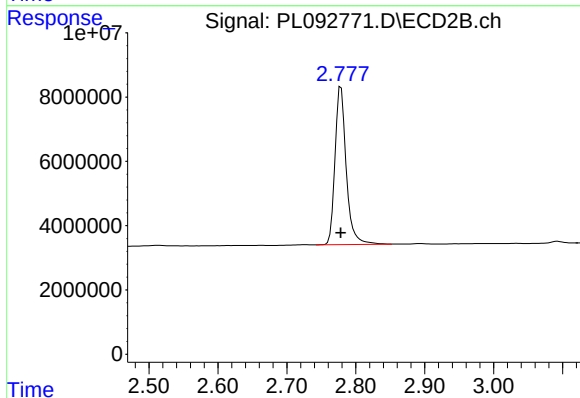


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.000 min
Response: 55641641
Conc: 20.45 ng/ml

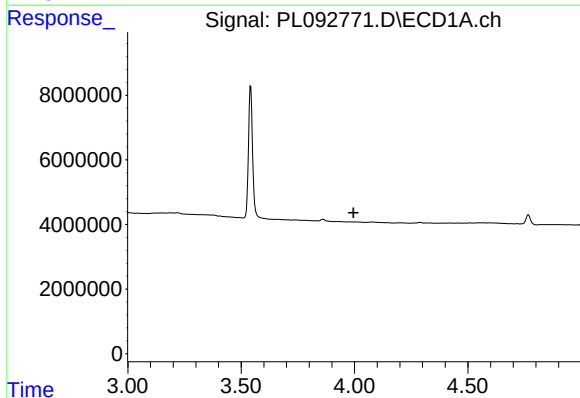


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

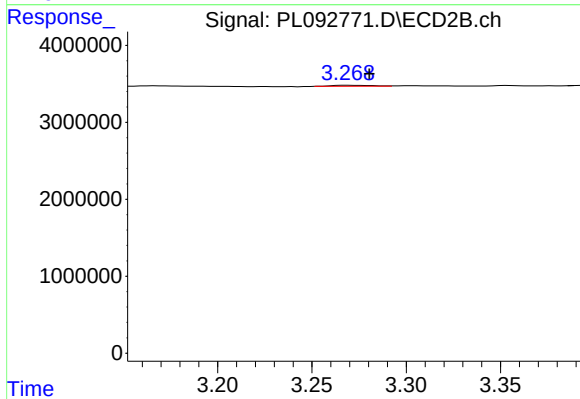

#2 alpha-BHC


R.T.: 3.269 min
Delta R.T.: -0.011 min
Response: 198243
Conc: 0.05 ng/ml

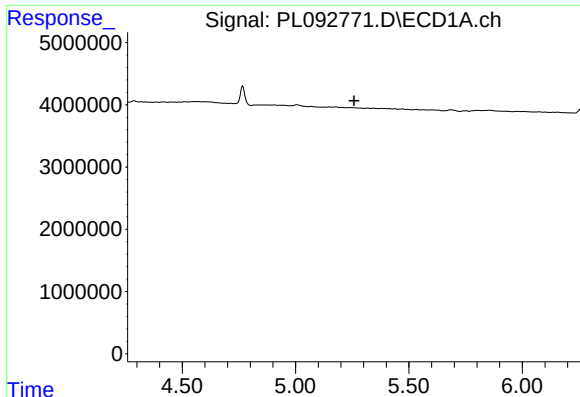

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164557BL

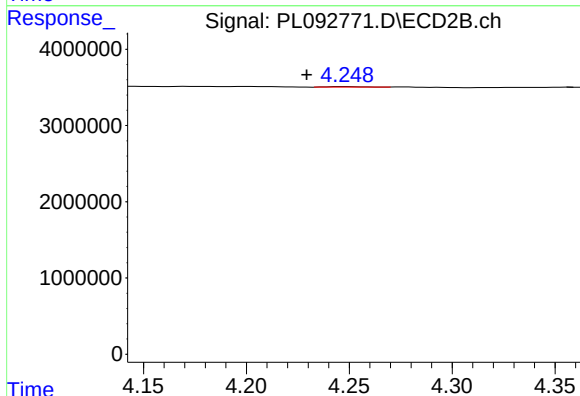


#5 Aldrin

R.T.: 4.248 min
Delta R.T.: 0.019 min
Response: 58742
Conc: 0.02 ng/ml

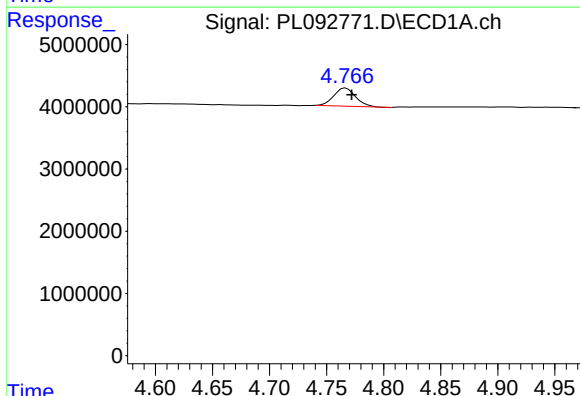


#7 delta-BHC

R.T.: 4.767 min
Delta R.T.: -0.005 min
Response: 3905773
Conc: 1.25 ng/ml

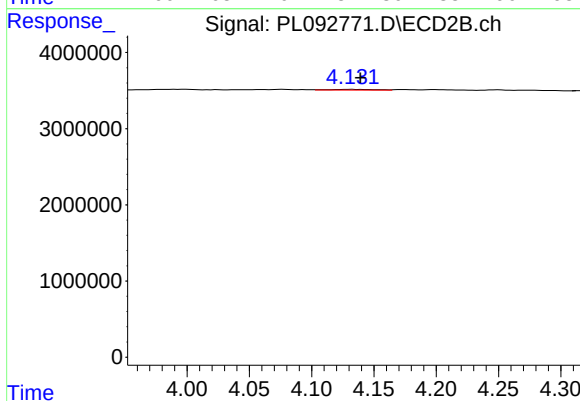

#7 delta-BHC


R.T.: 4.131 min
Delta R.T.: -0.008 min
Response: 229866
Conc: 0.06 ng/ml

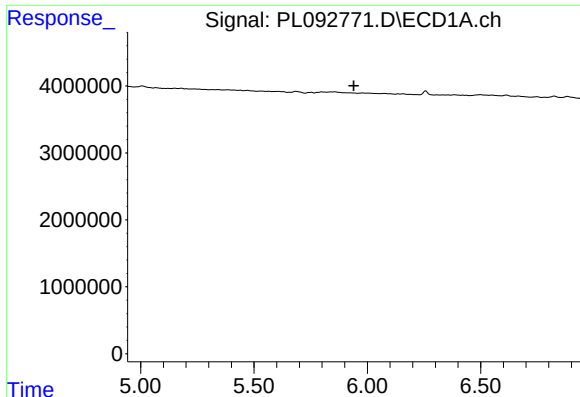

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164557BL

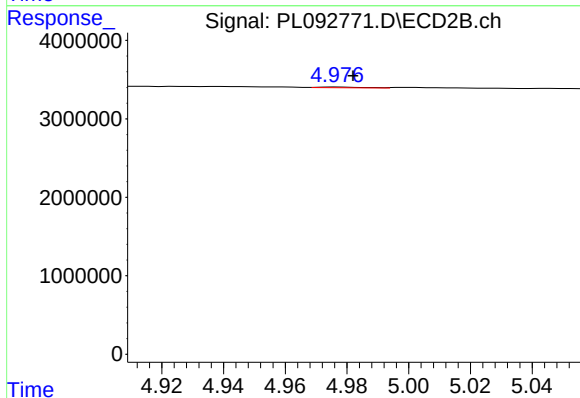


#10 gamma-Chlordane

R.T.: 4.977 min
Delta R.T.: -0.005 min
Response: 92626
Conc: 0.03 ng/ml

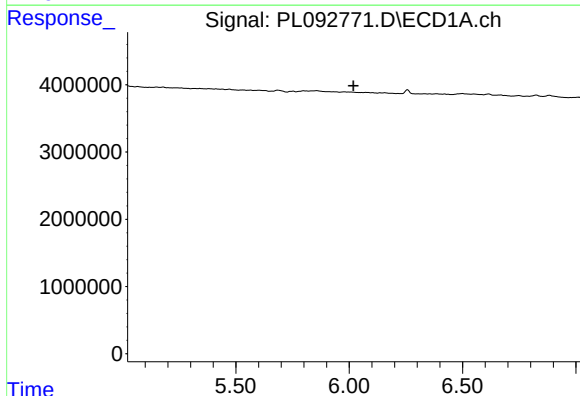


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.019 min
Response: 0
Conc: N.D.

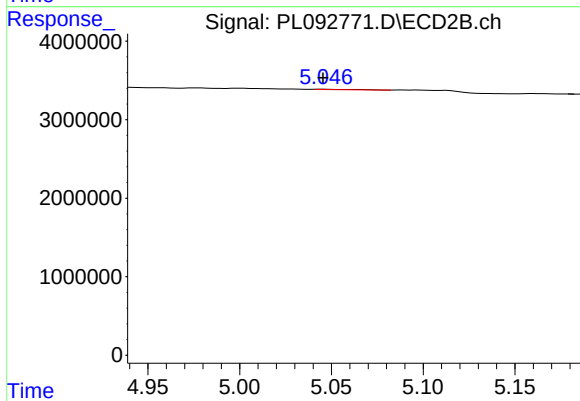

#11 alpha-Chlordane


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 81942
Conc: 0.02 ng/ml

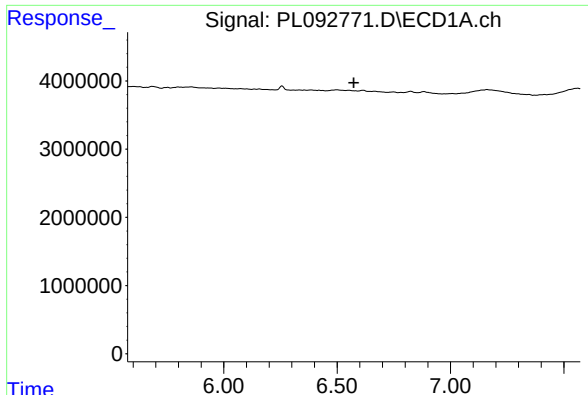

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164557BL

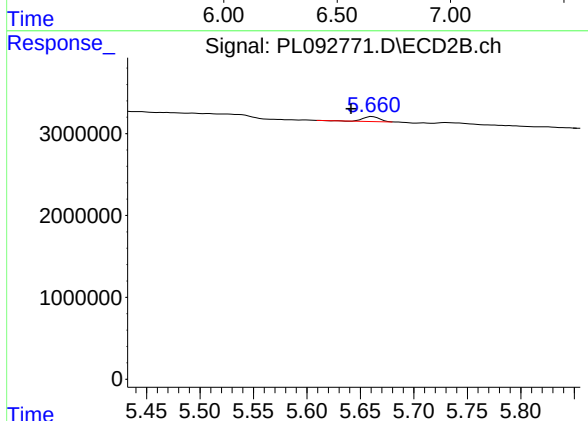


#14 Endrin

R.T.: 5.661 min
Delta R.T.: 0.020 min
Response: 631807
Conc: 0.22 ng/ml

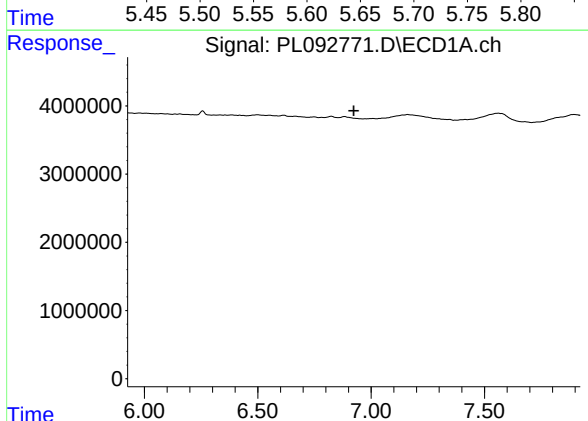


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.924 min
Response: 0
Conc: N.D.

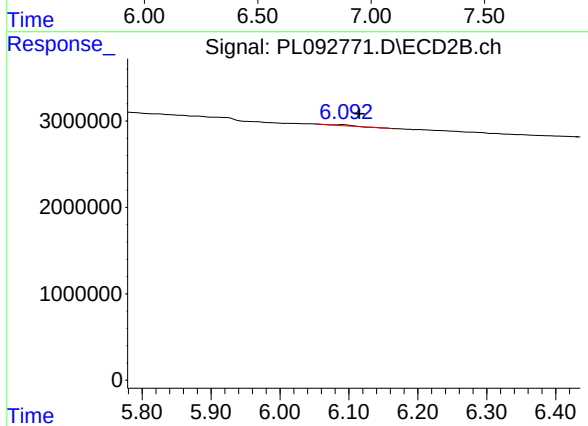

#18 Endrin aldehyde


R.T.: 6.091 min
Delta R.T.: -0.024 min
Response: 185598
Conc: 0.08 ng/ml

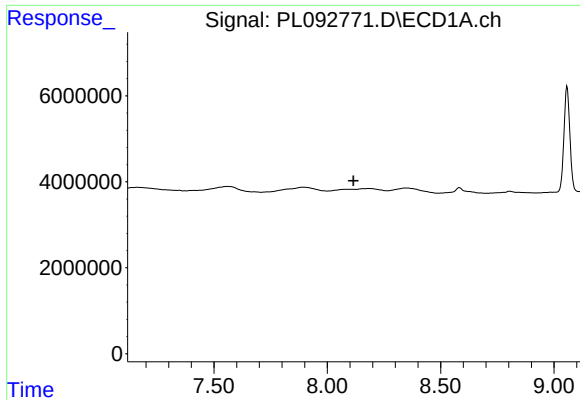

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164557BL

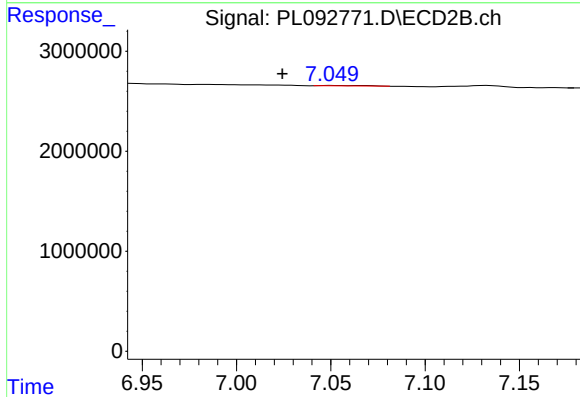


#22 Mirex

R.T.: 7.051 min
Delta R.T.: 0.027 min
Response: 53200
Conc: 0.02 ng/ml

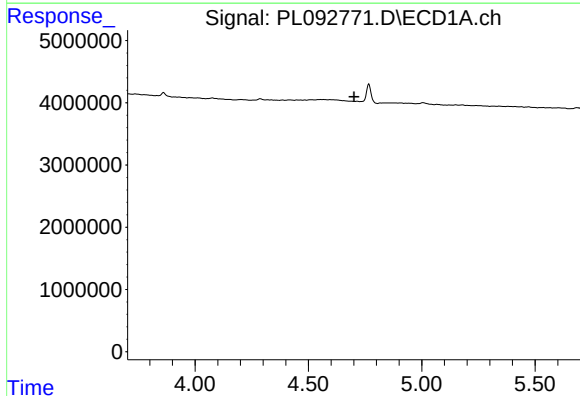


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.702 min
Response: 0
Conc: N.D.

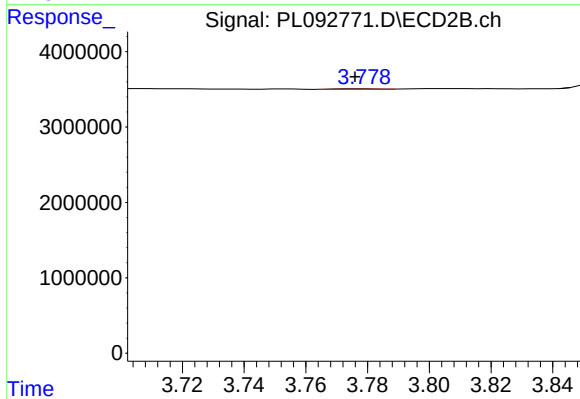

#23 Chlordane-1


R.T.: 3.777 min
Delta R.T.: 0.001 min
Response: 73483
Conc: 0.69 ng/ml

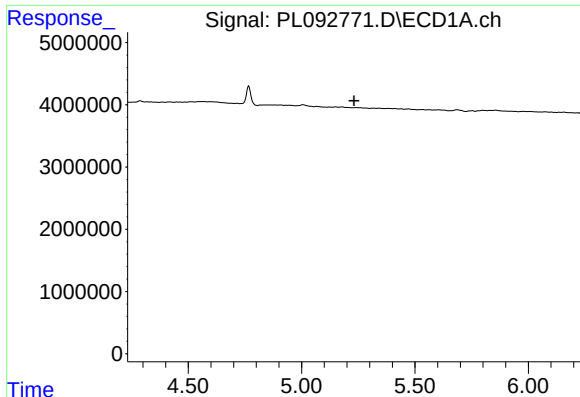

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164557BL

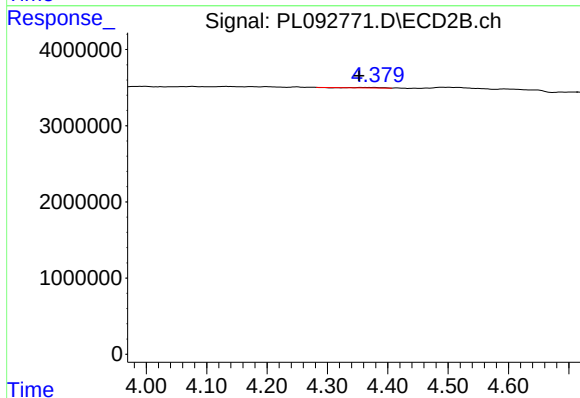


#24 Chlordane-2

R.T.: 4.356 min
Delta R.T.: 0.004 min
Response: 176818
Conc: 1.43 ng/ml

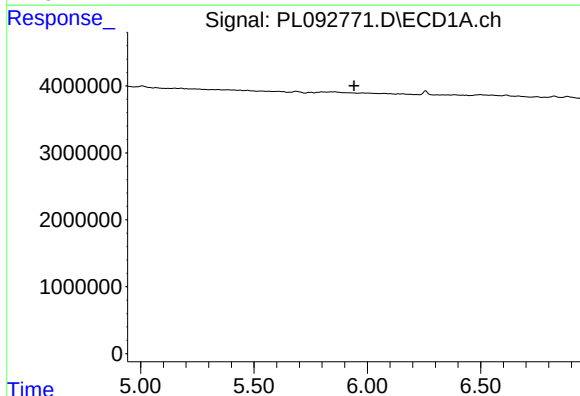


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

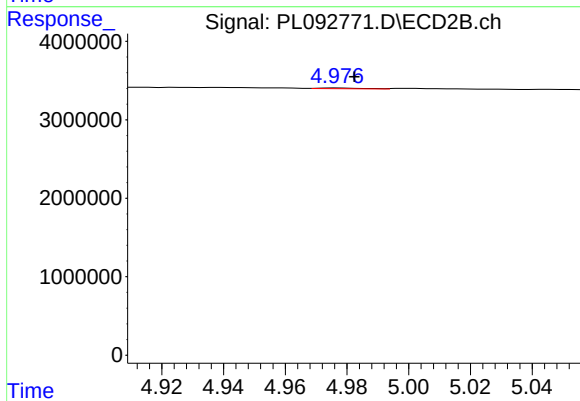

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: -0.005 min
Response: 92626
Conc: 0.26 ng/ml

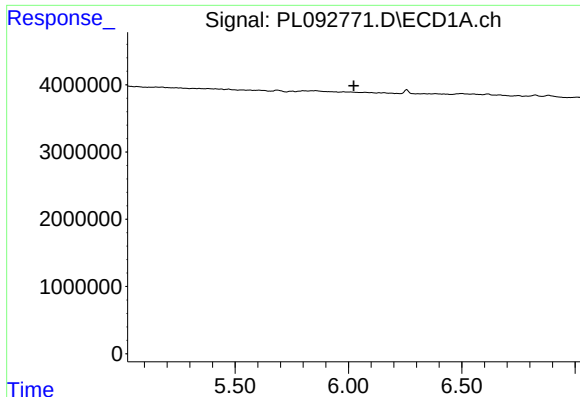

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164557BL

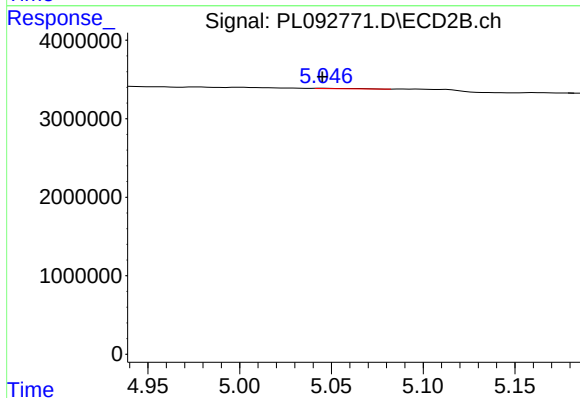


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.001 min
Response: 81942
Conc: 0.23 ng/ml

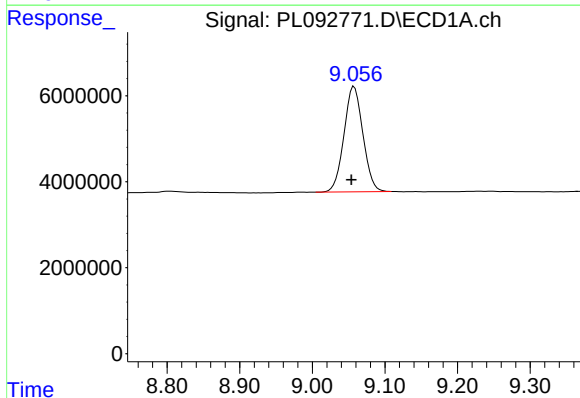

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.004 min
Response: 44493609
Conc: 23.12 ng/ml

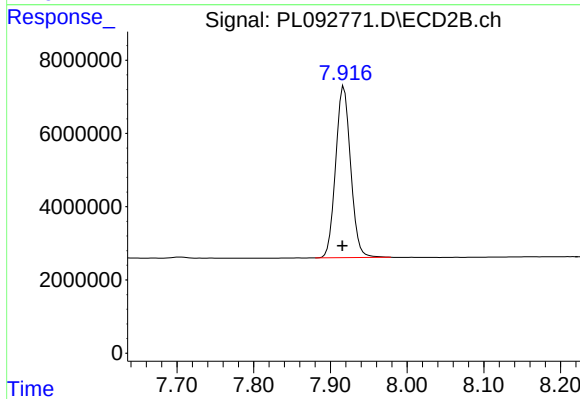

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.002 min
Response: 63486739
Conc: 23.26 ng/ml