

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
 Data File : PL092761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 14:35
 Operator : AR\AJ
 Sample : PB164399BS
 Misc : CH/BS
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164399BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:32:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.778	46199718	59512935	18.855	21.870
28) SA Decachlor...	9.058	7.918	36761827	52640779	19.102	19.288
Target Compounds						
23) Chlordane-1	4.704	3.776	21920530	19933686	199.296	187.781
24) Chlordane-2	5.234	4.353	22483262	23615337	196.165	190.672
25) Chlordane-3	5.944	4.983	74421234	67494441	190.670	186.098
26) Chlordane-4	6.025	5.046	89381625	65477405	186.989	187.178
27) Chlordane-5	6.874	5.942	18777403	23547460	198.366	185.694



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
Data File : PL092761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 14:35
Operator : AR\AJ
Sample : PB164399BS
Misc : CH/BS
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164399BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:32:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

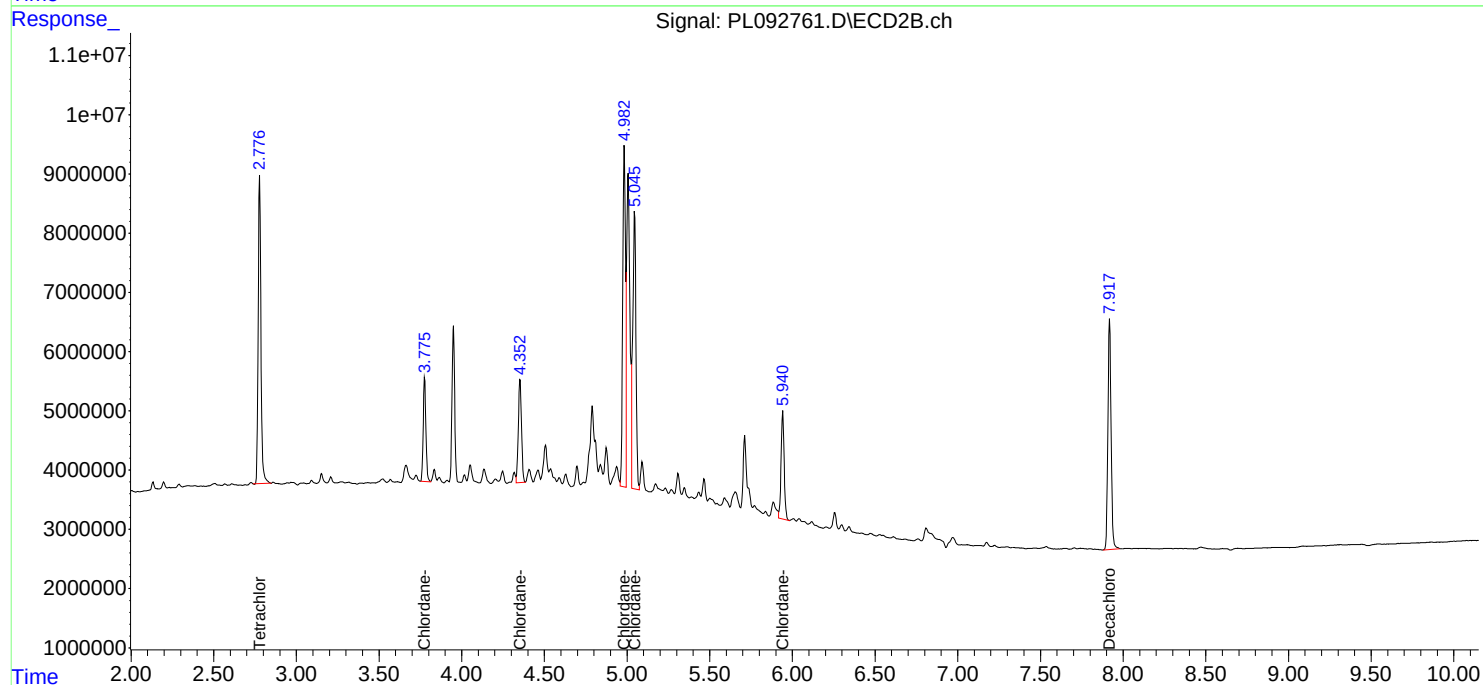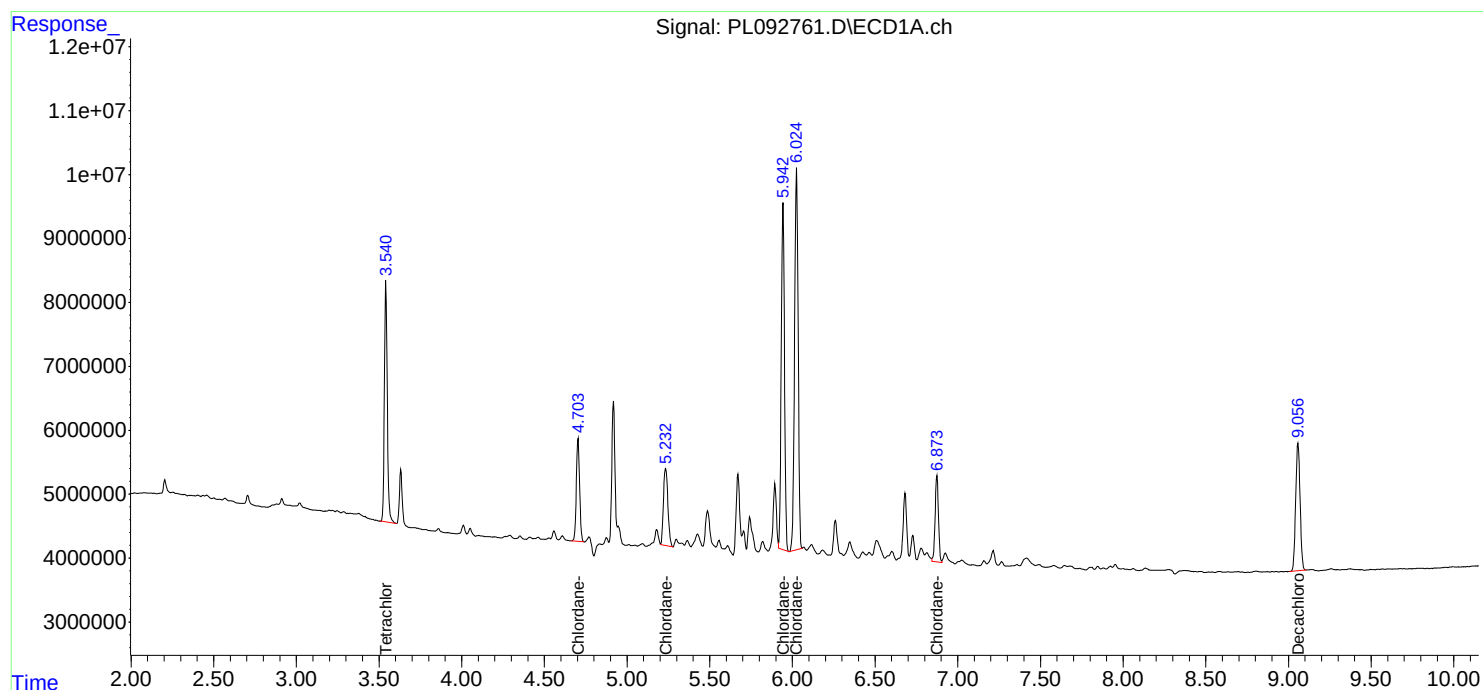


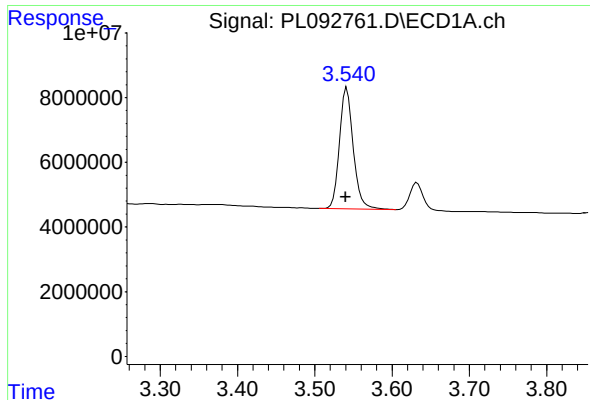

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 46199718
Conc: 18.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164399BS

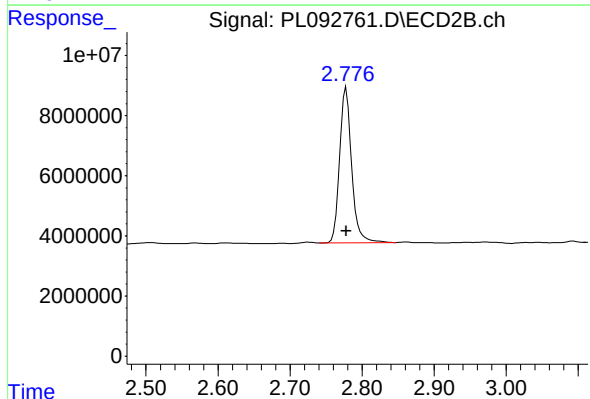


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 59512935
Conc: 21.87 ng/ml

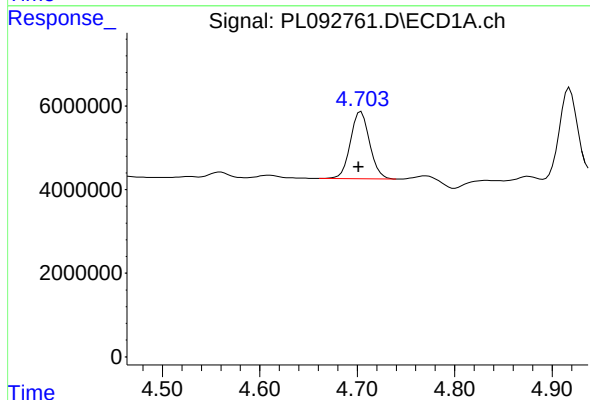


#23 Chlordane-1

R.T.: 4.704 min
Delta R.T.: 0.002 min
Response: 21920530
Conc: 199.30 ng/ml

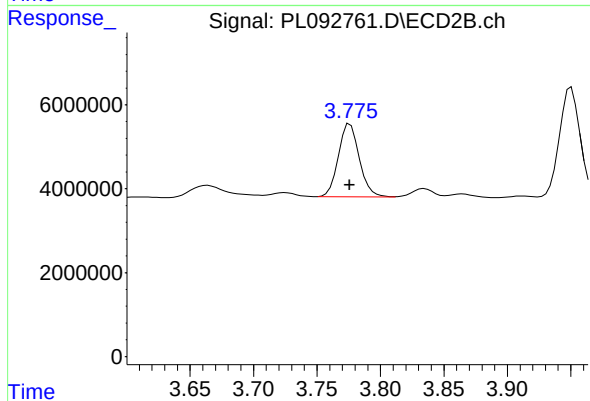

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 19933686
Conc: 187.78 ng/ml

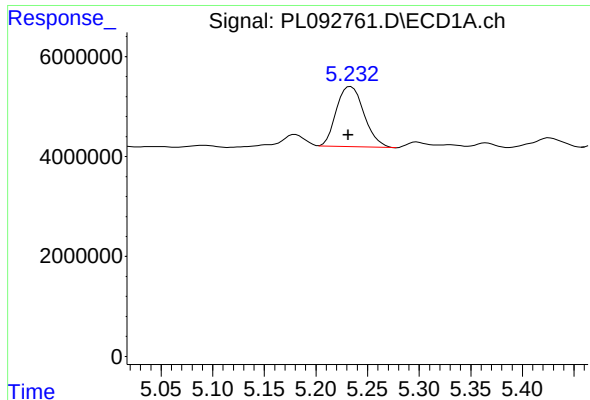

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.003 min
Response: 22483262
Conc: 196.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164399BS

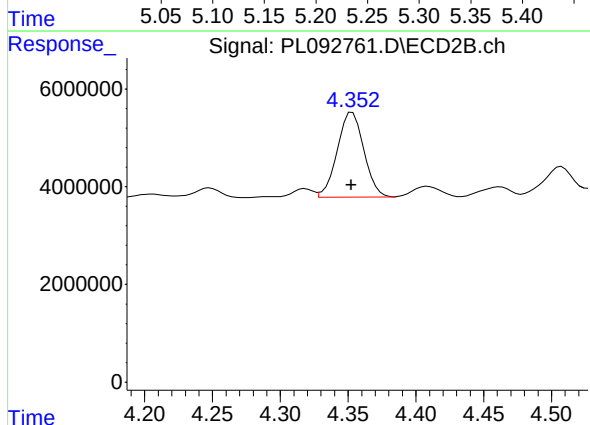


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 23615337
Conc: 190.67 ng/ml

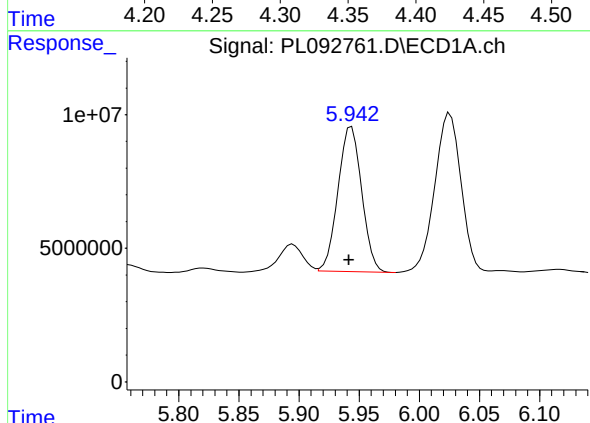


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.002 min
Response: 74421234
Conc: 190.67 ng/ml

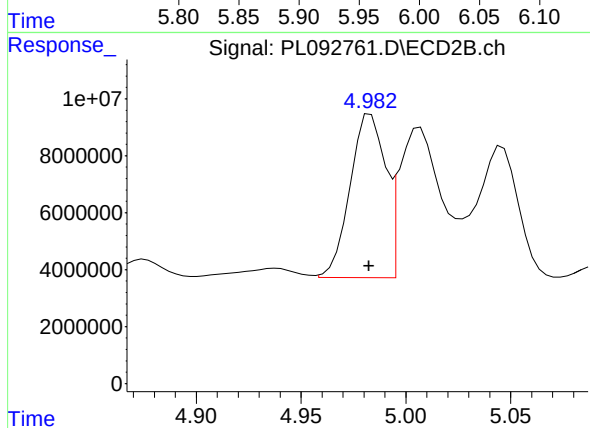

#25 Chlordane-3


R.T.: 4.983 min
Delta R.T.: 0.001 min
Response: 67494441
Conc: 186.10 ng/ml

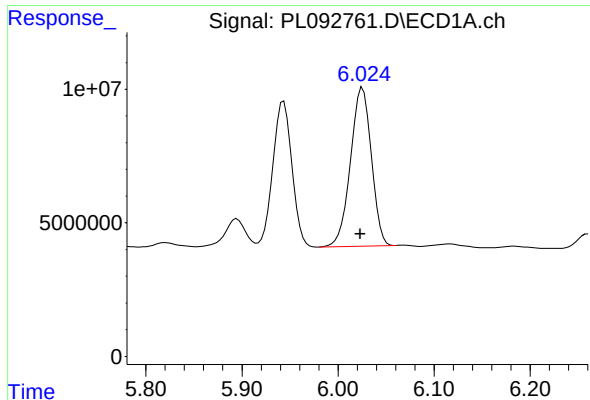

#26 Chlordane-4


R.T.: 6.025 min
Delta R.T.: 0.002 min
Response: 89381625
Conc: 186.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164399BS

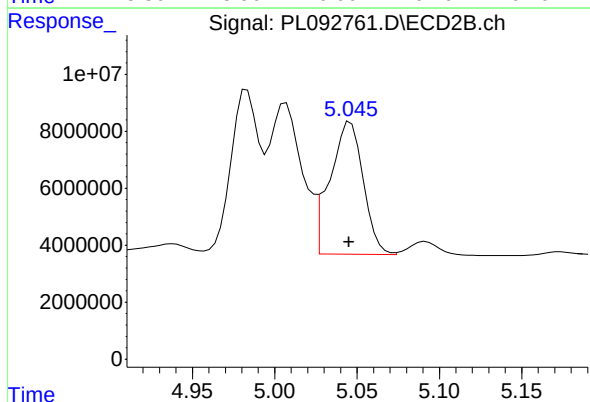


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 65477405
Conc: 187.18 ng/ml

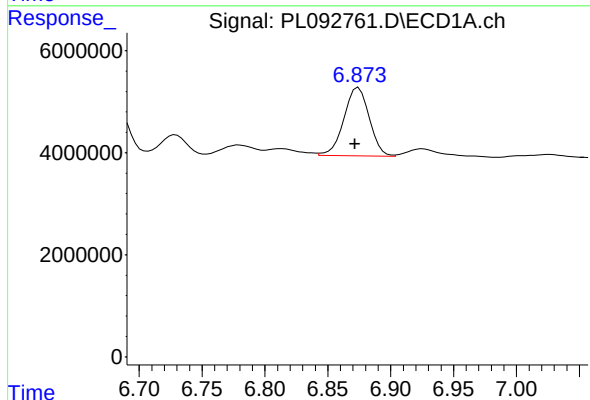


#27 Chlordane-5

R.T.: 6.874 min
Delta R.T.: 0.003 min
Response: 18777403
Conc: 198.37 ng/ml

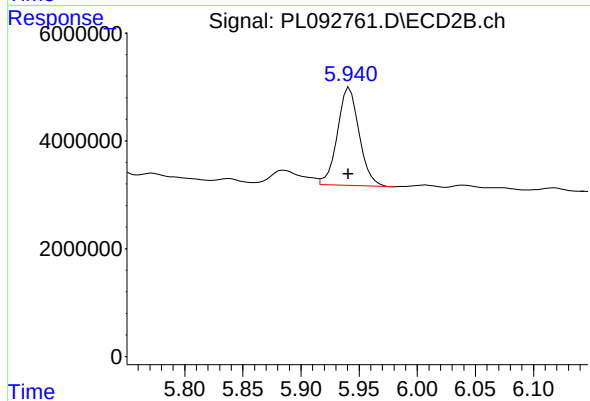

#27 Chlordane-5


R.T.: 5.942 min
Delta R.T.: 0.001 min
Response: 23547460
Conc: 185.69 ng/ml

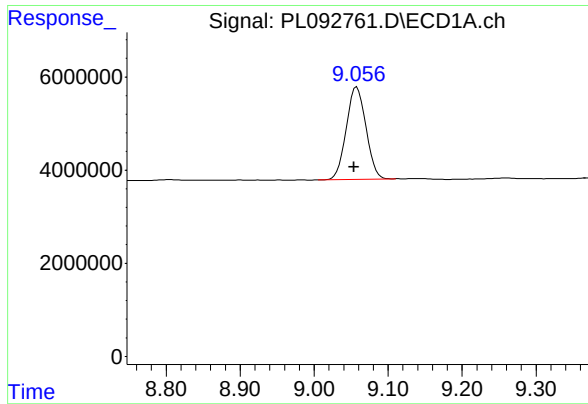

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.004 min
Response: 36761827
Conc: 19.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164399BS

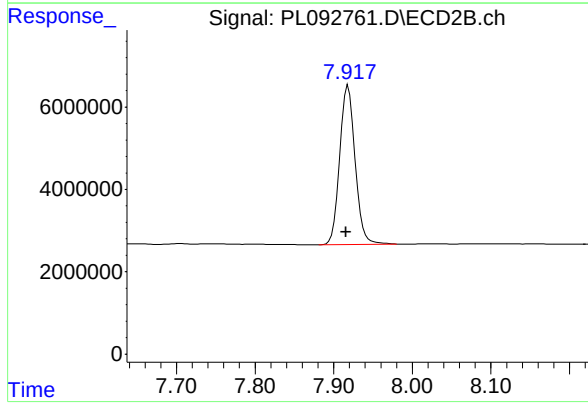

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.003 min
Response: 52640779
Conc: 19.29 ng/ml