

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
 Data File : PL092769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 18:34
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:20:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.778	111.3E6	153.3E6	45.433	56.340
28)	SA Decachlor...	9.058	7.918	86124201	129.6E6	44.750	47.499
Target Compounds							
23)	Chlordane-1	4.704	3.776	51834755	51274330	471.269	483.018
24)	Chlordane-2	5.234	4.353	52989954	59599410	462.335	481.211
25)	Chlordane-3	5.944	4.984	177.9E6	178.0E6	455.780	490.720
26)	Chlordane-4	6.026	5.046	219.0E6	169.2E6	458.204	483.797
27)	Chlordane-5	6.875	5.941	43228471	60847208	456.670	479.837



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
Data File : PL092769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 18:34
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:20:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

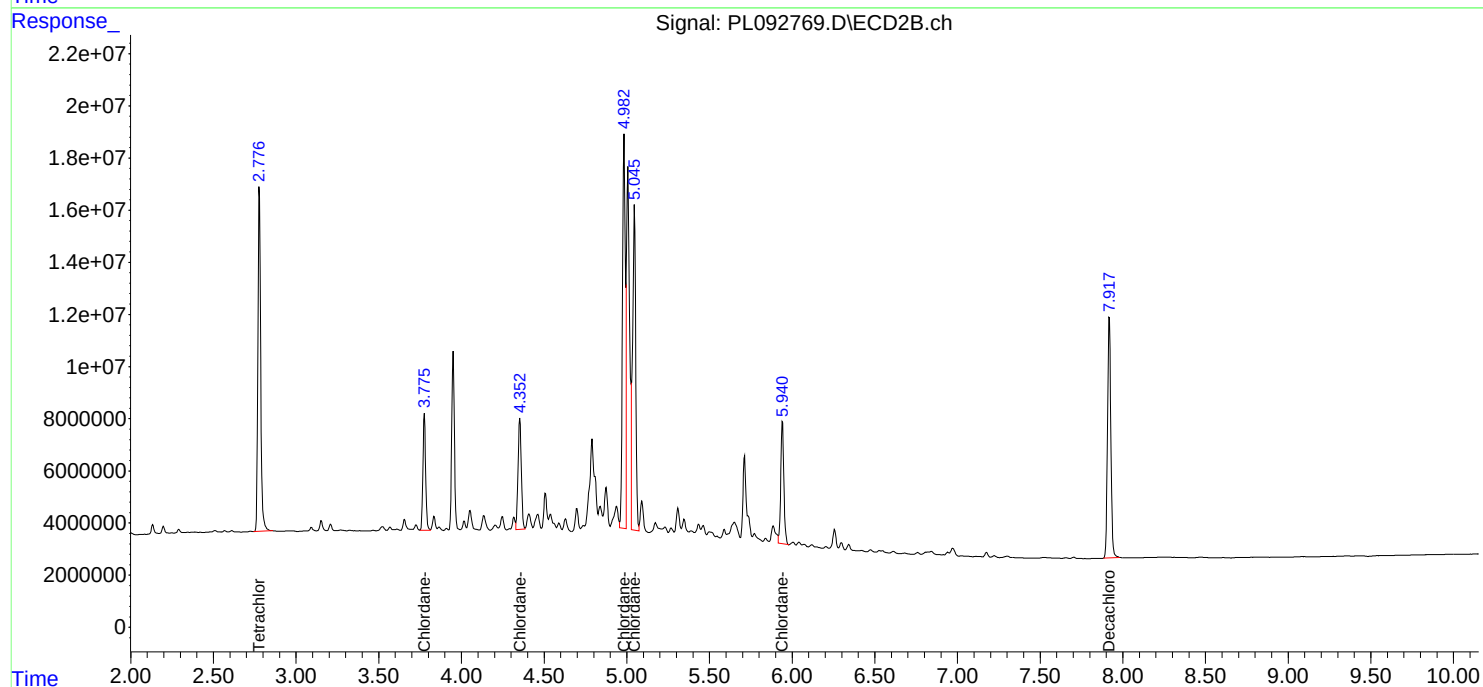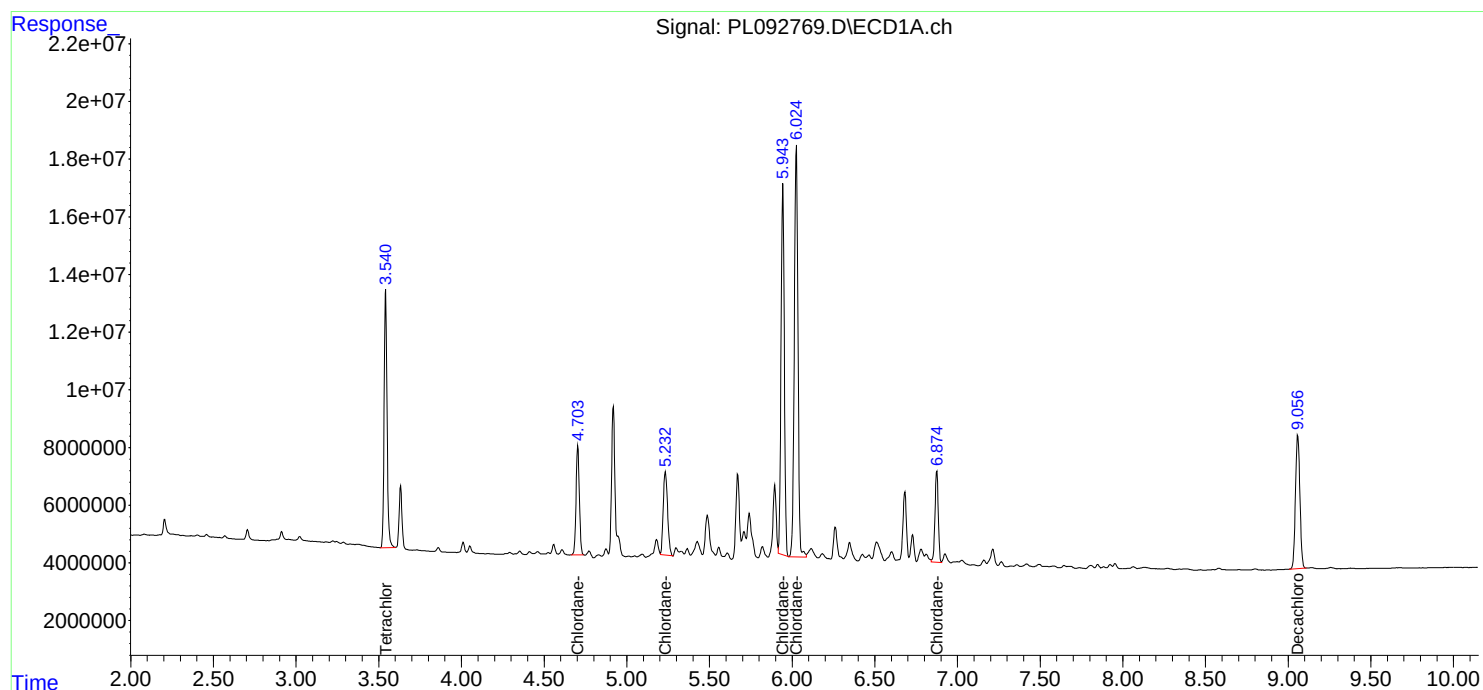


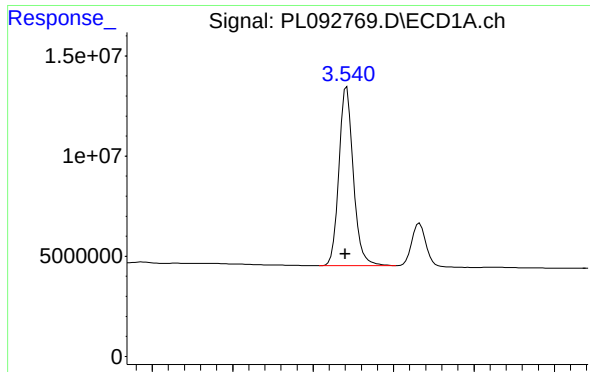

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 111322239
Conc: 45.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

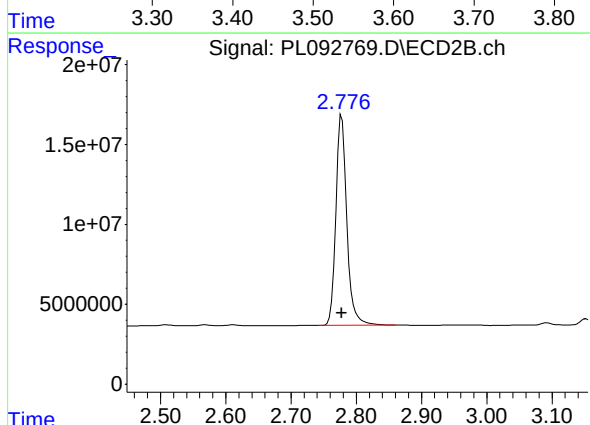


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 153310294
Conc: 56.34 ng/ml

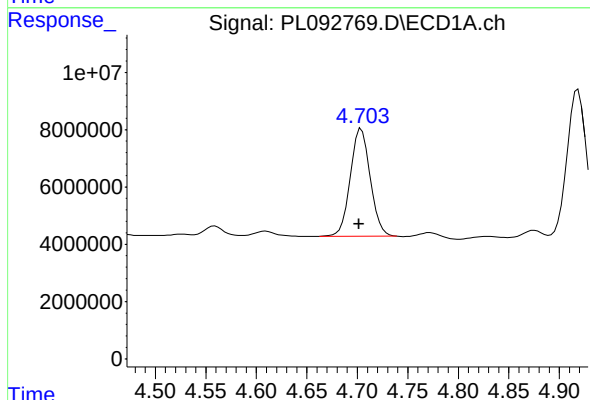


#23 Chlordane-1

R.T.: 4.704 min
Delta R.T.: 0.002 min
Response: 51834755
Conc: 471.27 ng/ml

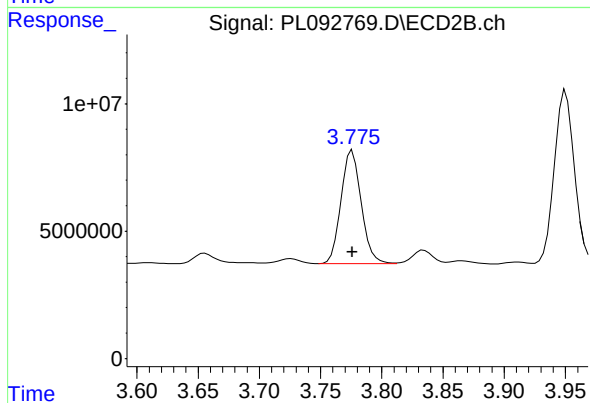

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 51274330
Conc: 483.02 ng/ml

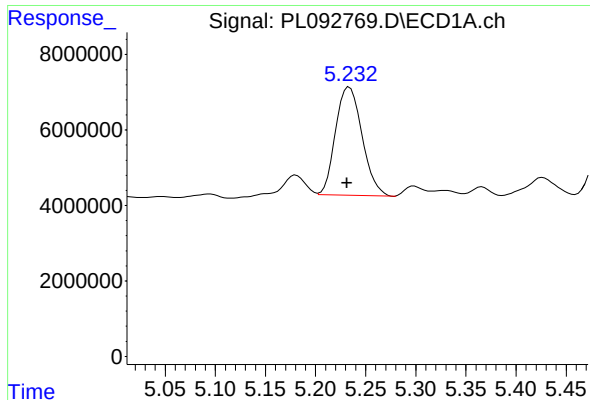

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.002 min
Response: 52989954
Conc: 462.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

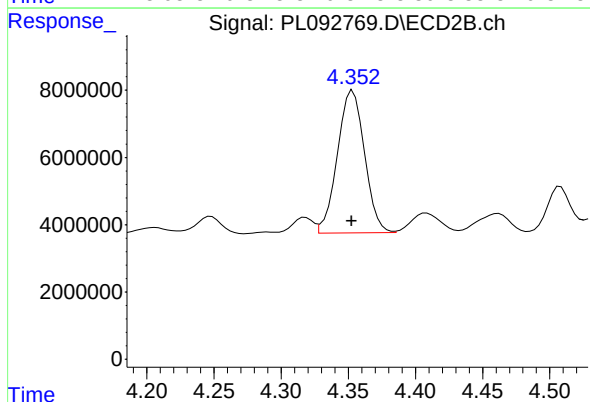


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 59599410
Conc: 481.21 ng/ml

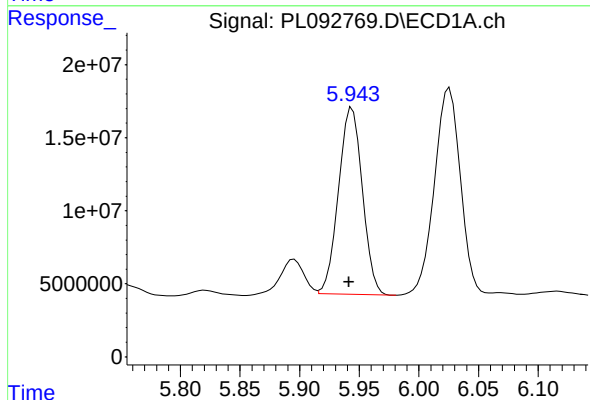


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.003 min
Response: 177897799
Conc: 455.78 ng/ml

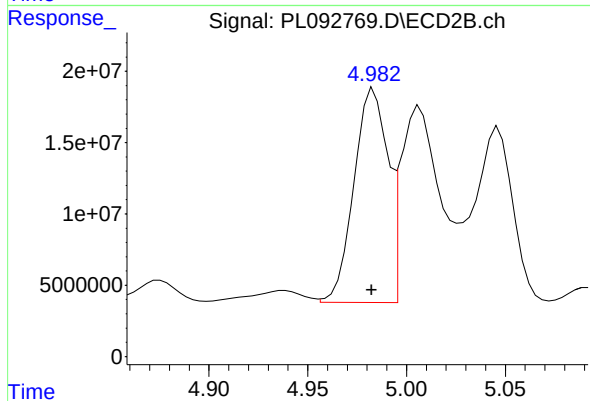

#25 Chlordane-3


R.T.: 4.984 min
Delta R.T.: 0.001 min
Response: 177975674
Conc: 490.72 ng/ml

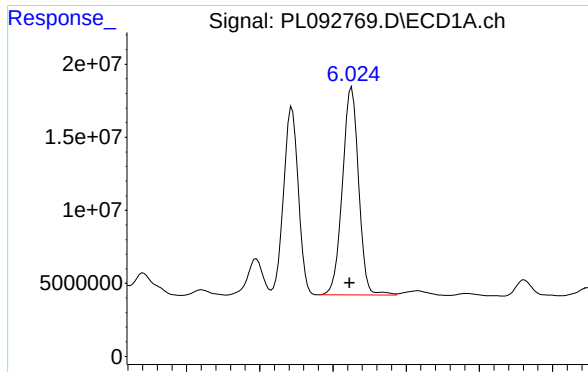

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.003 min
Response: 219024132
Conc: 458.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

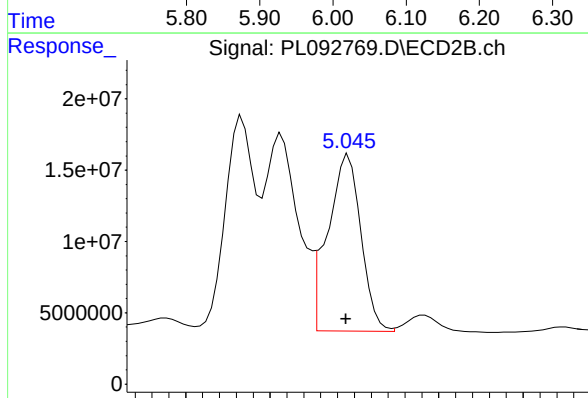


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.001 min
Response: 169238624
Conc: 483.80 ng/ml

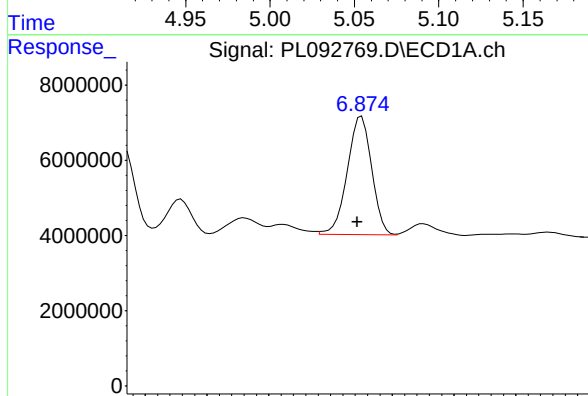


#27 Chlordane-5

R.T.: 6.875 min
Delta R.T.: 0.004 min
Response: 43228471
Conc: 456.67 ng/ml

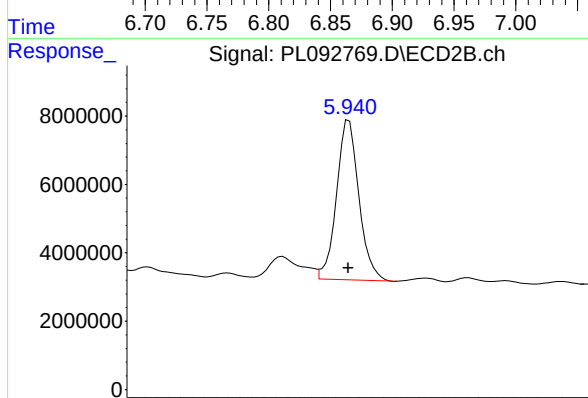

#27 Chlordane-5


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 60847208
Conc: 479.84 ng/ml

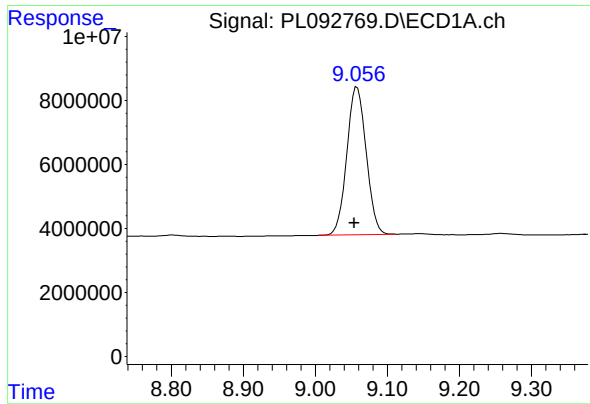

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.004 min
Response: 86124201
Conc: 44.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

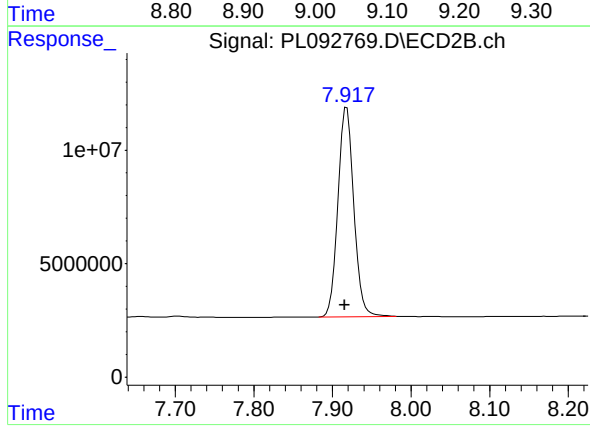

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.002 min
Response: 129634871
Conc: 47.50 ng/ml