

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
 Data File : PL092777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 20:25
 Operator : AR\AJ
 Sample : P4643-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/01/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:56:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.779	51410873	57229667	20.982m	21.031
28) SA Decachlor...	9.059	7.917	36141801	46213410	18.779	16.933m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103124\
Data File : PL092777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 20:25
Operator : AR\AJ
Sample : P4643-09
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-9


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/01/2024
Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:56:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

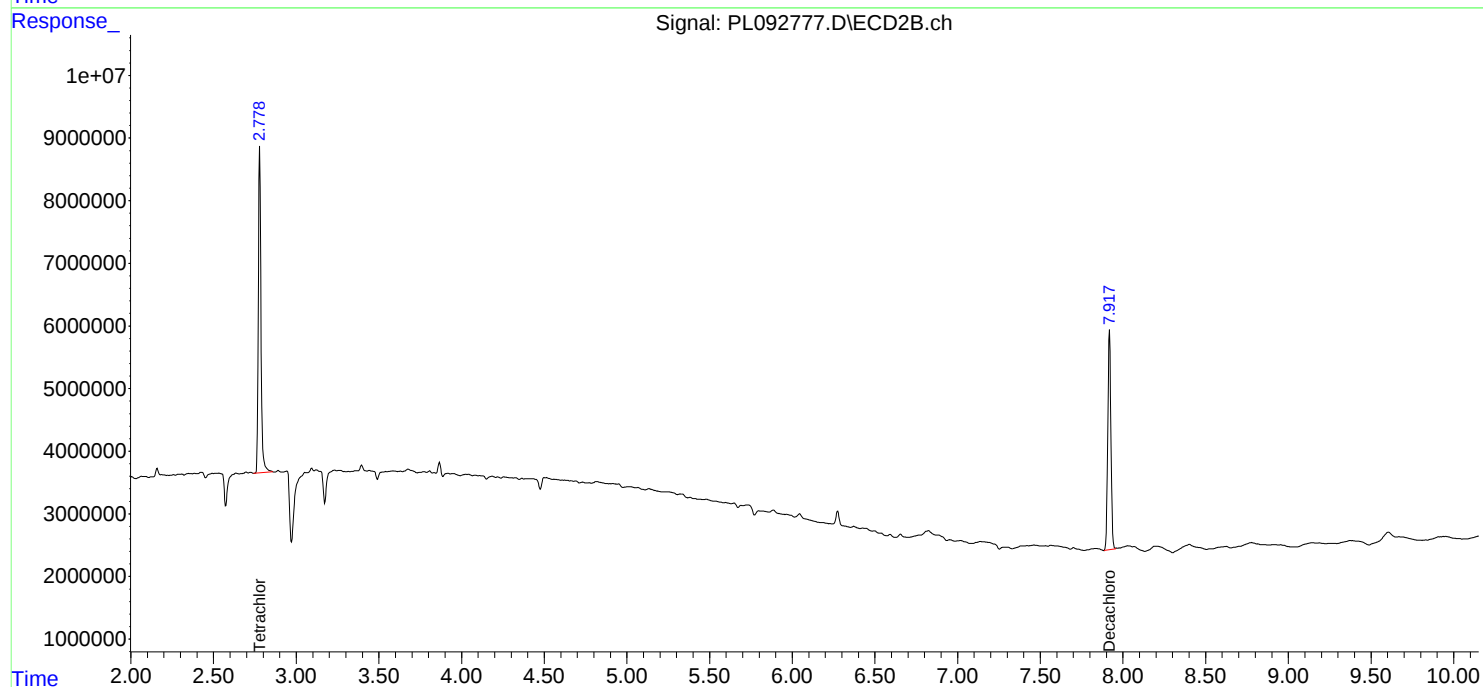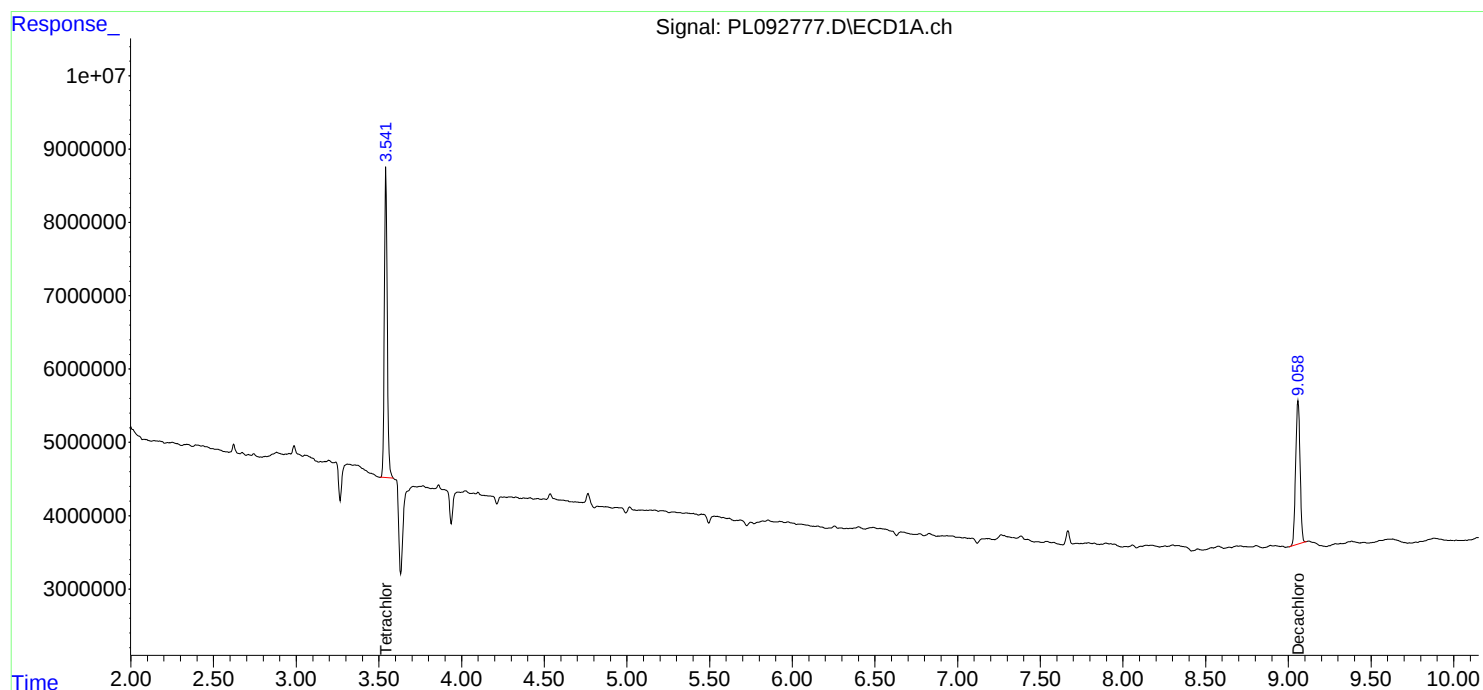

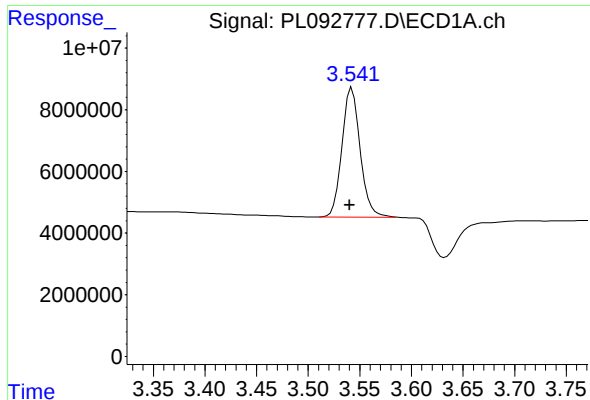


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.001 min
Response: 51410873
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/01/2024
Supervised By :Ankita Jodhani 11/04/2024

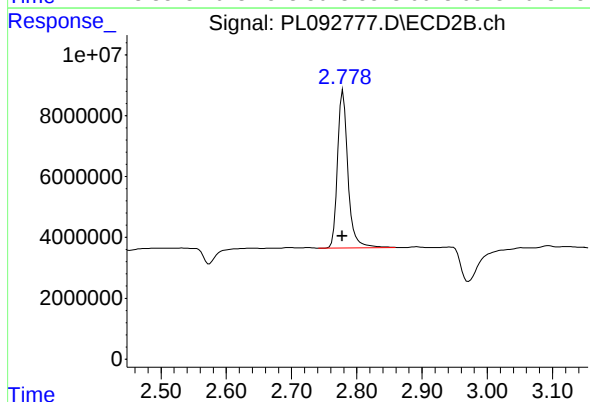


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.001 min
Response: 57229667
Conc: 21.03 ng/ml

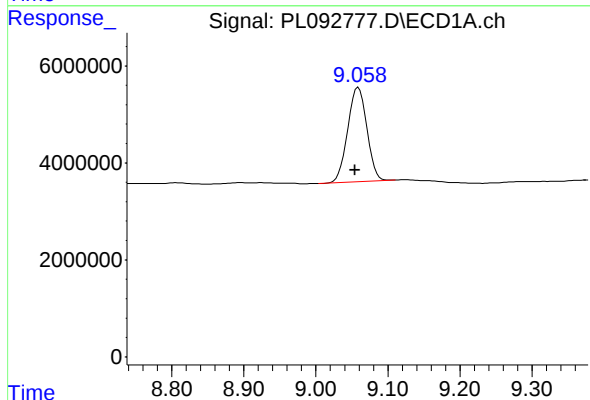

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.005 min
Response: 36141801
Conc: 18.78 ng/ml

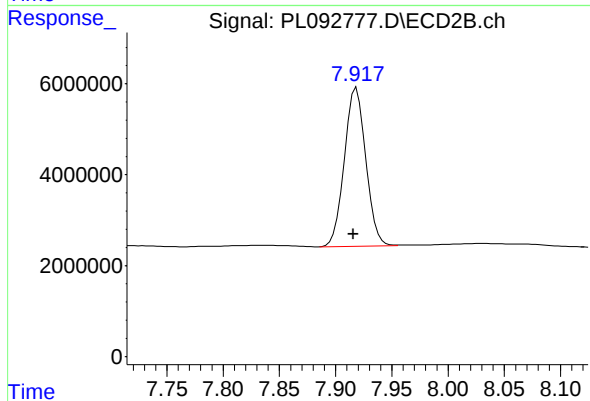

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: 0.001 min
Response: 46213410
Conc: 16.93 ng/ml m