

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
 Data File : PL097702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 12:03
 Operator : AR\AJ
 Sample : Q3488-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:53:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	2.818	44373741	55661655	10.844	9.248
28)	SA Decachlor...	9.020f	7.998f	35064499	40061579	11.786	7.495 #
Target Compounds							
15)	B Endosulfa...	0.000	5.963f	0	5325766	N.D.	0.758 #
27)	Chlordane-5	0.000	5.963f	0	5325766	N.D.	17.742 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
Data File : PL097702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 12:03
Operator : AR\AJ
Sample : Q3488-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:53:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

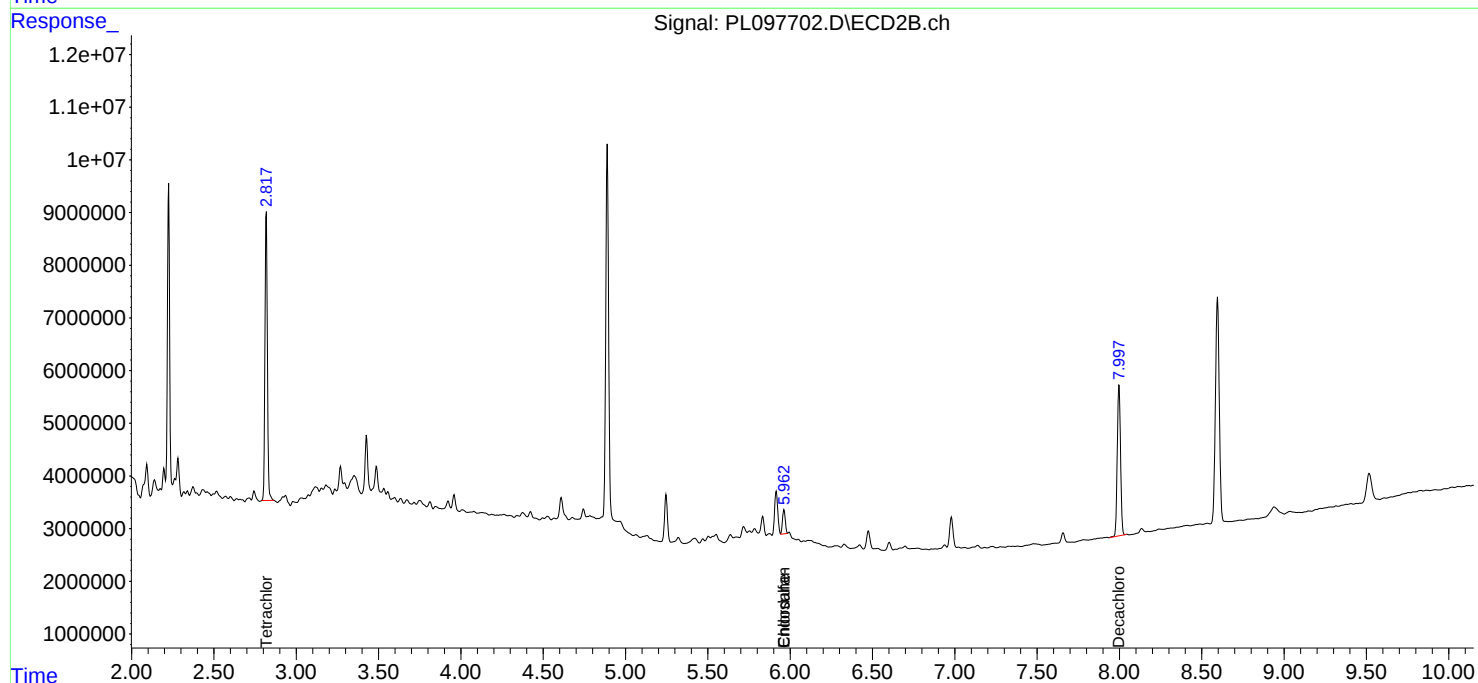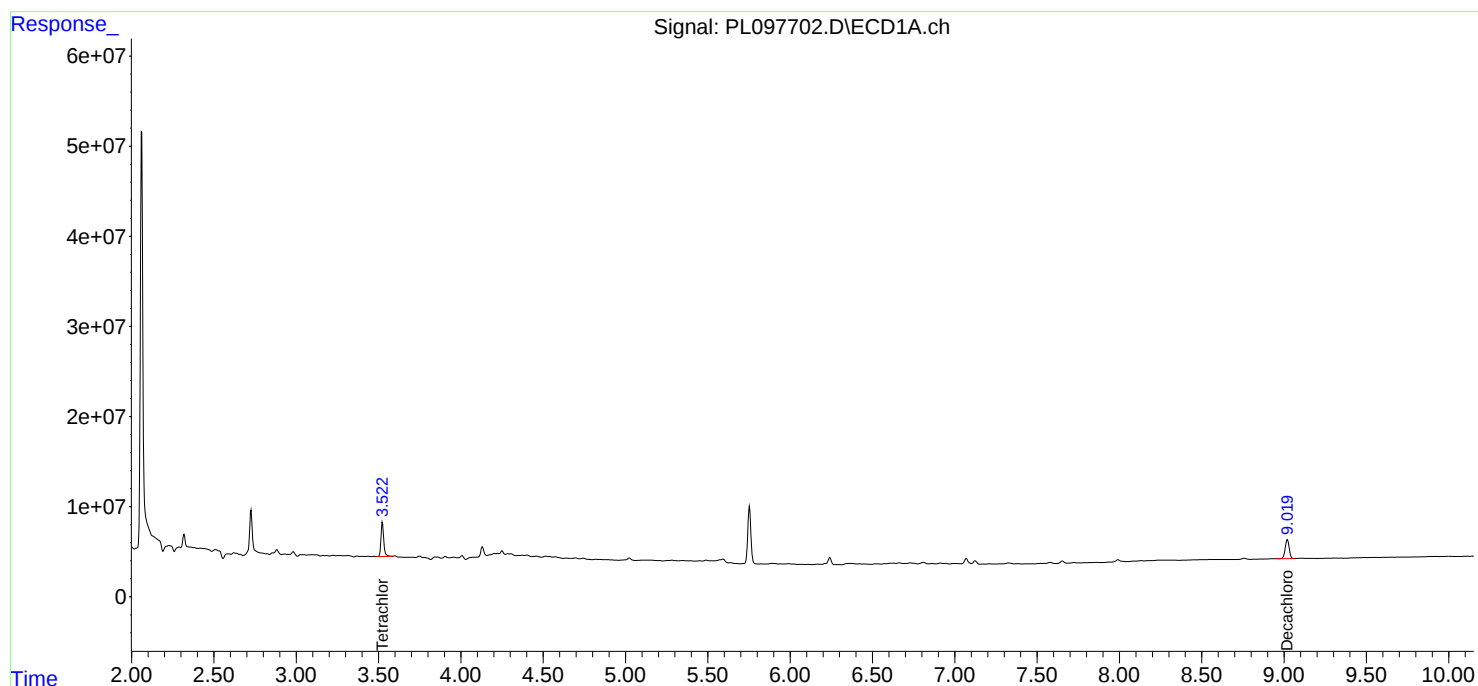


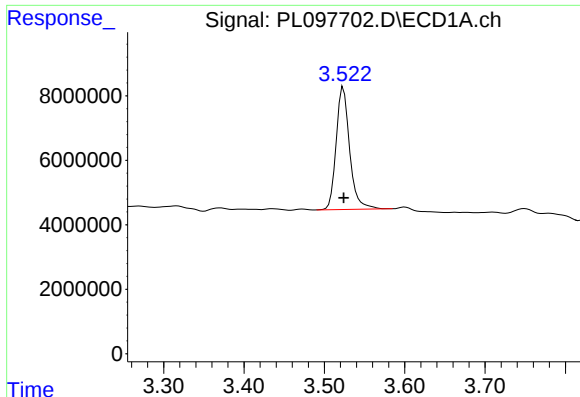

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 44373741
Conc: 10.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

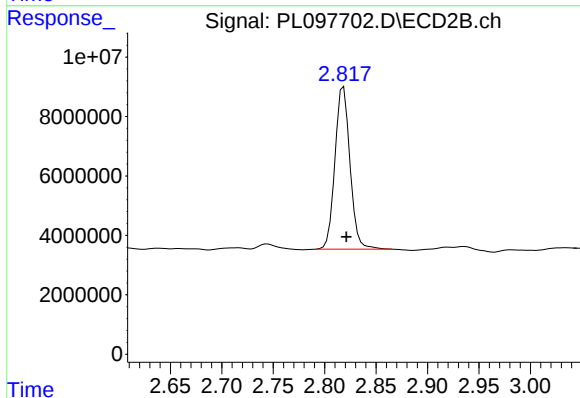


#1 Tetrachloro-m-xylene

R.T.: 2.818 min
Delta R.T.: -0.003 min
Response: 55661655
Conc: 9.25 ng/ml

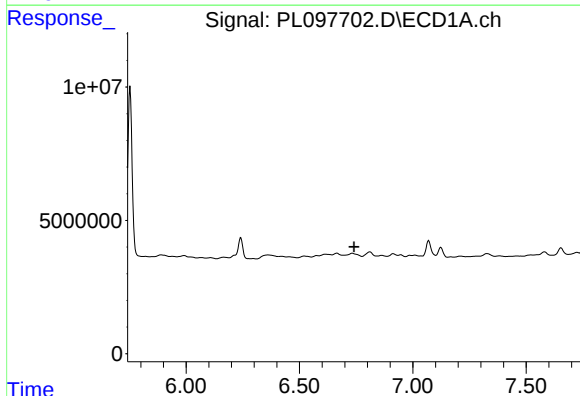


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.741 min
Response: 0
Conc: N.D.

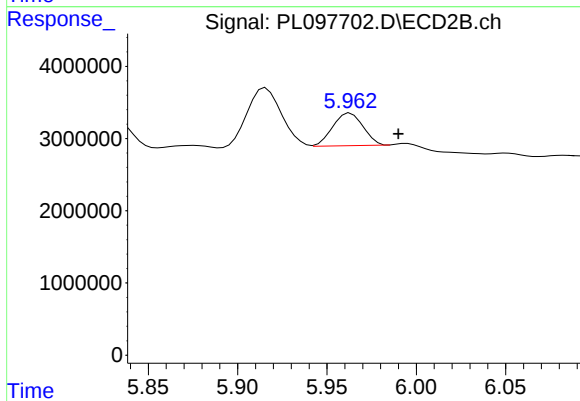

#15 Endosulfan II


R.T.: 5.963 min
Delta R.T.: -0.027 min
Response: 5325766
Conc: 0.76 ng/ml

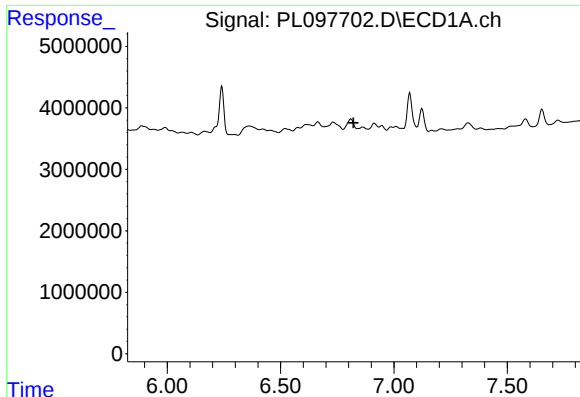

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.822 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

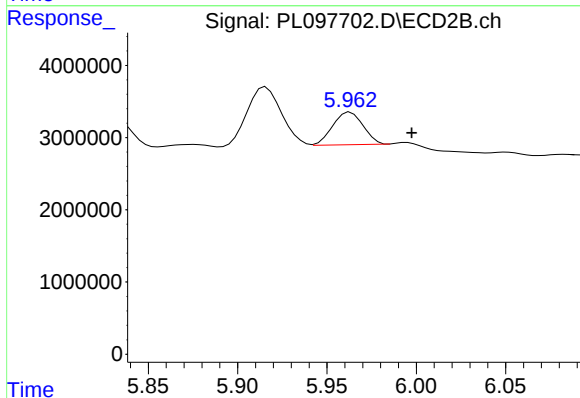


#27 Chlordane-5

R.T.: 5.963 min
Delta R.T.: -0.034 min
Response: 5325766
Conc: 17.74 ng/ml

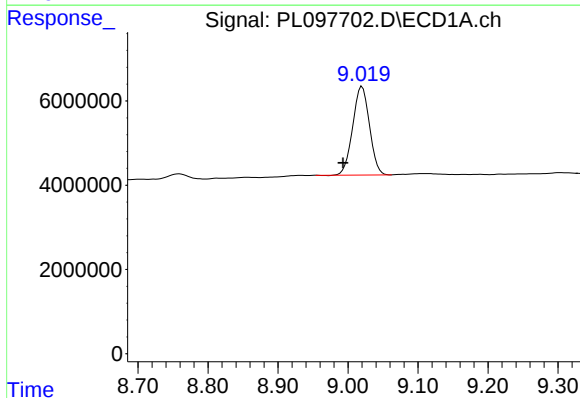

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.027 min
Response: 35064499
Conc: 11.79 ng/ml

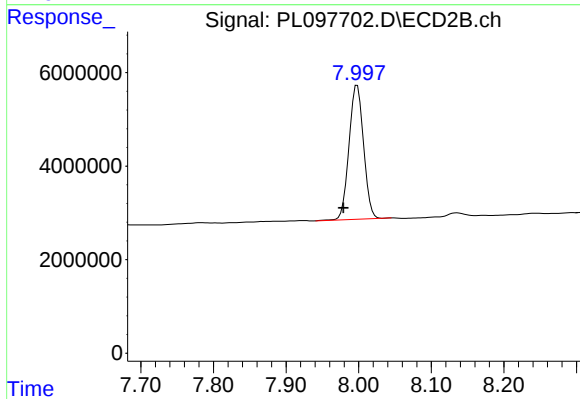

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: 0.019 min
Response: 40061579
Conc: 7.50 ng/ml