

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
 Data File : PL097703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 12:17
 Operator : AR\AJ
 Sample : Q3490-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:53:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.819	0	8550373	N.D.	1.421 #
Target Compounds						
13) MA Dieldrin	0.000	5.394f	0	13904446	N.D.	1.730 #
16) A 4,4'-DDD	0.000	5.818f	0	11586141	N.D.	1.807 #
23) Chlordane-1	0.000	3.814	0	3823540	N.D.	15.307 #
24) Chlordane-2	0.000	4.381f	0	4994130	N.D.	17.525 #
27) Chlordane-5	6.802f	0.000	10685195	0	63.017	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
Data File : PL097703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 12:17
Operator : AR\AJ
Sample : Q3490-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:53:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

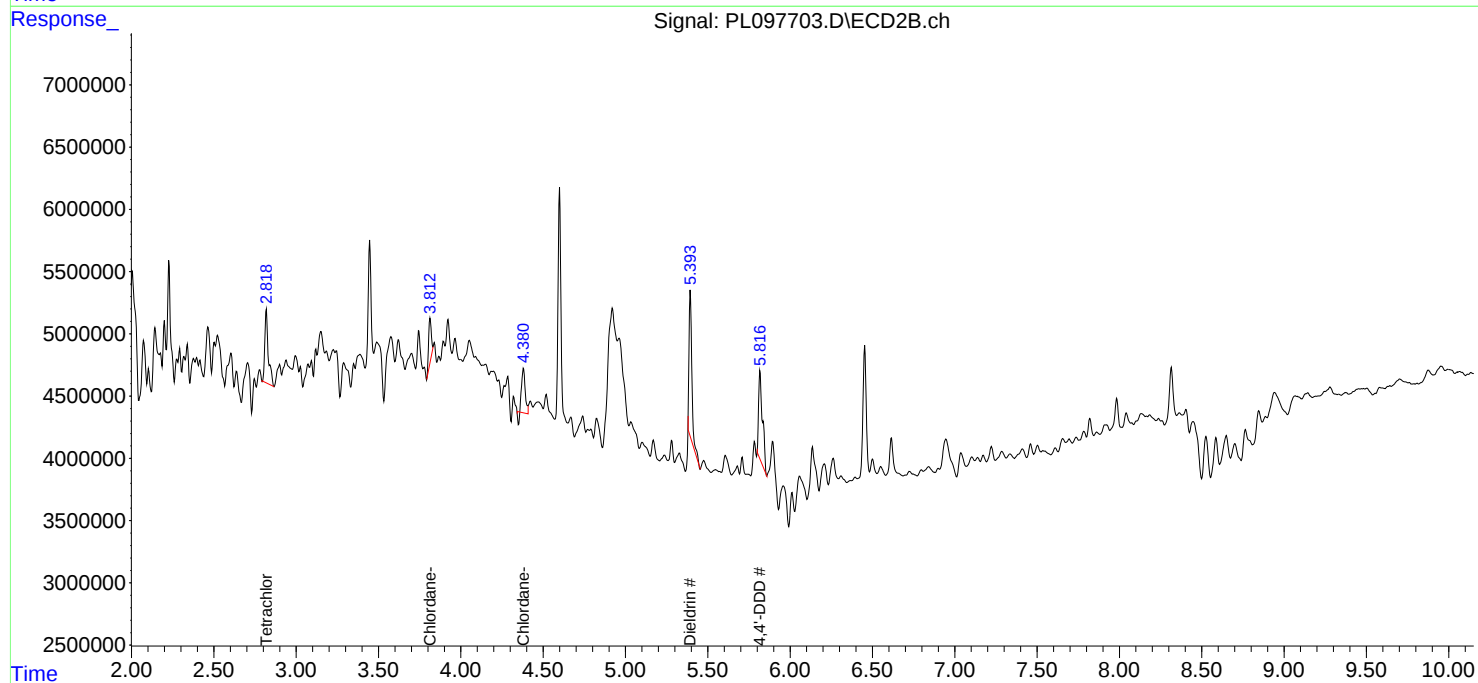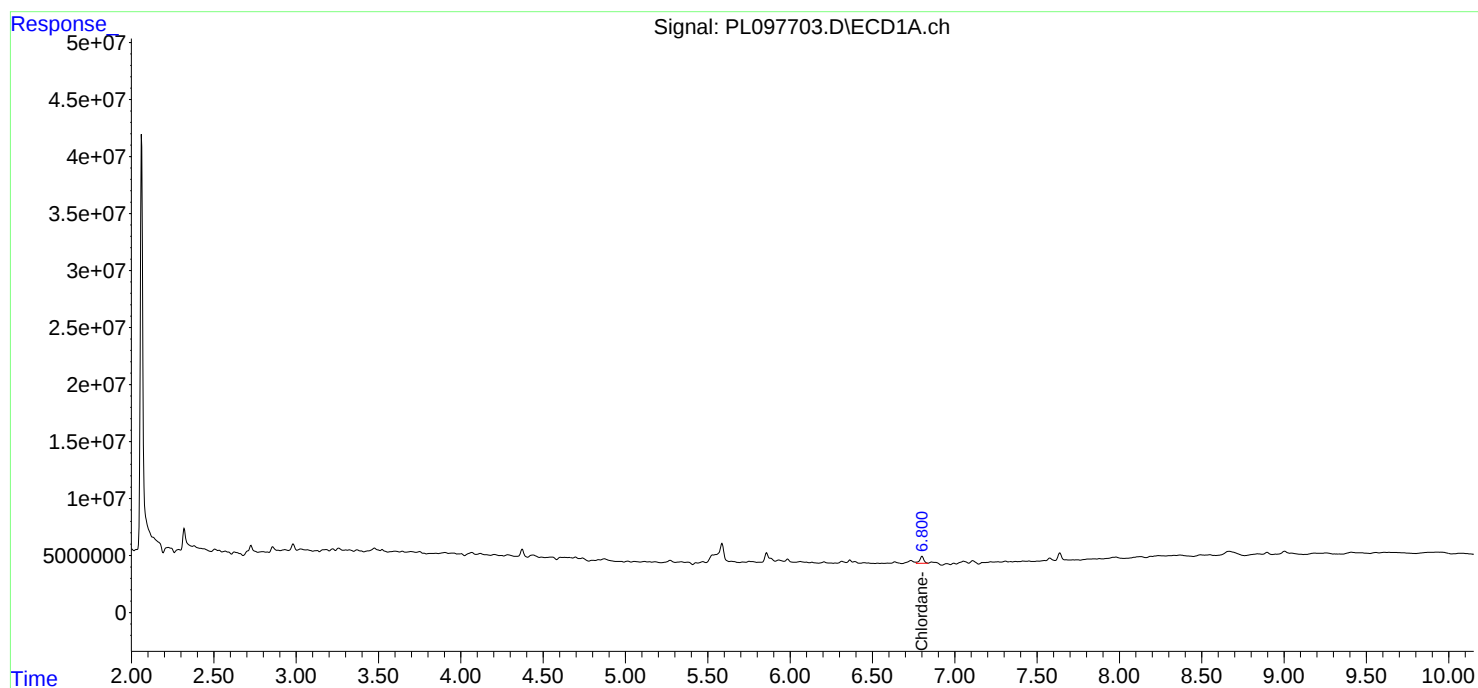


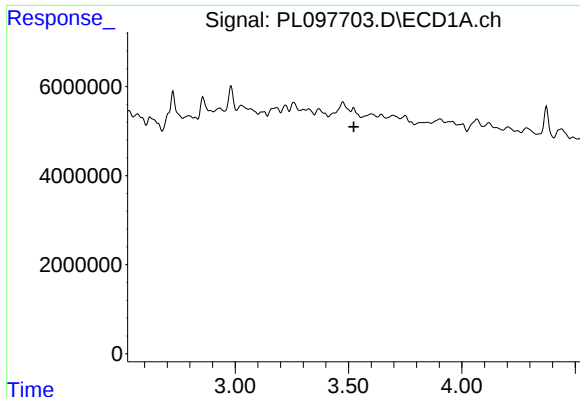

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

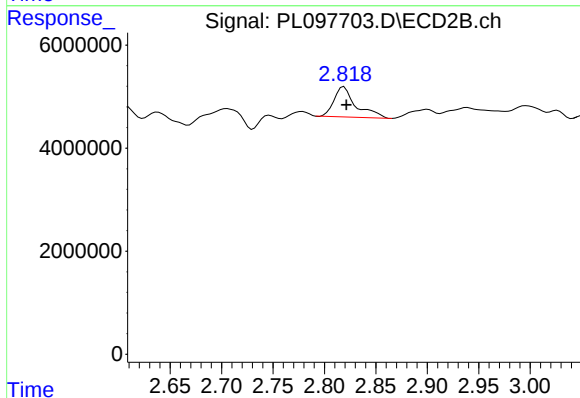


#1 Tetrachloro-m-xylene

R.T.: 2.819 min
Delta R.T.: -0.002 min
Response: 8550373
Conc: 1.42 ng/ml

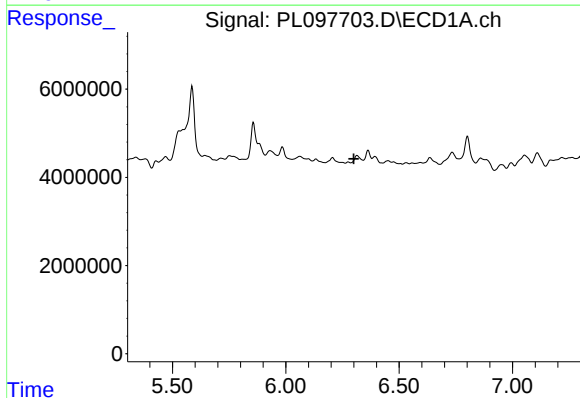


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.300 min
Response: 0
Conc: N.D.

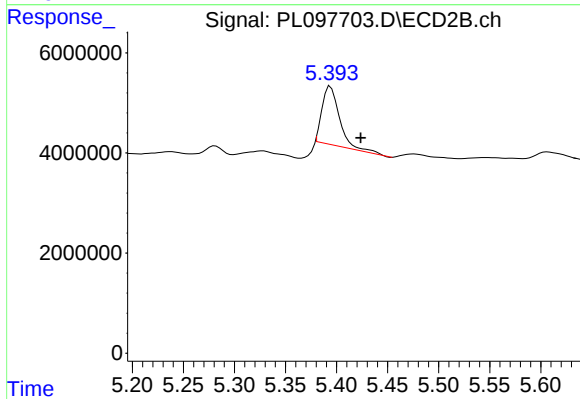

#13 Dieldrin


R.T.: 5.394 min
Delta R.T.: -0.029 min
Response: 13904446
Conc: 1.73 ng/ml

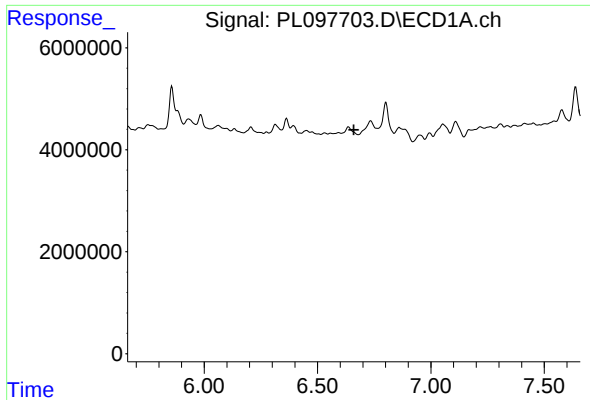

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

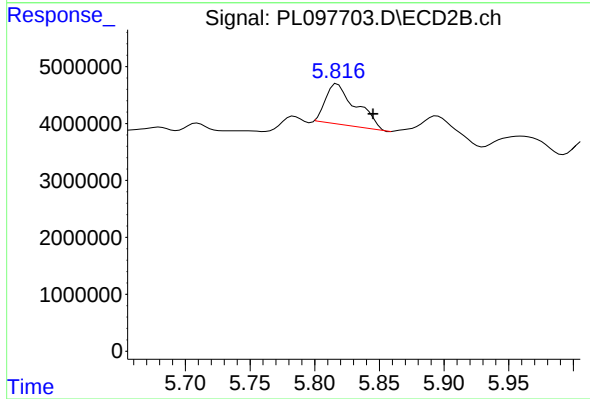


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: -0.028 min
Response: 11586141
Conc: 1.81 ng/ml

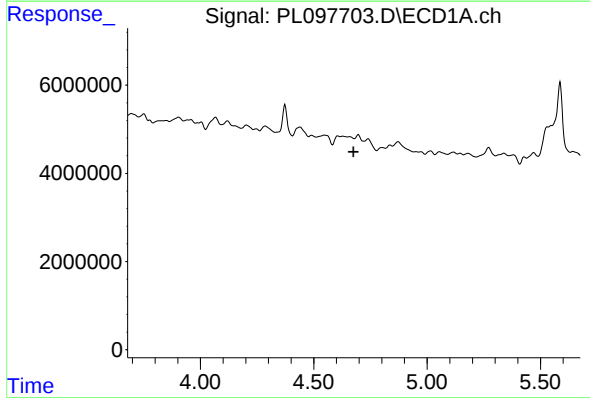


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.675 min
Response: 0
Conc: N.D.

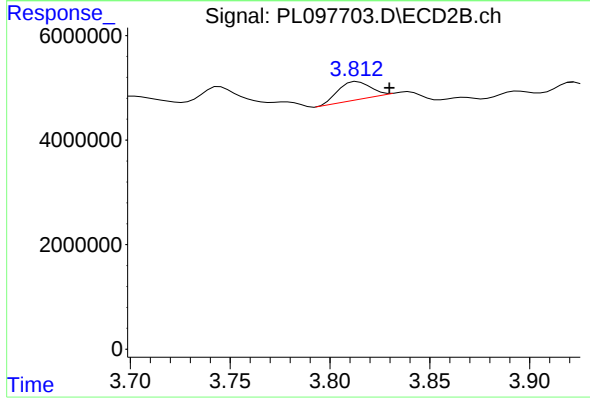

#23 Chlordane-1


R.T.: 3.814 min
Delta R.T.: -0.016 min
Response: 3823540
Conc: 15.31 ng/ml

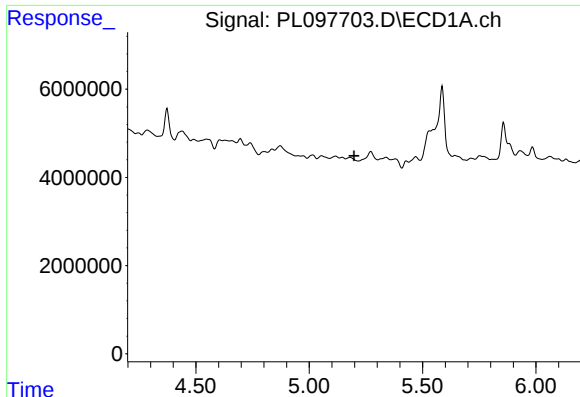

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

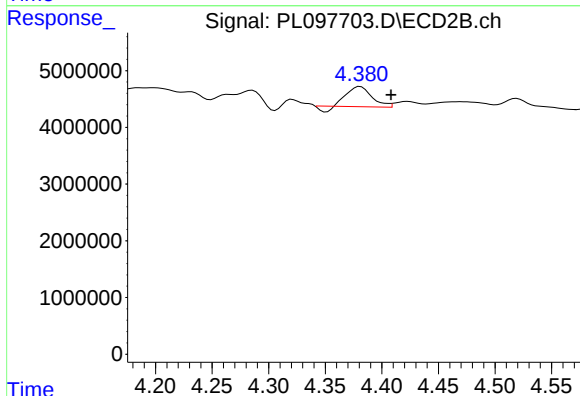


#24 Chlordane-2

R.T.: 4.381 min
Delta R.T.: -0.027 min
Response: 4994130
Conc: 17.52 ng/ml

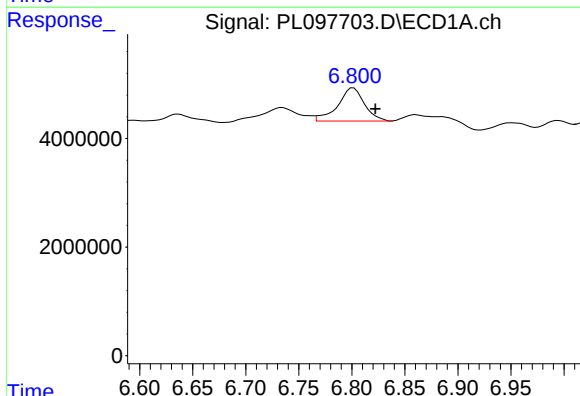


#27 Chlordane-5

R.T.: 6.802 min
Delta R.T.: -0.021 min
Response: 10685195
Conc: 63.02 ng/ml

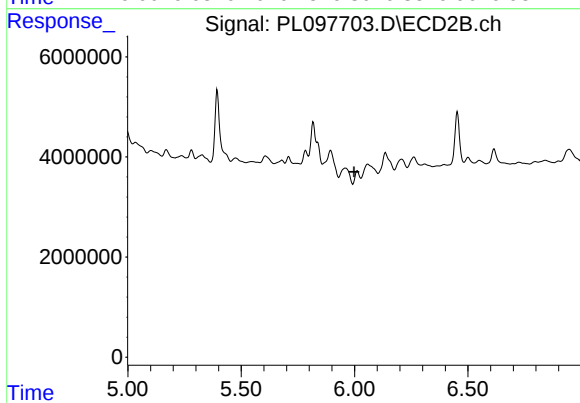

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

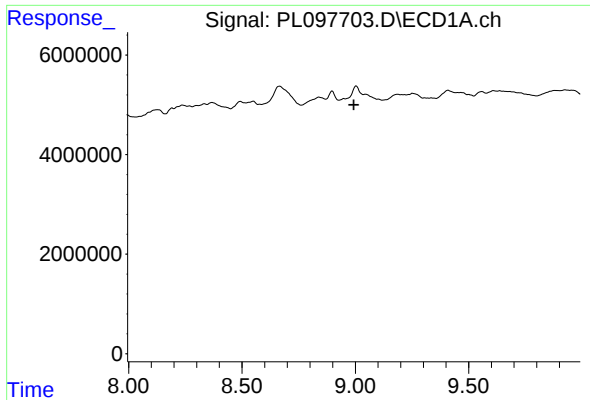

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.993 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

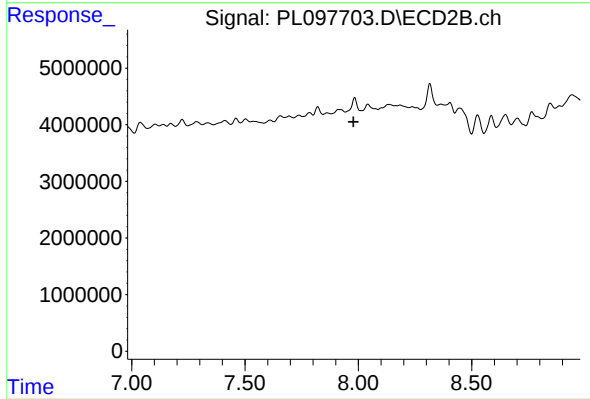

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.979 min
Response: 0
Conc: N.D.