

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
 Data File : PL097709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 14:14
 Operator : AR\AJ
 Sample : Q3496-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:54:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	2.822	99453870	93452175	24.305	15.526 #
28)	SA Decachlor...	9.001	7.984	40843381	64403730	13.728	12.050
Target Compounds							
2)	A alpha-BHC	0.000	3.339	0	6366846	N.D.	0.654 #
4)	MA Heptachlor	4.876	4.013	4321089	8446662	0.676	0.932 #
6)	B beta-BHC	0.000	3.967	0	23177804	N.D.	5.866 #
7)	B delta-BHC	4.720	0.000	18109923	0	3.046	N.D. #
9)	A Endosulfan I	0.000	5.166	0	12111082	N.D.	1.609 #
16)	A 4,4'-DDD	0.000	5.818f	0	11447419	N.D.	1.786 #
23)	Chlordane-1	0.000	3.843	0	6935514	N.D.	27.765 #
24)	Chlordane-2	0.000	4.420	0	7095568	N.D.	24.899 #
27)	Chlordane-5	6.800f	0.000	7641936	0	45.069	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
Data File : PL097709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 14:14
Operator : AR\AJ
Sample : Q3496-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:54:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

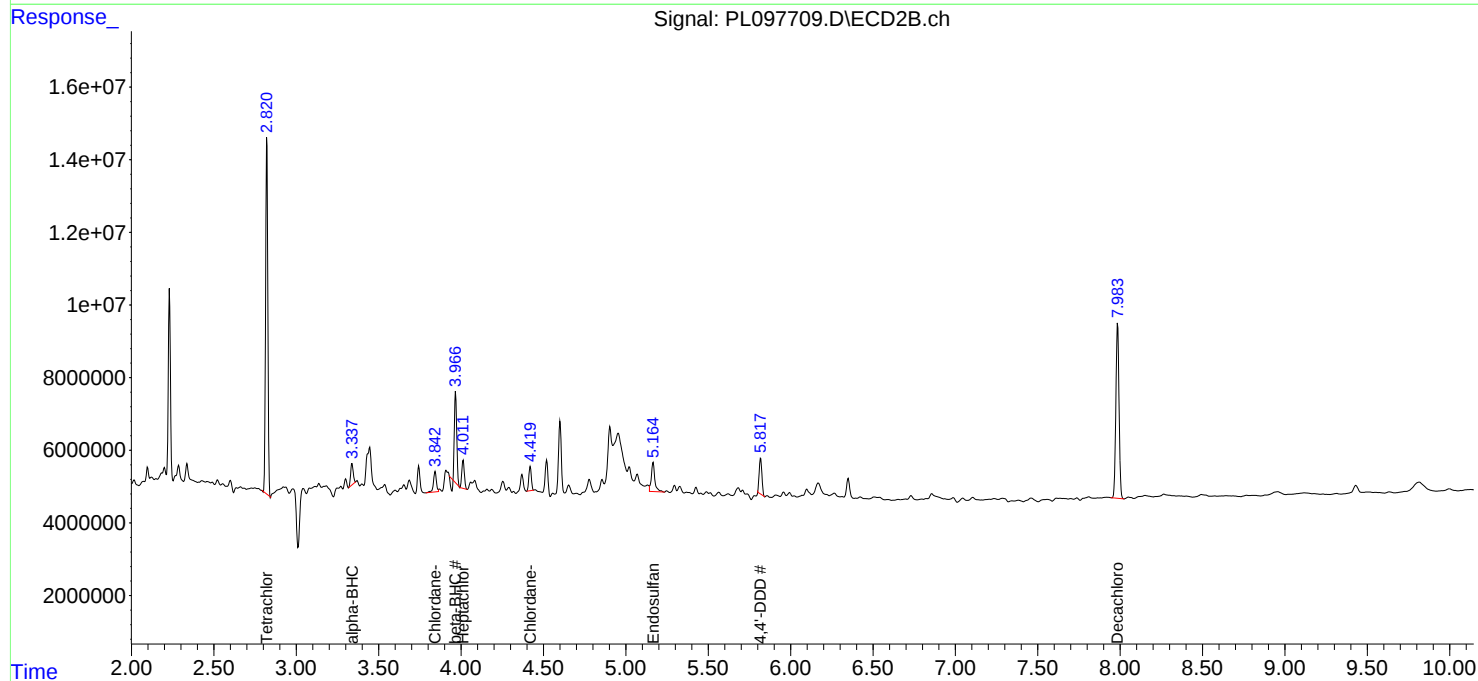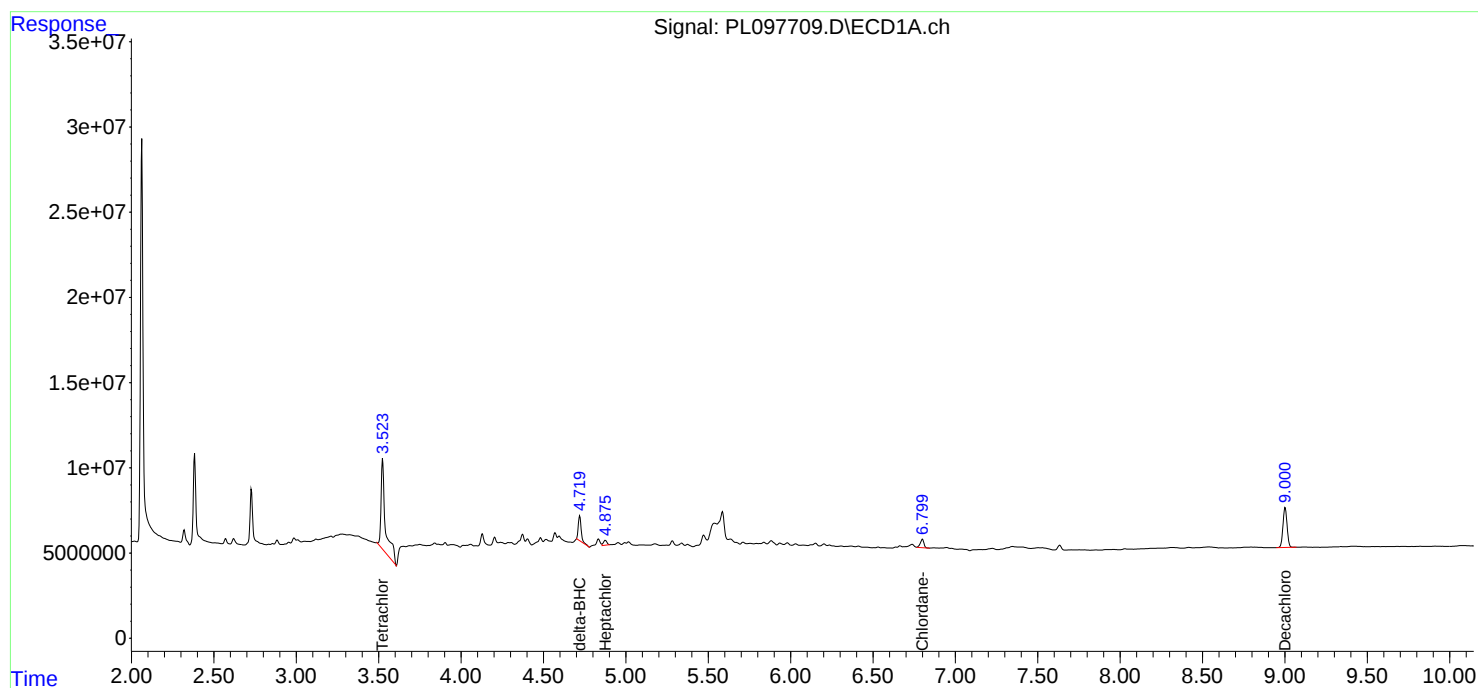


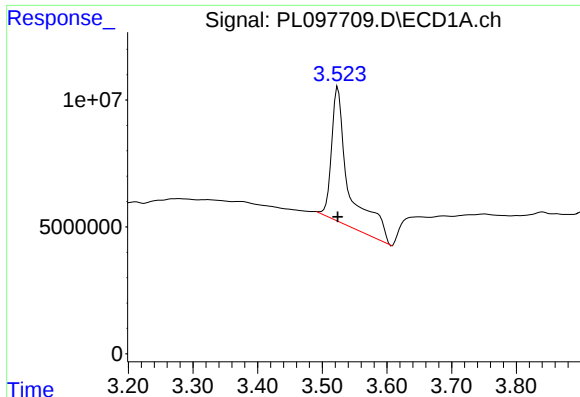

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 99453870
Conc: 24.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

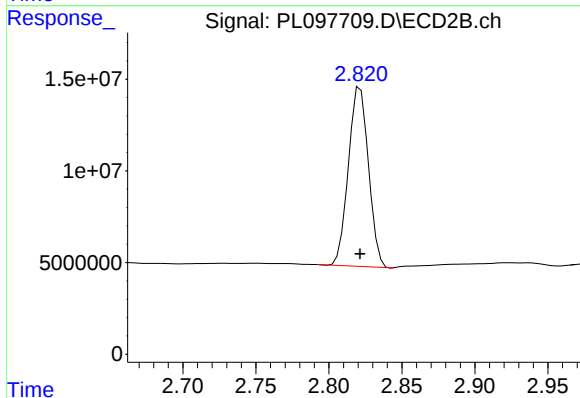


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 93452175
Conc: 15.53 ng/ml

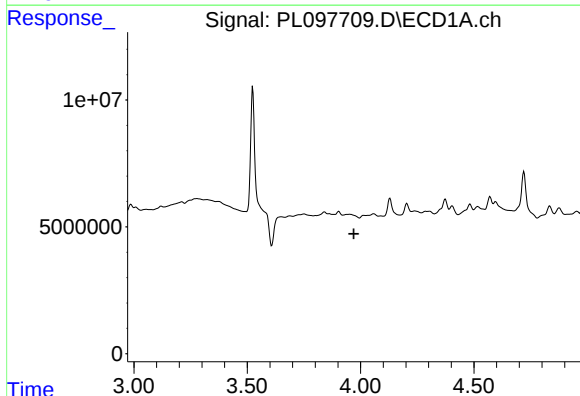


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

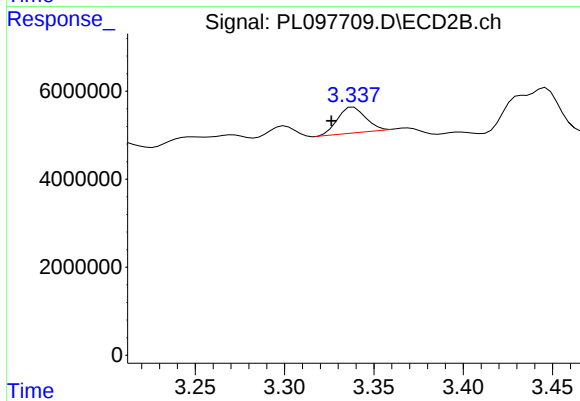

#2 alpha-BHC


R.T.: 3.339 min
Delta R.T.: 0.013 min
Response: 6366846
Conc: 0.65 ng/ml

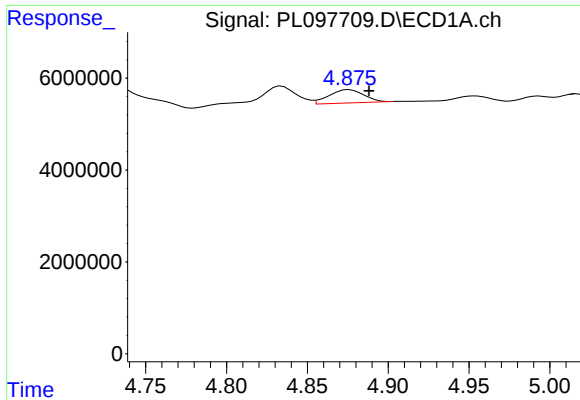

#4 Heptachlor


R.T.: 4.876 min
Delta R.T.: -0.012 min
Response: 4321089
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

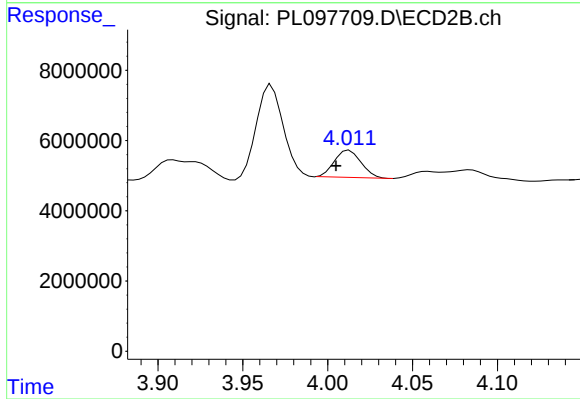


#4 Heptachlor

R.T.: 4.013 min
Delta R.T.: 0.008 min
Response: 8446662
Conc: 0.93 ng/ml

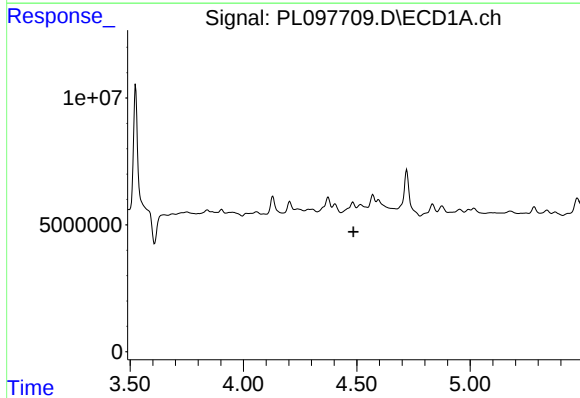


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.486 min
Response: 0
Conc: N.D.

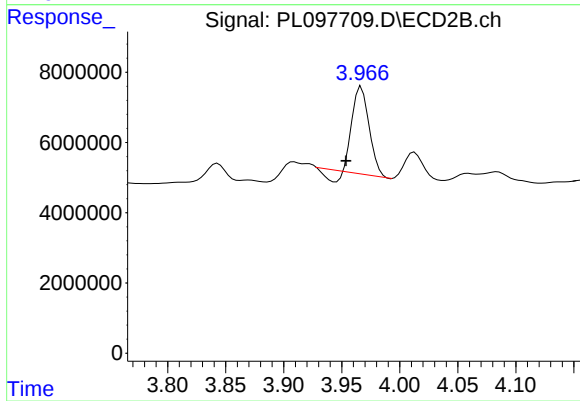

#6 beta-BHC


R.T.: 3.967 min
Delta R.T.: 0.013 min
Response: 23177804
Conc: 5.87 ng/ml

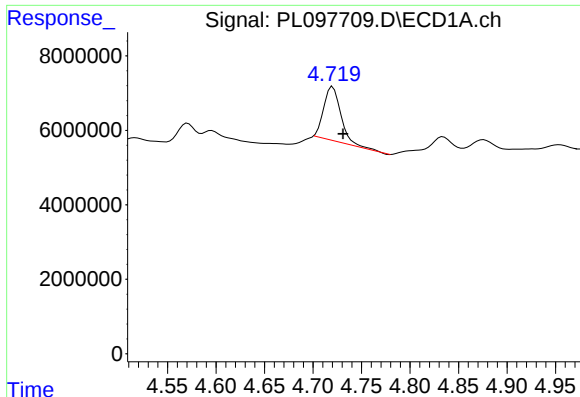

#7 delta-BHC


R.T.: 4.720 min
Delta R.T.: -0.011 min
Response: 18109923
Conc: 3.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

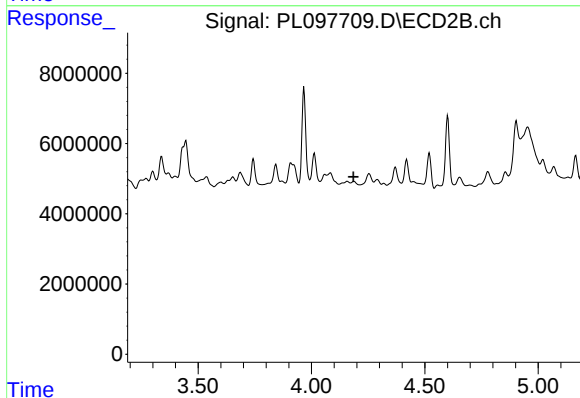


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.186 min
Response: 0
Conc: N.D.

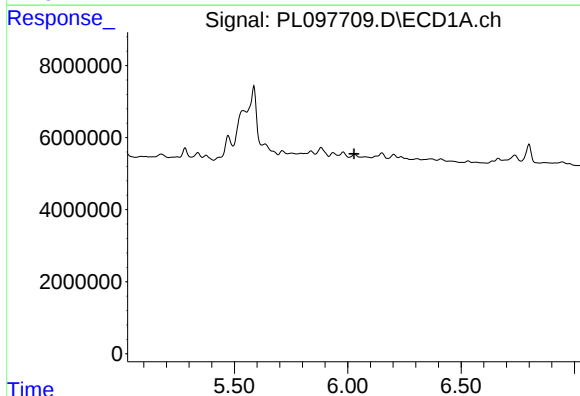


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.028 min
Response: 0
Conc: N.D.

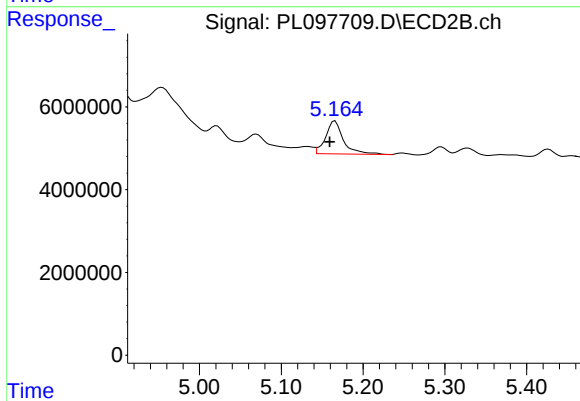

#9 Endosulfan I


R.T.: 5.166 min
Delta R.T.: 0.007 min
Response: 12111082
Conc: 1.61 ng/ml

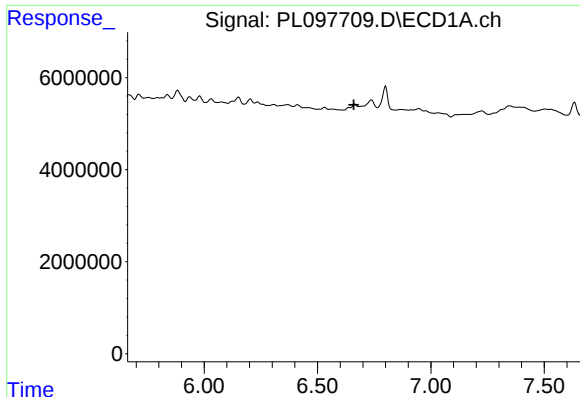

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

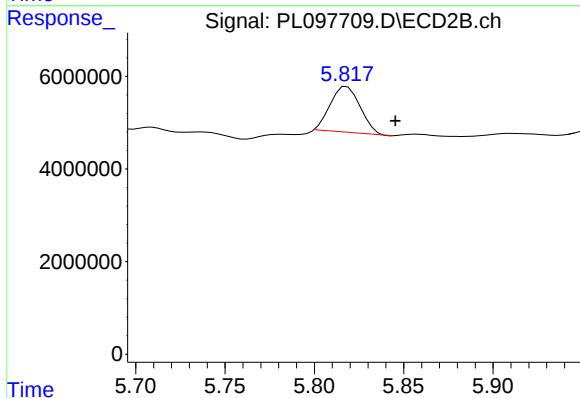


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: -0.027 min
Response: 11447419
Conc: 1.79 ng/ml

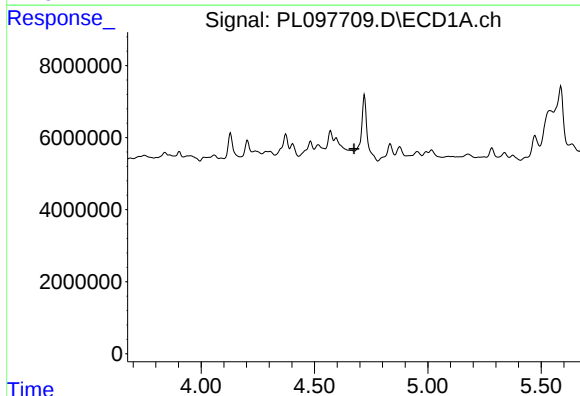


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.675 min
Response: 0
Conc: N.D.

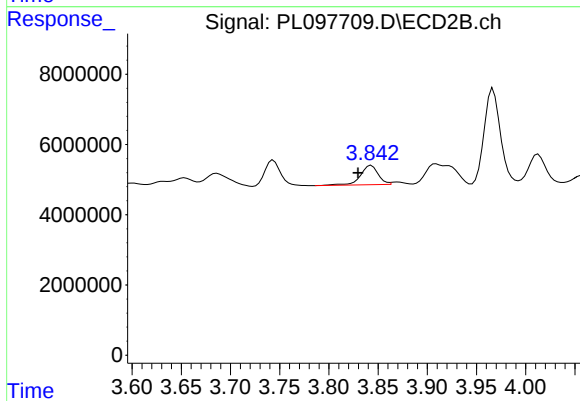

#23 Chlordane-1


R.T.: 3.843 min
Delta R.T.: 0.013 min
Response: 6935514
Conc: 27.77 ng/ml

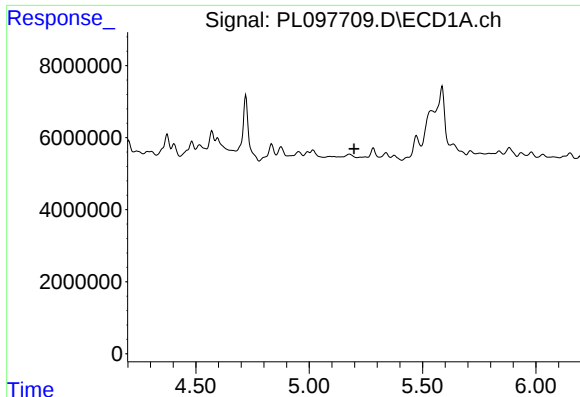

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

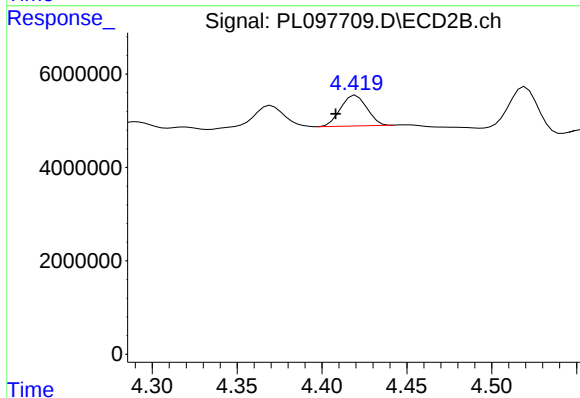


#24 Chlordane-2

R.T.: 4.420 min
Delta R.T.: 0.012 min
Response: 7095568
Conc: 24.90 ng/ml

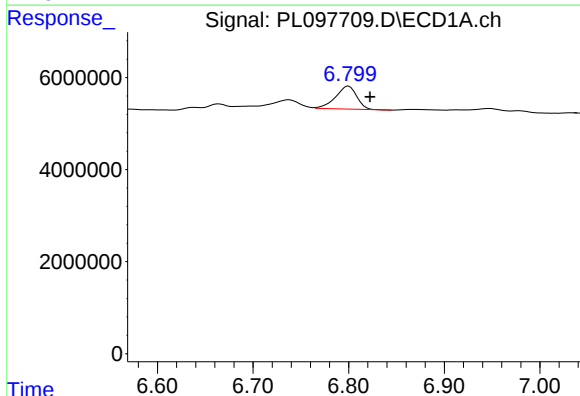


#27 Chlordane-5

R.T.: 6.800 min
Delta R.T.: -0.022 min
Response: 7641936
Conc: 45.07 ng/ml

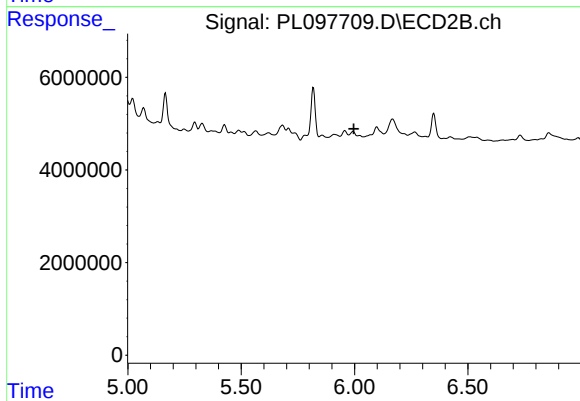

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

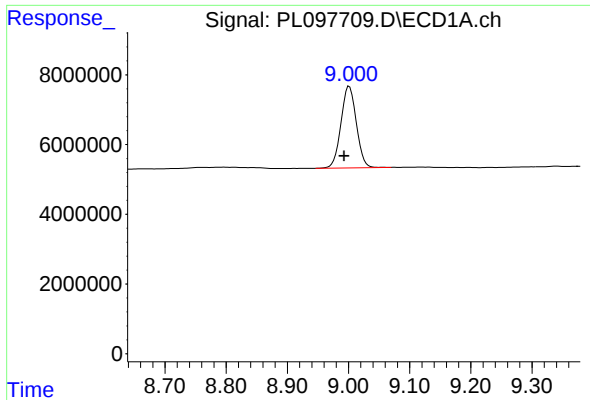

#28 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.008 min
Response: 40843381
Conc: 13.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

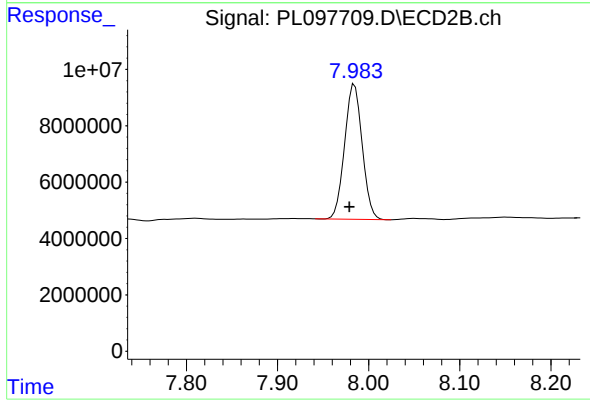

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: 0.005 min
Response: 64403730
Conc: 12.05 ng/ml