

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
 Data File : PL097710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 14:27
 Operator : AR\AJ
 Sample : Q3497-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:55:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	2.822	41776968	58844603	10.210	9.776
28)	SA Decachlor...	9.002	7.983	27320875	36545644	9.183	6.838 #
Target Compounds							
10)	B gamma-Chl...	5.904	5.043	11236391	18890818	2.050	2.183
11)	B alpha-Chl...	5.984	5.106	25714345	30154075	4.684	3.632
15)	B Endosulfa...	0.000	6.000	0	10432352	N.D.	1.486 #
24)	Chlordane-2	5.196	4.414	26491044	33242131	117.548	116.648
25)	Chlordane-3	5.904	5.043	11236391	18890818	13.501	21.186 #
26)	Chlordane-4	5.984	5.106	25714345	30154075	25.322	39.716 #
27)	Chlordane-5	6.826	6.000	6813204	10432352	40.182	34.753



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
Data File : PL097710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 14:27
Operator : AR\AJ
Sample : Q3497-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:55:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

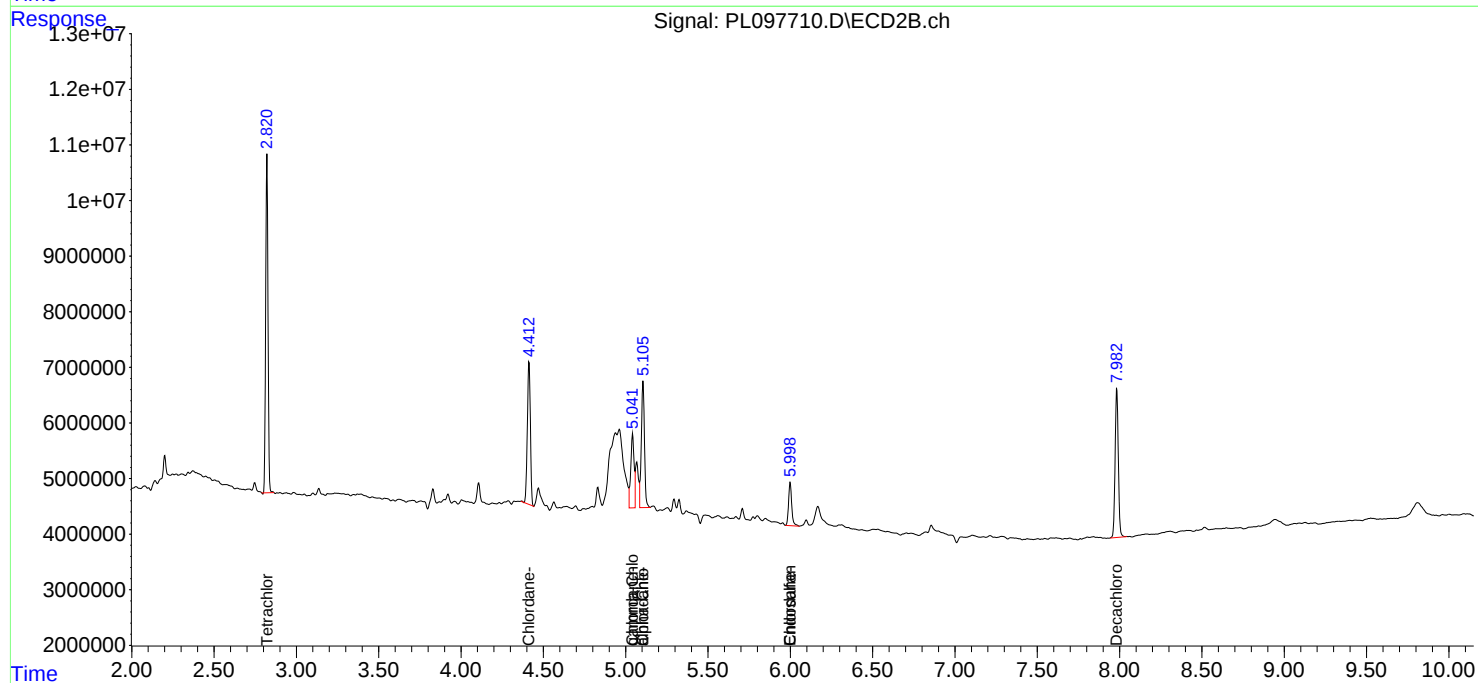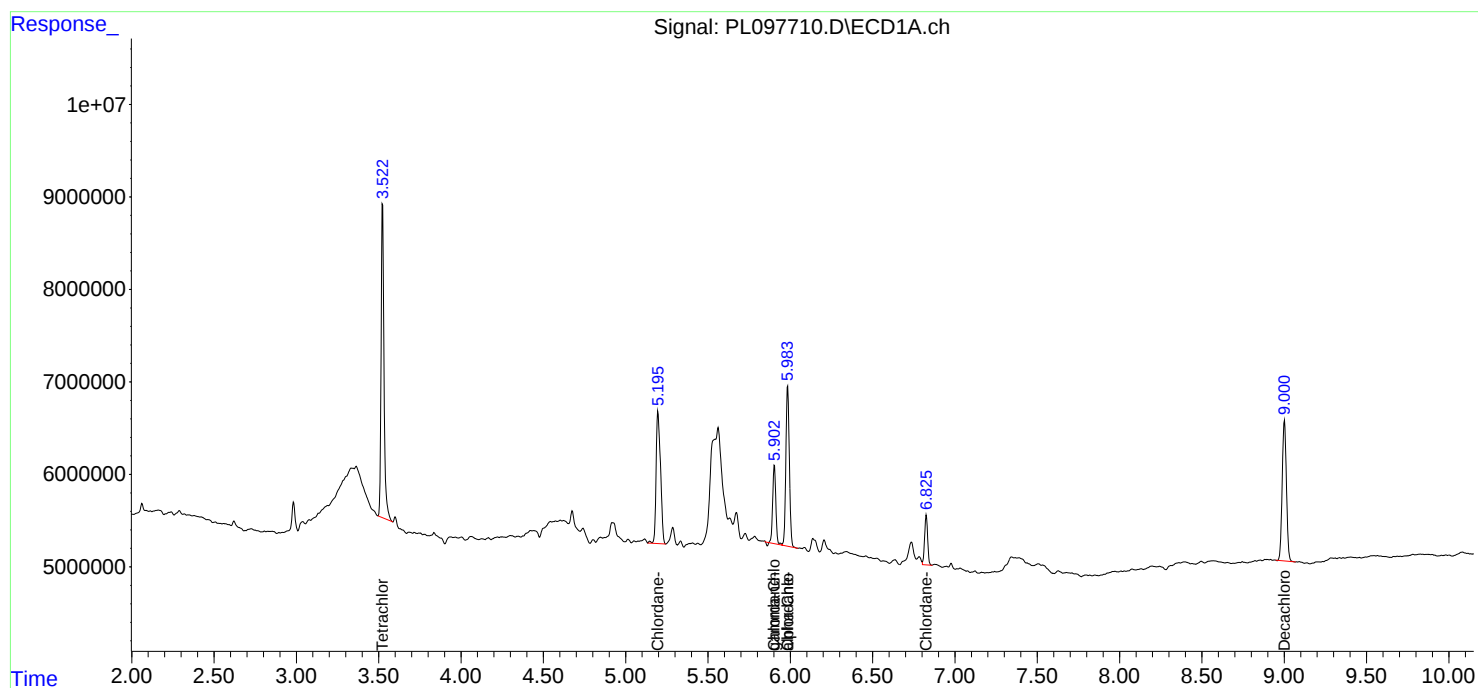


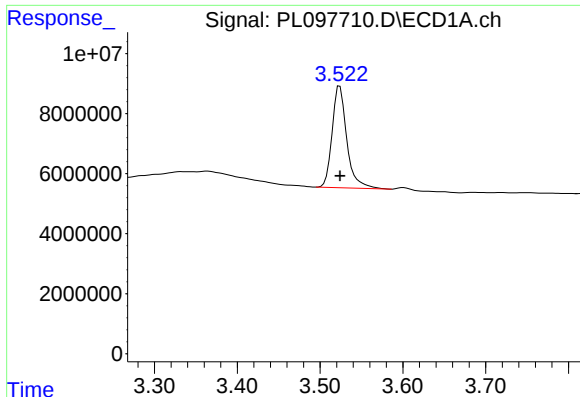

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 41776968
Conc: 10.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

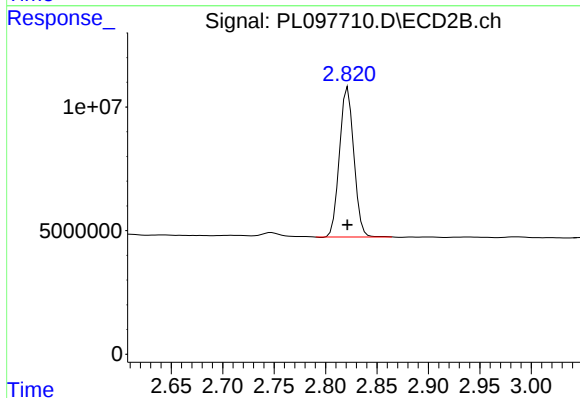


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 58844603
Conc: 9.78 ng/ml

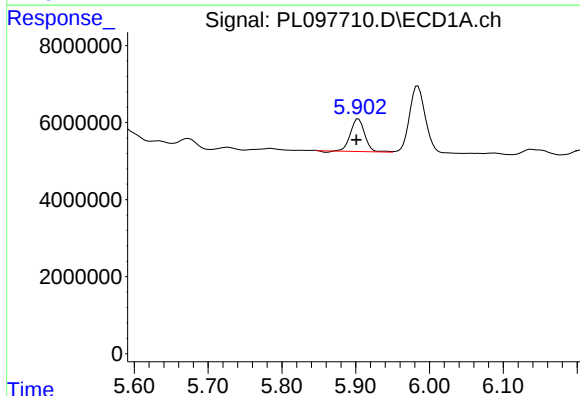


#10 gamma-Chlordane

R.T.: 5.904 min
Delta R.T.: 0.003 min
Response: 11236391
Conc: 2.05 ng/ml

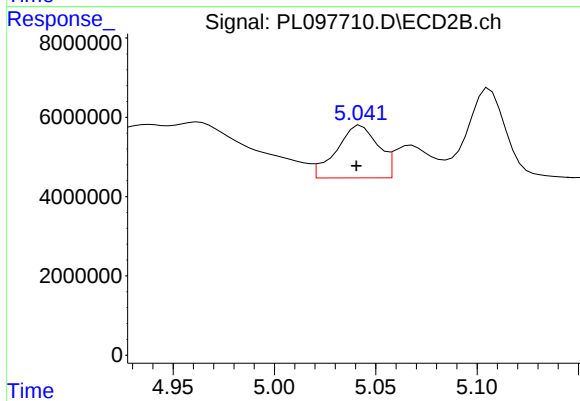

#10 gamma-Chlordane


R.T.: 5.043 min
Delta R.T.: 0.002 min
Response: 18890818
Conc: 2.18 ng/ml

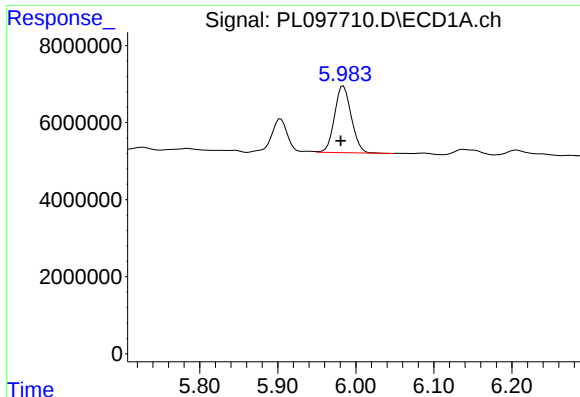

#11 alpha-Chlordane


R.T.: 5.984 min
Delta R.T.: 0.004 min
Response: 25714345
Conc: 4.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

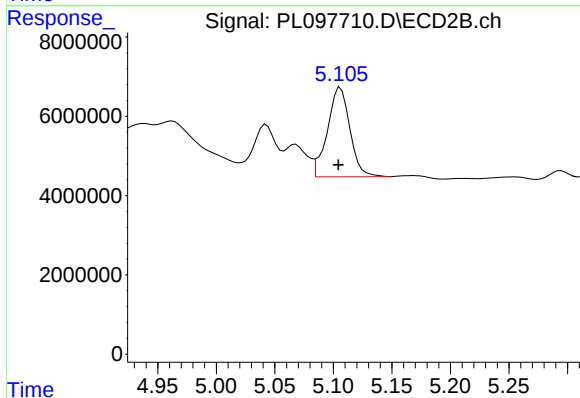


#11 alpha-Chlordane

R.T.: 5.106 min
Delta R.T.: 0.002 min
Response: 30154075
Conc: 3.63 ng/ml

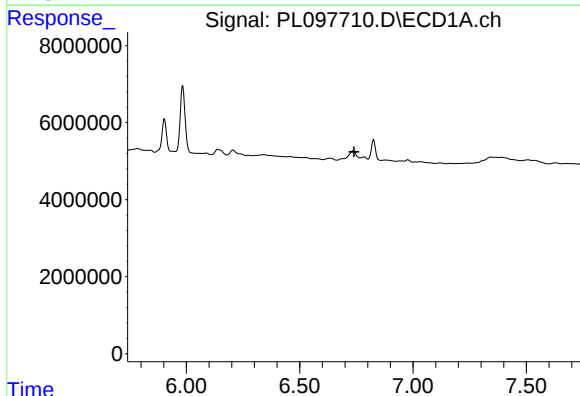


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.741 min
Response: 0
Conc: N.D.

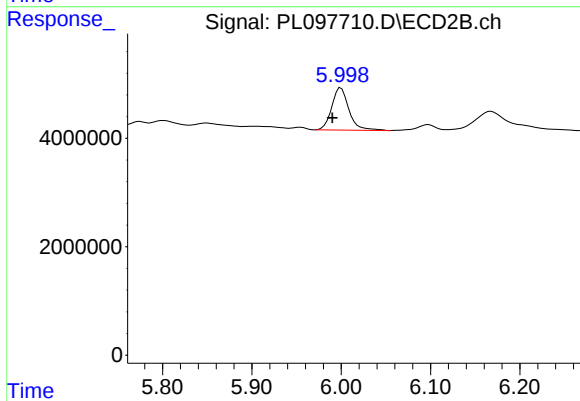

#15 Endosulfan II


R.T.: 6.000 min
Delta R.T.: 0.010 min
Response: 10432352
Conc: 1.49 ng/ml

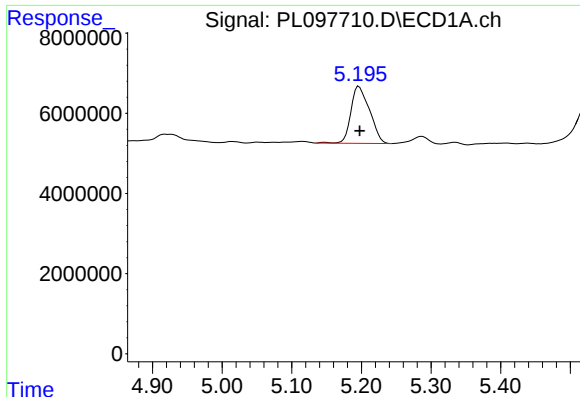

#24 Chlordane-2


R.T.: 5.196 min
Delta R.T.: -0.001 min
Response: 26491044
Conc: 117.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

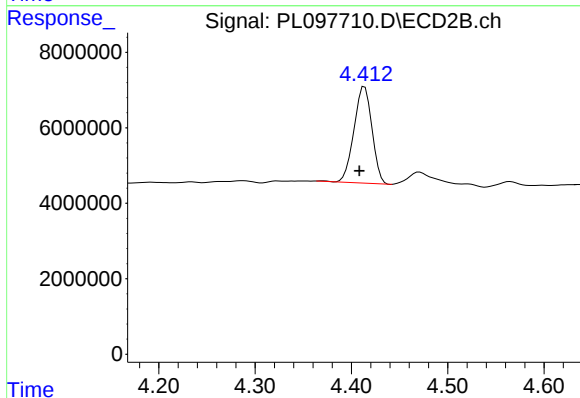


#24 Chlordane-2

R.T.: 4.414 min
Delta R.T.: 0.006 min
Response: 33242131
Conc: 116.65 ng/ml

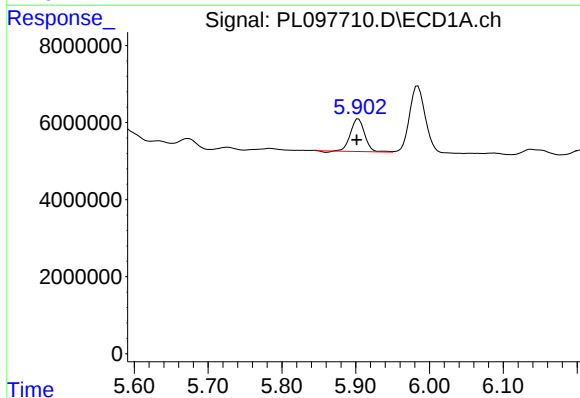


#25 Chlordane-3

R.T.: 5.904 min
Delta R.T.: 0.003 min
Response: 11236391
Conc: 13.50 ng/ml

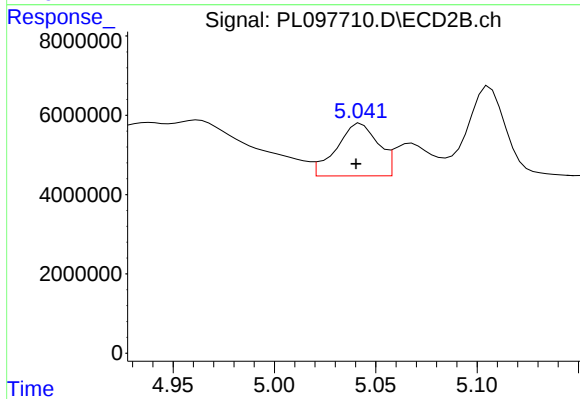

#25 Chlordane-3


R.T.: 5.043 min
Delta R.T.: 0.002 min
Response: 18890818
Conc: 21.19 ng/ml

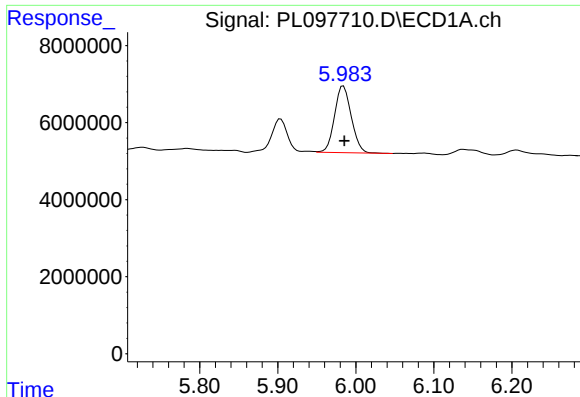

#26 Chlordane-4


R.T.: 5.984 min
Delta R.T.: -0.001 min
Response: 25714345
Conc: 25.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

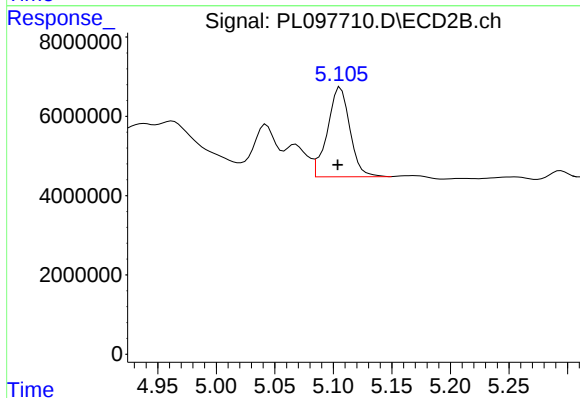


#26 Chlordane-4

R.T.: 5.106 min
Delta R.T.: 0.002 min
Response: 30154075
Conc: 39.72 ng/ml

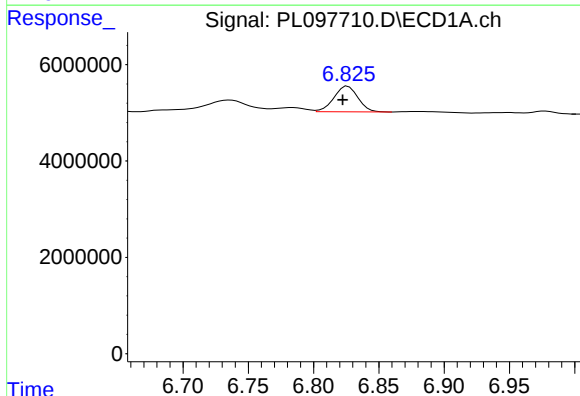


#27 Chlordane-5

R.T.: 6.826 min
Delta R.T.: 0.004 min
Response: 6813204
Conc: 40.18 ng/ml

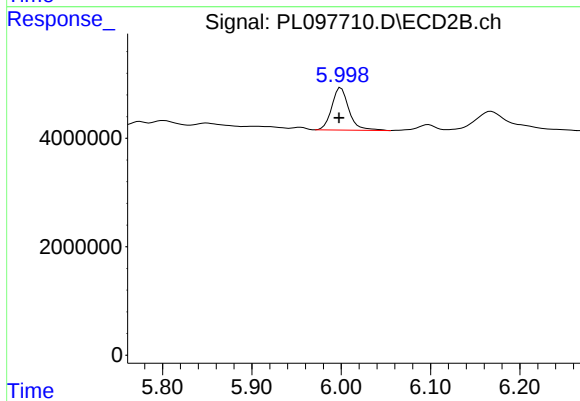

#27 Chlordane-5


R.T.: 6.000 min
Delta R.T.: 0.002 min
Response: 10432352
Conc: 34.75 ng/ml

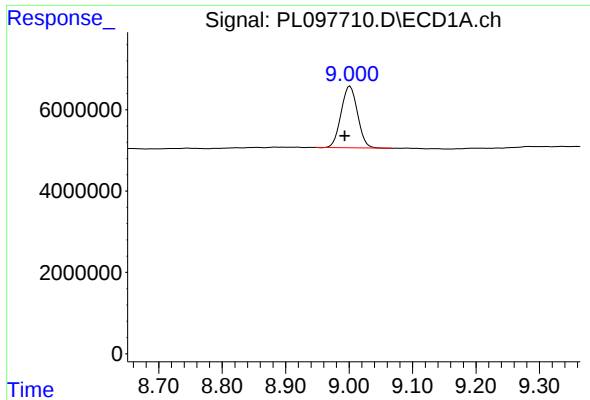

#28 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.009 min
Response: 27320875
Conc: 9.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

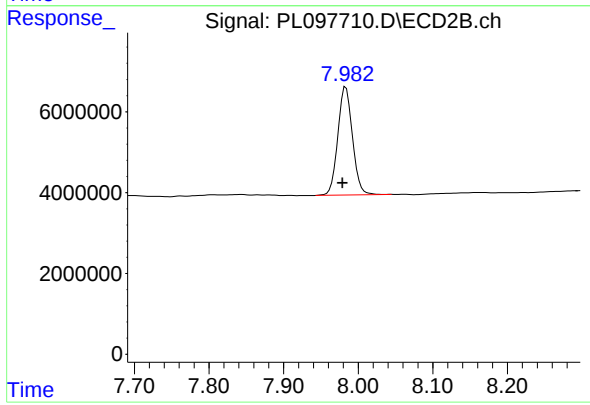

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: 0.004 min
Response: 36545644
Conc: 6.84 ng/ml