

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
 Data File : PL097711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 14:41
 Operator : AR\AJ
 Sample : Q3500-01 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:55:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.822	0	5974061	N.D.	0.993 #
28)	SA Decachlor...	9.005	7.981	6274933	2216651	2.109	0.415 #
Target Compounds							
7)	B delta-BHC	4.742	0.000	10347530	0	1.741	N.D. #
8)	B Heptachlo...	5.641	0.000	4212235	0	0.722	N.D. #
10)	B gamma-Chl...	5.880f	0.000	7642641	0	1.394	N.D. #
13)	MA Dieldrin	0.000	5.428	0	9447080	N.D.	1.175 #
15)	B Endosulfa...	6.731	5.997	10038377	6557830	2.205	0.934 #
16)	A 4,4'-DDD	6.651	5.818f	6688661	8152612	1.871	1.272 #
17)	MA 4,4'-DDT	6.952f	0.000	4707661	0	1.168	N.D. #
20)	A Methoxychlor	0.000	6.653f	0	9251514	N.D.	2.490 #
21)	B Endrin ke...	7.570	0.000	16121695	0	3.873	N.D. #
25)	Chlordane-3	5.880f	0.000	7642641	0	9.183	N.D. #
27)	Chlordane-5	6.797f	5.997	24597611	6557830	145.068	21.846 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
Data File : PL097711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 14:41
Operator : AR\AJ
Sample : Q3500-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:55:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

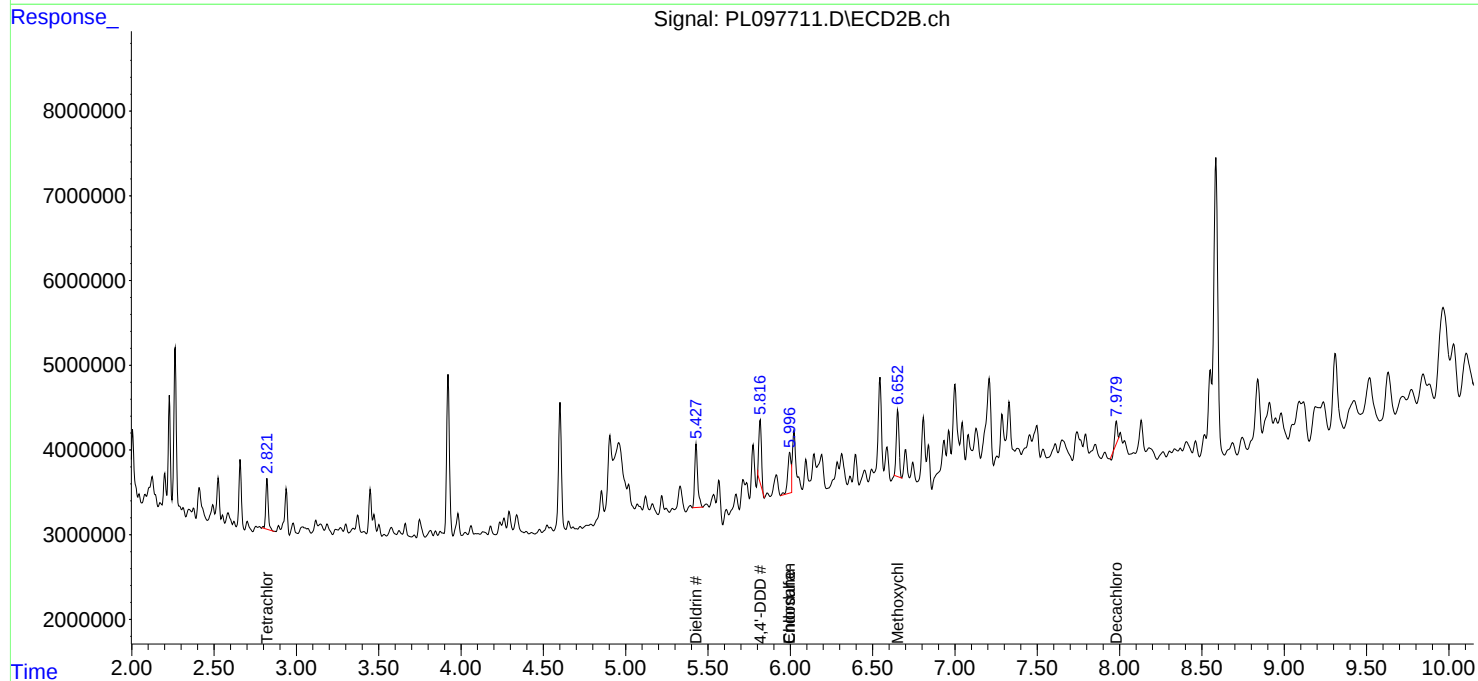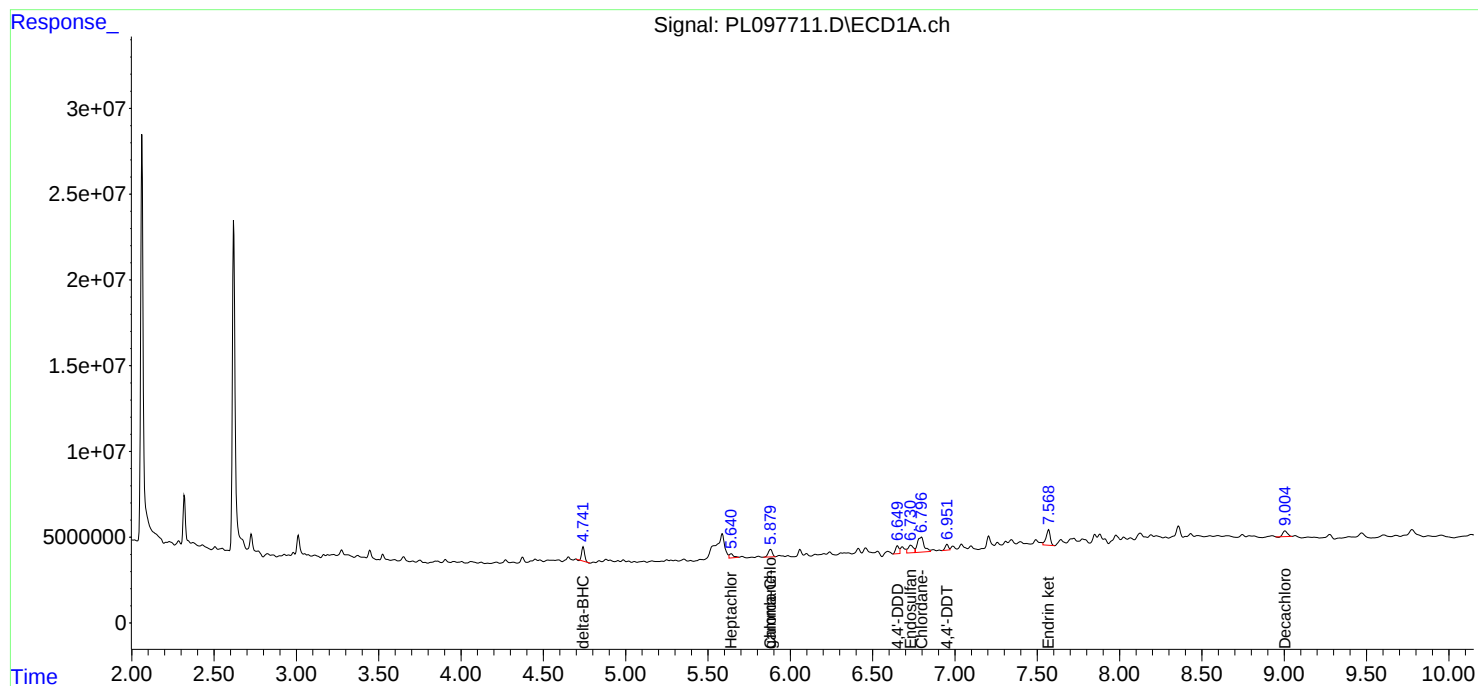


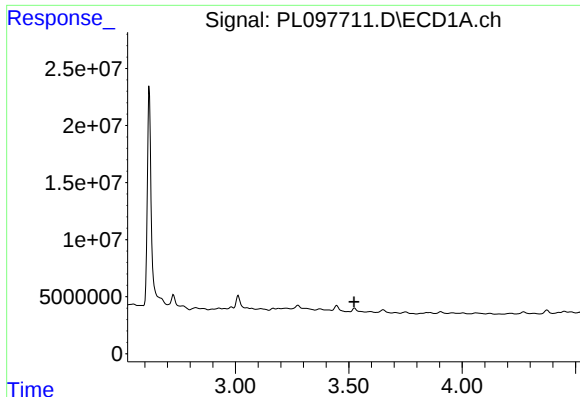

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

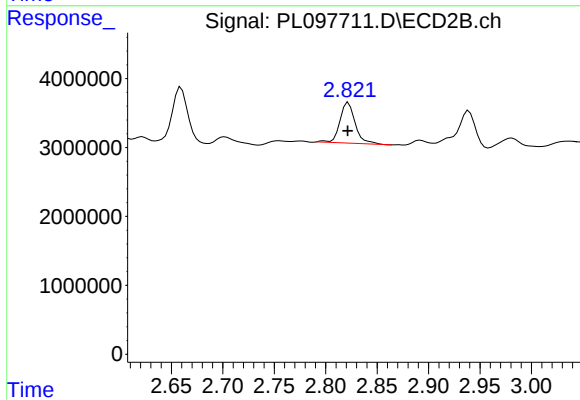


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 5974061
Conc: 0.99 ng/ml

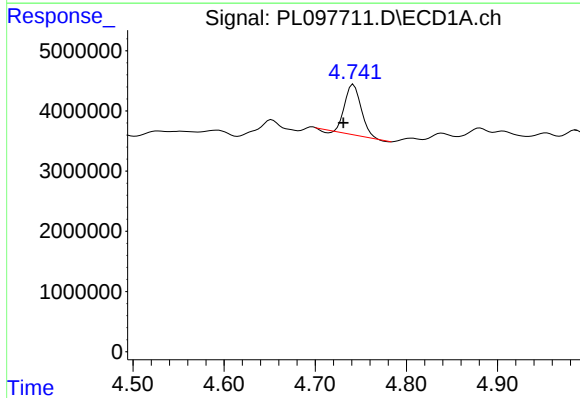


#7 delta-BHC

R.T.: 4.742 min
Delta R.T.: 0.011 min
Response: 10347530
Conc: 1.74 ng/ml

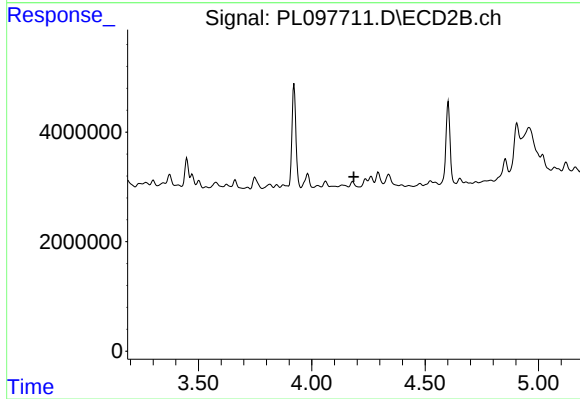

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.186 min
Response: 0
Conc: N.D.

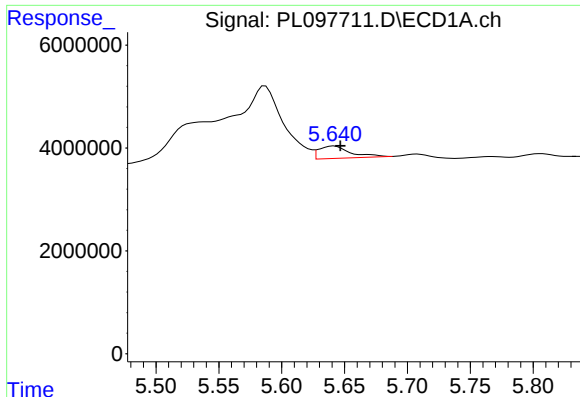

#8 Heptachlor epoxide


R.T.: 5.641 min
Delta R.T.: -0.005 min
Response: 4212235
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

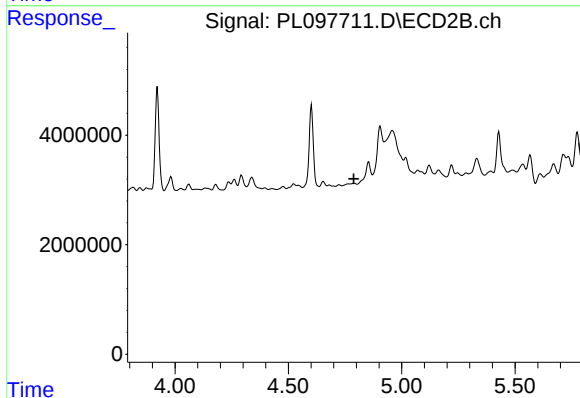


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.789 min
Response: 0
Conc: N.D.

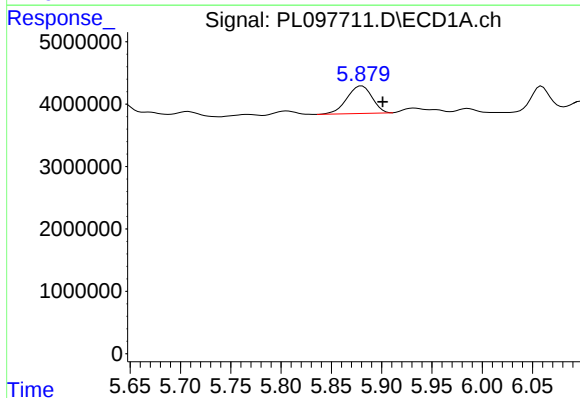


#10 gamma-Chlordane

R.T.: 5.880 min
Delta R.T.: -0.021 min
Response: 7642641
Conc: 1.39 ng/ml

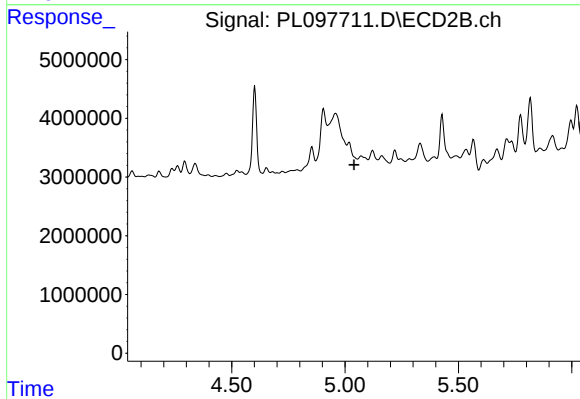

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

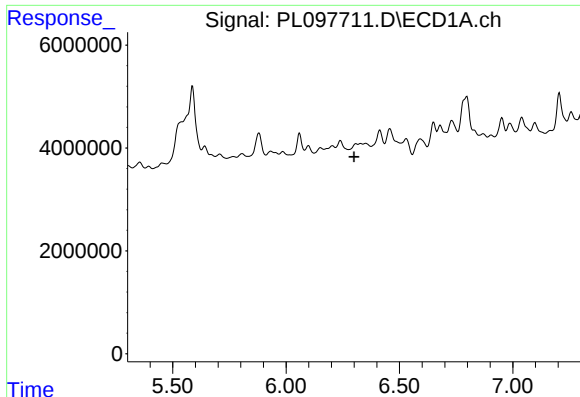

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.300 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

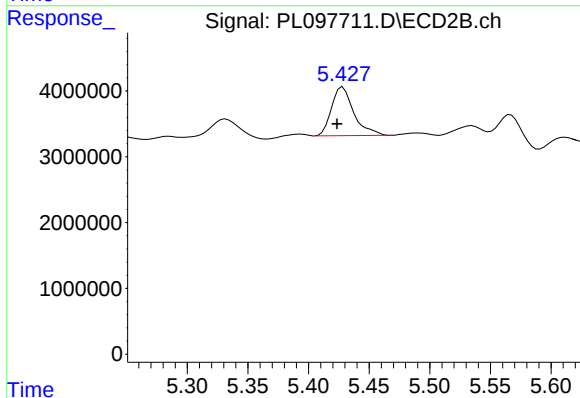


#13 Dieldrin

R.T.: 5.428 min
Delta R.T.: 0.005 min
Response: 9447080
Conc: 1.18 ng/ml

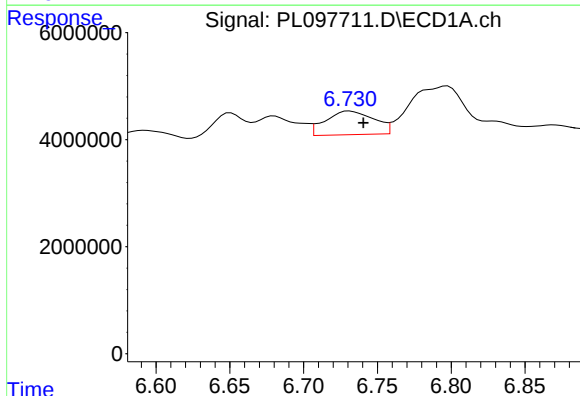


#15 Endosulfan II

R.T.: 6.731 min
Delta R.T.: -0.009 min
Response: 10038377
Conc: 2.20 ng/ml

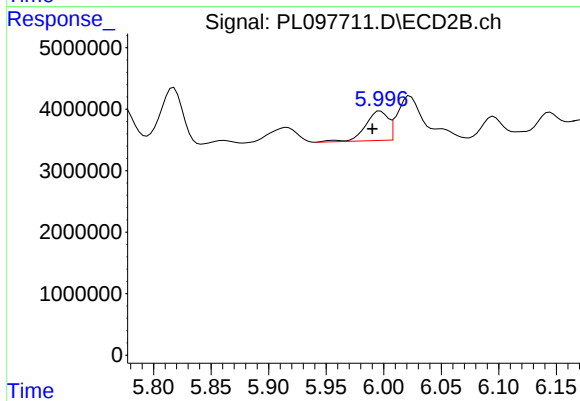

#15 Endosulfan II


R.T.: 5.997 min
Delta R.T.: 0.007 min
Response: 6557830
Conc: 0.93 ng/ml

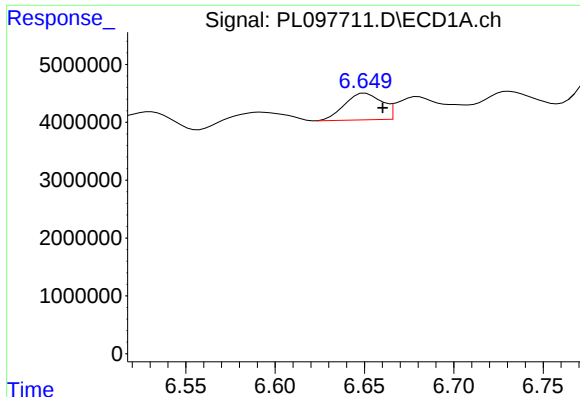

#16 4,4'-DDD


R.T.: 6.651 min
Delta R.T.: -0.010 min
Response: 6688661
Conc: 1.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

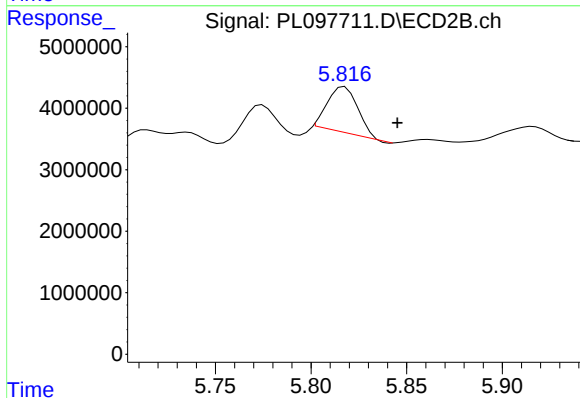


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: -0.028 min
Response: 8152612
Conc: 1.27 ng/ml

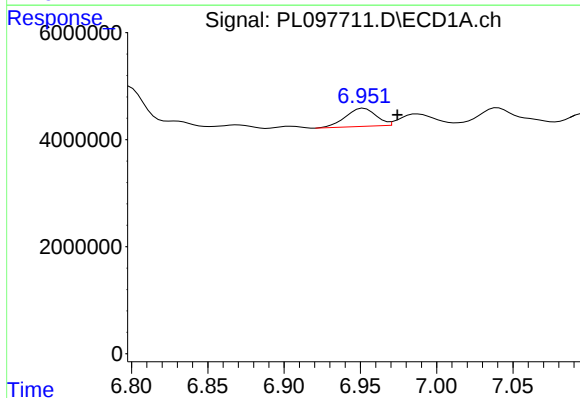


#17 4,4'-DDT

R.T.: 6.952 min
Delta R.T.: -0.022 min
Response: 4707661
Conc: 1.17 ng/ml

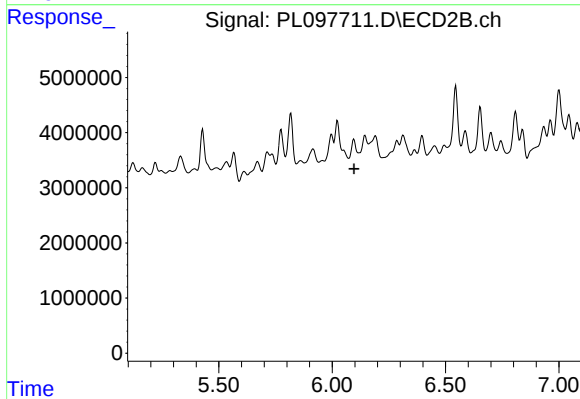

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.097 min
Response: 0
Conc: N.D.

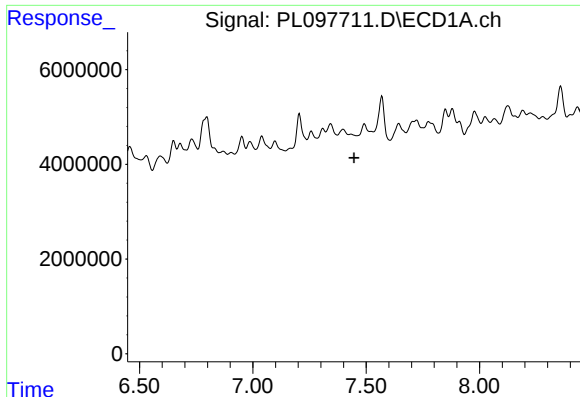

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

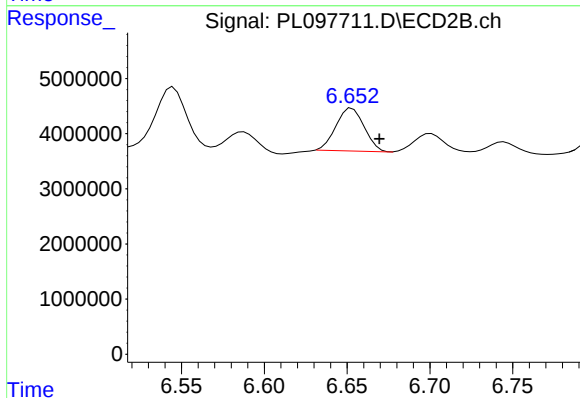


#20 Methoxychlor

R.T.: 6.653 min
Delta R.T.: -0.016 min
Response: 9251514
Conc: 2.49 ng/ml

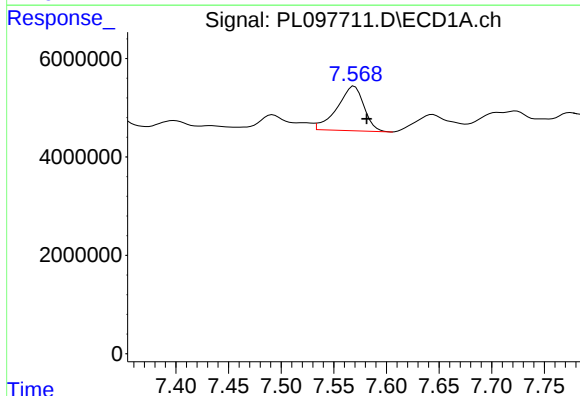


#21 Endrin ketone

R.T.: 7.570 min
Delta R.T.: -0.012 min
Response: 16121695
Conc: 3.87 ng/ml

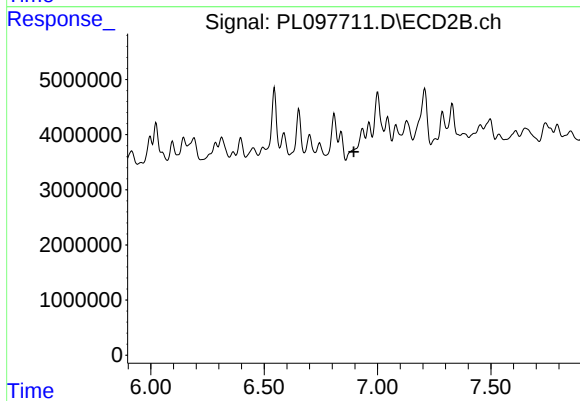

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.896 min
Response: 0
Conc: N.D.

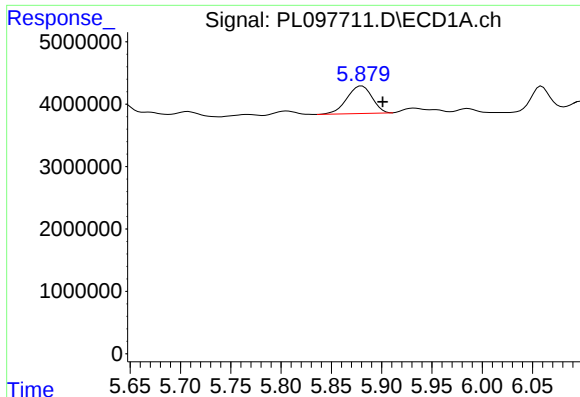

#25 Chlordane-3


R.T.: 5.880 min
Delta R.T.: -0.021 min
Response: 7642641
Conc: 9.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

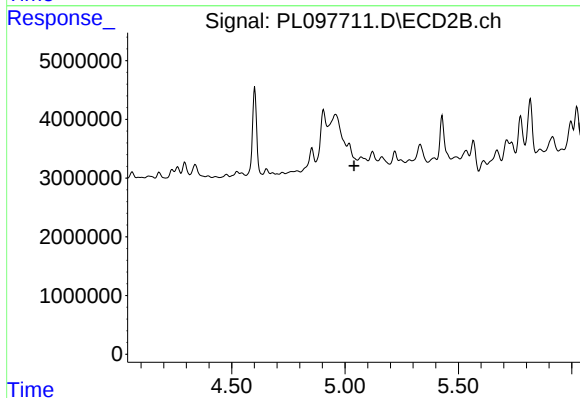


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

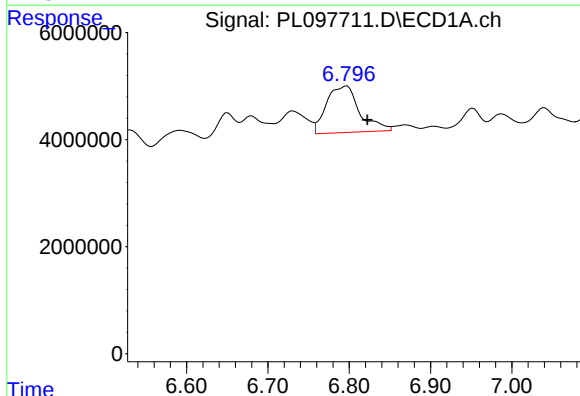


#27 Chlordane-5

R.T.: 6.797 min
Delta R.T.: -0.025 min
Response: 24597611
Conc: 145.07 ng/ml

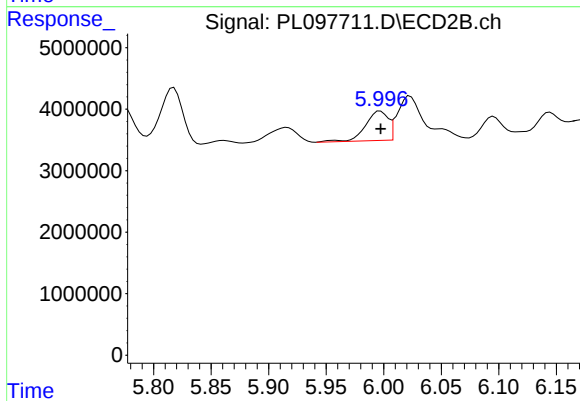

#27 Chlordane-5


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 6557830
Conc: 21.85 ng/ml

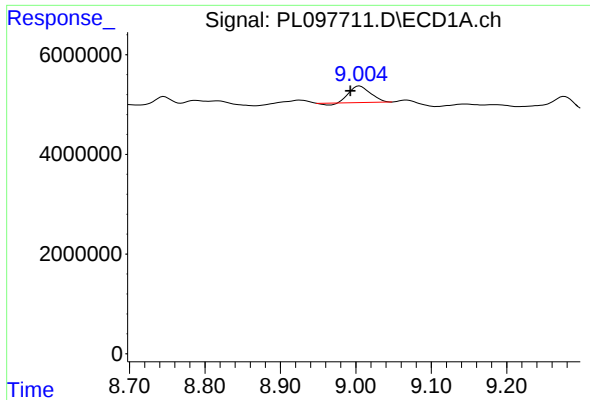

#28 Decachlorobiphenyl

R.T.: 9.005 min
Delta R.T.: 0.012 min
Response: 6274933
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

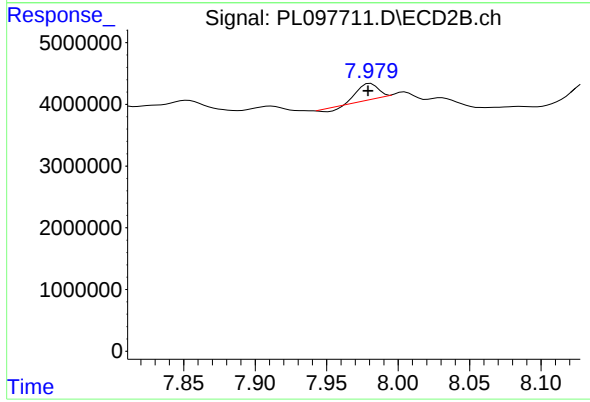

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.002 min
Response: 2216651
Conc: 0.41 ng/ml