

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
 Data File : PL097714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 15:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:55:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.822	94128288	142.1E6	23.004	23.614
28)	SA Decachlor...	9.001	7.983	68615226	109.6E6	23.063	20.505
Target Compounds							
14)	MA Endrin	0.000	5.710	0	6702774	N.D.	0.958 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
Data File : PL097714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 15:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:55:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

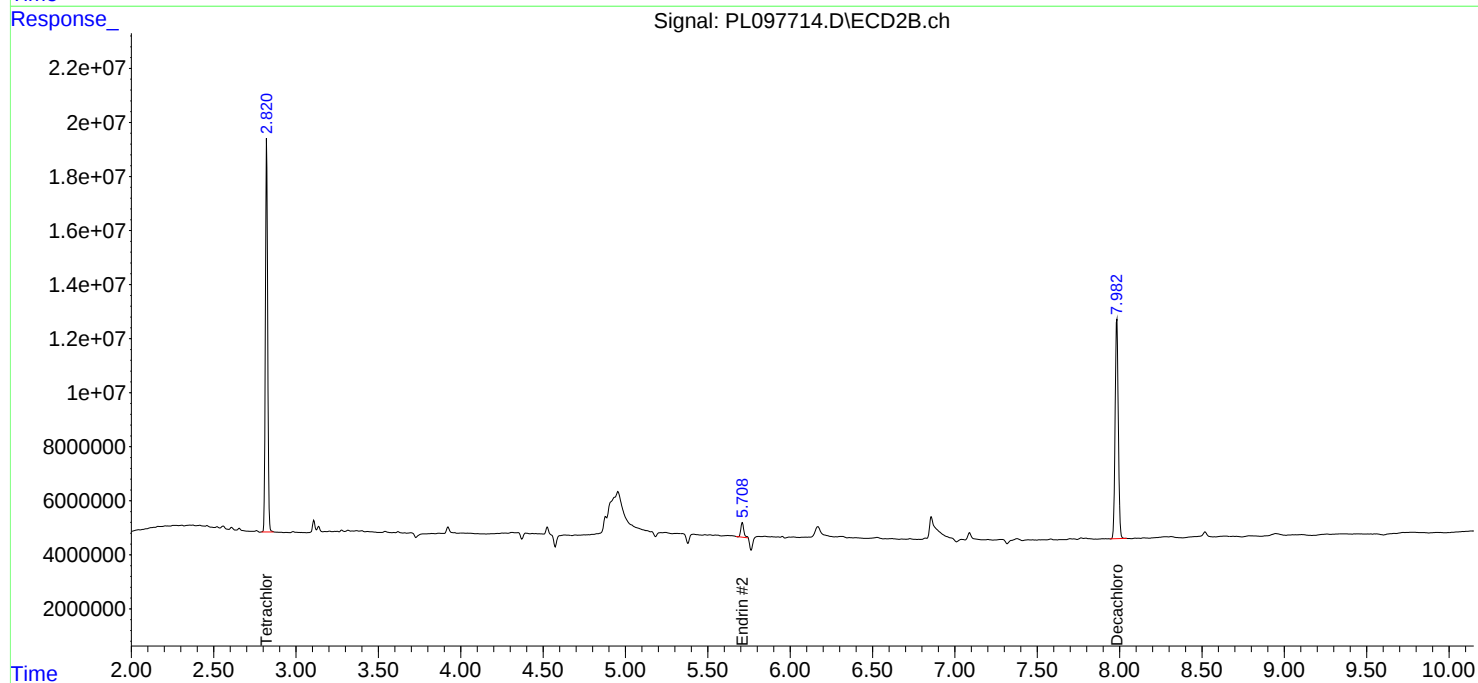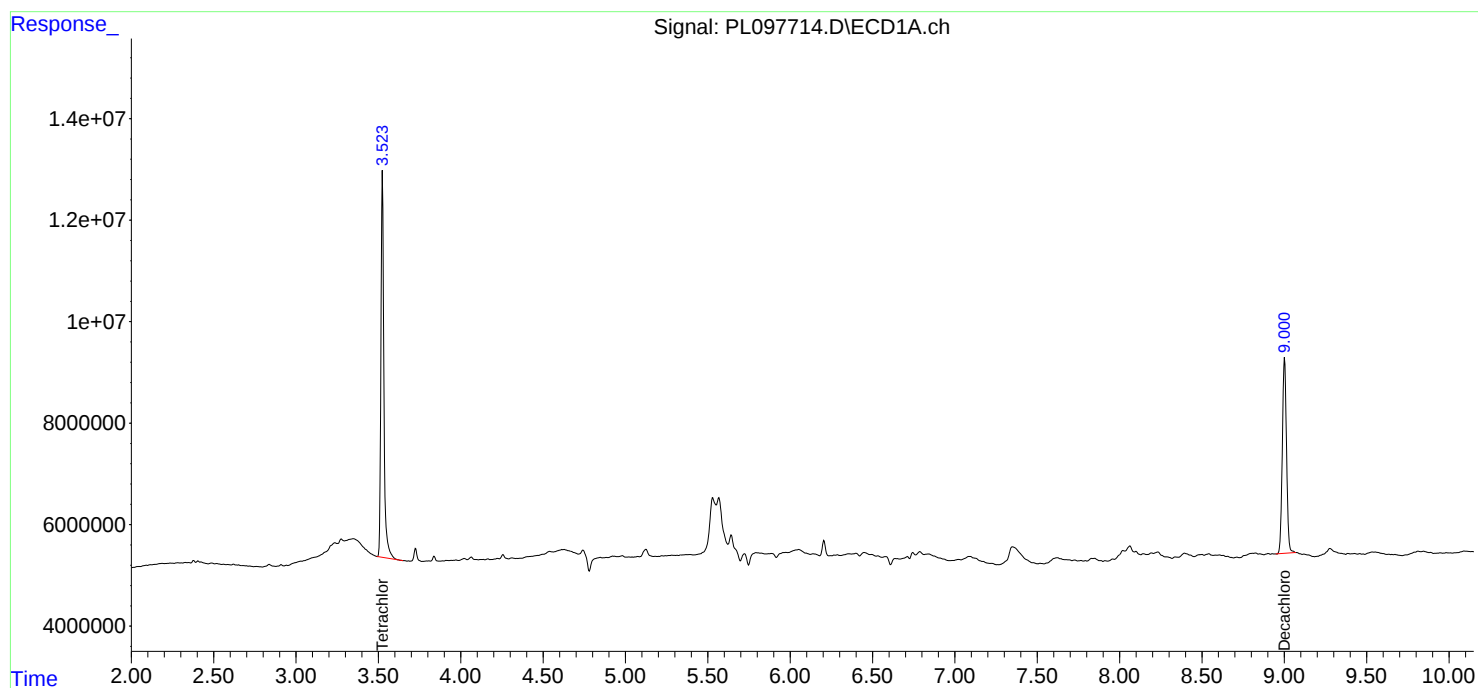


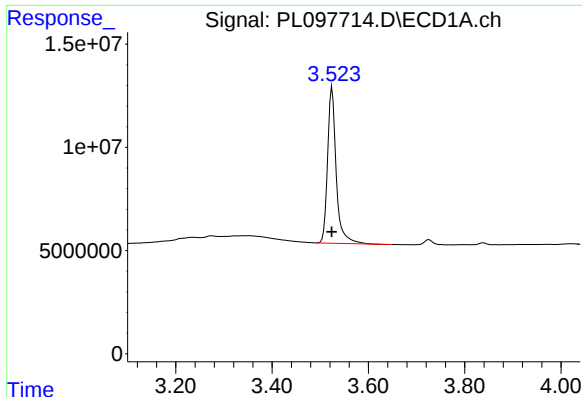

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 94128288
Conc: 23.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

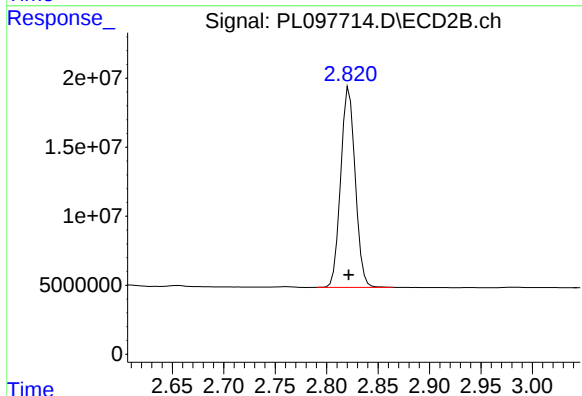


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 142134857
Conc: 23.61 ng/ml

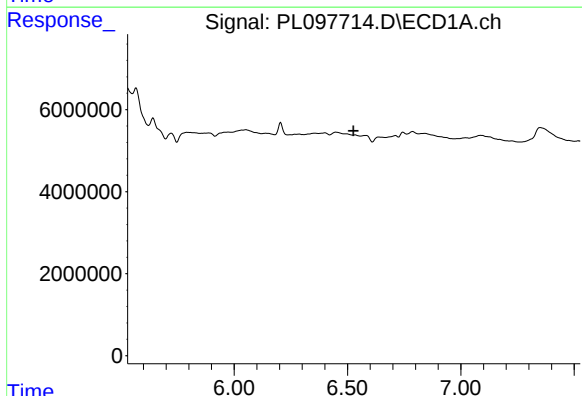


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

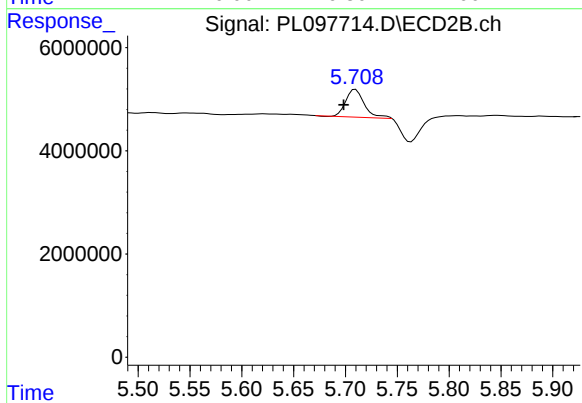

#14 Endrin

R.T.: 5.710 min
Delta R.T.: 0.011 min
Response: 6702774
Conc: 0.96 ng/ml

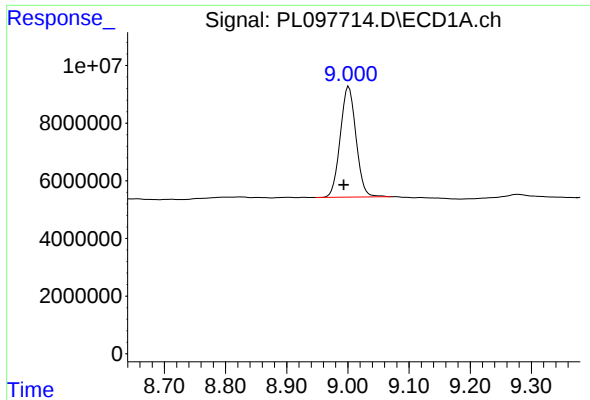

#28 Decachlorobiphenyl


R.T.: 9.001 min

Delta R.T.: 0.009 min

Response: 68615226

Conc: 23.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

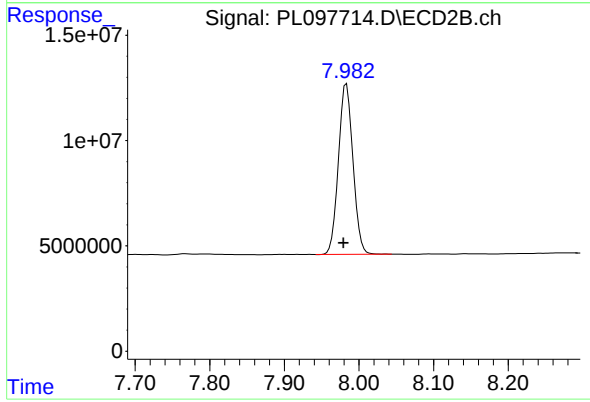

#28 Decachlorobiphenyl

R.T.: 7.983 min

Delta R.T.: 0.004 min

Response: 109593678

Conc: 20.50 ng/ml