

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
 Data File : PL097703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 12:17
 Operator : AR\AJ
 Sample : Q3490-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LAW-25-0151

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/03/2025
 Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:53:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.521	2.818	1419008	6983179	0.347m	1.160m#
28) SA Decachlor...	9.002	7.983	4148743	3058370	1.394m	0.572m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103125\
Data File : PL097703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 12:17
Operator : AR\AJ
Sample : Q3490-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LAW-25-0151


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:53:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

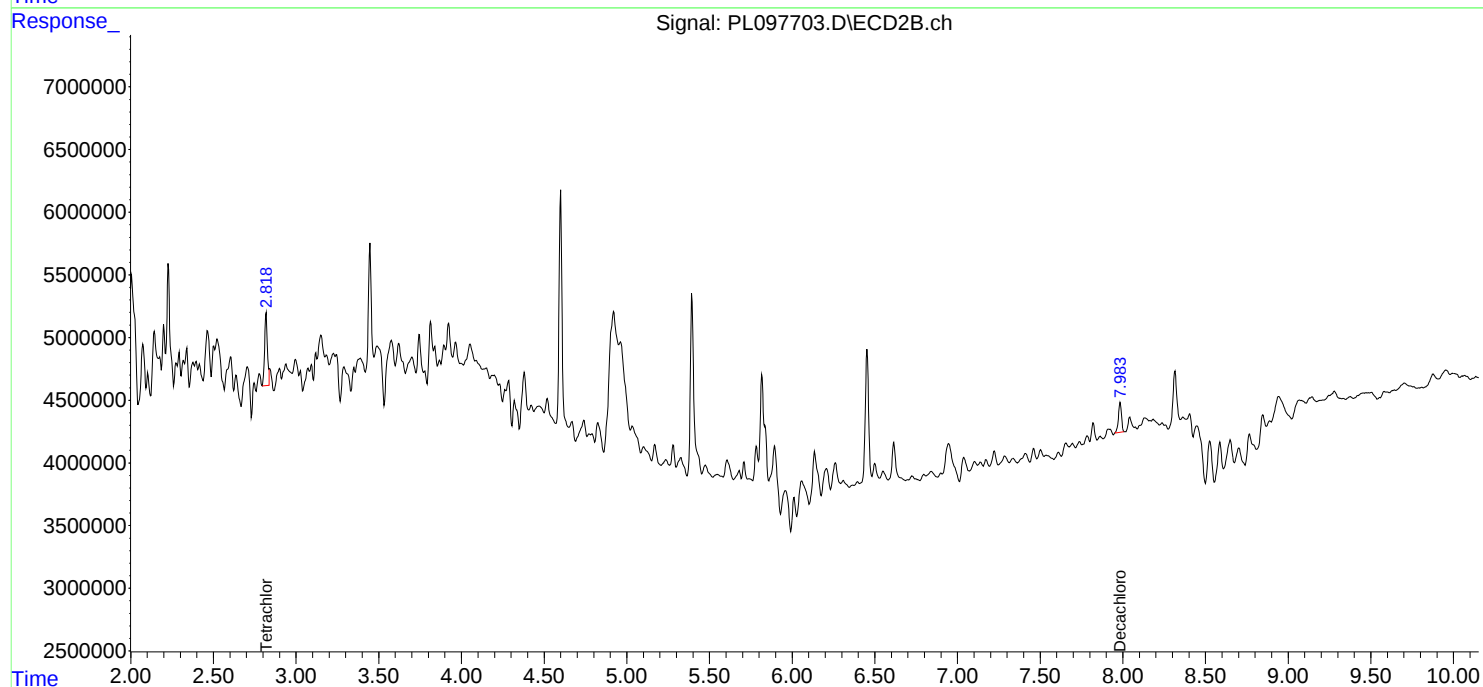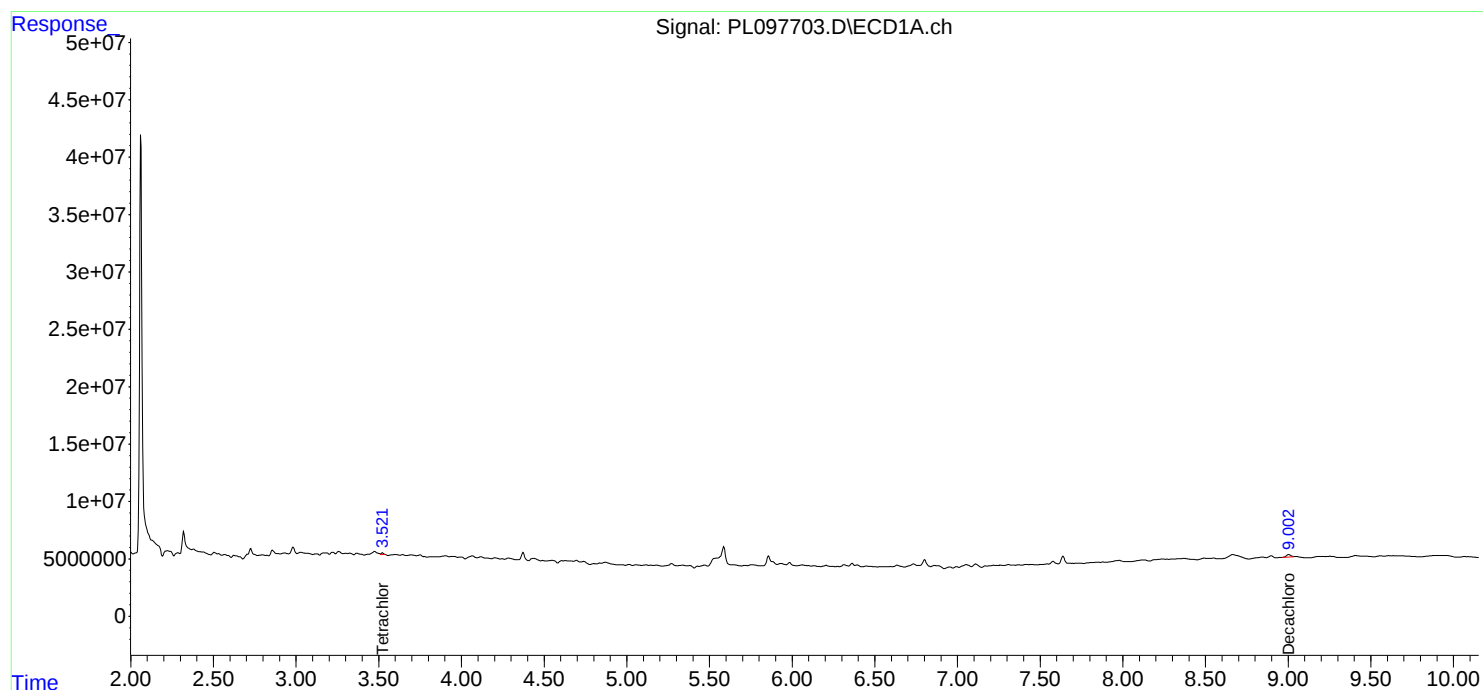

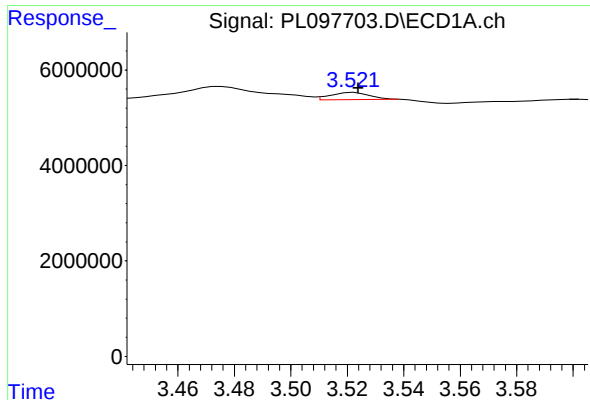


#1 Tetrachloro-m-xylene

R.T.: 3.521 min
Delta R.T.: -0.003 min
Response: 1419008
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
LAW-25-0151


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

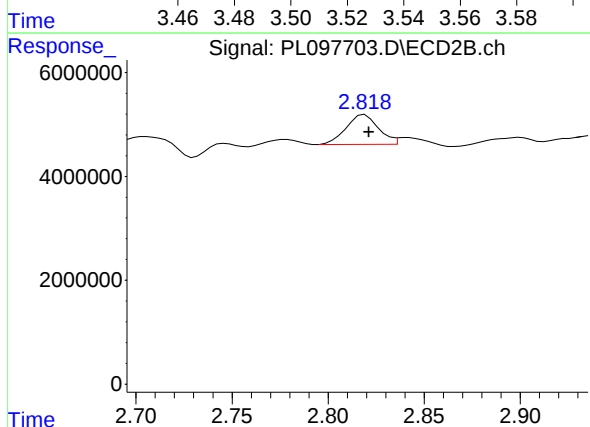


#1 Tetrachloro-m-xylene

R.T.: 2.818 min
Delta R.T.: -0.004 min
Response: 6983179
Conc: 1.16 ng/ml m

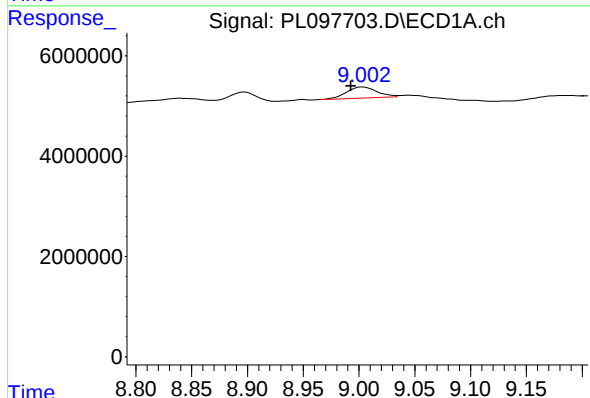

#28 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.009 min
Response: 4148743
Conc: 1.39 ng/ml m

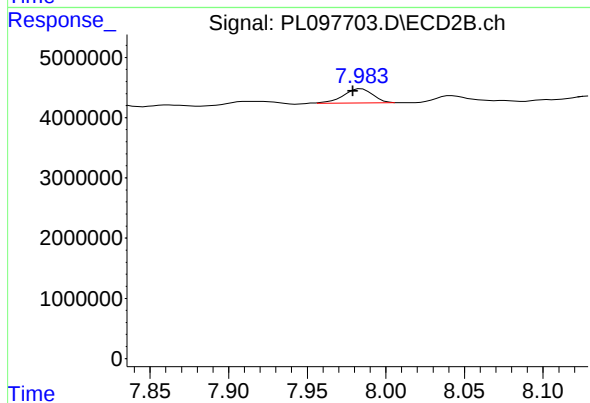

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: 0.004 min
Response: 3058370
Conc: 0.57 ng/ml m