

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
 Data File : PL041614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 13:09
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:06:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.480	4.103	125.5E6	67543099	19.703	21.928
28)	SA Decachlor...	8.224	9.237	126.9E6	53574958	19.157	20.910
Target Compounds							
2)	A alpha-BHC	0.000	4.458f	0	1085544	N.D.	0.237 #
6)	B beta-BHC	4.417f	0.000	1124070	0	0.298	N.D. #
9)	A Endosulfan I	0.000	6.314f	0	7894846	N.D.	2.540 #
10)	B gamma-Chl...	0.000	6.170f	0	3260569	N.D.	0.966 #
11)	B alpha-Chl...	0.000	6.314	0	7894846	N.D.	2.333 #
14)	MA Endrin	6.091f	0.000	1195181	0	0.163	N.D. #
16)	A 4,4'-DDD	6.091f	0.000	1195181	0	0.206	N.D. #
19)	B Endosulfa...	6.716f	0.000	1854664	0	0.290	N.D. #
25)	Chlordane-3	0.000	6.170	0	3260569	N.D.	7.245 #
26)	Chlordane-4	0.000	6.314	0	7894846	N.D.	15.100 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
Data File : PL041614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 13:09
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:06:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

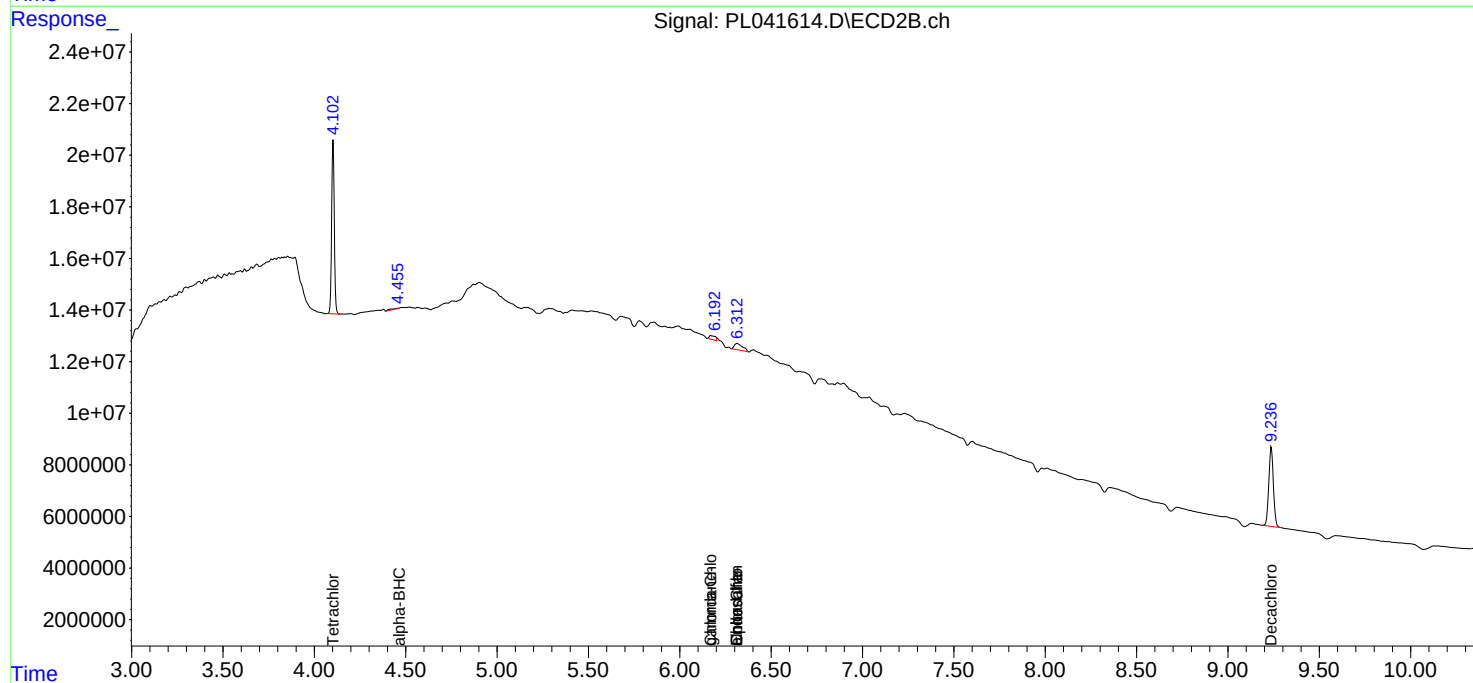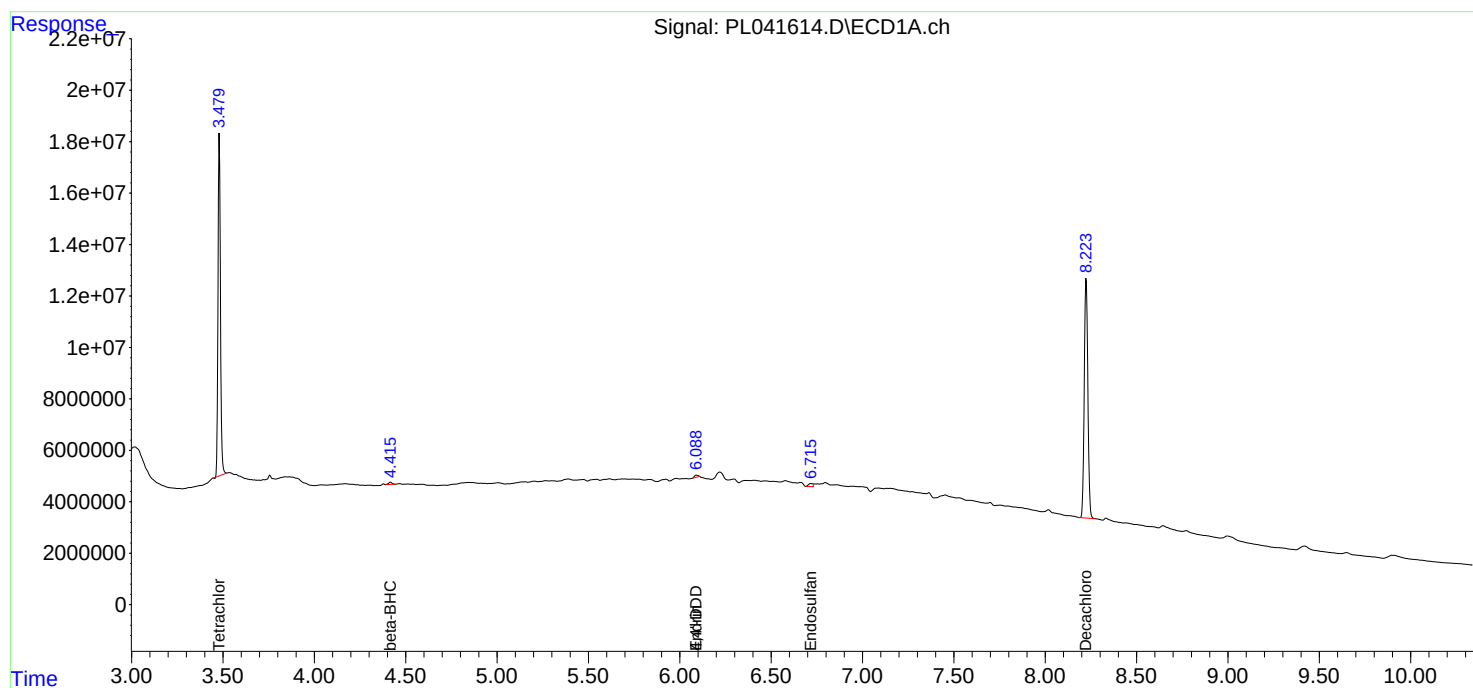


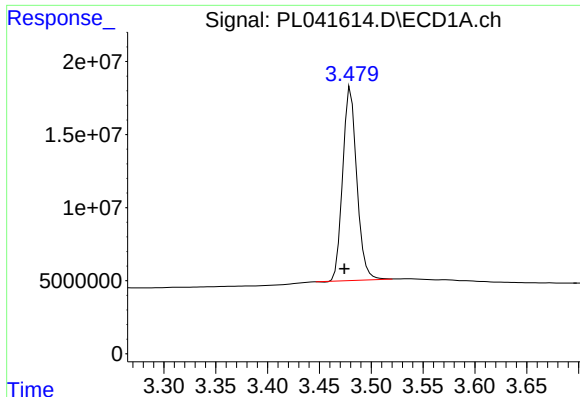

#1 Tetrachloro-m-xylene


R.T.: 3.480 min
Delta R.T.: 0.006 min
Response: 125515786
Conc: 19.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

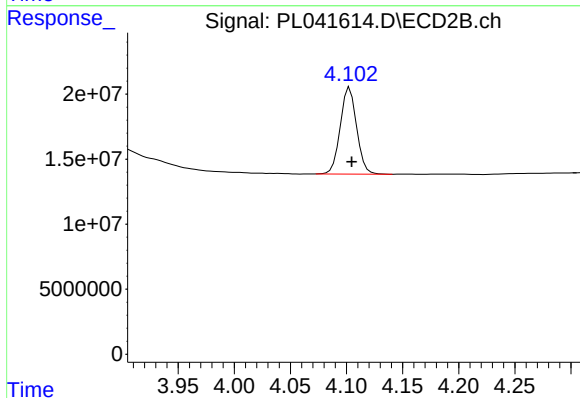


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.002 min
Response: 67543099
Conc: 21.93 ng/ml

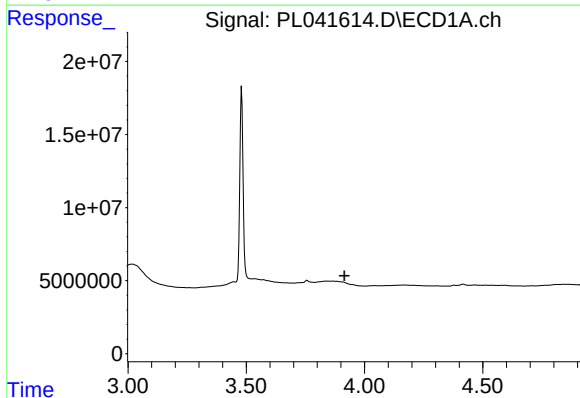


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.915 min
Response: 0
Conc: N.D.

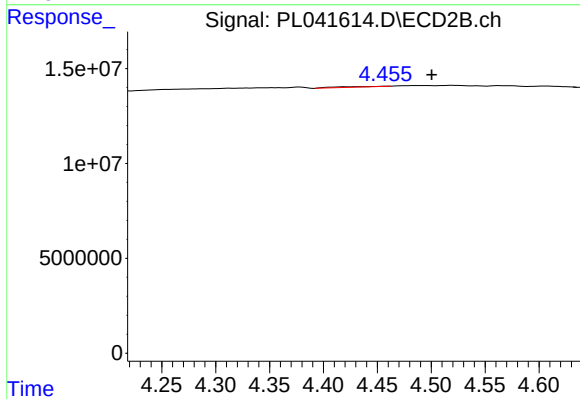

#2 alpha-BHC


R.T.: 4.458 min
Delta R.T.: -0.043 min
Response: 1085544
Conc: 0.24 ng/ml

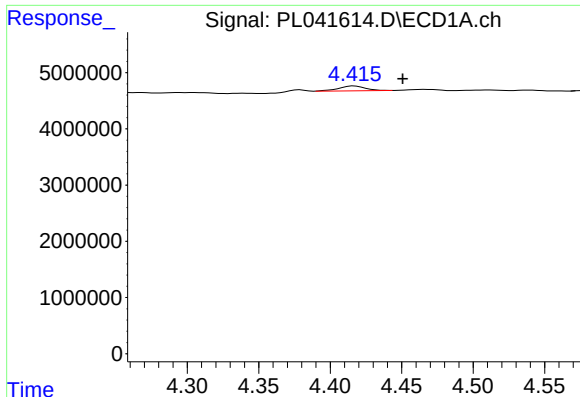

#6 beta-BHC


R.T.: 4.417 min
Delta R.T.: -0.034 min
Response: 1124070
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

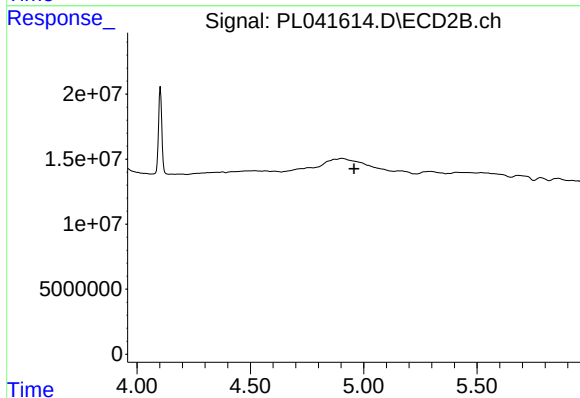


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

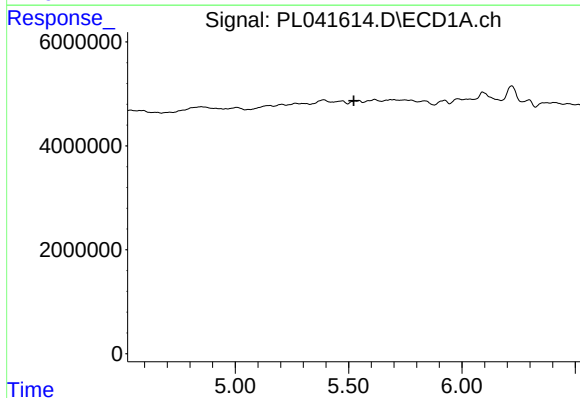


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

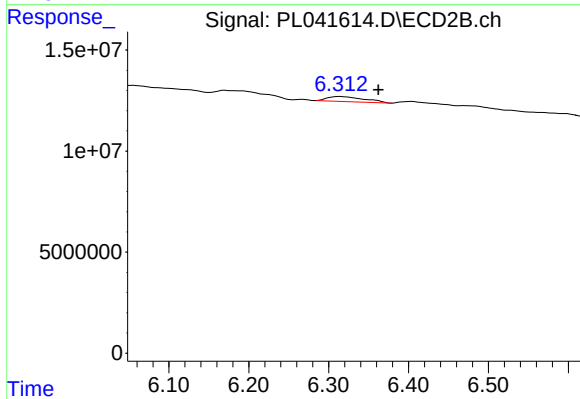

#9 Endosulfan I


R.T.: 6.314 min
Delta R.T.: -0.049 min
Response: 7894846
Conc: 2.54 ng/ml

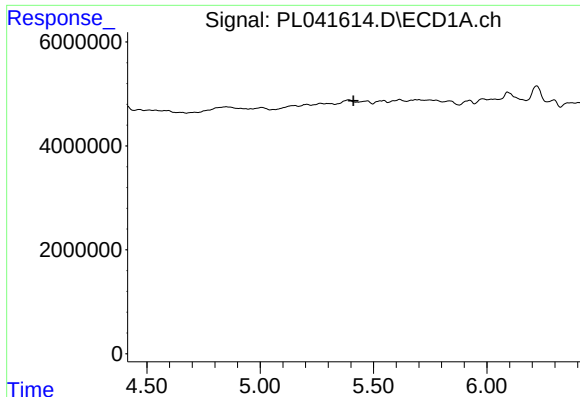

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

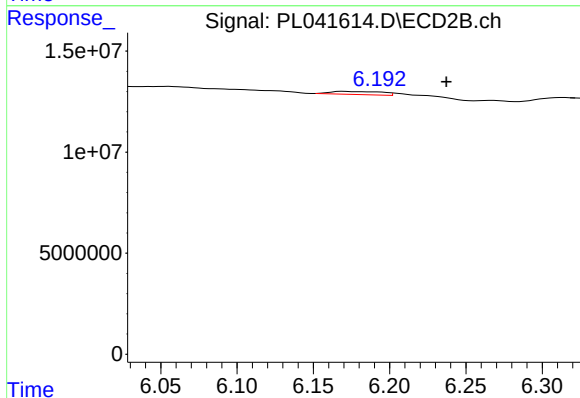


#10 gamma-Chlordane

R.T.: 6.170 min
Delta R.T.: -0.068 min
Response: 3260569
Conc: 0.97 ng/ml

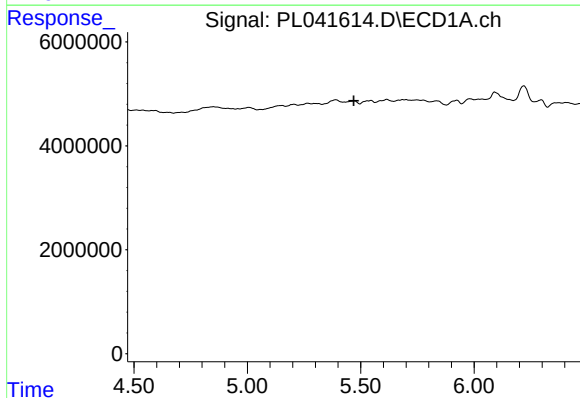


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

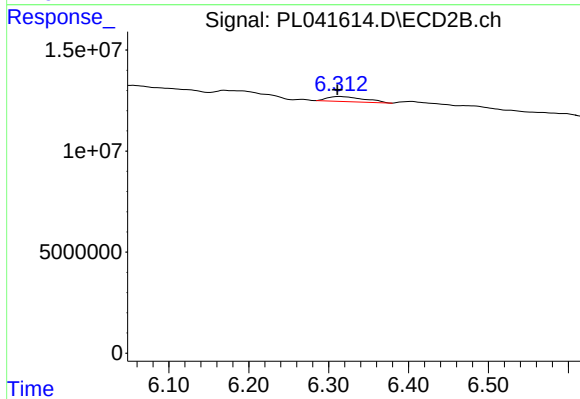

#11 alpha-Chlordane


R.T.: 6.314 min
Delta R.T.: 0.002 min
Response: 7894846
Conc: 2.33 ng/ml

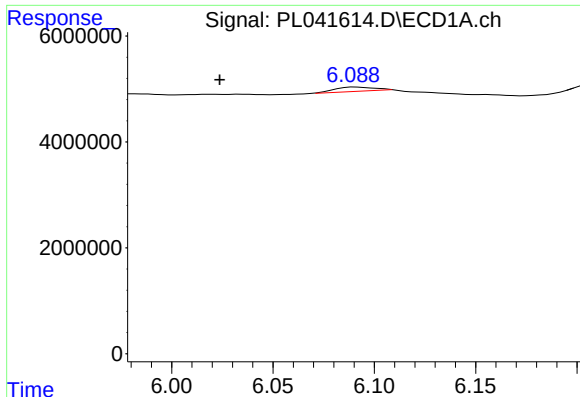

#14 Endrin


R.T.: 6.091 min
Delta R.T.: 0.067 min
Response: 1195181
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

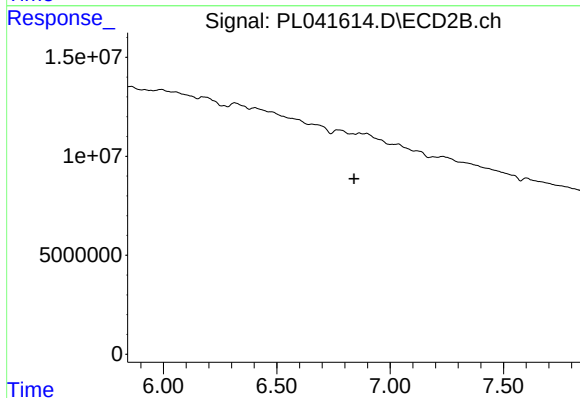


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.840 min
Response: 0
Conc: N.D.

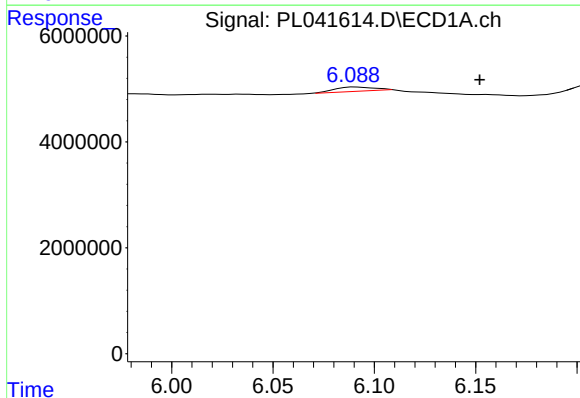


#16 4,4'-DDD

R.T.: 6.091 min
Delta R.T.: -0.061 min
Response: 1195181
Conc: 0.21 ng/ml

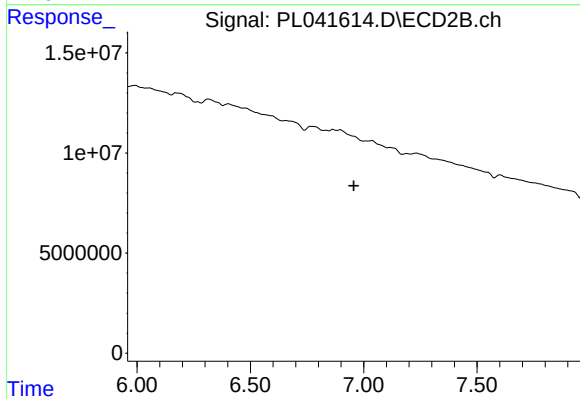

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

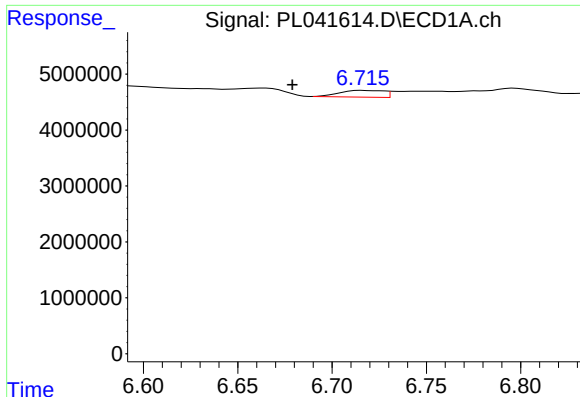

#19 Endosulfan Sulfate


R.T.: 6.716 min
Delta R.T.: 0.037 min
Response: 1854664
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

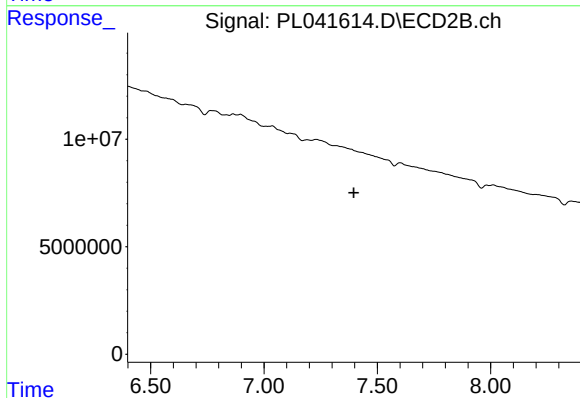


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.396 min
Response: 0
Conc: N.D.

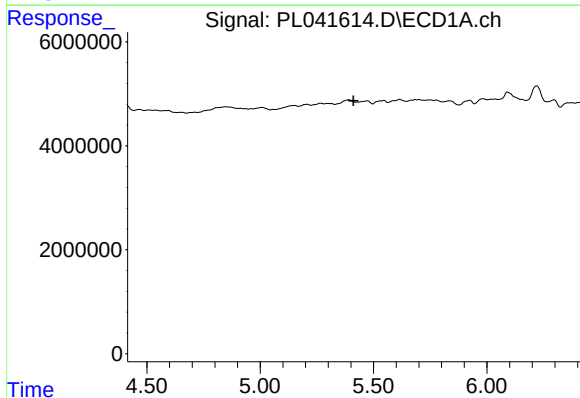


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

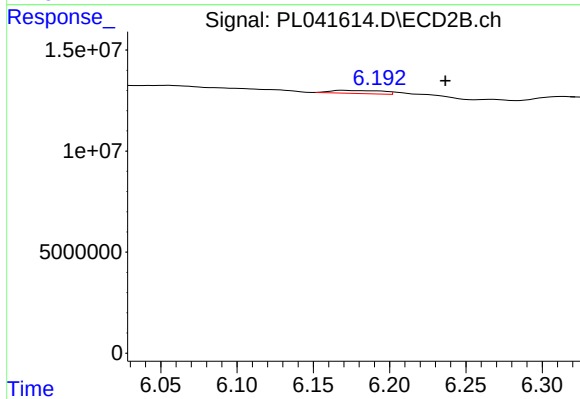

#25 Chlordane-3


R.T.: 6.170 min
Delta R.T.: -0.067 min
Response: 3260569
Conc: 7.25 ng/ml

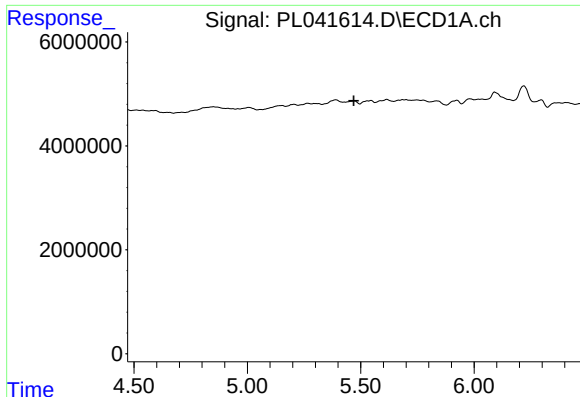

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

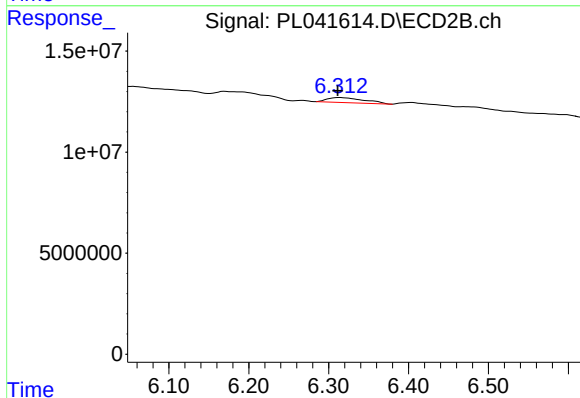


#26 Chlordane-4

R.T.: 6.314 min
Delta R.T.: 0.002 min
Response: 7894846
Conc: 15.10 ng/ml

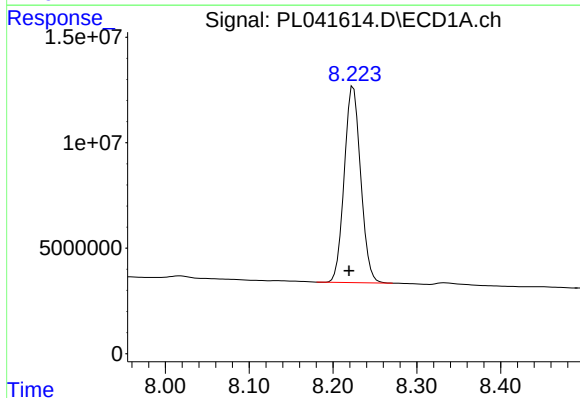

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: 0.005 min
Response: 126898865
Conc: 19.16 ng/ml

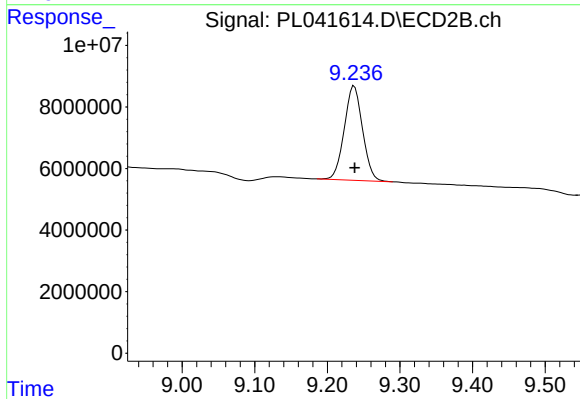

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 53574958
Conc: 20.91 ng/ml